

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
 Data File : PL043512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2018 18:39
 Operator : AJ\SJ
 Sample : J6193-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-122718-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 22:35:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.100	142.4E6	74162422	23.216	25.022
28)	SA Decachlor...	8.199	9.229	128.0E6	54640895	19.599	20.947
Target Compounds							
2)	A alpha-BHC	3.894	0.000	7245078	0	0.766	N.D. #
3)	MA gamma-BHC...	0.000	4.745f	0	762738	N.D.	0.182 #
6)	B beta-BHC	4.446	4.922f	-97437	2129276	N.D.	1.258
7)	B delta-BHC	0.000	5.146f	0	5255272	N.D.	1.223 #
8)	B Heptachlo...	0.000	5.999	0	3484948	N.D.	0.919 #
14)	MA Endrin	6.065f	0.000	963023	0	0.134	N.D. #
16)	A 4,4'-DDD	6.095f	0.000	338951	0	0.060	N.D. #
23)	Chlordane-1	4.335	5.146	2590739	5255272	9.642	37.184 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
Data File : PL043512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2018 18:39
Operator : AJ\SJ
Sample : J6193-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 22:35:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

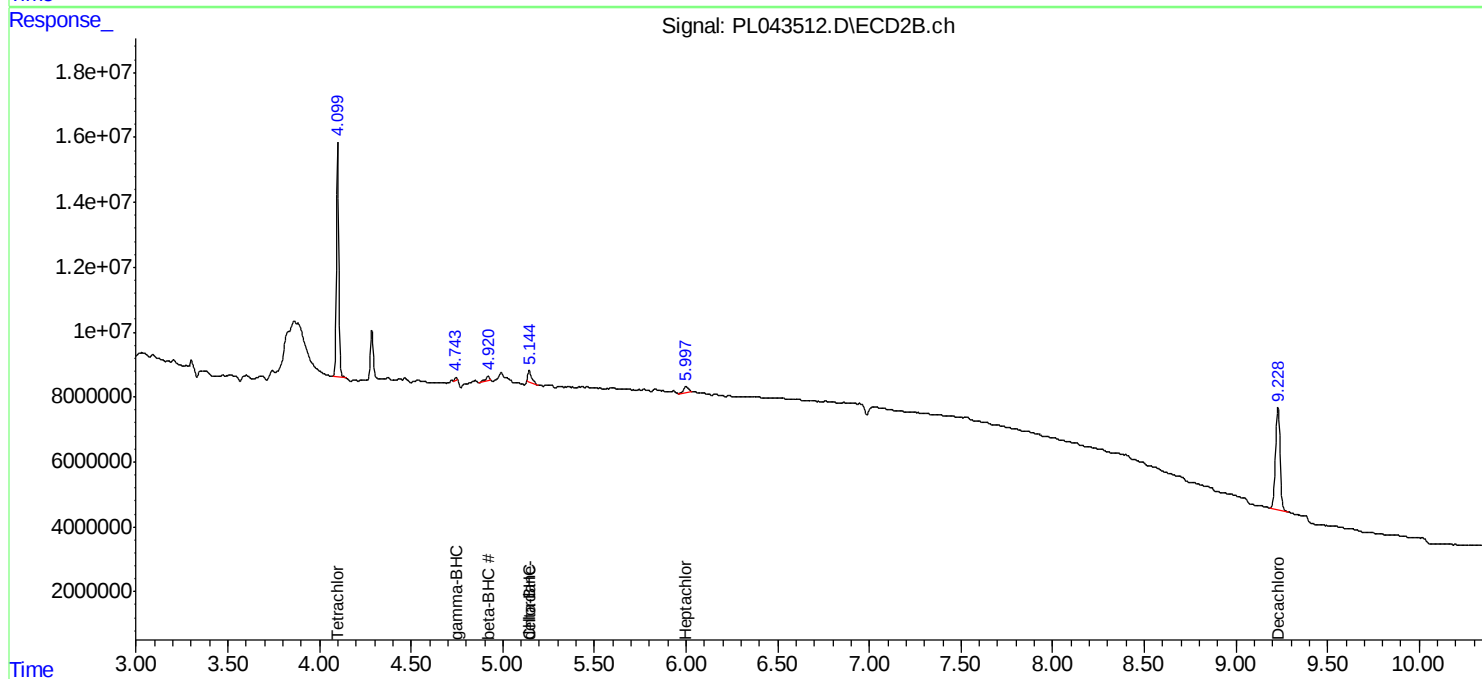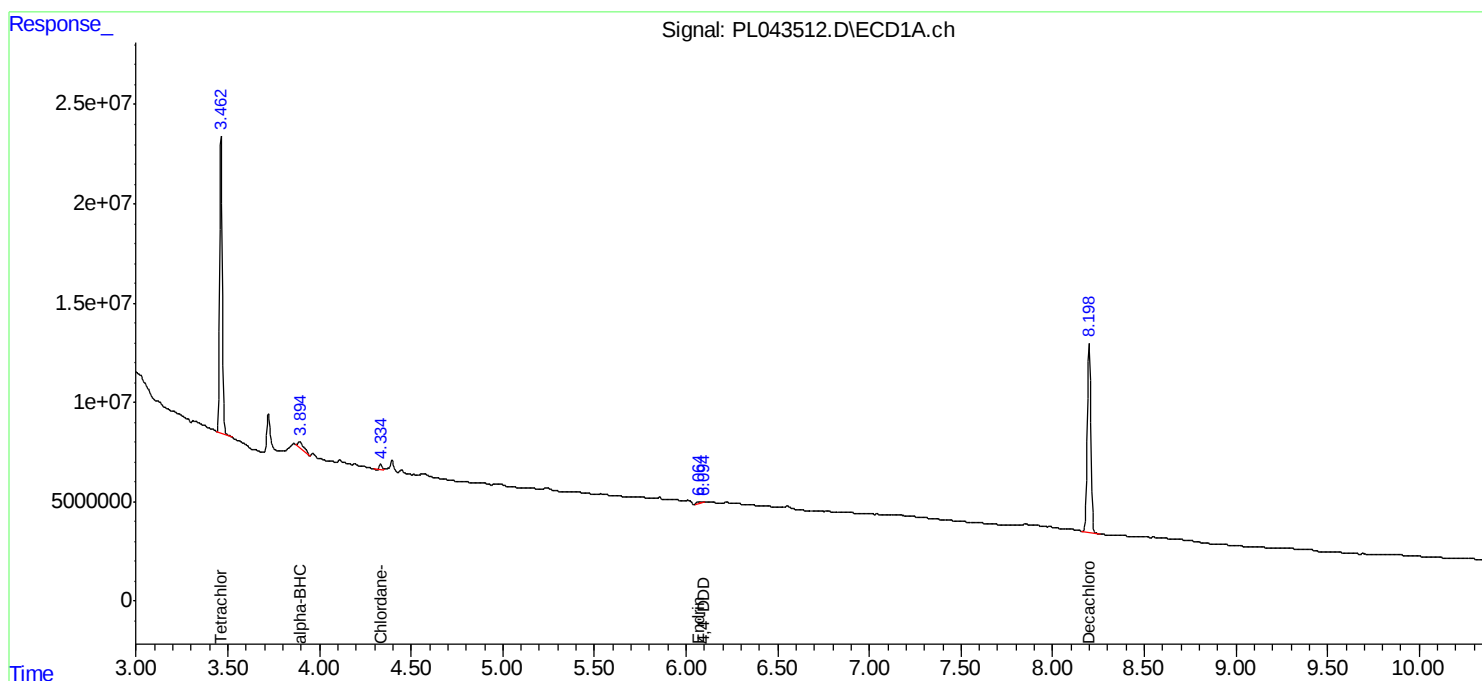


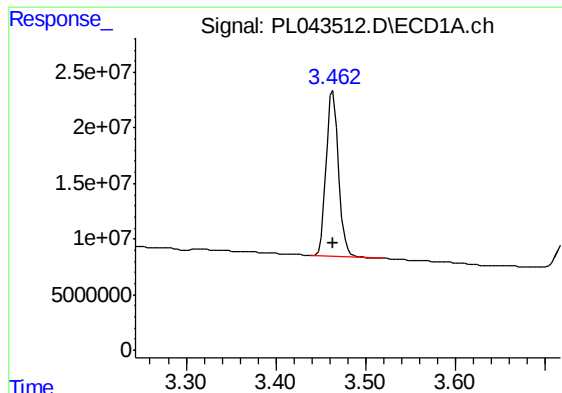

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 142382319
Conc: 23.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-C

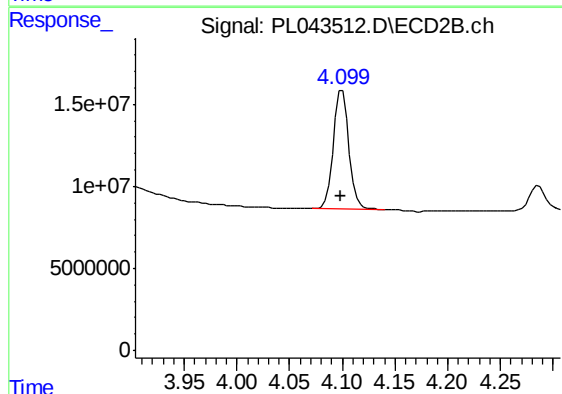


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 74162422
Conc: 25.02 ng/ml

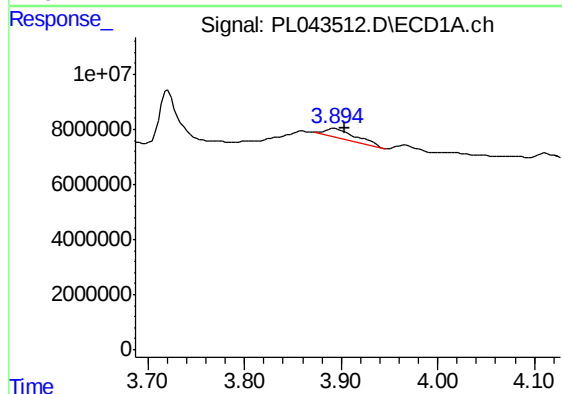


#2 alpha-BHC

R.T.: 3.894 min
Delta R.T.: -0.010 min
Response: 7245078
Conc: 0.77 ng/ml

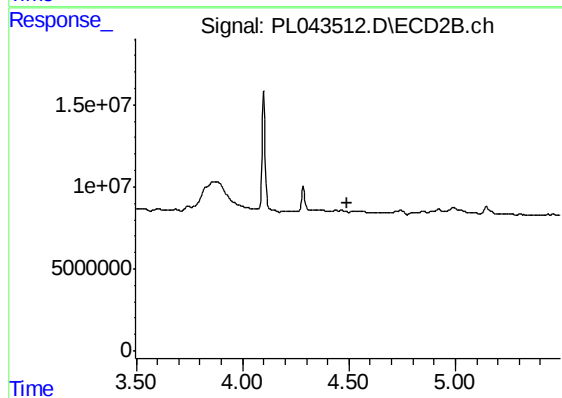

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

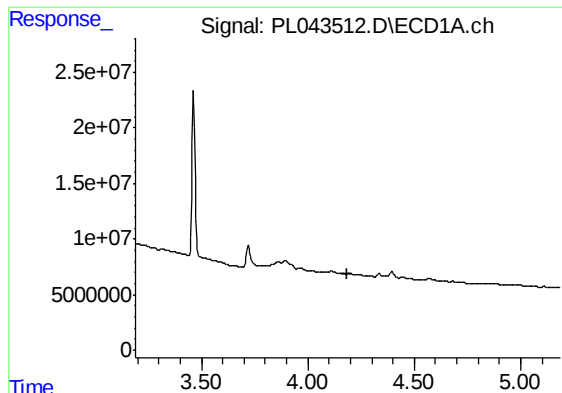

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-C

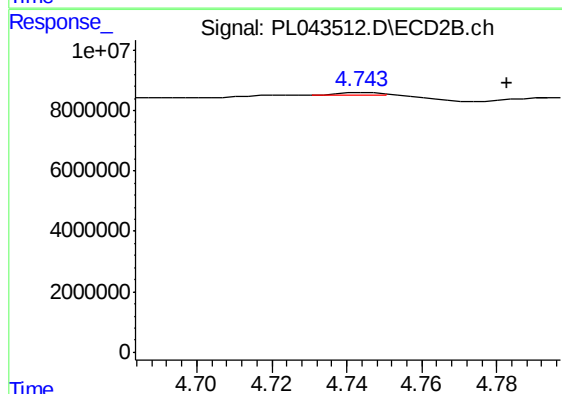


#3 gamma-BHC (Lindane)

R.T.: 4.745 min
Delta R.T.: -0.038 min
Response: 762738
Conc: 0.18 ng/ml

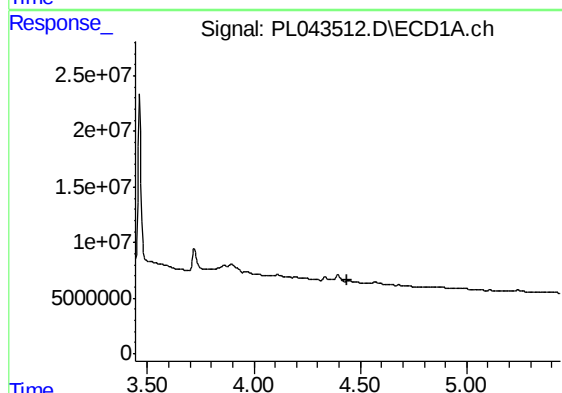


#6 beta-BHC

R.T.: 4.446 min
Delta R.T.: 0.005 min
Response: -97437
Conc: N.D.

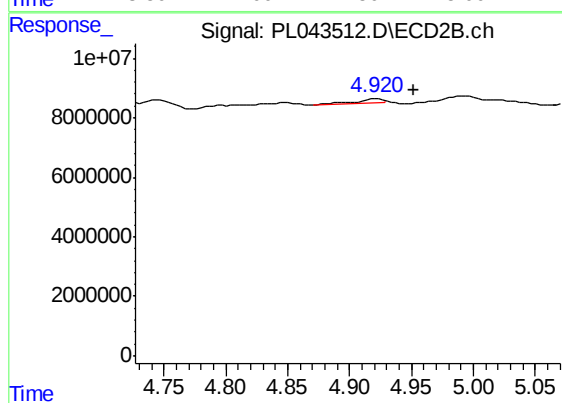

#6 beta-BHC


R.T.: 4.922 min
Delta R.T.: -0.030 min
Response: 2129276
Conc: 1.26 ng/ml

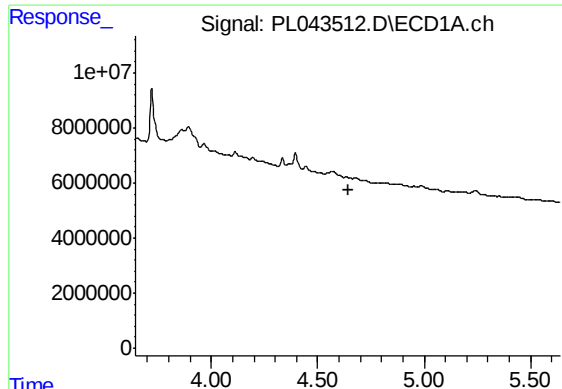

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-C

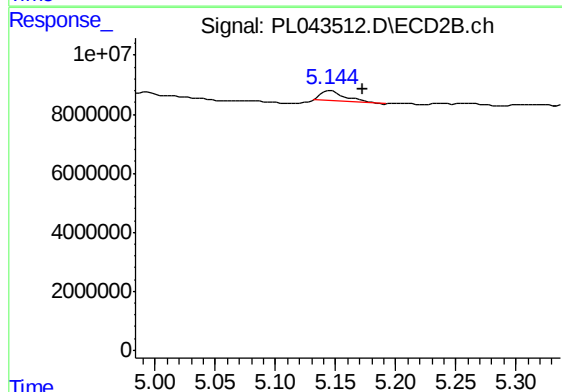


#7 delta-BHC

R.T.: 5.146 min
Delta R.T.: -0.027 min
Response: 5255272
Conc: 1.22 ng/ml

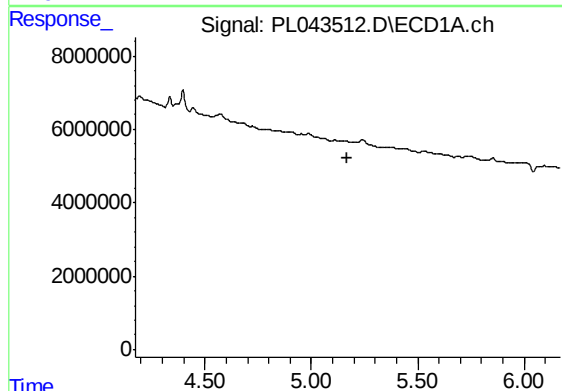


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

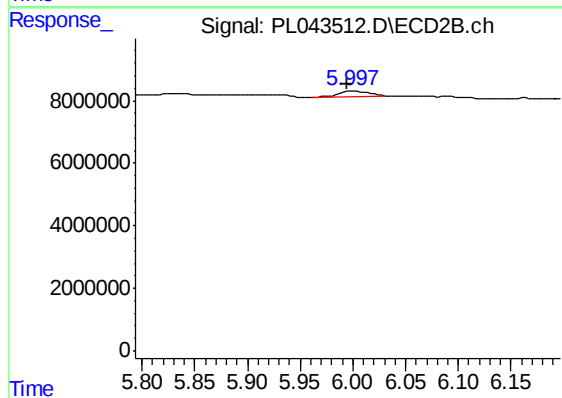

#8 Heptachlor epoxide


R.T.: 5.999 min
Delta R.T.: 0.004 min
Response: 3484948
Conc: 0.92 ng/ml

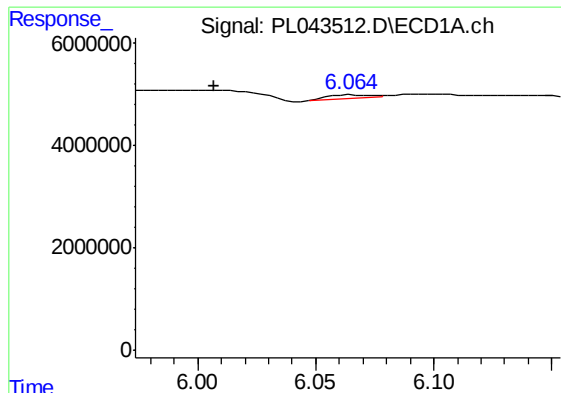

#14 Endrin


R.T.: 6.065 min
Delta R.T.: 0.058 min
Response: 963023
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-C

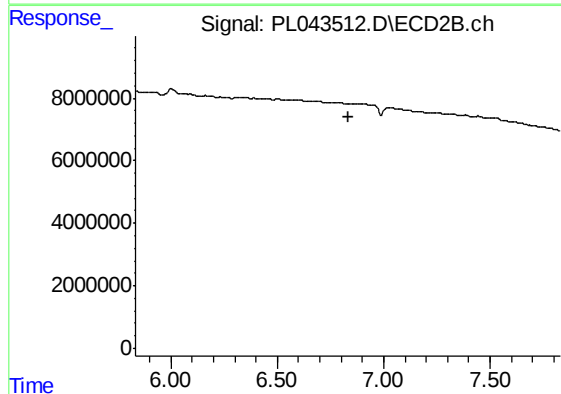


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

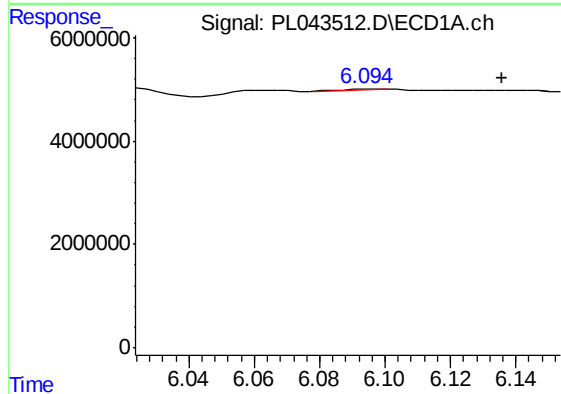


#16 4,4'-DDD

R.T.: 6.095 min
Delta R.T.: -0.041 min
Response: 338951
Conc: 0.06 ng/ml

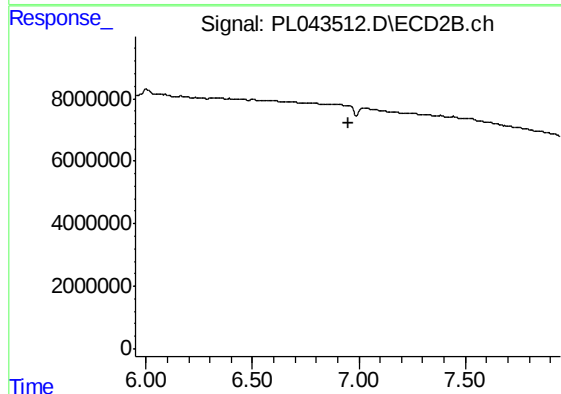

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

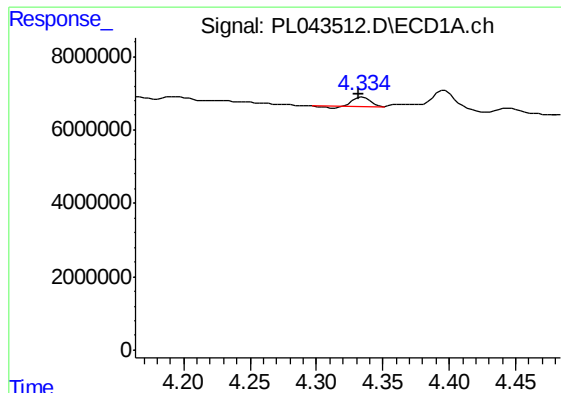

#23 Chlordane-1


R.T.: 4.335 min
Delta R.T.: 0.003 min
Response: 2590739
Conc: 9.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-C

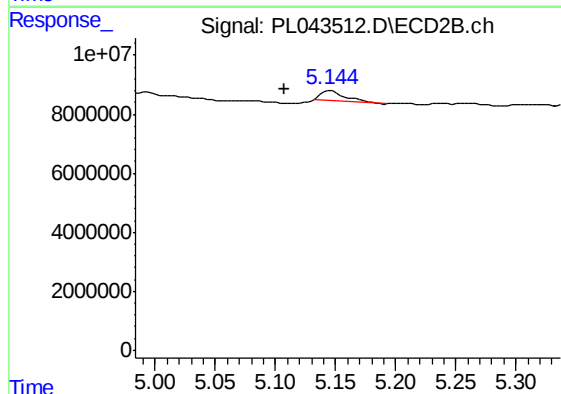


#23 Chlordane-1

R.T.: 5.146 min
Delta R.T.: 0.038 min
Response: 5255272
Conc: 37.18 ng/ml

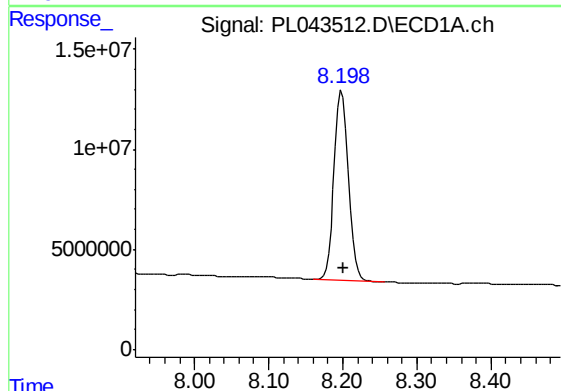

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: -0.002 min
Response: 127978146
Conc: 19.60 ng/ml

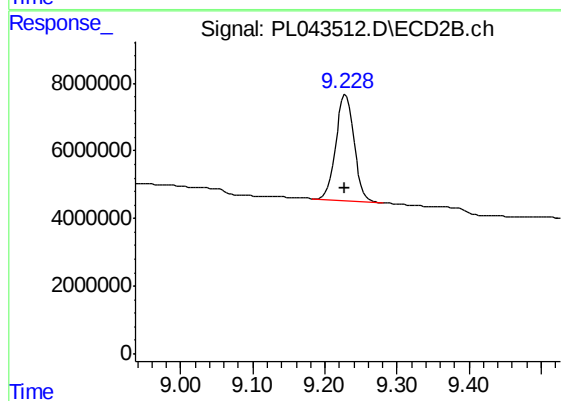

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: 0.002 min
Response: 54640895
Conc: 20.95 ng/ml