

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
 Data File : PL043513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2018 18:53
 Operator : AJ\SJ
 Sample : J6193-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-122718-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 22:35:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.100	139.0E6	72937427	22.657	24.609
28)	SA Decachlor...	8.200	9.231	126.4E6	56616878	19.358	21.705
Target Compounds							
3)	MA gamma-BHC...	0.000	4.747f	0	1347393	N.D.	0.321 #
4)	MA Heptachlor	4.447	0.000	1467924	0	0.165	N.D. #
6)	B beta-BHC	4.447	0.000	1467924	0	0.398	N.D. #
7)	B delta-BHC	0.000	5.148	0	8571020	N.D.	1.994 #
8)	B Heptachlo...	0.000	6.000	0	6256939	N.D.	1.650 #
14)	MA Endrin	6.069f	0.000	708681	0	0.098	N.D. #
16)	A 4,4'-DDD	6.069f	0.000	708681	0	0.125	N.D. #
23)	Chlordane-1	4.397	5.148	6514665	8571020	24.245	60.644 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
Data File : PL043513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2018 18:53
Operator : AJ\SJ
Sample : J6193-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 22:35:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

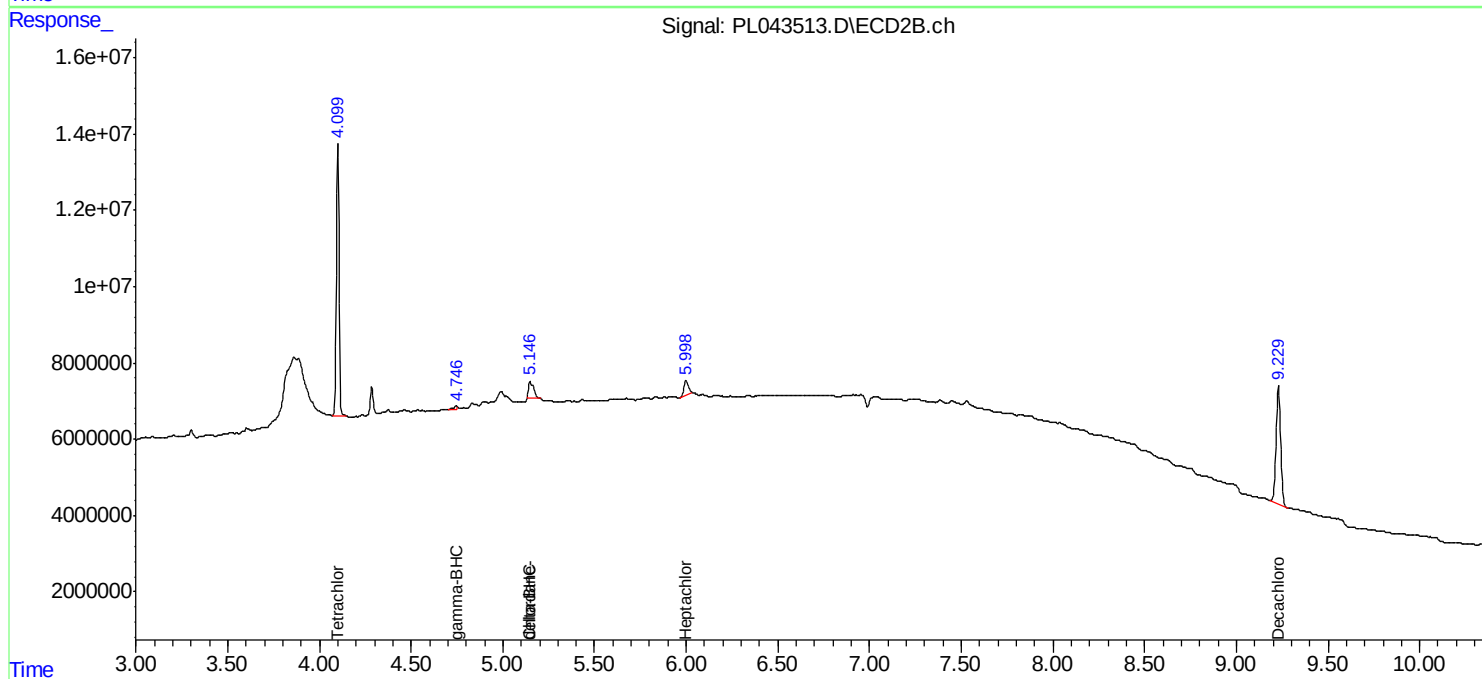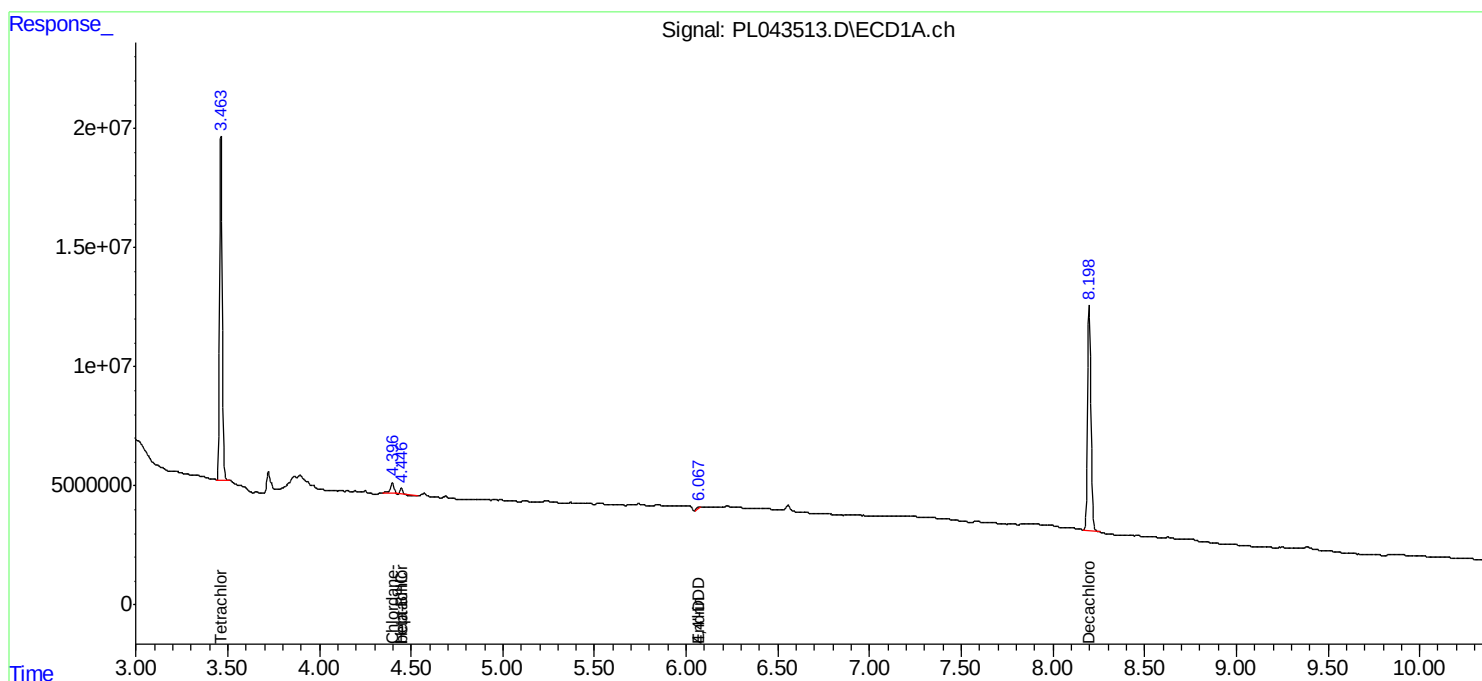


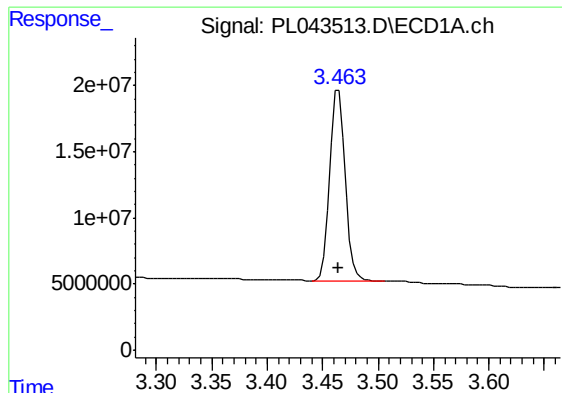

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 138952777
Conc: 22.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-D

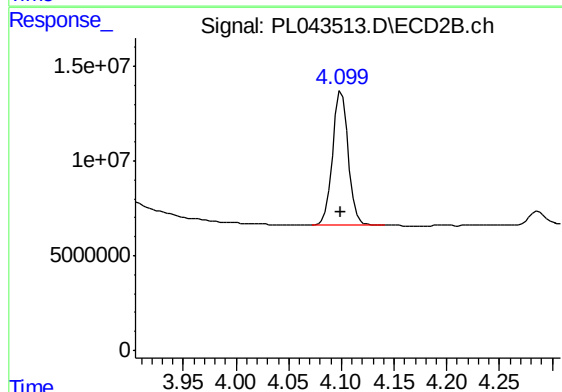


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.001 min
Response: 72937427
Conc: 24.61 ng/ml

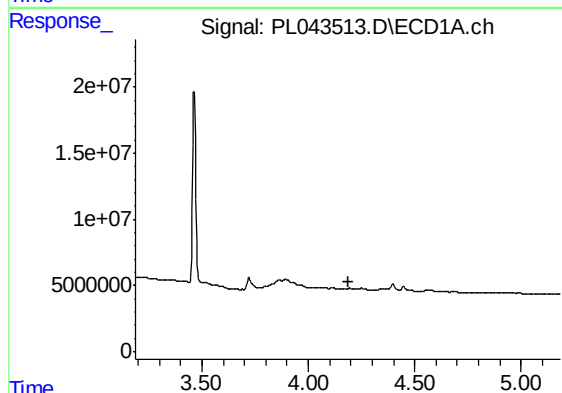


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

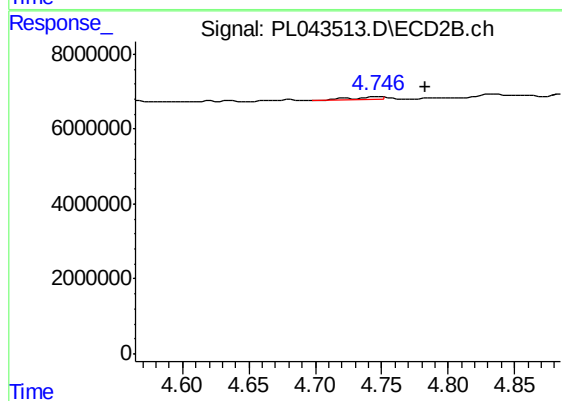

#3 gamma-BHC (Lindane)


R.T.: 4.747 min
Delta R.T.: -0.036 min
Response: 1347393
Conc: 0.32 ng/ml

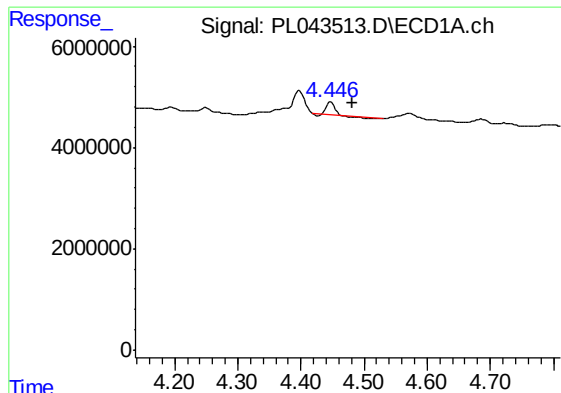

#4 Heptachlor


R.T.: 4.447 min
Delta R.T.: -0.035 min
Response: 1467924
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-D

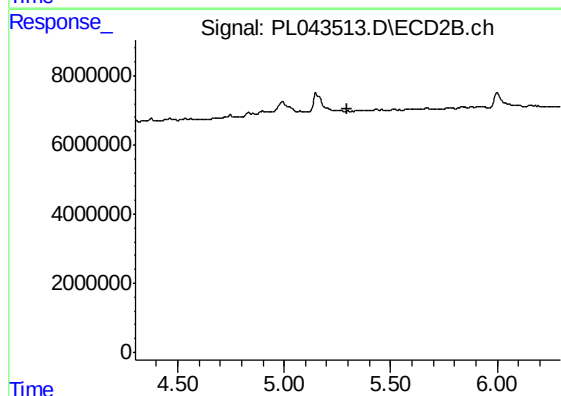


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.298 min
Response: 0
Conc: N.D.

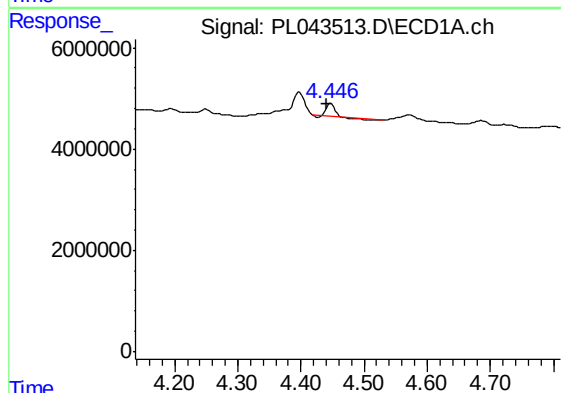


#6 beta-BHC

R.T.: 4.447 min
Delta R.T.: 0.007 min
Response: 1467924
Conc: 0.40 ng/ml

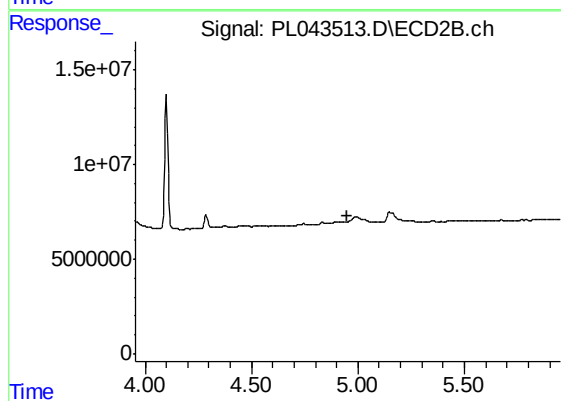

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

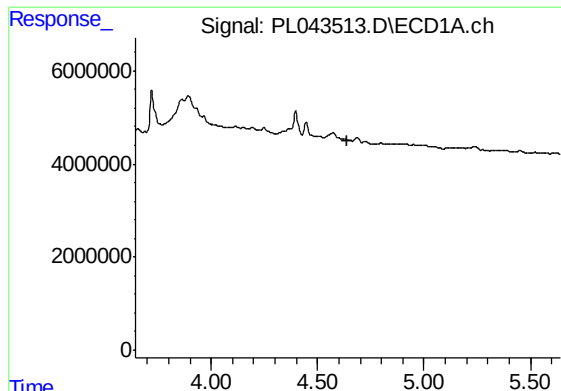

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-D

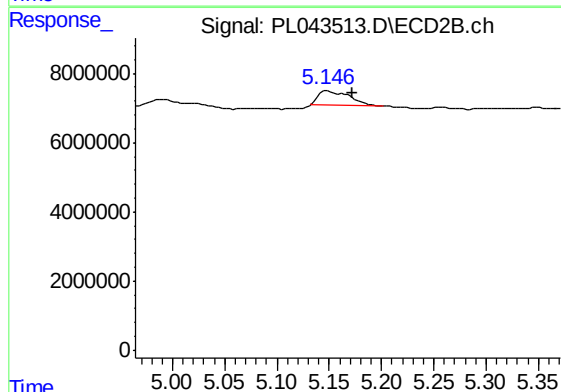


#7 delta-BHC

R.T.: 5.148 min
Delta R.T.: -0.025 min
Response: 8571020
Conc: 1.99 ng/ml

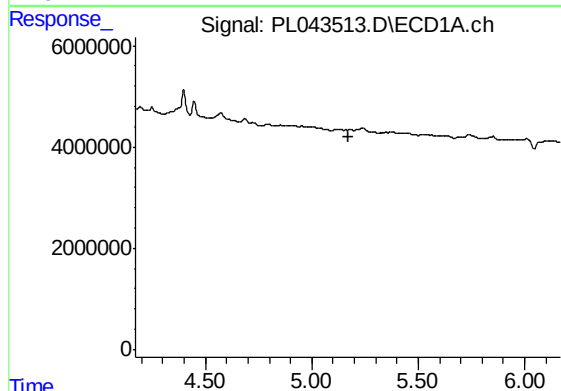


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

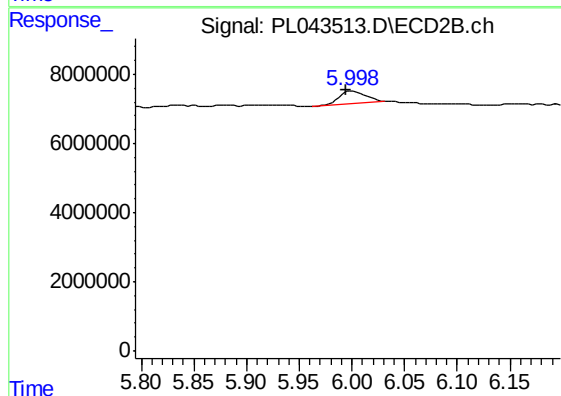

#8 Heptachlor epoxide


R.T.: 6.000 min
Delta R.T.: 0.005 min
Response: 6256939
Conc: 1.65 ng/ml

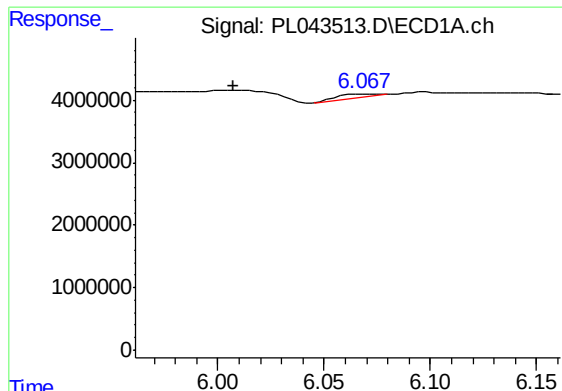

#14 Endrin


R.T.: 6.069 min
Delta R.T.: 0.062 min
Response: 708681
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-D

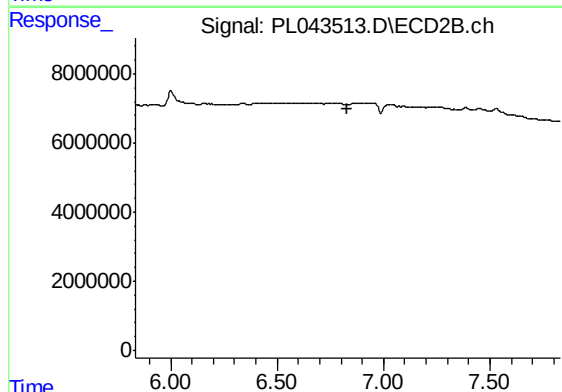


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

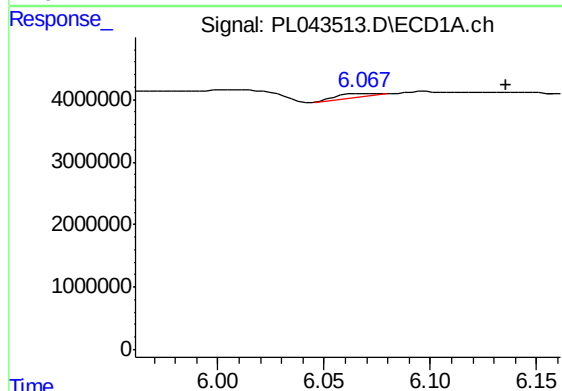


#16 4,4'-DDD

R.T.: 6.069 min
Delta R.T.: -0.067 min
Response: 708681
Conc: 0.12 ng/ml

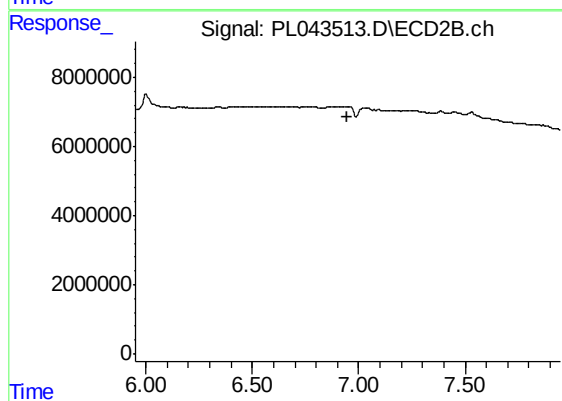

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

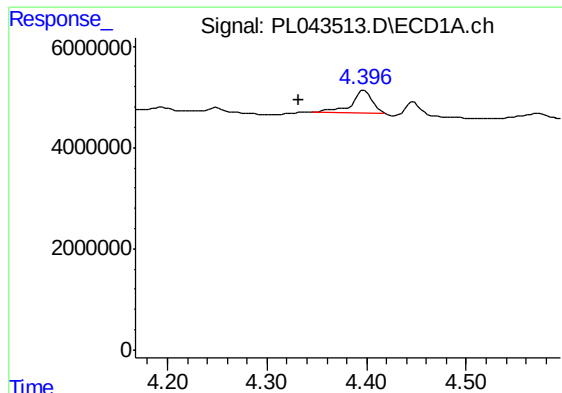

#23 Chlordane-1


R.T.: 4.397 min
Delta R.T.: 0.065 min
Response: 6514665
Conc: 24.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-122718-D

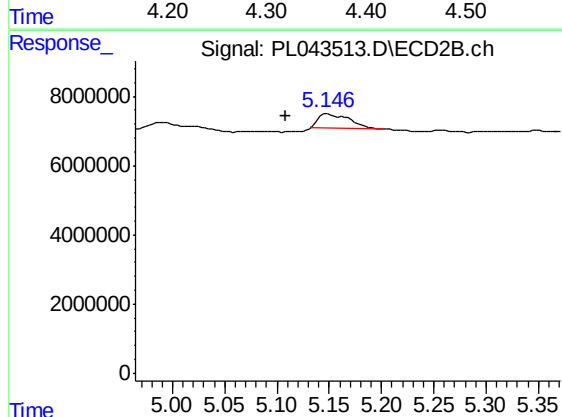


#23 Chlordane-1

R.T.: 5.148 min
Delta R.T.: 0.040 min
Response: 8571020
Conc: 60.64 ng/ml

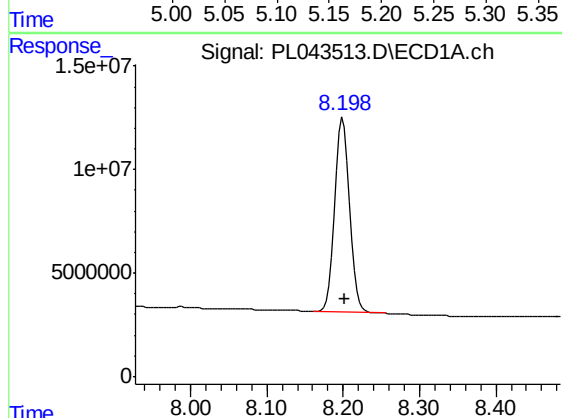

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: -0.002 min
Response: 126408918
Conc: 19.36 ng/ml

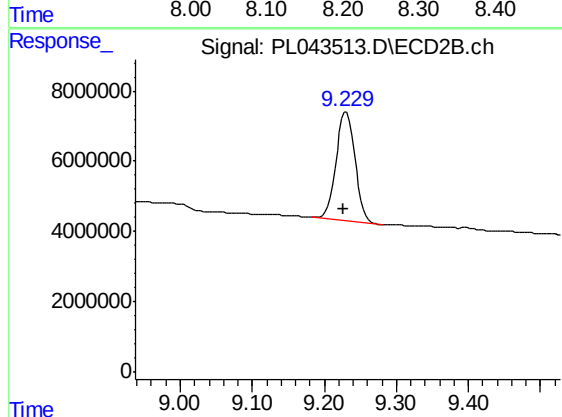

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 56616878
Conc: 21.70 ng/ml