

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
 Data File : PL043515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2018 19:21
 Operator : AJ\SJ
 Sample : J6584-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RECLAIMER-PIT

Manual Integrations
 APPROVED

Sohil
 1/2/2019 8:47:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 22:36:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.100	120.1E6	58140568	19.589m	19.616
28)	SA Decachlor...	8.199	9.230	97597797	43663427	14.946	16.739

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122818\
Data File : PL043515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2018 19:21
Operator : AJ\SJ
Sample : J6584-02
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RECLAIMER-PIT


Manual Integrations
APPROVED

Sohil
1/2/2019 8:47:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 22:36:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

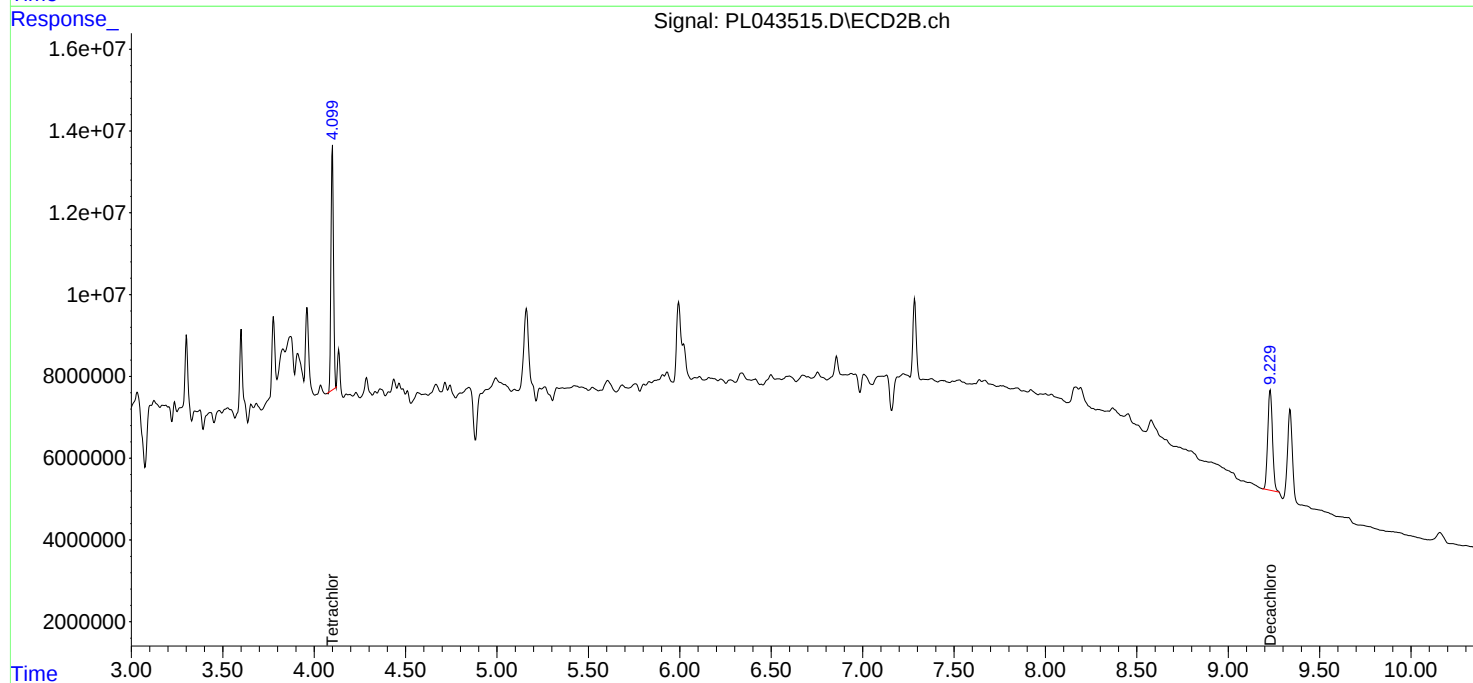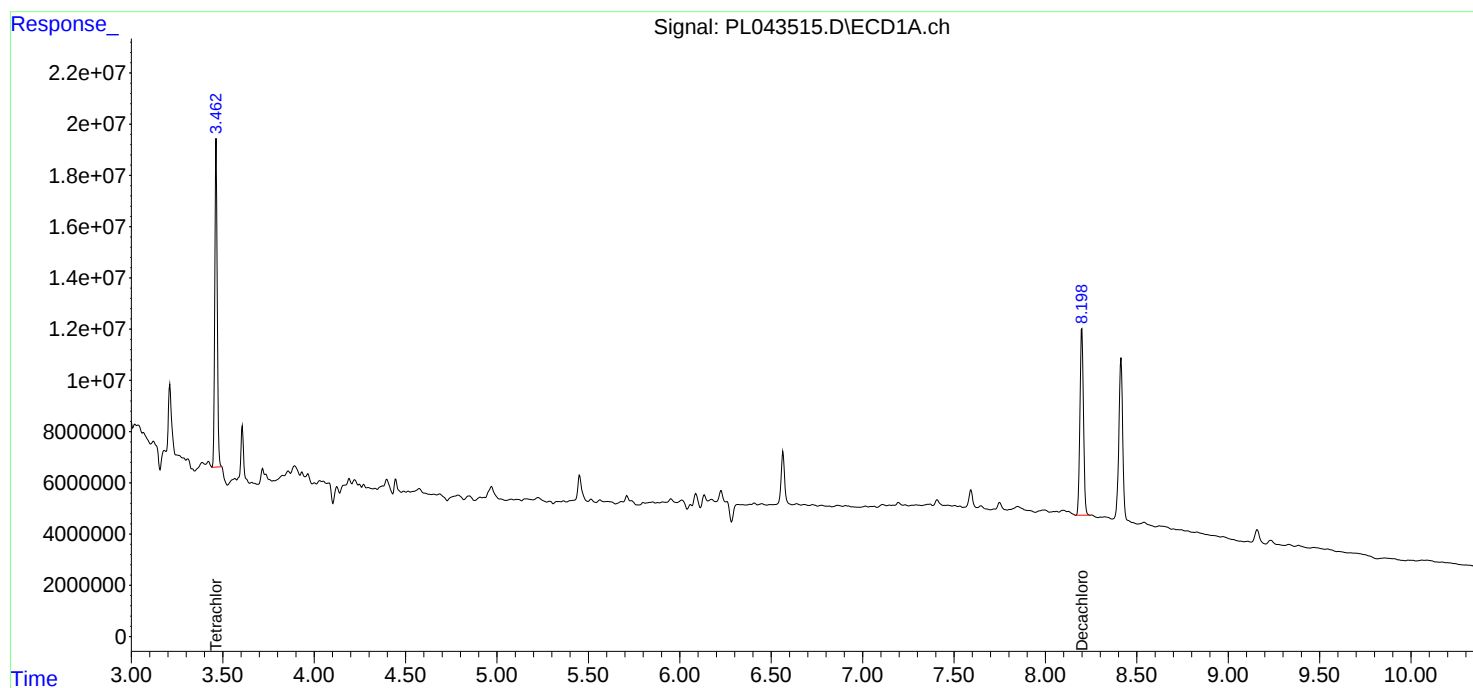

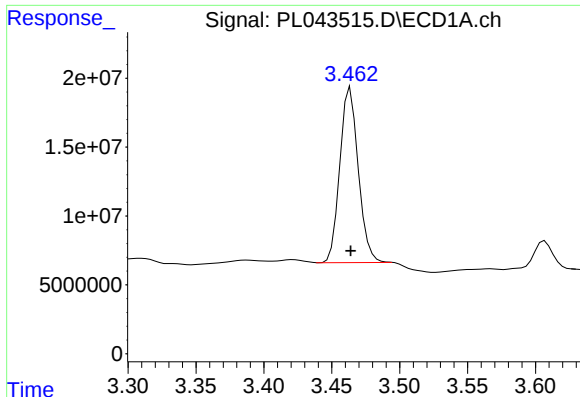


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: -0.002 min
Response: 120138144
Conc: 19.59 ng/ml m

Instrument :
ECD_L
ClientSampleId :
RECLAIMER-PIT


Manual Integrations
APPROVED

Sohil
1/2/2019 8:47:25 AM

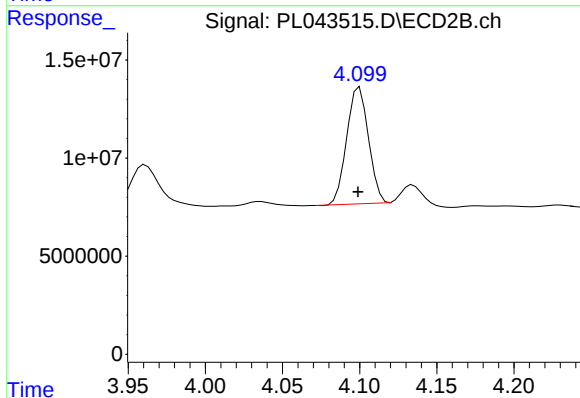


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 58140568
Conc: 19.62 ng/ml

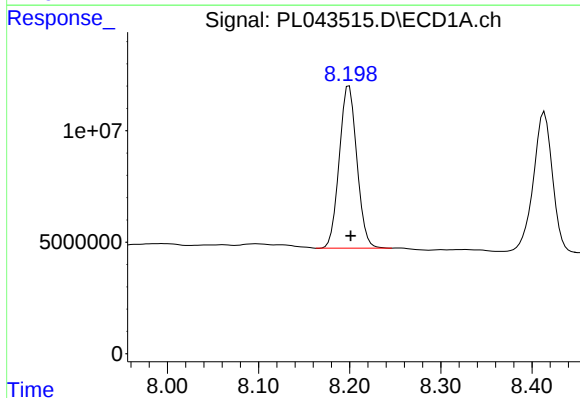

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: -0.002 min
Response: 97597797
Conc: 14.95 ng/ml

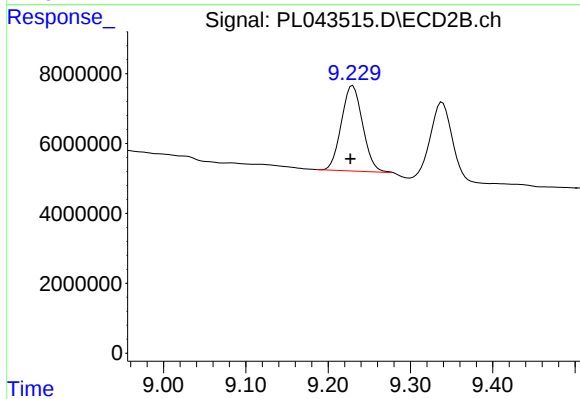

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.003 min
Response: 43663427
Conc: 16.74 ng/ml