

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122821\
 Data File : PL071691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 09:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 15:17:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.563	5.499	11608178	27630763	17.892	16.192
28)	SA Decachlor...	10.325	11.393	14828970	22242014	19.919	17.747
Target Compounds							
5)	MB Aldrin	0.000	7.506	0	25342	N.D.	0.012 #
7)	B delta-BHC	0.000	6.976f	0	99577	N.D.	0.047 #
8)	B Heptachlo...	0.000	7.970	0	1309953	N.D.	0.666 #
10)	B gamma-Chl...	0.000	8.236	0	504333	N.D.	0.259 #
13)	MA Dieldrin	7.699	0.000	44234	0	0.054	N.D. #
14)	MA Endrin	8.006f	0.000	438443	0	0.589	N.D. #
15)	B Endosulfa...	0.000	9.108f	0	528618	N.D.	0.356 #
16)	A 4,4'-DDD	0.000	9.011f	0	659909	N.D.	0.508 #
18)	B Endrin al...	0.000	9.286f	0	137689	N.D.	0.119 #
24)	Chlordane-2	0.000	7.473	0	38386	N.D.	0.521 #
25)	Chlordane-3	0.000	8.236	0	504333	N.D.	1.825 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122821\
Data File : PL071691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 09:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 15:17:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

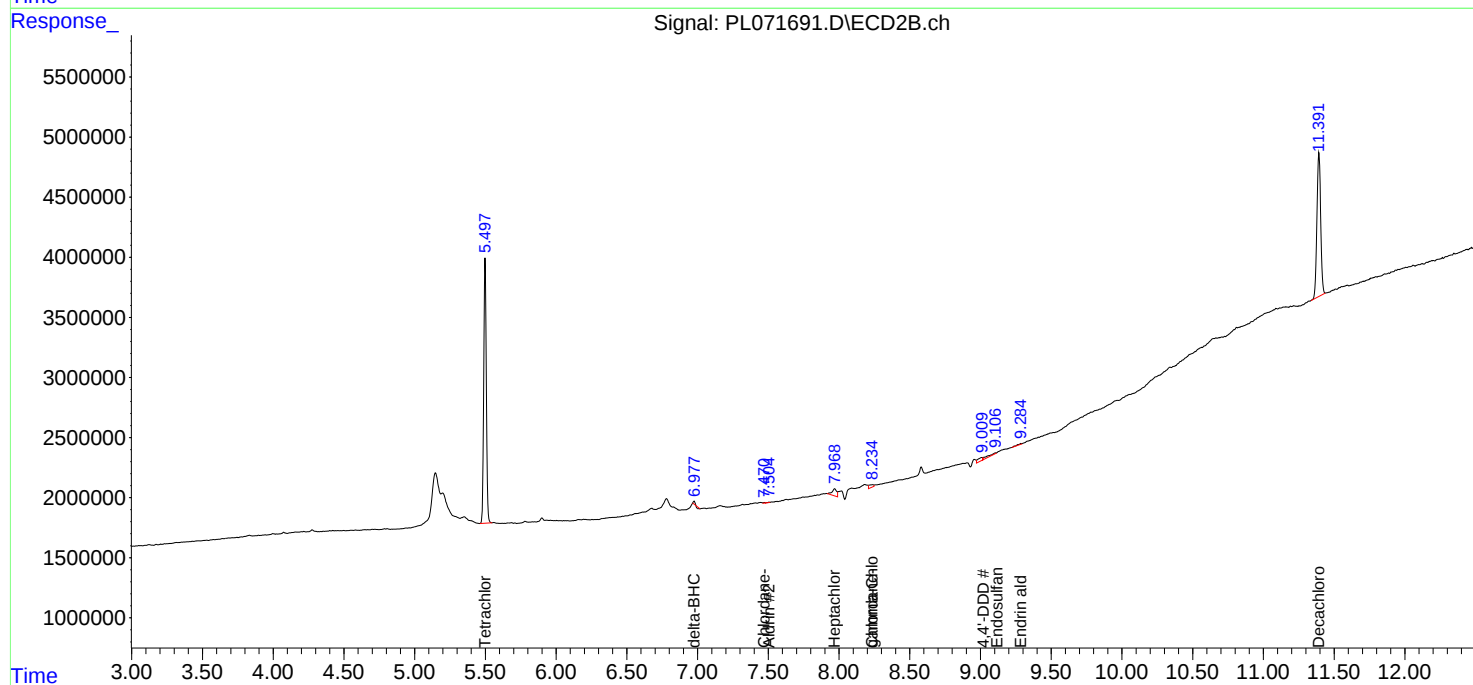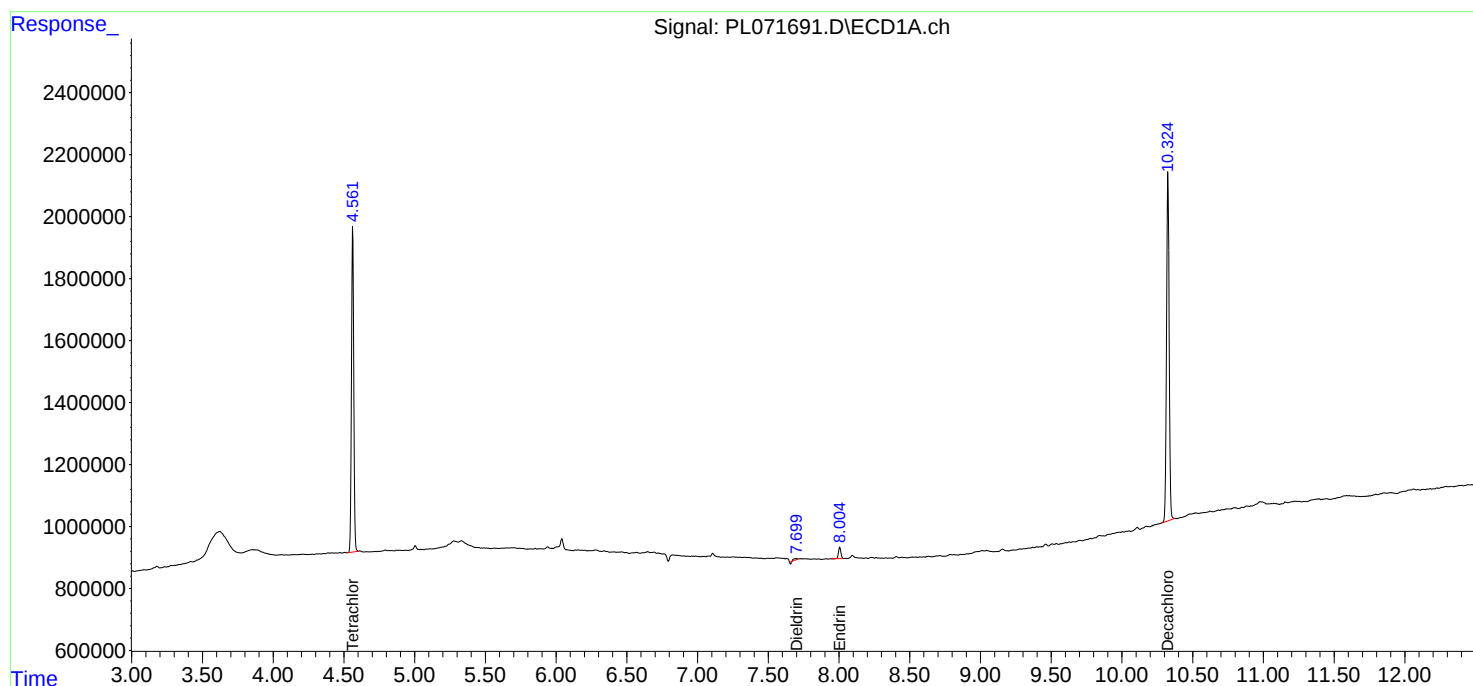


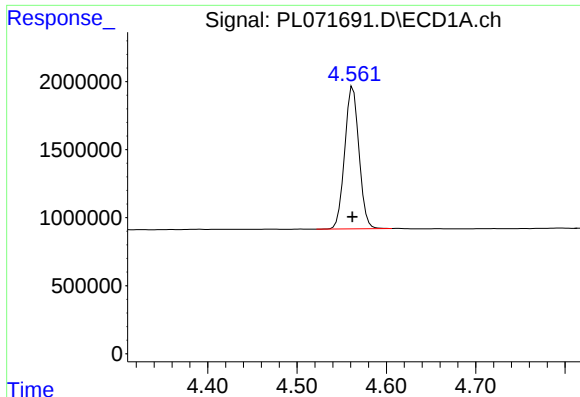

#1 Tetrachloro-m-xylene


R.T.: 4.563 min
Delta R.T.: 0.000 min
Response: 11608178
Conc: 17.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

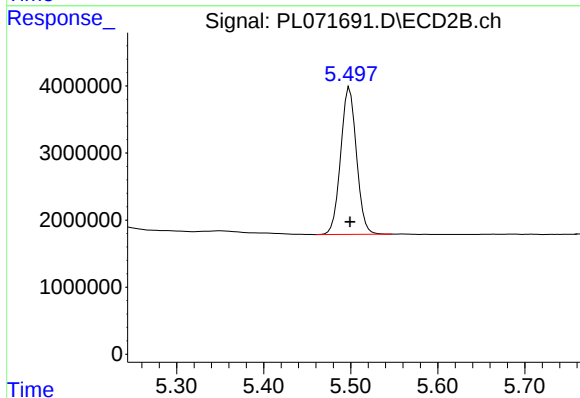


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 27630763
Conc: 16.19 ng/ml

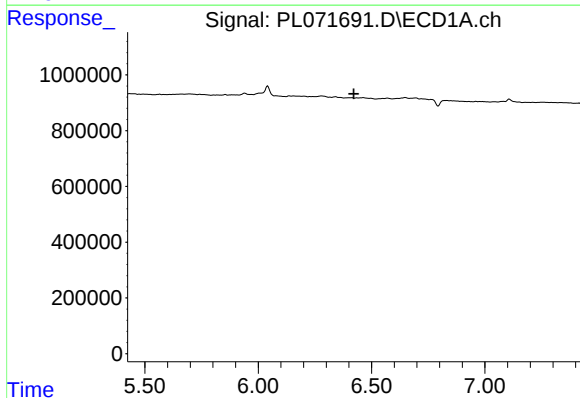


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

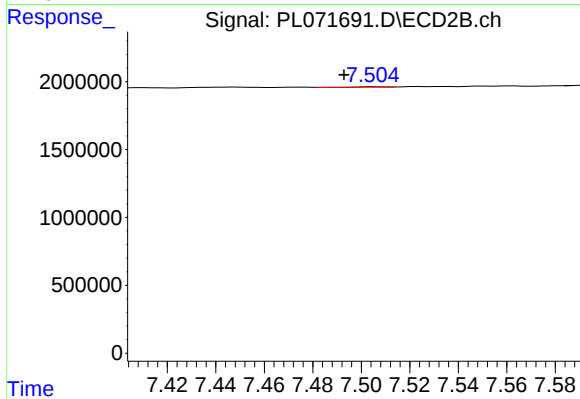

#5 Aldrin


R.T.: 7.506 min
Delta R.T.: 0.013 min
Response: 25342
Conc: 0.01 ng/ml

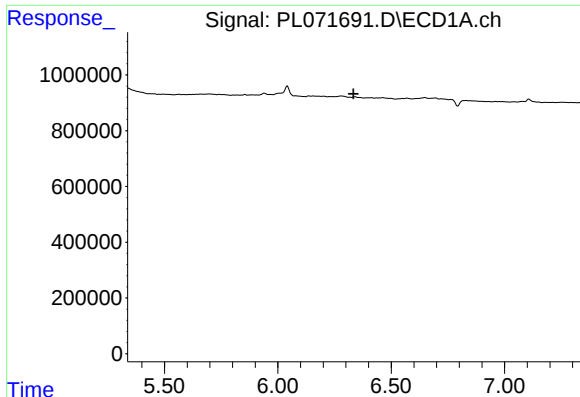

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

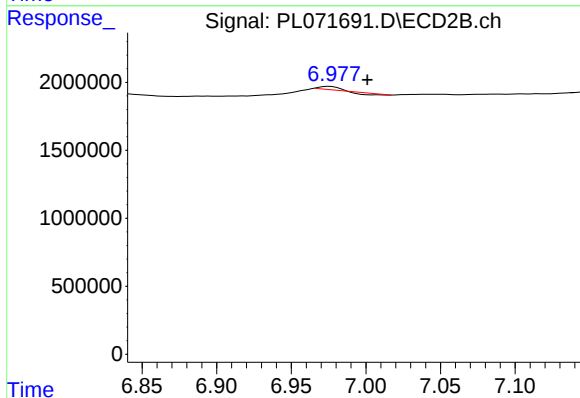


#7 delta-BHC

R.T.: 6.976 min
Delta R.T.: -0.025 min
Response: 99577
Conc: 0.05 ng/ml

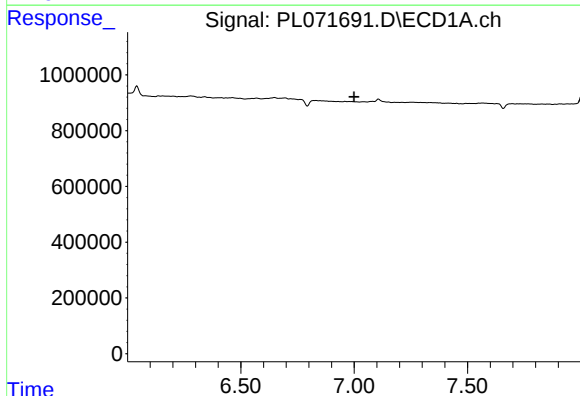


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

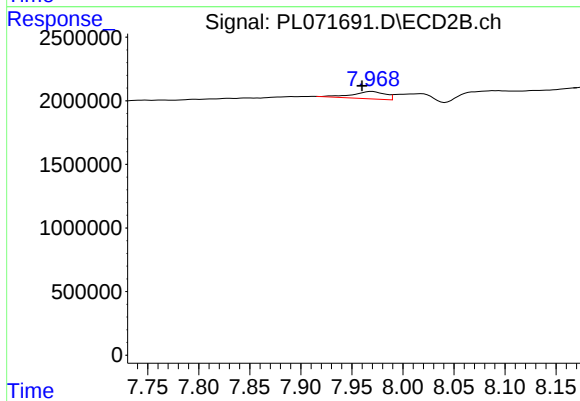

#8 Heptachlor epoxide


R.T.: 7.970 min
Delta R.T.: 0.009 min
Response: 1309953
Conc: 0.67 ng/ml

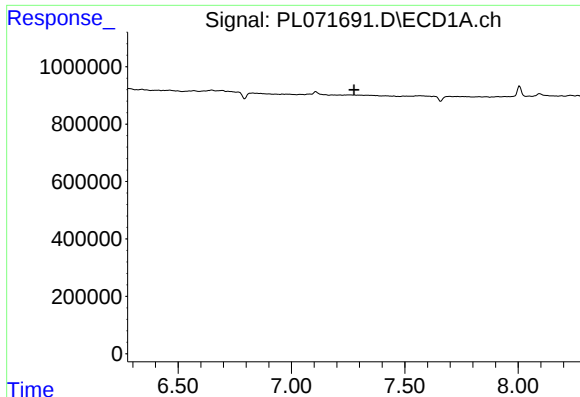

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

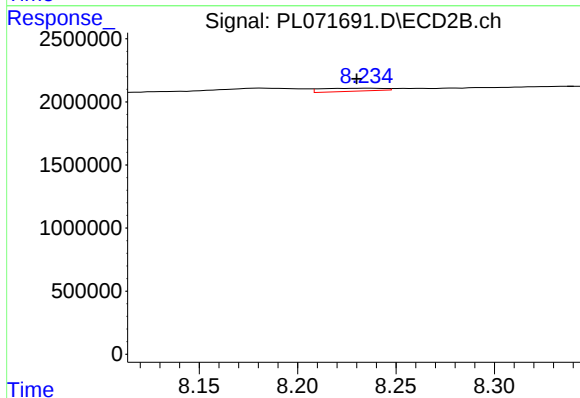


#10 gamma-Chlordane

R.T.: 8.236 min
Delta R.T.: 0.006 min
Response: 504333
Conc: 0.26 ng/ml

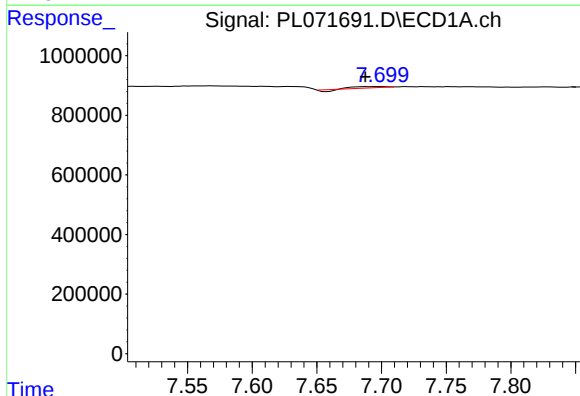


#13 Dieldrin

R.T.: 7.699 min
Delta R.T.: 0.012 min
Response: 44234
Conc: 0.05 ng/ml

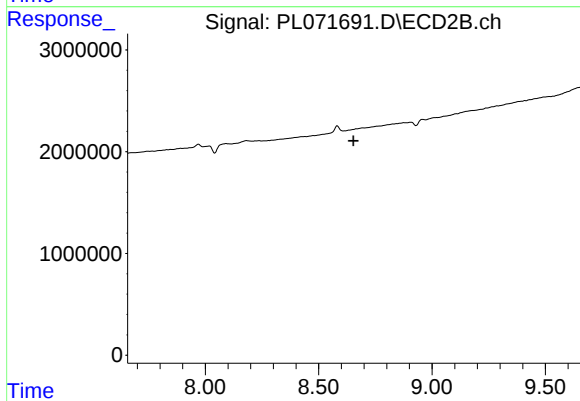

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.654 min
Response: 0
Conc: N.D.

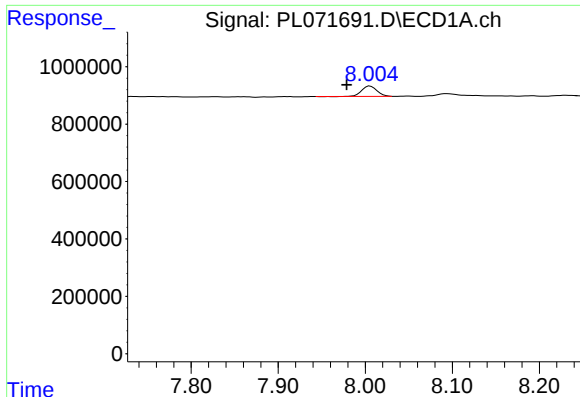

#14 Endrin


R.T.: 8.006 min
Delta R.T.: 0.027 min
Response: 438443
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

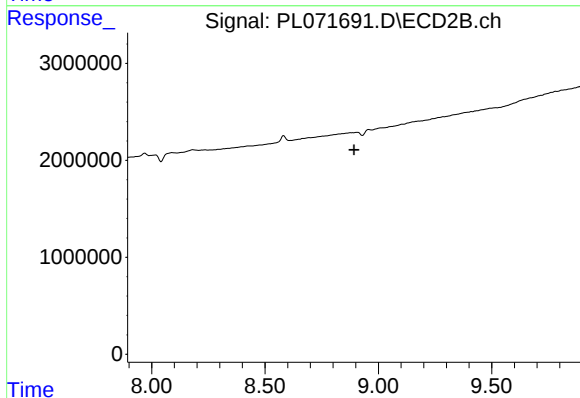


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

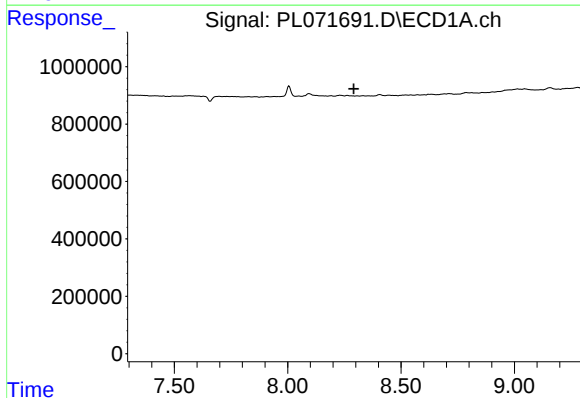


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.291 min
Response: 0
Conc: N.D.

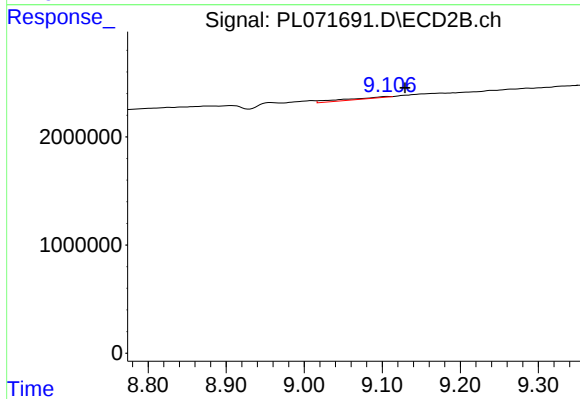

#15 Endosulfan II


R.T.: 9.108 min
Delta R.T.: -0.022 min
Response: 528618
Conc: 0.36 ng/ml

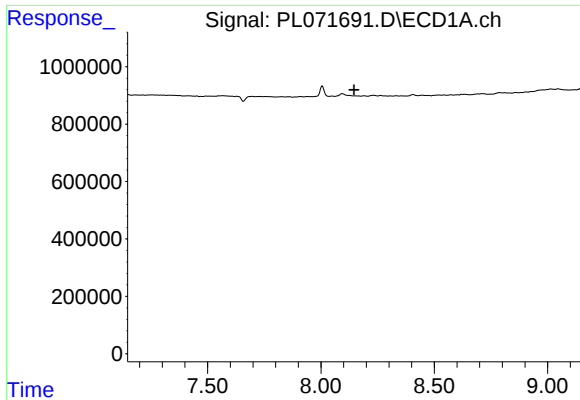

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

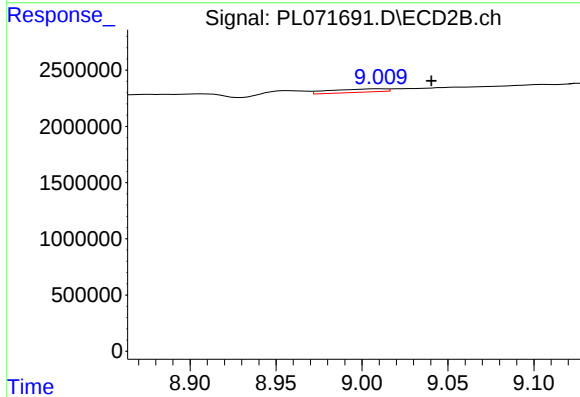


#16 4,4'-DDD

R.T.: 9.011 min
Delta R.T.: -0.029 min
Response: 659909
Conc: 0.51 ng/ml

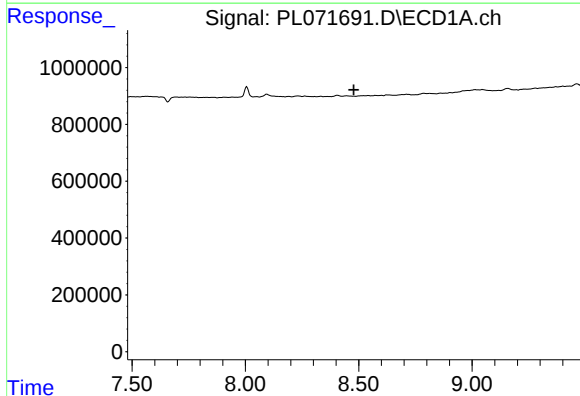


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

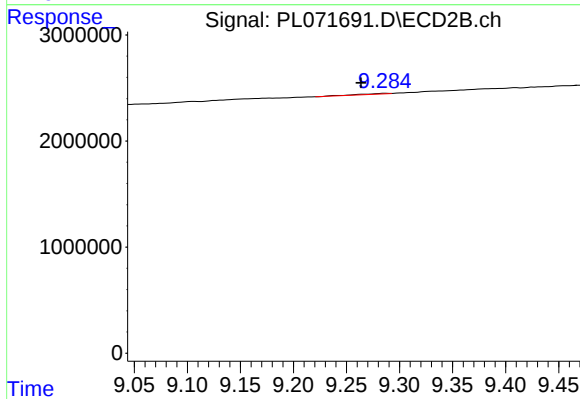

#18 Endrin aldehyde


R.T.: 9.286 min
Delta R.T.: 0.022 min
Response: 137689
Conc: 0.12 ng/ml

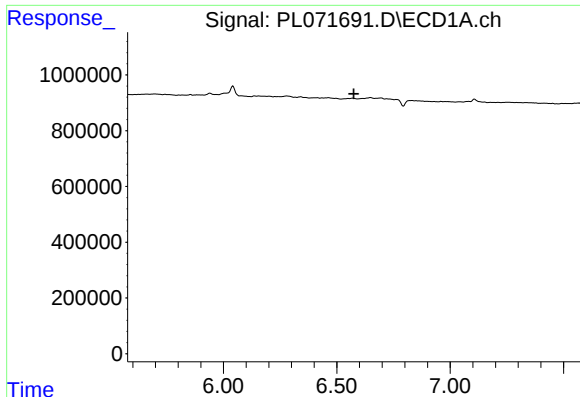

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

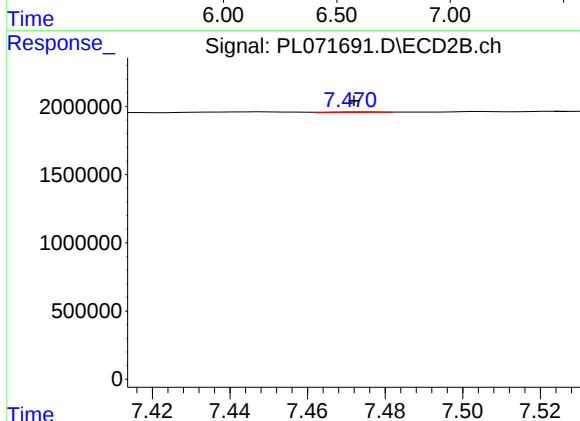


#24 Chlordane-2

R.T.: 7.473 min
Delta R.T.: 0.001 min
Response: 38386
Conc: 0.52 ng/ml

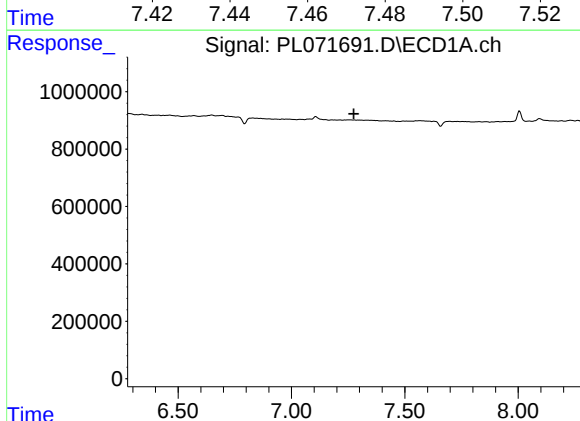


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

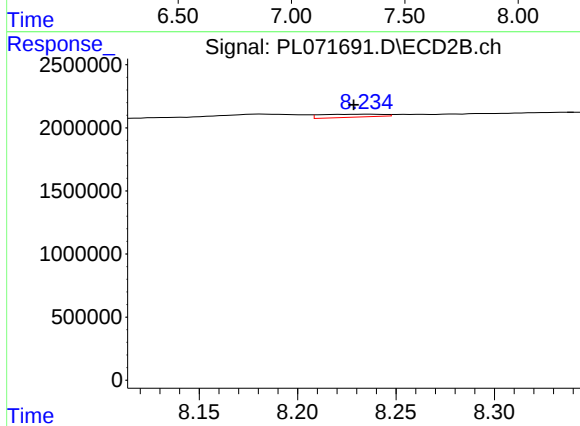

#25 Chlordane-3


R.T.: 8.236 min
Delta R.T.: 0.008 min
Response: 504333
Conc: 1.83 ng/ml

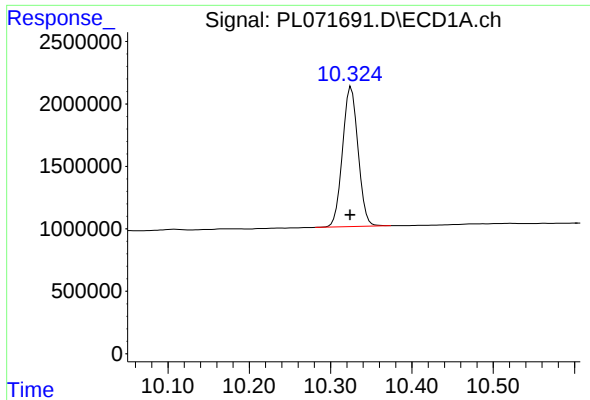

#28 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: 0.002 min
Response: 14828970
Conc: 19.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

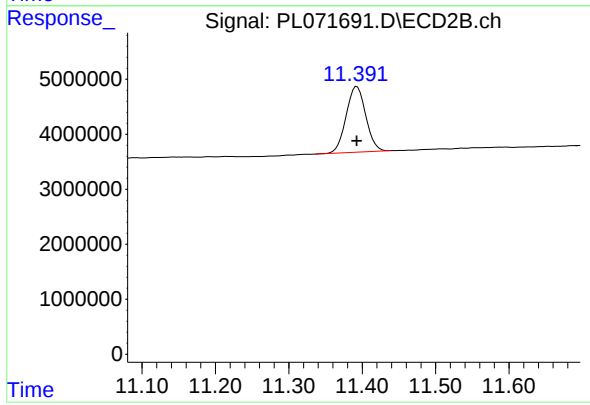

#28 Decachlorobiphenyl

R.T.: 11.393 min
Delta R.T.: 0.000 min
Response: 22242014
Conc: 17.75 ng/ml