

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 19:51
 Operator : AR\AJ
 Sample : CHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 00:18:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 00:16:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.674	310.0E6	165.2E6	104.856	107.402
28)	SA Decachlor...	8.982	7.864	270.4E6	125.0E6	99.097	99.832
Target Compounds							
23)	Chlordane-1	4.587	3.677	136.9E6	48637749	1052.464	1068.962
24)	Chlordane-2	5.123	4.259	142.1E6	55284006	1006.774	1031.444
25)	Chlordane-3	5.837	4.894	583.9E6	172.4E6	1078.206	1096.731
26)	Chlordane-4	5.920	4.957	705.1E6	180.6E6	1050.823	1079.078
27)	Chlordane-5	6.773	5.631	114.5E6	48377602	1049.649	1051.406



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 19:51
Operator : AR\AJ
Sample : CHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 00:18:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 00:16:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

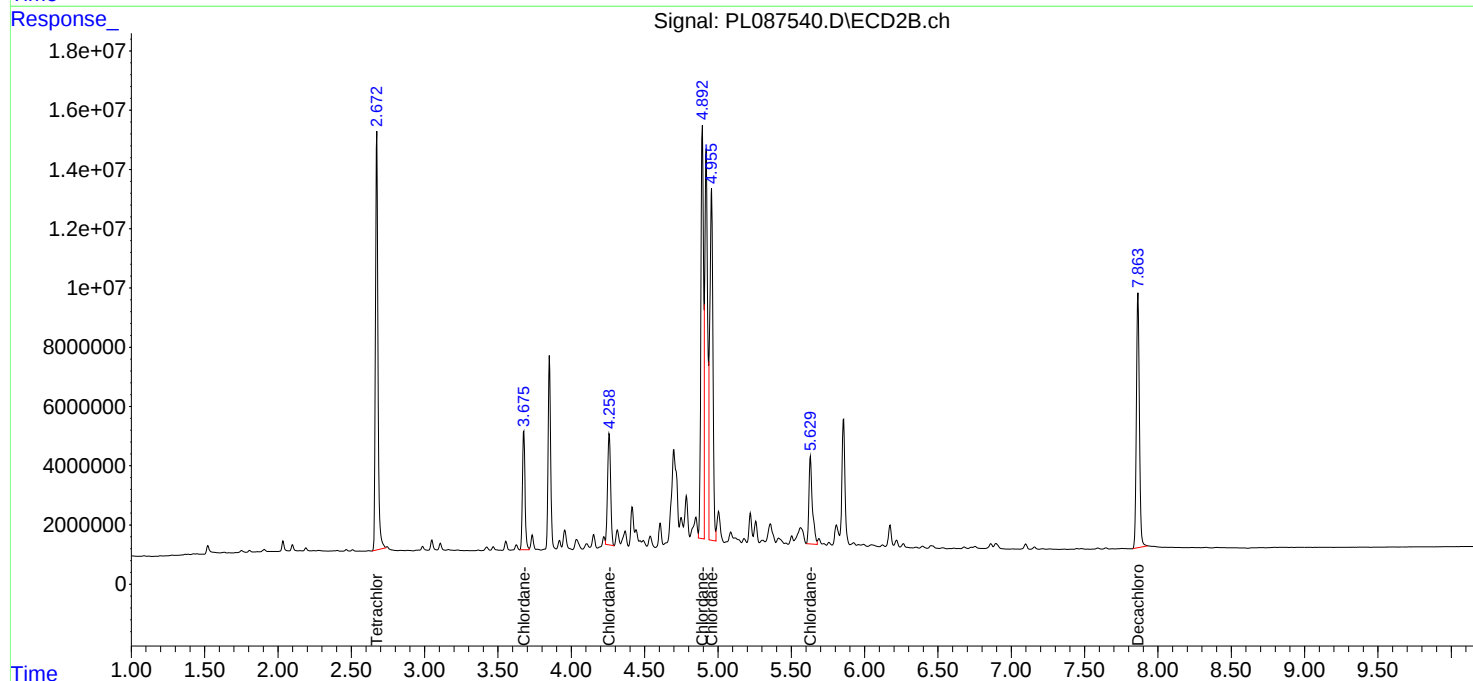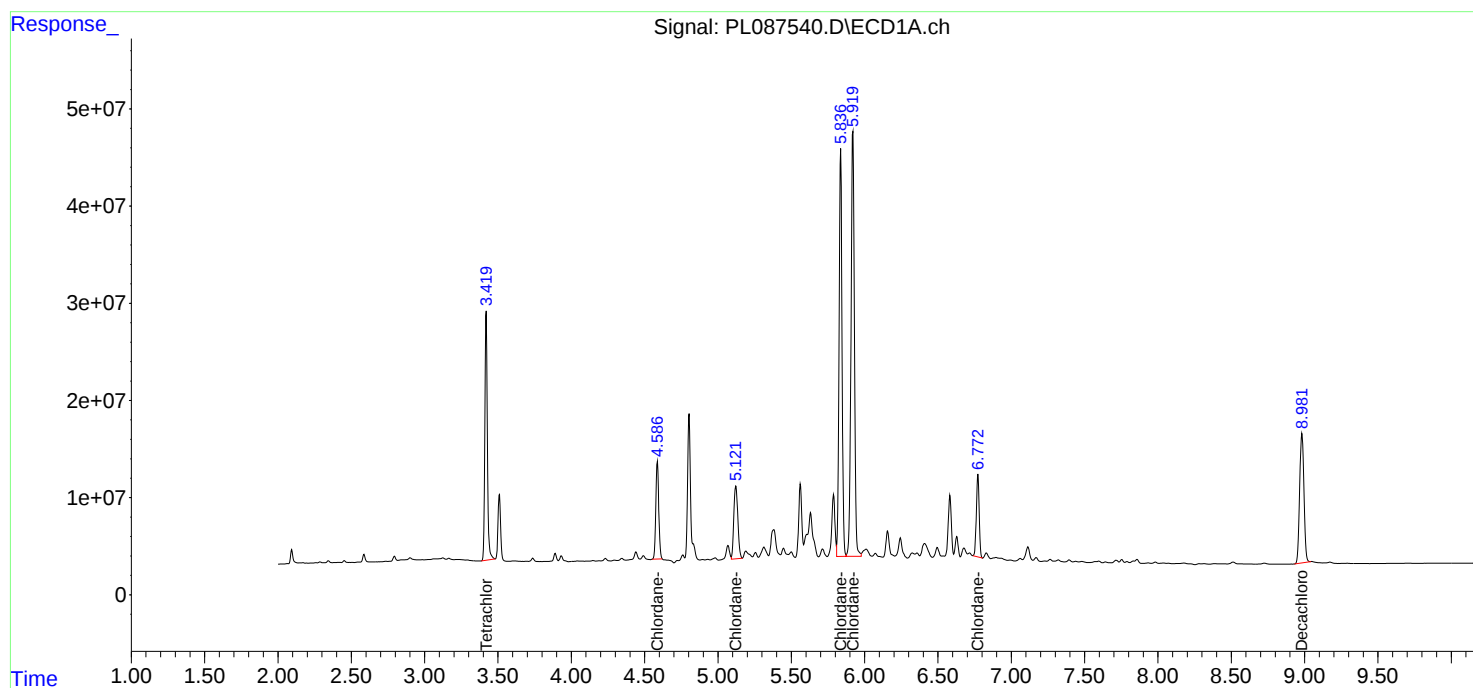


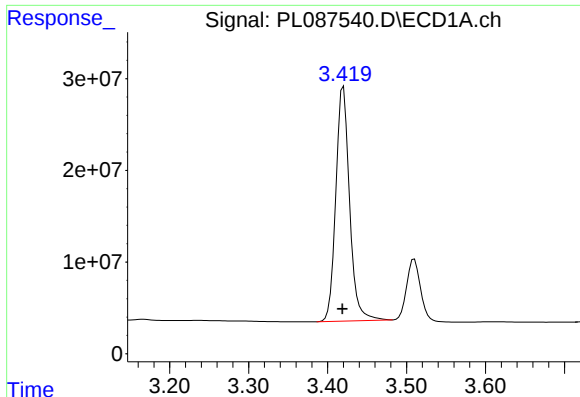

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.001 min
Response: 309950413
Conc: 104.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

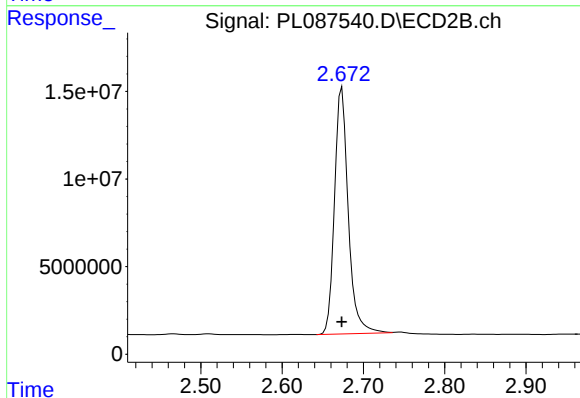


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: 0.000 min
Response: 165199209
Conc: 107.40 ng/ml

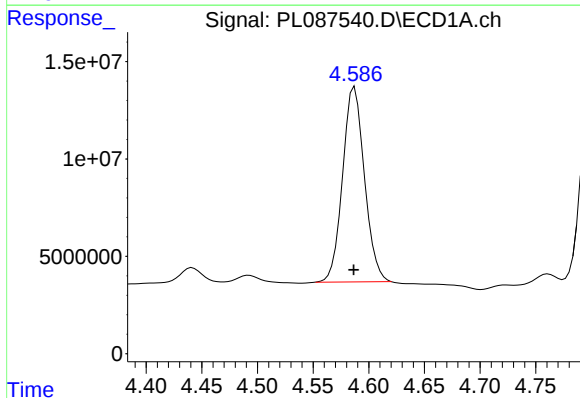


#23 Chlordane-1

R.T.: 4.587 min
Delta R.T.: 0.000 min
Response: 136897286
Conc: 1052.46 ng/ml

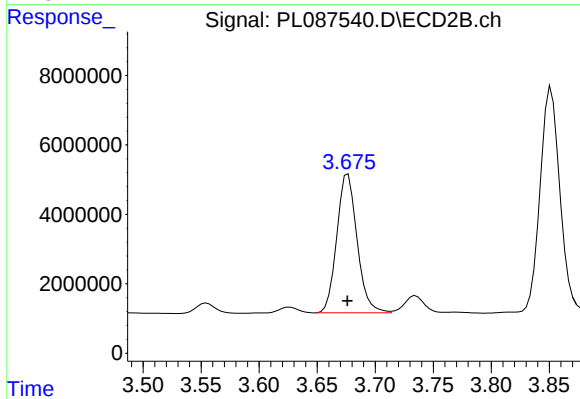

#23 Chlordane-1


R.T.: 3.677 min
Delta R.T.: 0.000 min
Response: 48637749
Conc: 1068.96 ng/ml

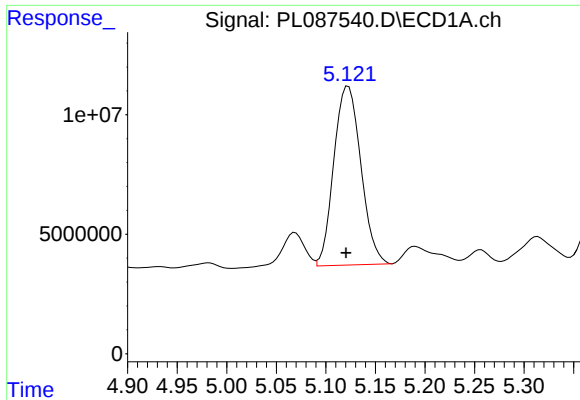

#24 Chlordane-2


R.T.: 5.123 min
Delta R.T.: 0.002 min
Response: 142051094
Conc: 1006.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

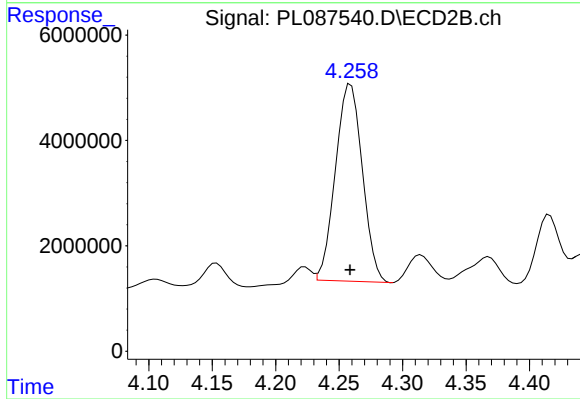


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 55284006
Conc: 1031.44 ng/ml

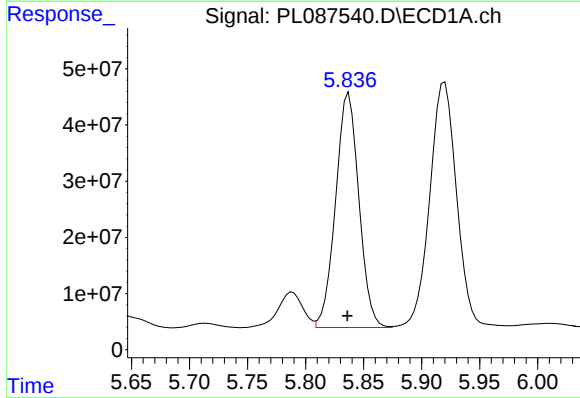


#25 Chlordane-3

R.T.: 5.837 min
Delta R.T.: 0.001 min
Response: 583918292
Conc: 1078.21 ng/ml

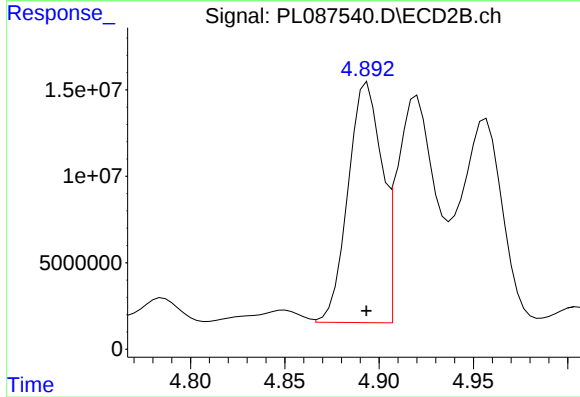

#25 Chlordane-3


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 172435128
Conc: 1096.73 ng/ml

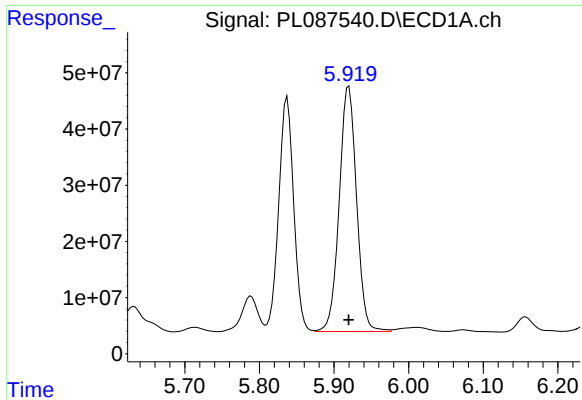

#26 Chlordane-4


R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 705050079
Conc: 1050.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

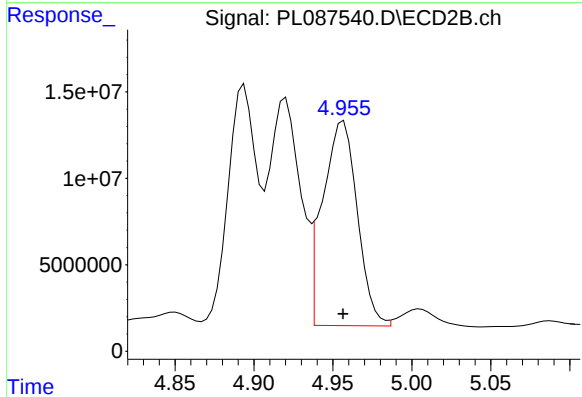


#26 Chlordane-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 180587679
Conc: 1079.08 ng/ml

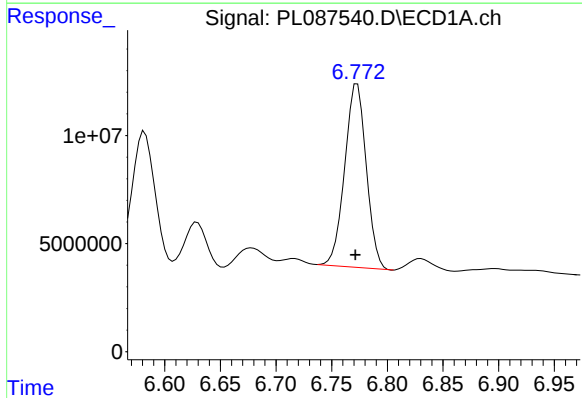


#27 Chlordane-5

R.T.: 6.773 min
Delta R.T.: 0.002 min
Response: 114461661
Conc: 1049.65 ng/ml

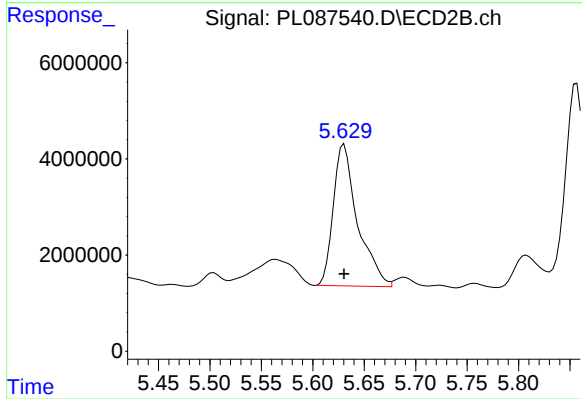

#27 Chlordane-5


R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 48377602
Conc: 1051.41 ng/ml

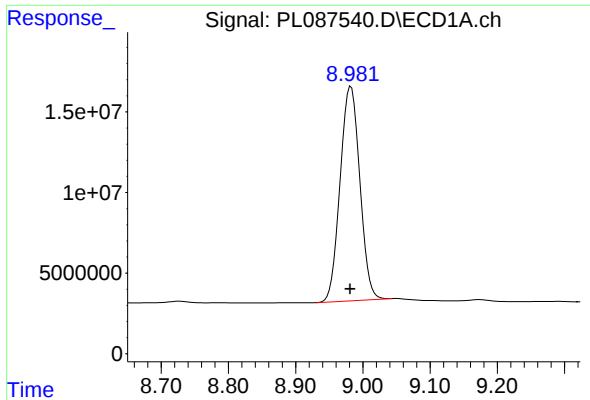

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.001 min
Response: 270418308
Conc: 99.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

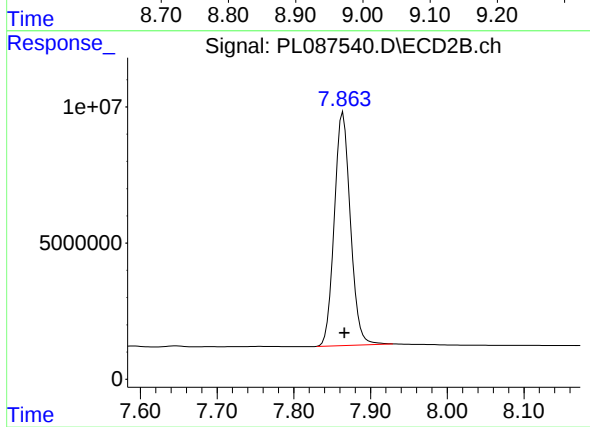

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: -0.001 min
Response: 125038344
Conc: 99.83 ng/ml