

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 22:24
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL122823CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 00:19:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 00:16:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.674	147.1E6	76789814	49.755	49.924
28)	SA Decachlor...	8.981	7.865	138.3E6	63499209	50.695	50.698
Target Compounds							
23)	Chlordane-1	4.587	3.676	65651978	22835943	504.731	501.889
24)	Chlordane-2	5.121	4.259	71423737	27207491	506.209	507.615
25)	Chlordane-3	5.836	4.893	275.2E6	78807191	508.147	501.234
26)	Chlordane-4	5.920	4.956	337.9E6	82929093	503.560	495.532
27)	Chlordane-5	6.773	5.630	55643997	24751267	510.273	537.927



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 22:24
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL122823CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 00:19:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 00:16:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

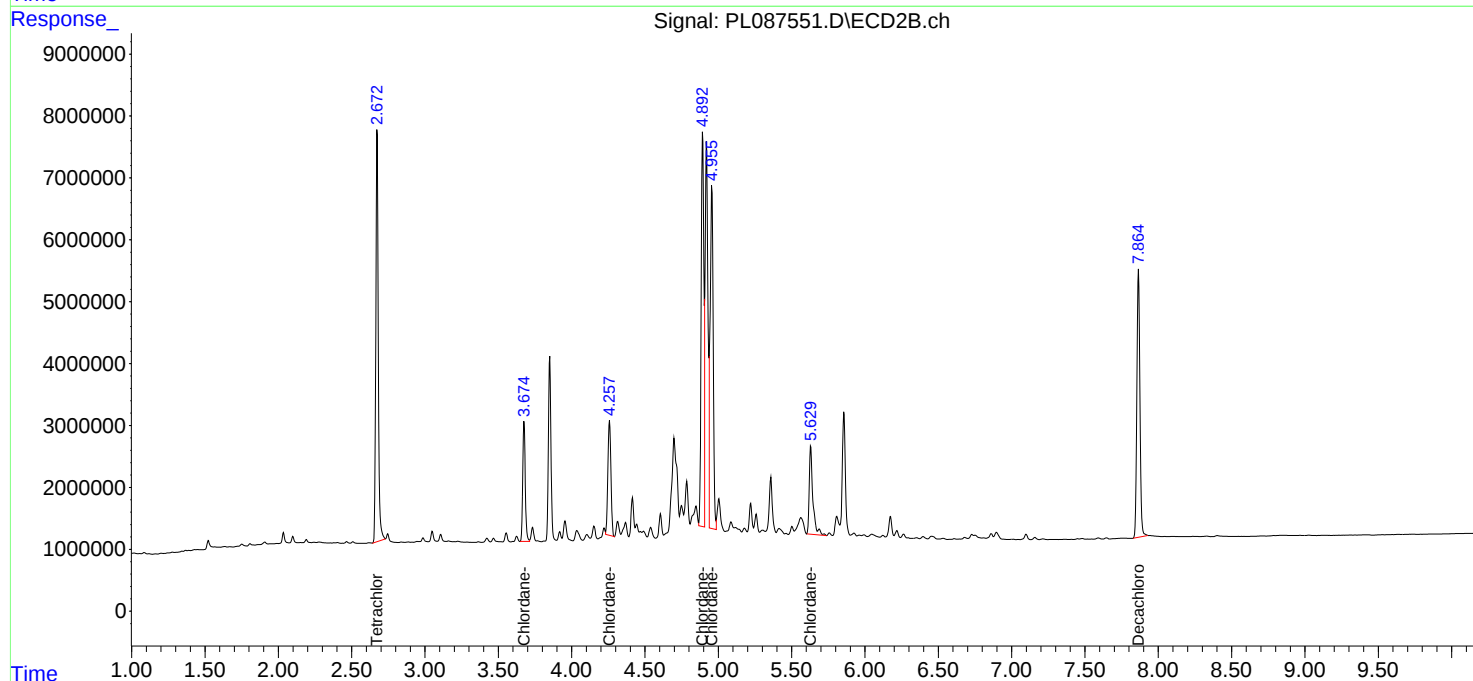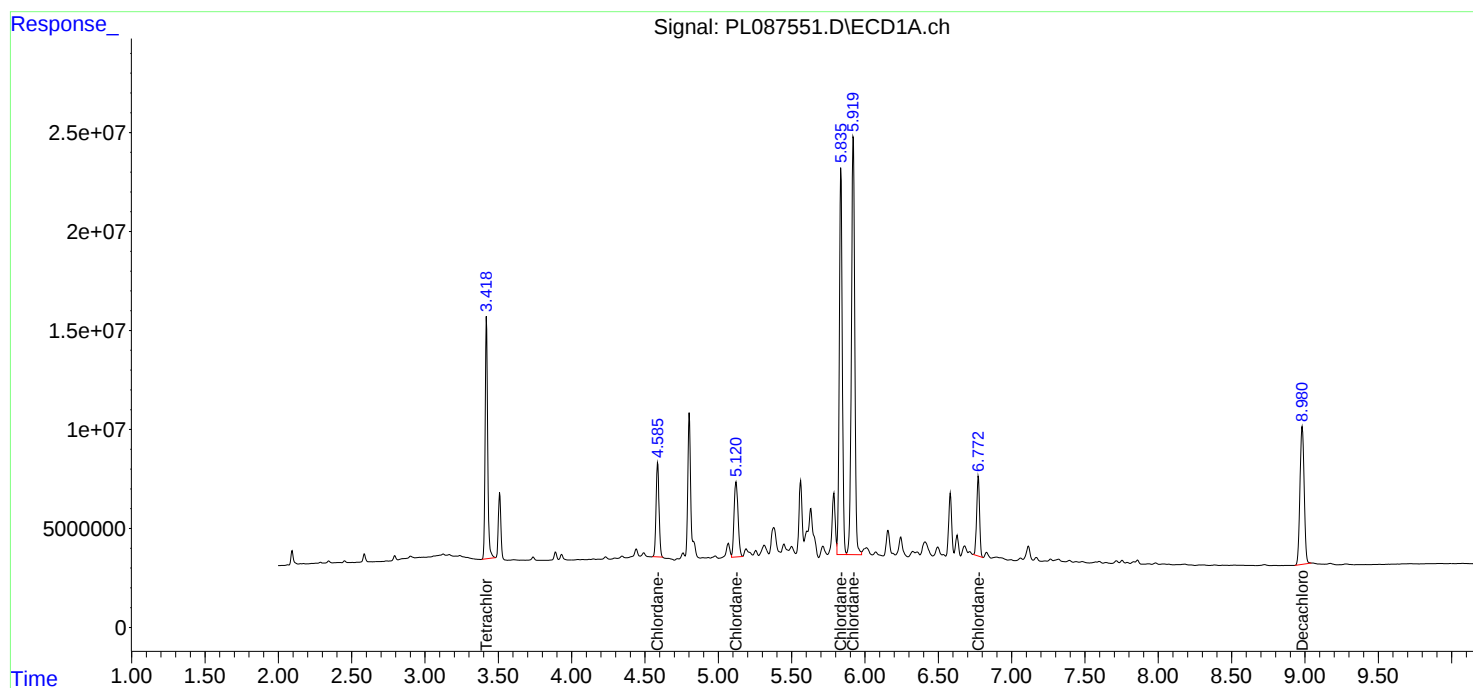


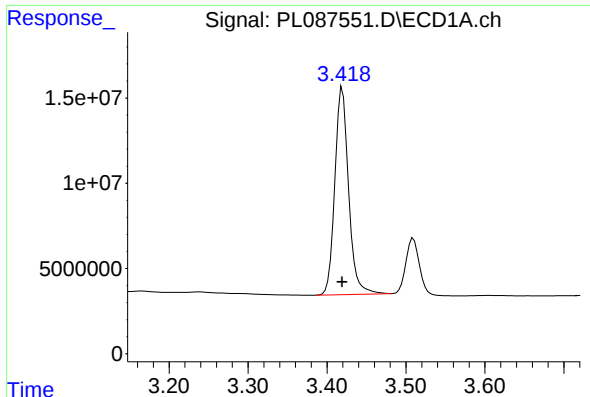

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 147075137
Conc: 49.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122823CHLOR

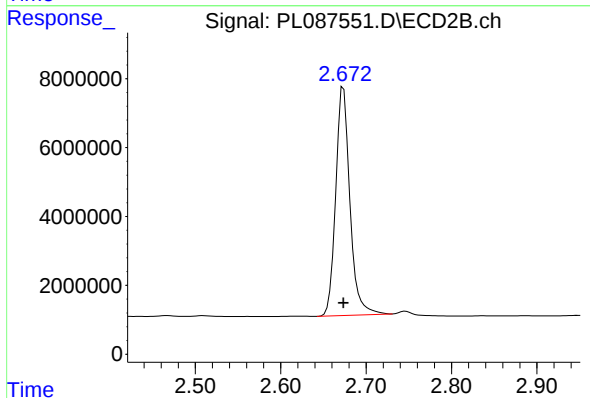


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: 0.000 min
Response: 76789814
Conc: 49.92 ng/ml

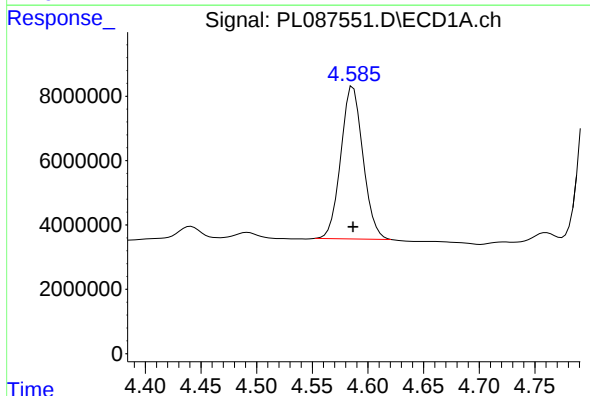


#23 Chlordane-1

R.T.: 4.587 min
Delta R.T.: 0.000 min
Response: 65651978
Conc: 504.73 ng/ml

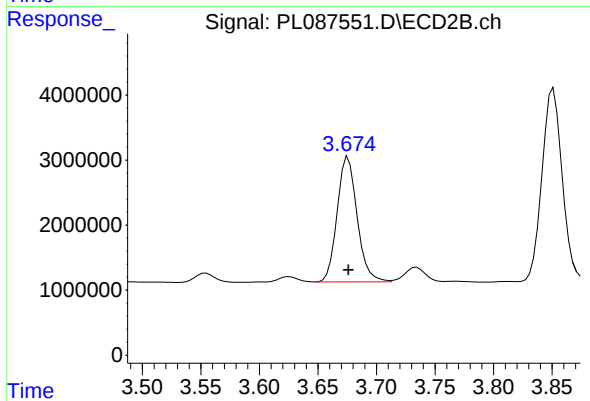

#23 Chlordane-1


R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 22835943
Conc: 501.89 ng/ml

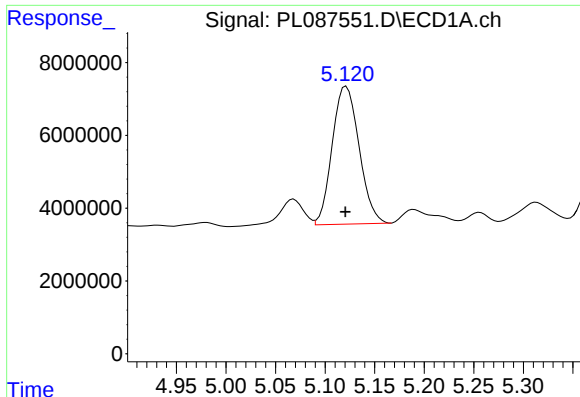

#24 Chlordane-2


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 71423737
Conc: 506.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122823CHLOR

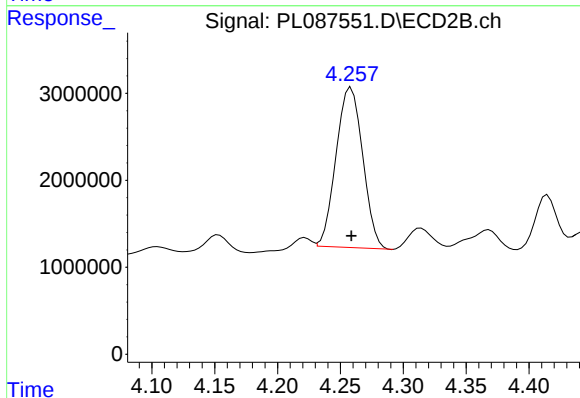


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 27207491
Conc: 507.62 ng/ml

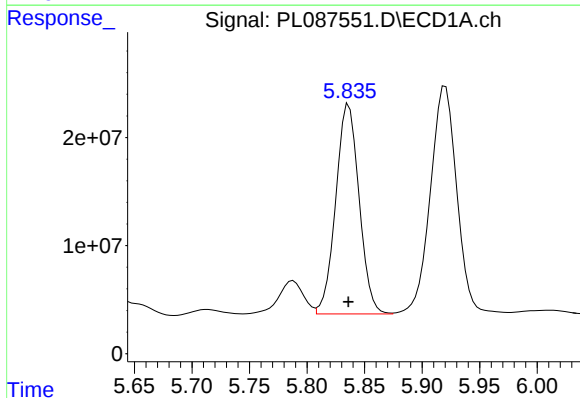


#25 Chlordane-3

R.T.: 5.836 min
Delta R.T.: 0.000 min
Response: 275194611
Conc: 508.15 ng/ml

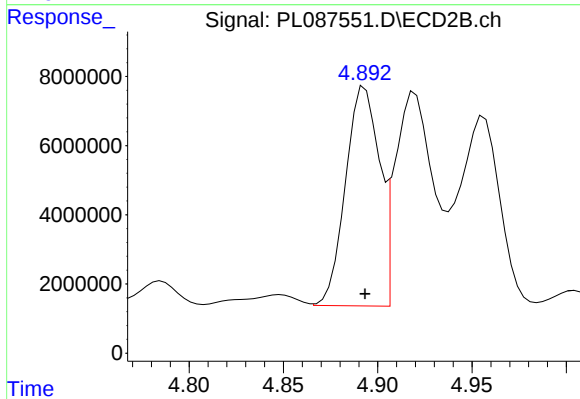

#25 Chlordane-3


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 78807191
Conc: 501.23 ng/ml

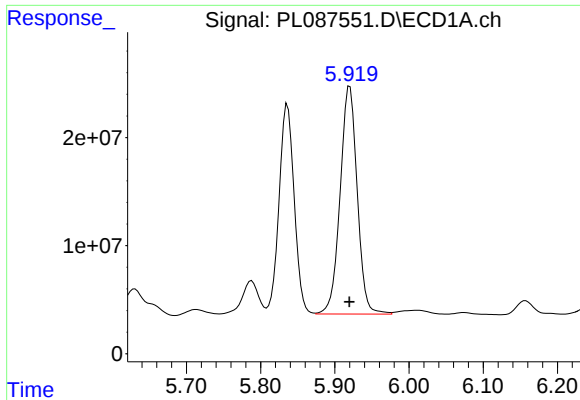

#26 Chlordane-4


R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 337863582
Conc: 503.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122823CHLOR

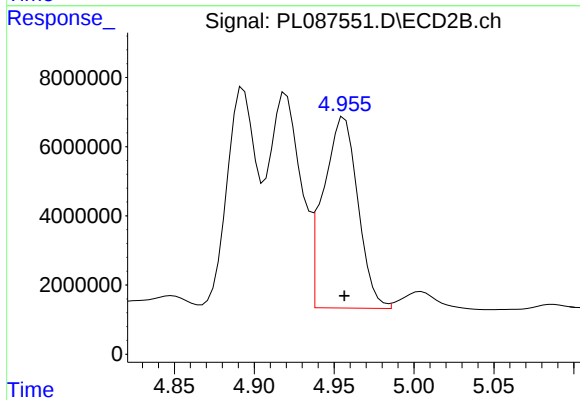


#26 Chlordane-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 82929093
Conc: 495.53 ng/ml

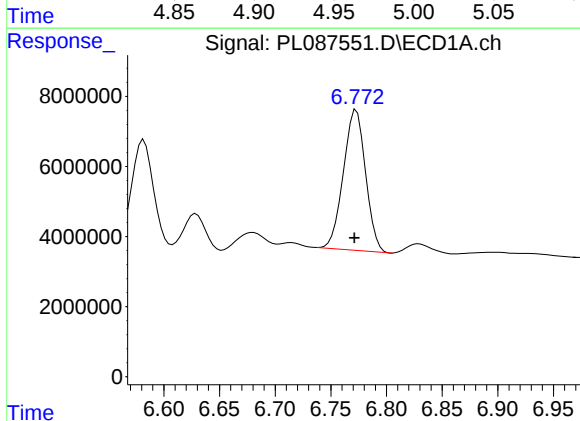


#27 Chlordane-5

R.T.: 6.773 min
Delta R.T.: 0.002 min
Response: 55643997
Conc: 510.27 ng/ml

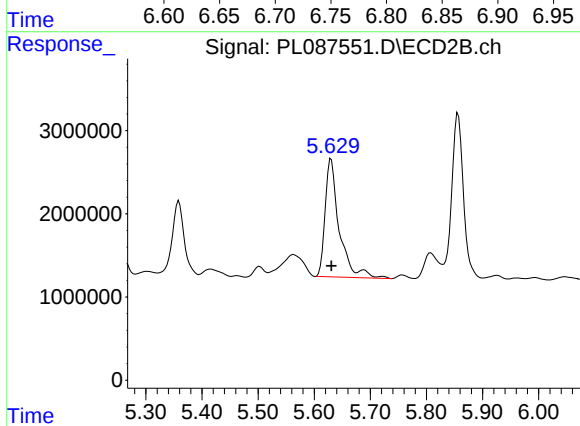

#27 Chlordane-5

R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 24751267
Conc: 537.93 ng/ml

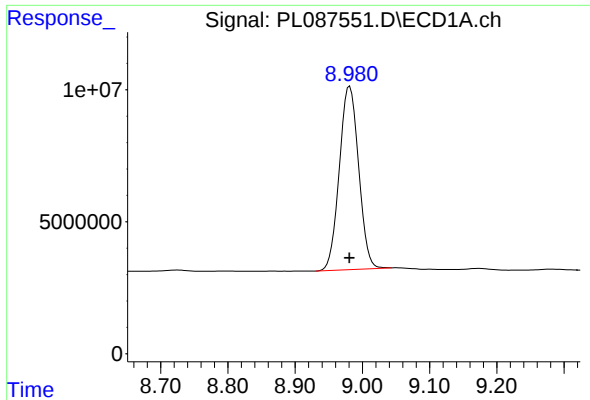

#28 Decachlorobiphenyl


R.T.: 8.981 min

Delta R.T.: 0.000 min

Response: 138336531

Conc: 50.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122823CHLOR

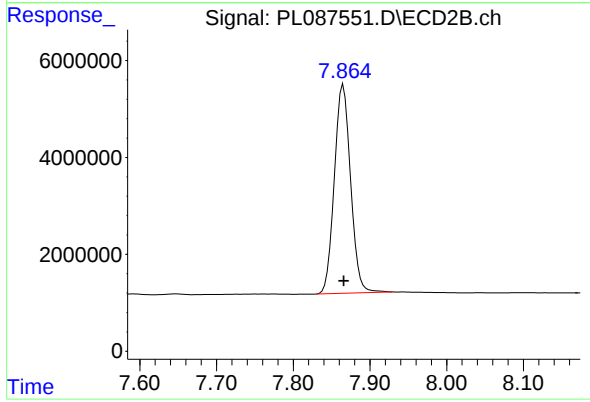

#28 Decachlorobiphenyl

R.T.: 7.865 min

Delta R.T.: 0.000 min

Response: 63499209

Conc: 50.70 ng/ml