

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 19:51
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 00:31:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 00:31:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.674	310.0E6	165.2E6	102.370	103.569
28)	SA Decachlor...	8.982	7.864	270.4E6	124.4E6	99.546	99.994
Target Compounds							
23)	Chlordane-1	4.587	3.677	136.9E6	48637749	1025.562	1033.332
24)	Chlordane-2	5.123	4.259	142.1E6	55284006	1003.375	1015.479
25)	Chlordane-3	5.837	4.894	583.9E6	172.4E6	1037.631	1046.134
26)	Chlordane-4	5.920	4.957	705.1E6	180.6E6	1024.782	1038.035
27)	Chlordane-5	6.773	5.631	114.5E6	48377602	1022.564	1025.059



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 19:51
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 00:31:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 00:31:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

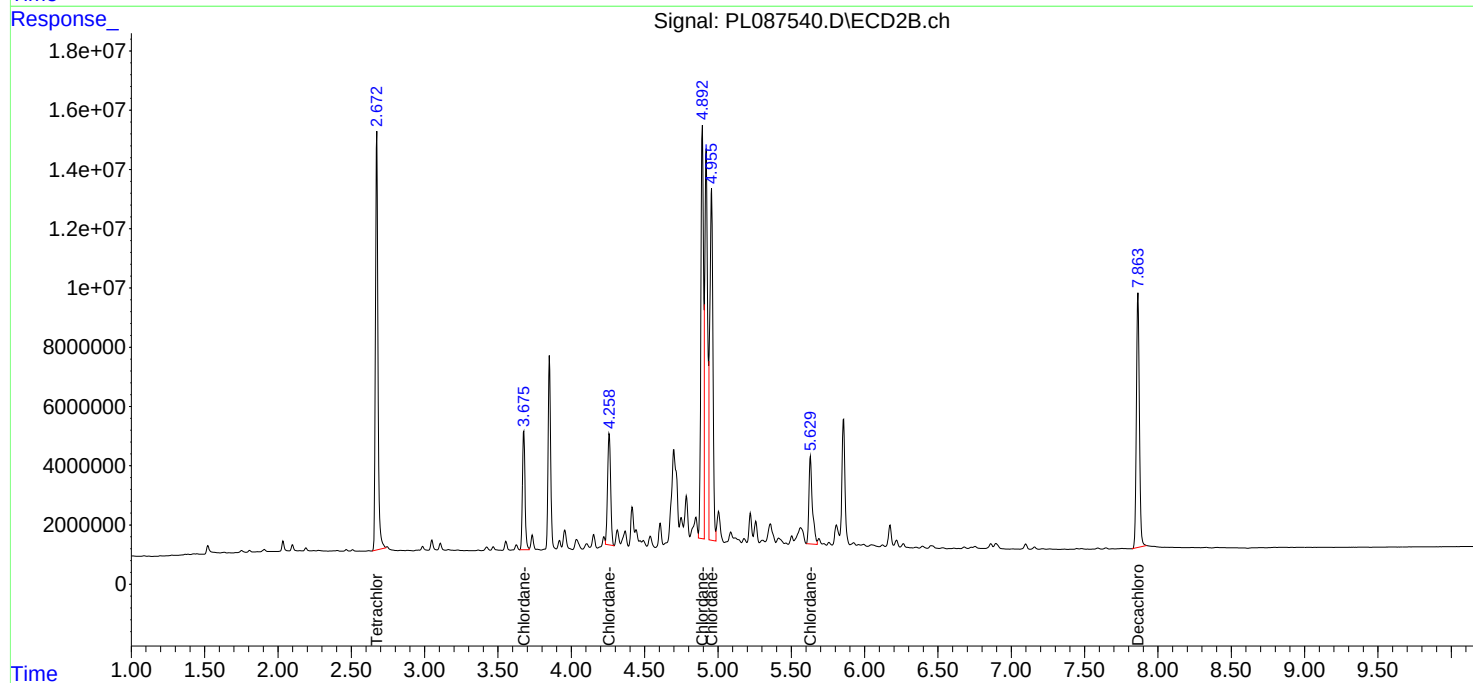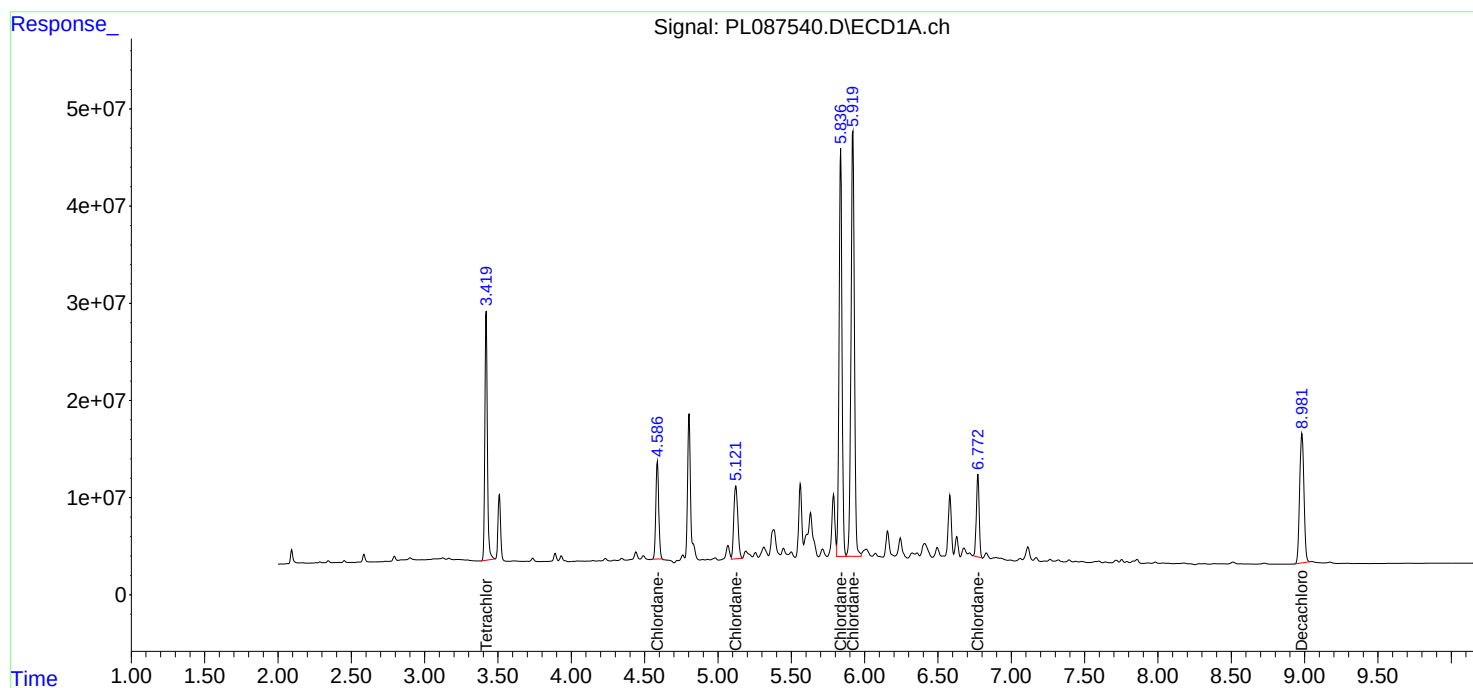


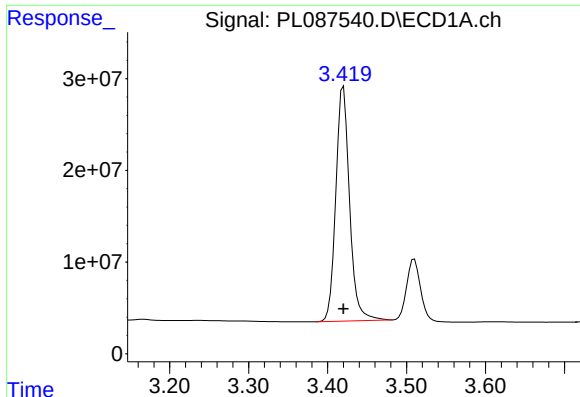

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 309950413
Conc: 102.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

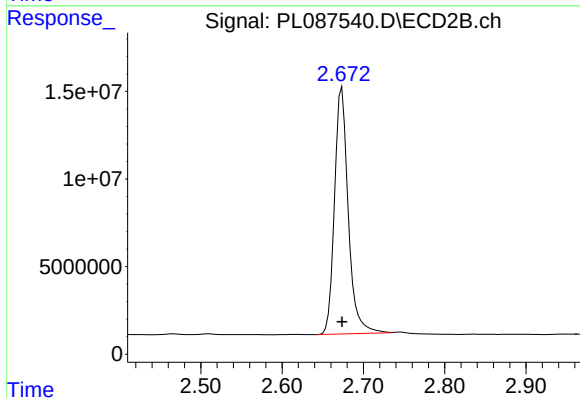


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: 0.000 min
Response: 165199209
Conc: 103.57 ng/ml

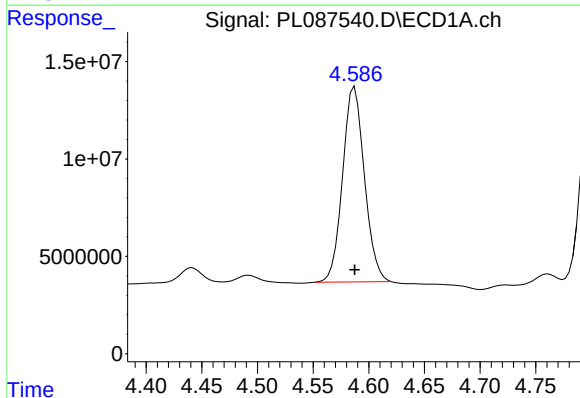


#23 Chlordane-1

R.T.: 4.587 min
Delta R.T.: 0.000 min
Response: 136897286
Conc: 1025.56 ng/ml

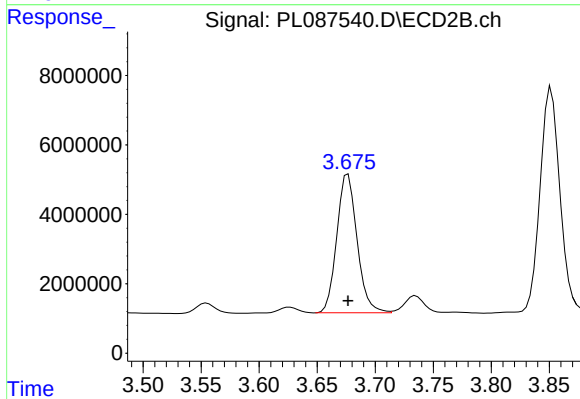

#23 Chlordane-1


R.T.: 3.677 min
Delta R.T.: 0.000 min
Response: 48637749
Conc: 1033.33 ng/ml

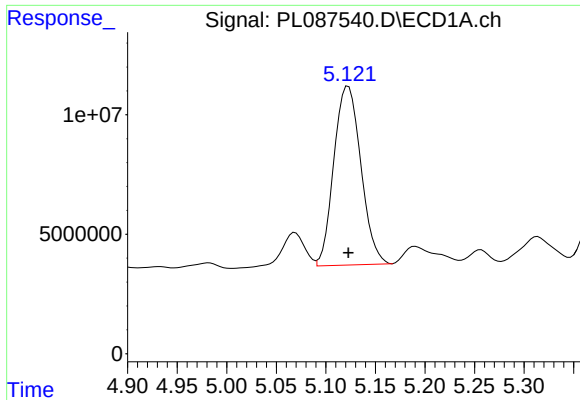

#24 Chlordane-2


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 142051094
Conc: 1003.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

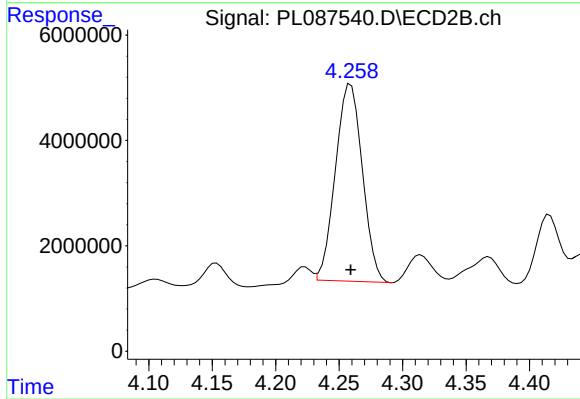


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 55284006
Conc: 1015.48 ng/ml

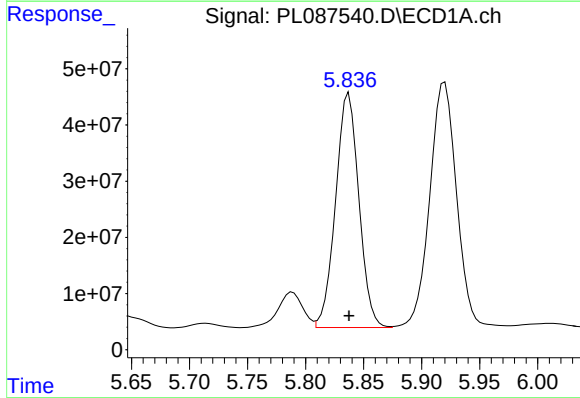


#25 Chlordane-3

R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 583918292
Conc: 1037.63 ng/ml

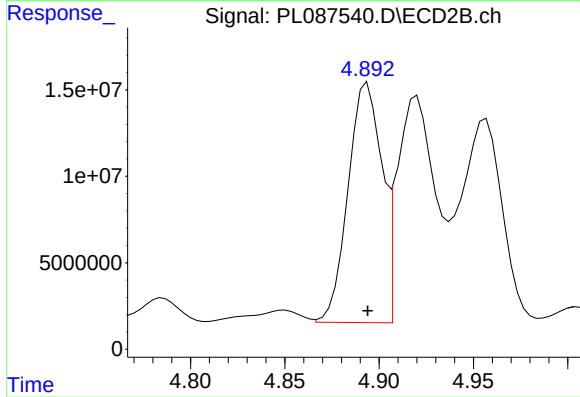

#25 Chlordane-3


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 172435128
Conc: 1046.13 ng/ml

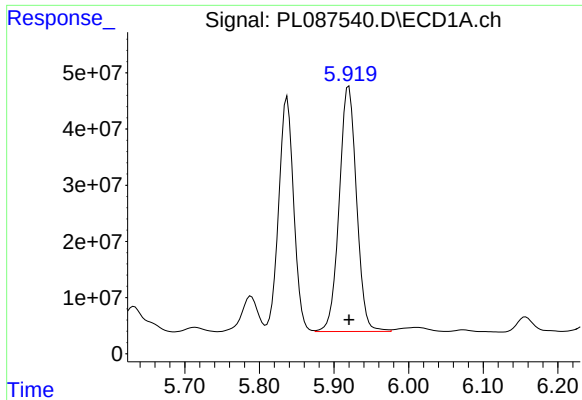

#26 Chlordane-4


R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 705050079
Conc: 1024.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

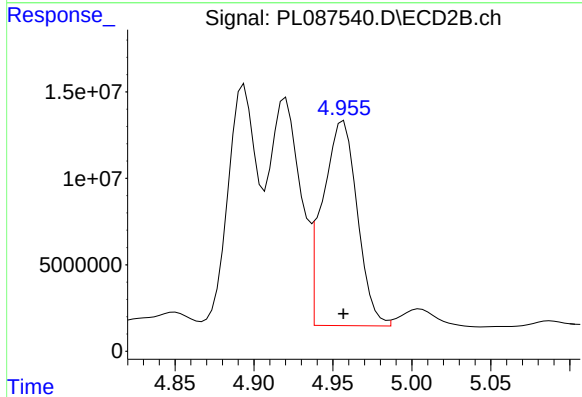


#26 Chlordane-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 180587679
Conc: 1038.04 ng/ml

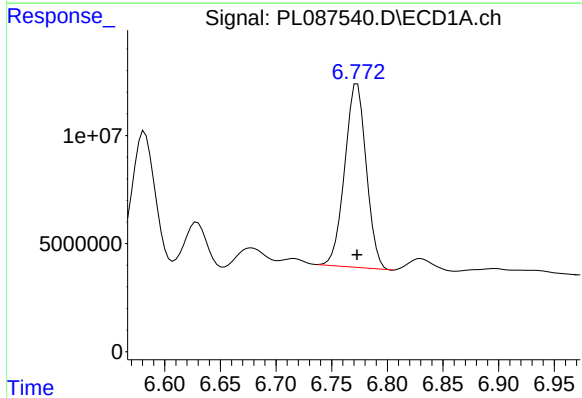


#27 Chlordane-5

R.T.: 6.773 min
Delta R.T.: 0.000 min
Response: 114461661
Conc: 1022.56 ng/ml

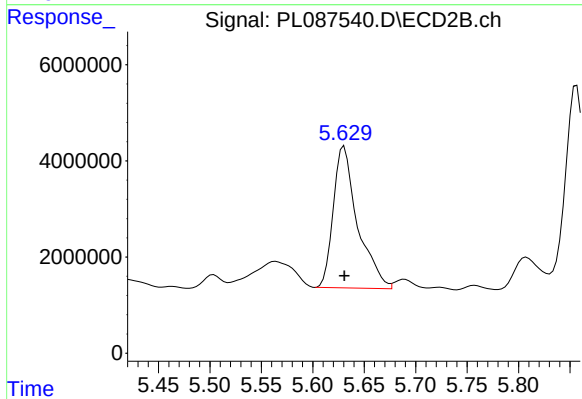

#27 Chlordane-5

R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 48377602
Conc: 1025.06 ng/ml

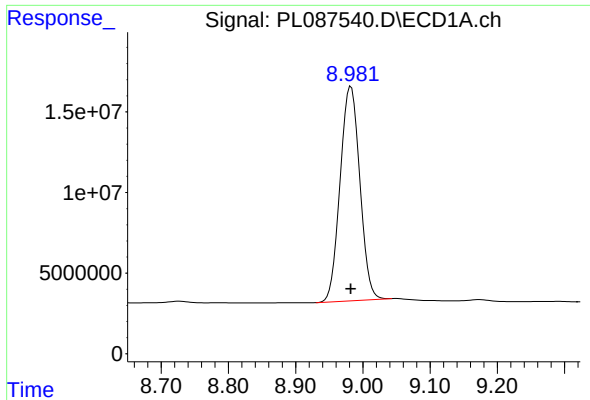

#28 Decachlorobiphenyl


R.T.: 8.982 min

Delta R.T.: 0.000 min

Response: 270418308

Conc: 99.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

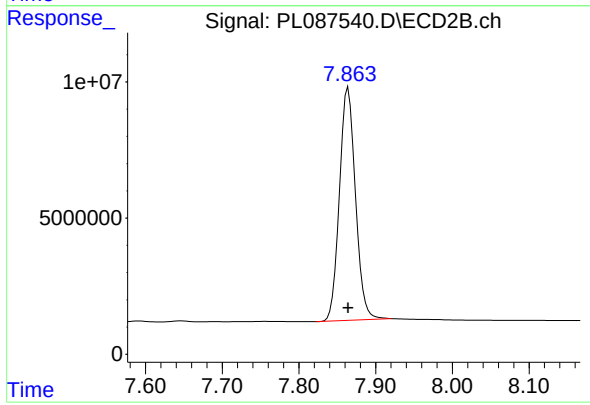

#28 Decachlorobiphenyl

R.T.: 7.864 min

Delta R.T.: 0.000 min

Response: 124391407

Conc: 99.99 ng/ml