

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087541.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 20:05
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 00:33:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 00:33:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.674	223.8E6	117.5E6	74.274	74.120
28)	SA Decachlor...	8.982	7.865	198.1E6	91097277	73.597	73.810
Target Compounds							
23)	Chlordane-1	4.586	3.676	98376355	34792230	741.272	742.750
24)	Chlordane-2	5.121	4.259	104.1E6	40391210	740.046	744.595
25)	Chlordane-3	5.836	4.893	415.6E6	121.2E6	742.293	740.287
26)	Chlordane-4	5.920	4.956	505.2E6	127.2E6	739.431	737.164
27)	Chlordane-5	6.772	5.630	82366907	34583524	740.500	738.432



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087541.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 20:05
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 00:33:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 00:33:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

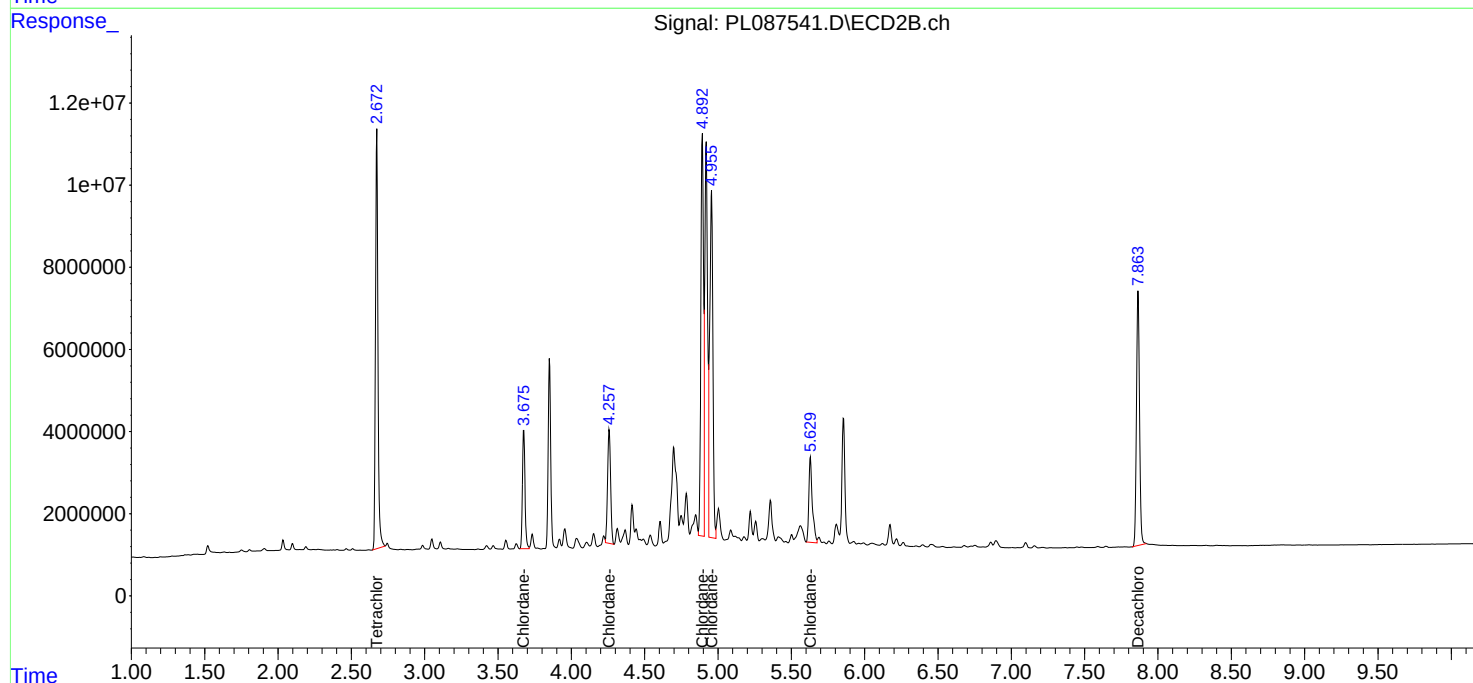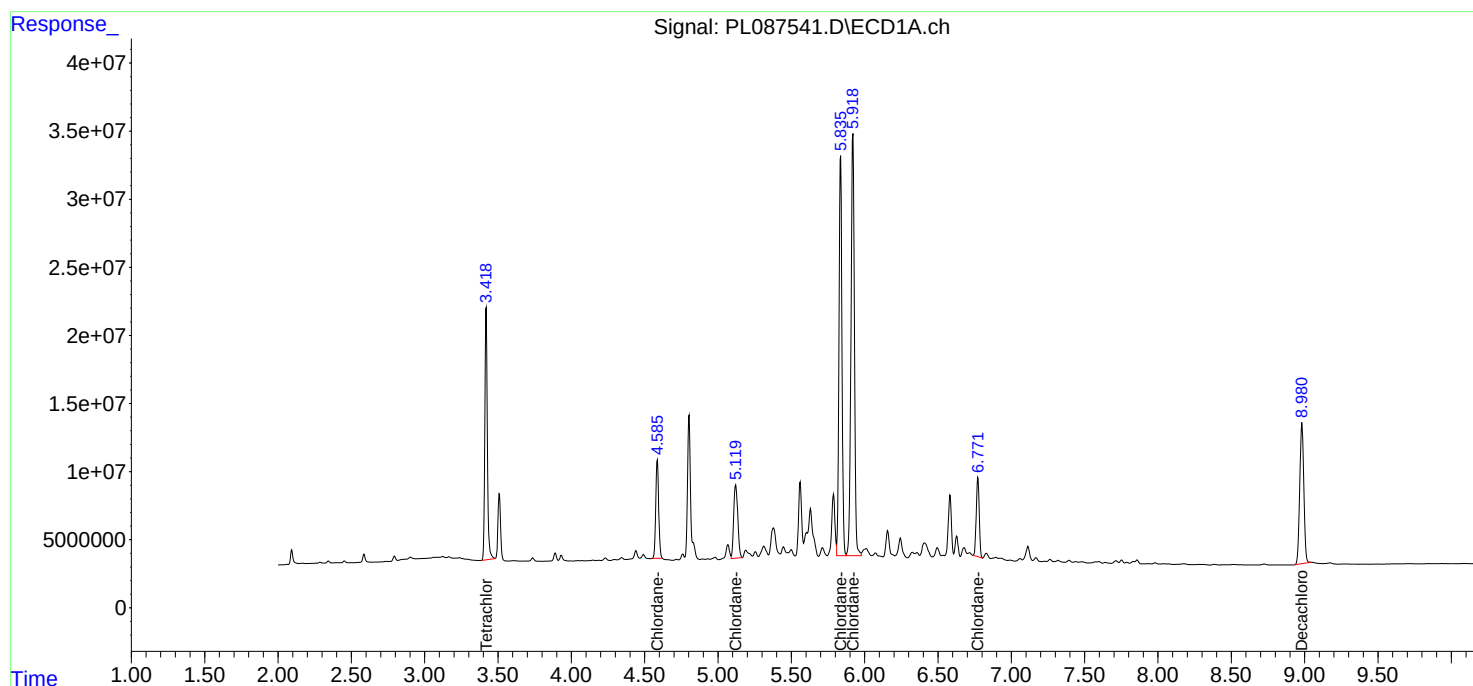


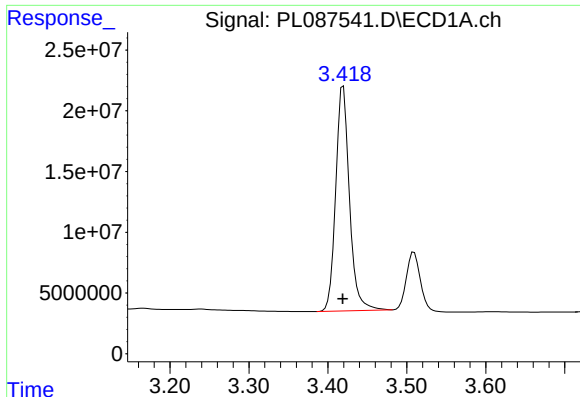

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 223799319
Conc: 74.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

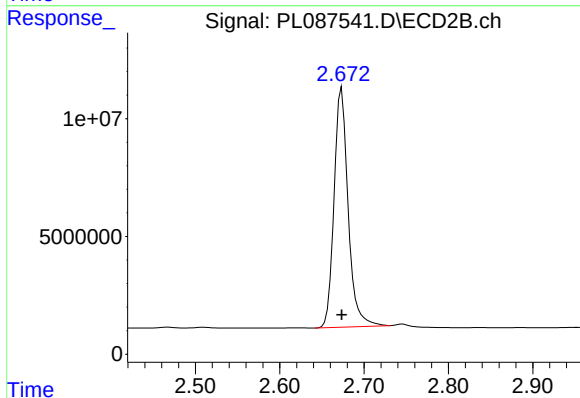


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: 0.000 min
Response: 117536517
Conc: 74.12 ng/ml

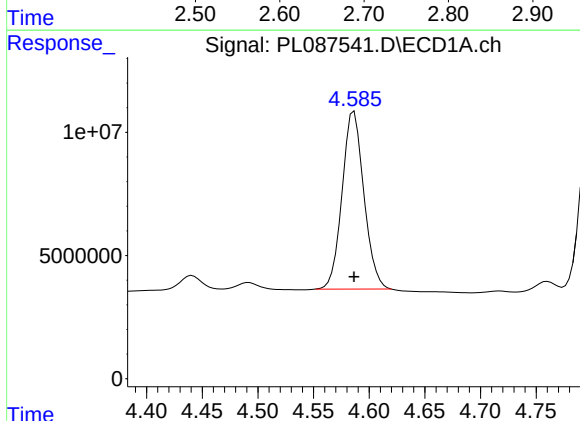


#23 Chlordane-1

R.T.: 4.586 min
Delta R.T.: 0.000 min
Response: 98376355
Conc: 741.27 ng/ml

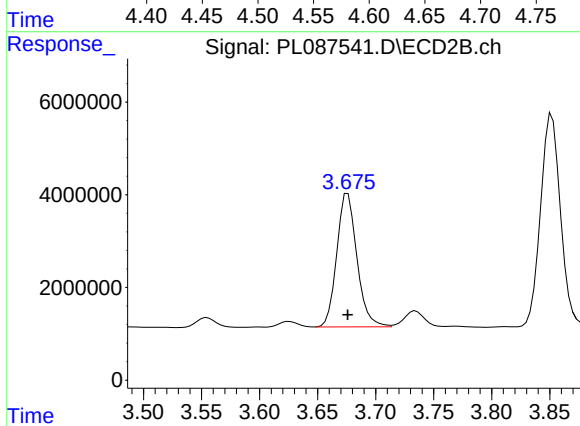

#23 Chlordane-1


R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 34792230
Conc: 742.75 ng/ml

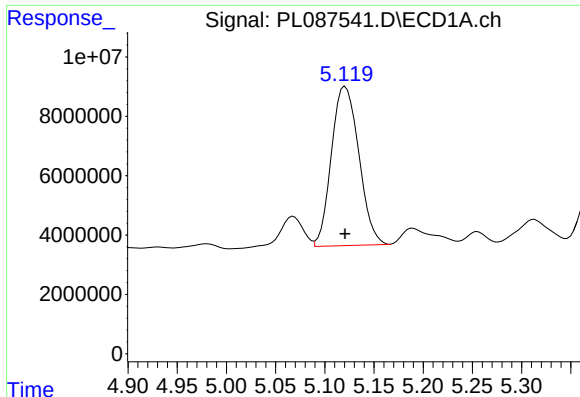

#24 Chlordane-2


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 104080092
Conc: 740.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

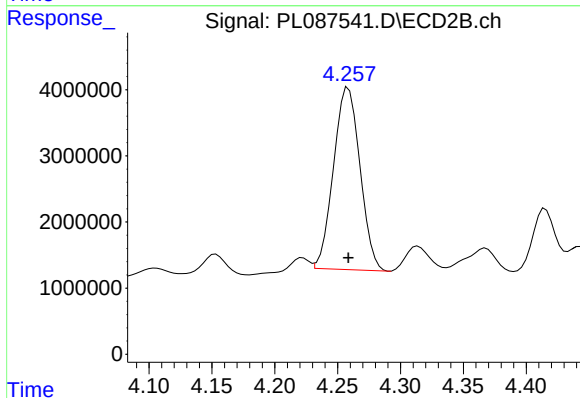


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 40391210
Conc: 744.60 ng/ml

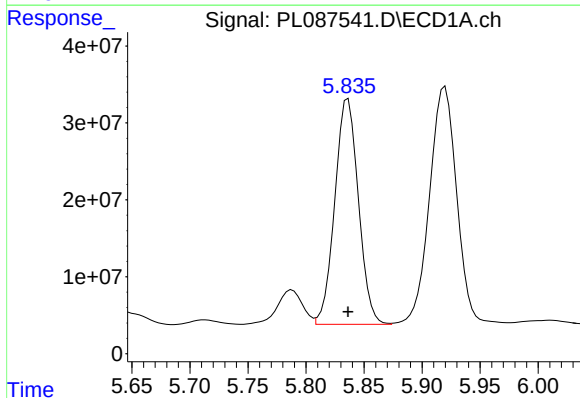


#25 Chlordane-3

R.T.: 5.836 min
Delta R.T.: 0.000 min
Response: 415583533
Conc: 742.29 ng/ml

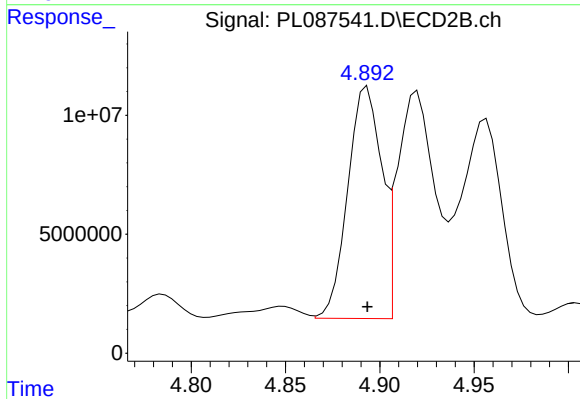

#25 Chlordane-3


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 121237016
Conc: 740.29 ng/ml

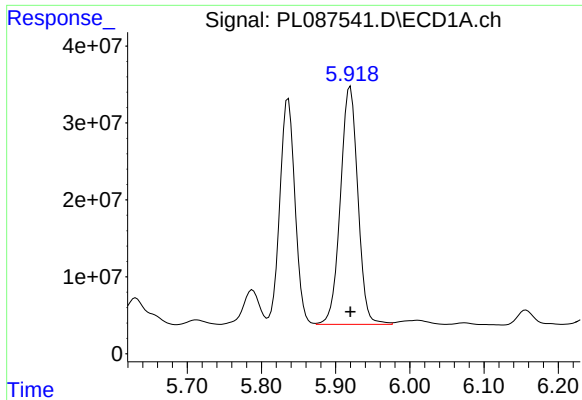

#26 Chlordane-4


R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 505169083
Conc: 739.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

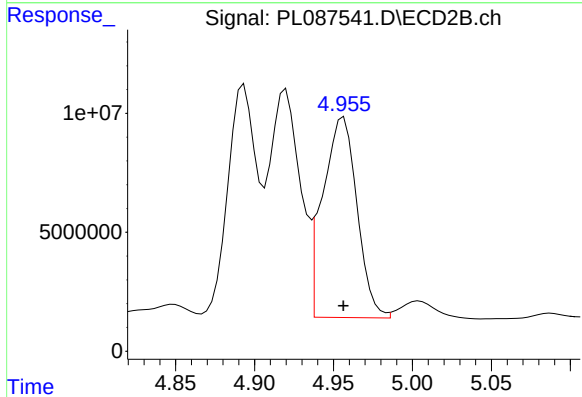


#26 Chlordane-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 127156661
Conc: 737.16 ng/ml

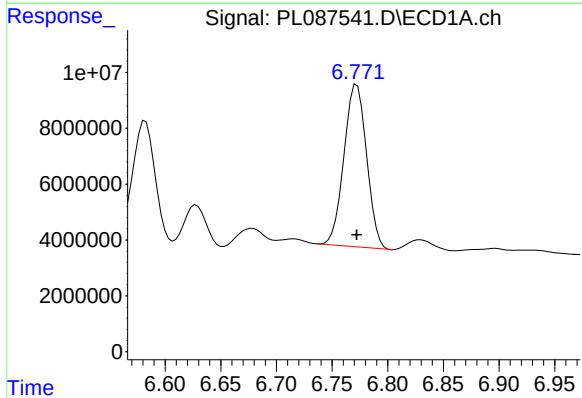


#27 Chlordane-5

R.T.: 6.772 min
Delta R.T.: 0.000 min
Response: 82366907
Conc: 740.50 ng/ml

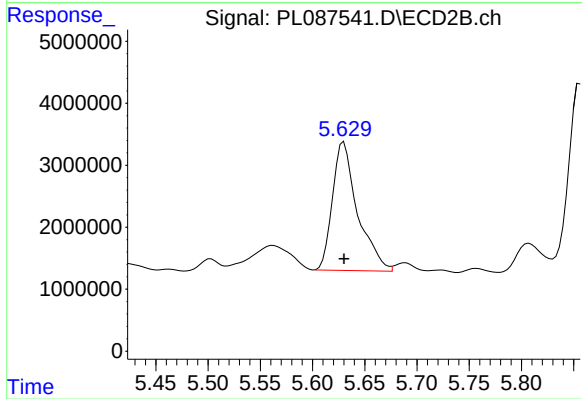

#27 Chlordane-5


R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 34583524
Conc: 738.43 ng/ml

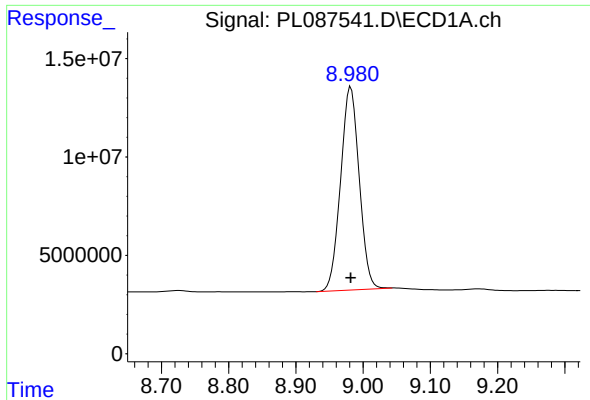

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 198072123
Conc: 73.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

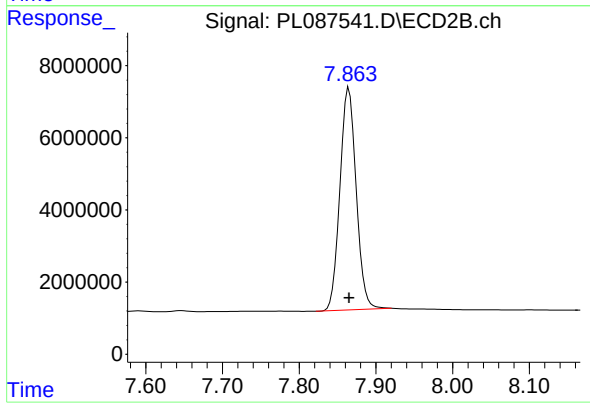

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: 0.000 min
Response: 91097277
Conc: 73.81 ng/ml