

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087542.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 20:19
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 00:30:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 00:22:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.674	147.8E6	76907017	50.000	50.000
28)	SA Decachlor...	8.981	7.866	136.4E6	62203549	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.587	3.676	65036552	22749995	500.000	500.000
24)	Chlordane-2	5.120	4.259	70547671	26799317	500.000	500.000
25)	Chlordane-3	5.836	4.893	270.8E6	78613238	500.000	500.000
26)	Chlordane-4	5.920	4.956	335.5E6	83676821	500.000	500.000
27)	Chlordane-5	6.773	5.630	54705055	23006141	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087542.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 20:19
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 00:30:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 00:22:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

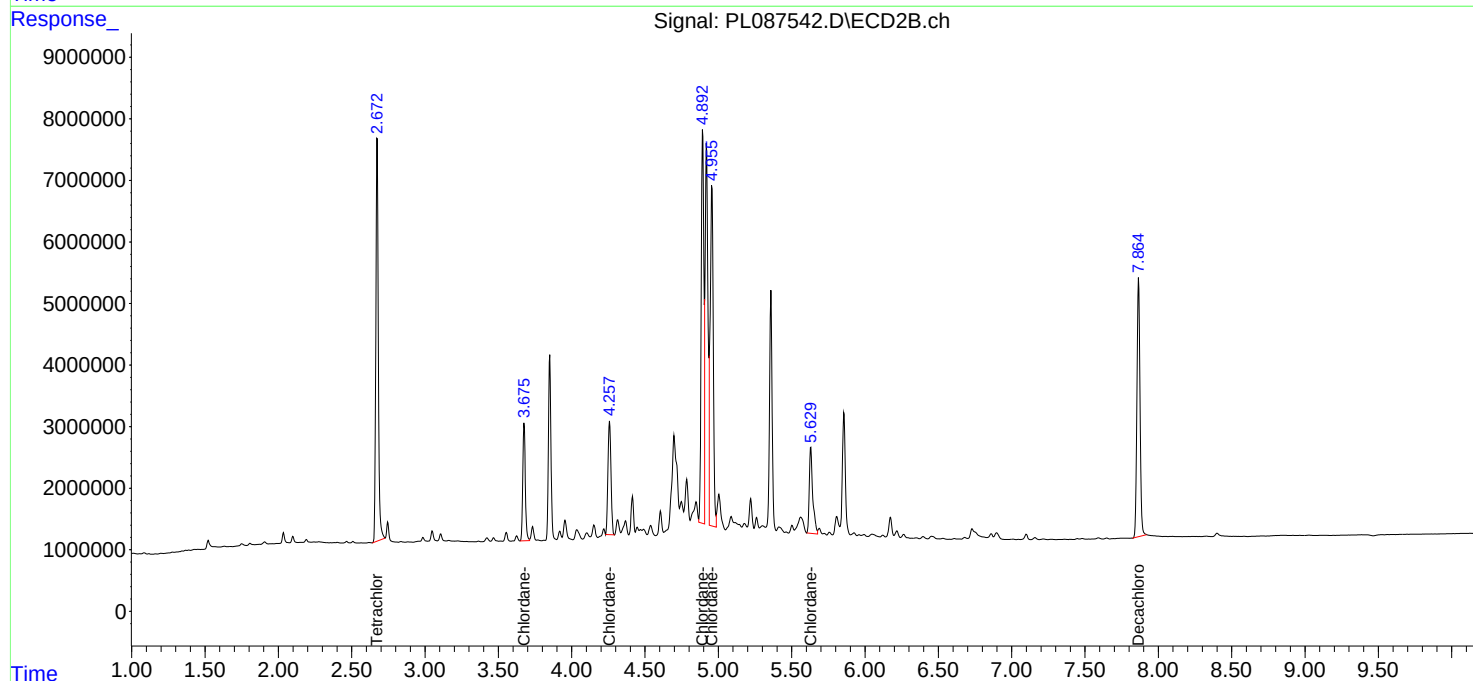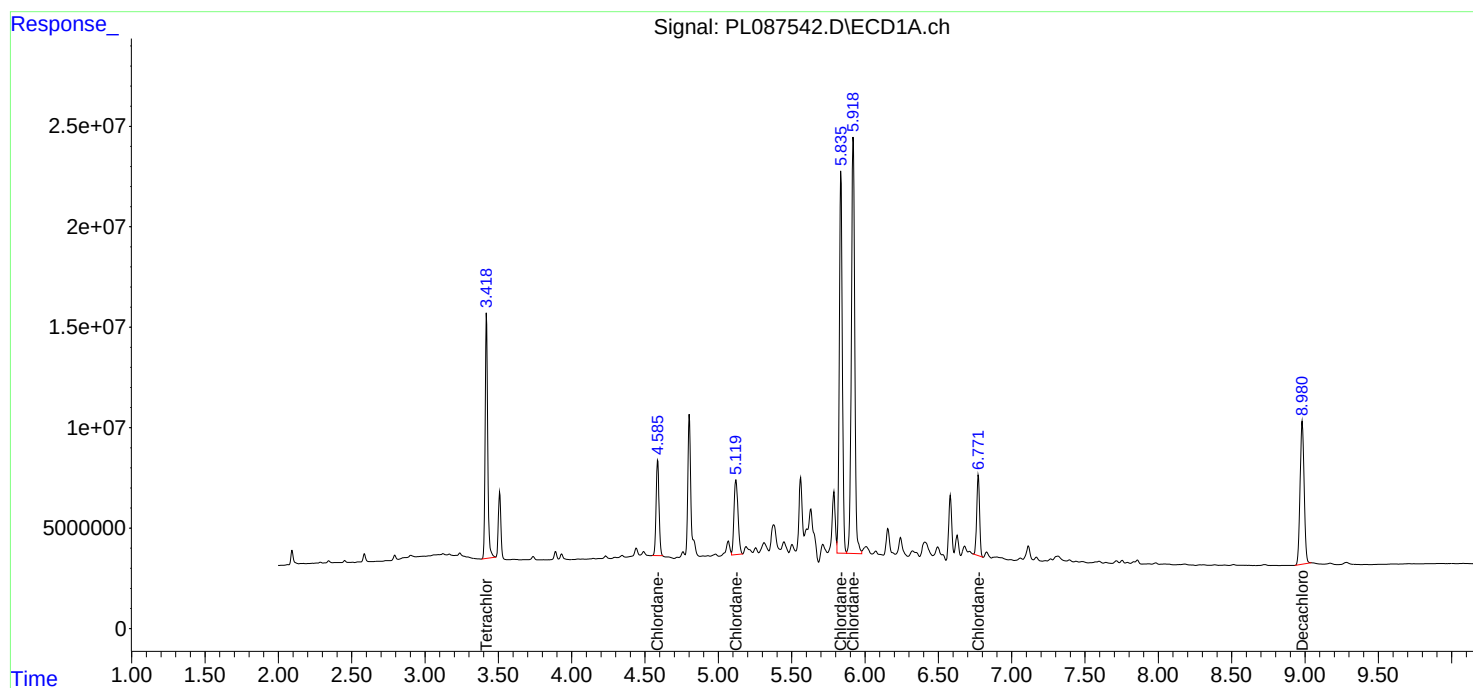


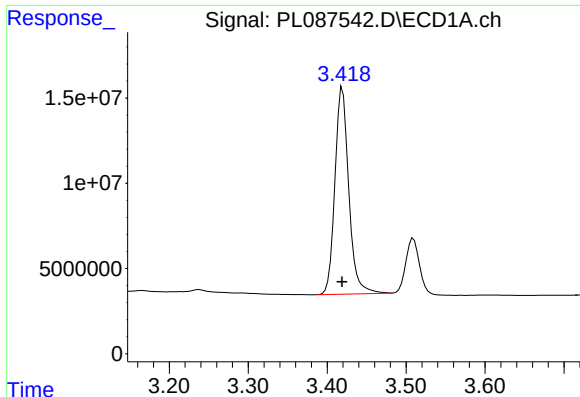

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 147798595
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

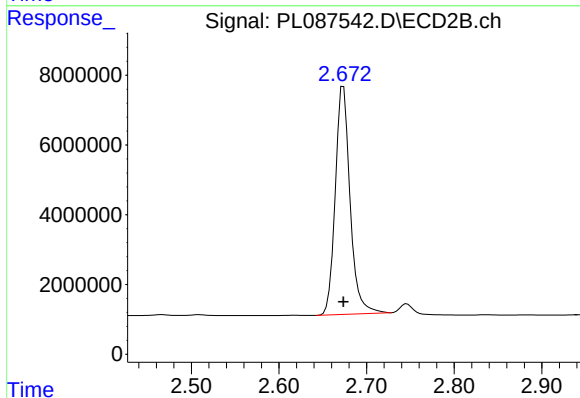


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: 0.000 min
Response: 76907017
Conc: 50.00 ng/ml

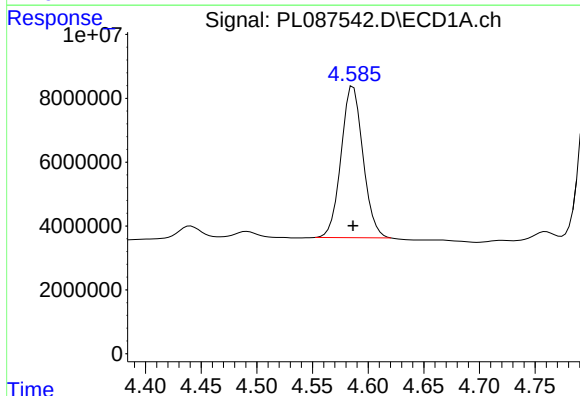


#23 Chlordane-1

R.T.: 4.587 min
Delta R.T.: 0.000 min
Response: 65036552
Conc: 500.00 ng/ml

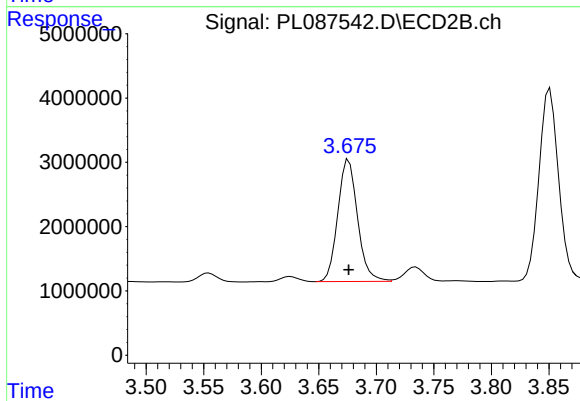

#23 Chlordane-1


R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 22749995
Conc: 500.00 ng/ml

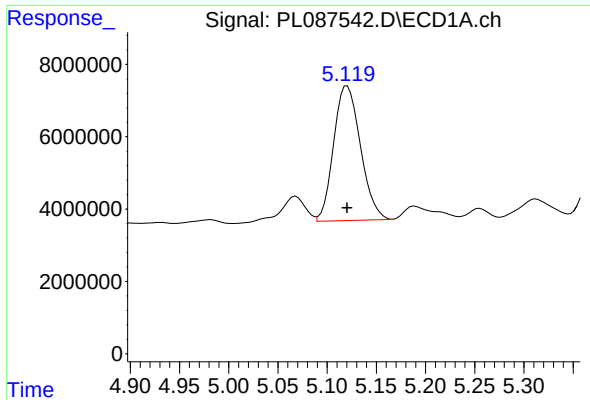

#24 Chlordane-2


R.T.: 5.120 min
Delta R.T.: 0.000 min
Response: 70547671
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

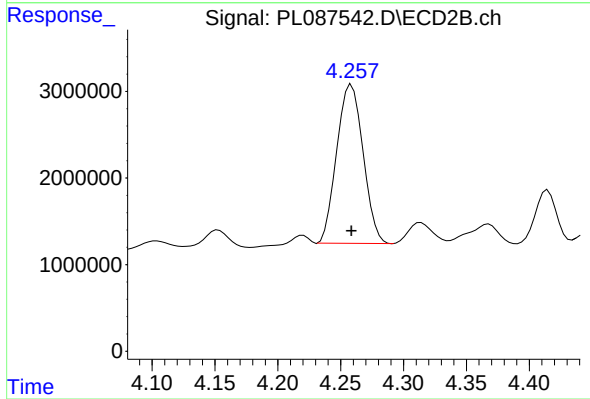


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 26799317
Conc: 500.00 ng/ml

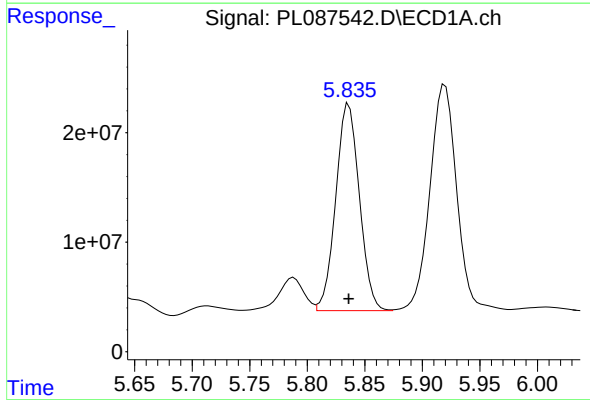


#25 Chlordane-3

R.T.: 5.836 min
Delta R.T.: 0.000 min
Response: 270782459
Conc: 500.00 ng/ml

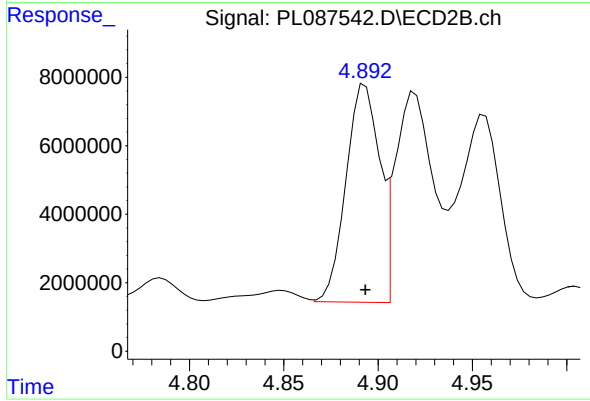

#25 Chlordane-3


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 78613238
Conc: 500.00 ng/ml

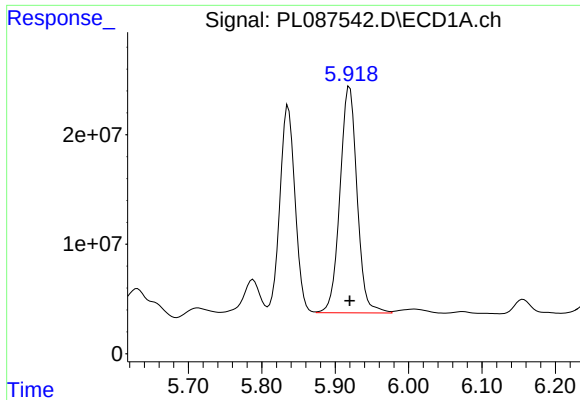

#26 Chlordane-4


R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 335475151
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

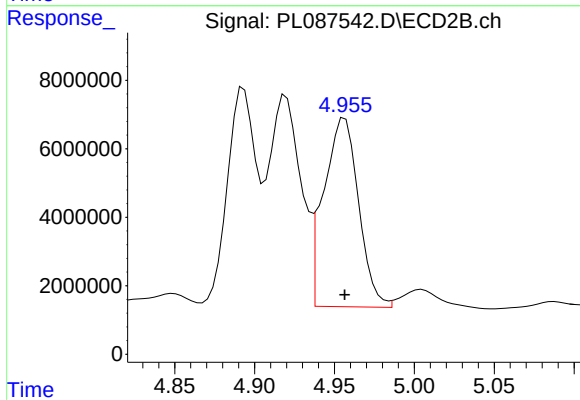


#26 Chlordane-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 83676821
Conc: 500.00 ng/ml

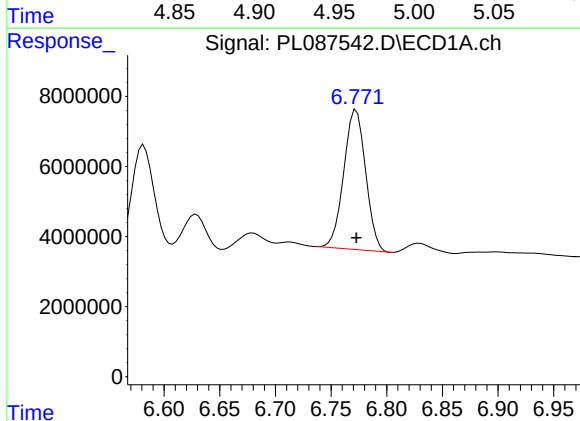


#27 Chlordane-5

R.T.: 6.773 min
Delta R.T.: 0.000 min
Response: 54705055
Conc: 500.00 ng/ml

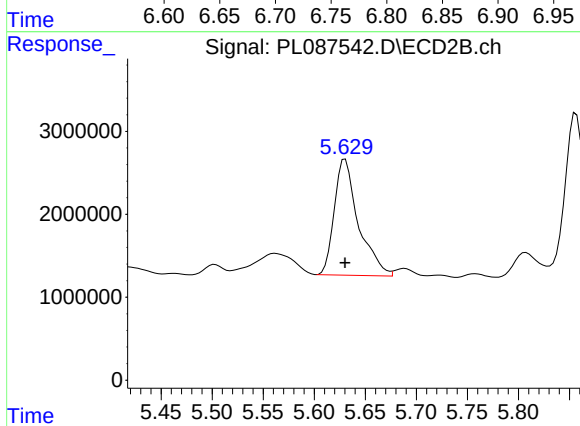

#27 Chlordane-5


R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 23006141
Conc: 500.00 ng/ml

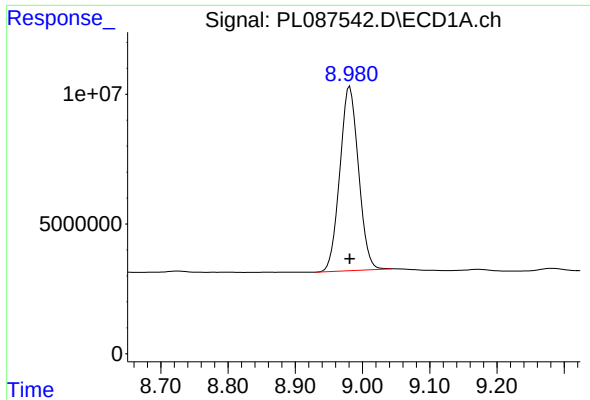

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 136441261
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

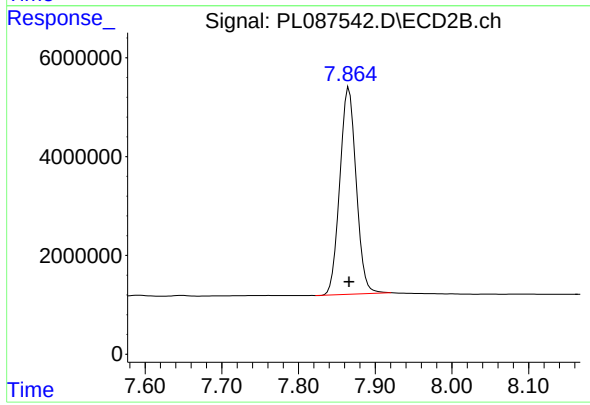

#28 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 62203549
Conc: 50.00 ng/ml