

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 20:33
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 00:36:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 00:36:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.674	77662054	39579018	25.576	24.969
28)	SA Decachlor...	8.982	7.865	75012876	33986827	27.094	26.856
Target Compounds							
23)	Chlordane-1	4.587	3.676	33942885	11836011	254.296	252.002
24)	Chlordane-2	5.122	4.259	37964762	14809376	264.665	266.866
25)	Chlordane-3	5.837	4.893	140.7E6	38945634	251.035	240.742
26)	Chlordane-4	5.920	4.956	178.0E6	42818275	257.801	248.670
27)	Chlordane-5	6.773	5.630	28966321	11867488	257.731	252.538



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 20:33
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 00:36:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 00:36:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

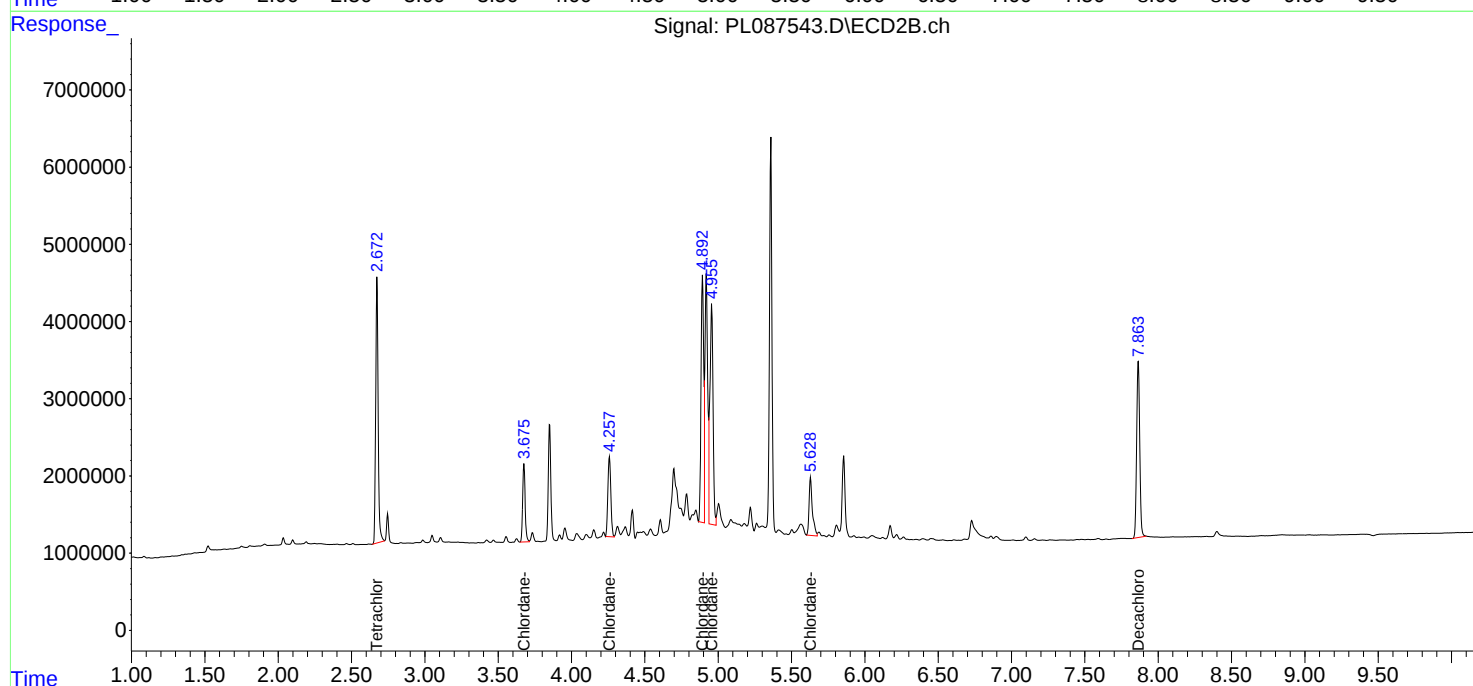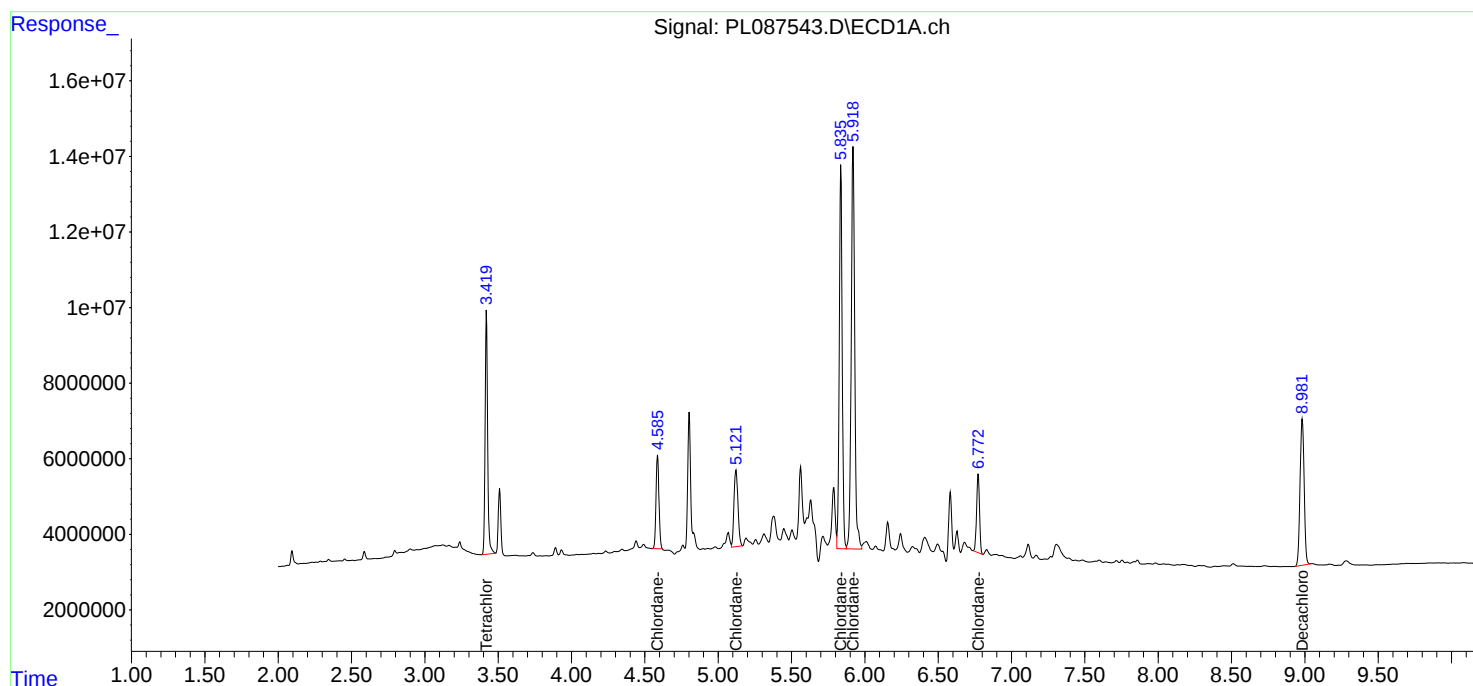


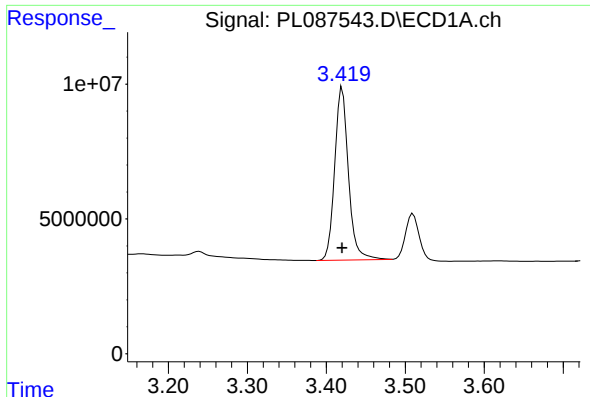

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 77662054
Conc: 25.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

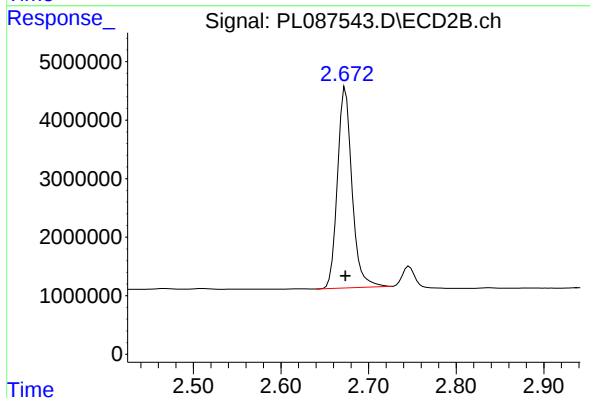


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: 0.000 min
Response: 39579018
Conc: 24.97 ng/ml

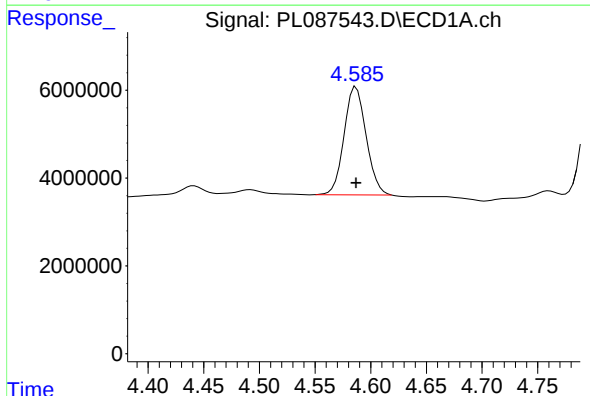


#23 Chlordane-1

R.T.: 4.587 min
Delta R.T.: 0.000 min
Response: 33942885
Conc: 254.30 ng/ml

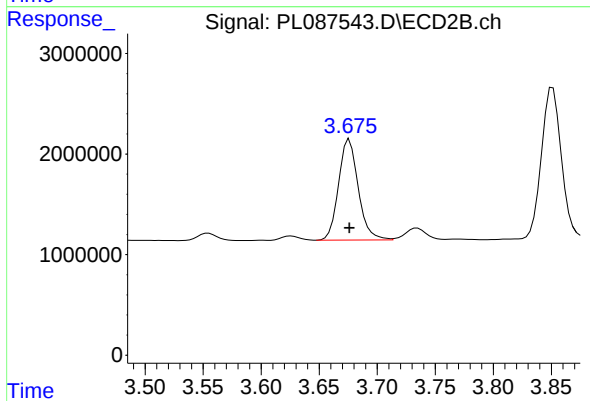

#23 Chlordane-1


R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 11836011
Conc: 252.00 ng/ml

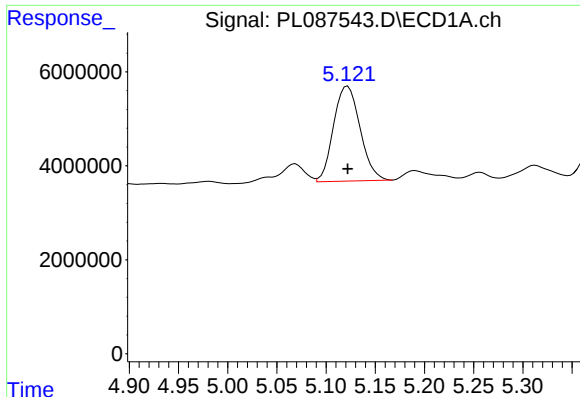

#24 Chlordane-2


R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 37964762
Conc: 264.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

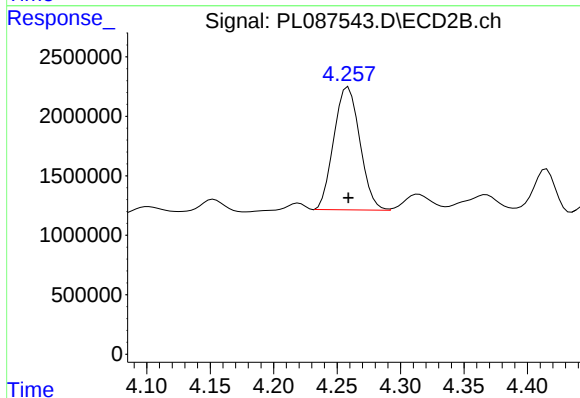


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 14809376
Conc: 266.87 ng/ml

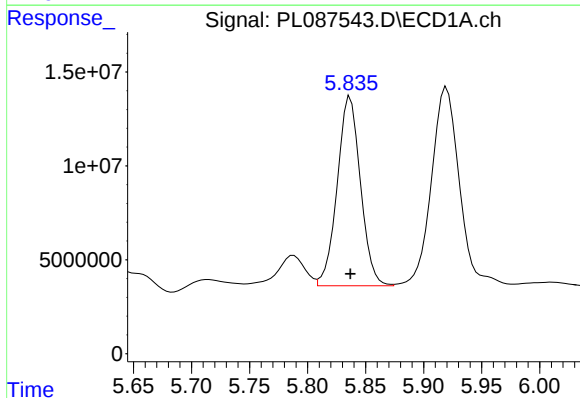


#25 Chlordane-3

R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 140740039
Conc: 251.04 ng/ml

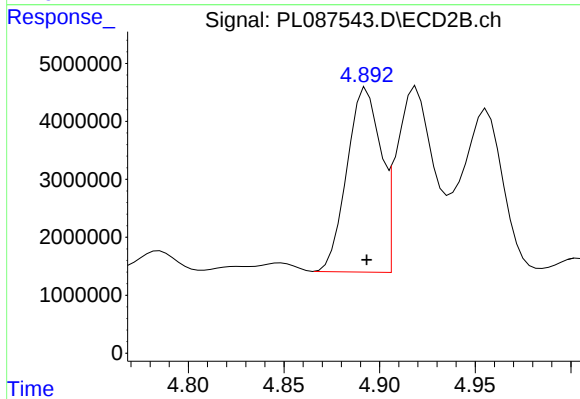

#25 Chlordane-3


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 38945634
Conc: 240.74 ng/ml

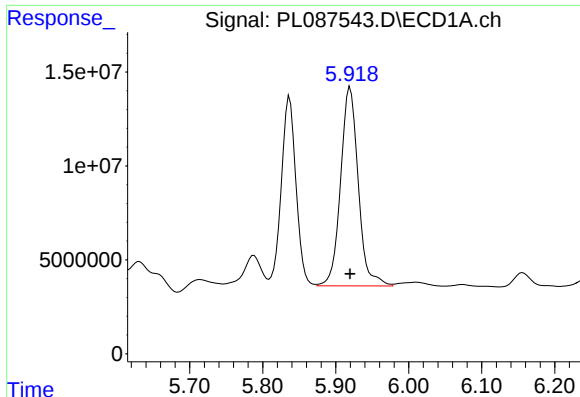

#26 Chlordane-4


R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 177977780
Conc: 257.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

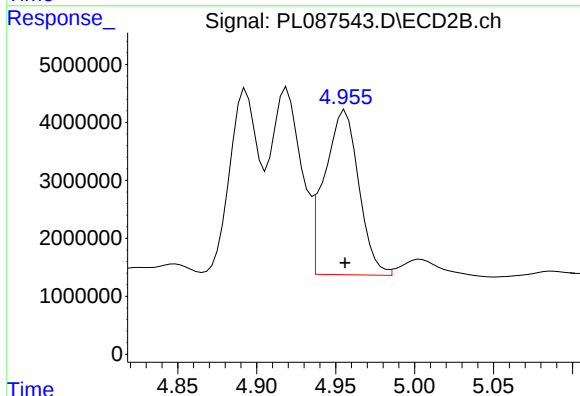


#26 Chlordane-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 42818275
Conc: 248.67 ng/ml

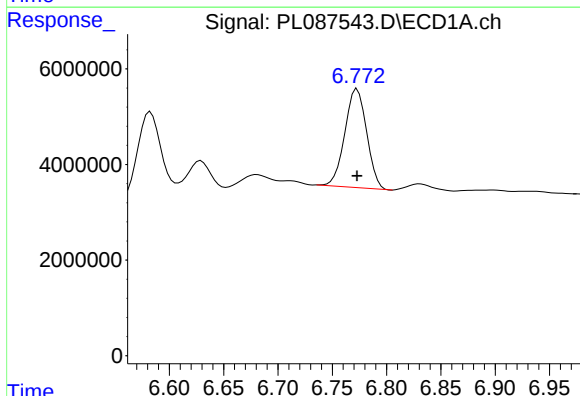


#27 Chlordane-5

R.T.: 6.773 min
Delta R.T.: 0.000 min
Response: 28966321
Conc: 257.73 ng/ml

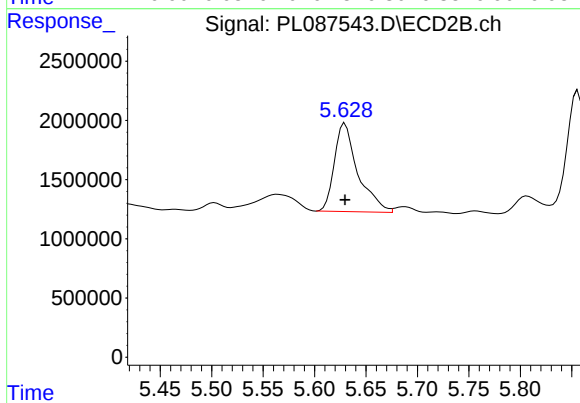

#27 Chlordane-5


R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 11867488
Conc: 252.54 ng/ml

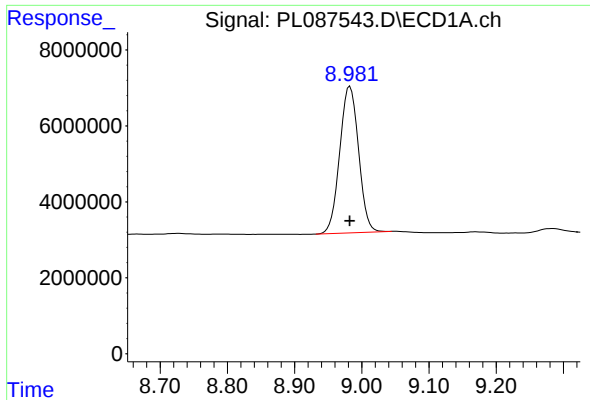

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 75012876
Conc: 27.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

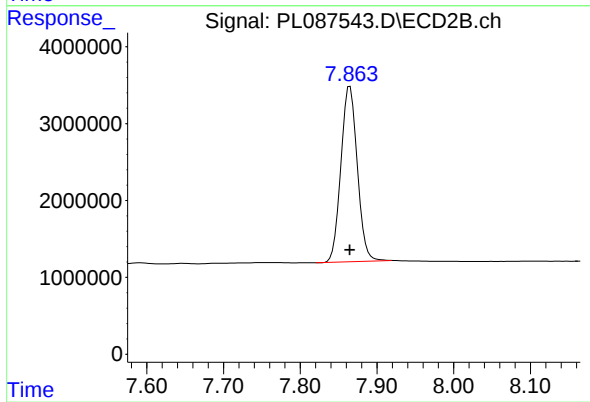

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: 0.000 min
Response: 33986827
Conc: 26.86 ng/ml