

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 20:46
 Operator : AR\AJ
 Sample : PCHLORICC050 (Sig #1); CHLORICC050 (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 00:41:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 00:41:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.673	15264707	7630035	5.022	4.850
28)	SA Decachlor...	8.981	7.865	16867060	7330740	5.837	5.615
Target Compounds							
23)	Chlordane-1	4.587	3.676	6673413	2290969	49.997	49.017
24)	Chlordane-2	5.120	4.259	8178194	2888393	55.457	51.626
25)	Chlordane-3	5.836	4.894	26938507	7209435	48.427	45.555
26)	Chlordane-4	5.920	4.957	34856127	8276657	50.391	48.442
27)	Chlordane-5	6.772	5.631	5715178	2369378	50.679	50.335



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 20:46
Operator : AR\AJ
Sample : PCHLORICC050 (Sig #1); CHLORICC050 (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 00:41:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 00:41:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

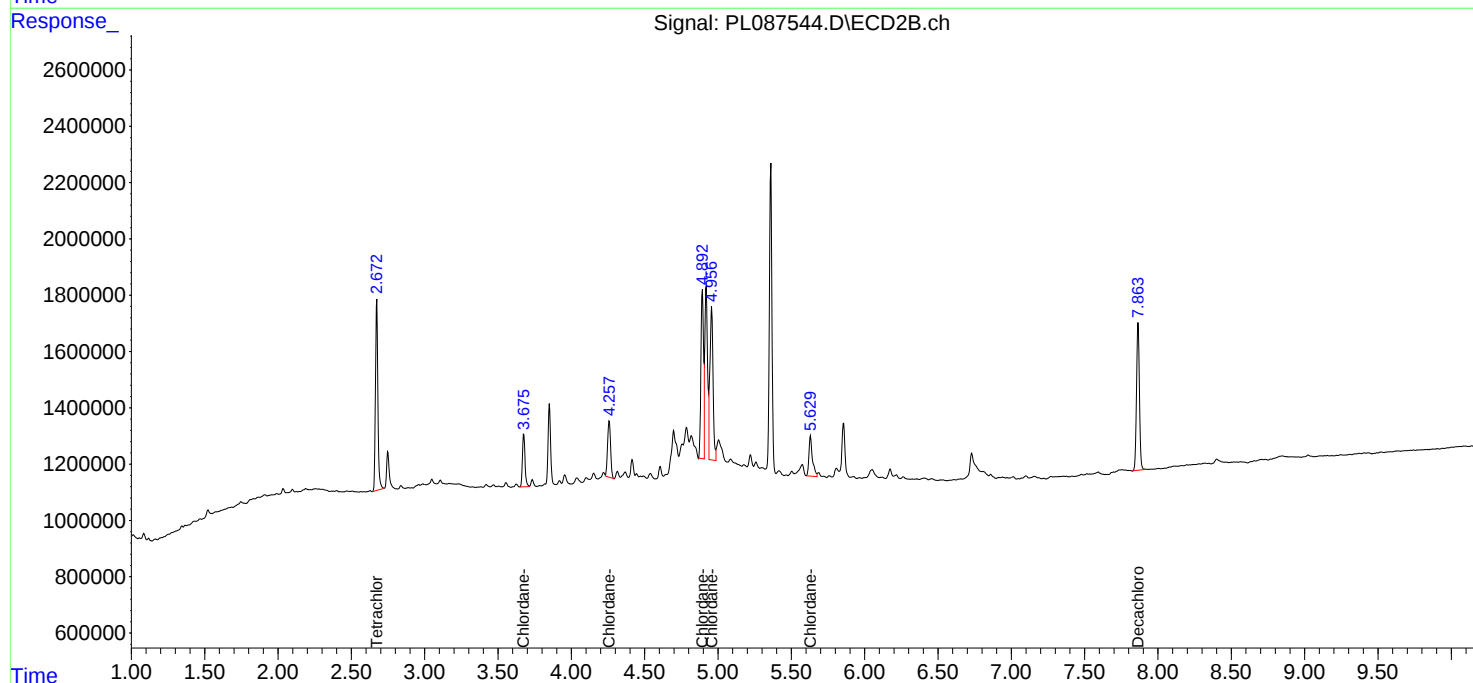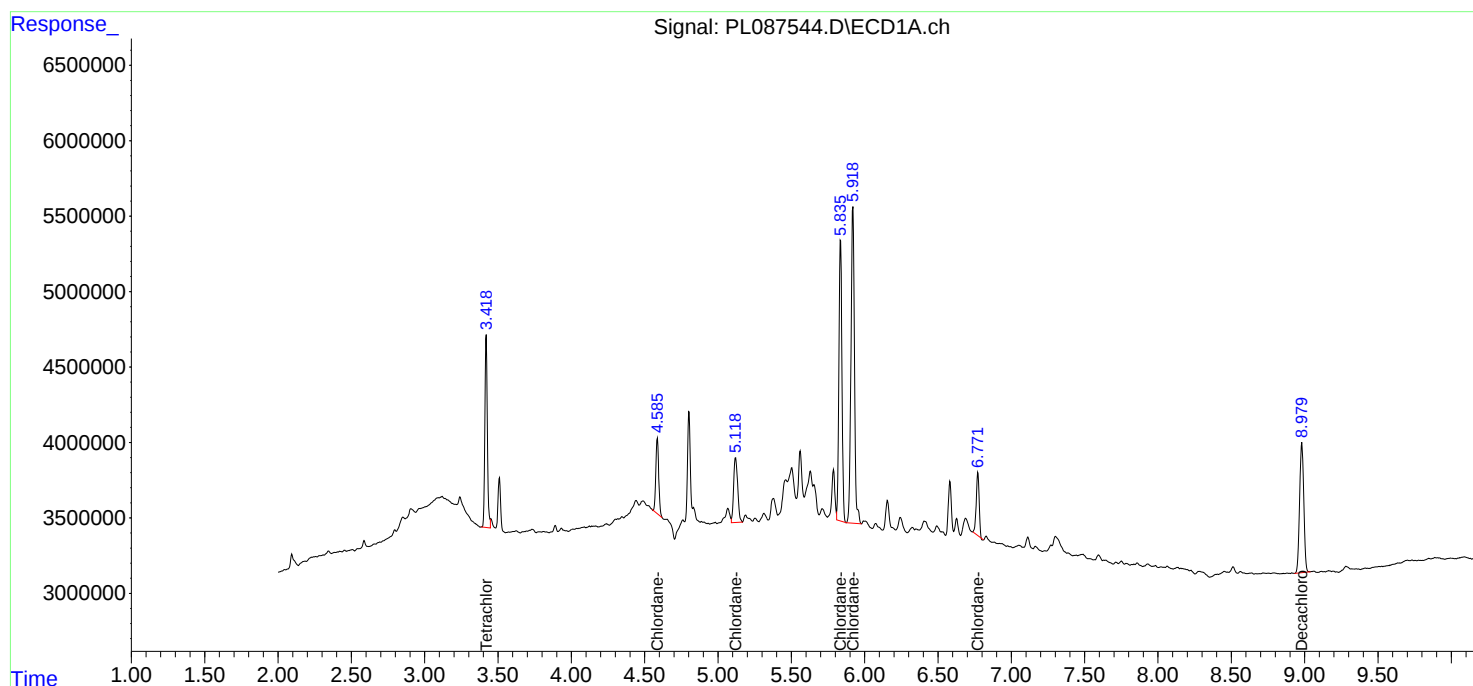


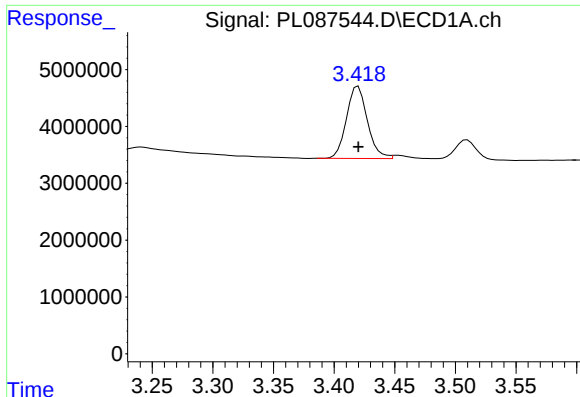

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 15264707
Conc: 5.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

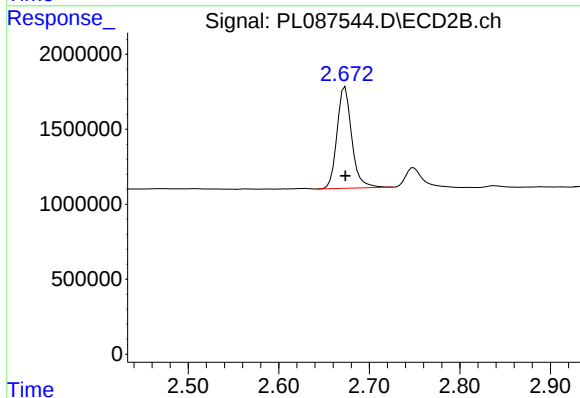


#1 Tetrachloro-m-xylene

R.T.: 2.673 min
Delta R.T.: 0.000 min
Response: 7630035
Conc: 4.85 ng/ml

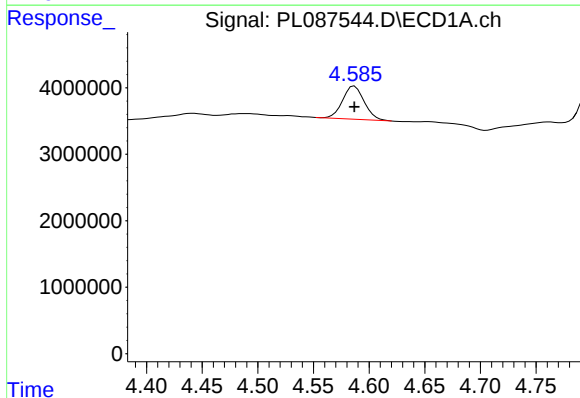


#23 Chlordane-1

R.T.: 4.587 min
Delta R.T.: 0.000 min
Response: 6673413
Conc: 50.00 ng/ml

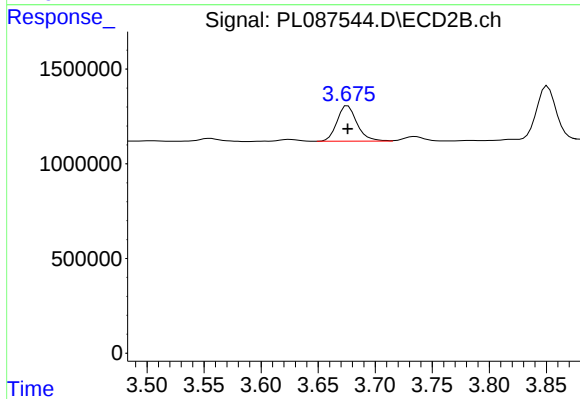

#23 Chlordane-1


R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 2290969
Conc: 49.02 ng/ml

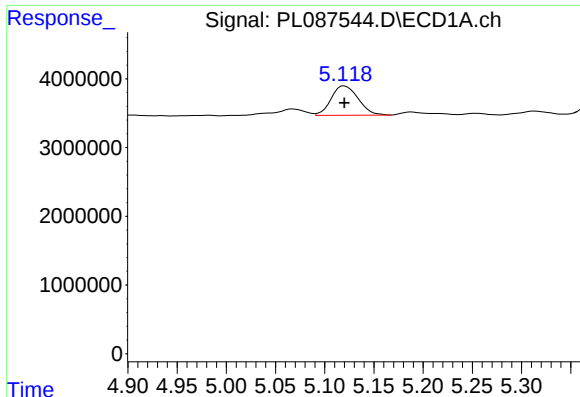

#24 Chlordane-2


R.T.: 5.120 min
Delta R.T.: 0.000 min
Response: 8178194
Conc: 55.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

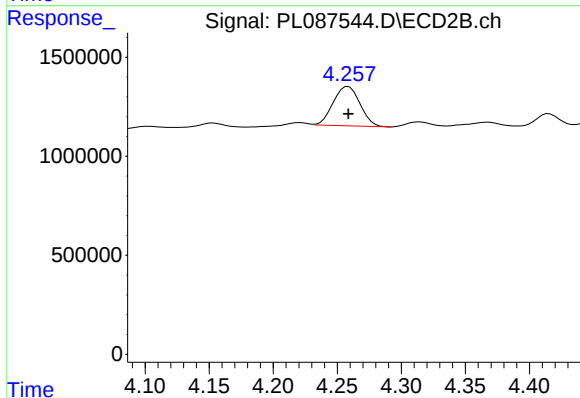


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 2888393
Conc: 51.63 ng/ml

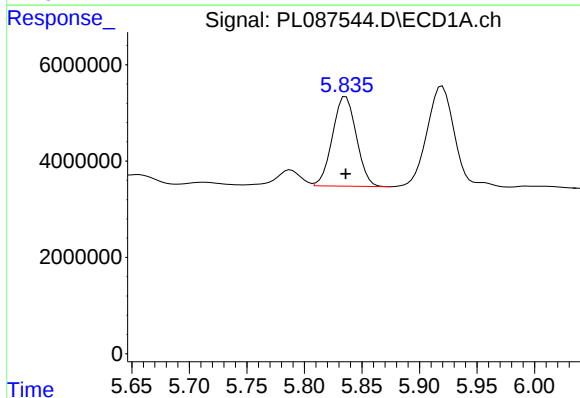


#25 Chlordane-3

R.T.: 5.836 min
Delta R.T.: 0.000 min
Response: 26938507
Conc: 48.43 ng/ml

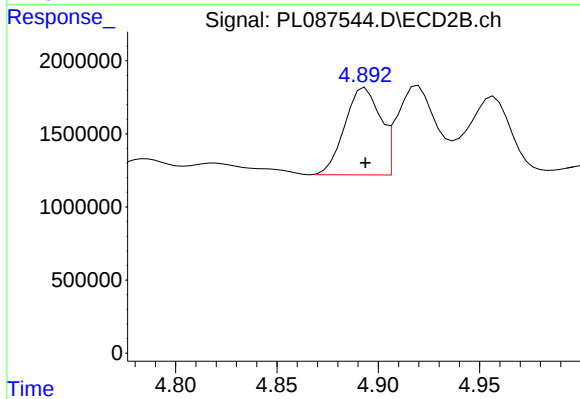

#25 Chlordane-3


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 7209435
Conc: 45.56 ng/ml

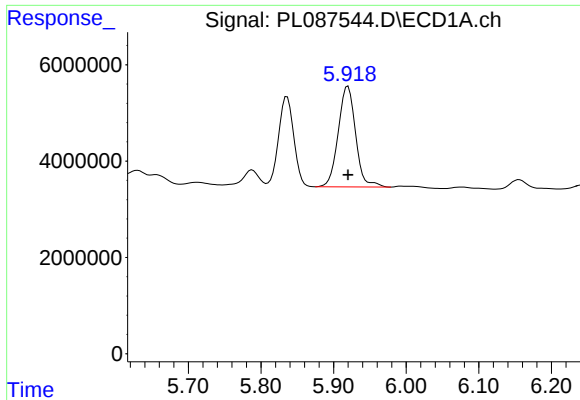

#26 Chlordane-4


R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 34856127
Conc: 50.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

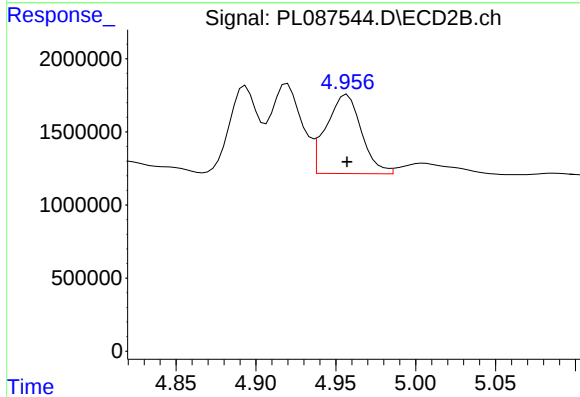


#26 Chlordane-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 8276657
Conc: 48.44 ng/ml

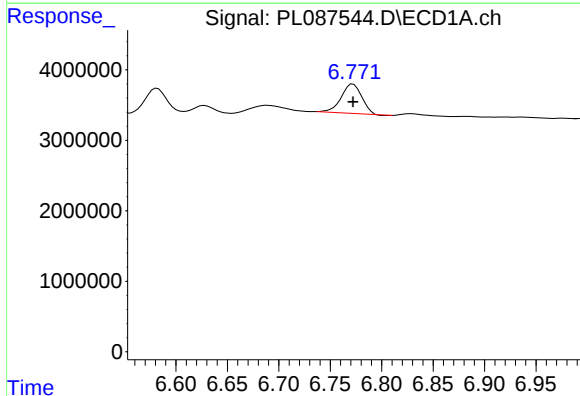


#27 Chlordane-5

R.T.: 6.772 min
Delta R.T.: 0.000 min
Response: 5715178
Conc: 50.68 ng/ml

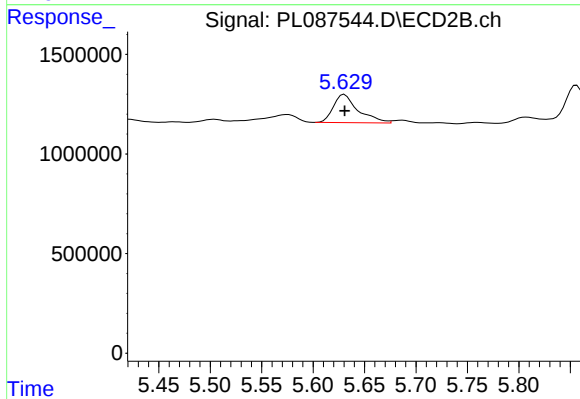

#27 Chlordane-5


R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 2369378
Conc: 50.34 ng/ml

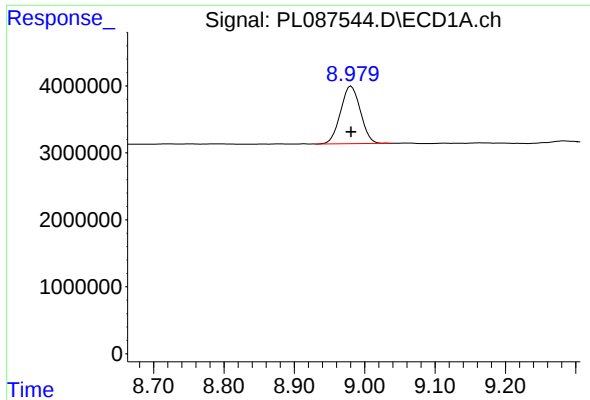

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 16867060
Conc: 5.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

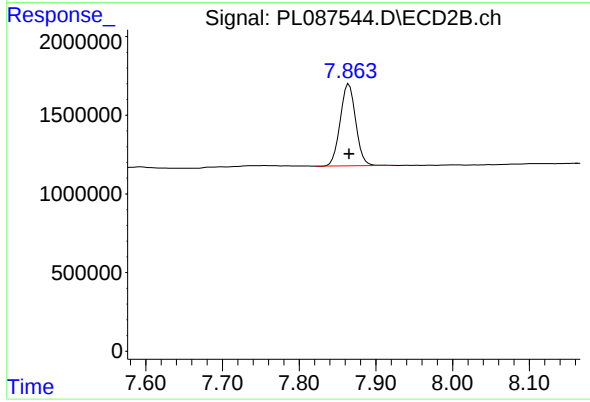

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: 0.000 min
Response: 7330740
Conc: 5.61 ng/ml