

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2023 02:07
 Operator : AR\AJ
 Sample : 06031-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MR-321-0-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/29/2023
 Supervised By : Ankita Jodhani 12/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 03:28:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.420	2.676	51930662	22484948	17.346m	18.562
28) SA Decachlor...	8.981	7.865	44421204	19877066	15.597	15.691

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2023 02:07
Operator : AR\AJ
Sample : 06031-02
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MR-321-0-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/29/2023
Supervised By : Ankita Jodhani 12/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 03:28:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

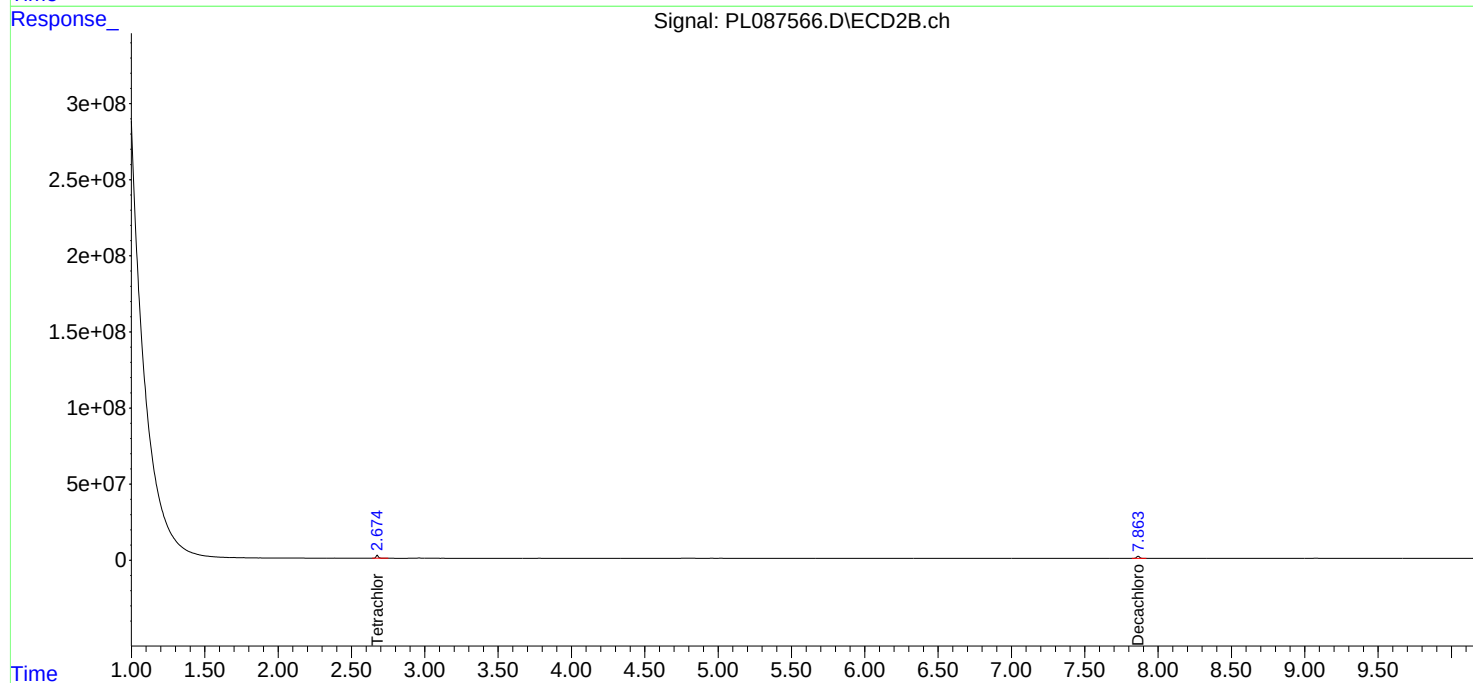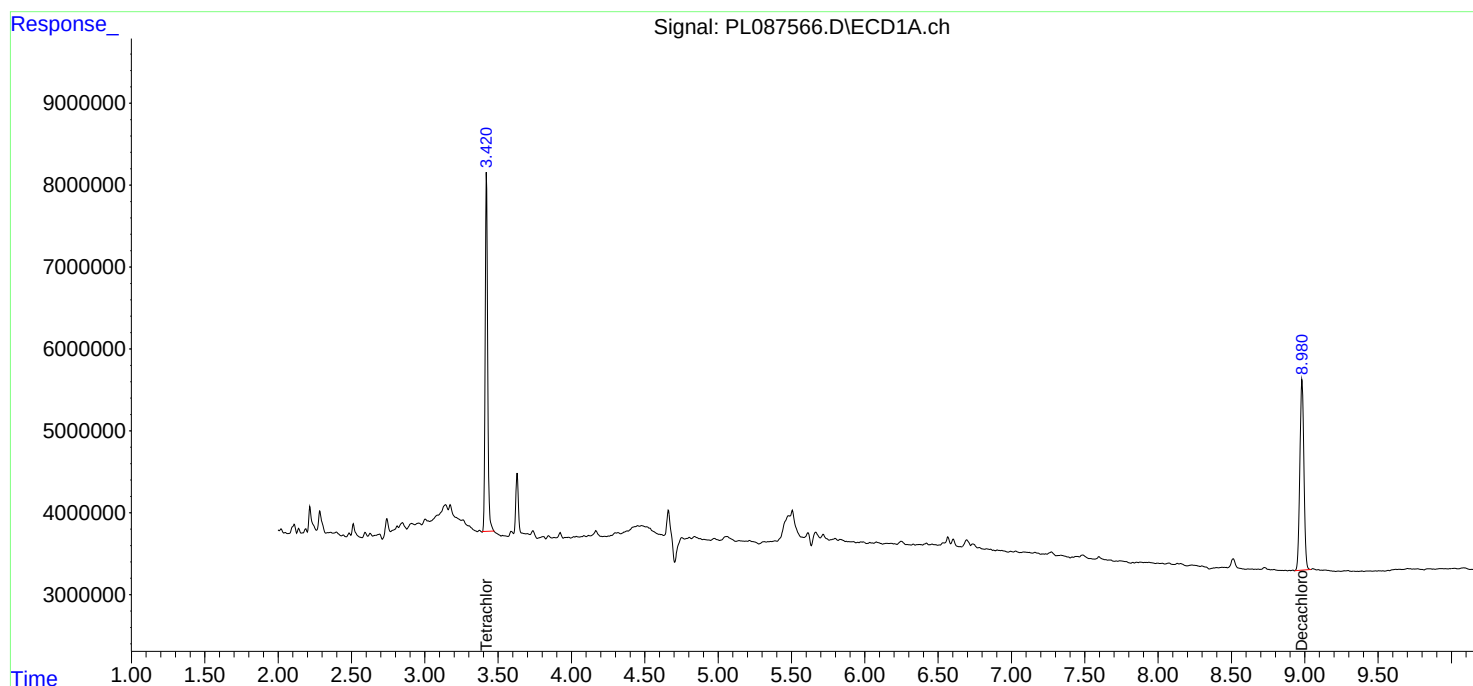

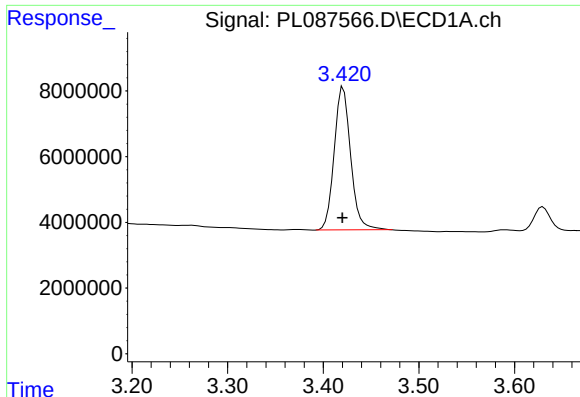


#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 51930662
Conc: 17.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-321-0-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/29/2023
Supervised By :Ankita Jodhani 12/29/2023

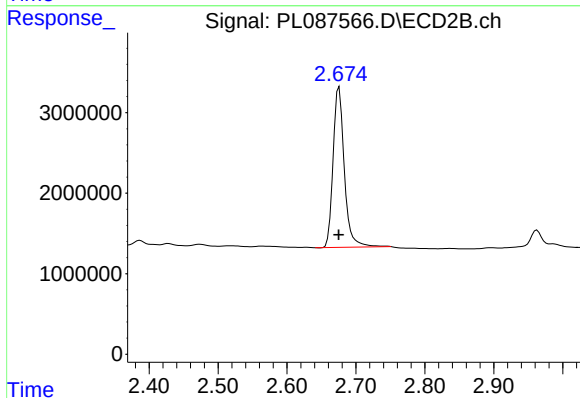


#1 Tetrachloro-m-xylene

R.T.: 2.676 min
Delta R.T.: 0.000 min
Response: 22484948
Conc: 18.56 ng/ml

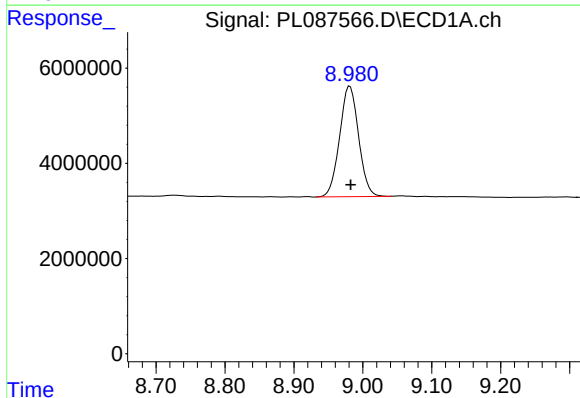

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: -0.001 min
Response: 44421204
Conc: 15.60 ng/ml

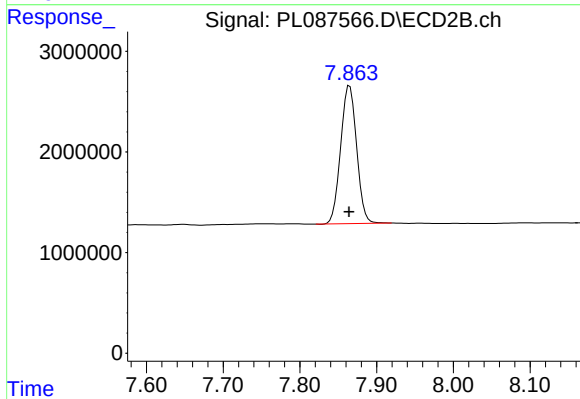

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: 0.000 min
Response: 19877066
Conc: 15.69 ng/ml