

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
 Data File : PL087581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2023 07:43
 Operator : AR\AJ
 Sample : 06034-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-05-122723

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/02/2024
 Supervised By :Ankita Jodhani 01/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 10:06:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.419	2.674	25995884	12382728	8.683m	10.222m
28) SA Decachlor...	8.982	7.864	37106620	14579901	13.029	11.509

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122823\
Data File : PL087581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2023 07:43
Operator : AR\AJ
Sample : 06034-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-05-122723


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/02/2024
Supervised By : Ankita Jodhani 01/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 10:06:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

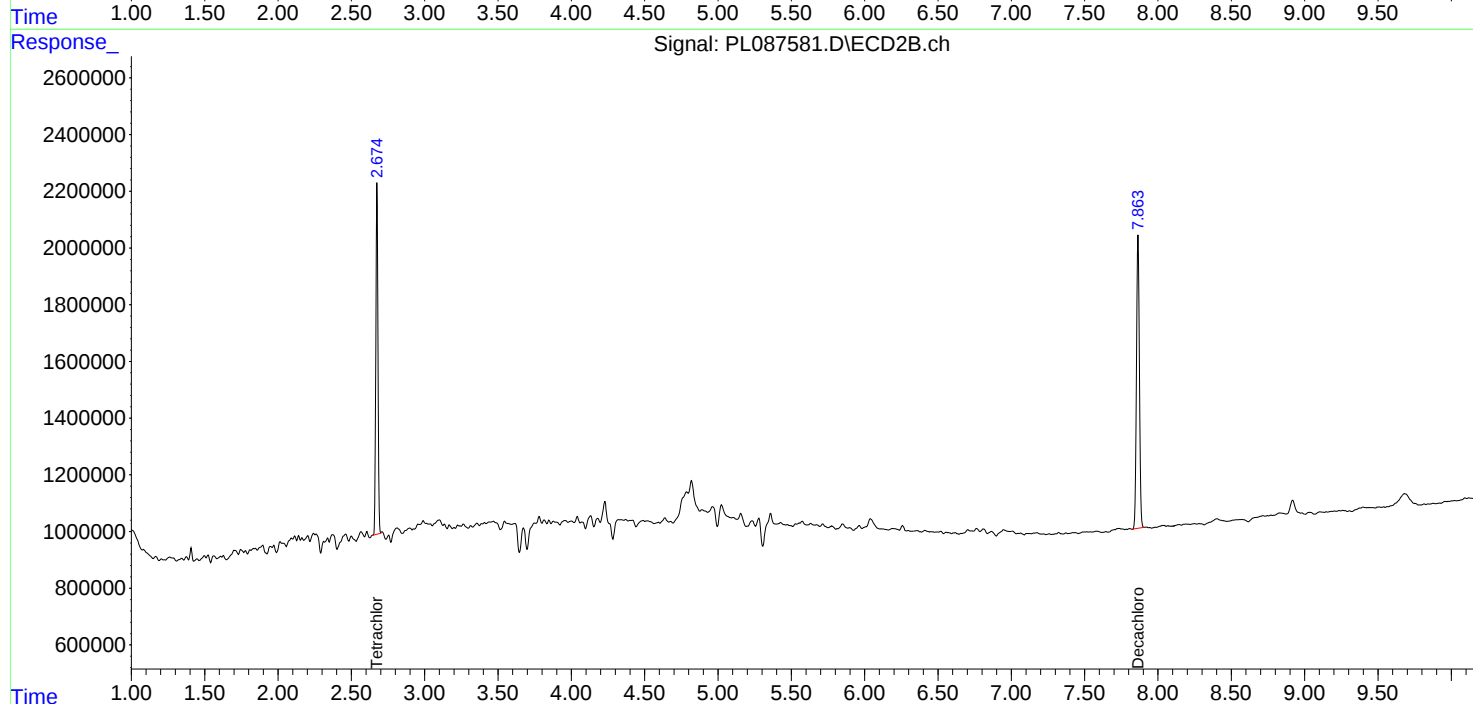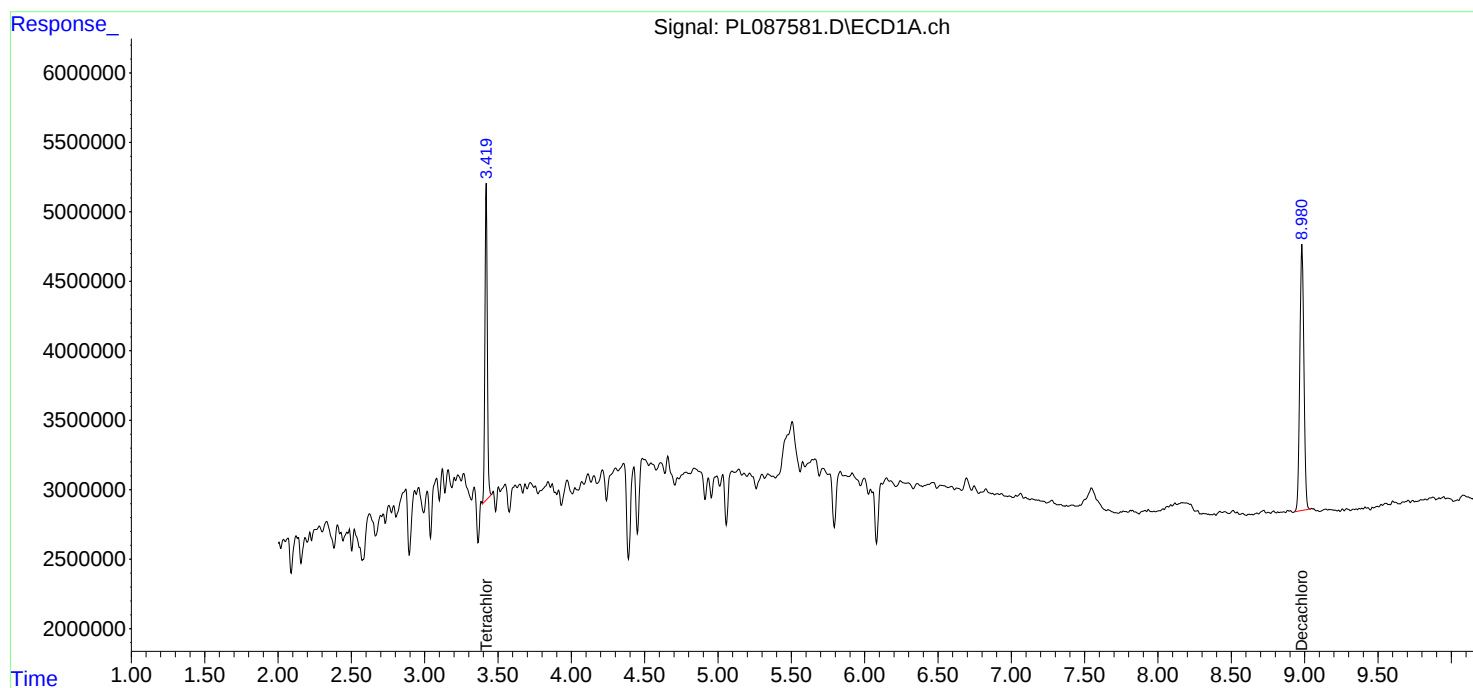

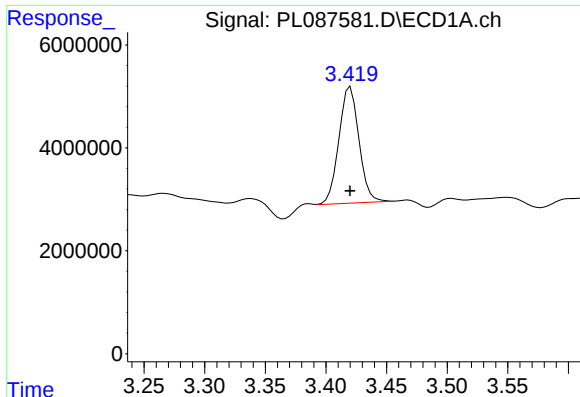


#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: -0.001 min
Response: 25995884
Conc: 8.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-05-122723


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/02/2024
Supervised By :Ankita Jodhani 01/02/2024

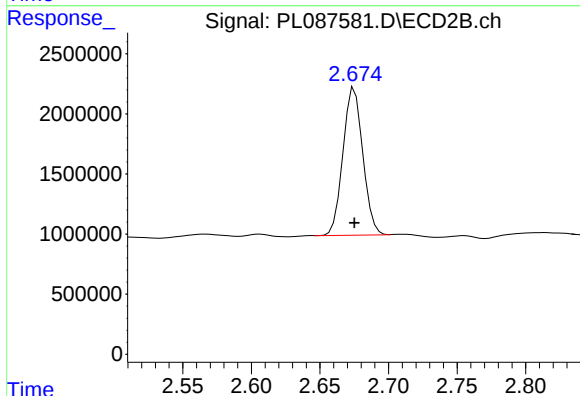


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: -0.001 min
Response: 12382728
Conc: 10.22 ng/ml m

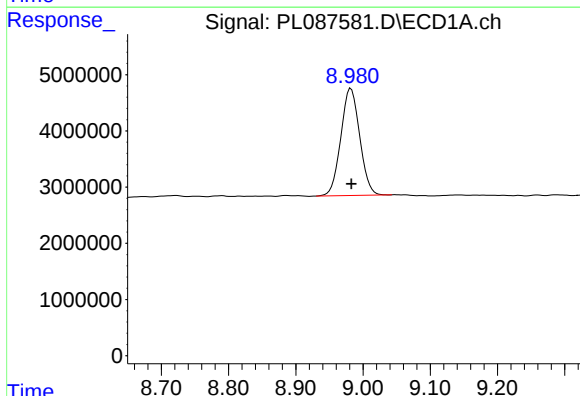

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 37106620
Conc: 13.03 ng/ml

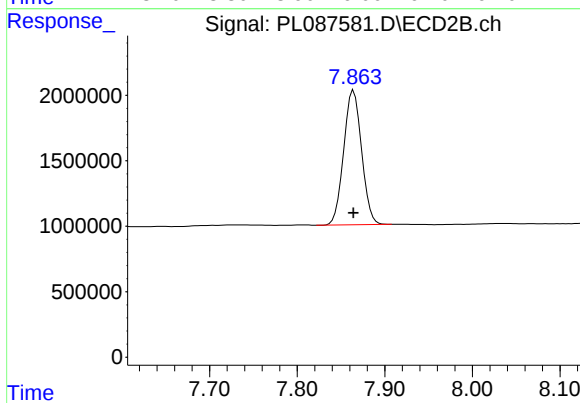

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 14579901
Conc: 11.51 ng/ml