

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122921\
 Data File : PL071714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2021 09:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 12:46:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.561	5.498	11788913	29357247	18.170	17.204
28)	SA Decachlor...	10.323	11.391	15239618	23252790	20.471	18.553
Target Compounds							
7)	B delta-BHC	0.000	6.975f	0	105445	N.D.	0.050 #
8)	B Heptachlo...	0.000	7.969	0	1202666	N.D.	0.611 #
10)	B gamma-Chl...	0.000	8.240	0	362507	N.D.	0.186 #
13)	MA Dieldrin	7.703f	0.000	140892	0	0.171	N.D. #
14)	MA Endrin	8.005f	8.907	508788	836995	0.684	0.555
15)	B Endosulfa...	0.000	9.158f	0	3350103	N.D.	2.253 #
19)	B Endosulfa...	0.000	9.506	0	121453	N.D.	0.086 #
24)	Chlordane-2	0.000	7.451f	0	42543	N.D.	0.577 #
25)	Chlordane-3	0.000	8.240	0	362507	N.D.	1.312 #
27)	Chlordane-5	0.000	9.175f	0	85436	N.D.	1.575 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122921\
Data File : PL071714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2021 09:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 12:46:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

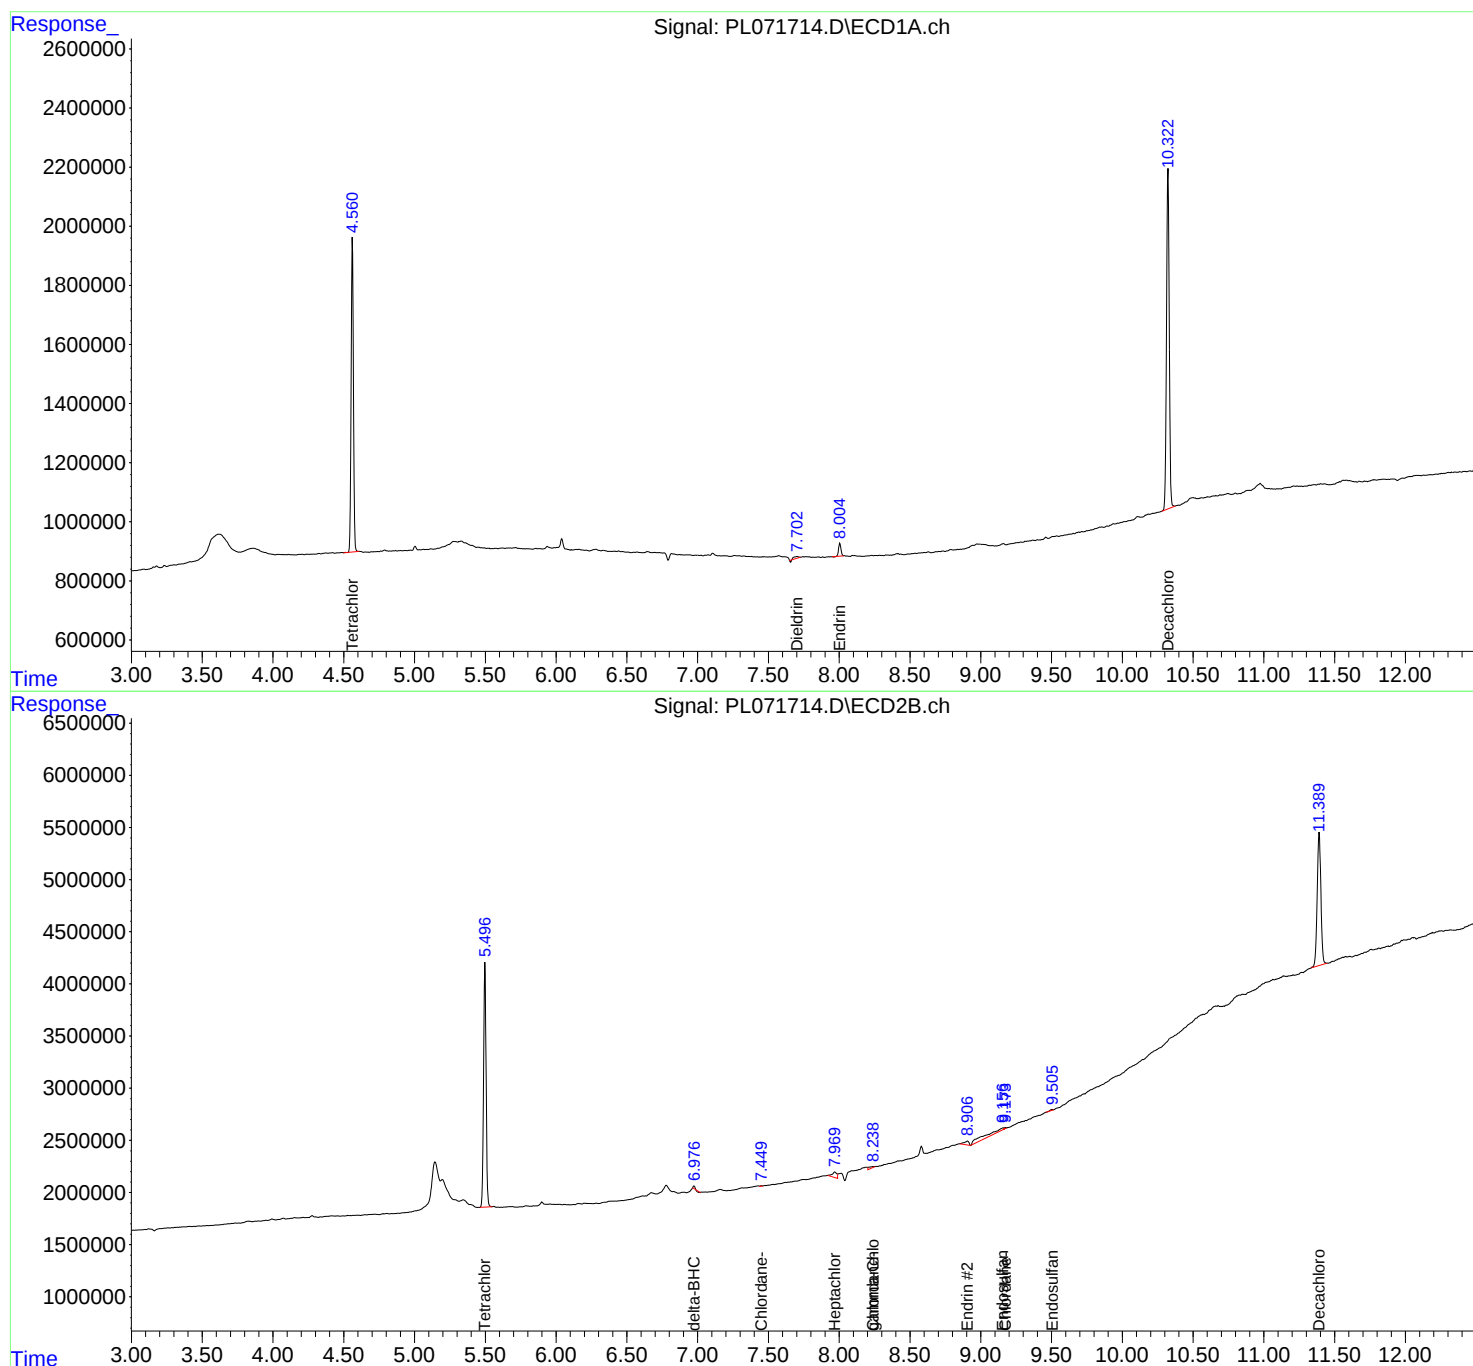


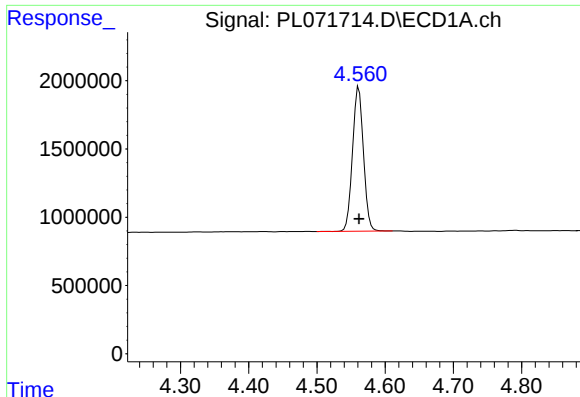

#1 Tetrachloro-m-xylene


R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 11788913
Conc: 18.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

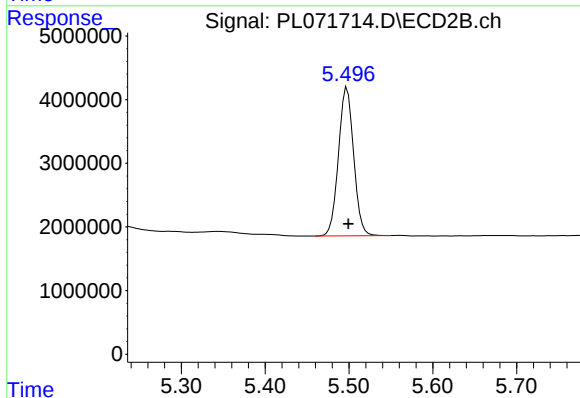


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: -0.002 min
Response: 29357247
Conc: 17.20 ng/ml

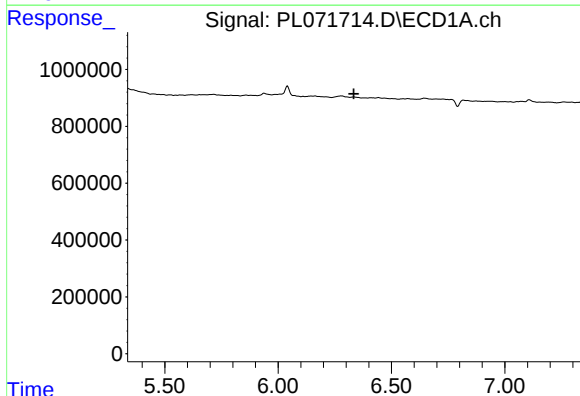


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.334 min
Response: 0
Conc: N.D.

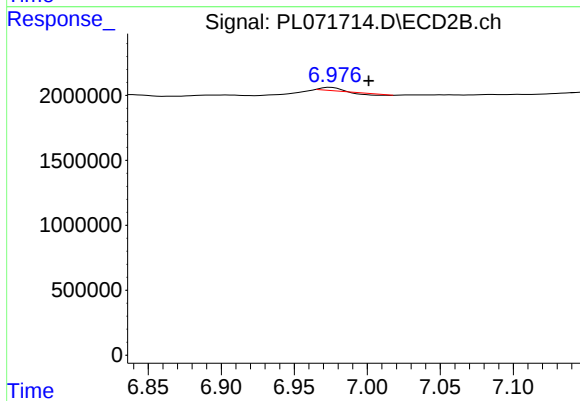

#7 delta-BHC


R.T.: 6.975 min
Delta R.T.: -0.026 min
Response: 105445
Conc: 0.05 ng/ml

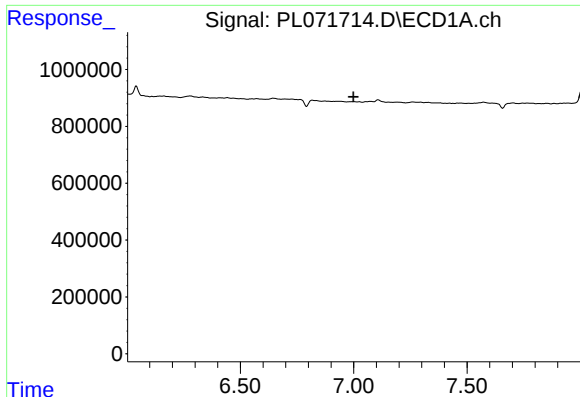

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.999 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

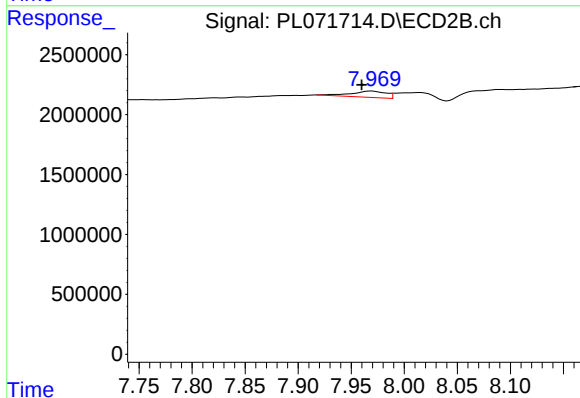


#8 Heptachlor epoxide

R.T.: 7.969 min
Delta R.T.: 0.009 min
Response: 1202666
Conc: 0.61 ng/ml

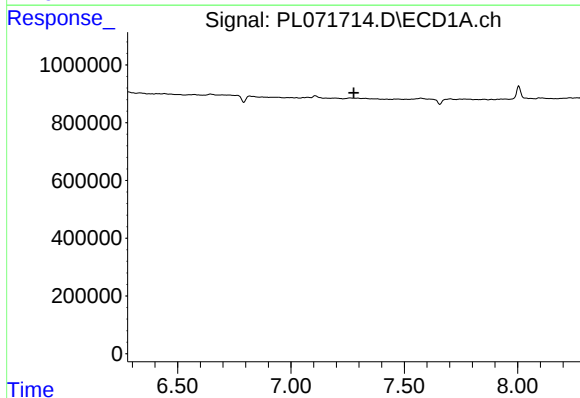


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

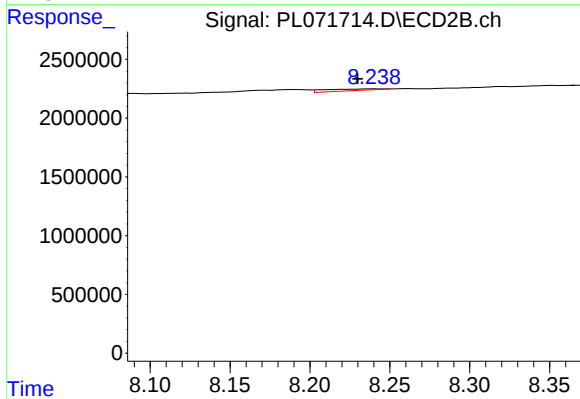

#10 gamma-Chlordane


R.T.: 8.240 min
Delta R.T.: 0.010 min
Response: 362507
Conc: 0.19 ng/ml

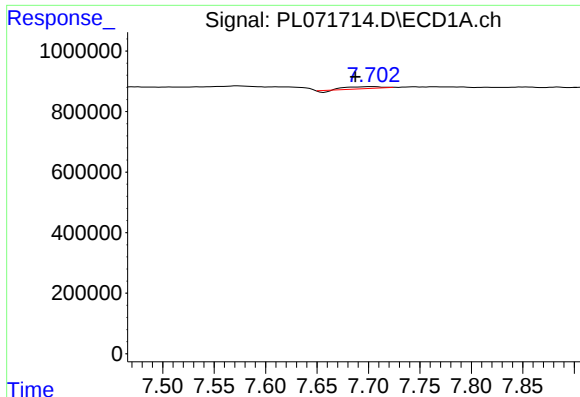

#13 Dieldrin


R.T.: 7.703 min
Delta R.T.: 0.016 min
Response: 140892
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

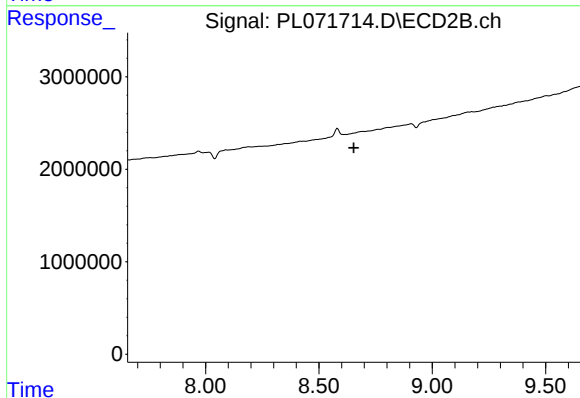


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.654 min
Response: 0
Conc: N.D.

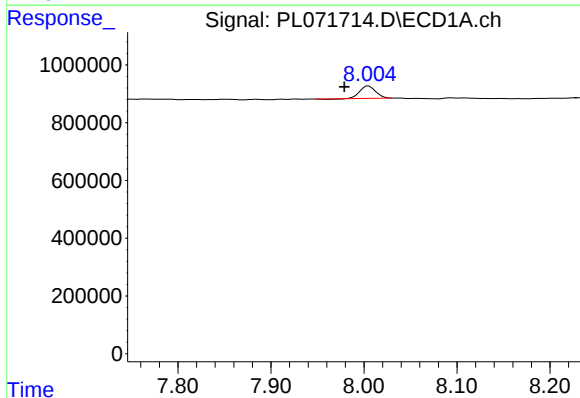


#14 Endrin

R.T.: 8.005 min
Delta R.T.: 0.026 min
Response: 508788
Conc: 0.68 ng/ml

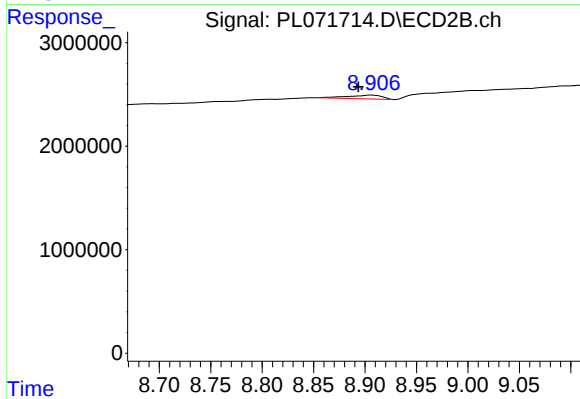

#14 Endrin


R.T.: 8.907 min
Delta R.T.: 0.014 min
Response: 836995
Conc: 0.56 ng/ml

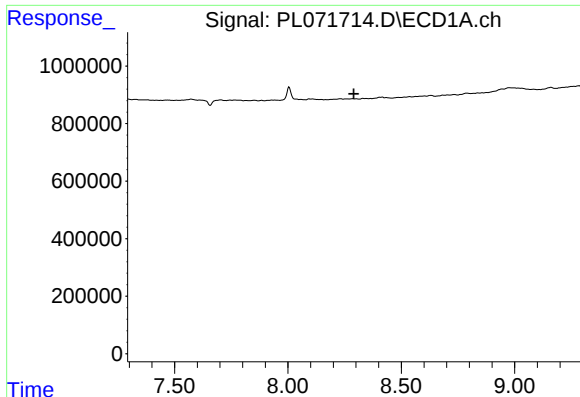

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

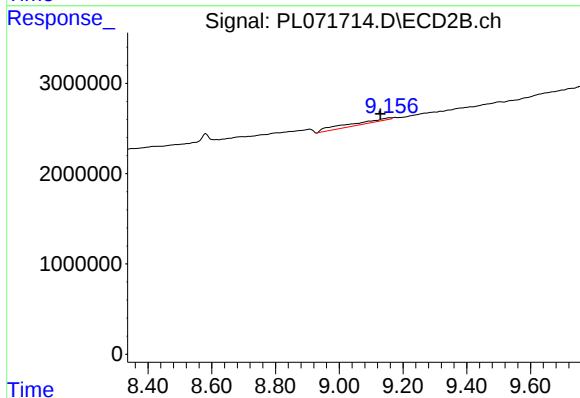


#15 Endosulfan II

R.T.: 9.158 min
Delta R.T.: 0.029 min
Response: 3350103
Conc: 2.25 ng/ml

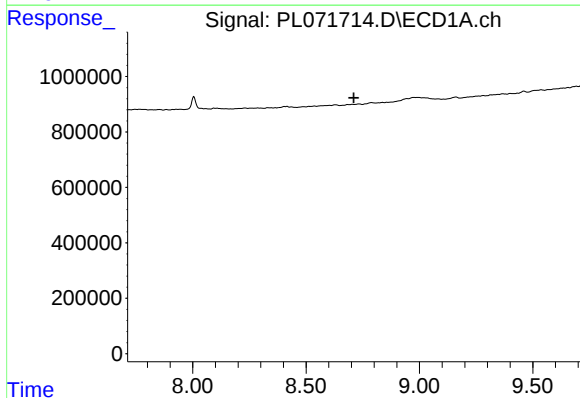


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

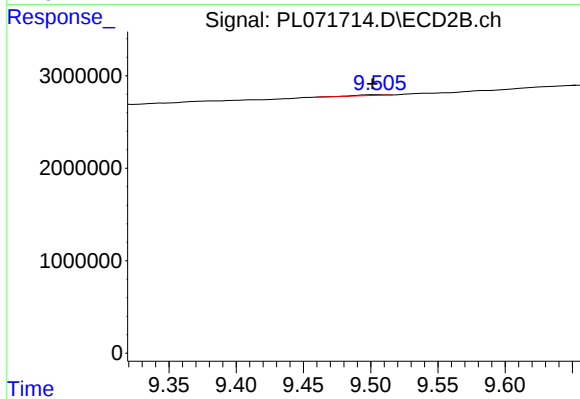

#19 Endosulfan Sulfate


R.T.: 9.506 min
Delta R.T.: 0.004 min
Response: 121453
Conc: 0.09 ng/ml

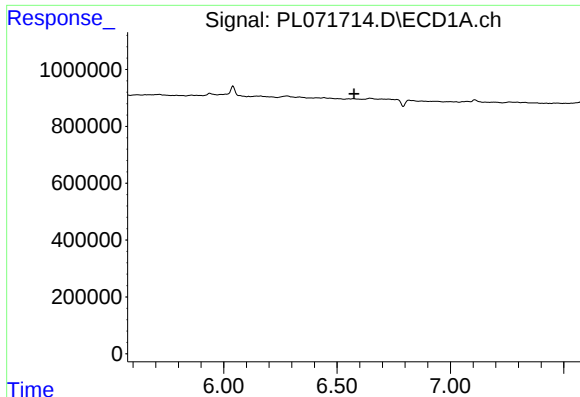

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

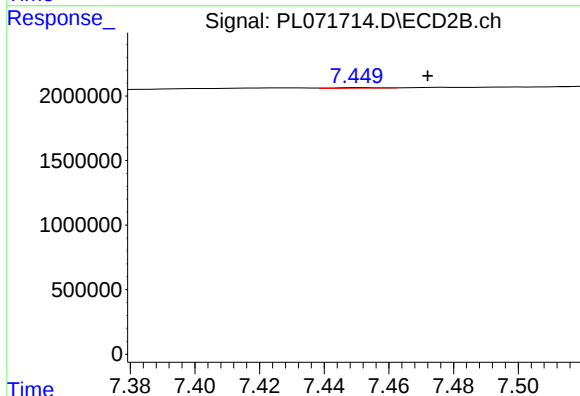


#24 Chlordane-2

R.T.: 7.451 min
Delta R.T.: -0.021 min
Response: 42543
Conc: 0.58 ng/ml

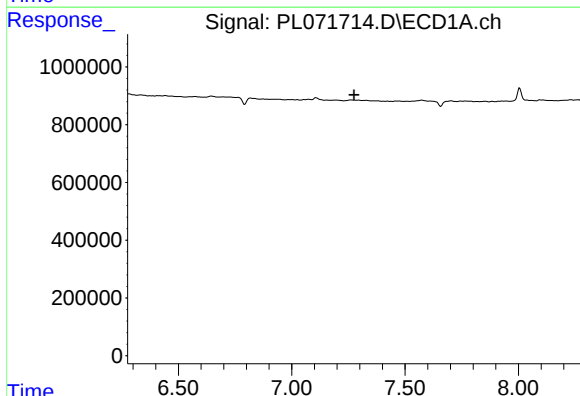


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

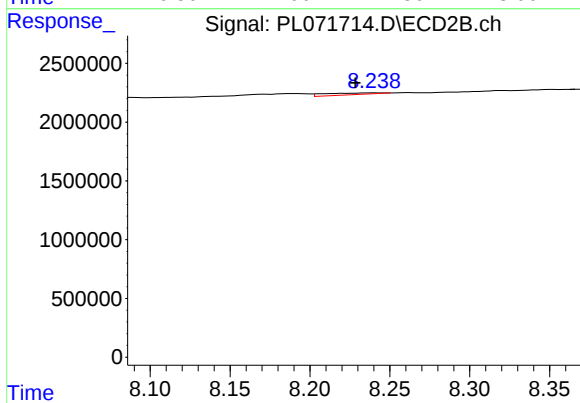

#25 Chlordane-3


R.T.: 8.240 min
Delta R.T.: 0.011 min
Response: 362507
Conc: 1.31 ng/ml

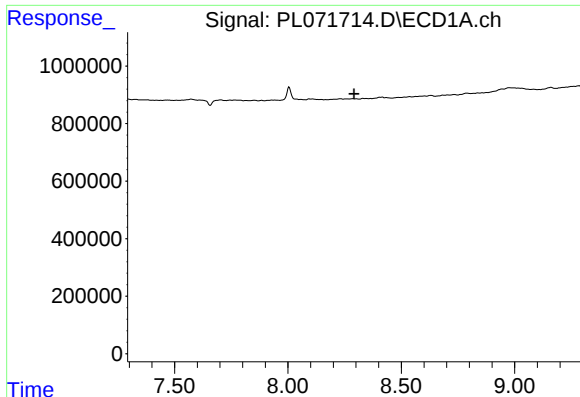

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.292 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

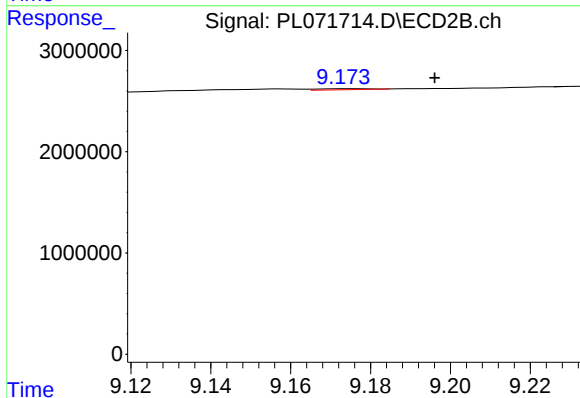


#27 Chlordane-5

R.T.: 9.175 min
Delta R.T.: -0.021 min
Response: 85436
Conc: 1.57 ng/ml

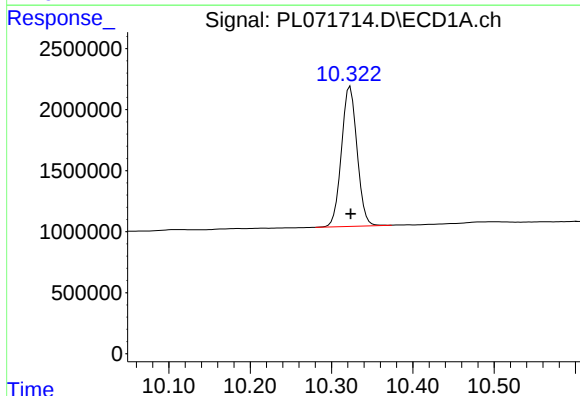

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: 0.000 min
Response: 15239618
Conc: 20.47 ng/ml

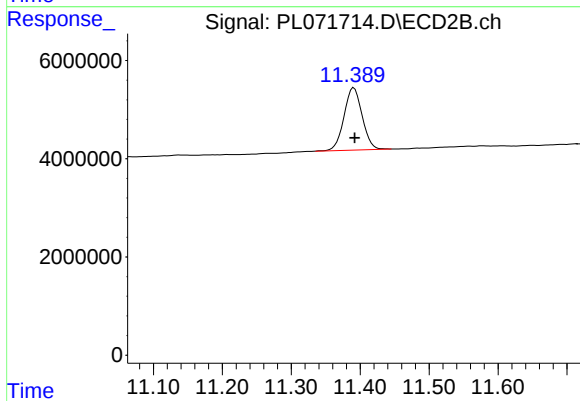

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: -0.001 min
Response: 23252790
Conc: 18.55 ng/ml