

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122921\
 Data File : PL071720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2021 12:10
 Operator : AR\AJ
 Sample : PB141745BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 12:47:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.566	5.498	11080196	27647562	17.078	16.202
28)	SA Decachlor...	10.327	11.394	15241165	23466324	20.473	18.724
Target Compounds							
4)	MA Heptachlor	0.000	7.147f	0	41408	N.D.	0.018 #
5)	MB Aldrin	0.000	7.485	0	116194	N.D.	0.053 #
7)	B delta-BHC	0.000	6.977f	0	243745	N.D.	0.116 #
10)	B gamma-Chl...	0.000	8.233	0	255406	N.D.	0.131 #
19)	B Endosulfa...	0.000	9.510	0	134716	N.D.	0.096 #
22)	Mirex	0.000	10.484f	0	28905	N.D.	0.027 #
24)	Chlordane-2	0.000	7.485	0	116194	N.D.	1.577 #
25)	Chlordane-3	0.000	8.233	0	255406	N.D.	0.924 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122921\
Data File : PL071720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2021 12:10
Operator : AR\AJ
Sample : PB141745BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 12:47:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

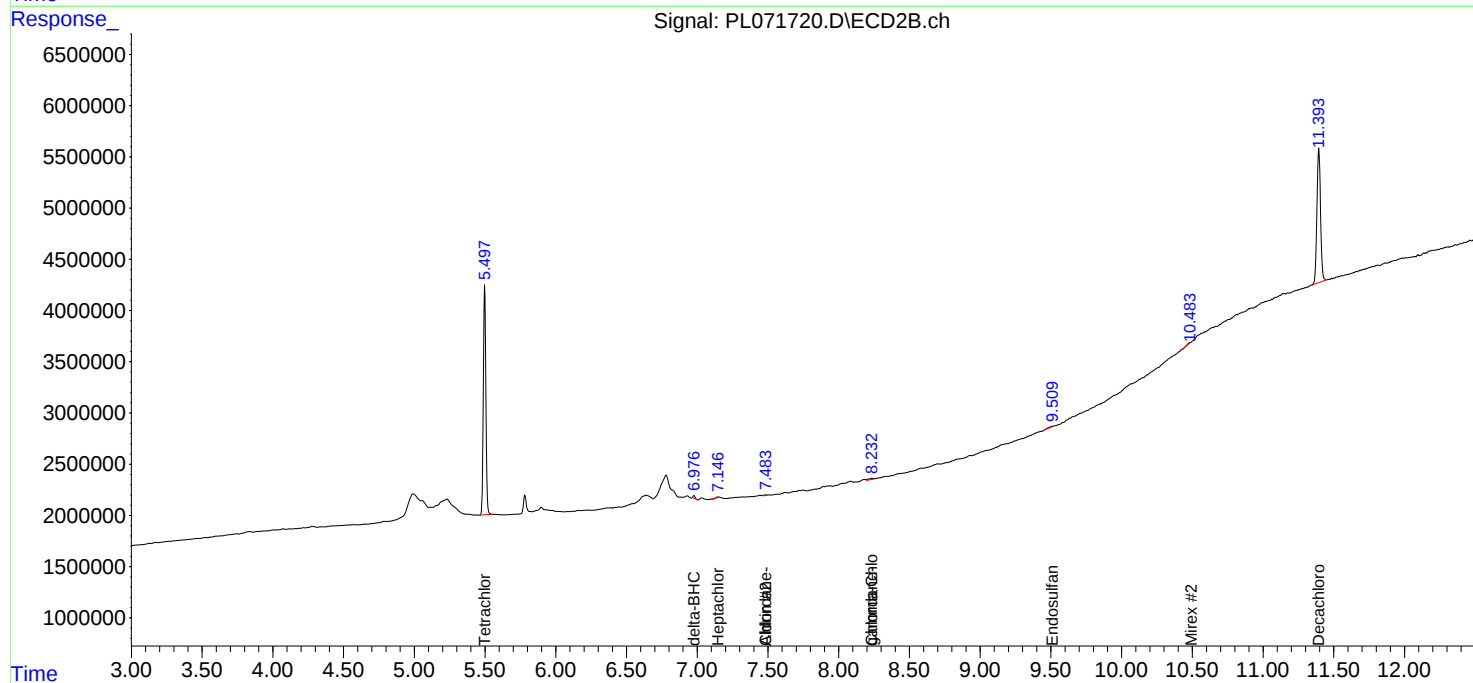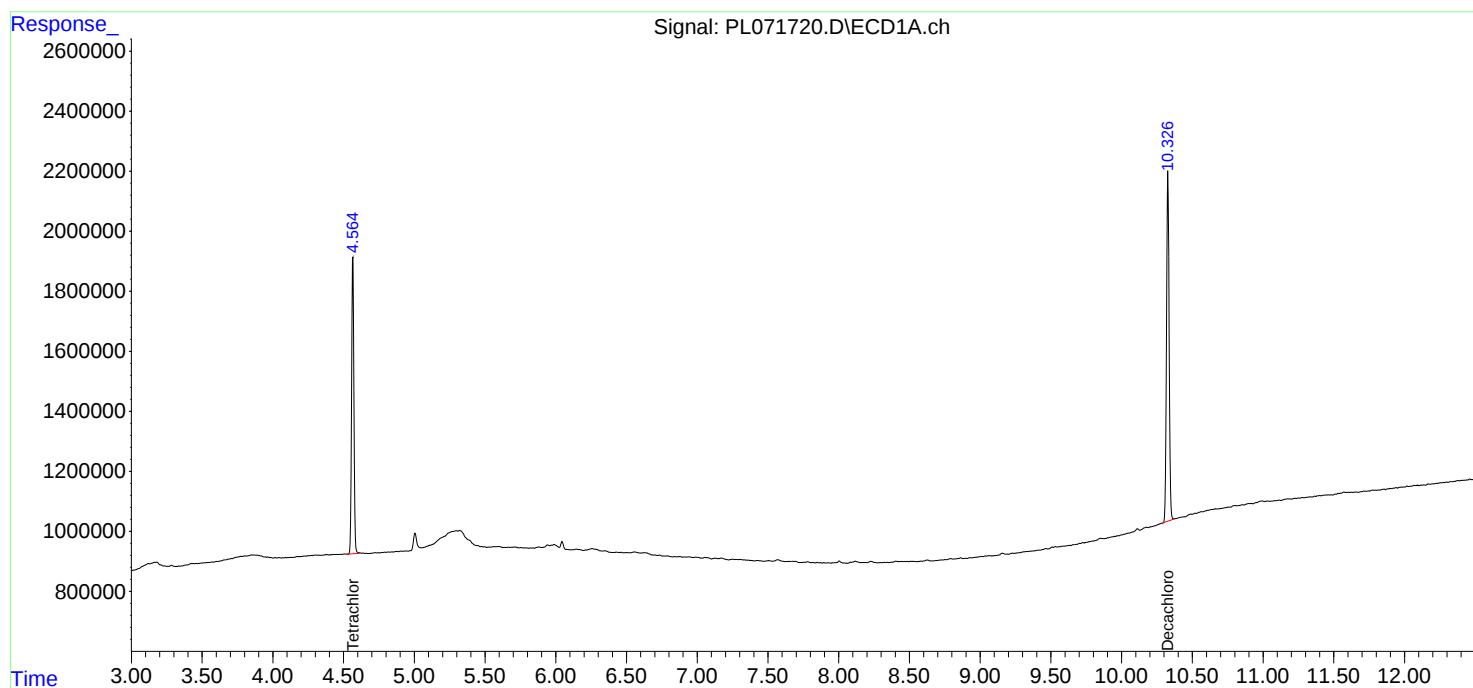


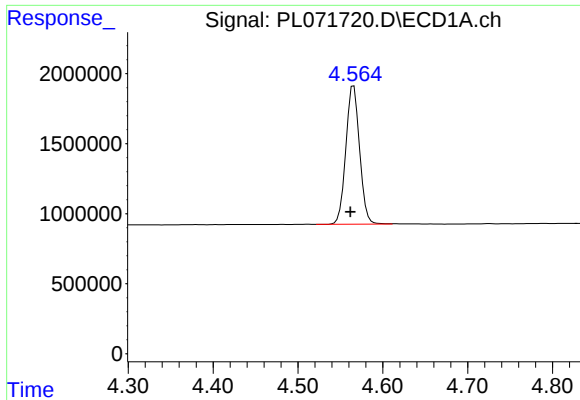

#1 Tetrachloro-m-xylene


R.T.: 4.566 min
Delta R.T.: 0.004 min
Response: 11080196
Conc: 17.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

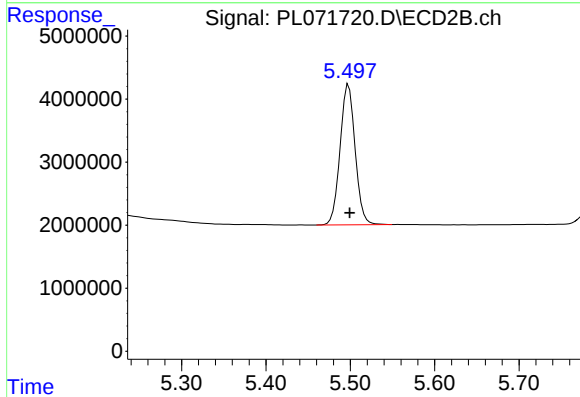


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: -0.001 min
Response: 27647562
Conc: 16.20 ng/ml

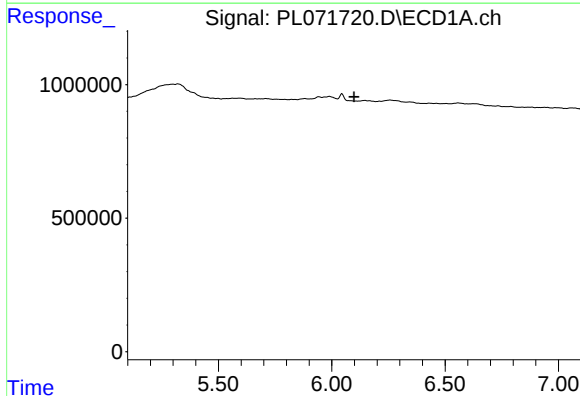


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

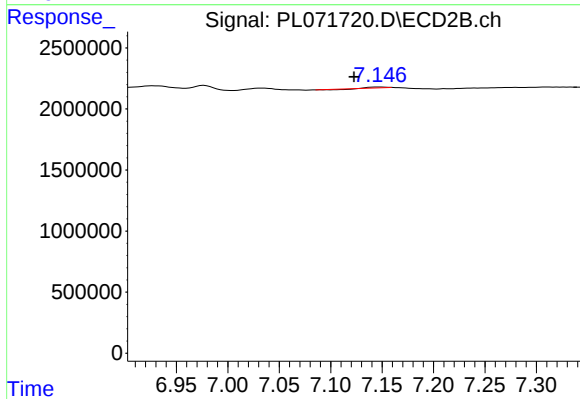

#4 Heptachlor


R.T.: 7.147 min
Delta R.T.: 0.024 min
Response: 41408
Conc: 0.02 ng/ml

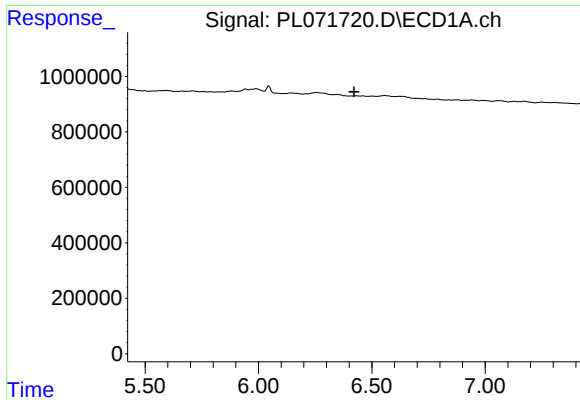

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

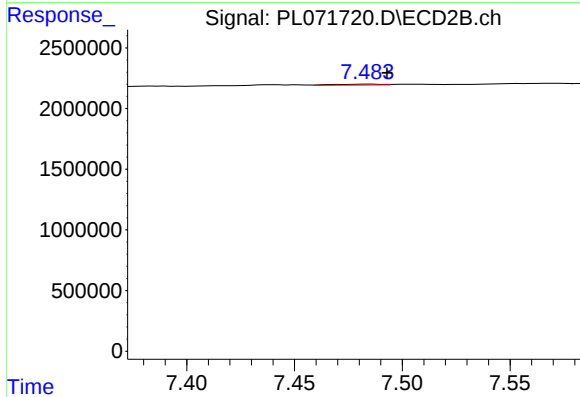


#5 Aldrin

R.T.: 7.485 min
Delta R.T.: -0.008 min
Response: 116194
Conc: 0.05 ng/ml

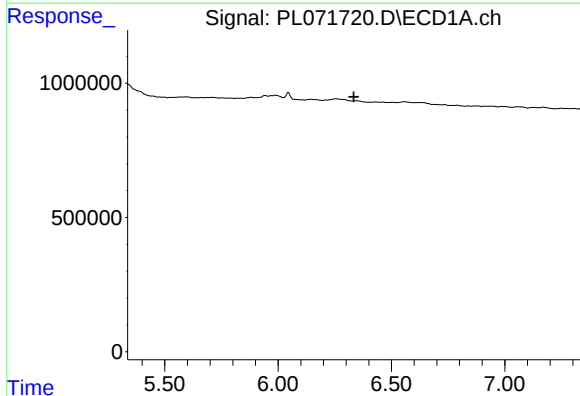


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.334 min
Response: 0
Conc: N.D.

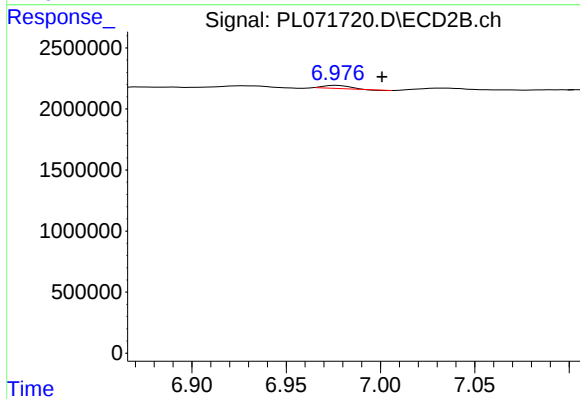

#7 delta-BHC


R.T.: 6.977 min
Delta R.T.: -0.024 min
Response: 243745
Conc: 0.12 ng/ml

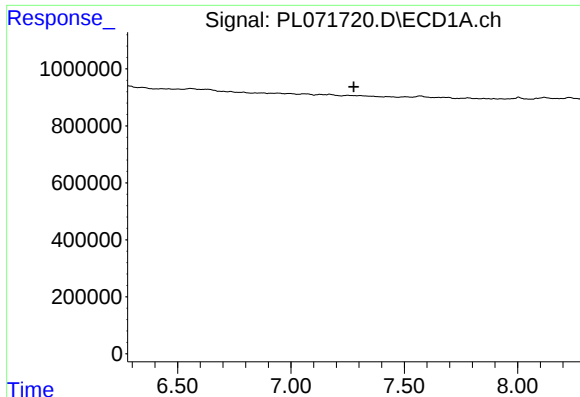

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

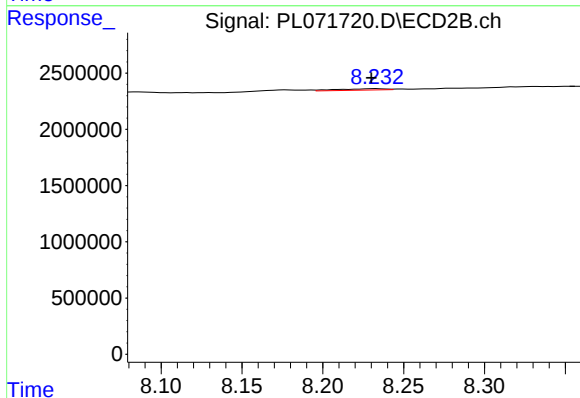


#10 gamma-Chlordane

R.T.: 8.233 min
Delta R.T.: 0.003 min
Response: 255406
Conc: 0.13 ng/ml

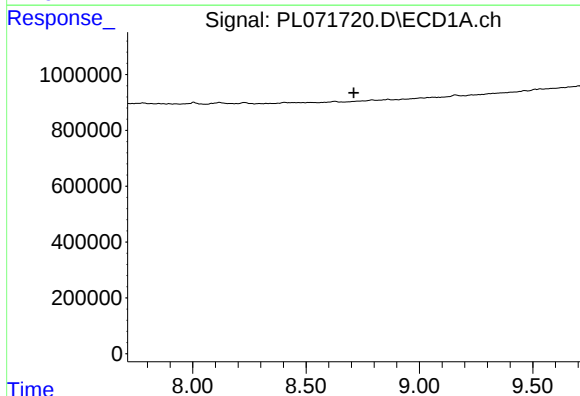


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

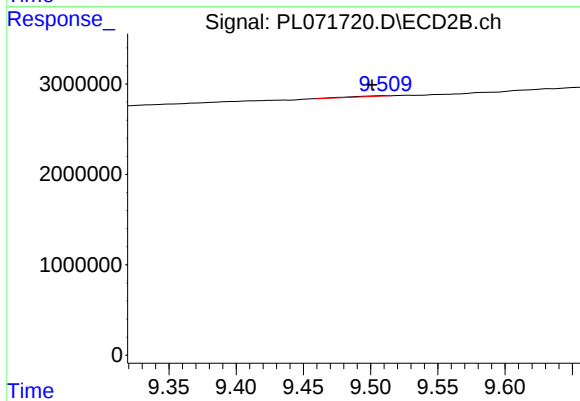

#19 Endosulfan Sulfate


R.T.: 9.510 min
Delta R.T.: 0.009 min
Response: 134716
Conc: 0.10 ng/ml

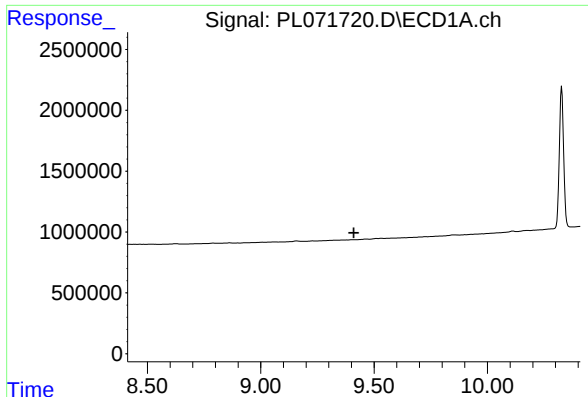

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

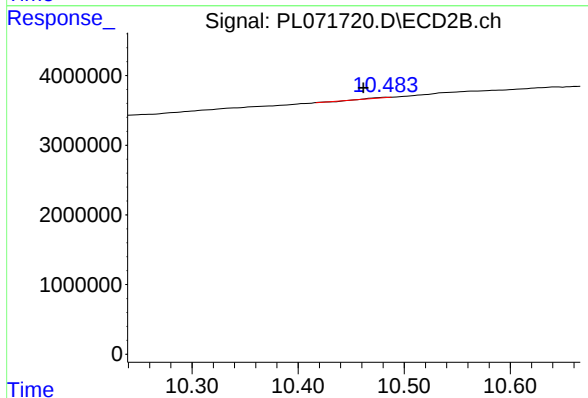


#22 Mirex

R.T.: 10.484 min
Delta R.T.: 0.023 min
Response: 28905
Conc: 0.03 ng/ml

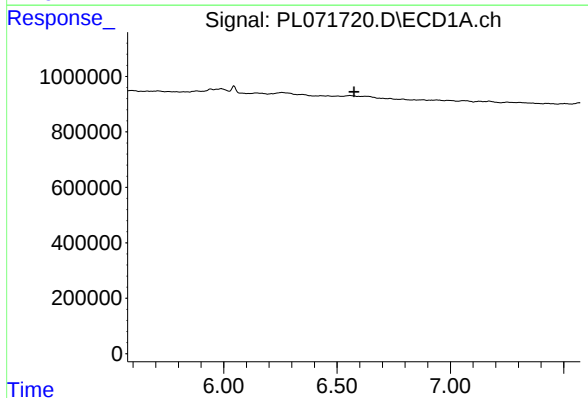


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

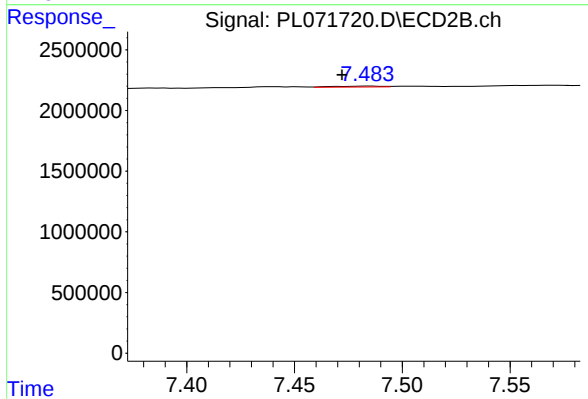

#24 Chlordane-2


R.T.: 7.485 min
Delta R.T.: 0.013 min
Response: 116194
Conc: 1.58 ng/ml

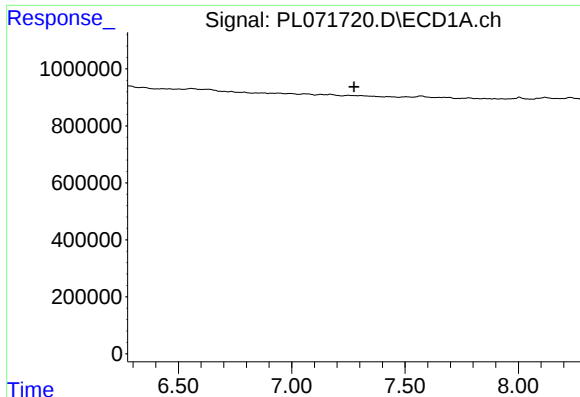

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

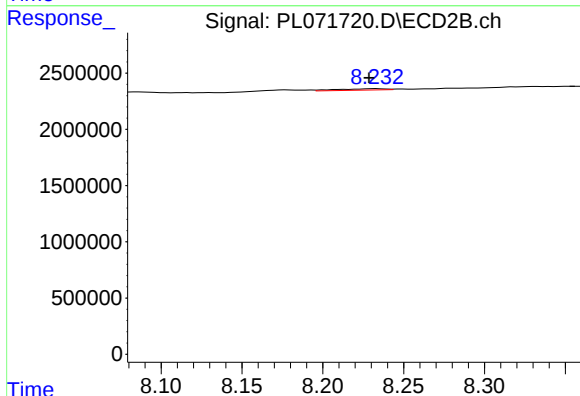


#25 Chlordane-3

R.T.: 8.233 min
Delta R.T.: 0.005 min
Response: 255406
Conc: 0.92 ng/ml

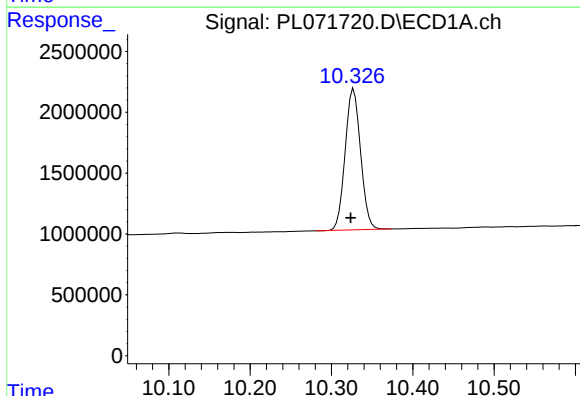

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.004 min
Response: 15241165
Conc: 20.47 ng/ml

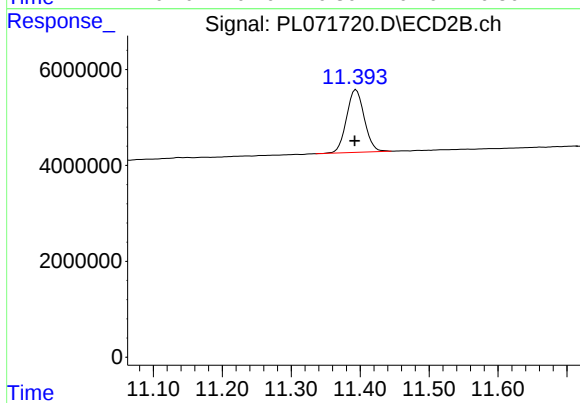

#28 Decachlorobiphenyl

R.T.: 11.394 min
Delta R.T.: 0.002 min
Response: 23466324
Conc: 18.72 ng/ml