

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122921\
 Data File : PL071717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2021 10:08
 Operator : AR\AJ
 Sample : M5219-01 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 M21013-N48854-1040

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/30/2021
 Supervised By :mohammad ahmed 12/30/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 12:46:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.567	5.495	1534757	5947208	2.366	3.485m#
28) SA Decachlor...	10.328	11.394	2248596	3665242	3.020	2.924

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122921\
Data File : PL071717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2021 10:08
Operator : AR\AJ
Sample : M5219-01 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
M21013-N48854-1040


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/30/2021
Supervised By :mohammad ahmed 12/30/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 12:46:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

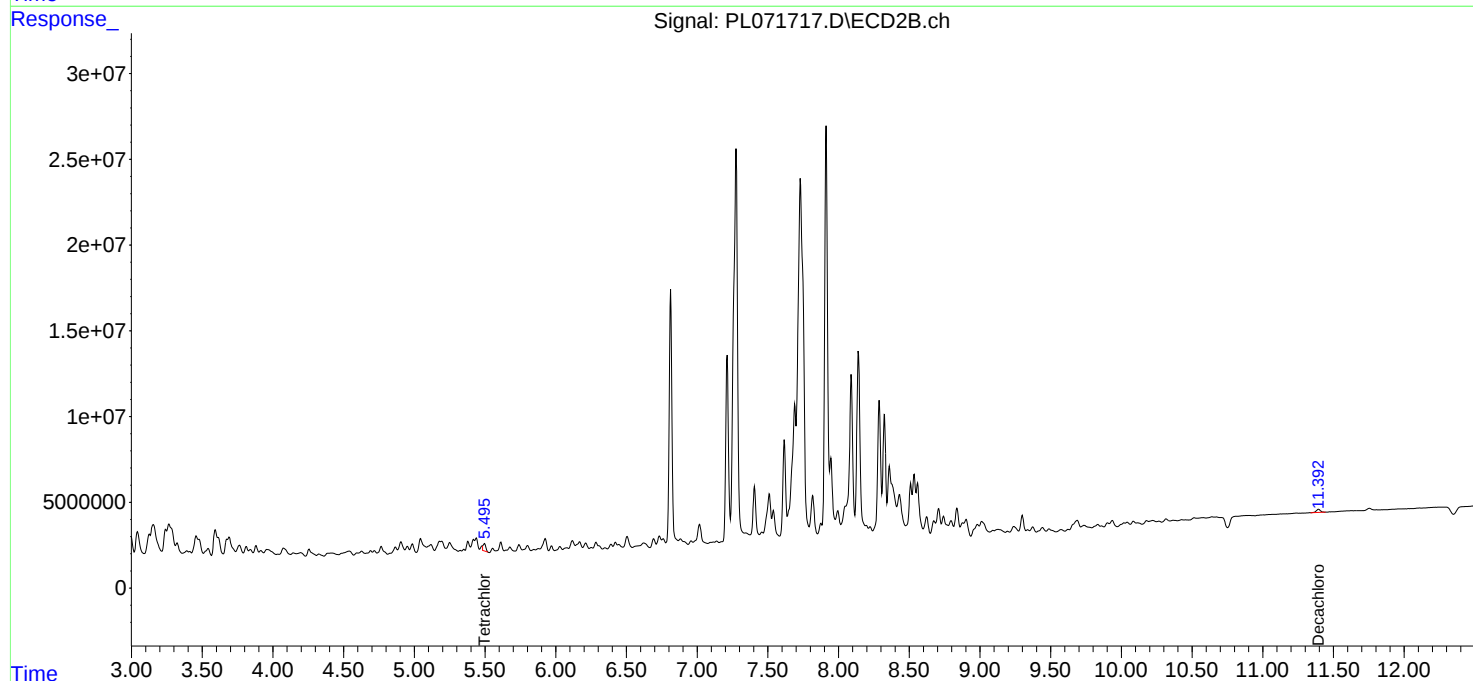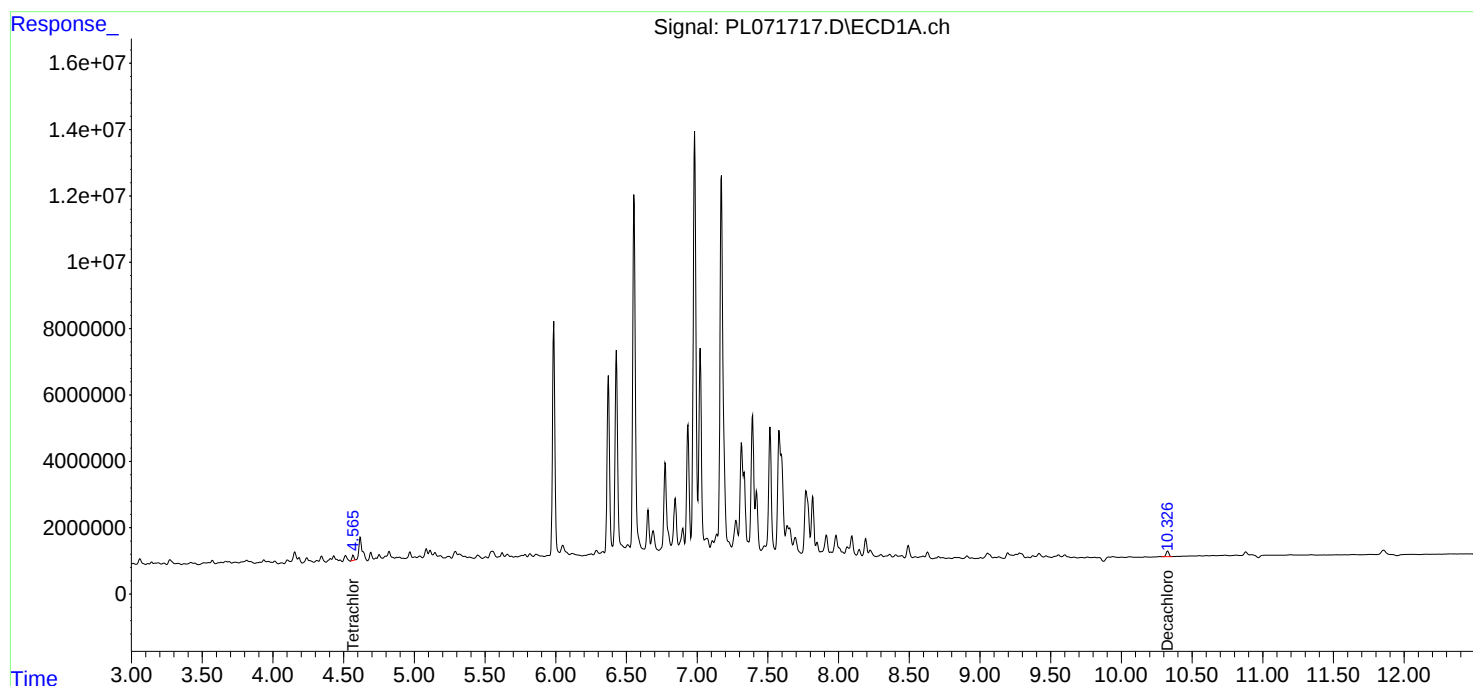

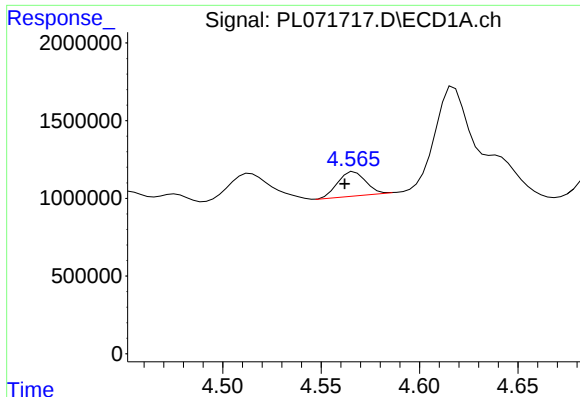


#1 Tetrachloro-m-xylene

R.T.: 4.567 min
Delta R.T.: 0.005 min
Response: 1534757
Conc: 2.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
M21013-N48854-1040


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/30/2021
Supervised By :mohammad ahmed 12/30/2021

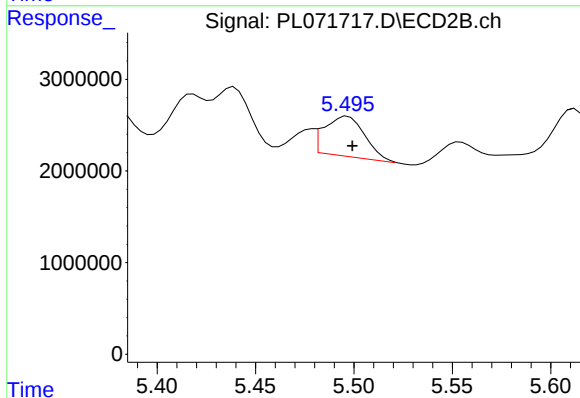


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: -0.004 min
Response: 5947208
Conc: 3.49 ng/ml m

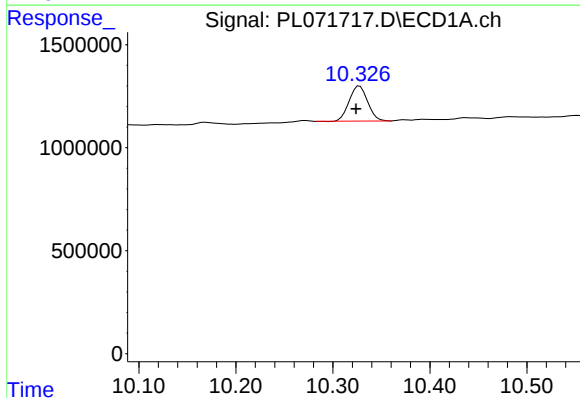

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.004 min
Response: 2248596
Conc: 3.02 ng/ml

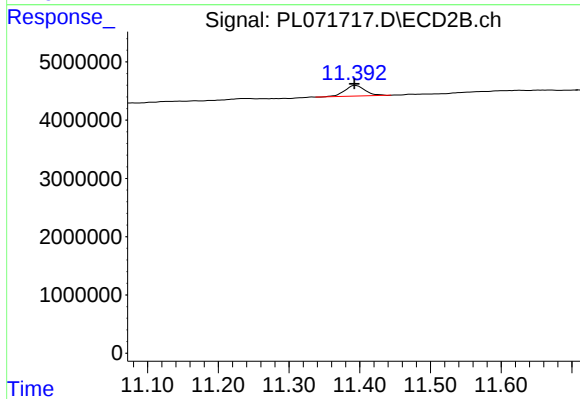

#28 Decachlorobiphenyl

R.T.: 11.394 min
Delta R.T.: 0.002 min
Response: 3665242
Conc: 2.92 ng/ml