

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122921\
 Data File : PL071722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2021 13:47
 Operator : AR\AJ
 Sample : M5241-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2S

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/30/2021
 Supervised By :mohammad ahmed 12/30/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 16:30:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.562	5.498	6997786	15809238	10.786	9.265m
2) SA Decachlor...	10.323	11.392	8935752	15021931	12.003	11.986

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122921\
Data File : PL071722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2021 13:47
Operator : AR\AJ
Sample : M5241-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-2S


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/30/2021
Supervised By :mohammad ahmed 12/30/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 16:30:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

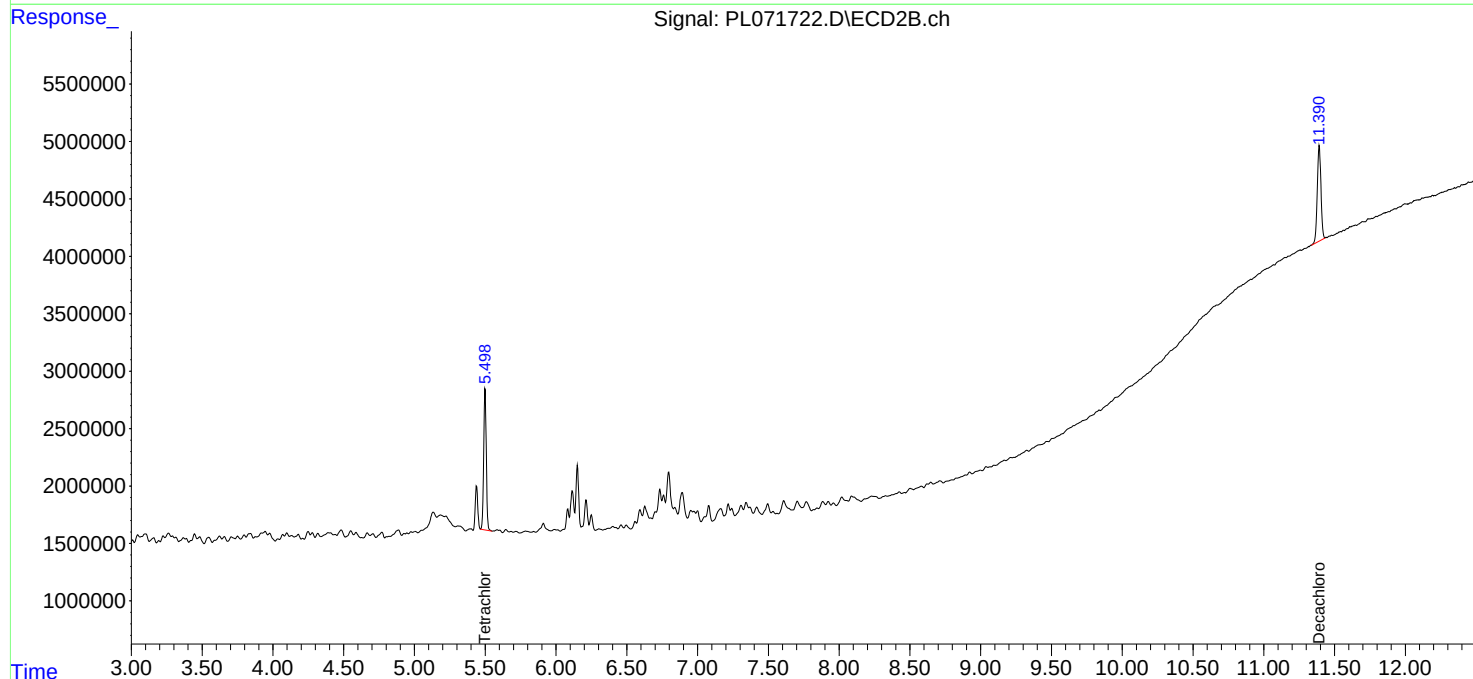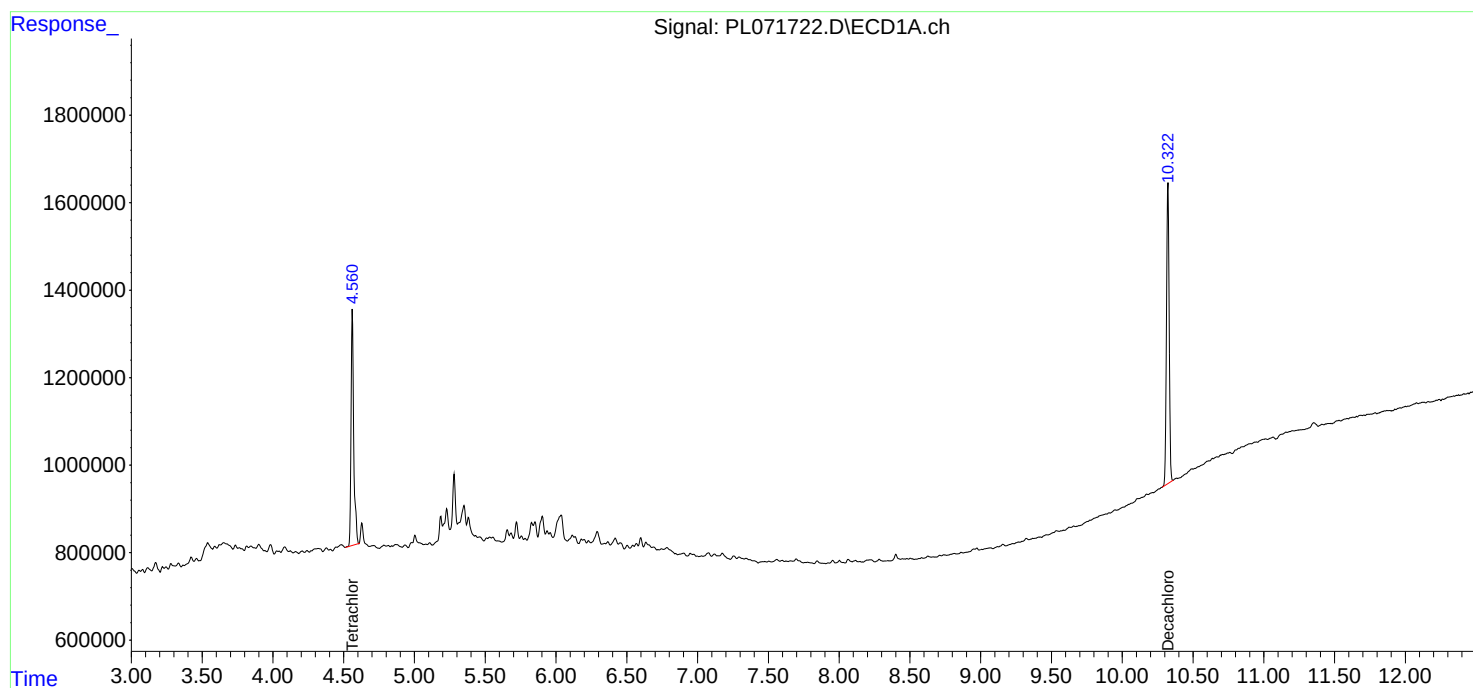

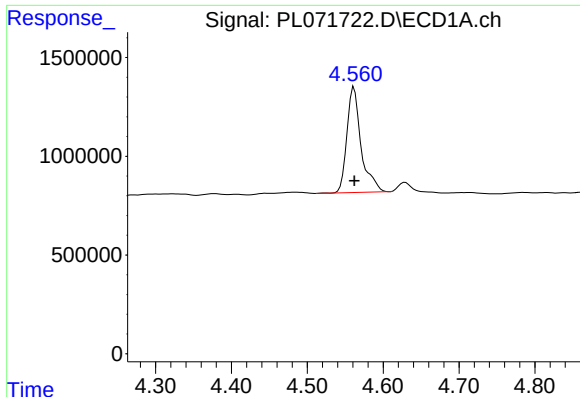


#1 Tetrachloro-m-xylene

R.T.: 4.562 min
Delta R.T.: 0.000 min
Response: 6997786
Conc: 10.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2S


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/30/2021
Supervised By :mohammad ahmed 12/30/2021

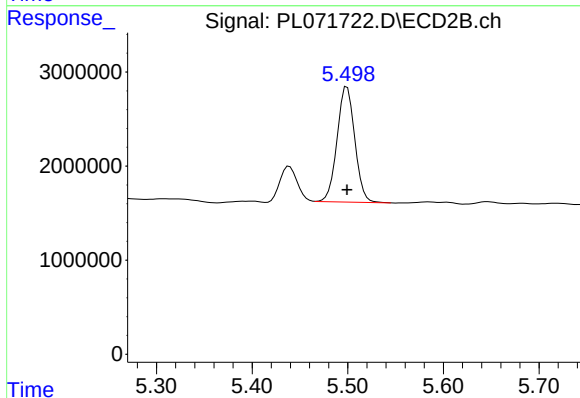


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: -0.001 min
Response: 15809238
Conc: 9.26 ng/ml m

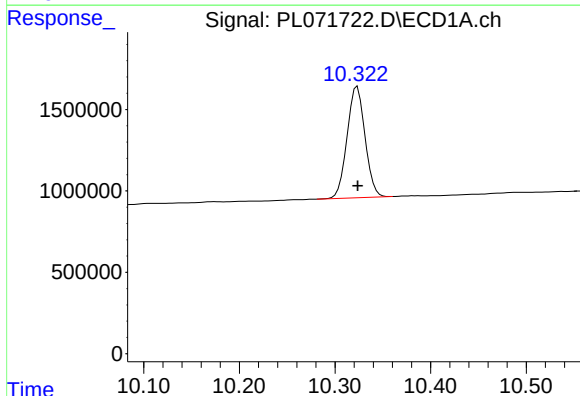

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: 0.000 min
Response: 8935752
Conc: 12.00 ng/ml

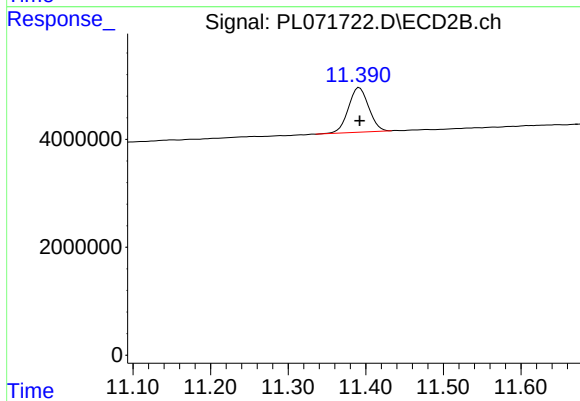

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 15021931
Conc: 11.99 ng/ml