

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123019\
 Data File : PL055373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2019 15:23
 Operator : SG\AJ
 Sample : K6442-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 00:53:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.048	152.2E6	38987120	14.471	14.755
28)	SA Decachlor...	8.314	9.150	116.5E6	32953354	12.558	14.928
Target Compounds							
23)	Chlordane-1	4.417	0.000	6356115	0	16.710	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123019\
Data File : PL055373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2019 15:23
Operator : SG\AJ
Sample : K6442-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 00:53:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

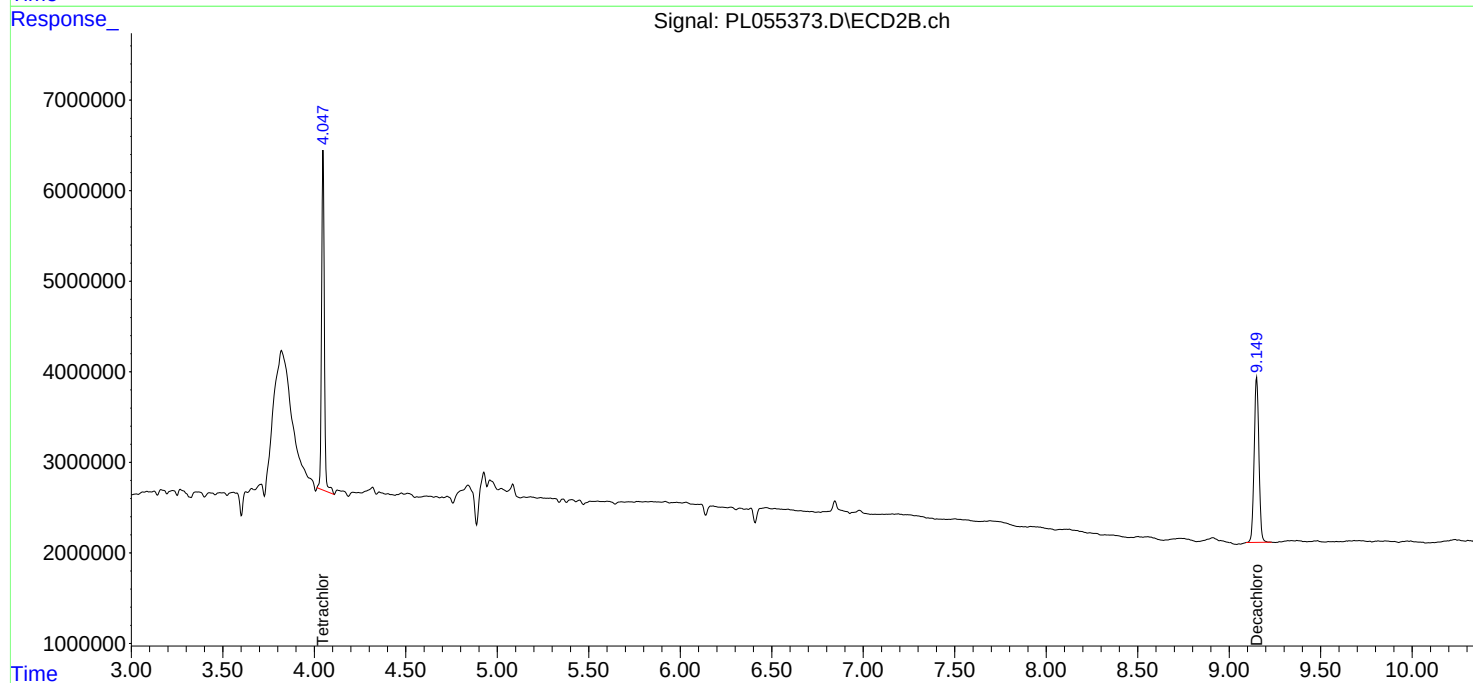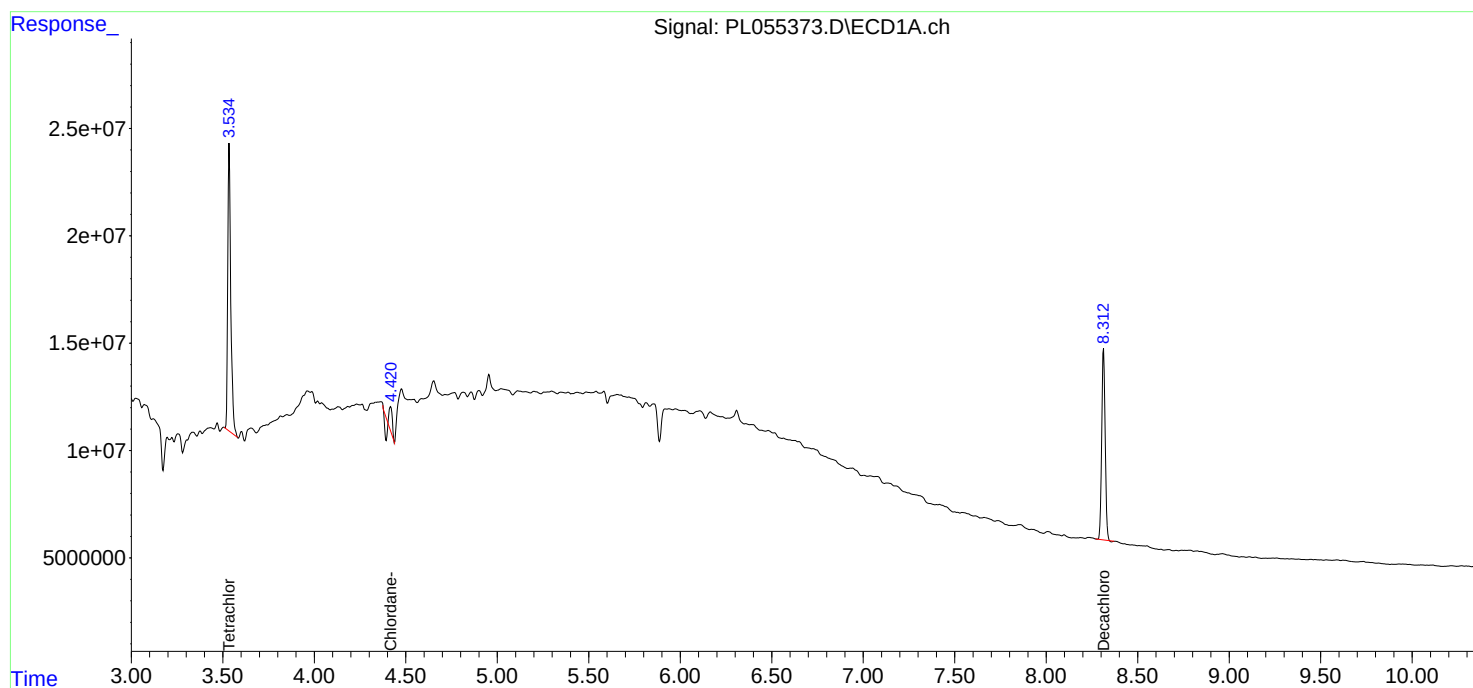


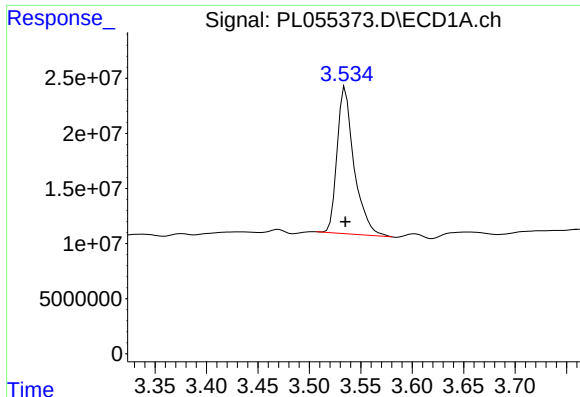

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 152185623
Conc: 14.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

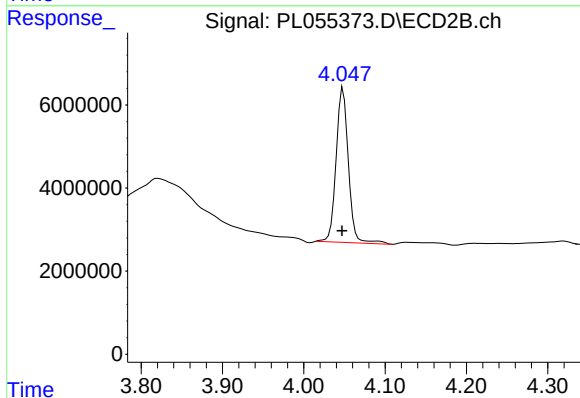


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.001 min
Response: 38987120
Conc: 14.76 ng/ml

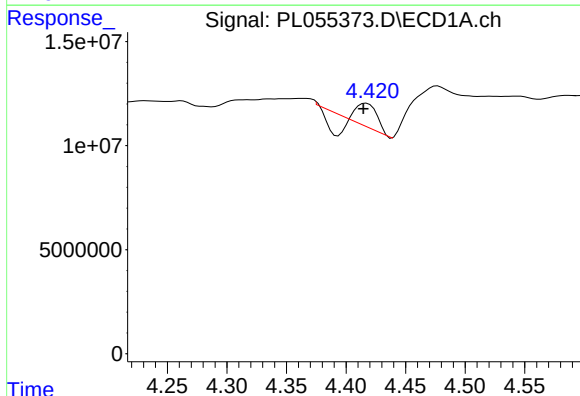


#23 Chlordane-1

R.T.: 4.417 min
Delta R.T.: 0.003 min
Response: 6356115
Conc: 16.71 ng/ml

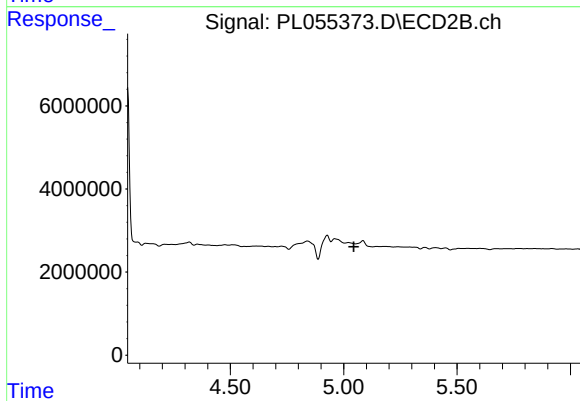

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.044 min
Response: 0
Conc: N.D.

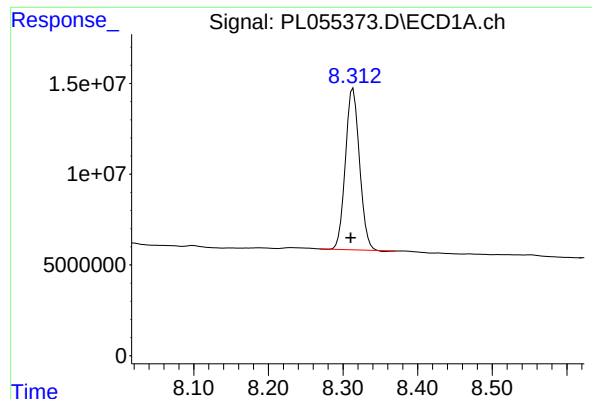

#28 Decachlorobiphenyl

R.T.: 8.314 min
Delta R.T.: 0.003 min
Response: 116523115
Conc: 12.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

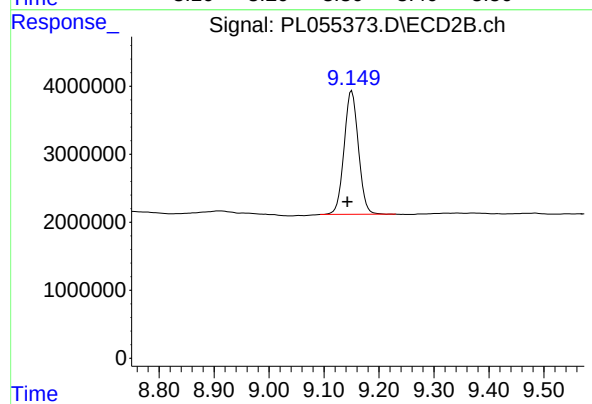

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: 0.008 min
Response: 32953354
Conc: 14.93 ng/ml