

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123019\
 Data File : PL055386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2019 18:58
 Operator : SG\AJ
 Sample : K6463-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 00:55:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	139.9E6	39167418	13.307	14.823
28)	SA Decachlor...	8.315	9.151	152.6E6	40994195	16.442	18.571
Target Compounds							
6)	B beta-BHC	4.487f	0.000	22411576	0	3.268	N.D. #
10)	B gamma-Chl...	0.000	6.163	0	2489107	N.D.	0.938 #
11)	B alpha-Chl...	0.000	6.237	0	5657835	N.D.	2.158 #
12)	B 4,4'-DDE	5.715	6.392	40336879	8847613	3.027	3.629
16)	A 4,4'-DDD	0.000	6.887	0	2497475	N.D.	1.314 #
17)	MA 4,4'-DDT	6.474	7.184	18500773	3826593	1.838	1.950
22)	Mirex	0.000	8.276f	0	2041133	N.D.	1.231 #
25)	Chlordane-3	0.000	6.163	0	2489107	N.D.	7.735 #
26)	Chlordane-4	0.000	6.237	0	5657835	N.D.	14.719 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123019\
Data File : PL055386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2019 18:58
Operator : SG\AJ
Sample : K6463-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 00:55:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

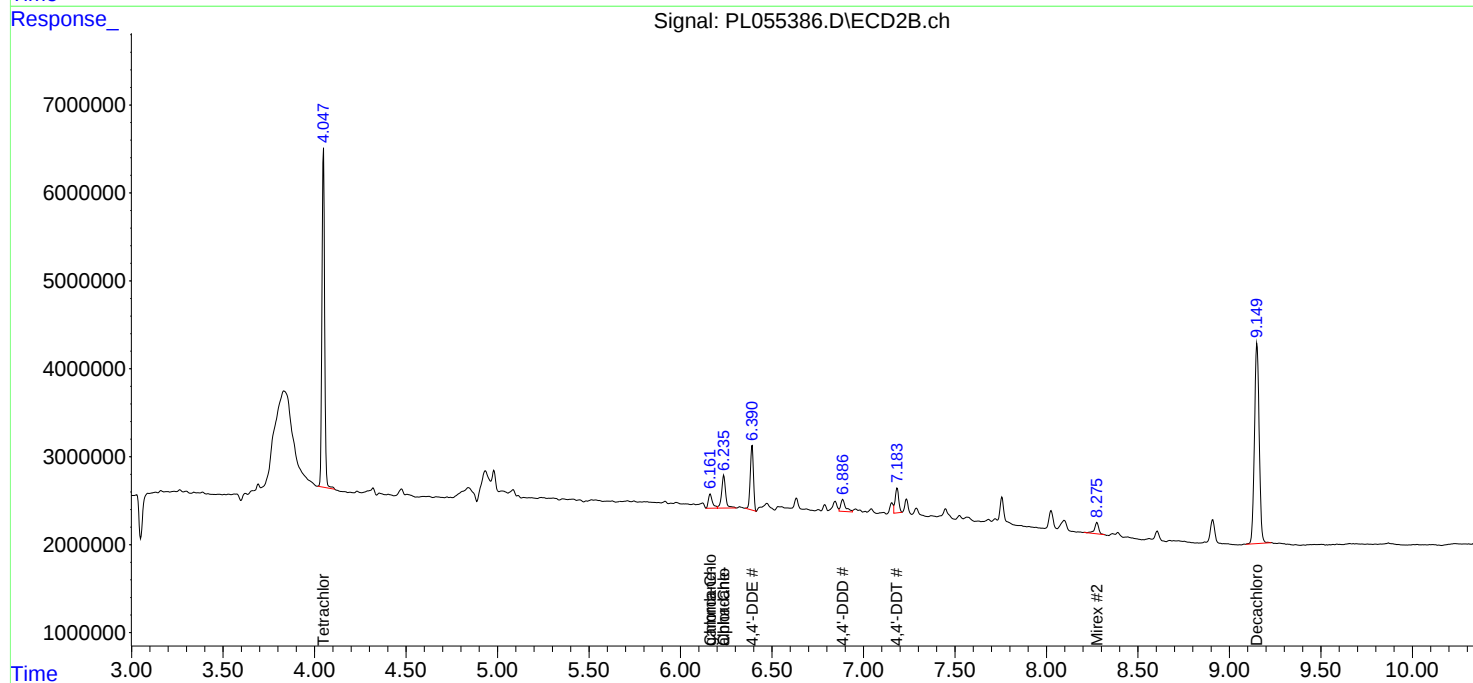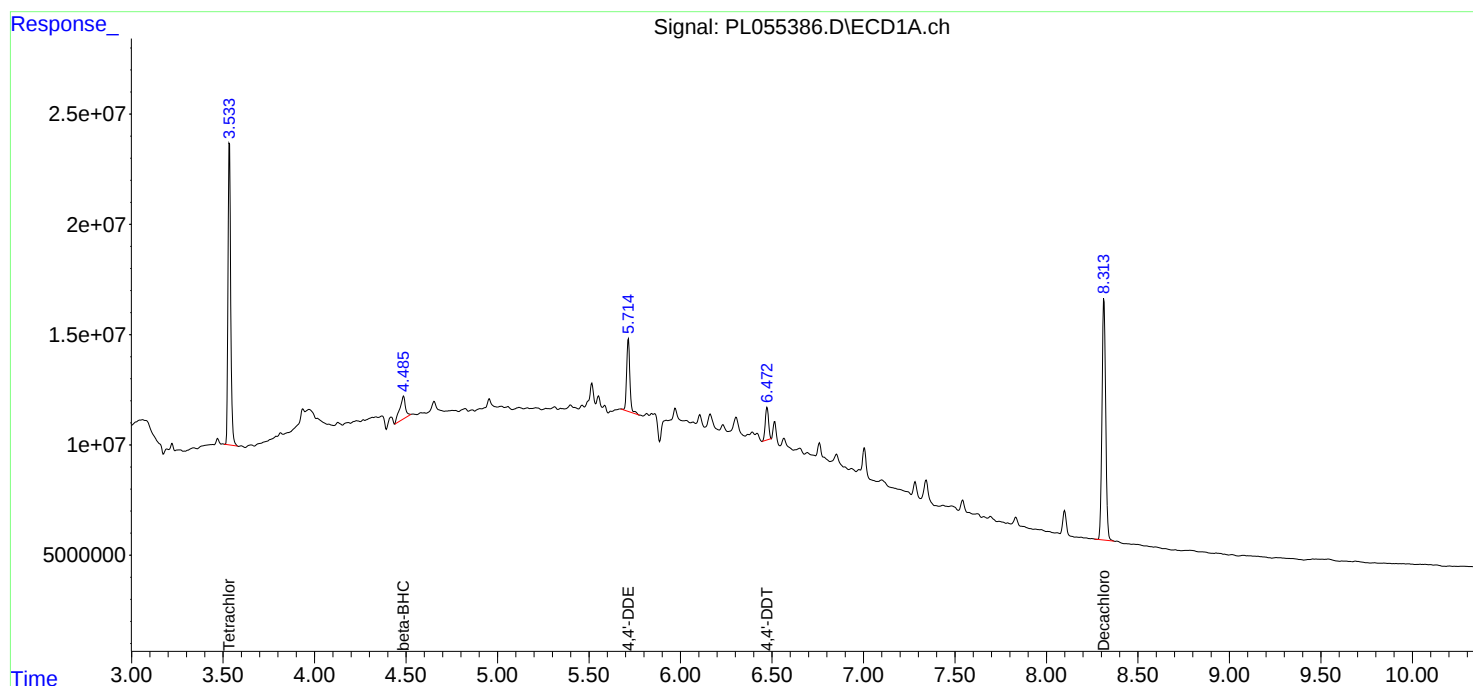


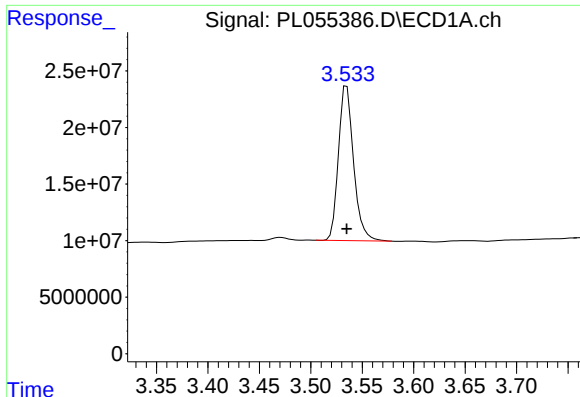

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 139940808
Conc: 13.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

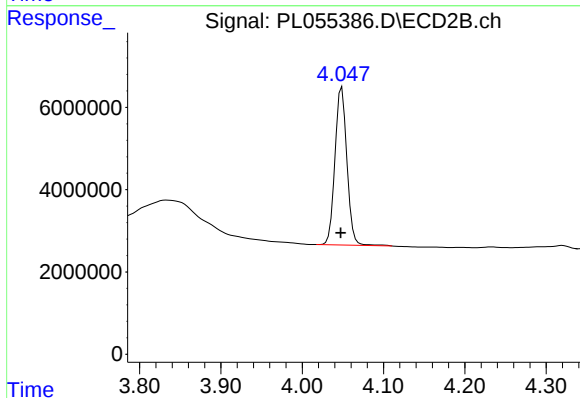


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 39167418
Conc: 14.82 ng/ml

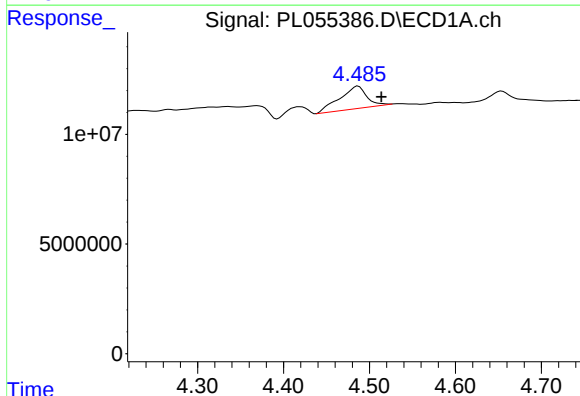


#6 beta-BHC

R.T.: 4.487 min
Delta R.T.: -0.027 min
Response: 22411576
Conc: 3.27 ng/ml

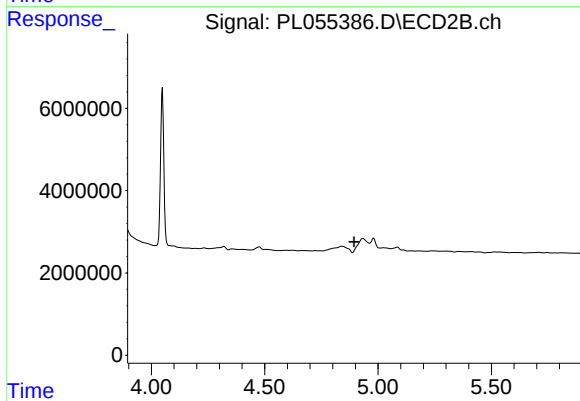

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.895 min
Response: 0
Conc: N.D.

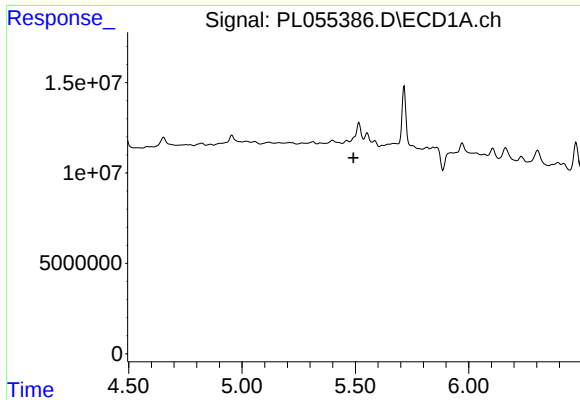

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

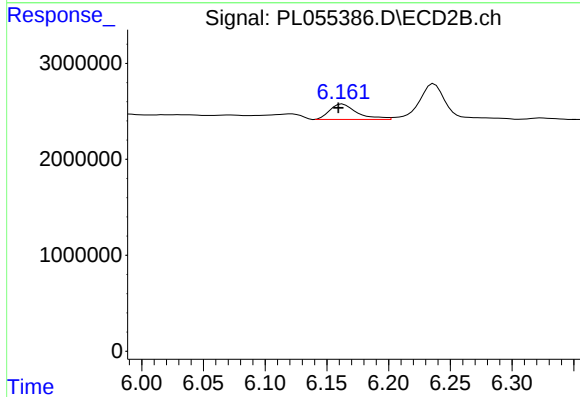


#10 gamma-Chlordane

R.T.: 6.163 min
Delta R.T.: 0.003 min
Response: 2489107
Conc: 0.94 ng/ml

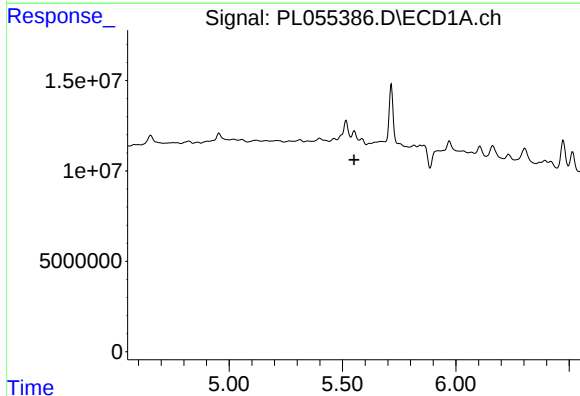


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.551 min
Response: 0
Conc: N.D.

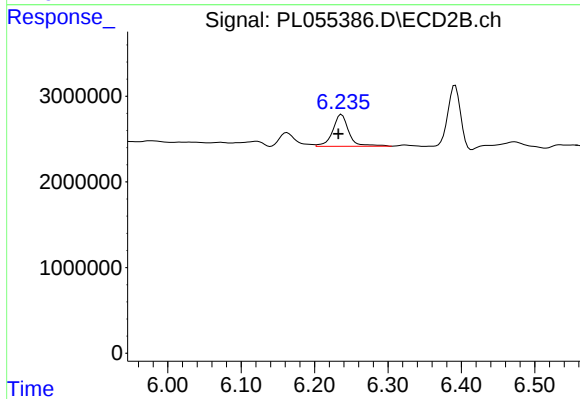

#11 alpha-Chlordane


R.T.: 6.237 min
Delta R.T.: 0.004 min
Response: 5657835
Conc: 2.16 ng/ml

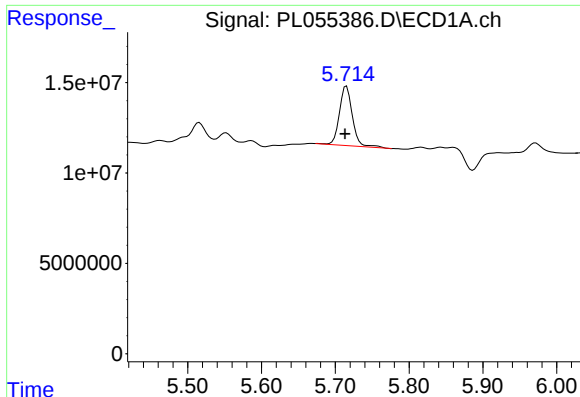

#12 4,4'-DDE


R.T.: 5.715 min
Delta R.T.: 0.002 min
Response: 40336879
Conc: 3.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

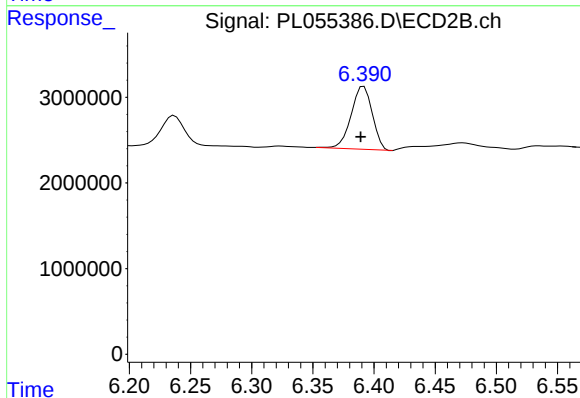


#12 4,4'-DDE

R.T.: 6.392 min
Delta R.T.: 0.003 min
Response: 8847613
Conc: 3.63 ng/ml

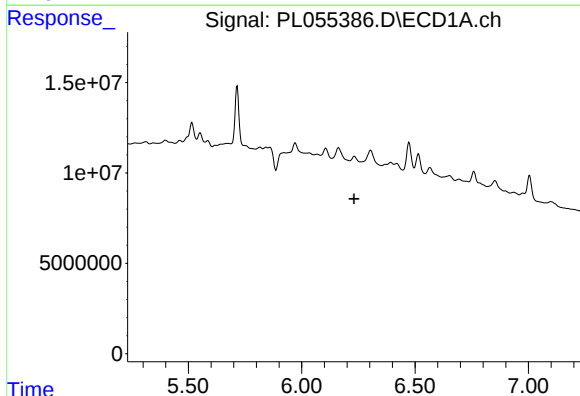


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

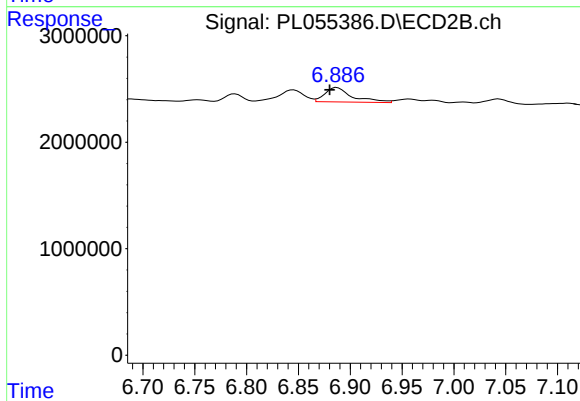

#16 4,4'-DDD


R.T.: 6.887 min
Delta R.T.: 0.007 min
Response: 2497475
Conc: 1.31 ng/ml

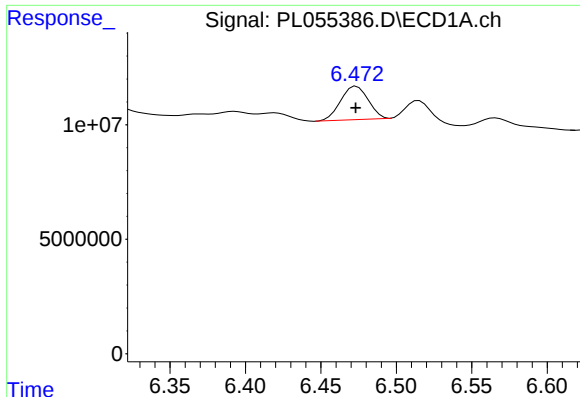

#17 4,4'-DDT


R.T.: 6.474 min
Delta R.T.: 0.000 min
Response: 18500773
Conc: 1.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

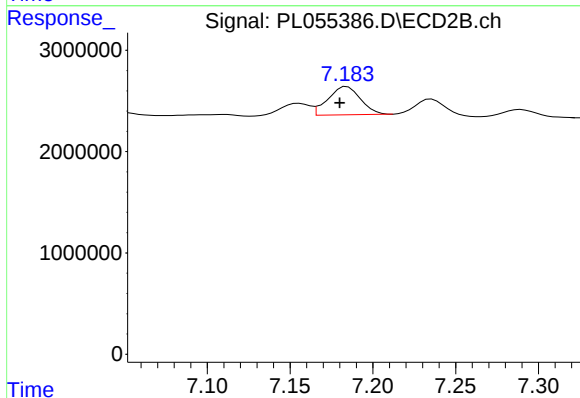


#17 4,4'-DDT

R.T.: 7.184 min
Delta R.T.: 0.005 min
Response: 3826593
Conc: 1.95 ng/ml

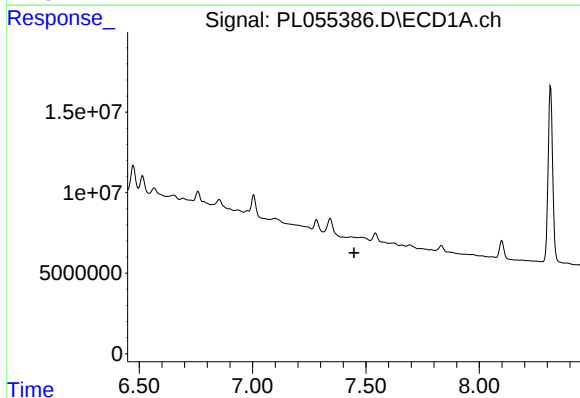


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.448 min
Response: 0
Conc: N.D.

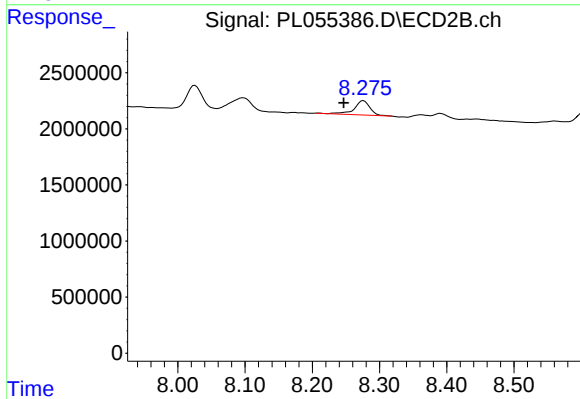

#22 Mirex


R.T.: 8.276 min
Delta R.T.: 0.029 min
Response: 2041133
Conc: 1.23 ng/ml

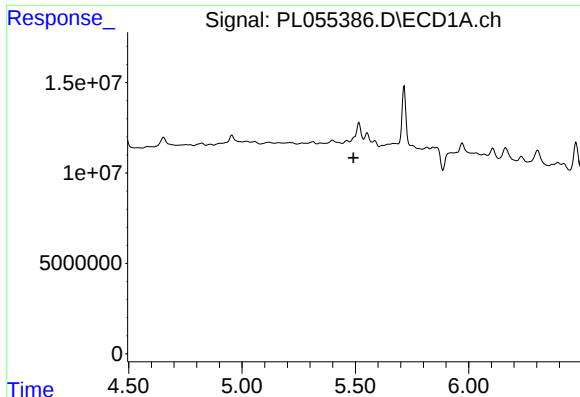

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

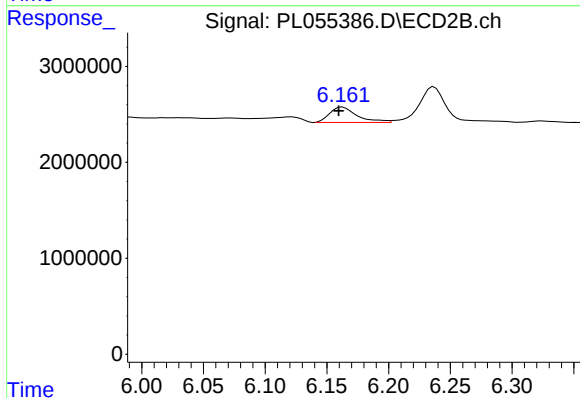


#25 Chlordane-3

R.T.: 6.163 min
Delta R.T.: 0.003 min
Response: 2489107
Conc: 7.73 ng/ml

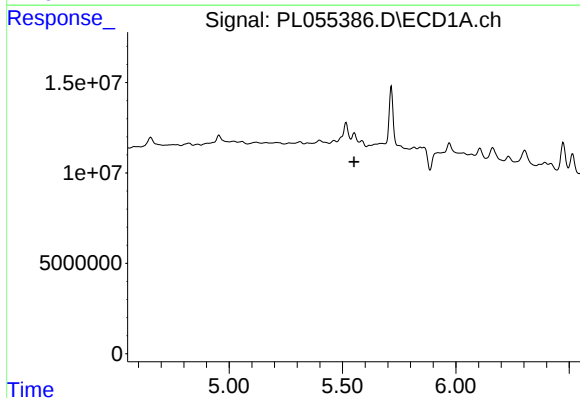


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

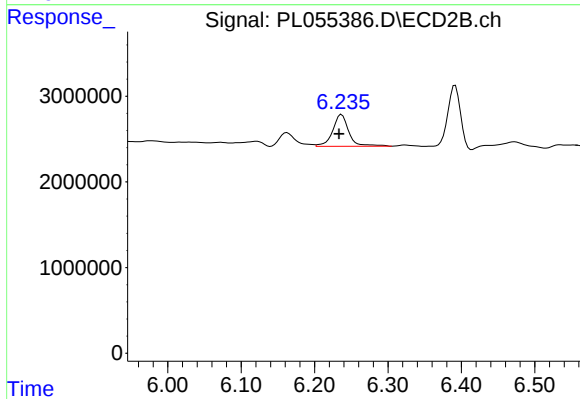

#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: 0.003 min
Response: 5657835
Conc: 14.72 ng/ml

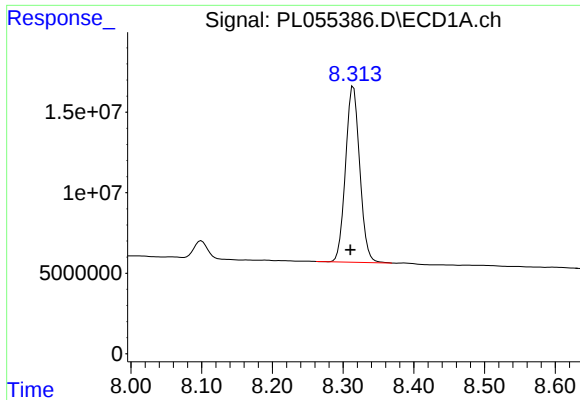

#28 Decachlorobiphenyl


R.T.: 8.315 min

Delta R.T.: 0.004 min

Response: 152556956

Conc: 16.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

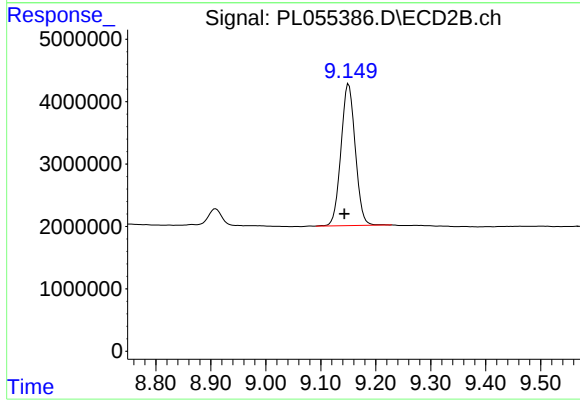

#28 Decachlorobiphenyl

R.T.: 9.151 min

Delta R.T.: 0.008 min

Response: 40994195

Conc: 18.57 ng/ml