

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123019\
 Data File : PL055397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2019 21:33
 Operator : SG\AJ
 Sample : K6465-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 00:57:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	257.4E6	68563616	24.473	25.949
28)	SA Decachlor...	8.313	9.152	155.9E6	39417227	16.805	17.856
Target Compounds							
3)	MA gamma-BHC...	0.000	4.710	0	5174355	N.D.	1.514 #
6)	B beta-BHC	0.000	4.874f	0	2434758	N.D.	1.483 #
9)	A Endosulfan I	5.630f	0.000	74441808	0	5.634	N.D. #
10)	B gamma-Chl...	0.000	6.156	0	6096323	N.D.	2.297 #
11)	B alpha-Chl...	0.000	6.236	0	4783364	N.D.	1.824 #
15)	B Endosulfa...	0.000	6.981	0	3801108	N.D.	1.603 #
16)	A 4,4'-DDD	0.000	6.885	0	4954631	N.D.	2.606 #
25)	Chlordane-3	0.000	6.156	0	6096323	N.D.	18.944 #
26)	Chlordane-4	0.000	6.236	0	4783364	N.D.	12.444 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123019\
Data File : PL055397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2019 21:33
Operator : SG\AJ
Sample : K6465-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 00:57:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

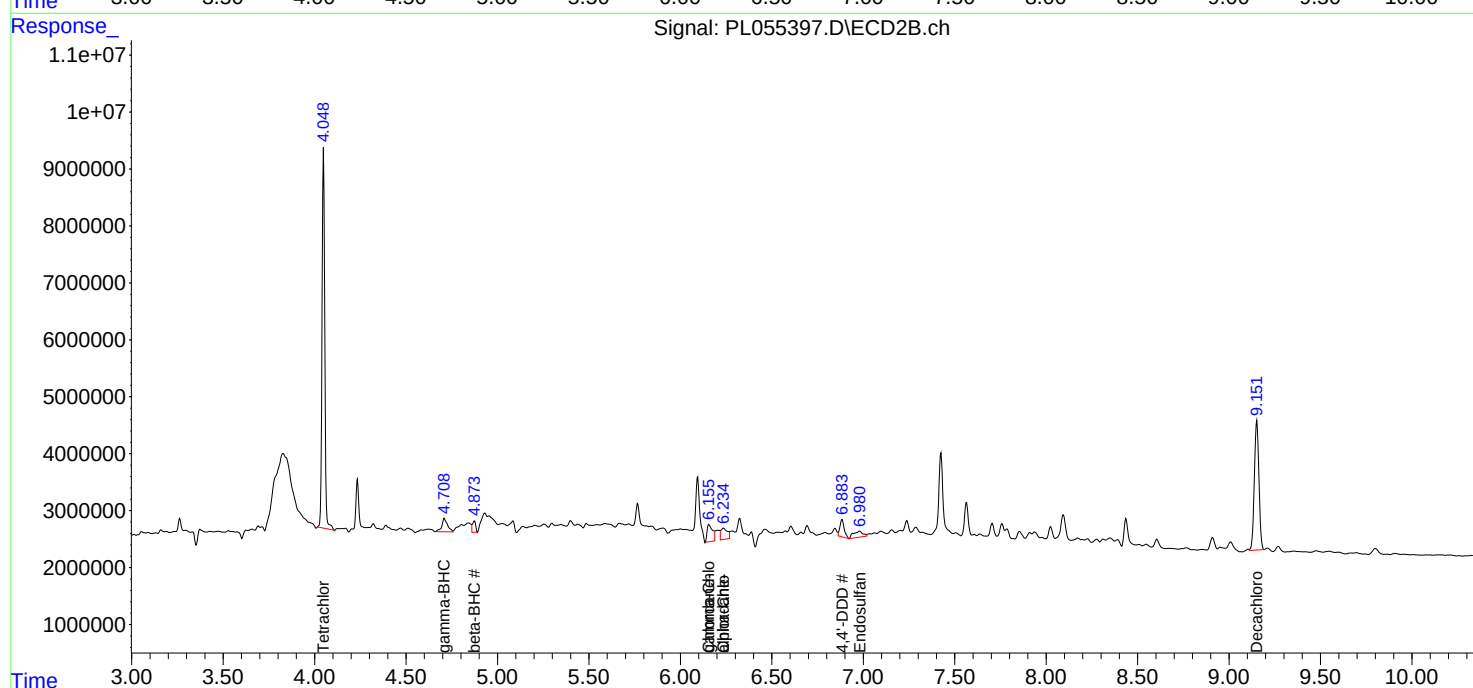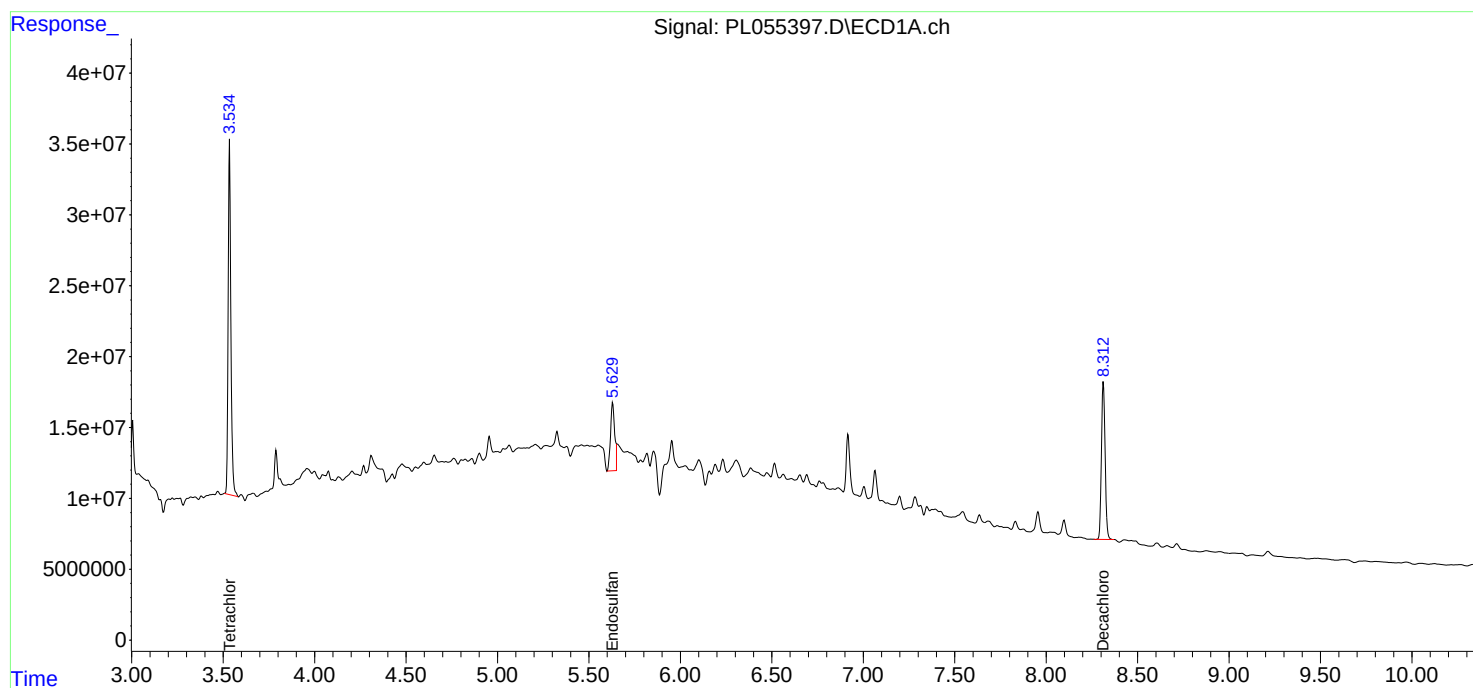


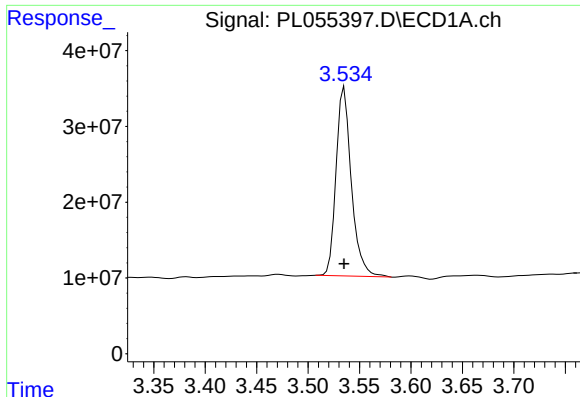

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 257366898
Conc: 24.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

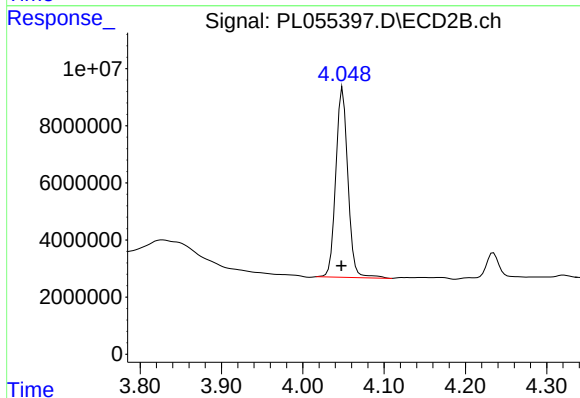


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 68563616
Conc: 25.95 ng/ml

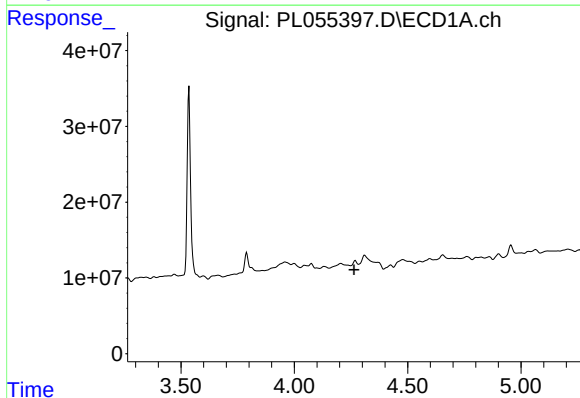


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.263 min
Response: 0
Conc: N.D.

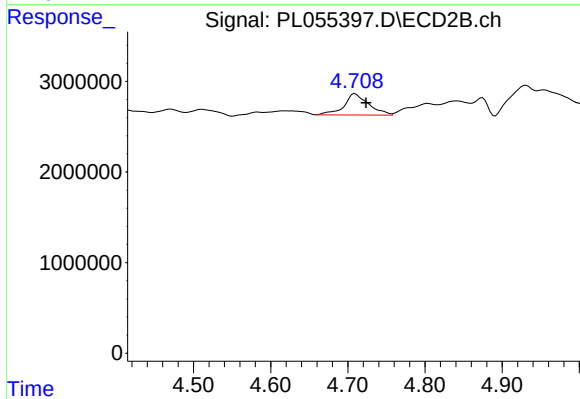

#3 gamma-BHC (Lindane)


R.T.: 4.710 min
Delta R.T.: -0.014 min
Response: 5174355
Conc: 1.51 ng/ml

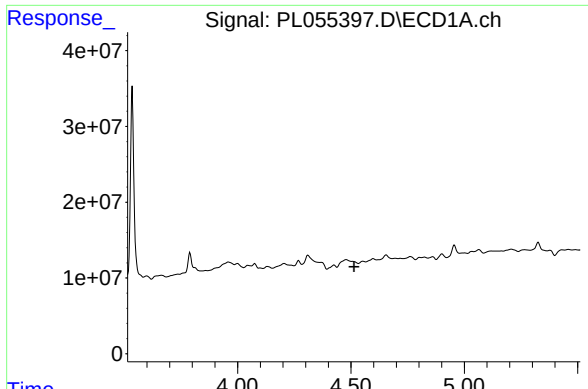

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.514 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

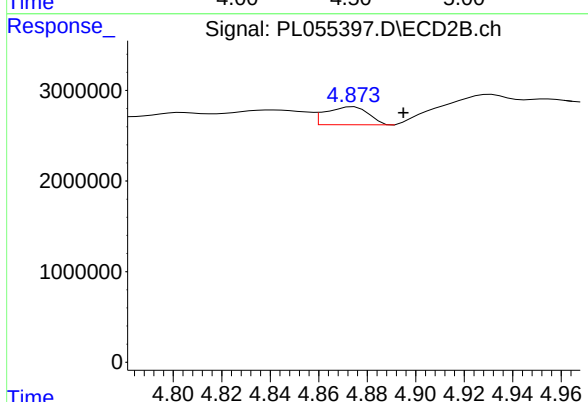


#6 beta-BHC

R.T.: 4.874 min
Delta R.T.: -0.020 min
Response: 2434758
Conc: 1.48 ng/ml

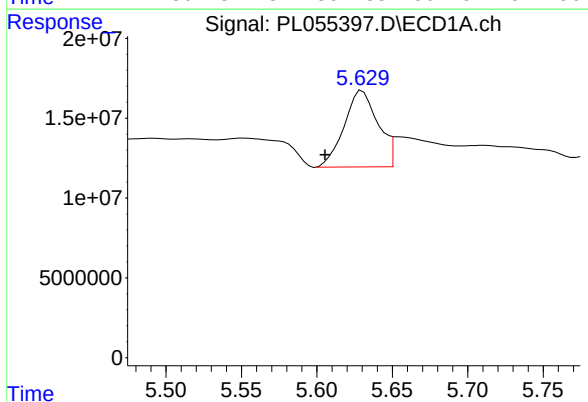


#9 Endosulfan I

R.T.: 5.630 min
Delta R.T.: 0.025 min
Response: 74441808
Conc: 5.63 ng/ml

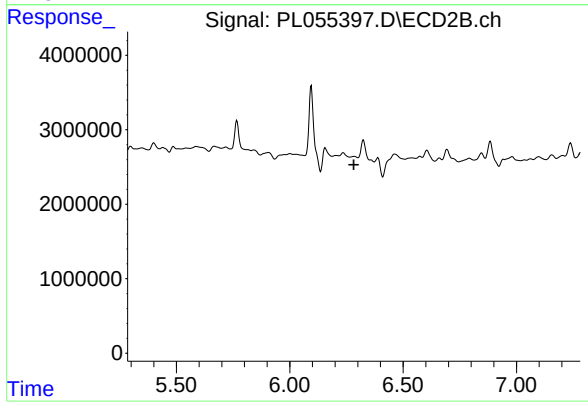

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.283 min
Response: 0
Conc: N.D.

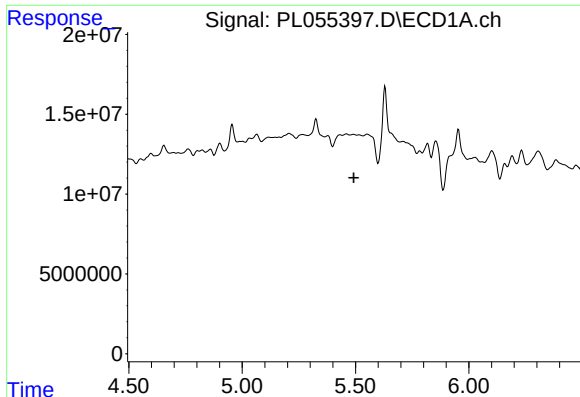

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

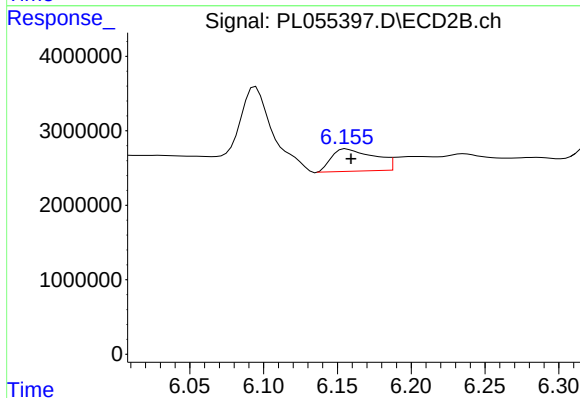


#10 gamma-Chlordane

R.T.: 6.156 min
Delta R.T.: -0.003 min
Response: 6096323
Conc: 2.30 ng/ml

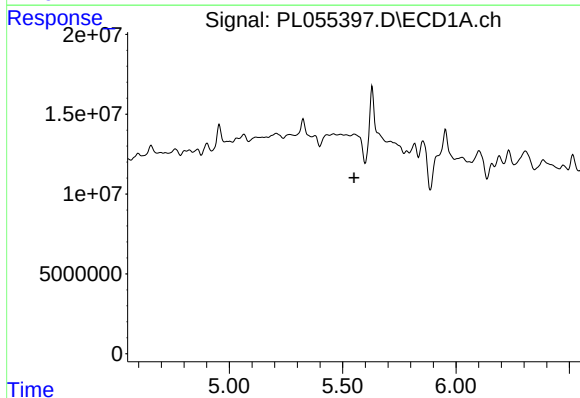


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

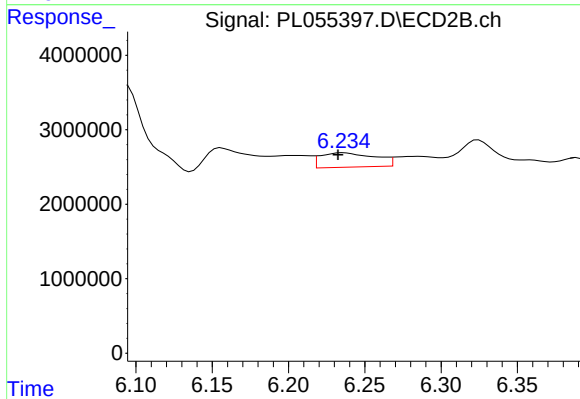

#11 alpha-Chlordane


R.T.: 6.236 min
Delta R.T.: 0.003 min
Response: 4783364
Conc: 1.82 ng/ml

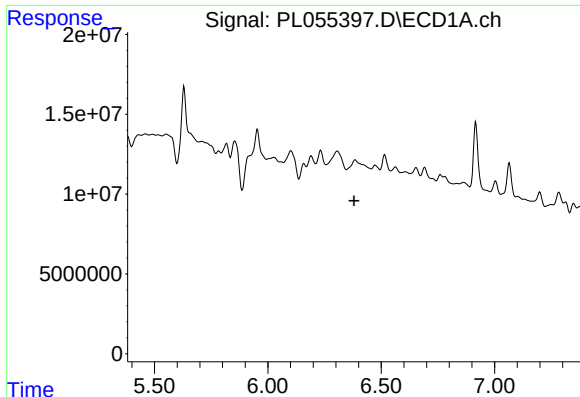

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.381 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

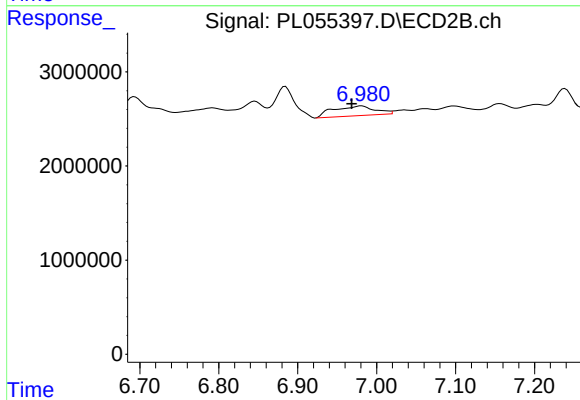


#15 Endosulfan II

R.T.: 6.981 min
Delta R.T.: 0.013 min
Response: 3801108
Conc: 1.60 ng/ml

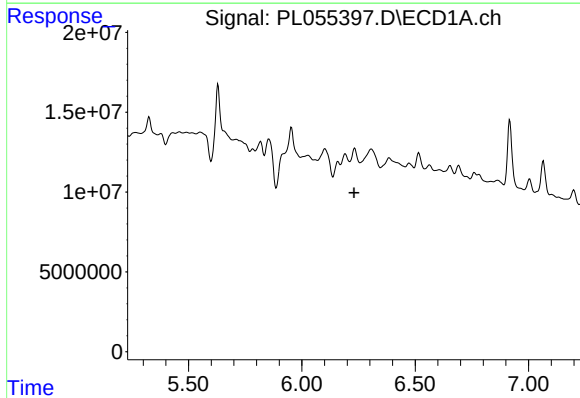


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

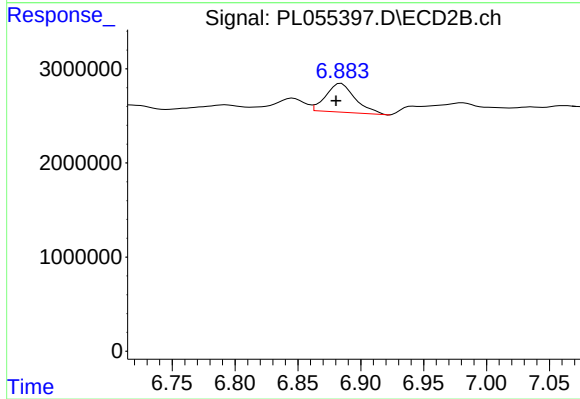

#16 4,4'-DDD


R.T.: 6.885 min
Delta R.T.: 0.004 min
Response: 4954631
Conc: 2.61 ng/ml

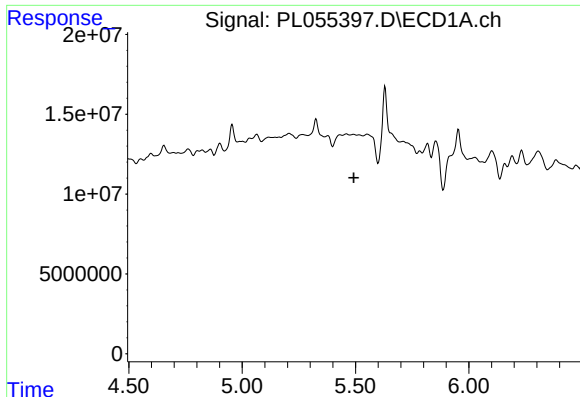

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

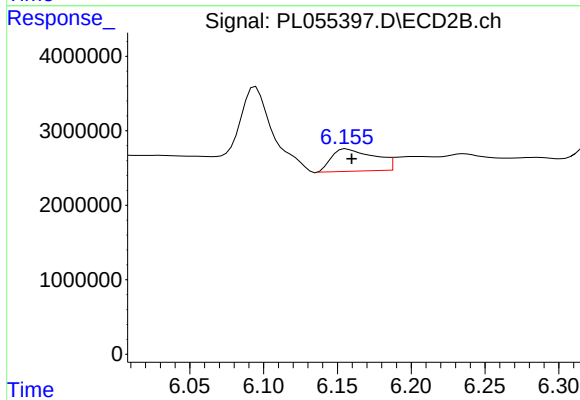


#25 Chlordane-3

R.T.: 6.156 min
Delta R.T.: -0.003 min
Response: 6096323
Conc: 18.94 ng/ml

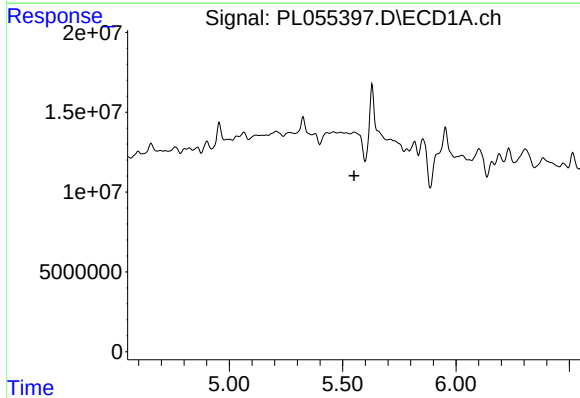


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

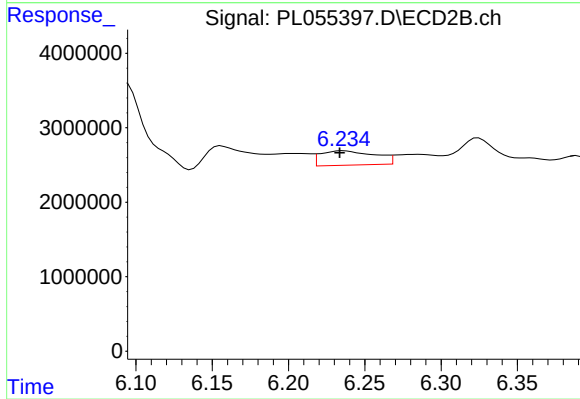

#26 Chlordane-4


R.T.: 6.236 min
Delta R.T.: 0.002 min
Response: 4783364
Conc: 12.44 ng/ml

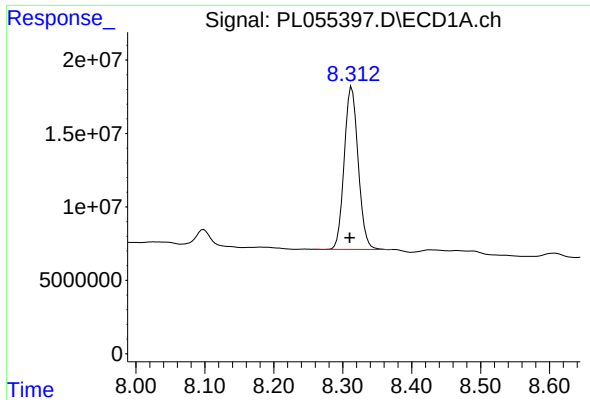

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: 0.003 min
Response: 155930029
Conc: 16.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

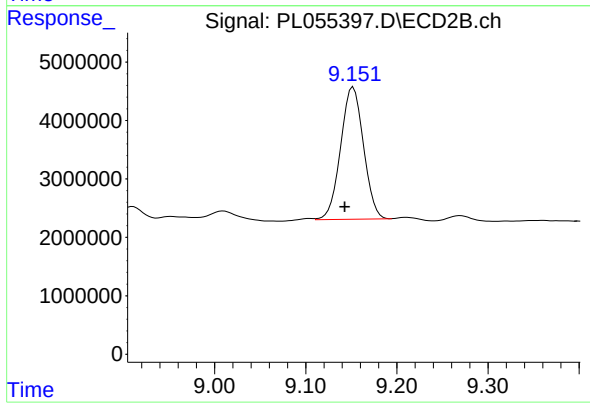

#28 Decachlorobiphenyl

R.T.: 9.152 min
Delta R.T.: 0.009 min
Response: 39417227
Conc: 17.86 ng/ml