

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123020\
 Data File : PL063859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2020 13:55
 Operator : AR\AJ
 Sample : L5242-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 15:55:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.110	43099854	35854619	14.376	14.044
28)	SA Decachlor...	8.176	9.264	41979721	27618395	15.237	14.008
Target Compounds							
6)	B beta-BHC	0.000	4.992	0	3379592	N.D.	1.925 #
10)	B gamma-Chl...	0.000	6.265	0	6737632	N.D.	2.435 #
11)	B alpha-Chl...	0.000	6.326	0	8434238	N.D.	3.056 #
13)	MA Dieldrin	0.000	6.621f	0	2339047	N.D.	0.898 #
17)	MA 4,4'-DDT	6.341	0.000	2498173	0	0.943	N.D. #
23)	Chlordane-1	4.299	0.000	7222177	0	70.473	N.D. #
25)	Chlordane-3	0.000	6.265	0	6737632	N.D.	19.664 #
26)	Chlordane-4	0.000	6.326	0	8434238	N.D.	20.520 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123020\
Data File : PL063859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2020 13:55
Operator : AR\AJ
Sample : L5242-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 15:55:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

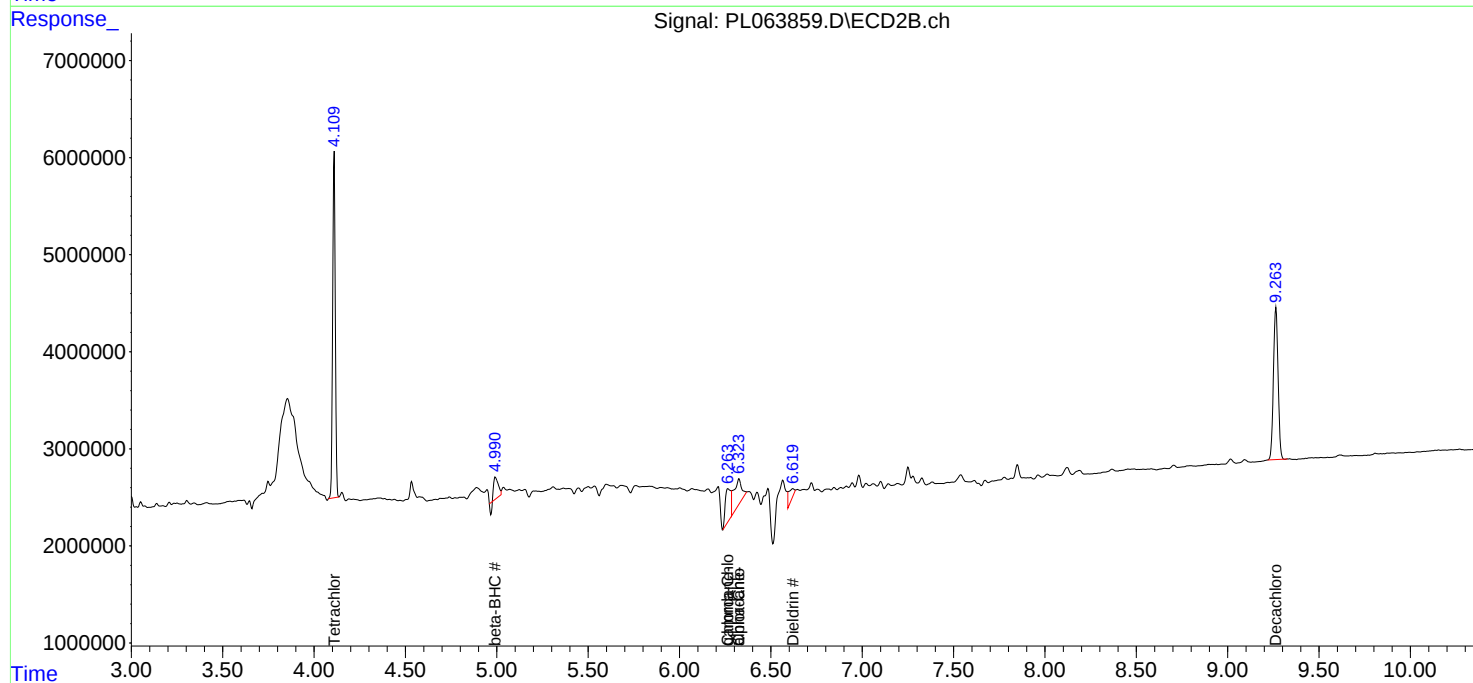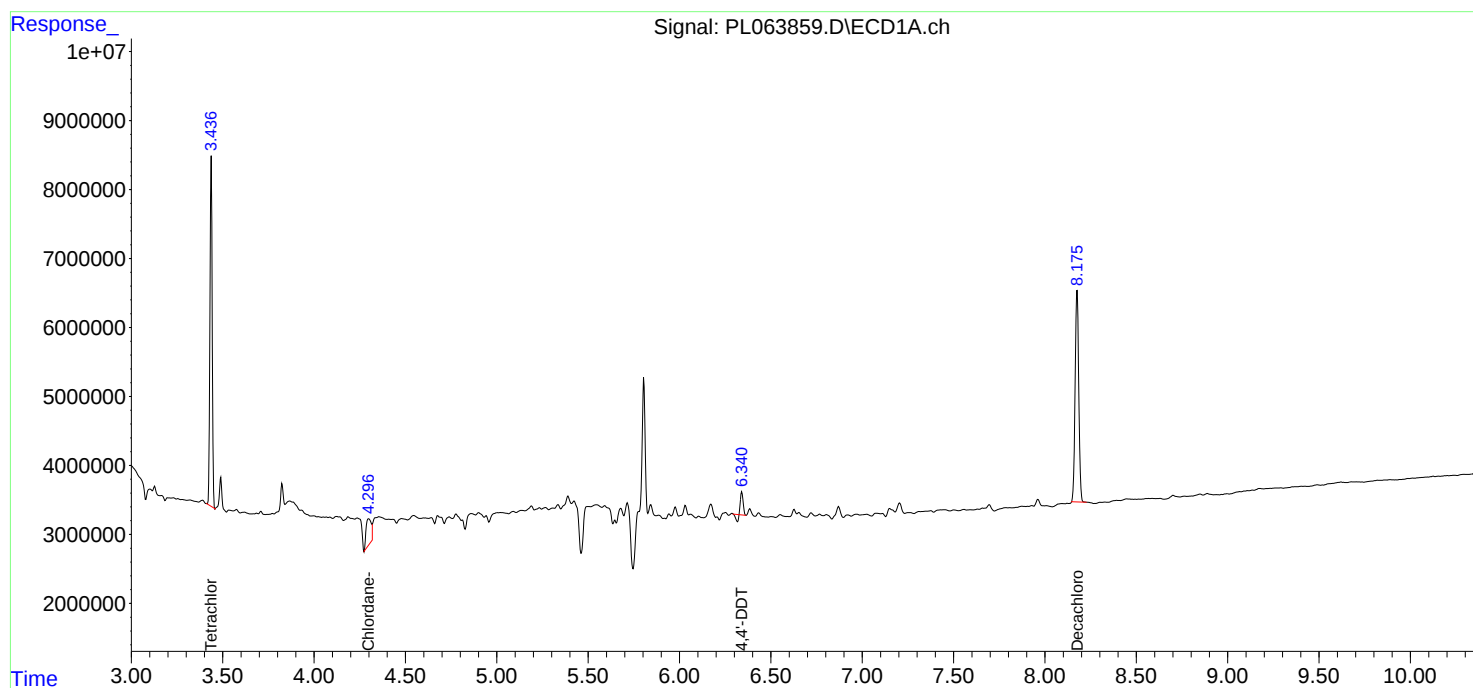


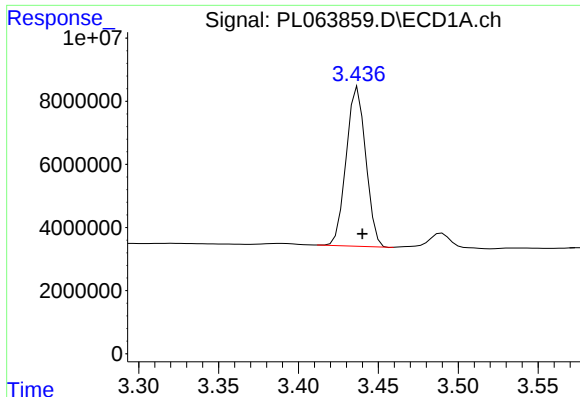

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: -0.003 min
Response: 43099854
Conc: 14.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

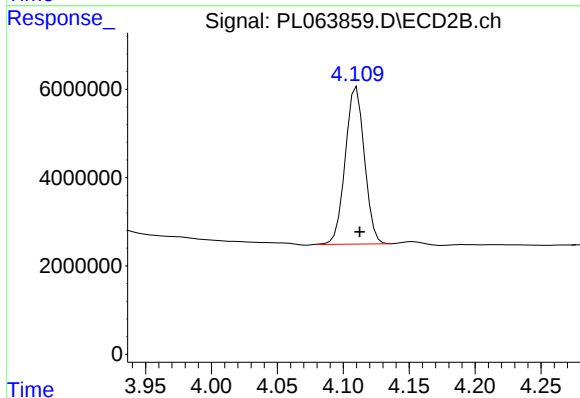


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.003 min
Response: 35854619
Conc: 14.04 ng/ml

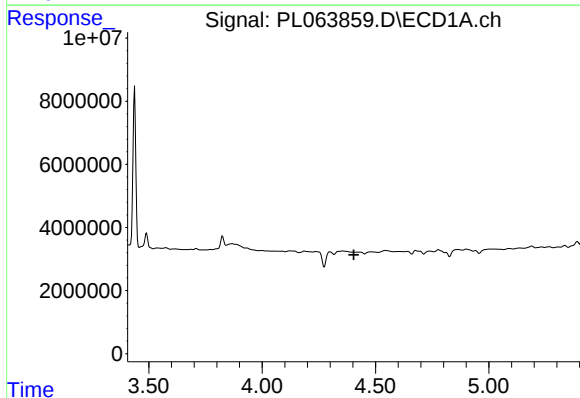


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.404 min
Response: 0
Conc: N.D.

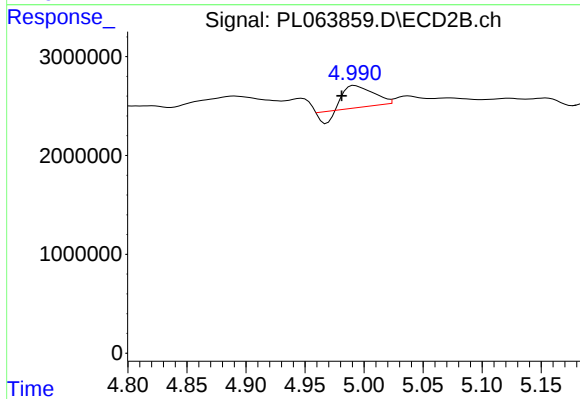

#6 beta-BHC


R.T.: 4.992 min
Delta R.T.: 0.011 min
Response: 3379592
Conc: 1.93 ng/ml

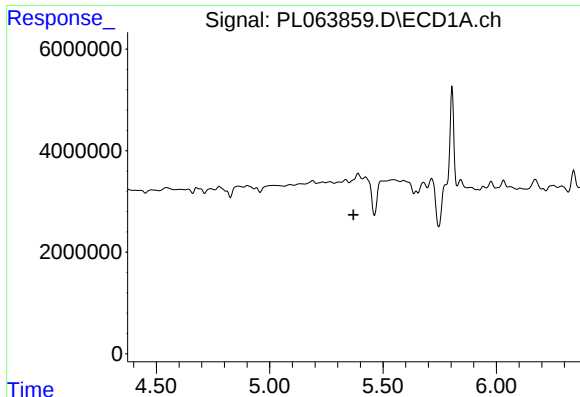

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

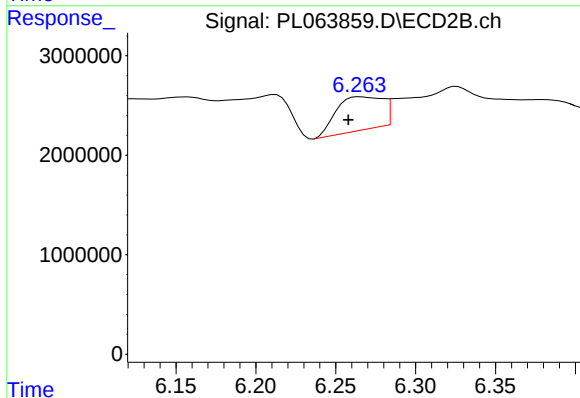


#10 gamma-Chlordane

R.T.: 6.265 min
Delta R.T.: 0.007 min
Response: 6737632
Conc: 2.44 ng/ml

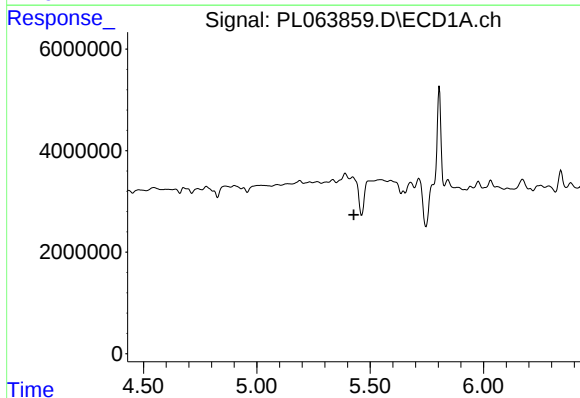


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.428 min
Response: 0
Conc: N.D.

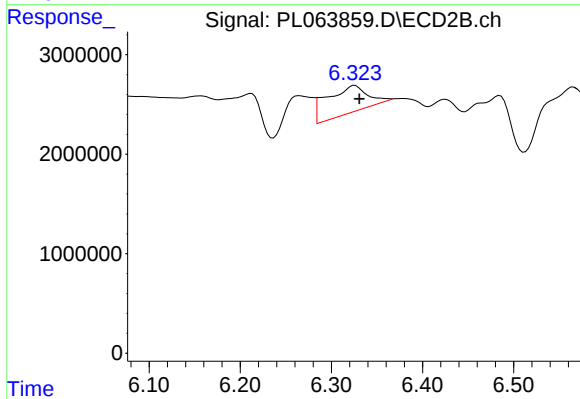

#11 alpha-Chlordane


R.T.: 6.326 min
Delta R.T.: -0.005 min
Response: 8434238
Conc: 3.06 ng/ml

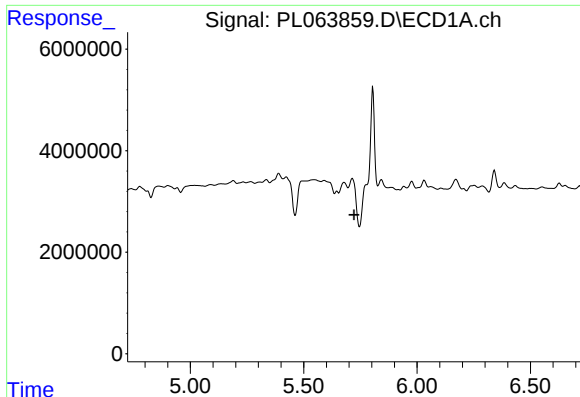

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.723 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

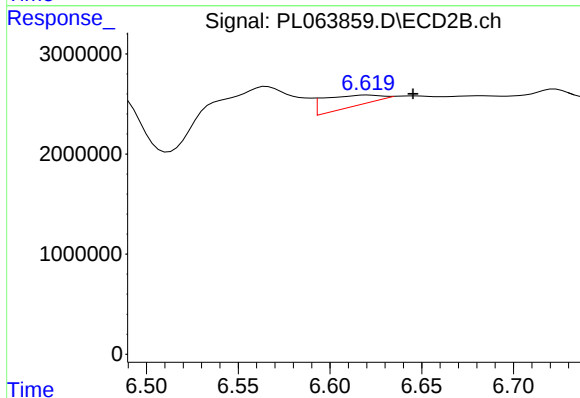


#13 Dieldrin

R.T.: 6.621 min
Delta R.T.: -0.024 min
Response: 2339047
Conc: 0.90 ng/ml

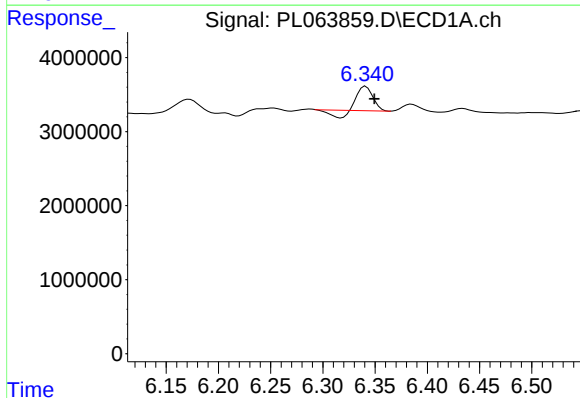


#17 4,4'-DDT

R.T.: 6.341 min
Delta R.T.: -0.008 min
Response: 2498173
Conc: 0.94 ng/ml

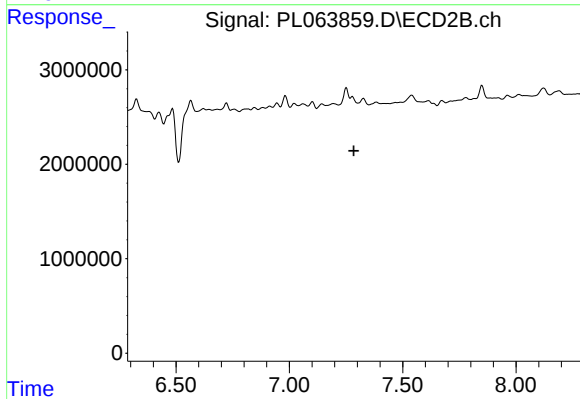

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

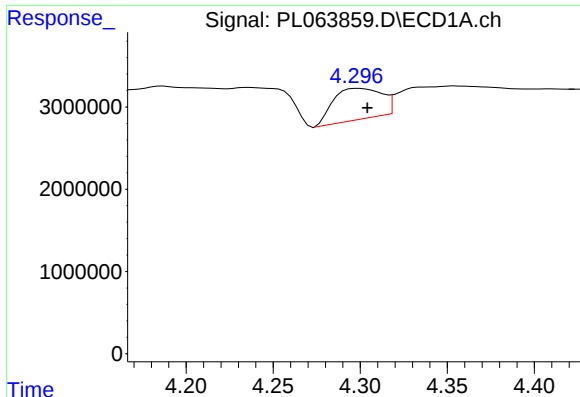

#23 Chlordane-1


R.T.: 4.299 min
Delta R.T.: -0.006 min
Response: 7222177
Conc: 70.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

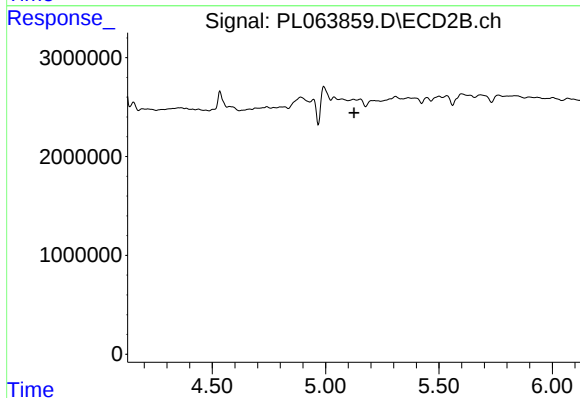


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.126 min
Response: 0
Conc: N.D.

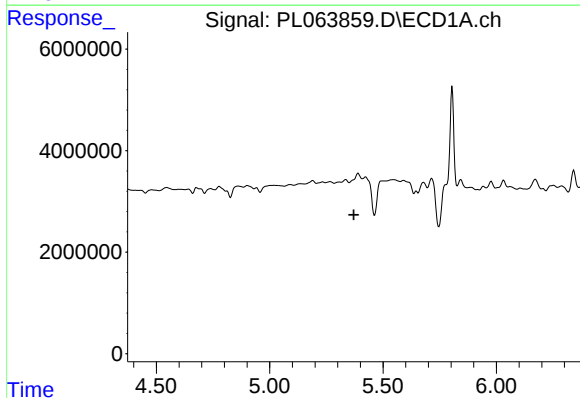


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.370 min
Response: 0
Conc: N.D.

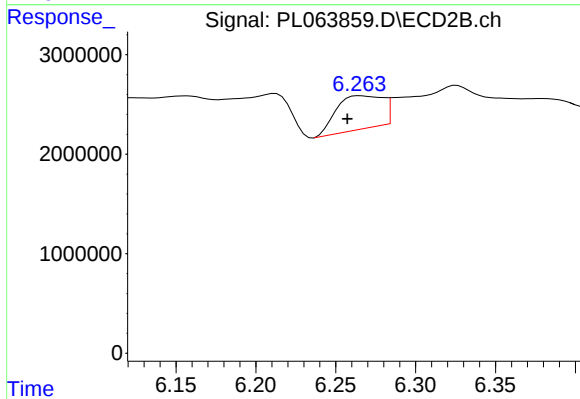

#25 Chlordane-3


R.T.: 6.265 min
Delta R.T.: 0.008 min
Response: 6737632
Conc: 19.66 ng/ml

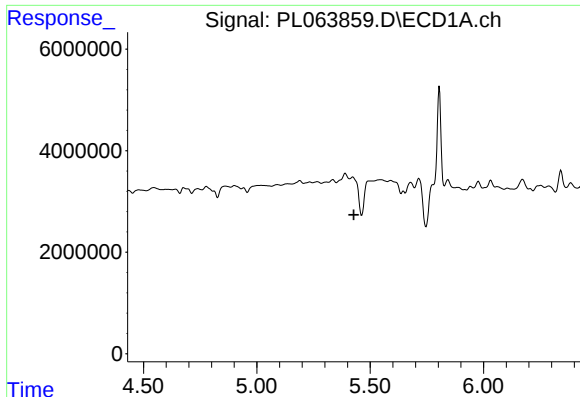

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

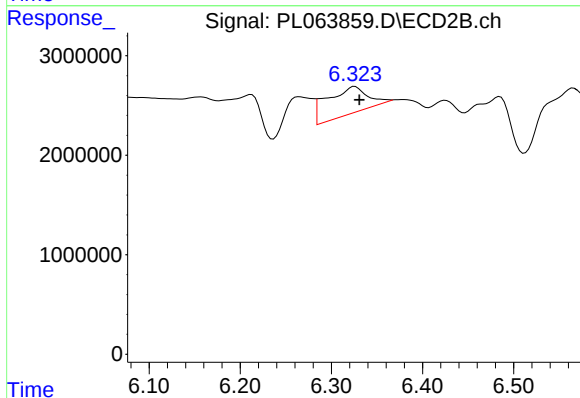


#26 Chlordane-4

R.T.: 6.326 min
Delta R.T.: -0.005 min
Response: 8434238
Conc: 20.52 ng/ml

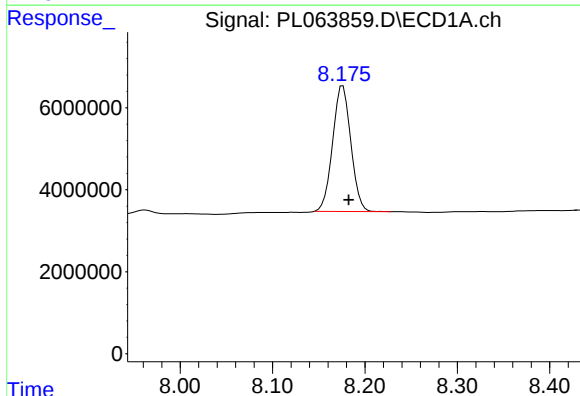

#28 Decachlorobiphenyl

R.T.: 8.176 min
Delta R.T.: -0.006 min
Response: 41979721
Conc: 15.24 ng/ml

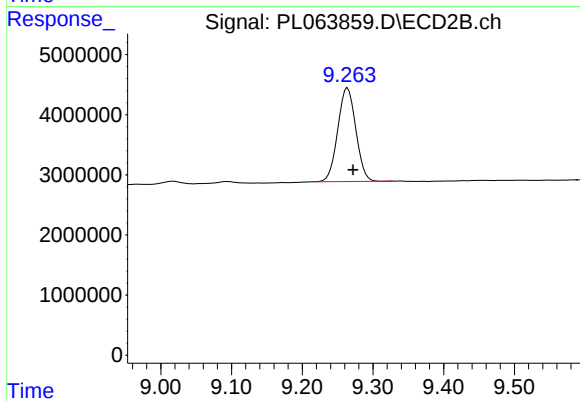

#28 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.008 min
Response: 27618395
Conc: 14.01 ng/ml