

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123020\
 Data File : PL063864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2020 15:06
 Operator : AR\AJ
 Sample : L5242-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 15:56:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.110	41045962	33541278	13.691	13.138
28)	SA Decachlor...	8.175	9.264	38786224	21919447	14.078	11.118
Target Compounds							
6)	B beta-BHC	0.000	4.993	0	2551037	N.D.	1.453 #
10)	B gamma-Chl...	5.388f	6.266	2992932	6833302	0.787	2.470 #
11)	B alpha-Chl...	0.000	6.326	0	6931716	N.D.	2.511 #
15)	B Endosulfa...	0.000	7.089	0	11650453	N.D.	4.942 #
17)	MA 4,4'-DDT	6.339	0.000	1755976	0	0.663	N.D. #
21)	B Endrin ke...	0.000	7.928f	0	3807069	N.D.	1.544 #
23)	Chlordane-1	4.294	0.000	3988886	0	38.923	N.D. #
25)	Chlordane-3	5.388f	6.266	2992932	6833302	9.159	19.943 #
26)	Chlordane-4	0.000	6.326	0	6931716	N.D.	16.864 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123020\
Data File : PL063864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2020 15:06
Operator : AR\AJ
Sample : L5242-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 15:56:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

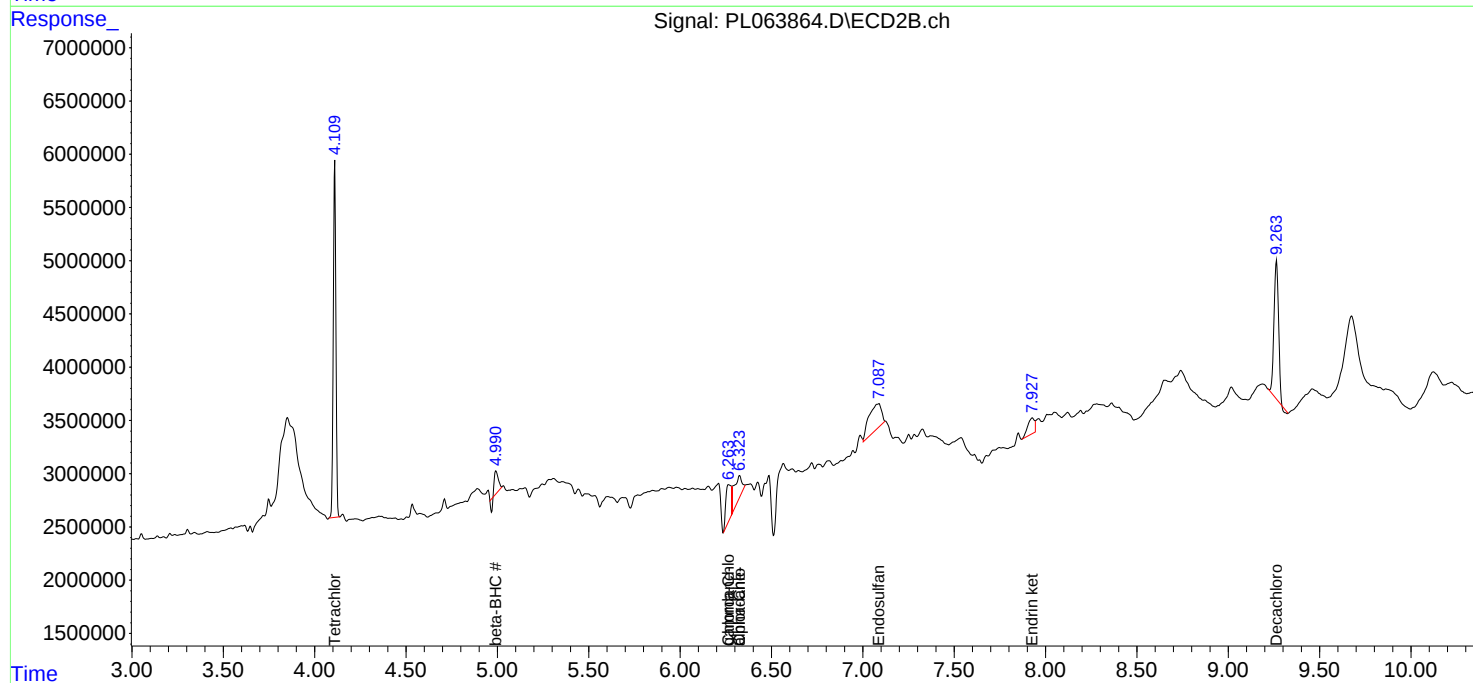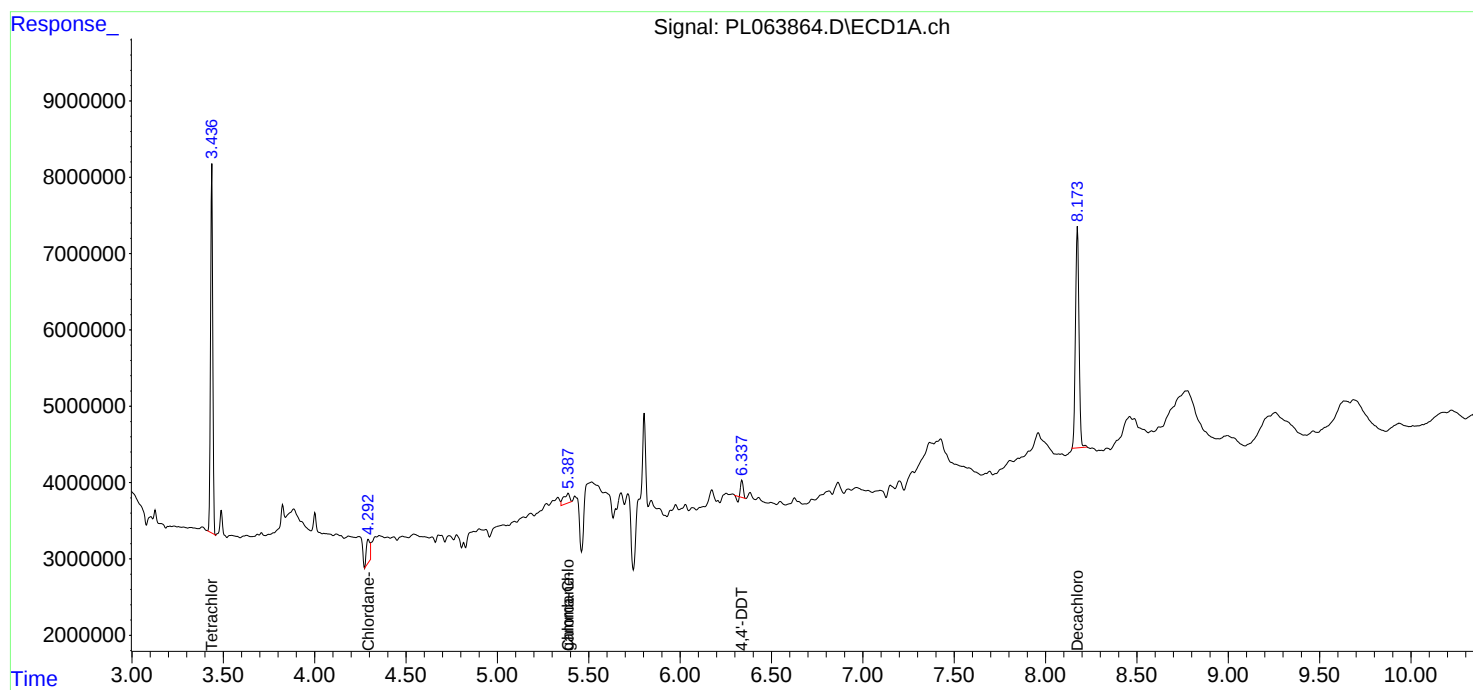


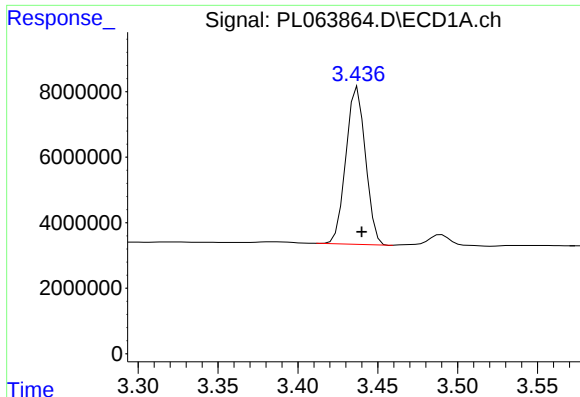

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 41045962
Conc: 13.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

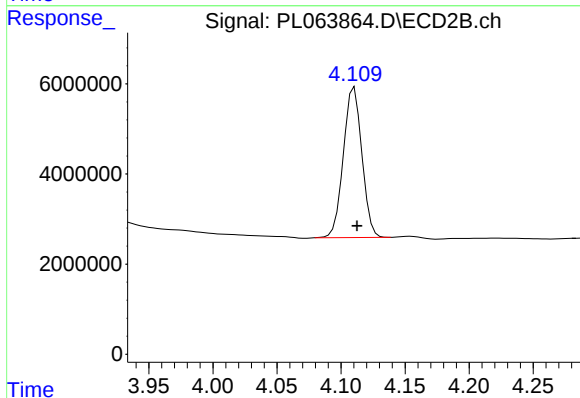


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.002 min
Response: 33541278
Conc: 13.14 ng/ml

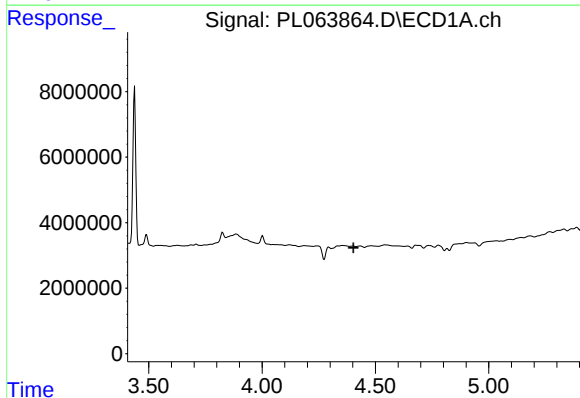


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.404 min
Response: 0
Conc: N.D.

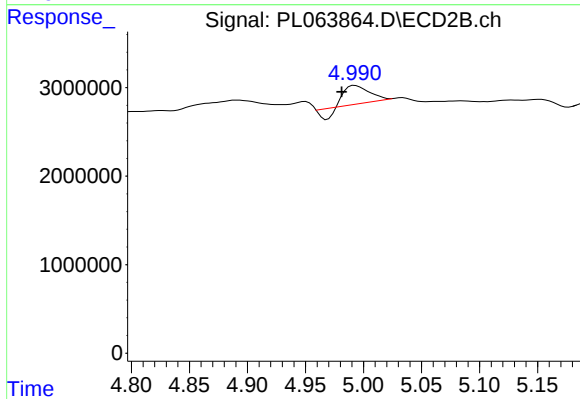

#6 beta-BHC


R.T.: 4.993 min
Delta R.T.: 0.011 min
Response: 2551037
Conc: 1.45 ng/ml

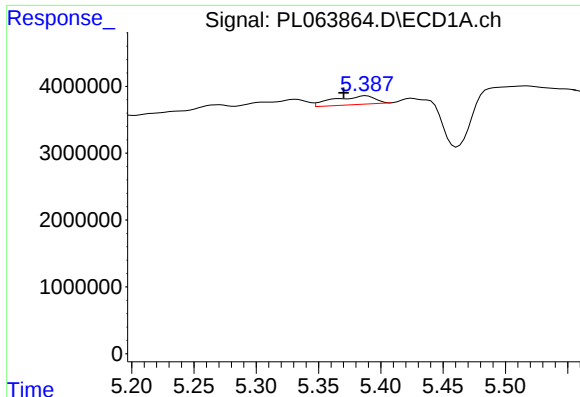

#10 gamma-Chlordane


R.T.: 5.388 min
Delta R.T.: 0.018 min
Response: 2992932
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

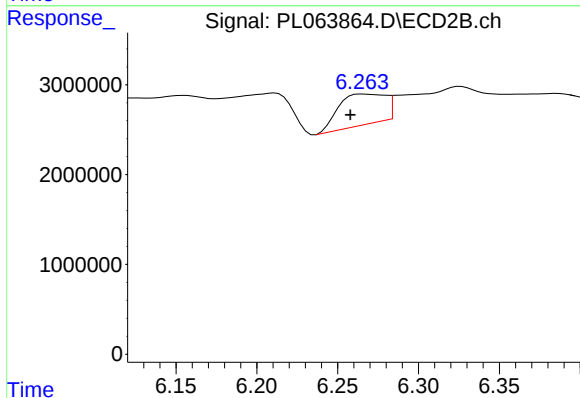


#10 gamma-Chlordane

R.T.: 6.266 min
Delta R.T.: 0.008 min
Response: 6833302
Conc: 2.47 ng/ml

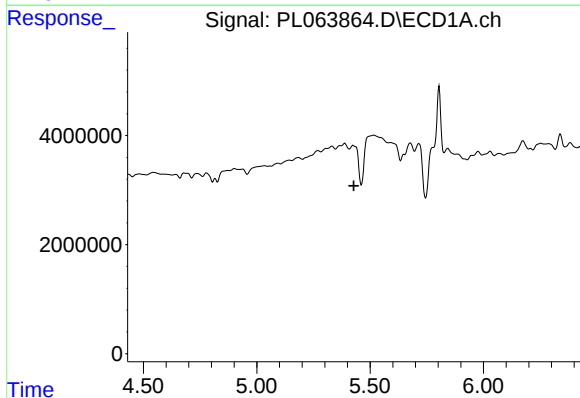


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.428 min
Response: 0
Conc: N.D.

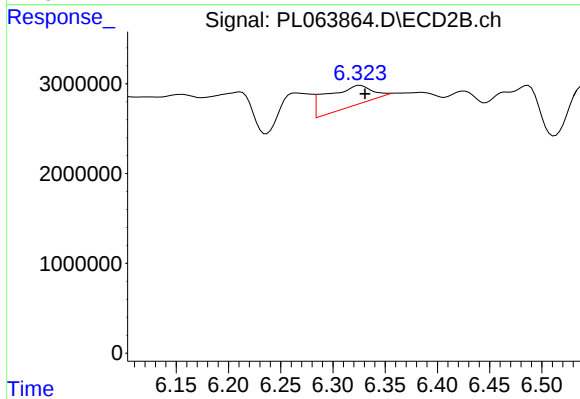

#11 alpha-Chlordane


R.T.: 6.326 min
Delta R.T.: -0.005 min
Response: 6931716
Conc: 2.51 ng/ml

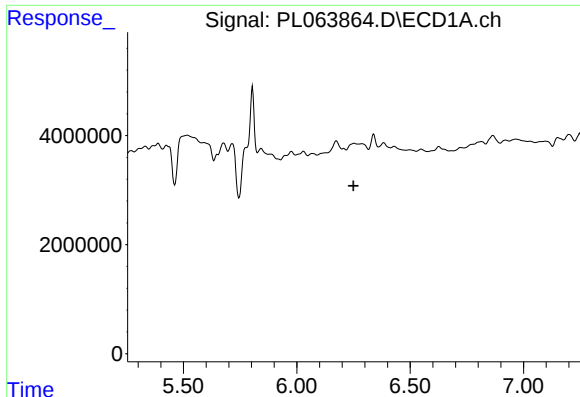

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

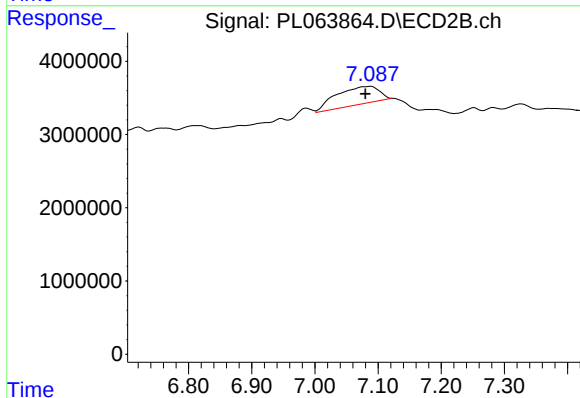


#15 Endosulfan II

R.T.: 7.089 min
Delta R.T.: 0.009 min
Response: 11650453
Conc: 4.94 ng/ml

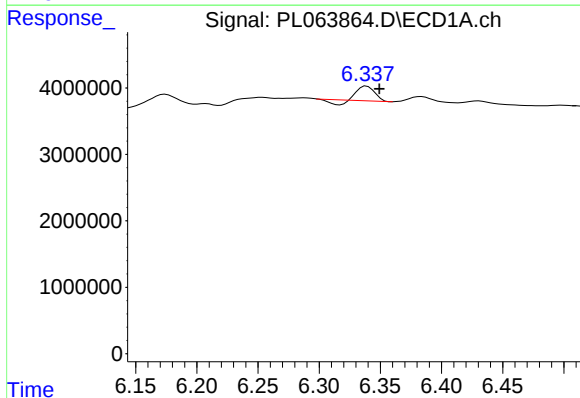


#17 4,4'-DDT

R.T.: 6.339 min
Delta R.T.: -0.010 min
Response: 1755976
Conc: 0.66 ng/ml

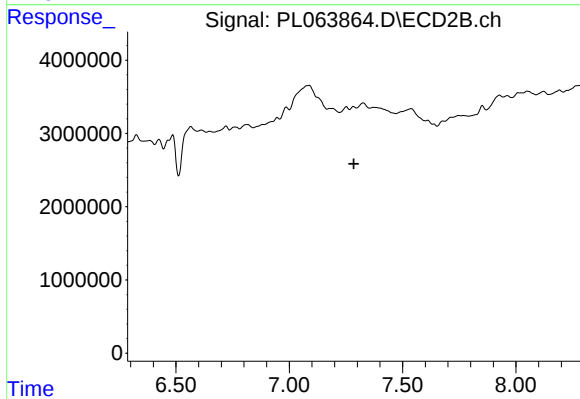

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

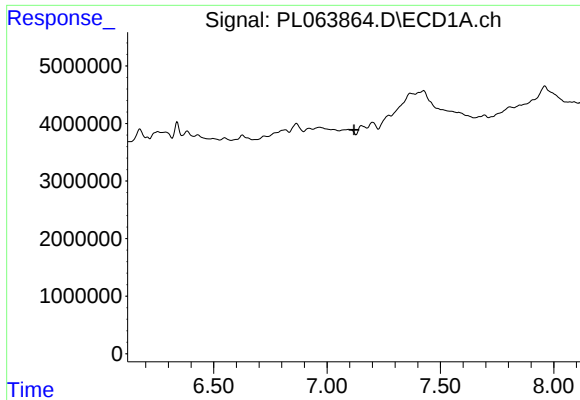

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

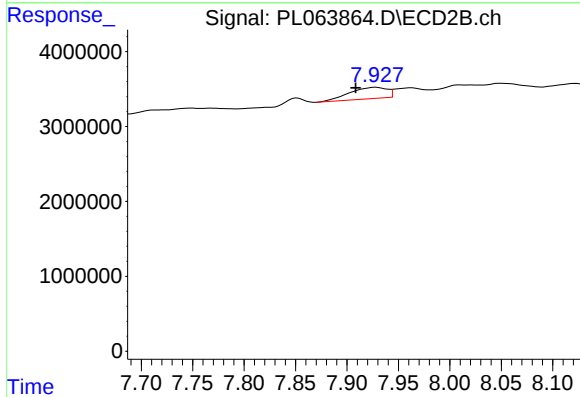


#21 Endrin ketone

R.T.: 7.928 min
Delta R.T.: 0.019 min
Response: 3807069
Conc: 1.54 ng/ml

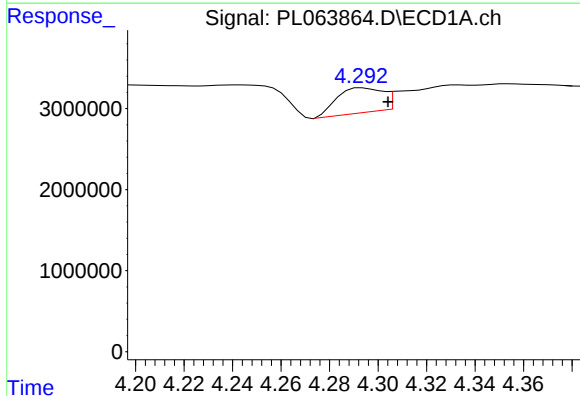


#23 Chlordane-1

R.T.: 4.294 min
Delta R.T.: -0.011 min
Response: 3988886
Conc: 38.92 ng/ml

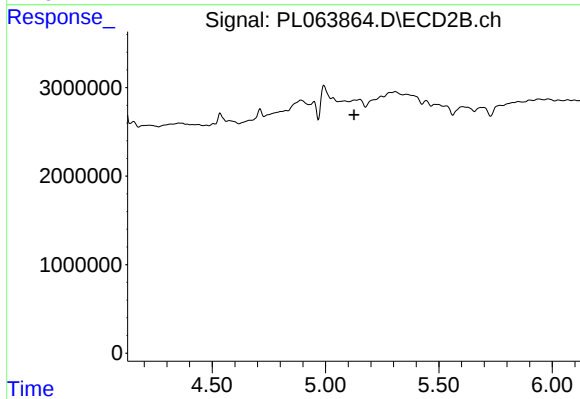

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

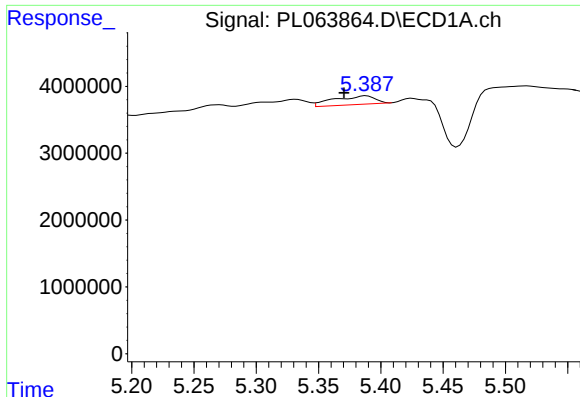

#25 Chlordane-3


R.T.: 5.388 min
Delta R.T.: 0.018 min
Response: 2992932
Conc: 9.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

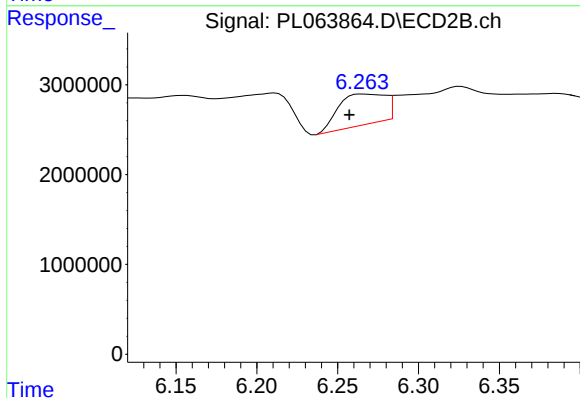


#25 Chlordane-3

R.T.: 6.266 min
Delta R.T.: 0.008 min
Response: 6833302
Conc: 19.94 ng/ml

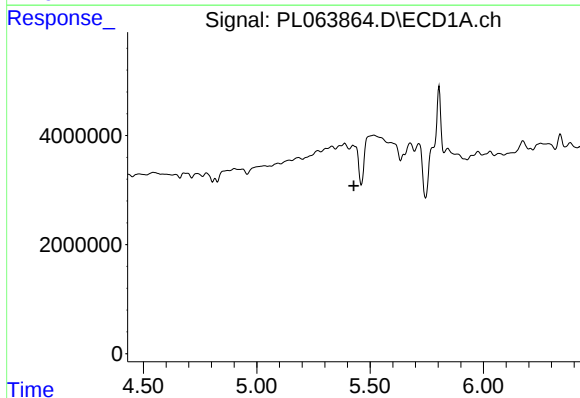


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.428 min
Response: 0
Conc: N.D.

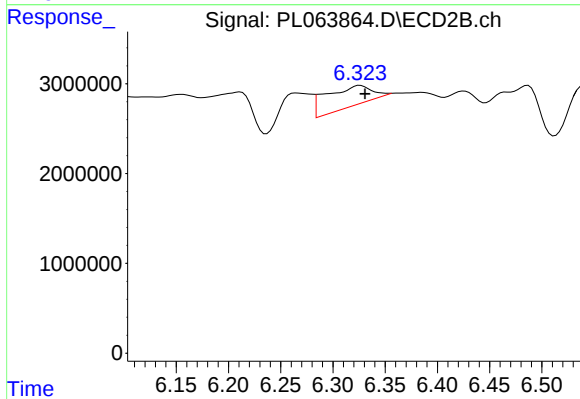

#26 Chlordane-4


R.T.: 6.326 min
Delta R.T.: -0.005 min
Response: 6931716
Conc: 16.86 ng/ml

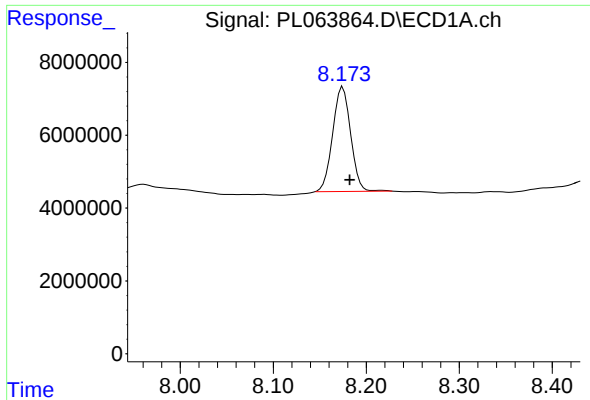

#28 Decachlorobiphenyl

R.T.: 8.175 min
Delta R.T.: -0.008 min
Response: 38786224
Conc: 14.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

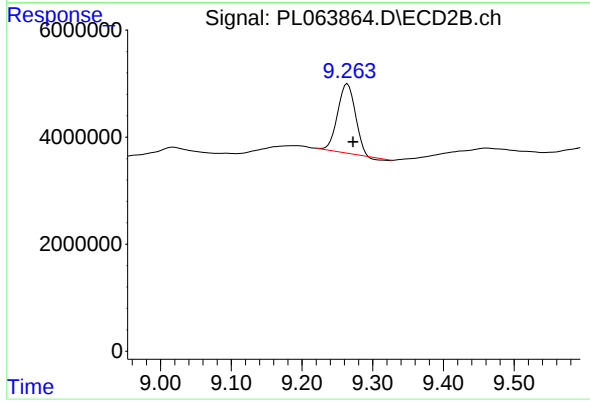

#28 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.008 min
Response: 21919447
Conc: 11.12 ng/ml