

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123020\
 Data File : PL063859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2020 13:55
 Operator : AR\AJ
 Sample : L5242-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-1(494+26)

Manual Integrations
 APPROVED

Ankita
 12/31/2020 1:11:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 15:55:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.110	43099854	35854619	14.376	14.044
28)	SA Decachlor...	8.176	9.264	41979721	27618395	15.237	14.008
Target Compounds							
17)	MA 4,4'-DDT	6.340	7.277	4830833	1065452	1.823m	0.548m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123020\
Data File : PL063859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2020 13:55
Operator : AR\AJ
Sample : L5242-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SAMPLE-1(494+26)


Manual Integrations
APPROVED

Ankita
12/31/2020 1:11:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 15:55:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

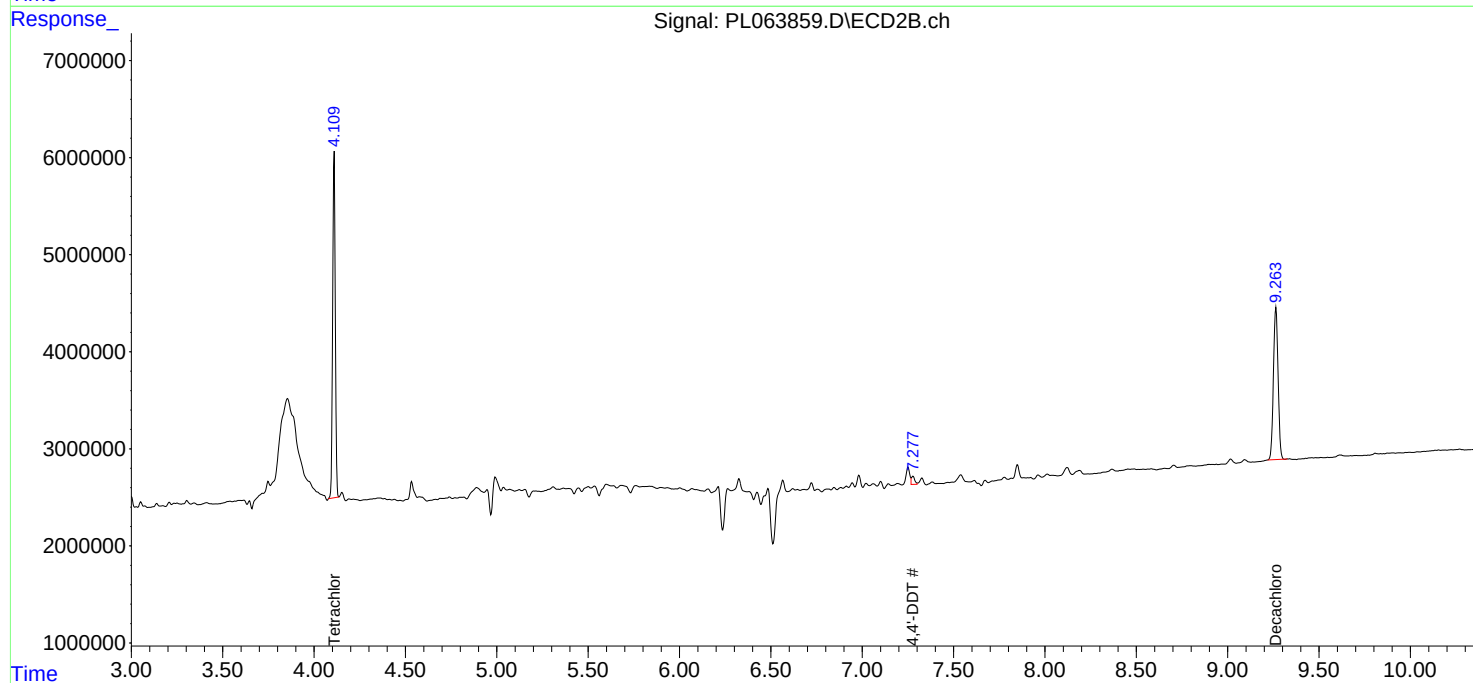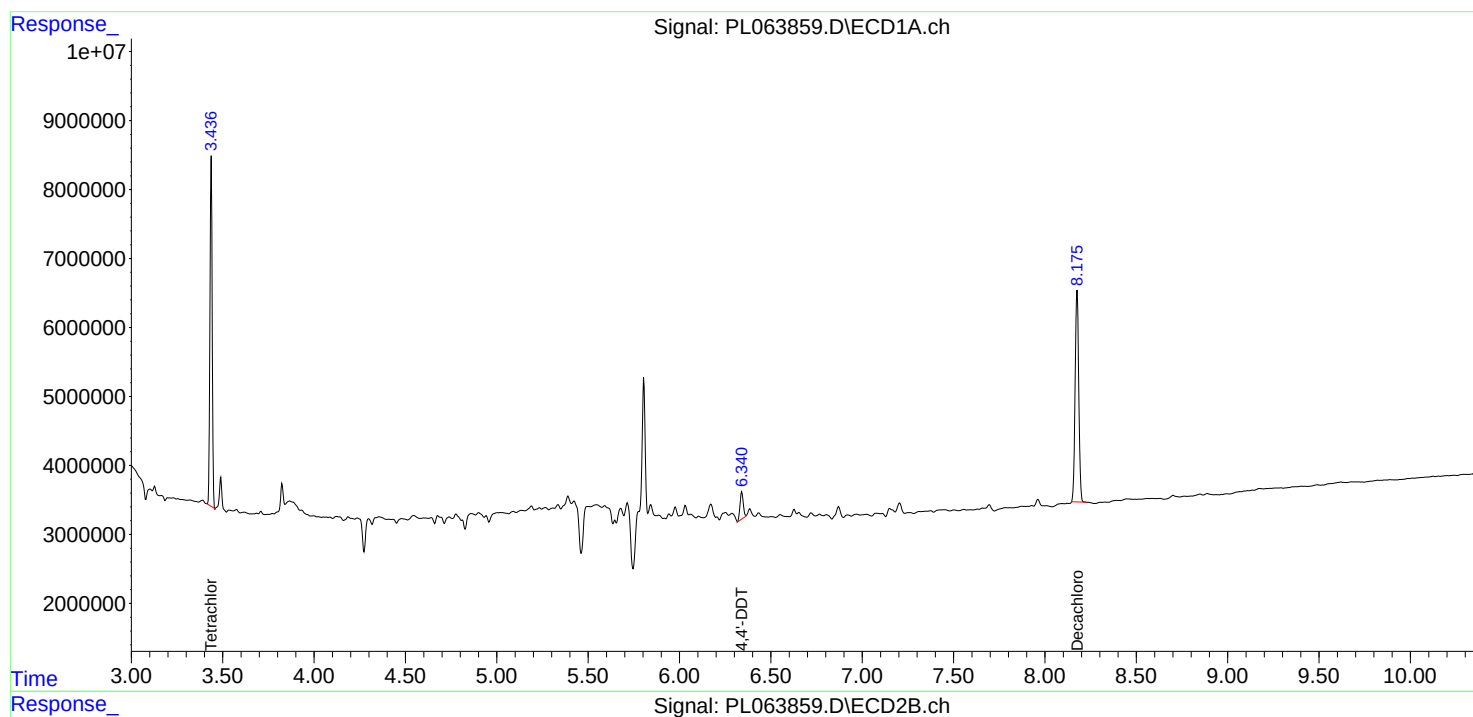

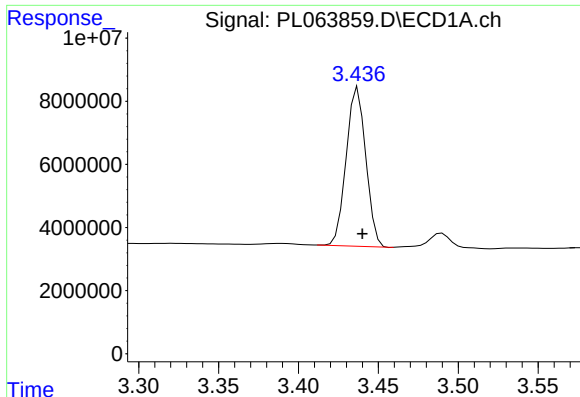


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: -0.003 min
Response: 43099854
Conc: 14.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-1(494+26)


Manual Integrations
APPROVED

Ankita
12/31/2020 1:11:05 PM

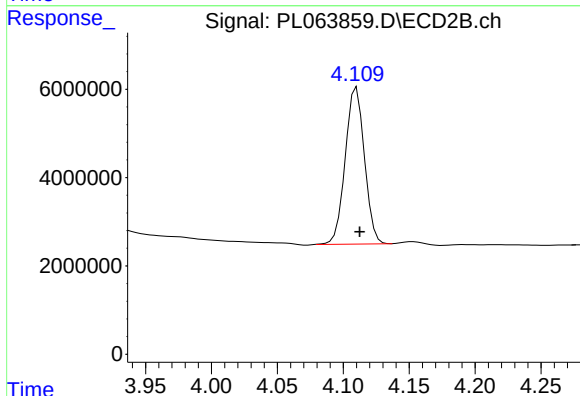


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.003 min
Response: 35854619
Conc: 14.04 ng/ml

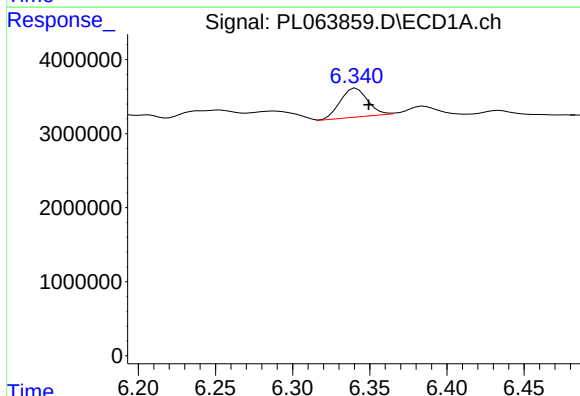


#17 4,4'-DDT

R.T.: 6.340 min
Delta R.T.: -0.010 min
Response: 4830833
Conc: 1.82 ng/ml m

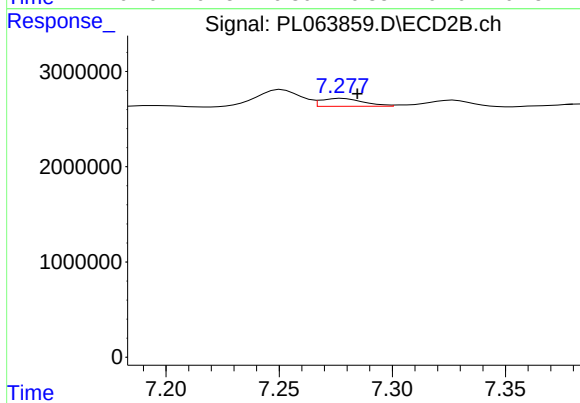

#17 4,4'-DDT

R.T.: 7.277 min
Delta R.T.: -0.008 min
Response: 1065452
Conc: 0.55 ng/ml m

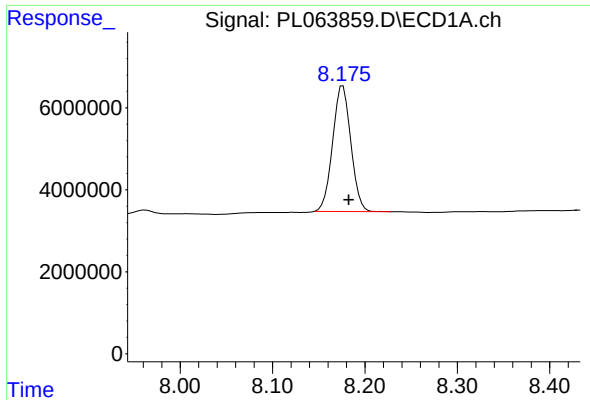

#28 Decachlorobiphenyl

R.T.: 8.176 min

Delta R.T.: -0.006 min


Response: 41979721

Conc: 15.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-1(494+26)

Manual Integrations
APPROVED

Ankita
12/31/2020 1:11:05 PM

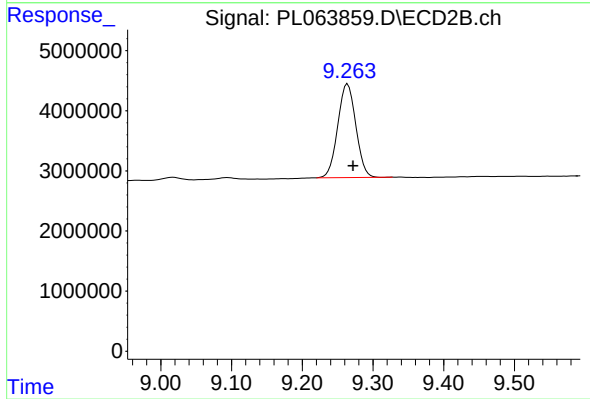

#28 Decachlorobiphenyl

R.T.: 9.264 min

Delta R.T.: -0.008 min

Response: 27618395

Conc: 14.01 ng/ml