

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123020\
 Data File : PL063865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2020 15:21
 Operator : AR\AJ
 Sample : L5242-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-5(454+26)

Manual Integrations
 APPROVED

Ankita
 12/31/2020 1:11:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 15:56:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.110	42718638	34313469	14.249	13.440
28)	SA Decachlor...	8.175	9.265	39940862	25962394	14.497	13.168
Target Compounds							
17)	MA 4,4'-DDT	6.338	7.279	6548640	1819798	2.471m	0.935 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123020\
Data File : PL063865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2020 15:21
Operator : AR\AJ
Sample : L5242-09
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SAMPLE-5(454+26)


Manual Integrations
APPROVED

Ankita
12/31/2020 1:11:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 15:56:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

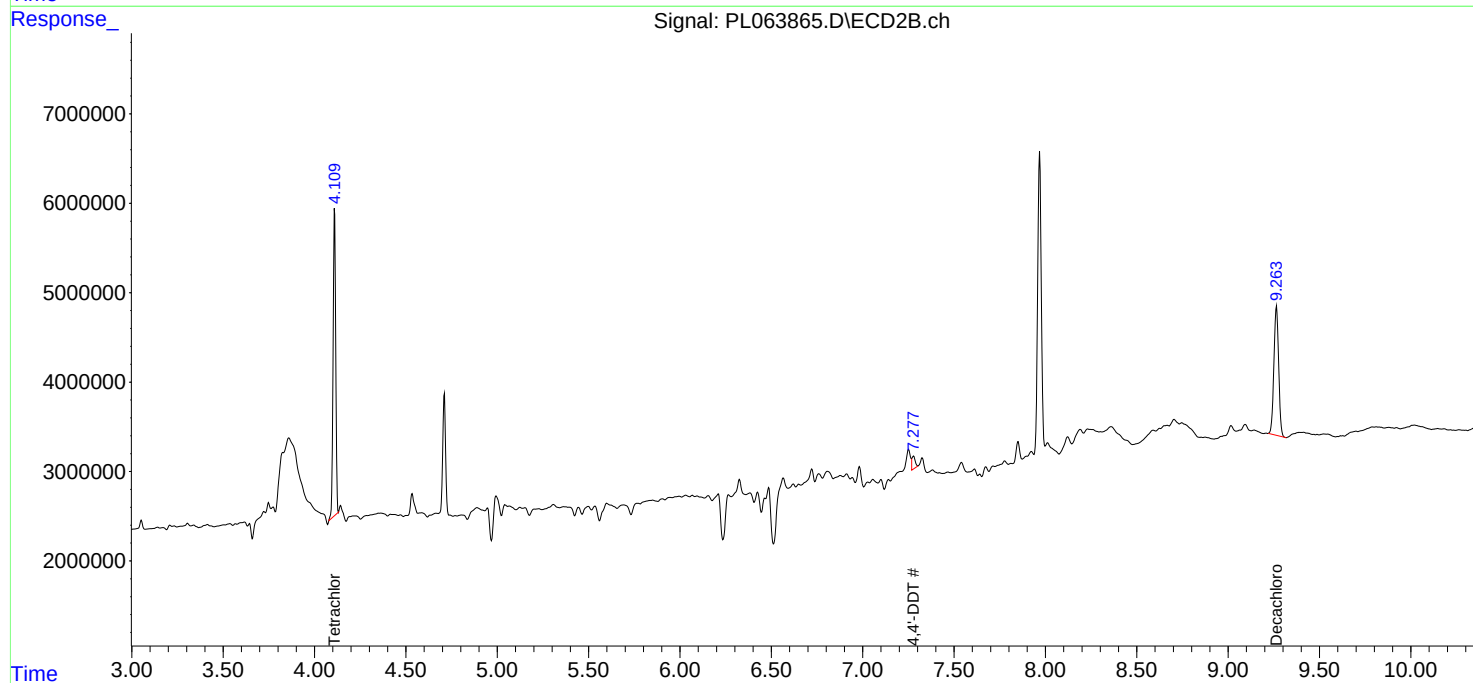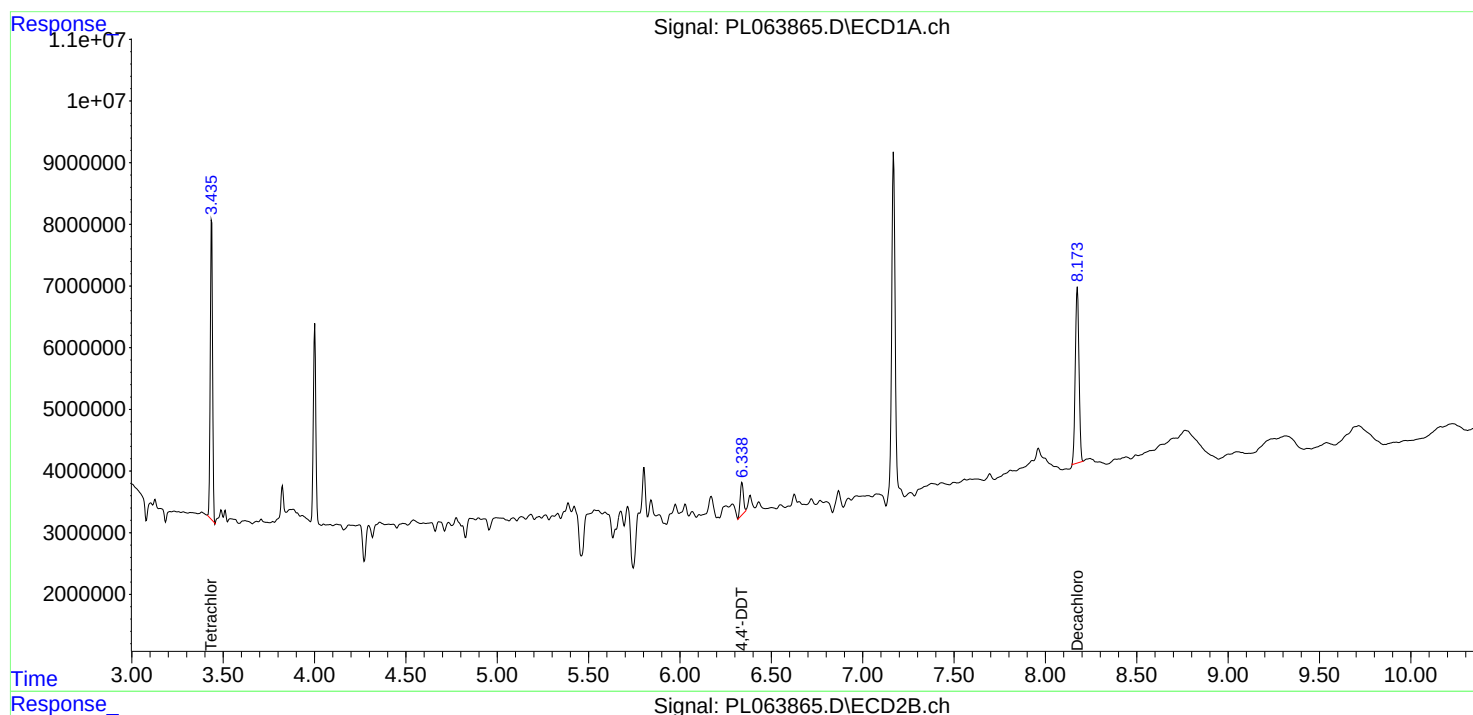

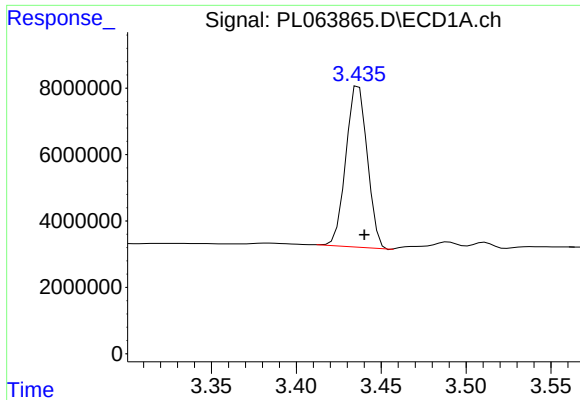


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: -0.003 min
Response: 42718638
Conc: 14.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-5(454+26)


Manual Integrations
APPROVED

Ankita
12/31/2020 1:11:12 PM

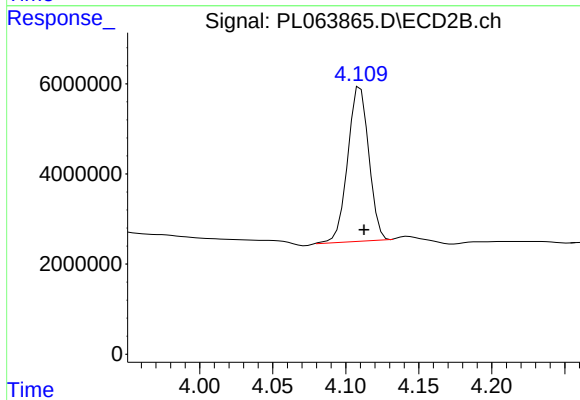


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.003 min
Response: 34313469
Conc: 13.44 ng/ml

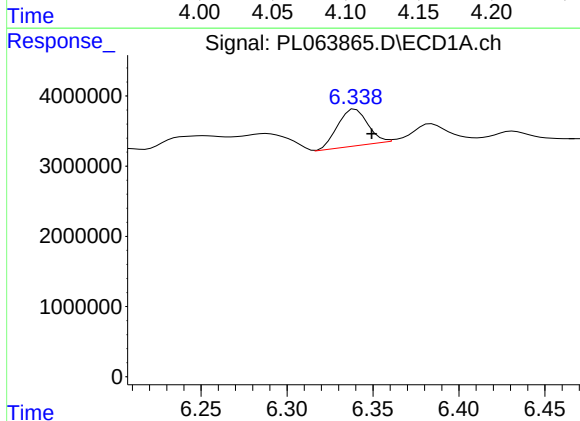


#17 4,4'-DDT

R.T.: 6.338 min
Delta R.T.: -0.011 min
Response: 6548640
Conc: 2.47 ng/ml m

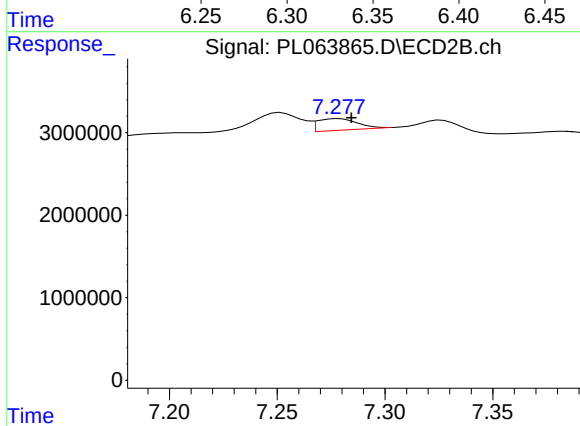

#17 4,4'-DDT

R.T.: 7.279 min
Delta R.T.: -0.006 min
Response: 1819798
Conc: 0.94 ng/ml

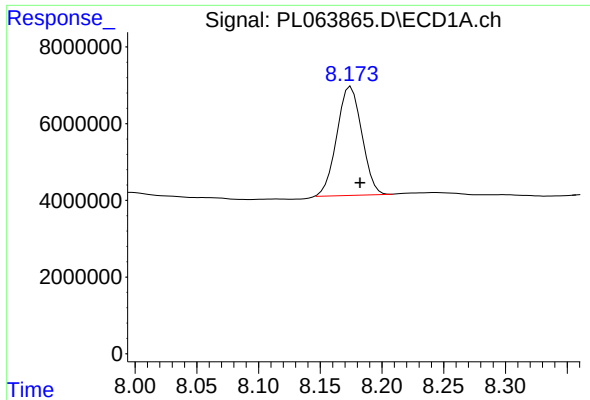


#28 Decachlorobiphenyl

R.T.: 8.175 min
Delta R.T.: -0.008 min
Response: 39940862
Conc: 14.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-5(454+26)

Manual Integrations
APPROVED

Ankita
12/31/2020 1:11:12 PM

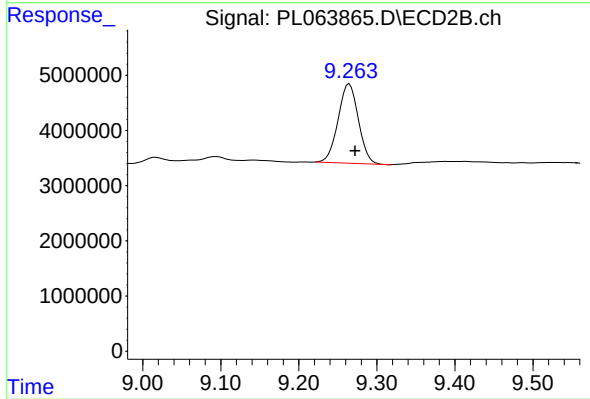

#28 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.007 min
Response: 25962394
Conc: 13.17 ng/ml