

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123021\
 Data File : PL071733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2021 12:29
 Operator : AR\AJ
 Sample : PB141761BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 05:23:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.561	5.497	13570653	34090075	20.916	19.977
28)	SA Decachlor...	10.322	11.388	17370075	26653538	23.332	21.267
Target Compounds							
2)	A alpha-BHC	5.271	0.000	408655	0	0.450	N.D. #
5)	MB Aldrin	0.000	7.496	0	37381	N.D.	0.017 #
8)	B Heptachlo...	0.000	7.975	0	43747	N.D.	0.022 #
10)	B gamma-Chl...	0.000	8.241	0	341603	N.D.	0.175 #
11)	B alpha-Chl...	0.000	8.292f	0	46947	N.D.	0.025 #
24)	Chlordane-2	0.000	7.474	0	78108	N.D.	1.060 #
25)	Chlordane-3	0.000	8.241	0	341603	N.D.	1.236 #
26)	Chlordane-4	0.000	8.292f	0	46947	N.D.	0.145 #
27)	Chlordane-5	0.000	9.192	0	621312	N.D.	11.453 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123021\
Data File : PL071733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2021 12:29
Operator : AR\AJ
Sample : PB141761BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 05:23:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

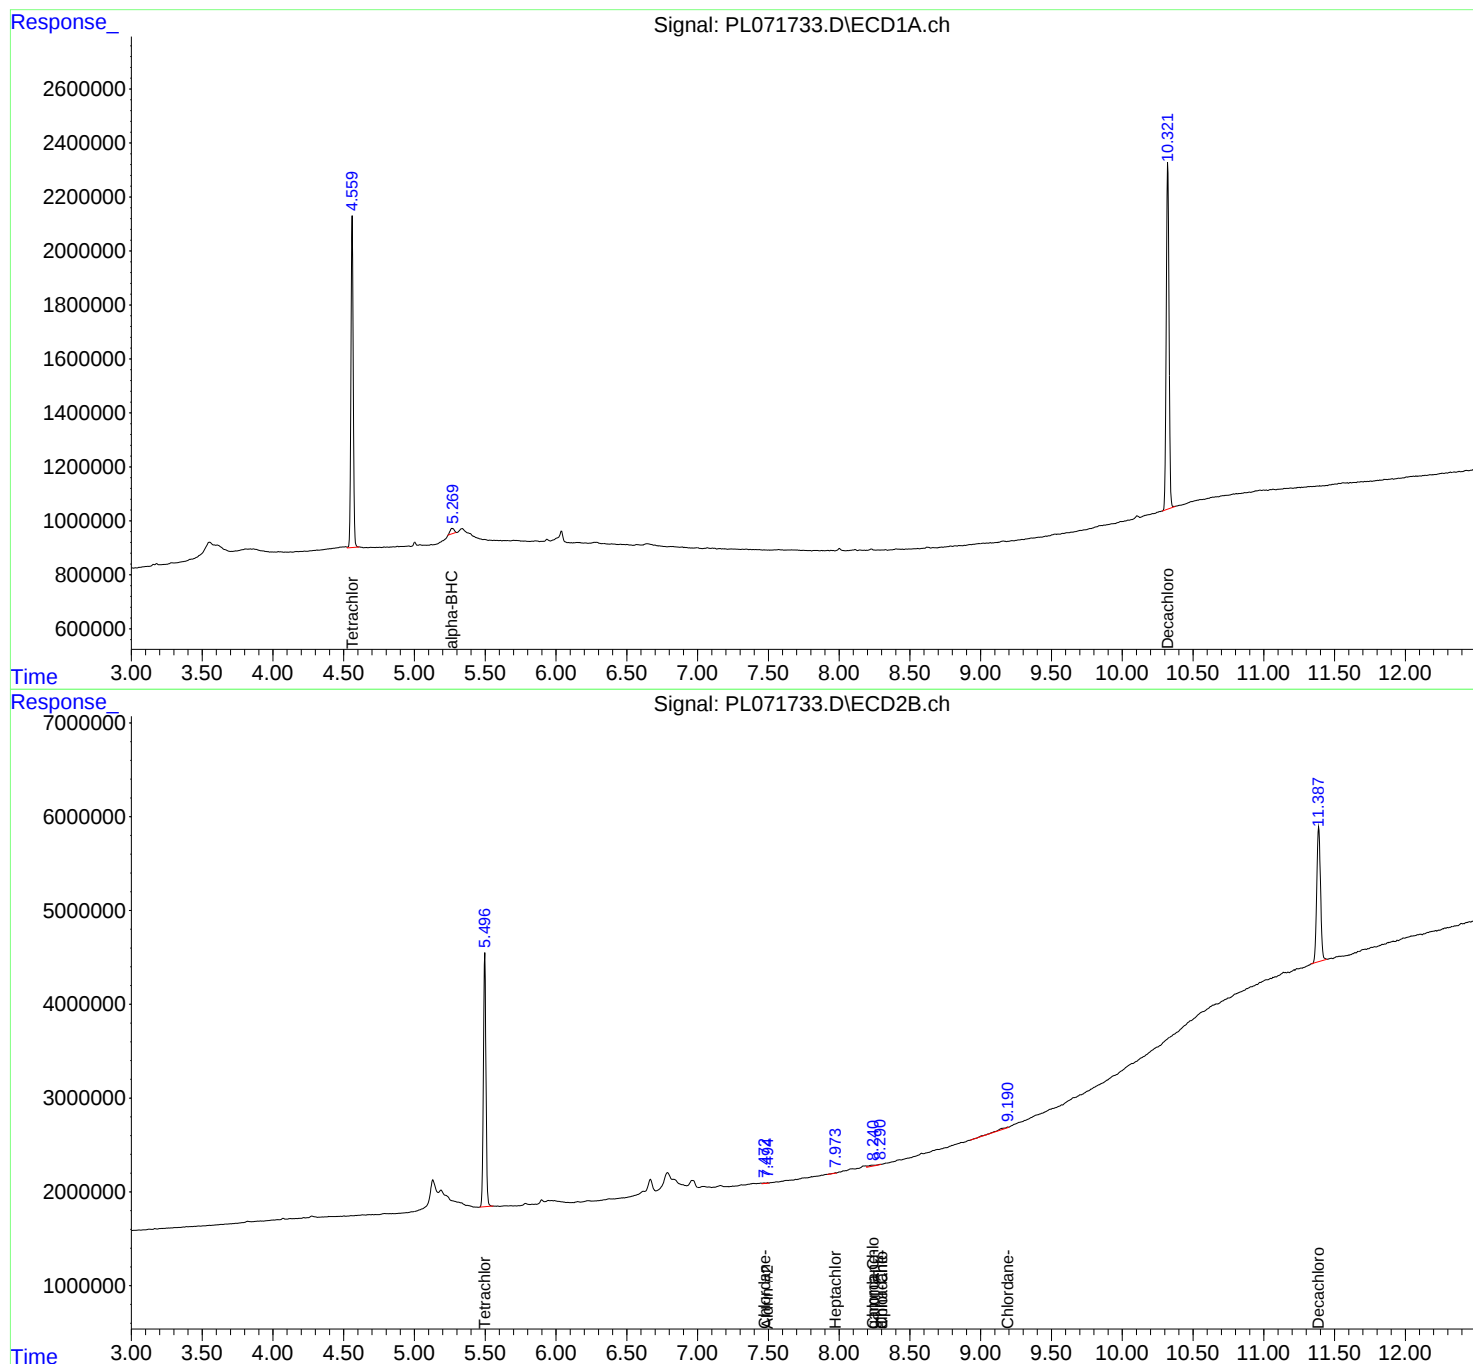


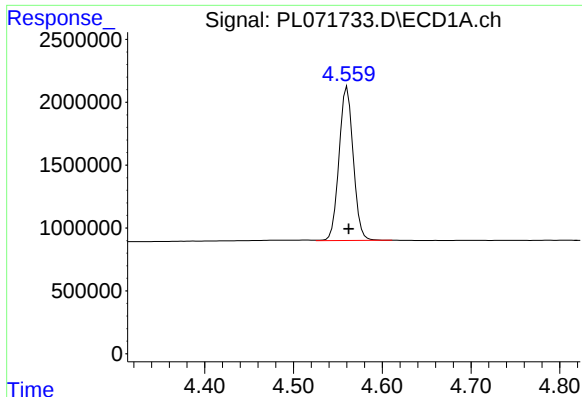

#1 Tetrachloro-m-xylene


R.T.: 4.561 min
Delta R.T.: -0.001 min
Response: 13570653
Conc: 20.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

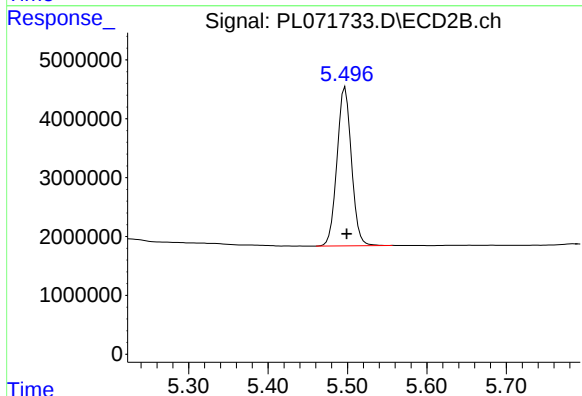


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: -0.002 min
Response: 34090075
Conc: 19.98 ng/ml

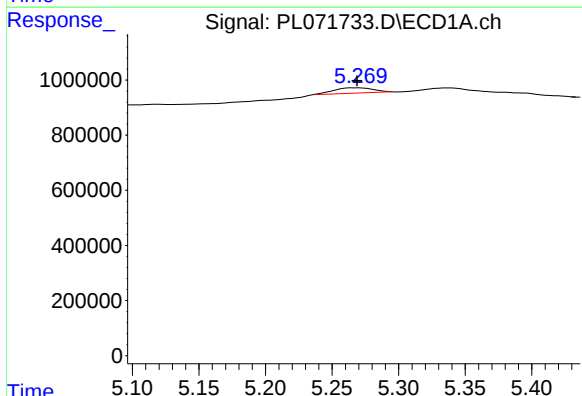


#2 alpha-BHC

R.T.: 5.271 min
Delta R.T.: 0.002 min
Response: 408655
Conc: 0.45 ng/ml

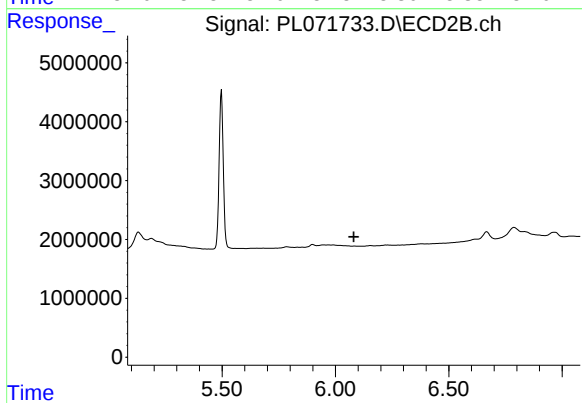

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.080 min
Response: 0
Conc: N.D.

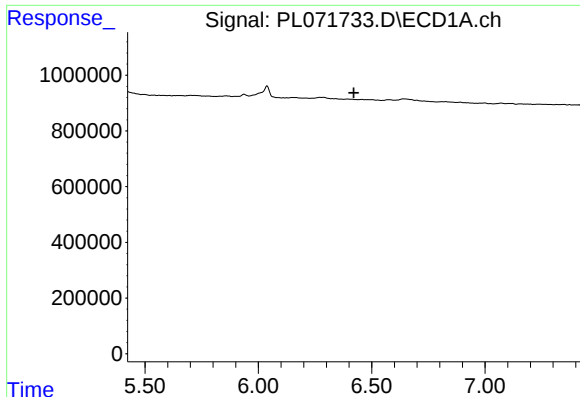

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

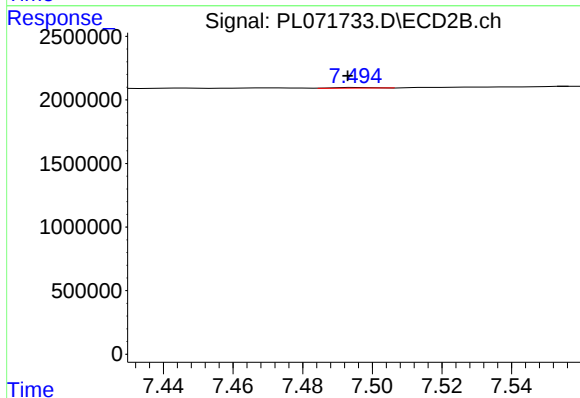


#5 Aldrin

R.T.: 7.496 min
Delta R.T.: 0.003 min
Response: 37381
Conc: 0.02 ng/ml

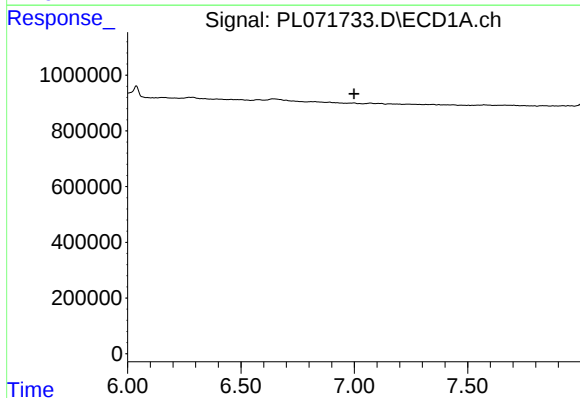


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

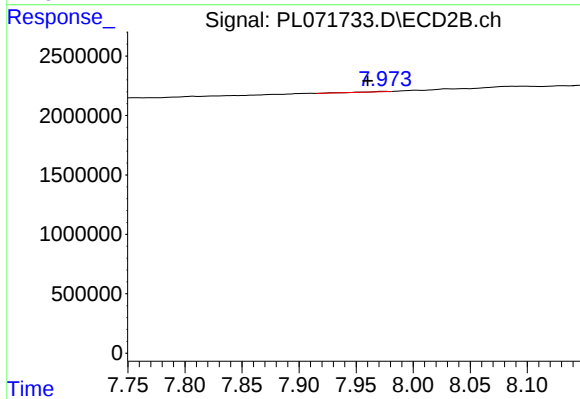

#8 Heptachlor epoxide


R.T.: 7.975 min
Delta R.T.: 0.015 min
Response: 43747
Conc: 0.02 ng/ml

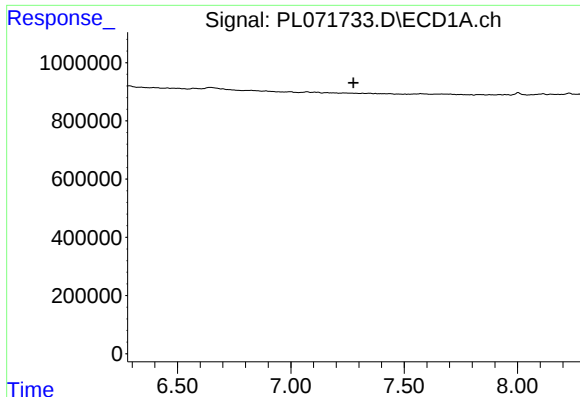

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

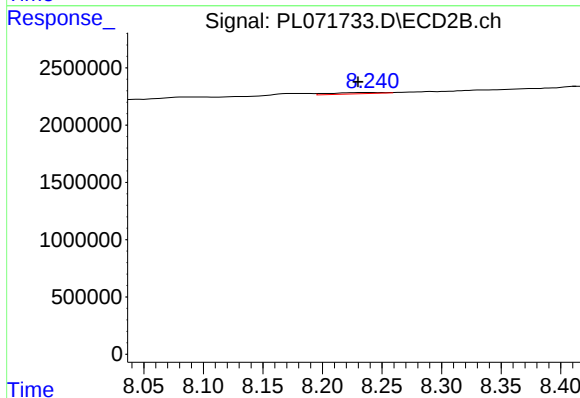


#10 gamma-Chlordane

R.T.: 8.241 min
Delta R.T.: 0.011 min
Response: 341603
Conc: 0.18 ng/ml

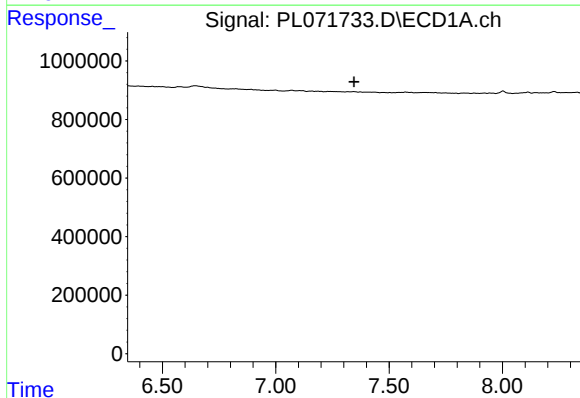


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

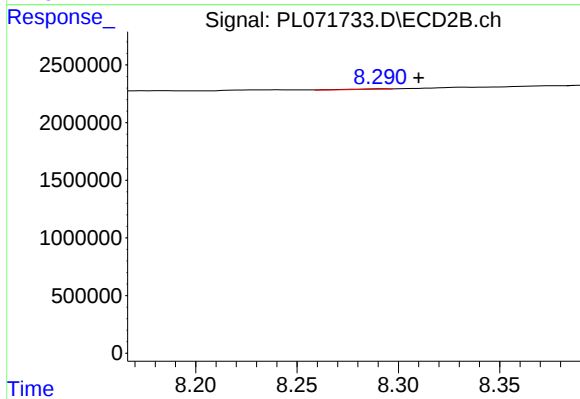

#11 alpha-Chlordane


R.T.: 8.292 min
Delta R.T.: -0.018 min
Response: 46947
Conc: 0.03 ng/ml

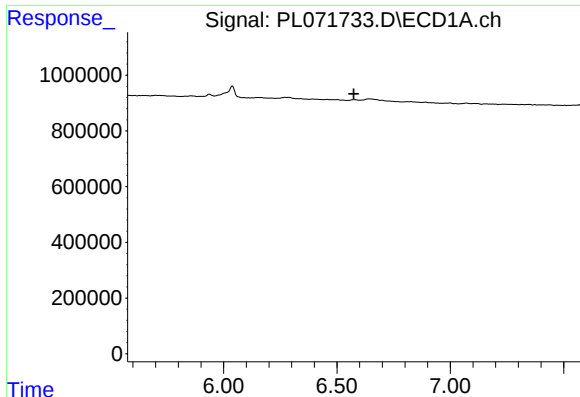

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

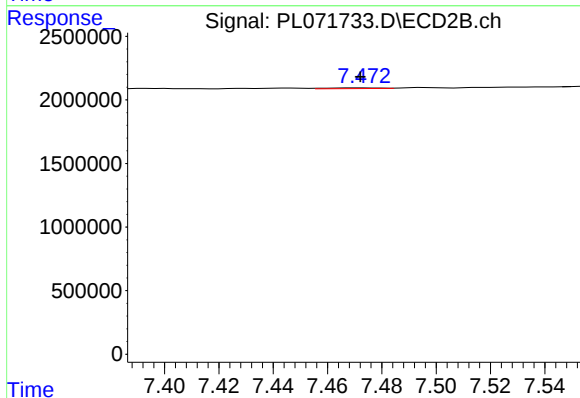


#24 Chlordane-2

R.T.: 7.474 min
Delta R.T.: 0.002 min
Response: 78108
Conc: 1.06 ng/ml

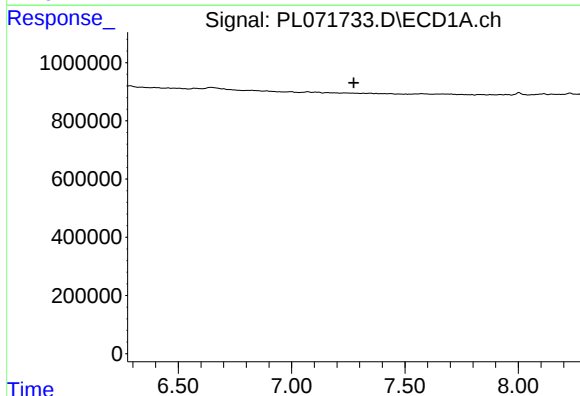


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

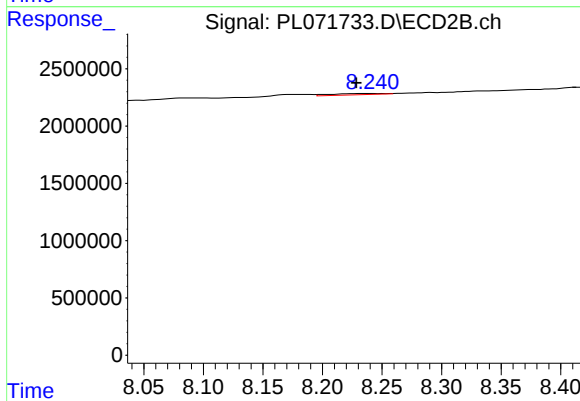

#25 Chlordane-3


R.T.: 8.241 min
Delta R.T.: 0.013 min
Response: 341603
Conc: 1.24 ng/ml

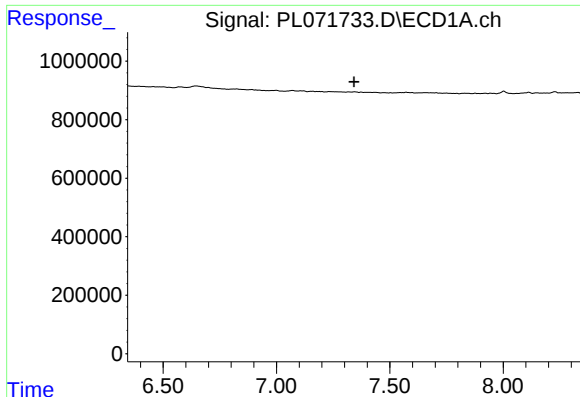

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

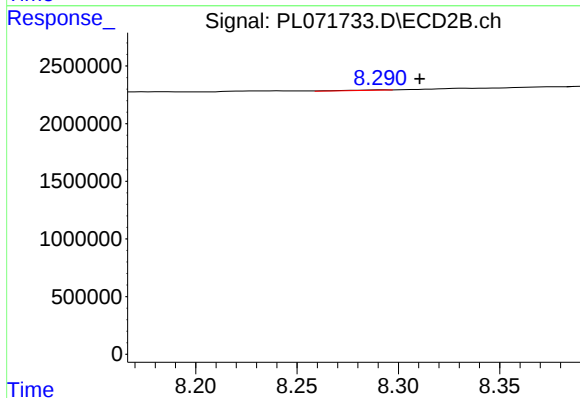


#26 Chlordane-4

R.T.: 8.292 min
Delta R.T.: -0.019 min
Response: 46947
Conc: 0.14 ng/ml

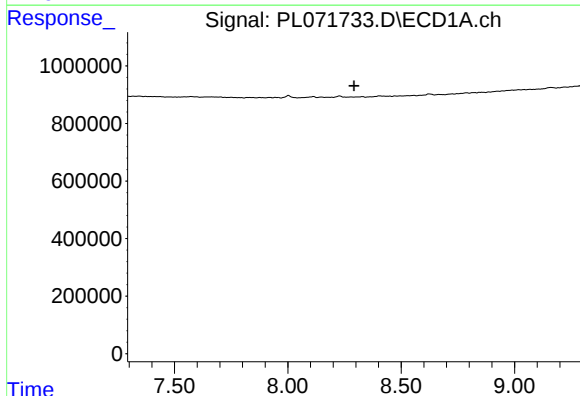


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.292 min
Response: 0
Conc: N.D.

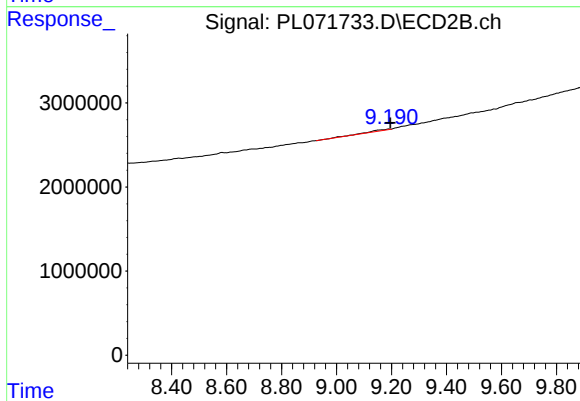

#27 Chlordane-5


R.T.: 9.192 min
Delta R.T.: -0.005 min
Response: 621312
Conc: 11.45 ng/ml

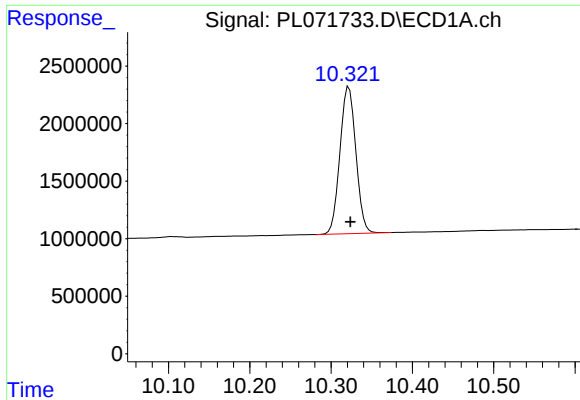

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: -0.002 min
Response: 17370075
Conc: 23.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

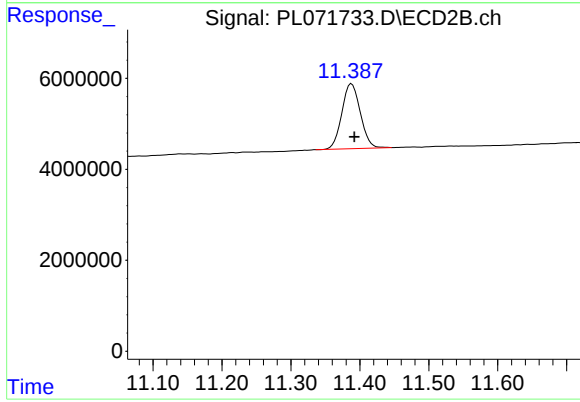

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: -0.004 min
Response: 26653538
Conc: 21.27 ng/ml