

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123021\
 Data File : PL071750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2021 19:17
 Operator : AR\AJ
 Sample : PB141777BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 05:28:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	10715526	28202399	16.516	16.527
28)	SA Decachlor...	10.318	11.385	14203395	22924907	19.079	18.292
Target Compounds							
5)	MB Aldrin	0.000	7.483	0	91682	N.D.	0.042 #
10)	B gamma-Chl...	0.000	8.231	0	276212	N.D.	0.142 #
14)	MA Endrin	0.000	8.881	0	56037	N.D.	0.037 #
17)	MA 4,4'-DDT	0.000	9.379f	0	89428	N.D.	0.066 #
19)	B Endosulfa...	0.000	9.530f	0	287740	N.D.	0.204 #
24)	Chlordane-2	0.000	7.483	0	91682	N.D.	1.244 #
25)	Chlordane-3	0.000	8.231	0	276212	N.D.	1.000 #
27)	Chlordane-5	0.000	9.206	0	20861	N.D.	0.385 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123021\
Data File : PL071750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2021 19:17
Operator : AR\AJ
Sample : PB141777BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 05:28:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

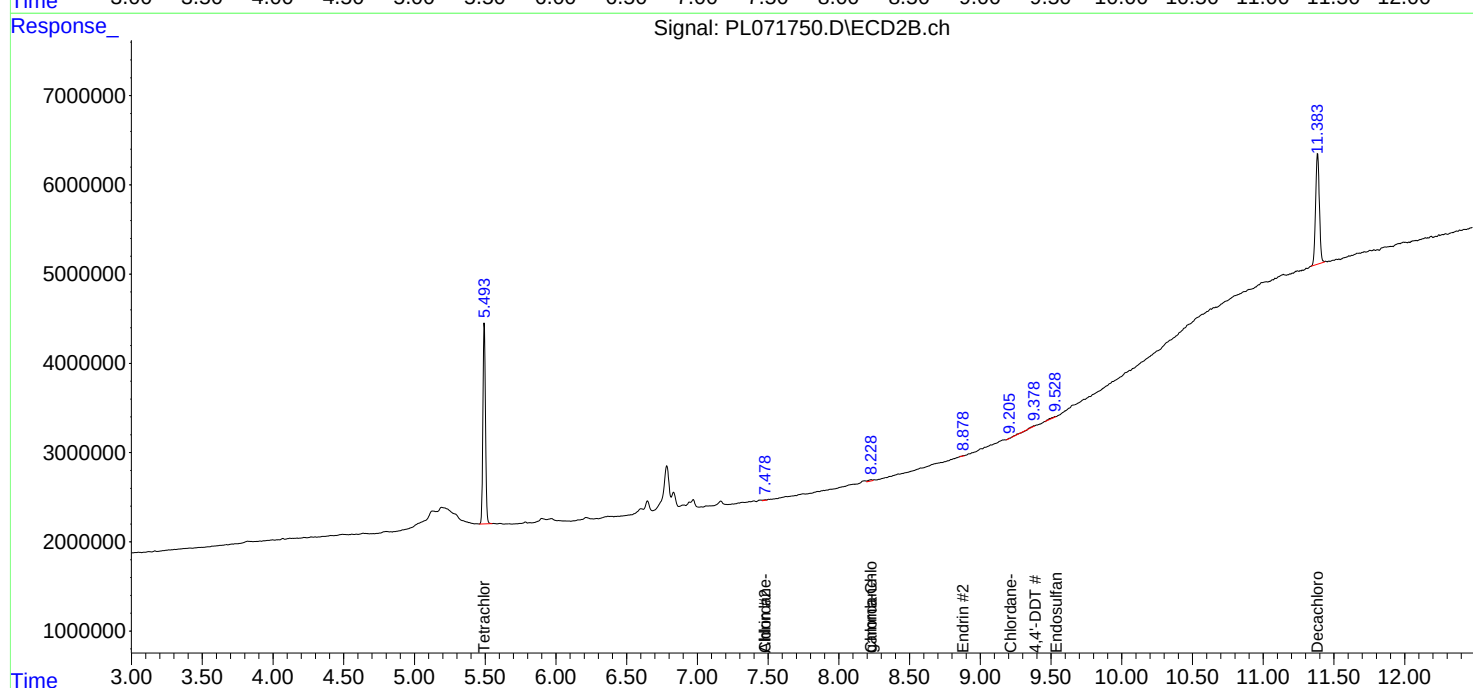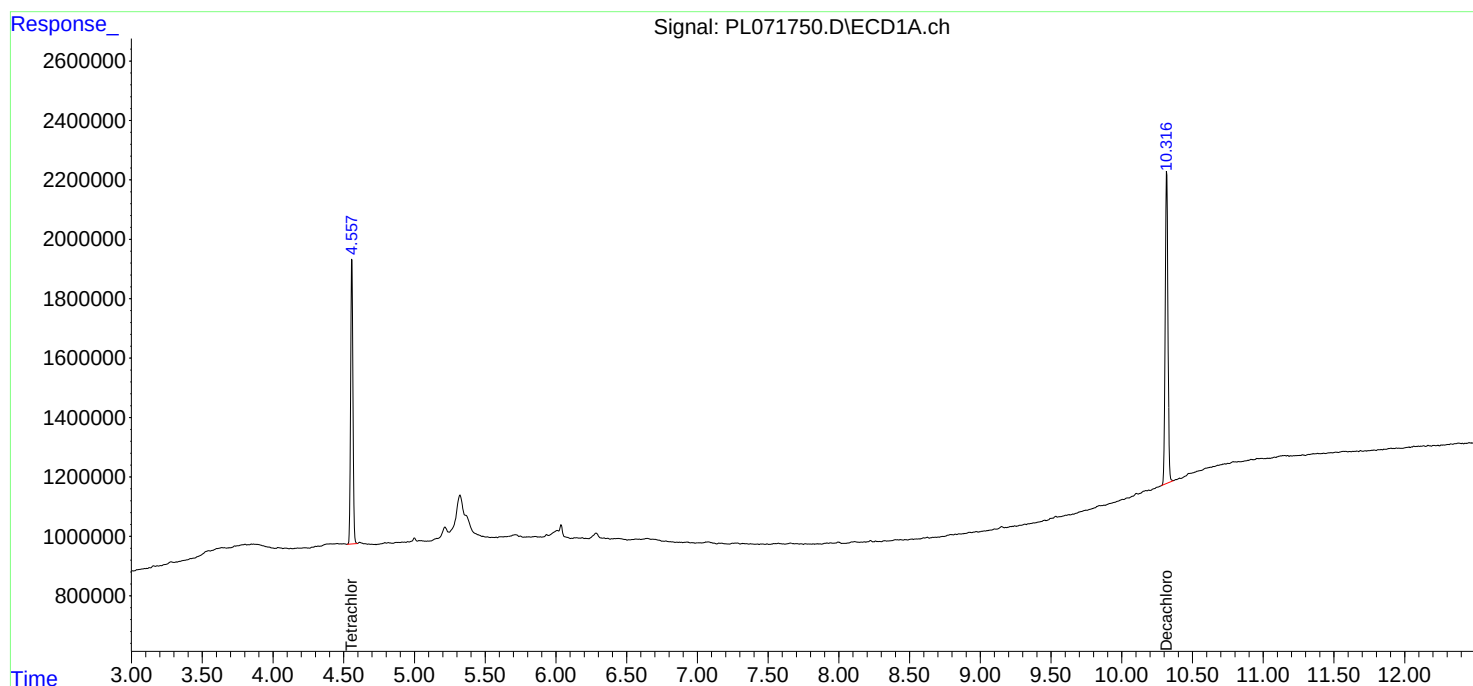


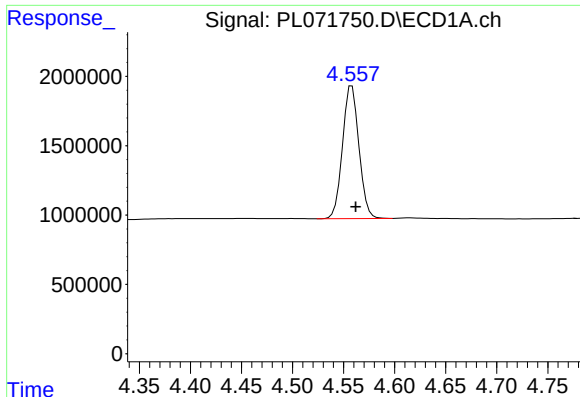

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: -0.004 min
Response: 10715526
Conc: 16.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

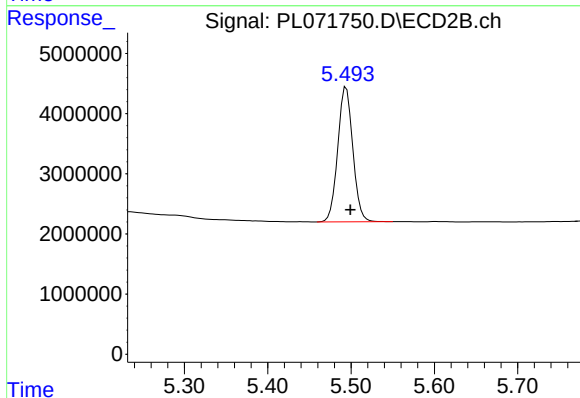


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: -0.005 min
Response: 28202399
Conc: 16.53 ng/ml

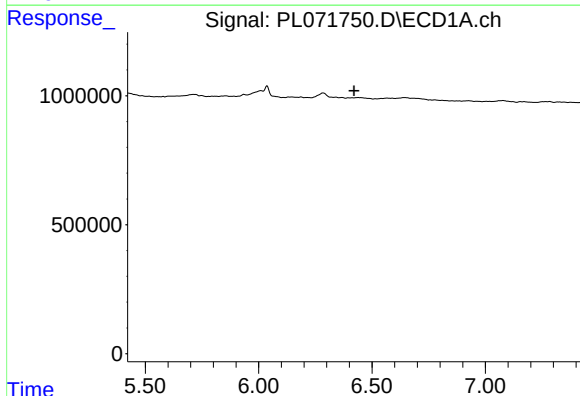


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

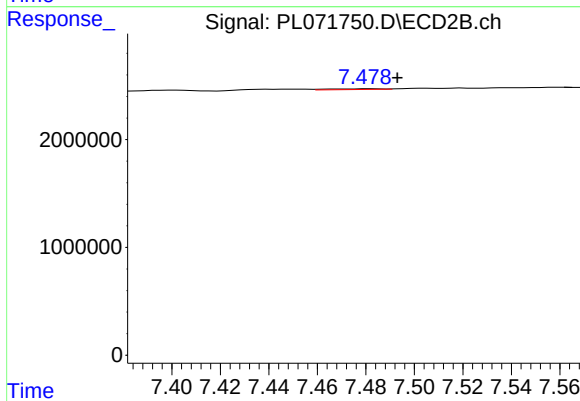

#5 Aldrin


R.T.: 7.483 min
Delta R.T.: -0.010 min
Response: 91682
Conc: 0.04 ng/ml

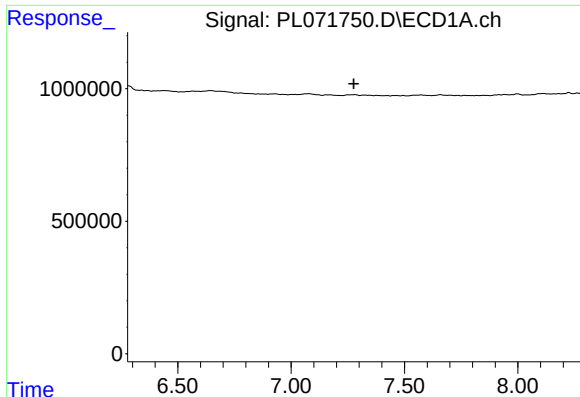

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

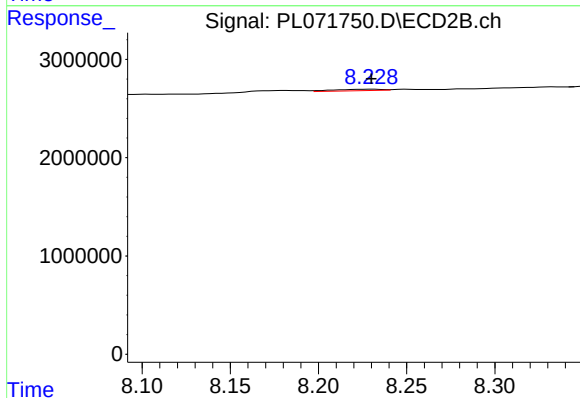


#10 gamma-Chlordane

R.T.: 8.231 min
Delta R.T.: 0.000 min
Response: 276212
Conc: 0.14 ng/ml

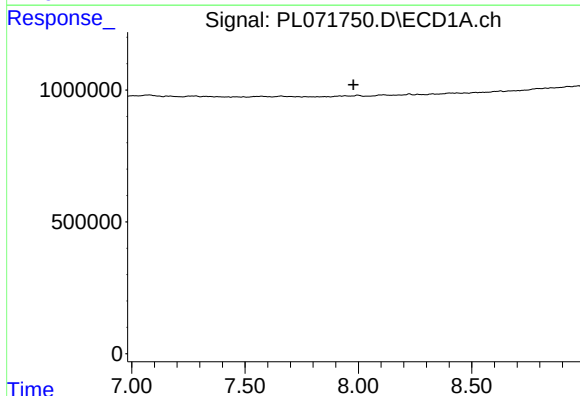


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 7.979 min
Response: 0
Conc: N.D.

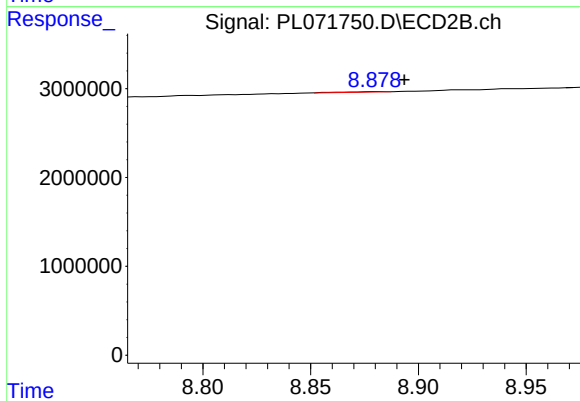

#14 Endrin


R.T.: 8.881 min
Delta R.T.: -0.012 min
Response: 56037
Conc: 0.04 ng/ml

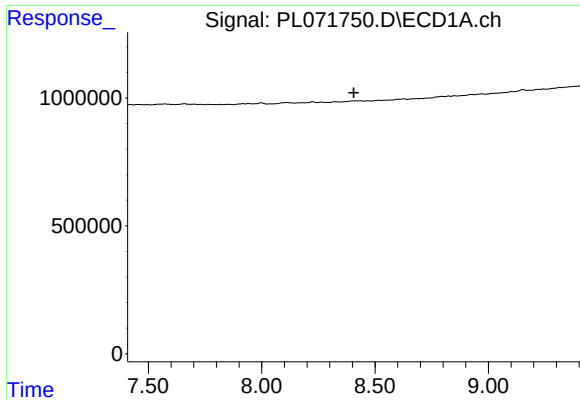

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

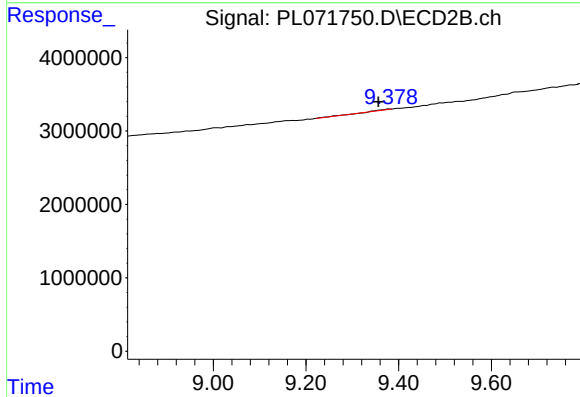


#17 4,4'-DDT

R.T.: 9.379 min
Delta R.T.: 0.023 min
Response: 89428
Conc: 0.07 ng/ml

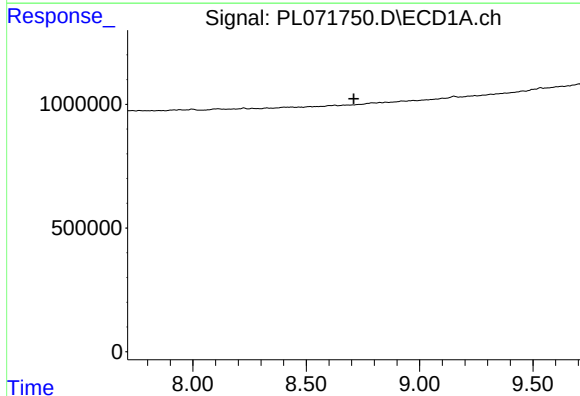


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

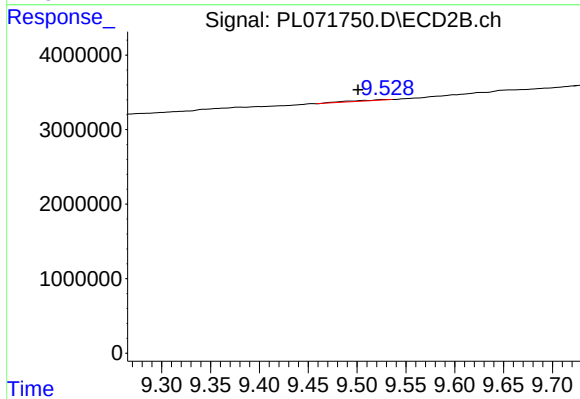

#19 Endosulfan Sulfate


R.T.: 9.530 min
Delta R.T.: 0.029 min
Response: 287740
Conc: 0.20 ng/ml

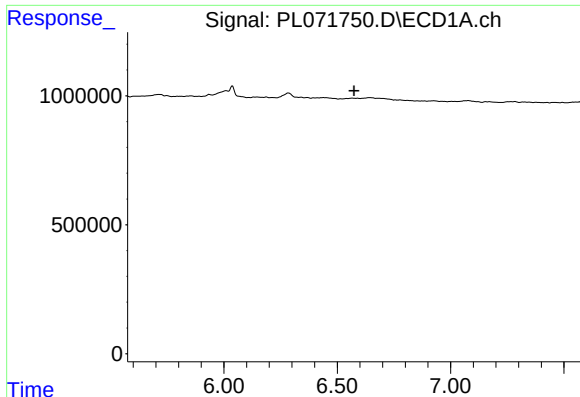

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 6.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

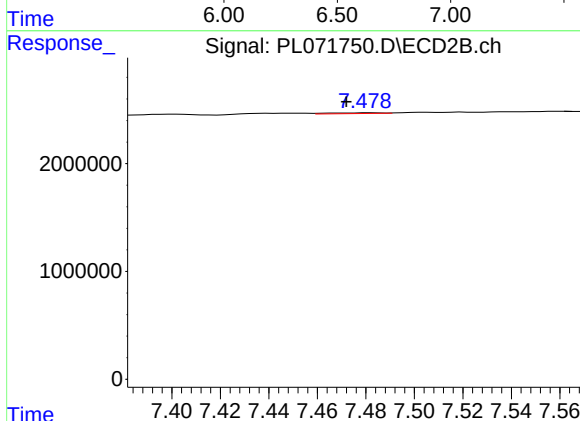


#24 Chlordane-2

R.T.: 7.483 min
Delta R.T.: 0.011 min
Response: 91682
Conc: 1.24 ng/ml

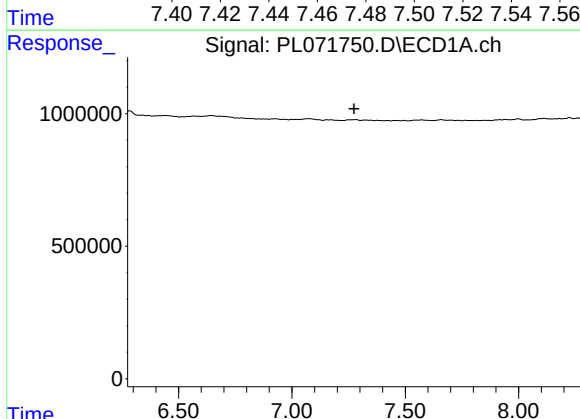


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.275 min
Response: 0
Conc: N.D.

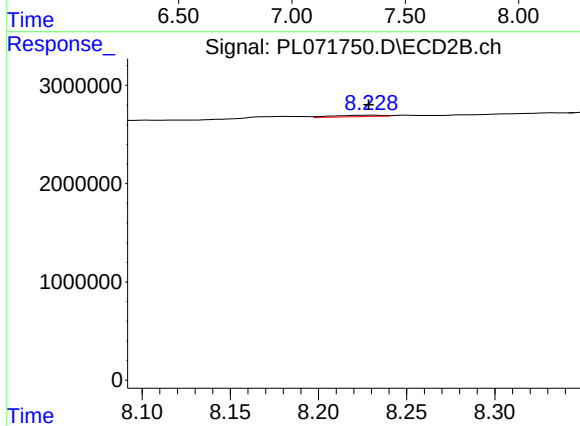

#25 Chlordane-3


R.T.: 8.231 min
Delta R.T.: 0.002 min
Response: 276212
Conc: 1.00 ng/ml

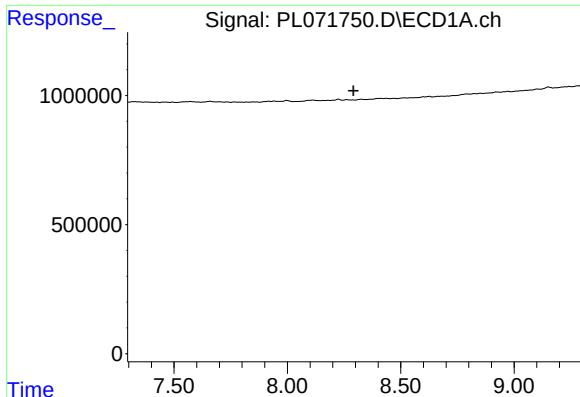

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.292 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

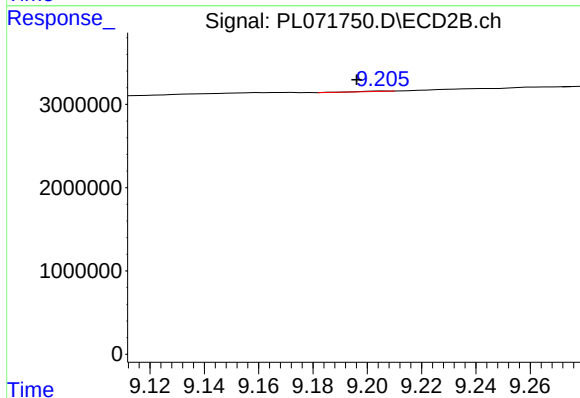


#27 Chlordane-5

R.T.: 9.206 min
Delta R.T.: 0.010 min
Response: 20861
Conc: 0.38 ng/ml

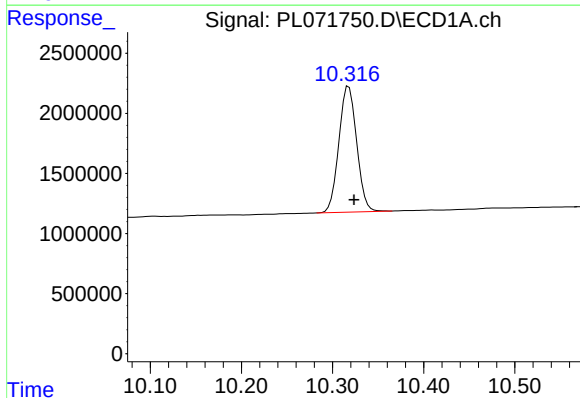

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.006 min
Response: 14203395
Conc: 19.08 ng/ml

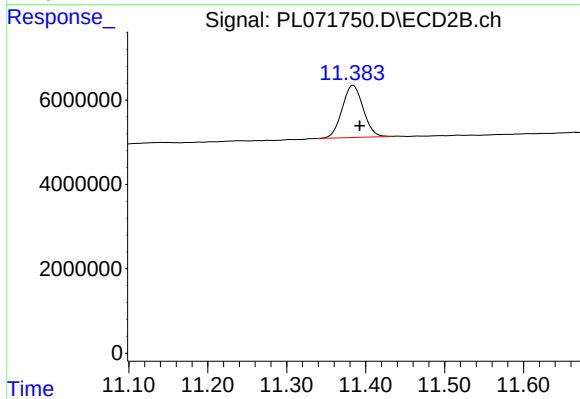

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.008 min
Response: 22924907
Conc: 18.29 ng/ml