

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123021\
 Data File : PL071753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2021 20:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 05:28:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	13684506	35606757	21.092	20.866
28)	SA Decachlor...	10.317	11.384	17015981	26997771	22.857	21.542
Target Compounds							
8)	B Heptachlo...	0.000	7.965	0	1513767	N.D.	0.770 #
10)	B gamma-Chl...	0.000	8.256f	0	5291162	N.D.	2.712 #
11)	B alpha-Chl...	0.000	8.329f	0	645825	N.D.	0.347 #
13)	MA Dieldrin	7.701	0.000	416349	0	0.505	N.D. #
14)	MA Endrin	8.000f	8.900	833706	722766	1.121	0.480 #
19)	B Endosulfa...	0.000	9.500	0	154039	N.D.	0.109 #
24)	Chlordane-2	0.000	7.458	0	40690	N.D.	0.552 #
25)	Chlordane-3	0.000	8.256f	0	5291162	N.D.	19.148 #
26)	Chlordane-4	0.000	8.329f	0	645825	N.D.	1.991 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123021\
Data File : PL071753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2021 20:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 05:28:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

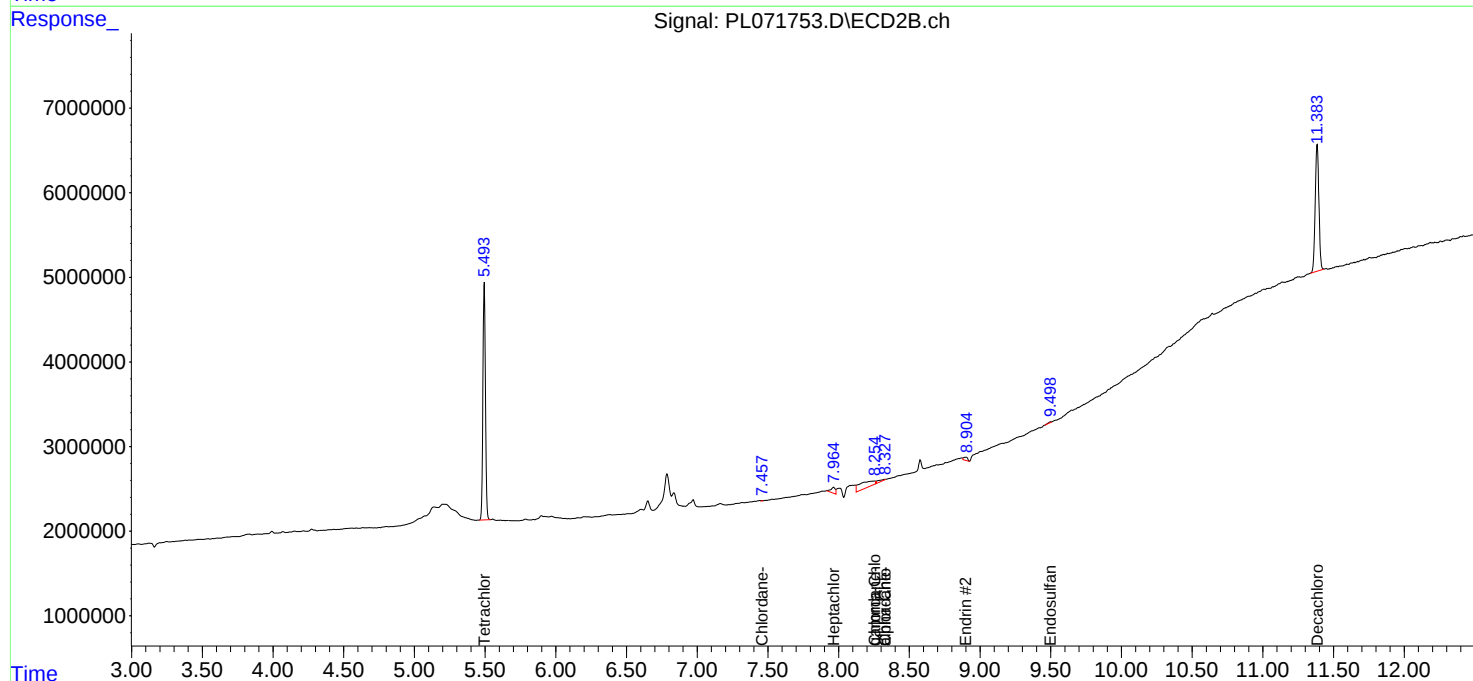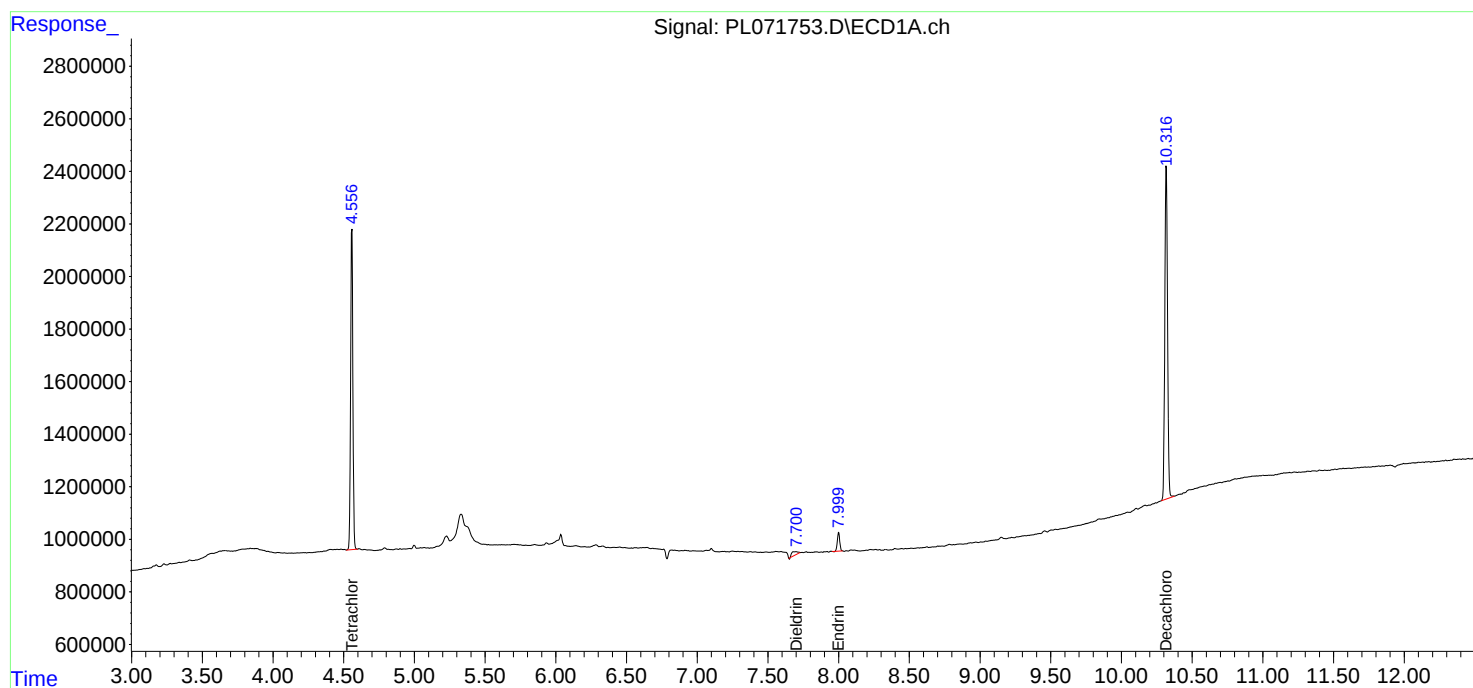


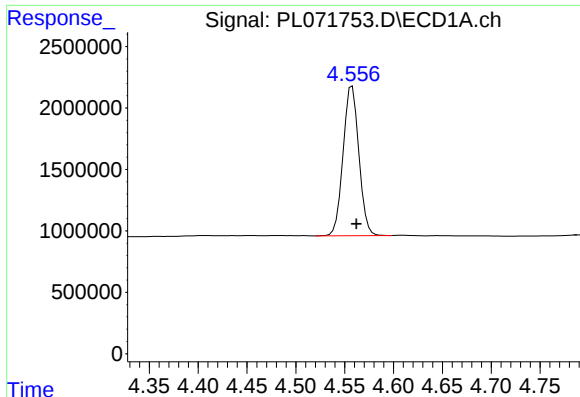

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: -0.004 min
Response: 13684506
Conc: 21.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

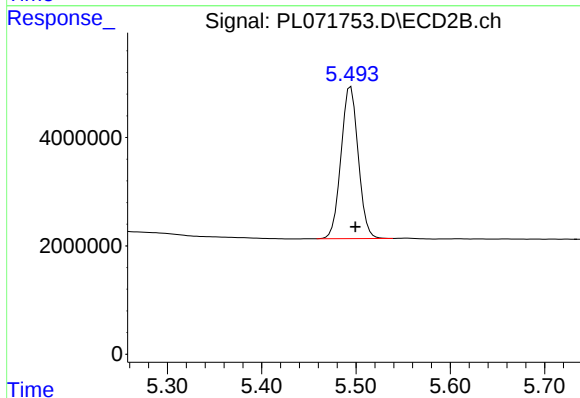


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: -0.005 min
Response: 35606757
Conc: 20.87 ng/ml

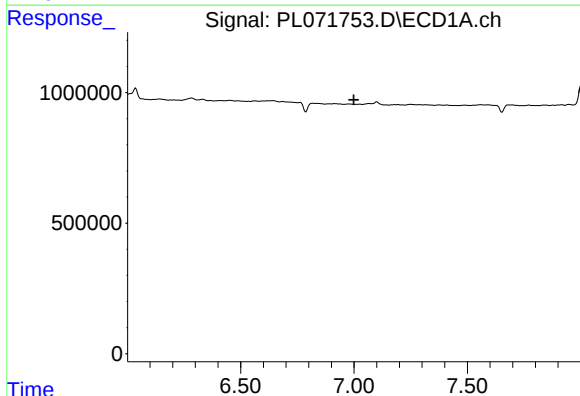


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

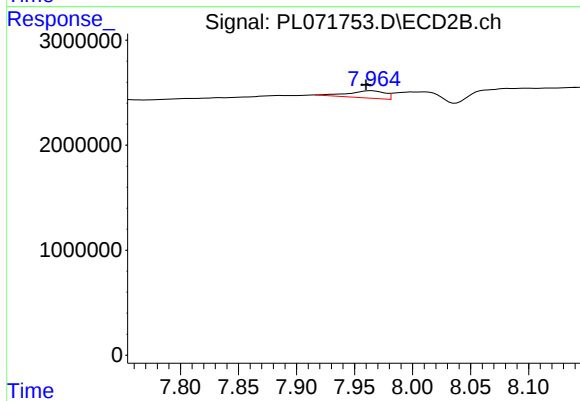

#8 Heptachlor epoxide


R.T.: 7.965 min
Delta R.T.: 0.005 min
Response: 1513767
Conc: 0.77 ng/ml

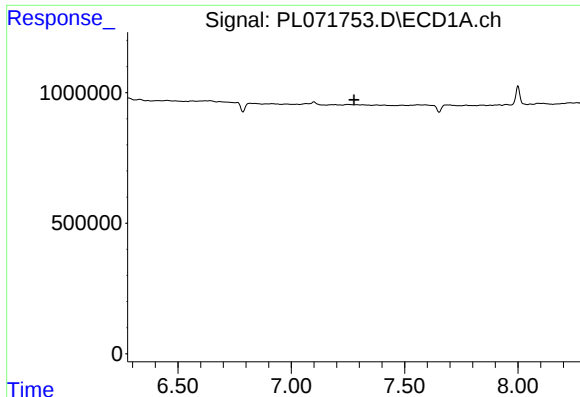

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

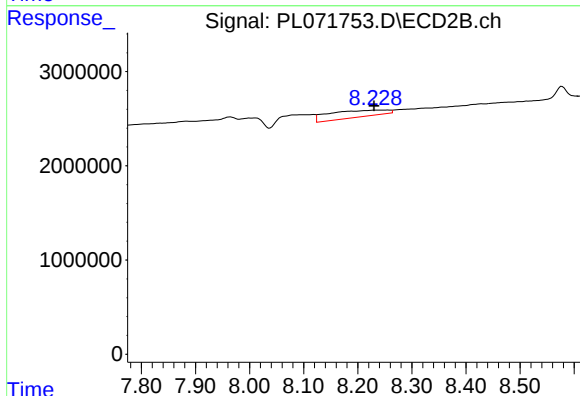


#10 gamma-Chlordane

R.T.: 8.256 min
Delta R.T.: 0.026 min
Response: 5291162
Conc: 2.71 ng/ml

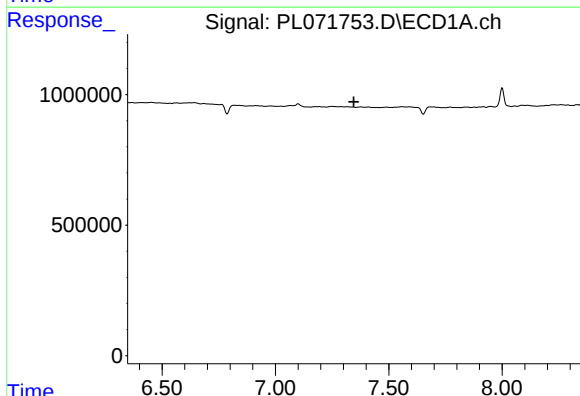


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

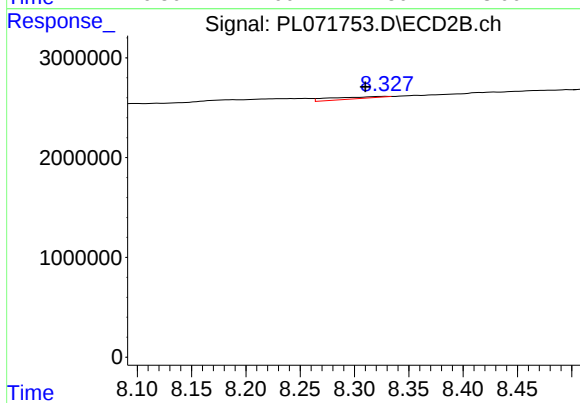

#11 alpha-Chlordane


R.T.: 8.329 min
Delta R.T.: 0.019 min
Response: 645825
Conc: 0.35 ng/ml

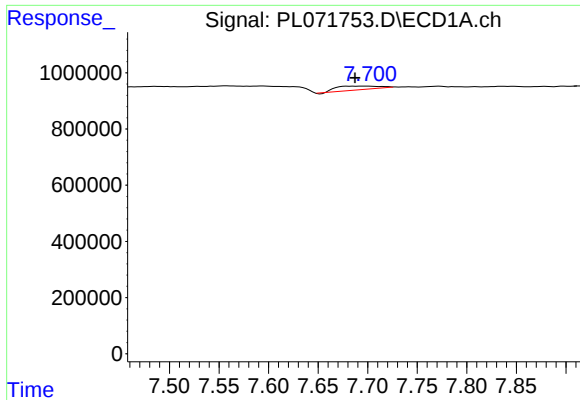

#13 Dieldrin


R.T.: 7.701 min
Delta R.T.: 0.013 min
Response: 416349
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

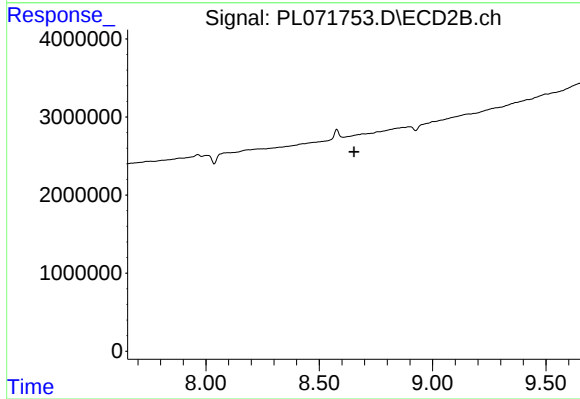


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.654 min
Response: 0
Conc: N.D.

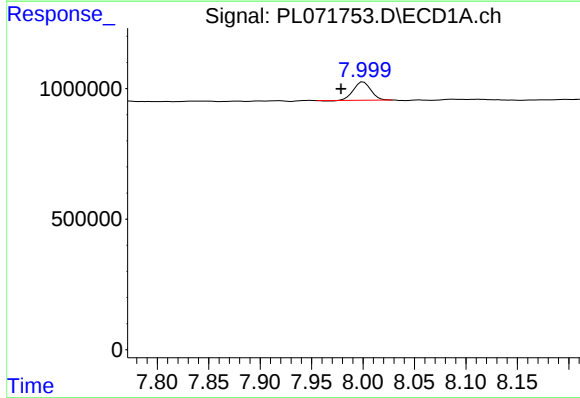


#14 Endrin

R.T.: 8.000 min
Delta R.T.: 0.022 min
Response: 833706
Conc: 1.12 ng/ml

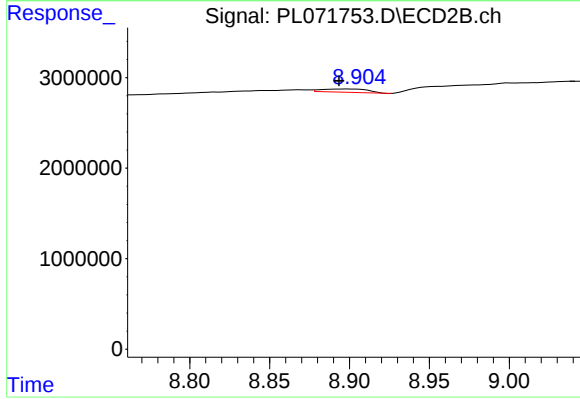

#14 Endrin


R.T.: 8.900 min
Delta R.T.: 0.006 min
Response: 722766
Conc: 0.48 ng/ml

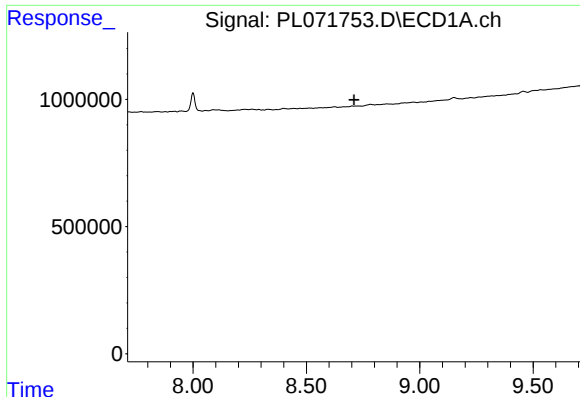

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

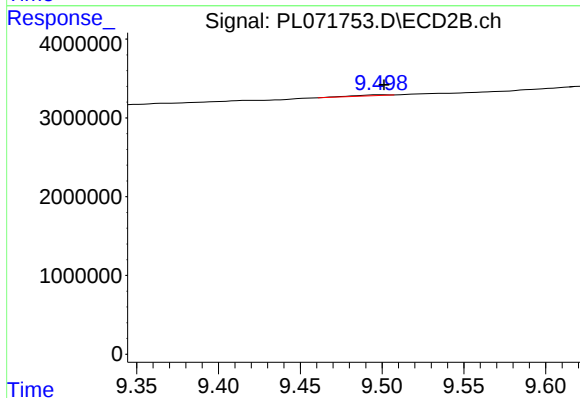


#19 Endosulfan Sulfate

R.T.: 9.500 min
Delta R.T.: 0.000 min
Response: 154039
Conc: 0.11 ng/ml

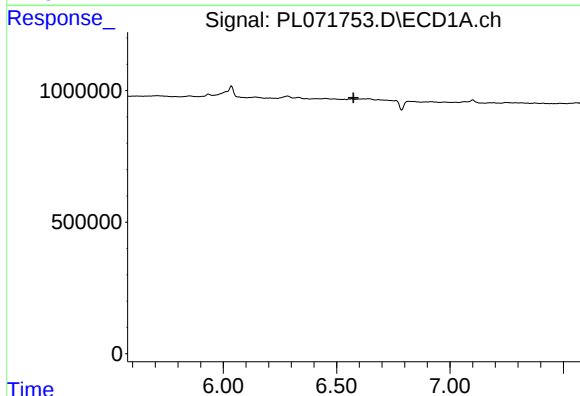


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.575 min
Response: 0
Conc: N.D.

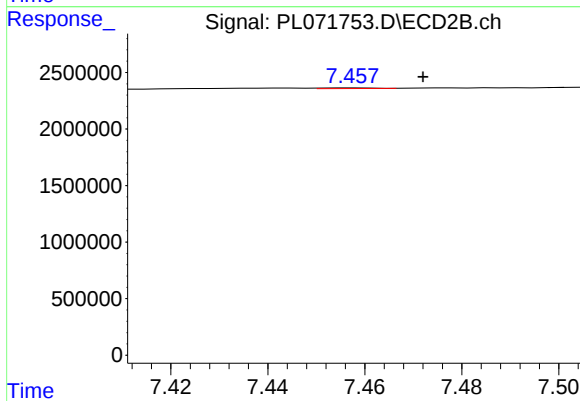

#24 Chlordane-2


R.T.: 7.458 min
Delta R.T.: -0.014 min
Response: 40690
Conc: 0.55 ng/ml

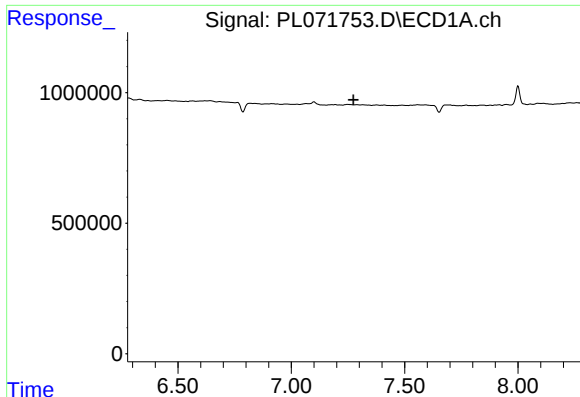

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

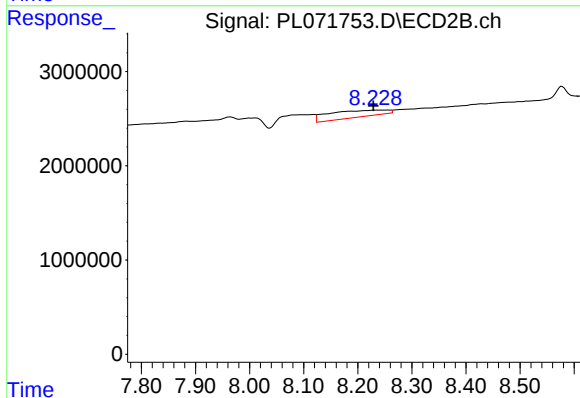


#25 Chlordane-3

R.T.: 8.256 min
Delta R.T.: 0.027 min
Response: 5291162
Conc: 19.15 ng/ml

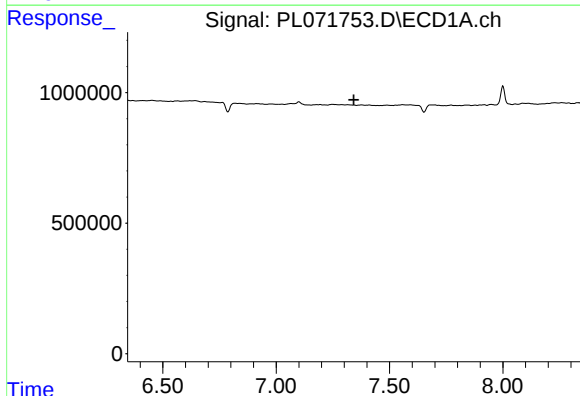


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

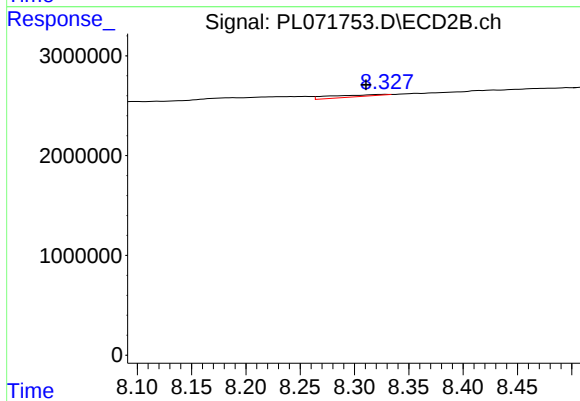

#26 Chlordane-4


R.T.: 8.329 min
Delta R.T.: 0.018 min
Response: 645825
Conc: 1.99 ng/ml

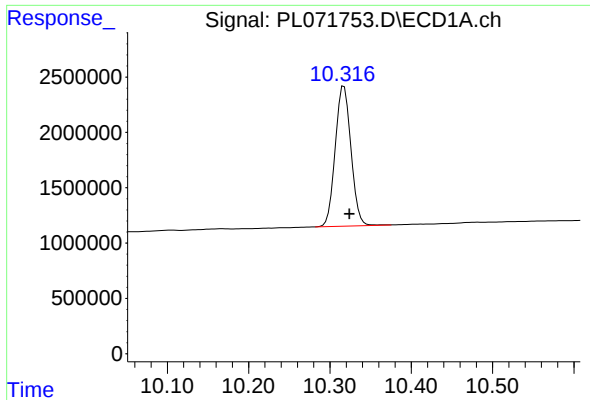

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.007 min
Response: 17015981
Conc: 22.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

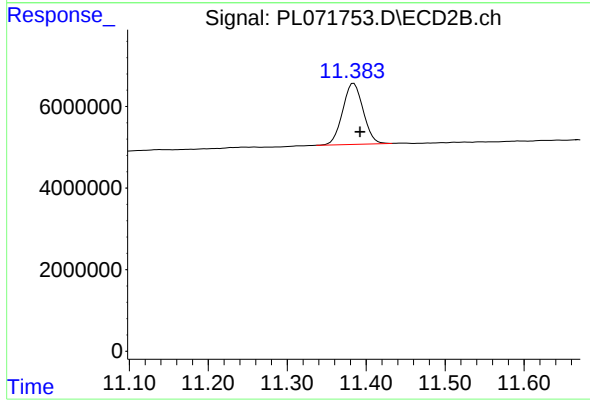

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.008 min
Response: 26997771
Conc: 21.54 ng/ml