

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123021\
 Data File : PL071759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2021 22:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 05:30:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 27 14:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	14084595	37138044	21.709	21.764
28)	SA Decachlor...	10.318	11.384	16186751	26907445	21.743	21.469
Target Compounds							
8)	B Heptachlo...	0.000	7.963	0	1390548	N.D.	0.707 #
10)	B gamma-Chl...	0.000	8.245	0	503234	N.D.	0.258 #
13)	MA Dieldrin	7.697	0.000	120285	0	0.146	N.D. #
14)	MA Endrin	8.000f	8.903	641317	688844	0.862	0.457 #
16)	A 4,4'-DDD	0.000	9.036	0	2882886	N.D.	2.220 #
18)	B Endrin al...	0.000	9.293f	0	197124	N.D.	0.170 #
24)	Chlordane-2	0.000	7.455f	0	74541	N.D.	1.012 #
25)	Chlordane-3	0.000	8.245f	0	503234	N.D.	1.821 #
27)	Chlordane-5	0.000	9.175f	0	1709275	N.D.	31.507 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123021\
Data File : PL071759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2021 22:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 05:30:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122721.M
Quant Title : GC Extractables
QLast Update : Mon Dec 27 14:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

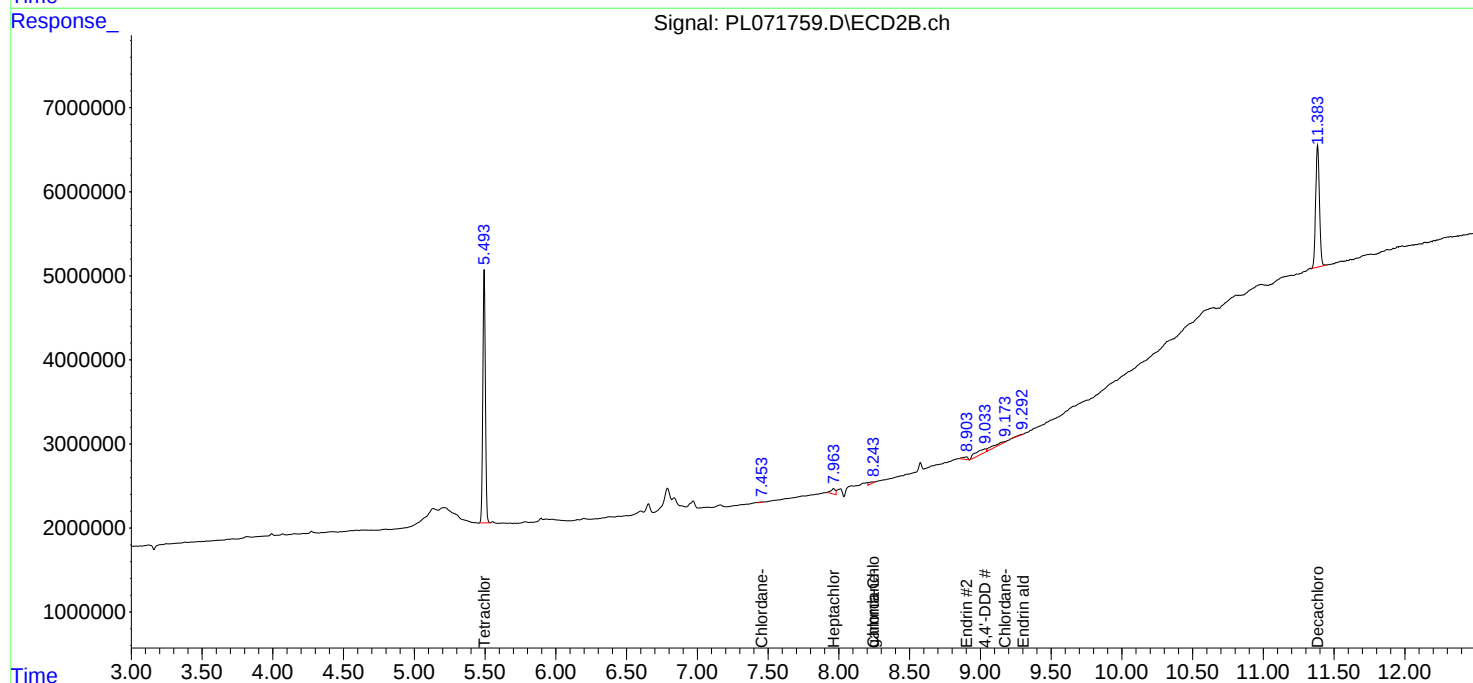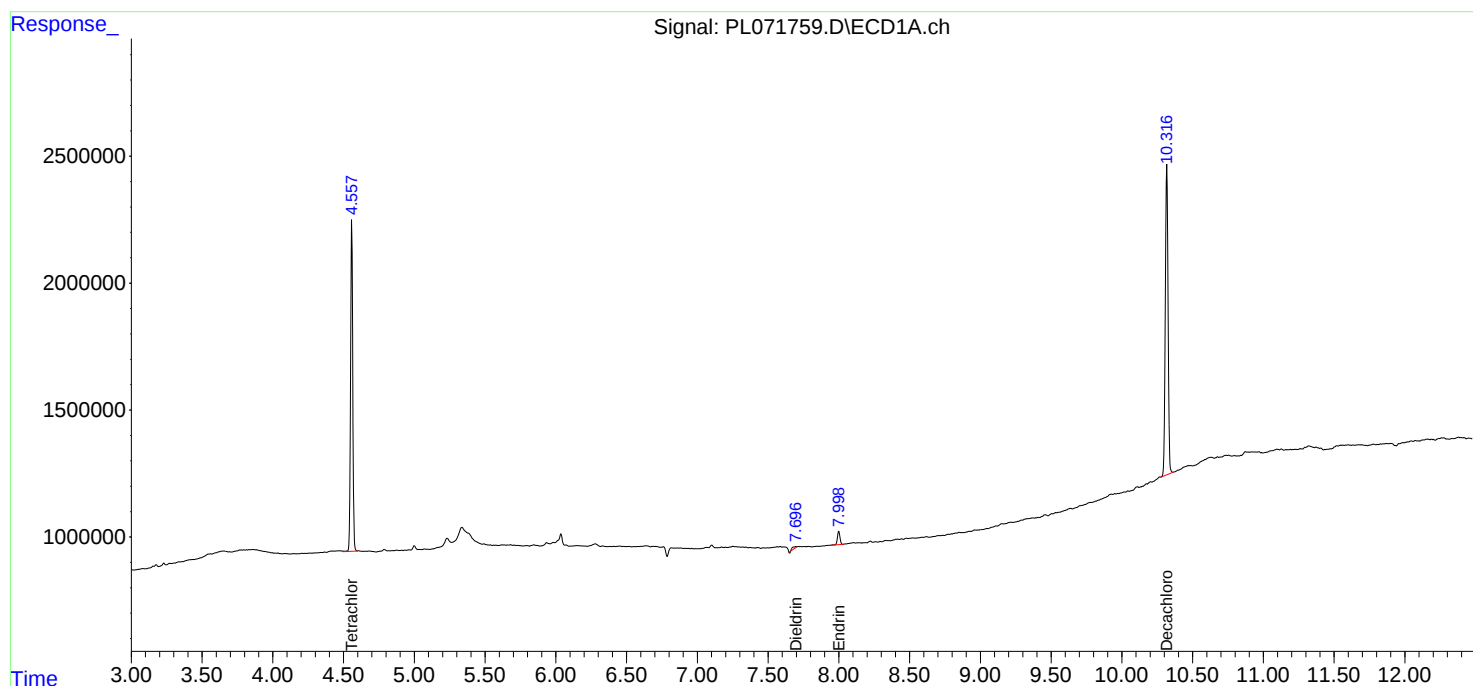


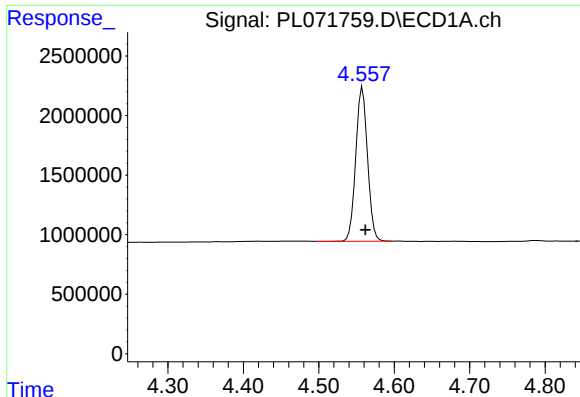

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: -0.004 min
Response: 14084595
Conc: 21.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

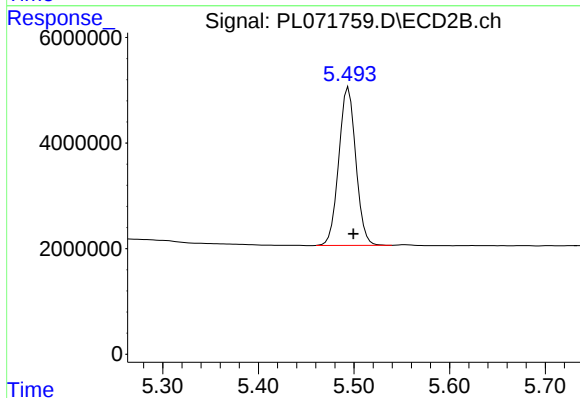


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: -0.005 min
Response: 37138044
Conc: 21.76 ng/ml

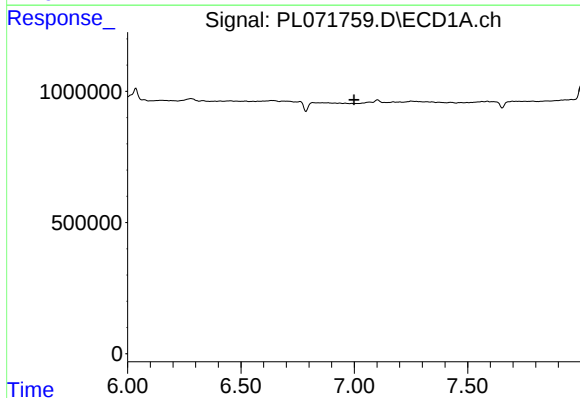


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

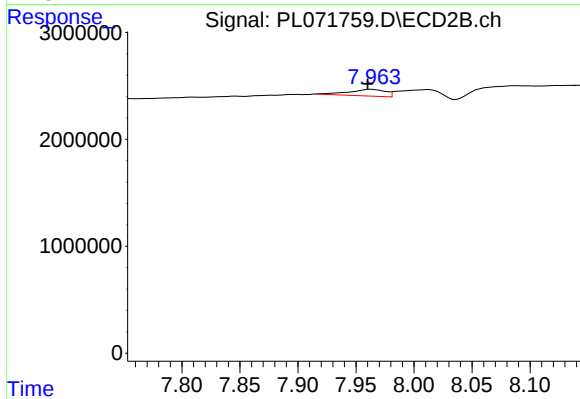

#8 Heptachlor epoxide


R.T.: 7.963 min
Delta R.T.: 0.003 min
Response: 1390548
Conc: 0.71 ng/ml

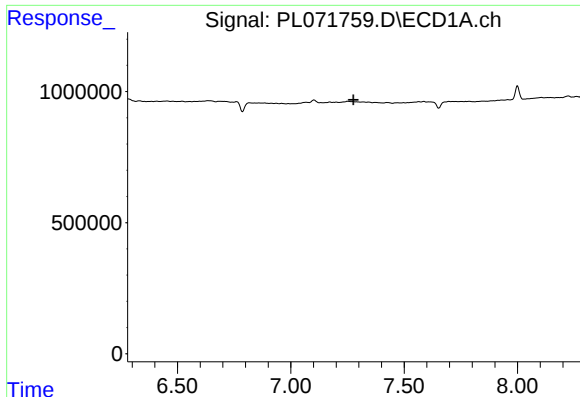

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

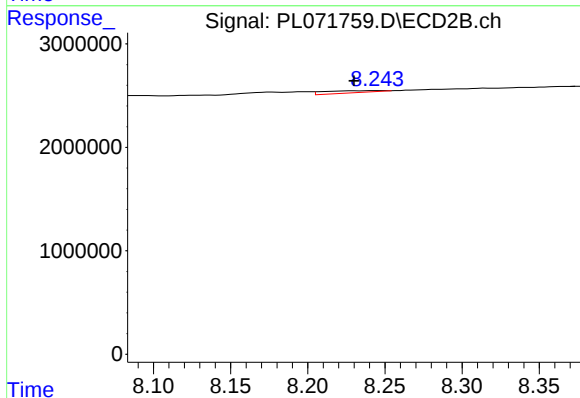


#10 gamma-Chlordane

R.T.: 8.245 min
Delta R.T.: 0.015 min
Response: 503234
Conc: 0.26 ng/ml

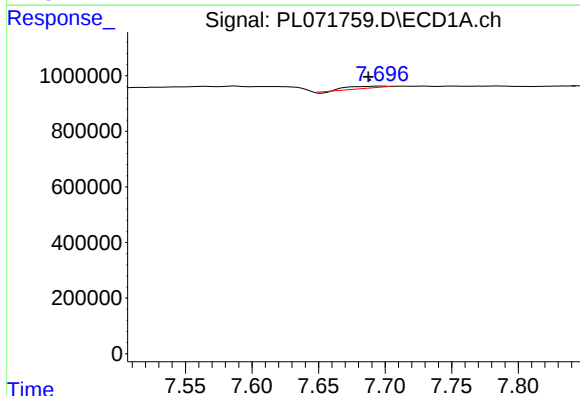


#13 Dieldrin

R.T.: 7.697 min
Delta R.T.: 0.010 min
Response: 120285
Conc: 0.15 ng/ml

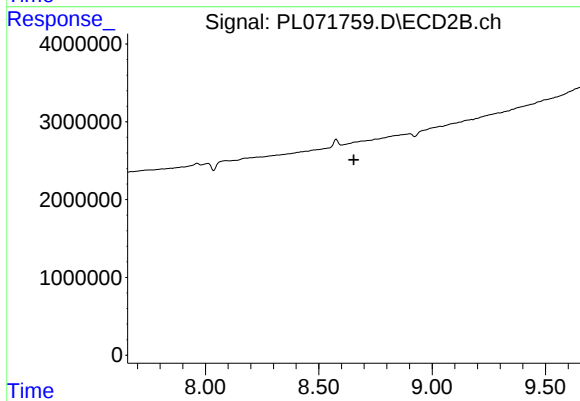

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.654 min
Response: 0
Conc: N.D.

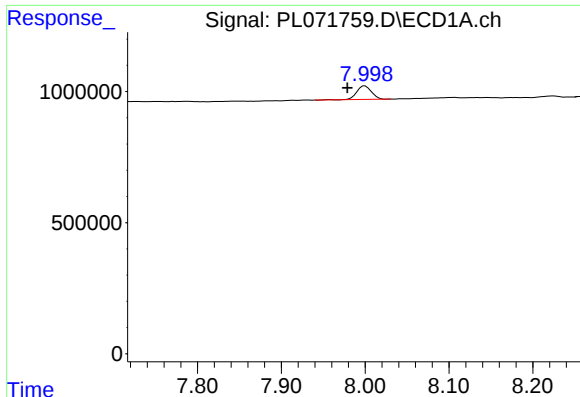

#14 Endrin


R.T.: 8.000 min
Delta R.T.: 0.021 min
Response: 641317
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

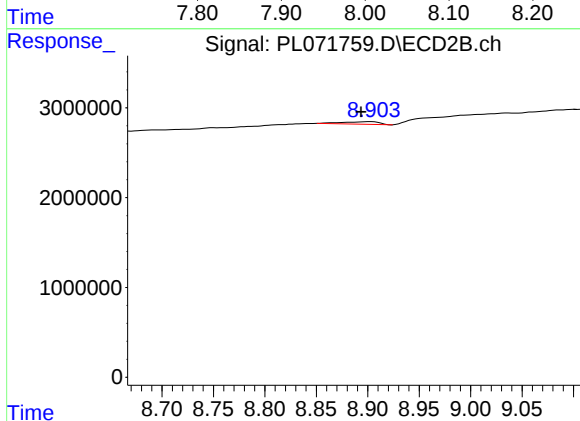


#14 Endrin

R.T.: 8.903 min
Delta R.T.: 0.010 min
Response: 688844
Conc: 0.46 ng/ml

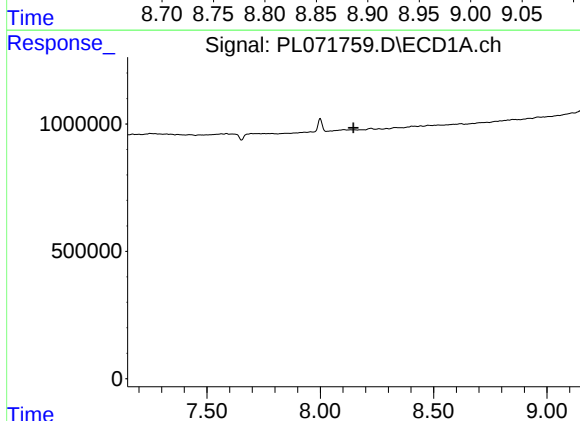


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.147 min
Response: 0
Conc: N.D.

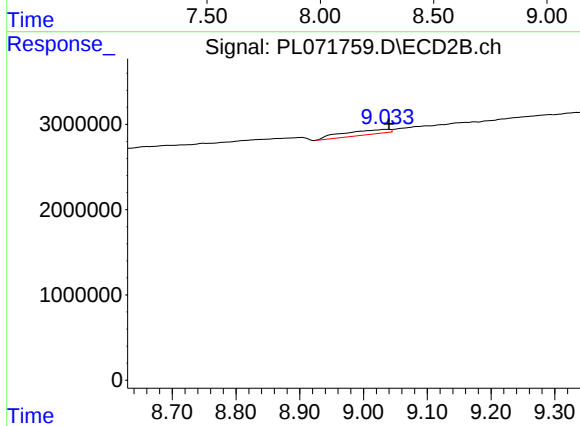

#16 4,4'-DDD


R.T.: 9.036 min
Delta R.T.: -0.004 min
Response: 2882886
Conc: 2.22 ng/ml

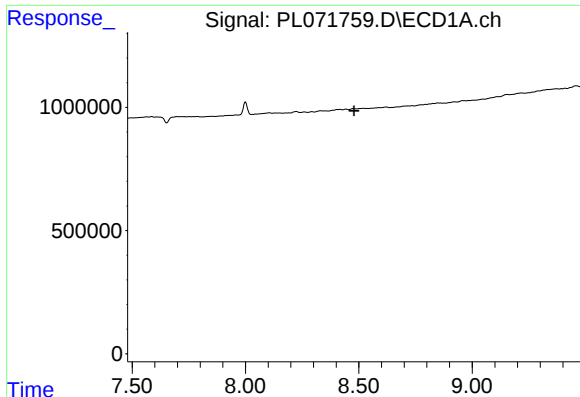

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

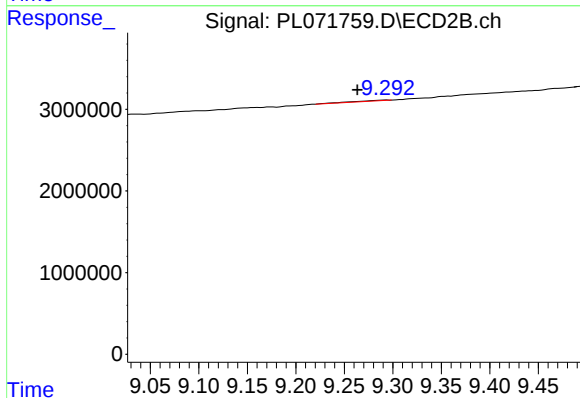


#18 Endrin aldehyde

R.T.: 9.293 min
Delta R.T.: 0.030 min
Response: 197124
Conc: 0.17 ng/ml

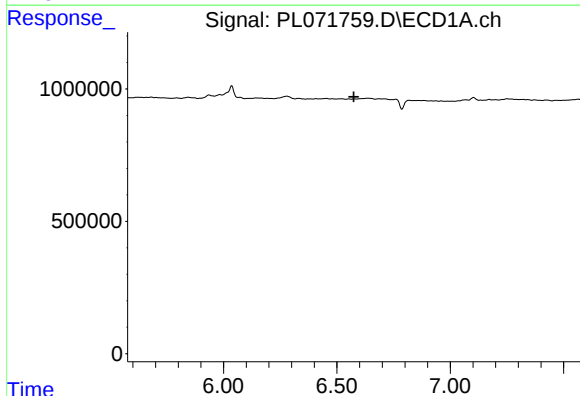


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.575 min
Response: 0
Conc: N.D.

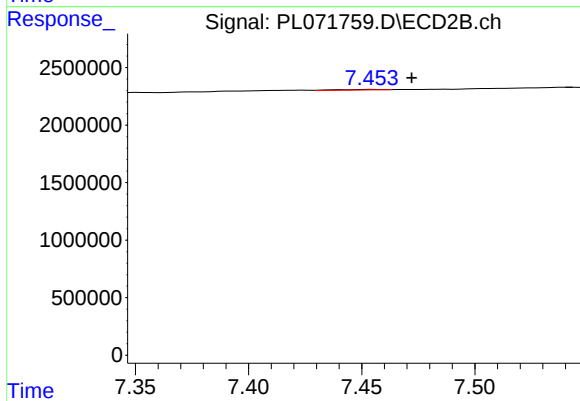

#24 Chlordane-2


R.T.: 7.455 min
Delta R.T.: -0.017 min
Response: 74541
Conc: 1.01 ng/ml

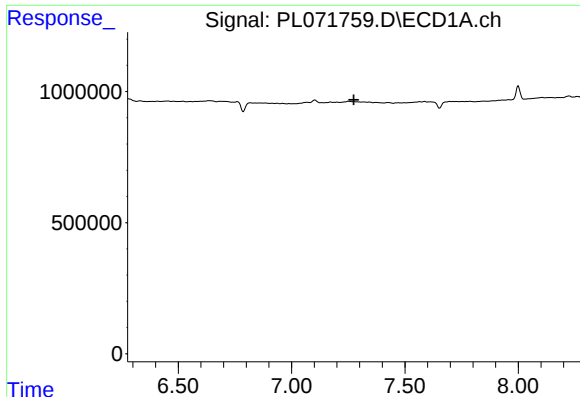

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

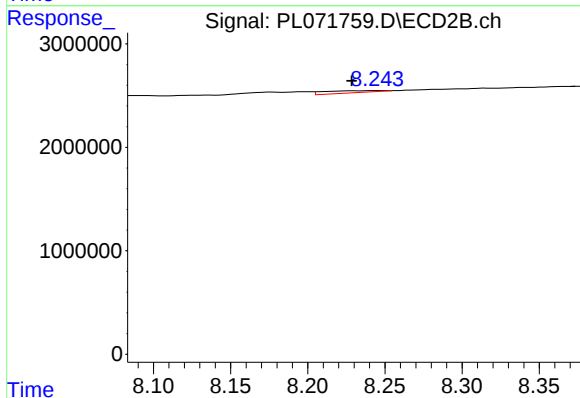


#25 Chlordane-3

R.T.: 8.245 min
Delta R.T.: 0.016 min
Response: 503234
Conc: 1.82 ng/ml

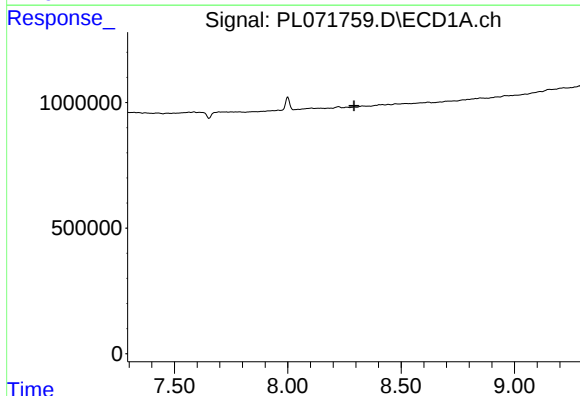


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.292 min
Response: 0
Conc: N.D.

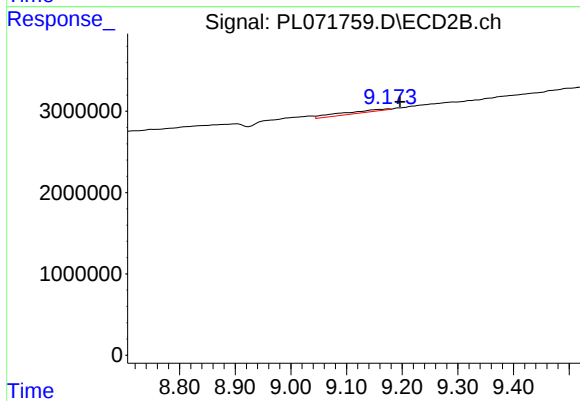

#27 Chlordane-5

R.T.: 9.175 min
Delta R.T.: -0.021 min
Response: 1709275
Conc: 31.51 ng/ml

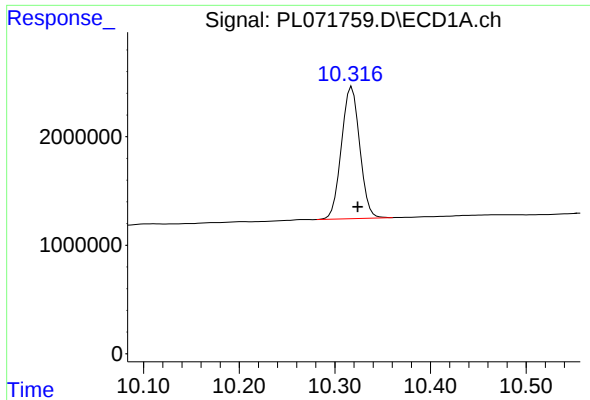

#28 Decachlorobiphenyl


R.T.: 10.318 min

Delta R.T.: -0.006 min

Response: 16186751

Conc: 21.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

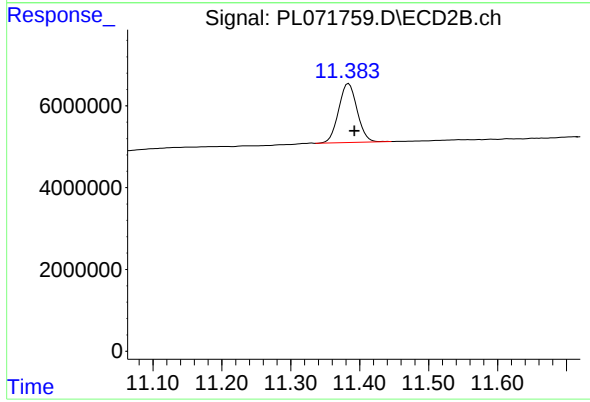

#28 Decachlorobiphenyl

R.T.: 11.384 min

Delta R.T.: -0.008 min

Response: 26907445

Conc: 21.47 ng/ml