

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
 Data File : PL079966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 16:02
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 17:25:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 17:24:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.363	2.695	136.6E6	214.0E6	100.418	100.633
28) SA Decachlor...	8.803	7.858	120.7E6	169.9E6	85.188	96.045
Target Compounds						
23) Chlordane-1	4.511	3.696	52821485	63041539	952.503	993.355
24) Chlordane-2	5.037	4.274	61537031	66496018	892.897	946.214
25) Chlordane-3	5.742	4.906	240.6E6	213.2E6	936.998	1009.826
26) Chlordane-4	5.824	4.969	291.7E6	208.7E6	919.256	1010.812
27) Chlordane-5	6.667	5.638	48959762	54080181	892.912	976.345



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
Data File : PL079966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 16:02
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 17:25:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 17:24:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

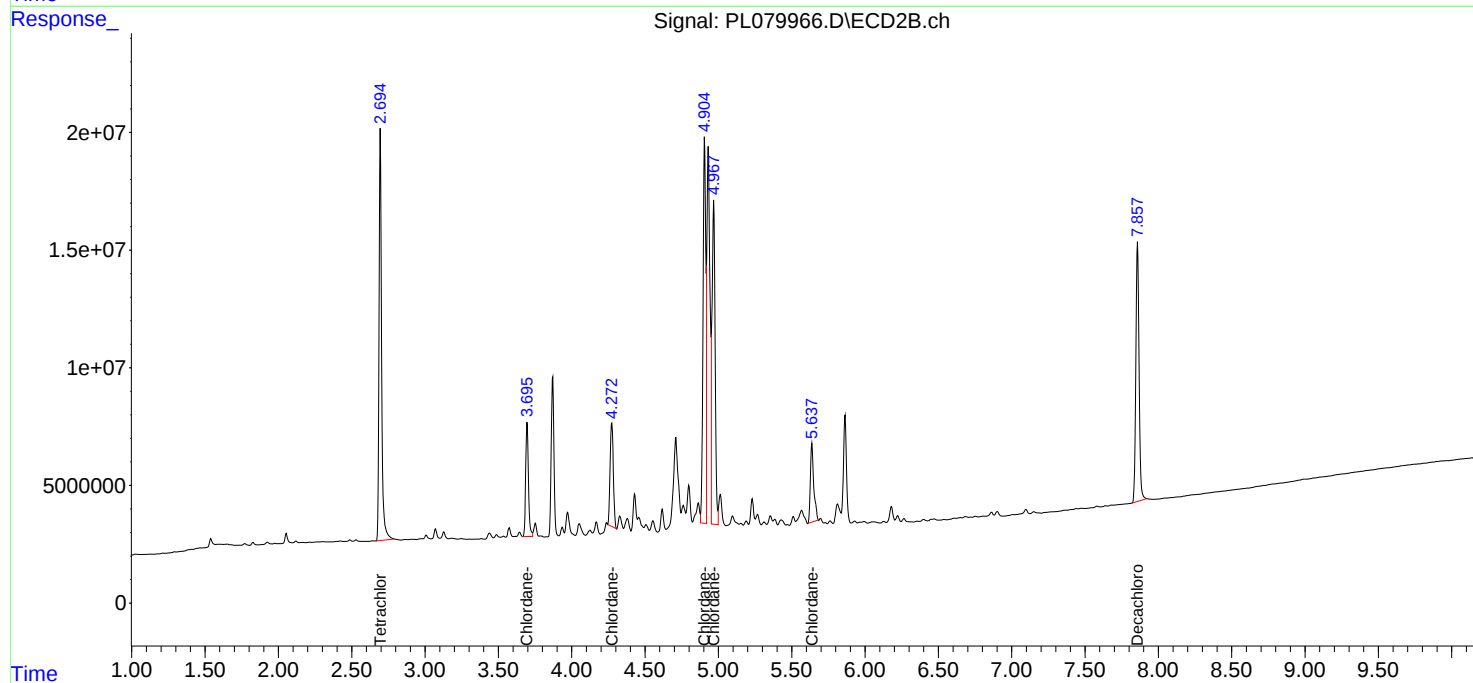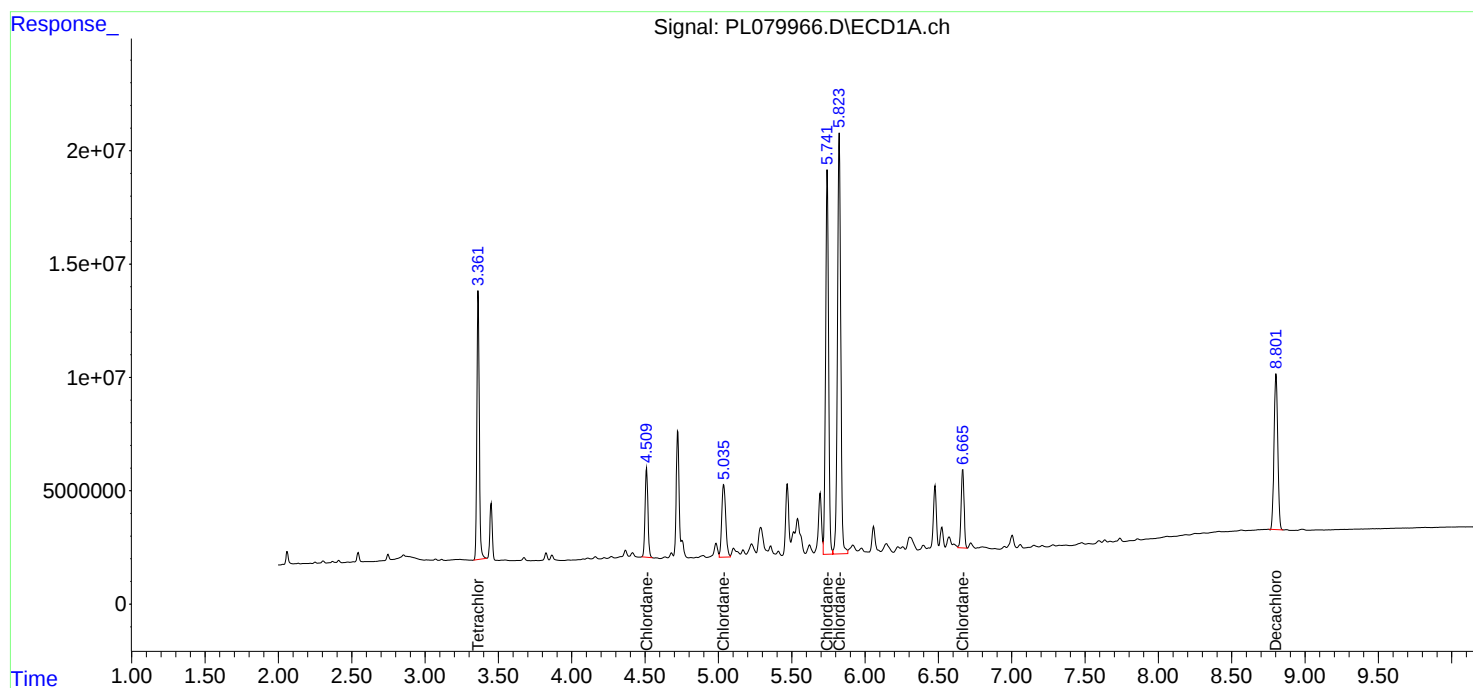


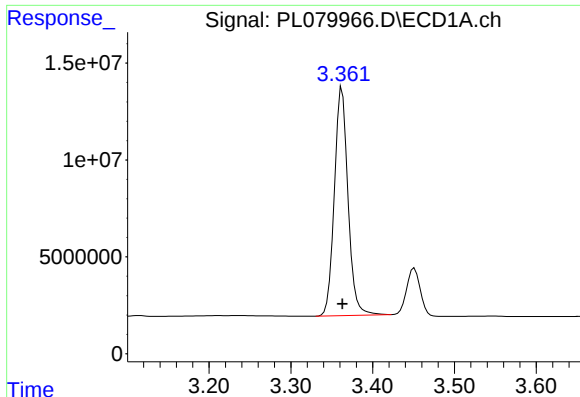

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 136613516
Conc: 100.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

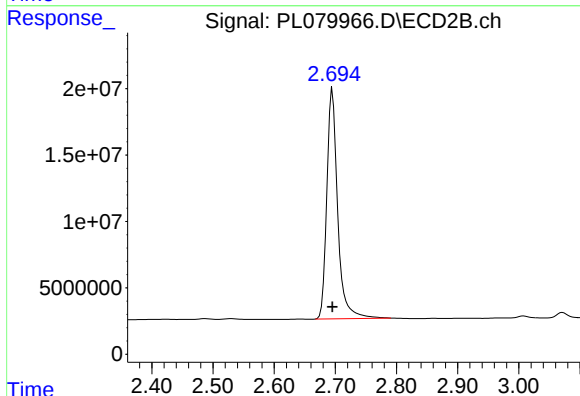


#1 Tetrachloro-m-xylene

R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 214001420
Conc: 100.63 ng/ml

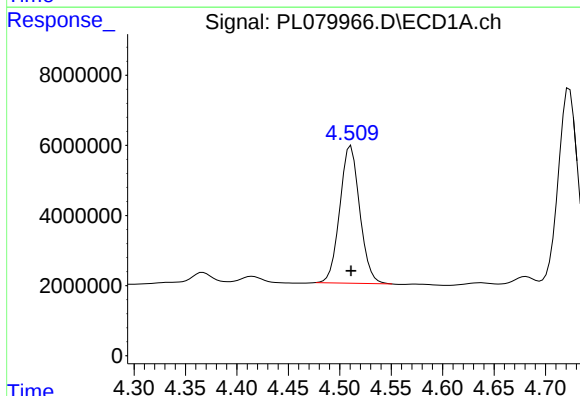


#23 Chlordane-1

R.T.: 4.511 min
Delta R.T.: 0.000 min
Response: 52821485
Conc: 952.50 ng/ml

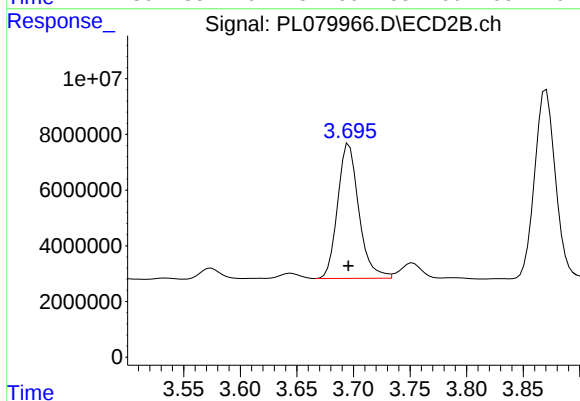

#23 Chlordane-1


R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 63041539
Conc: 993.35 ng/ml

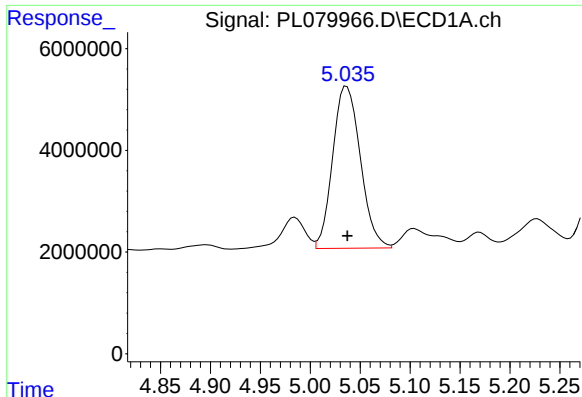

#24 Chlordane-2


R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 61537031
Conc: 892.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

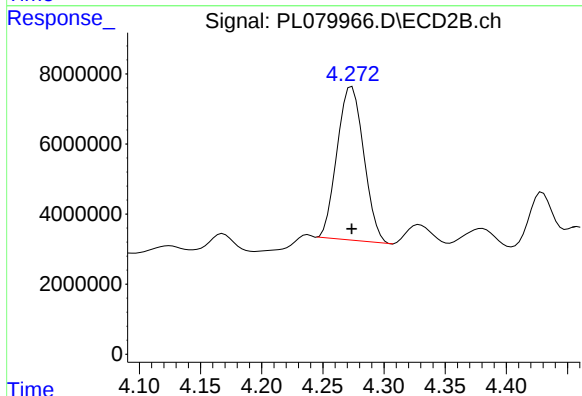


#24 Chlordane-2

R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 66496018
Conc: 946.21 ng/ml

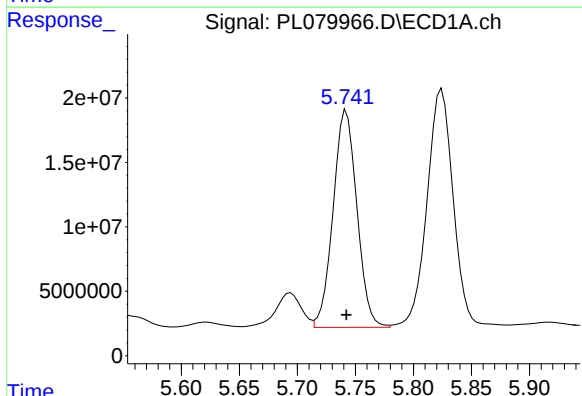


#25 Chlordane-3

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 240554556
Conc: 937.00 ng/ml

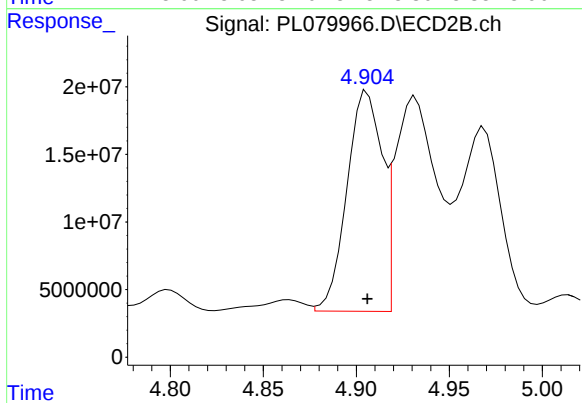

#25 Chlordane-3


R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 213193059
Conc: 1009.83 ng/ml

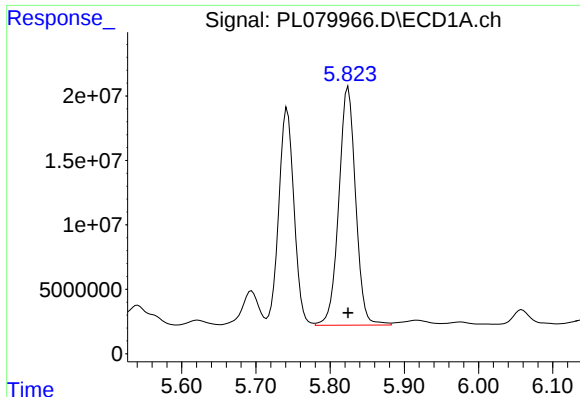

#26 Chlordane-4


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 291716243
Conc: 919.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

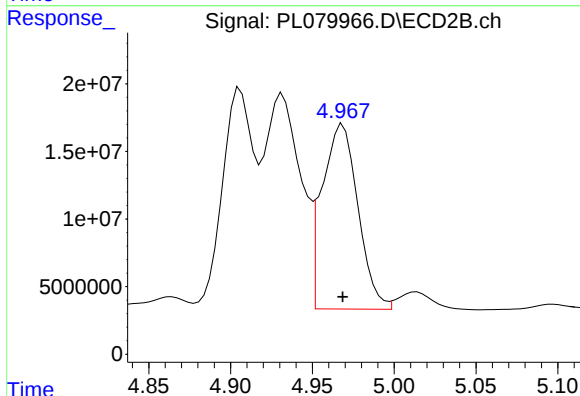


#26 Chlordane-4

R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 208711270
Conc: 1010.81 ng/ml

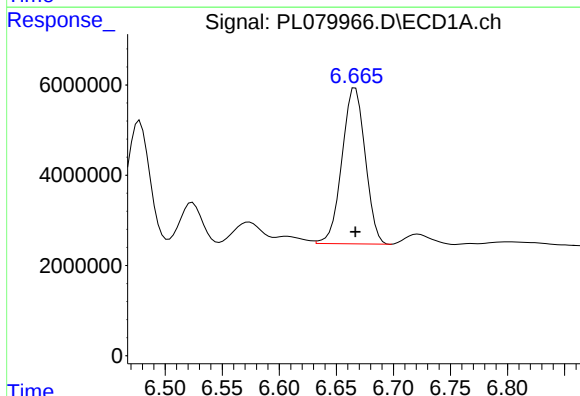


#27 Chlordane-5

R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 48959762
Conc: 892.91 ng/ml

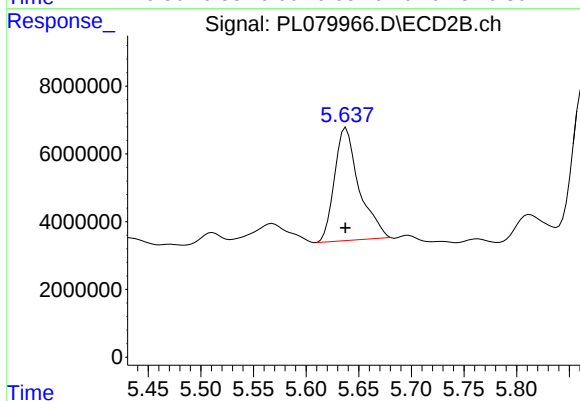

#27 Chlordane-5


R.T.: 5.638 min
Delta R.T.: 0.000 min
Response: 54080181
Conc: 976.35 ng/ml

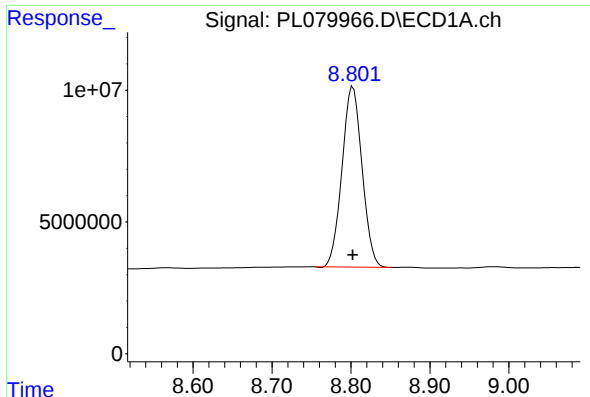

#28 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 120725404
Conc: 85.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

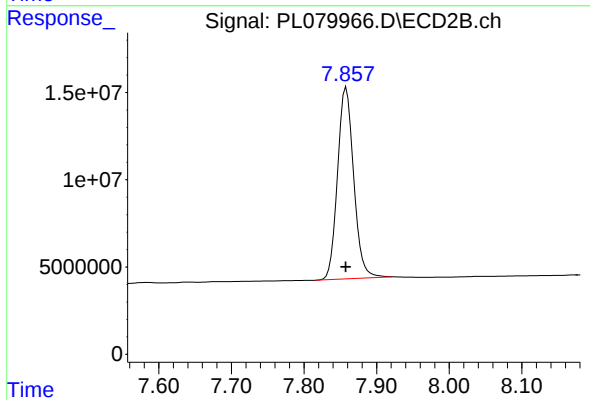

#28 Decachlorobiphenyl

R.T.: 7.858 min
Delta R.T.: 0.000 min
Response: 169880773
Conc: 96.04 ng/ml