

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
 Data File : PL079967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 16:16
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 17:25:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 17:24:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	2.695	100.8E6	158.7E6	74.077	74.650
28)	SA Decachlor...	8.803	7.858	95887992	127.8E6	67.662	72.247
Target Compounds							
23)	Chlordane-1	4.512	3.696	41696440	46826531	751.891	737.852
24)	Chlordane-2	5.038	4.274	49563519	50578515	719.162	719.714
25)	Chlordane-3	5.743	4.907	193.5E6	155.7E6	753.819	737.640
26)	Chlordane-4	5.826	4.969	237.8E6	154.1E6	749.258	746.288
27)	Chlordane-5	6.668	5.639	40166156	40362185	732.537	728.685



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
Data File : PL079967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 16:16
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 17:25:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 17:24:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

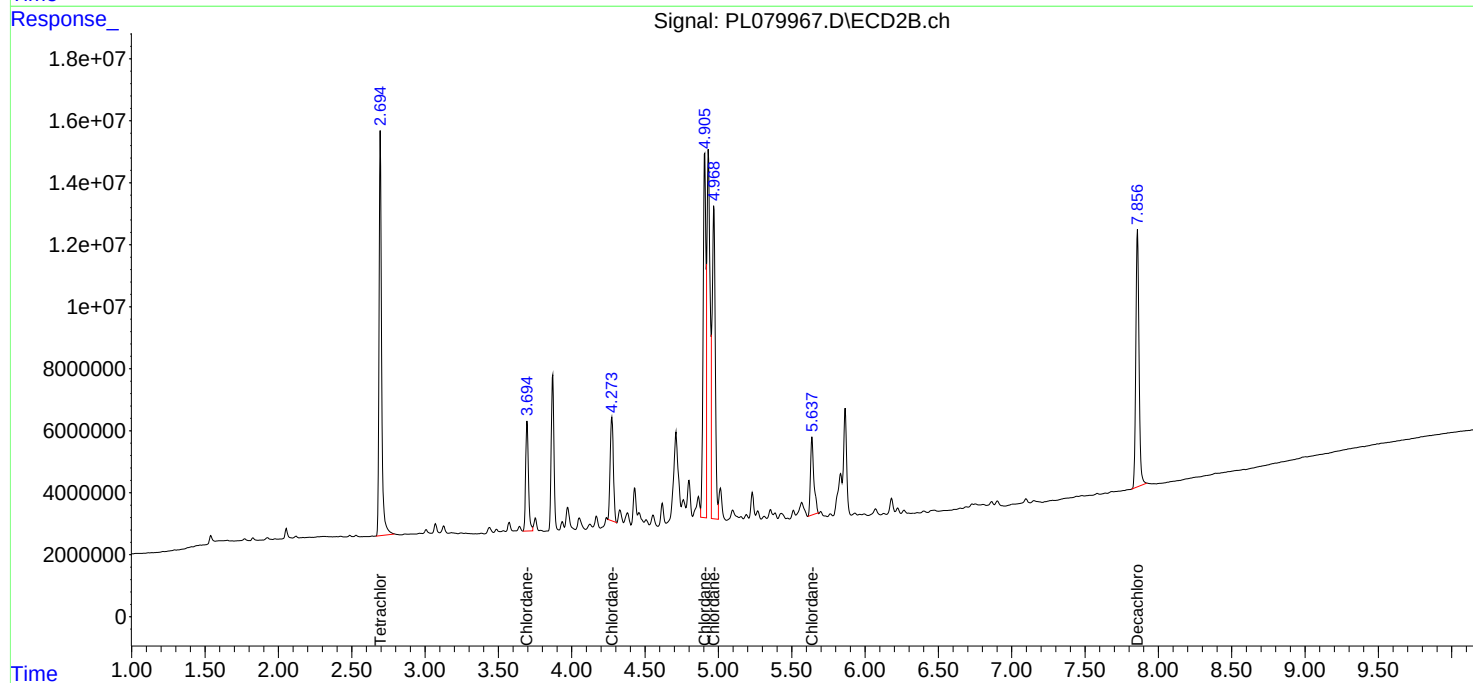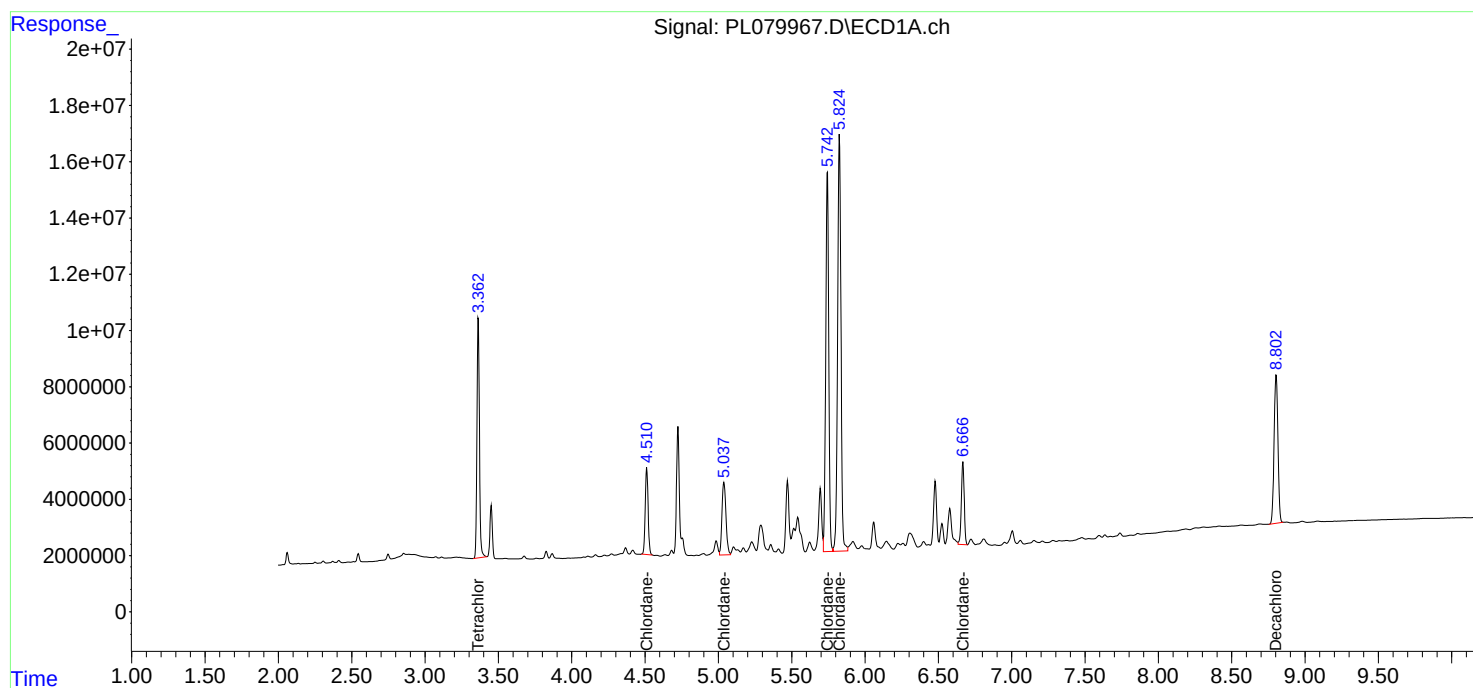


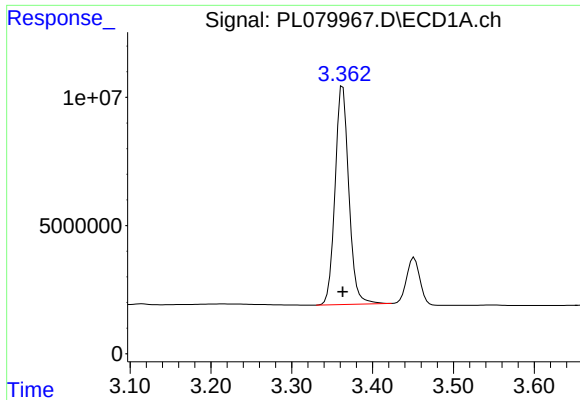

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 100779055
Conc: 74.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

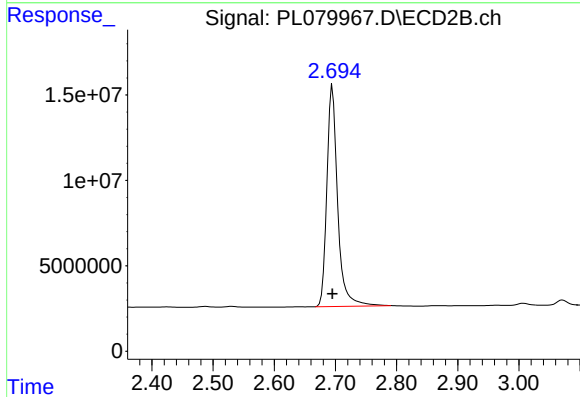


#1 Tetrachloro-m-xylene

R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 158745695
Conc: 74.65 ng/ml

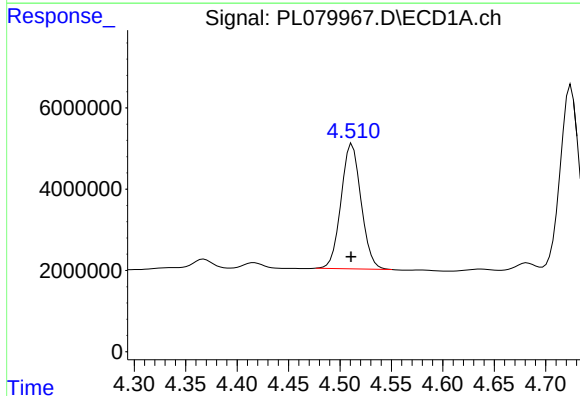


#23 Chlordane-1

R.T.: 4.512 min
Delta R.T.: 0.001 min
Response: 41696440
Conc: 751.89 ng/ml

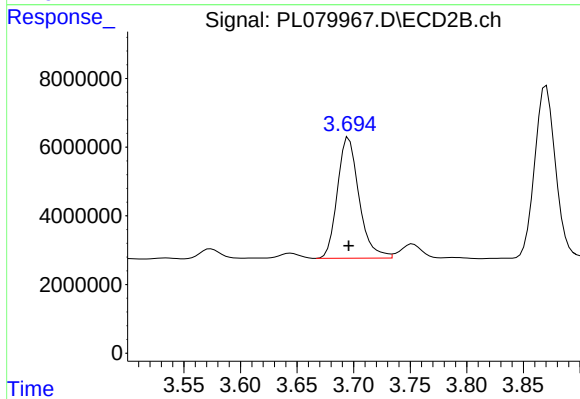

#23 Chlordane-1


R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 46826531
Conc: 737.85 ng/ml

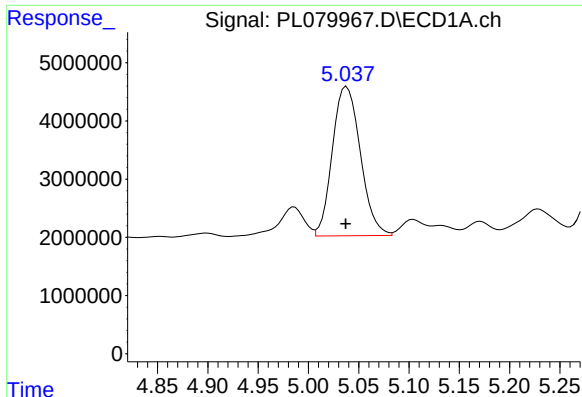

#24 Chlordane-2


R.T.: 5.038 min
Delta R.T.: 0.001 min
Response: 49563519
Conc: 719.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

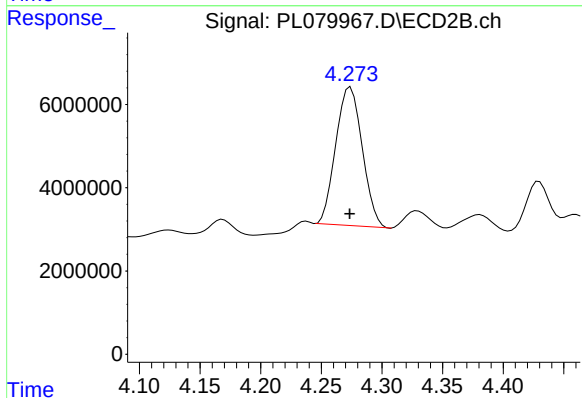


#24 Chlordane-2

R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 50578515
Conc: 719.71 ng/ml

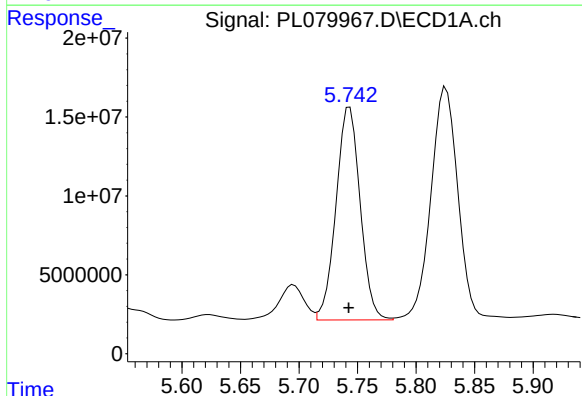


#25 Chlordane-3

R.T.: 5.743 min
Delta R.T.: 0.000 min
Response: 193527111
Conc: 753.82 ng/ml

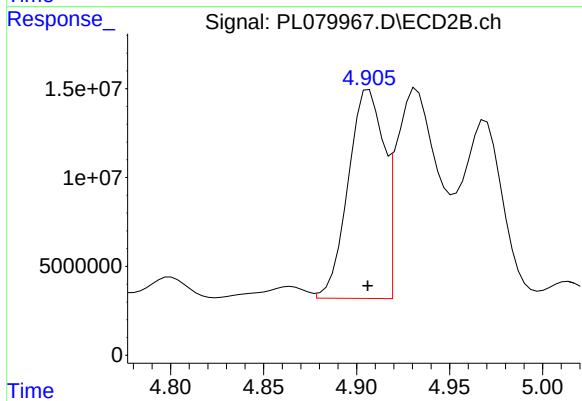

#25 Chlordane-3


R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 155729407
Conc: 737.64 ng/ml

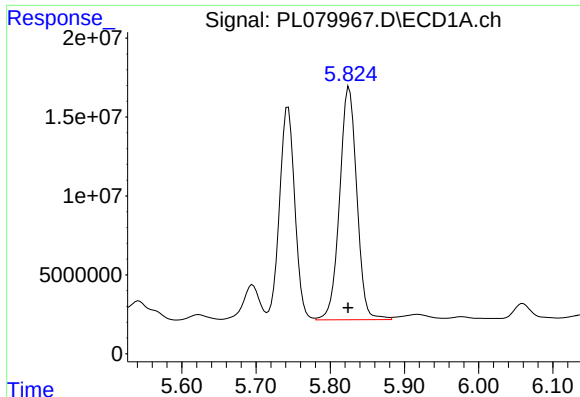

#26 Chlordane-4


R.T.: 5.826 min
Delta R.T.: 0.001 min
Response: 237769196
Conc: 749.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

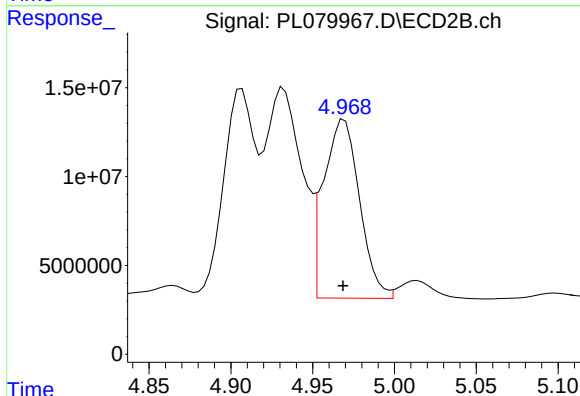


#26 Chlordane-4

R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 154092558
Conc: 746.29 ng/ml

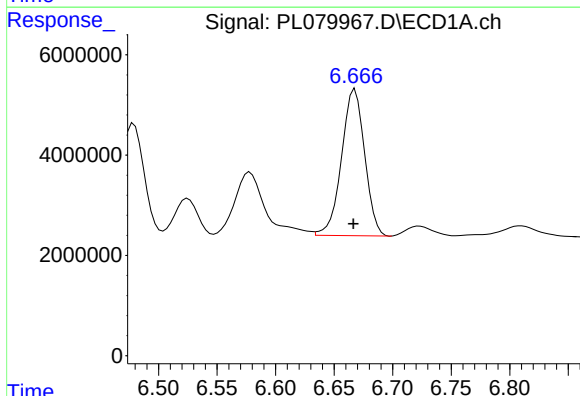


#27 Chlordane-5

R.T.: 6.668 min
Delta R.T.: 0.001 min
Response: 40166156
Conc: 732.54 ng/ml

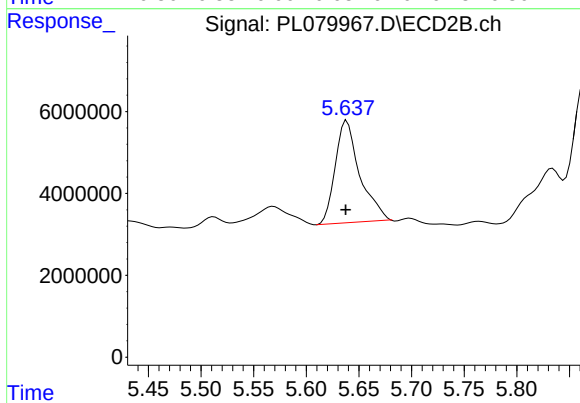

#27 Chlordane-5


R.T.: 5.639 min
Delta R.T.: 0.001 min
Response: 40362185
Conc: 728.69 ng/ml

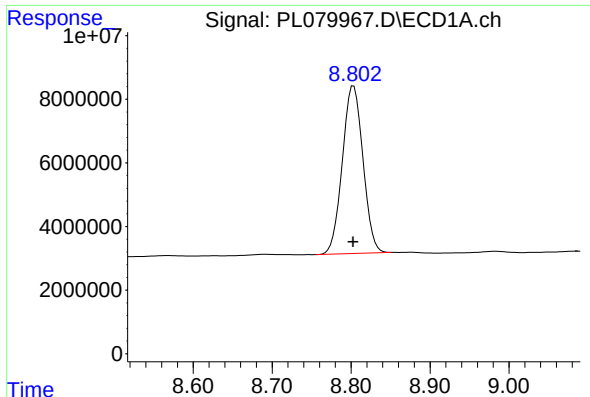

#28 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 95887992
Conc: 67.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

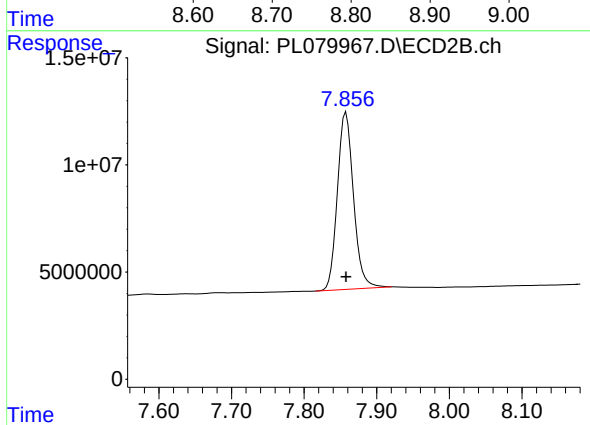

#28 Decachlorobiphenyl

R.T.: 7.858 min
Delta R.T.: 0.000 min
Response: 127788913
Conc: 72.25 ng/ml