

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
 Data File : PL079968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 16:30
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 17:25:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 17:24:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	2.695	68022728	106.3E6	50.000	50.000
28)	SA Decachlor...	8.802	7.858	70858210	88438350	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.511	3.696	27727720	31731641	500.000	500.000
24)	Chlordane-2	5.037	4.274	34459200	35137948	500.000	500.000
25)	Chlordane-3	5.742	4.906	128.4E6	105.6E6	500.000	500.000
26)	Chlordane-4	5.824	4.969	158.7E6	103.2E6	500.000	500.000
27)	Chlordane-5	6.667	5.638	27415795	27695217	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
Data File : PL079968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 16:30
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 17:25:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 17:24:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

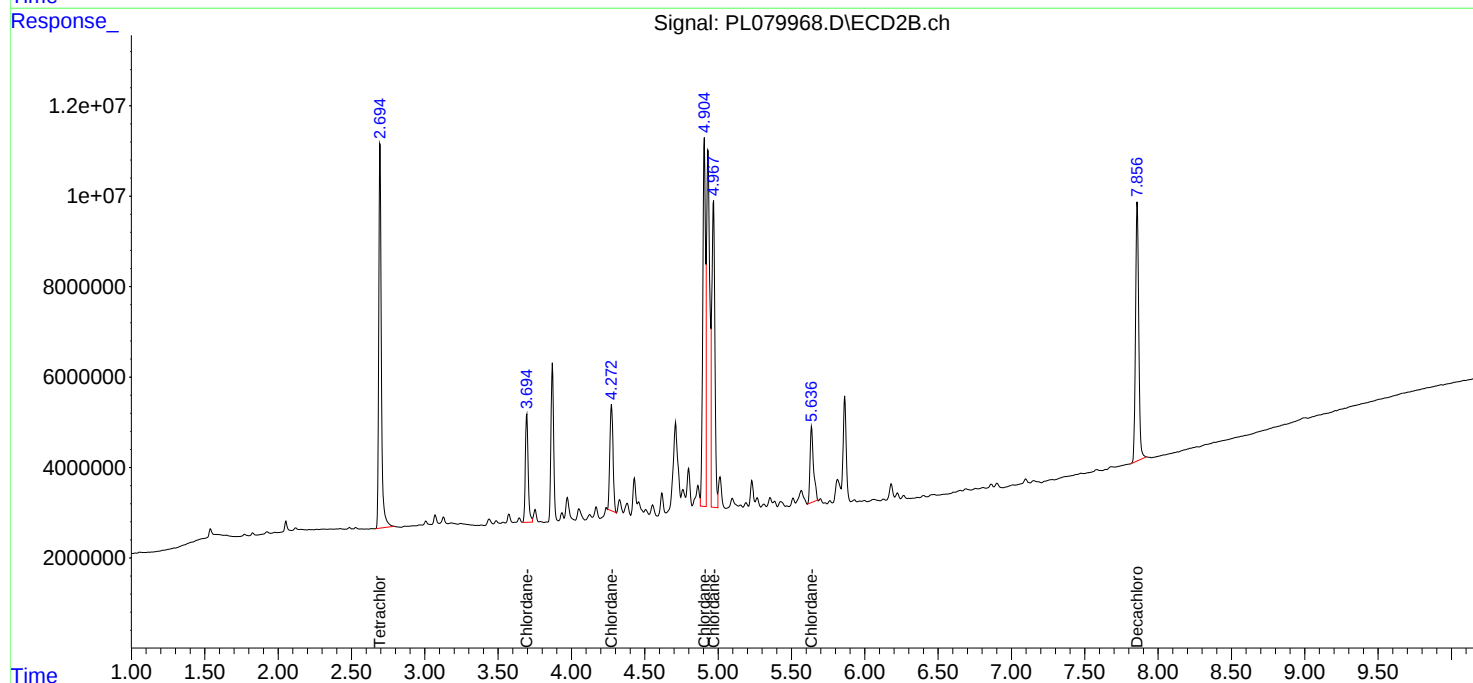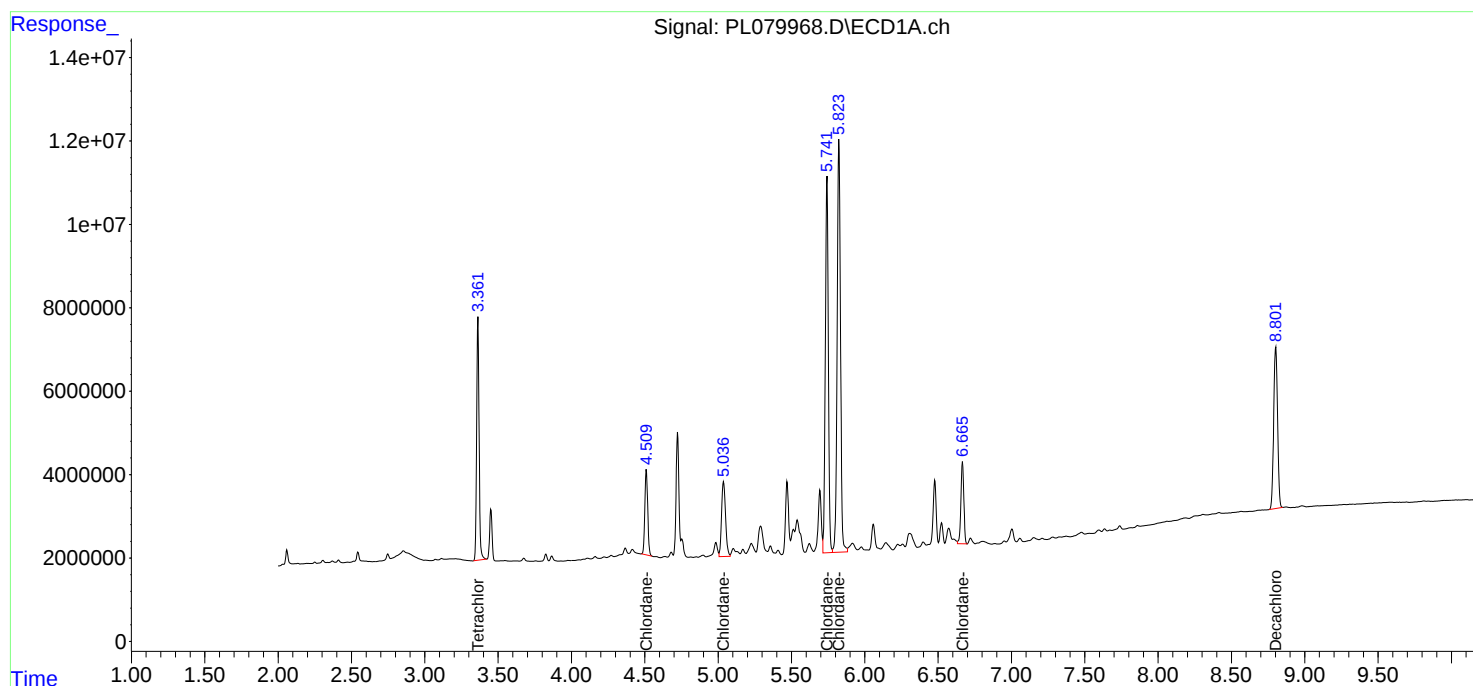


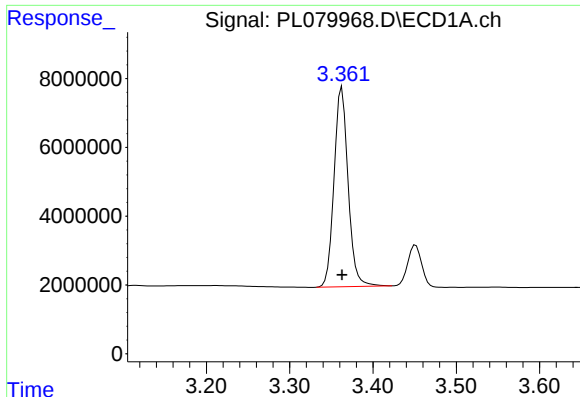

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 68022728
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

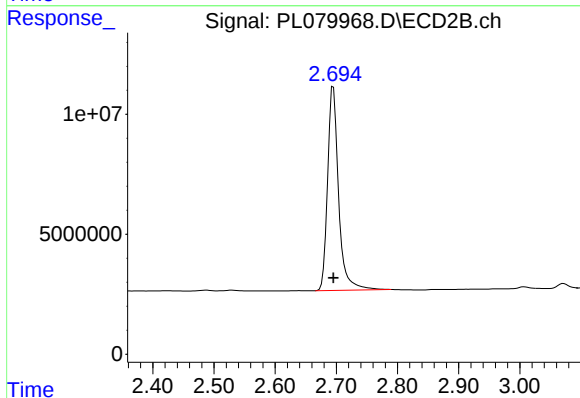


#1 Tetrachloro-m-xylene

R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 106327191
Conc: 50.00 ng/ml

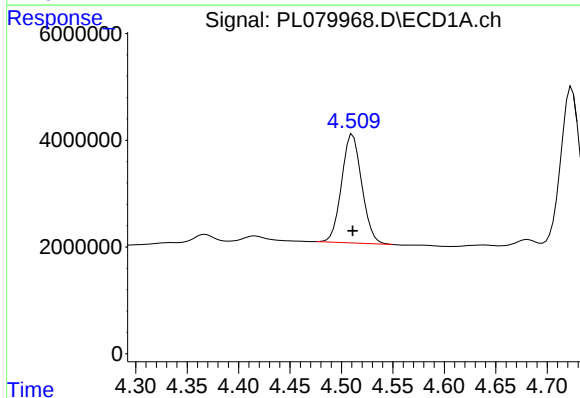


#23 Chlordane-1

R.T.: 4.511 min
Delta R.T.: 0.000 min
Response: 27727720
Conc: 500.00 ng/ml

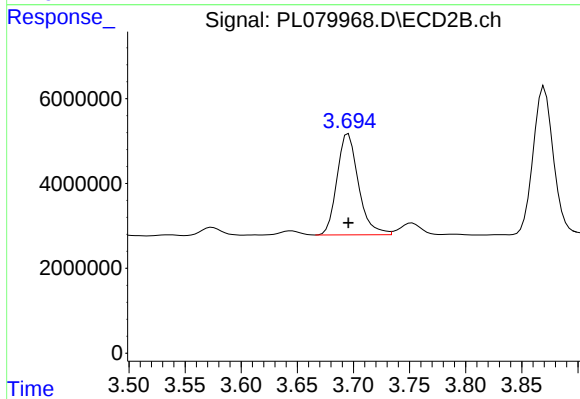

#23 Chlordane-1


R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 31731641
Conc: 500.00 ng/ml

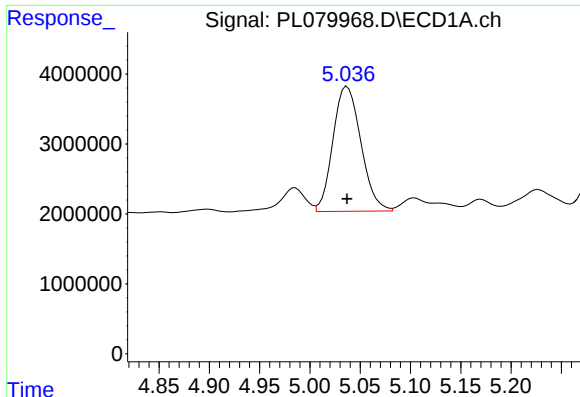

#24 Chlordane-2


R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 34459200
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

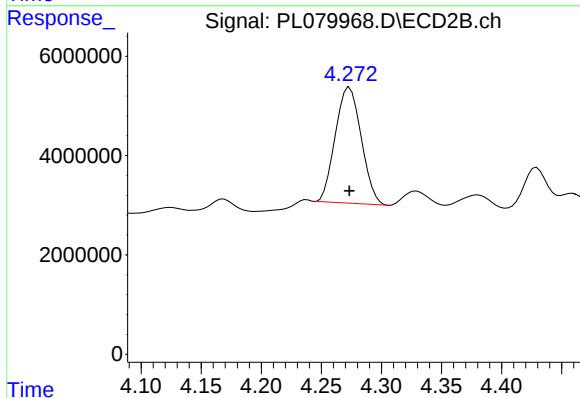


#24 Chlordane-2

R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 35137948
Conc: 500.00 ng/ml

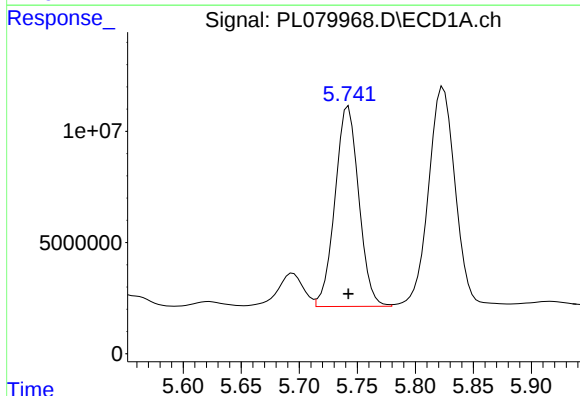


#25 Chlordane-3

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 128364520
Conc: 500.00 ng/ml

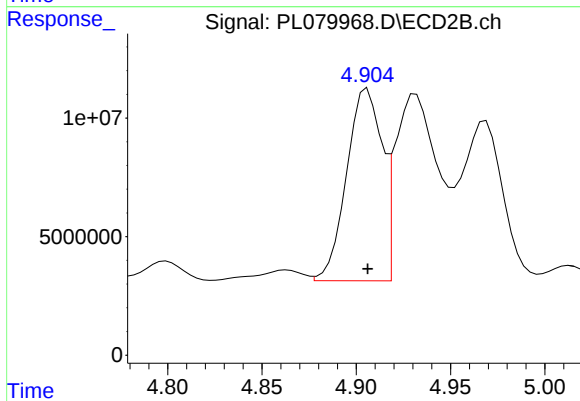

#25 Chlordane-3


R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 105559256
Conc: 500.00 ng/ml

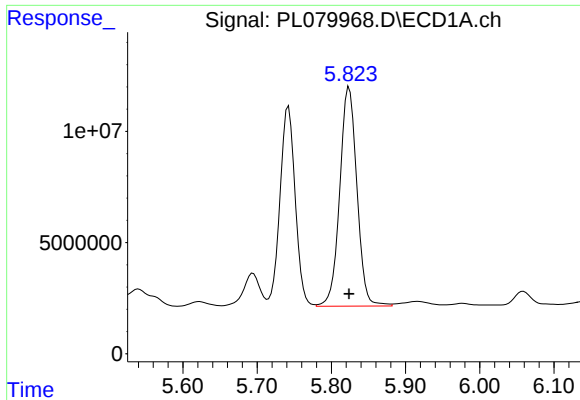

#26 Chlordane-4


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 158669811
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

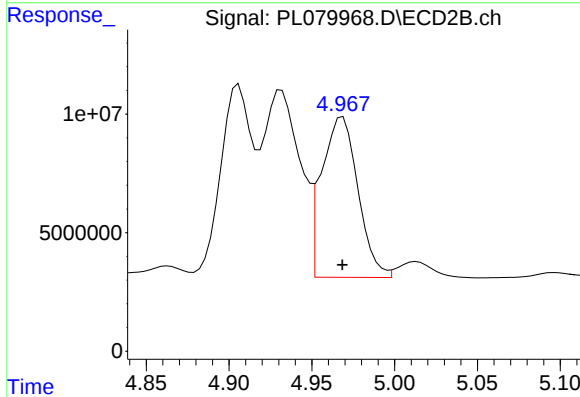


#26 Chlordane-4

R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 103239361
Conc: 500.00 ng/ml

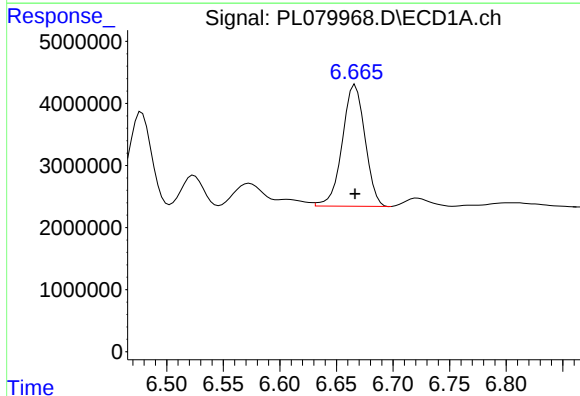


#27 Chlordane-5

R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 27415795
Conc: 500.00 ng/ml

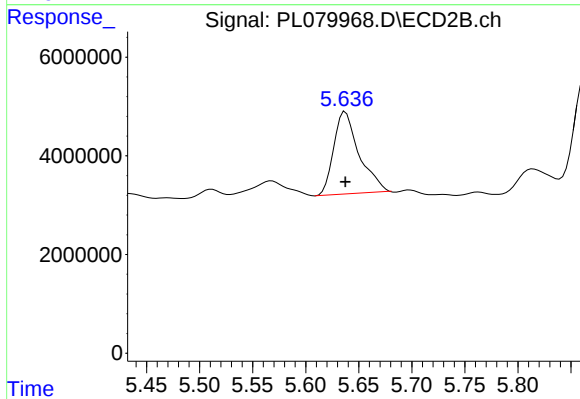

#27 Chlordane-5


R.T.: 5.638 min
Delta R.T.: 0.000 min
Response: 27695217
Conc: 500.00 ng/ml

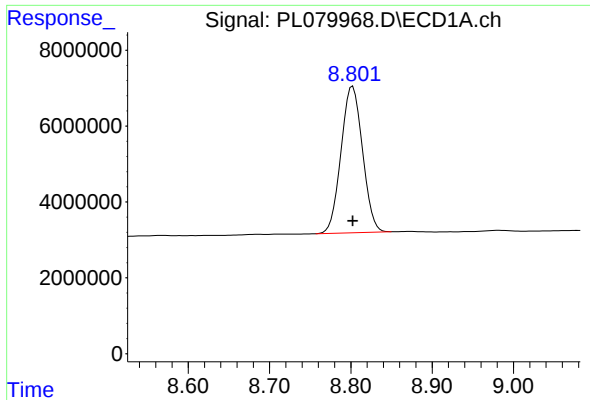

#28 Decachlorobiphenyl

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 70858210
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

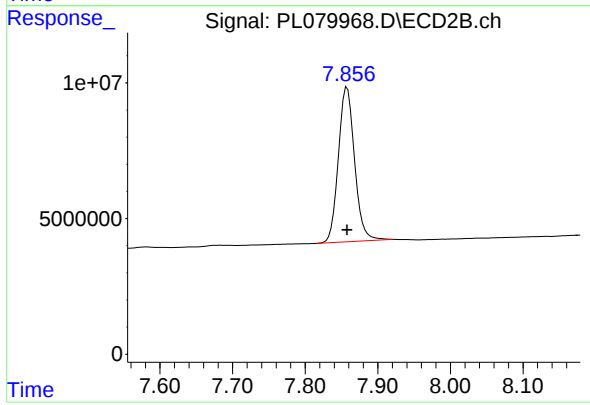

#28 Decachlorobiphenyl

R.T.: 7.858 min
Delta R.T.: 0.000 min
Response: 88438350
Conc: 50.00 ng/ml