

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
 Data File : PL079969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 16:44
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 17:25:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 17:24:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	2.695	33726561	51587399	24.791	24.259
28)	SA Decachlor...	8.803	7.858	35747118	43708249	25.224	24.711
Target Compounds							
23)	Chlordane-1	4.511	3.695	13338659	15726083	240.529	247.798
24)	Chlordane-2	5.037	4.274	17092663	17529615	248.013	249.440
25)	Chlordane-3	5.742	4.906	62111762	49192496	241.935	233.009
26)	Chlordane-4	5.825	4.968	76797959	48668027	242.006	235.705
27)	Chlordane-5	6.667	5.638	13125433	13906340	239.377	251.060



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
Data File : PL079969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 16:44
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 17:25:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 17:24:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

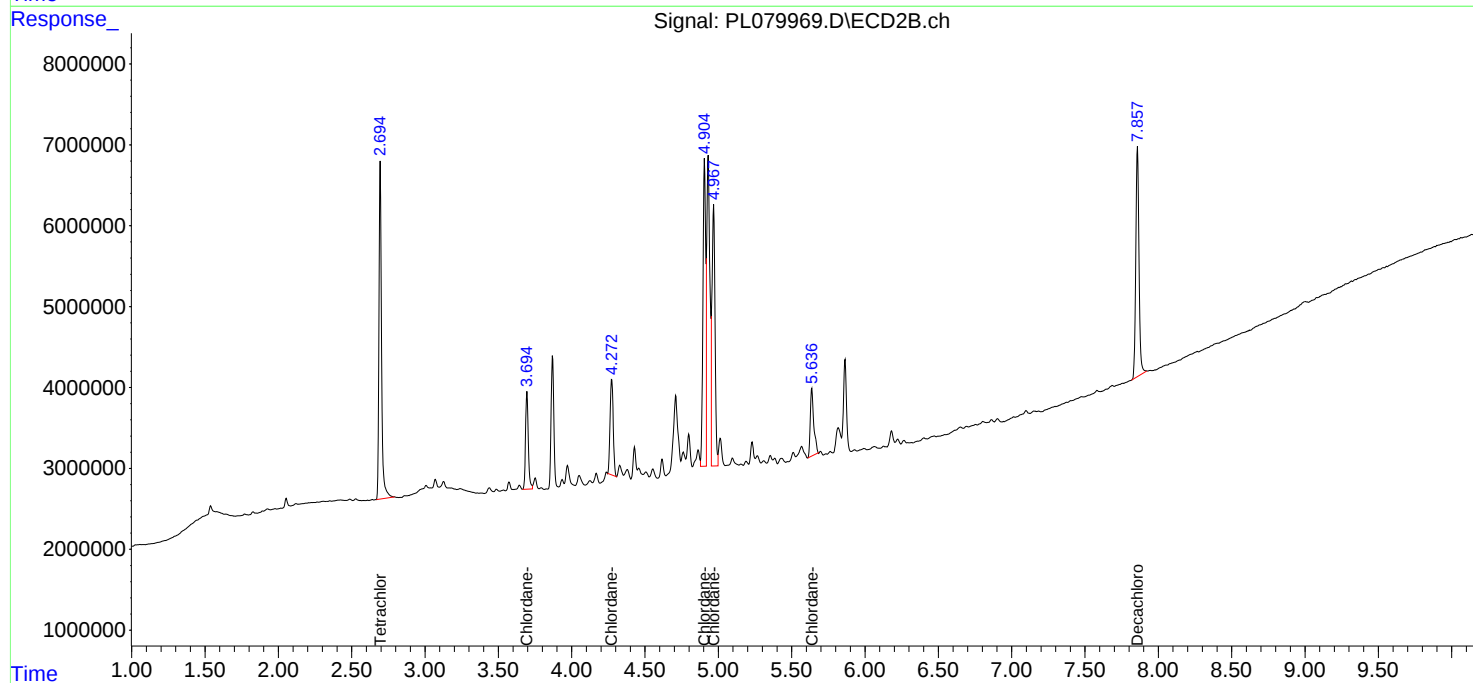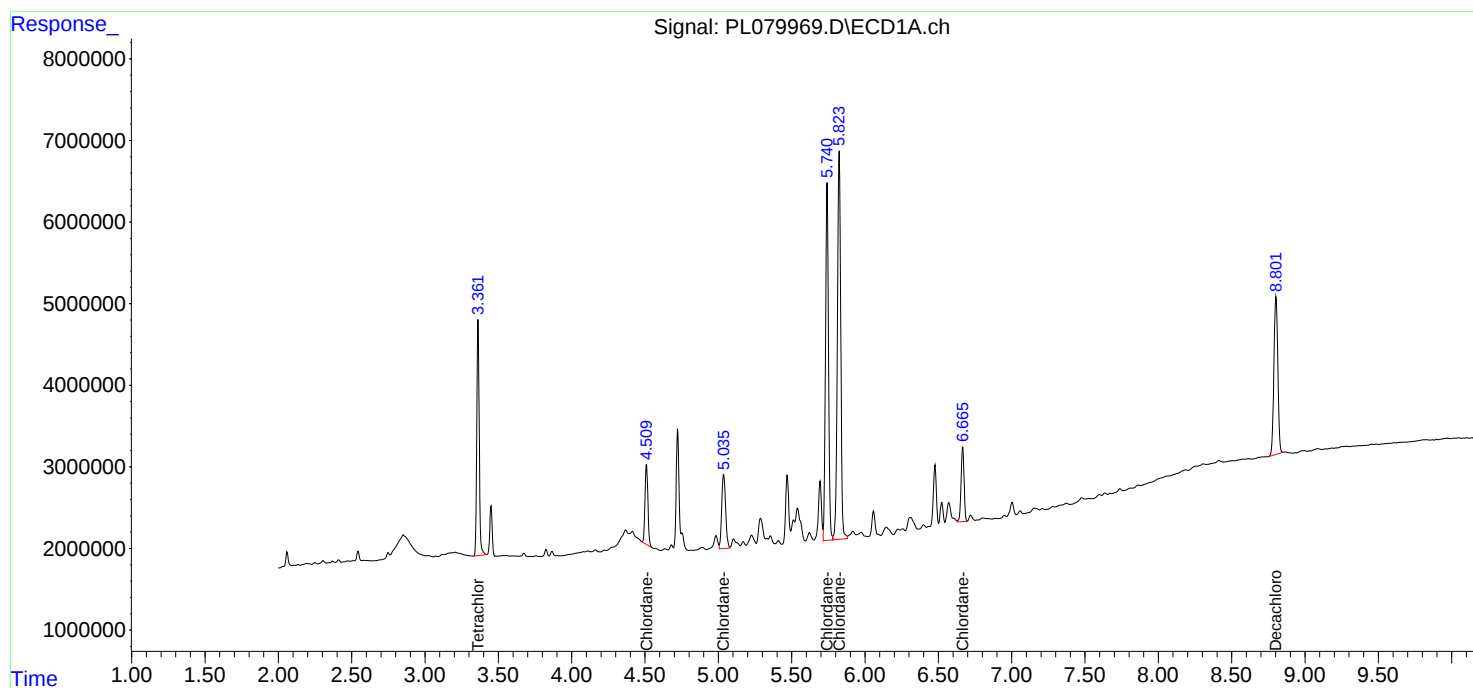


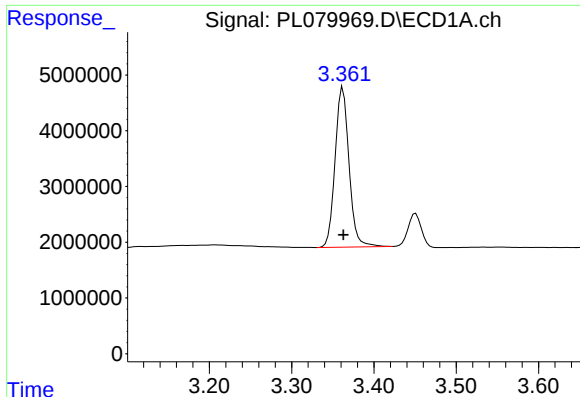

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 33726561
Conc: 24.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

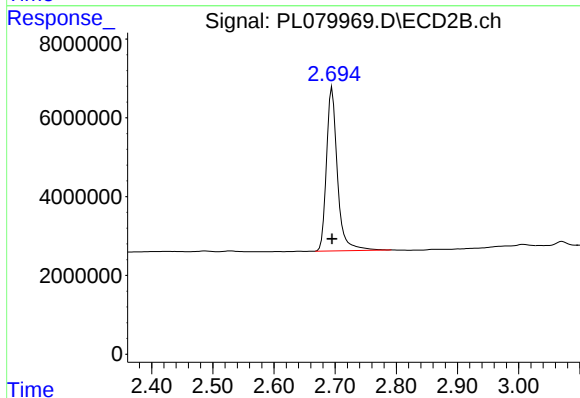


#1 Tetrachloro-m-xylene

R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 51587399
Conc: 24.26 ng/ml

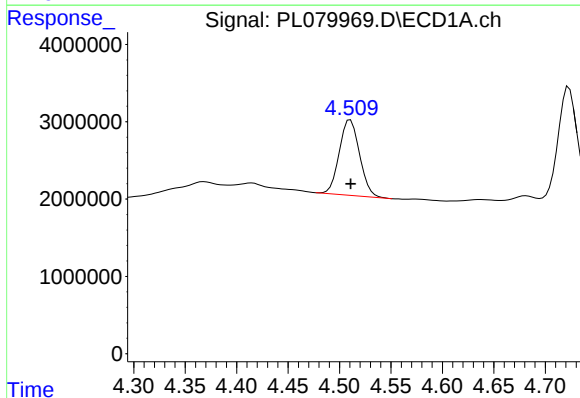


#23 Chlordane-1

R.T.: 4.511 min
Delta R.T.: 0.000 min
Response: 13338659
Conc: 240.53 ng/ml

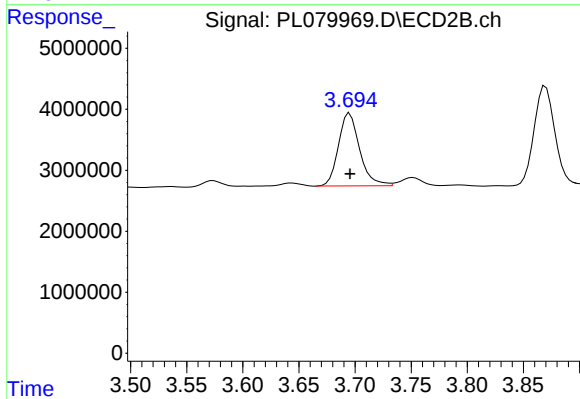

#23 Chlordane-1


R.T.: 3.695 min
Delta R.T.: 0.000 min
Response: 15726083
Conc: 247.80 ng/ml

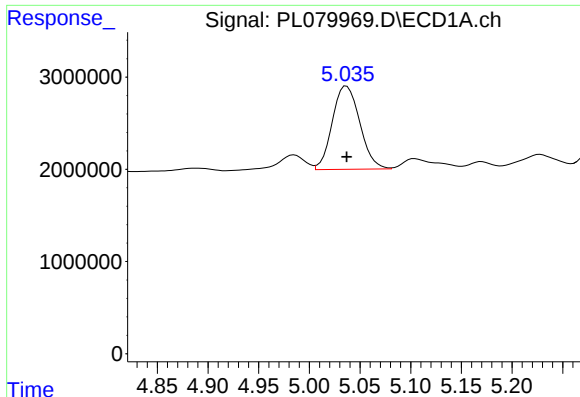

#24 Chlordane-2


R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 17092663
Conc: 248.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

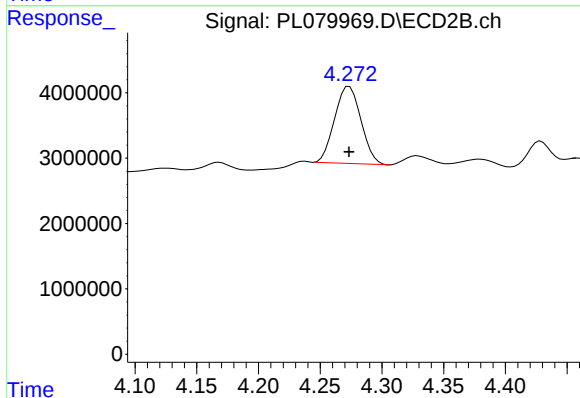


#24 Chlordane-2

R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 17529615
Conc: 249.44 ng/ml

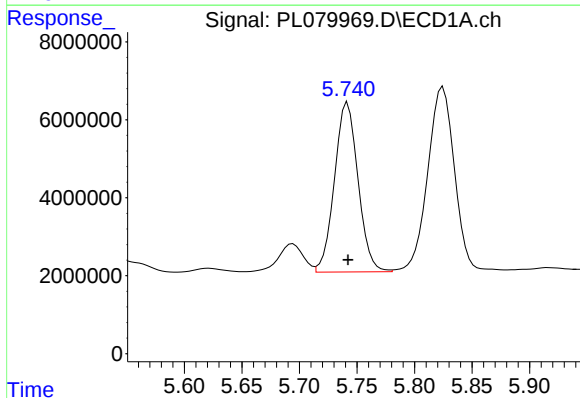


#25 Chlordane-3

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 62111762
Conc: 241.94 ng/ml

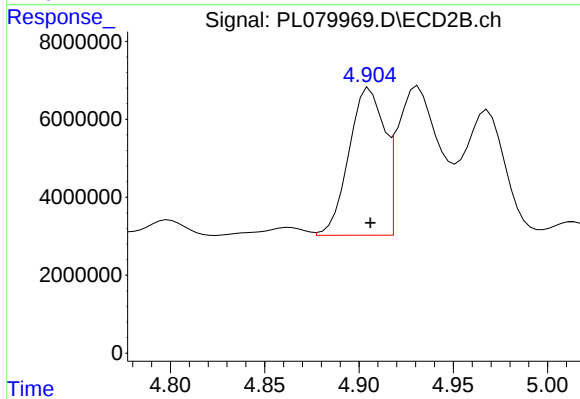

#25 Chlordane-3


R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 49192496
Conc: 233.01 ng/ml

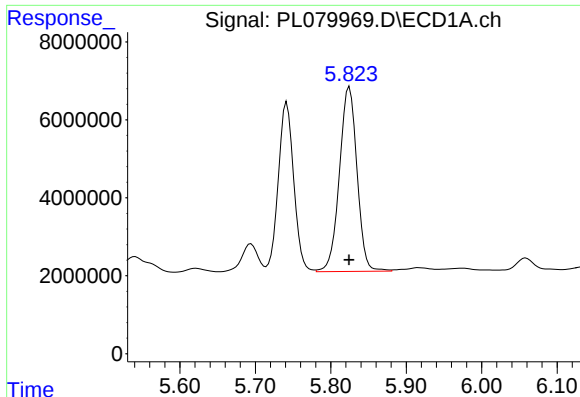

#26 Chlordane-4


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 76797959
Conc: 242.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

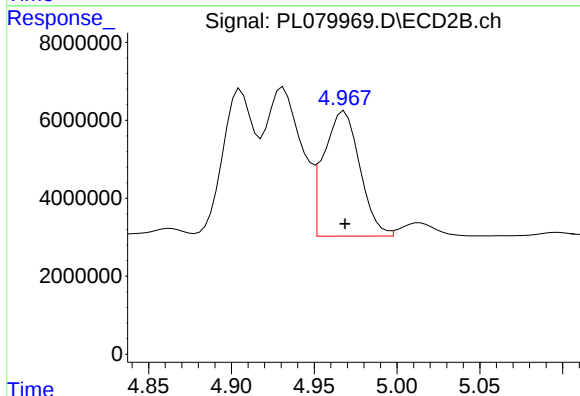


#26 Chlordane-4

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 48668027
Conc: 235.70 ng/ml

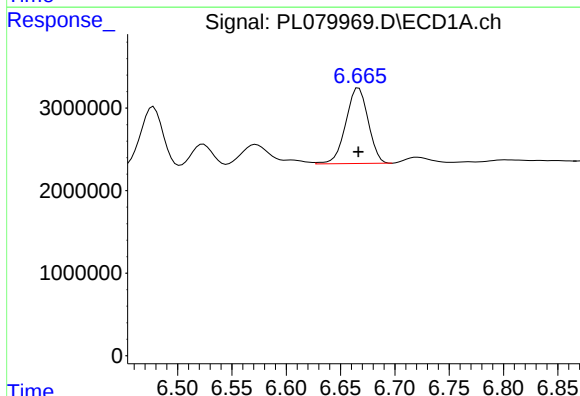


#27 Chlordane-5

R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 13125433
Conc: 239.38 ng/ml

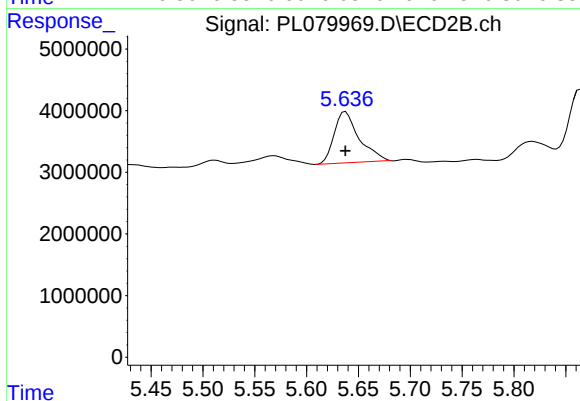

#27 Chlordane-5


R.T.: 5.638 min
Delta R.T.: 0.000 min
Response: 13906340
Conc: 251.06 ng/ml

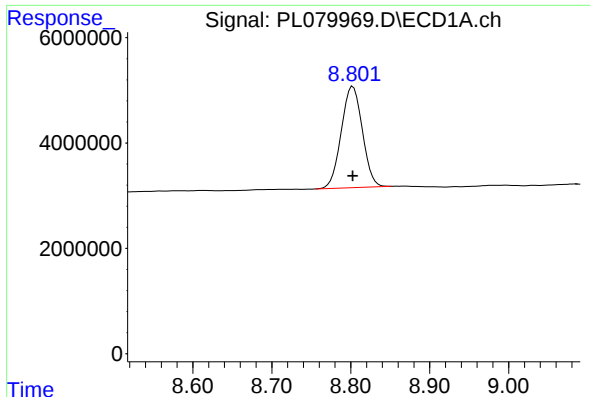

#28 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 35747118
Conc: 25.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

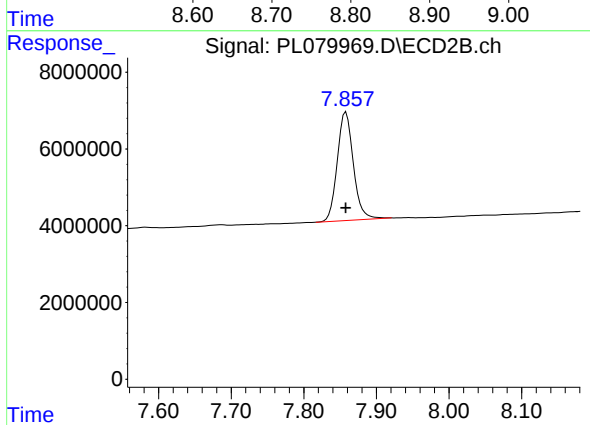

#28 Decachlorobiphenyl

R.T.: 7.858 min
Delta R.T.: 0.000 min
Response: 43708249
Conc: 24.71 ng/ml