

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
 Data File : PL079977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 18:35
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL123022CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 05:14:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 30 05:13:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	2.695	68969334	107.7E6	50.933	52.109
28)	SA Decachlor...	8.803	7.857	71823980	90550111	51.562	52.510
Target Compounds							
23)	Chlordane-1	4.511	3.695	27850467	31884888	517.527	506.828
24)	Chlordane-2	5.037	4.273	34365472	35000465	506.643	515.928
25)	Chlordane-3	5.742	4.906	129.8E6	104.3E6	509.737	514.963
26)	Chlordane-4	5.825	4.968	159.1E6	102.2E6	515.584	510.886
27)	Chlordane-5	6.667	5.637	26478309	28683655	489.086	529.032



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123022\
Data File : PL079977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 18:35
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL123022CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 05:14:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL123022.M
Quant Title : GC Extractables
QLast Update : Fri Dec 30 05:13:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

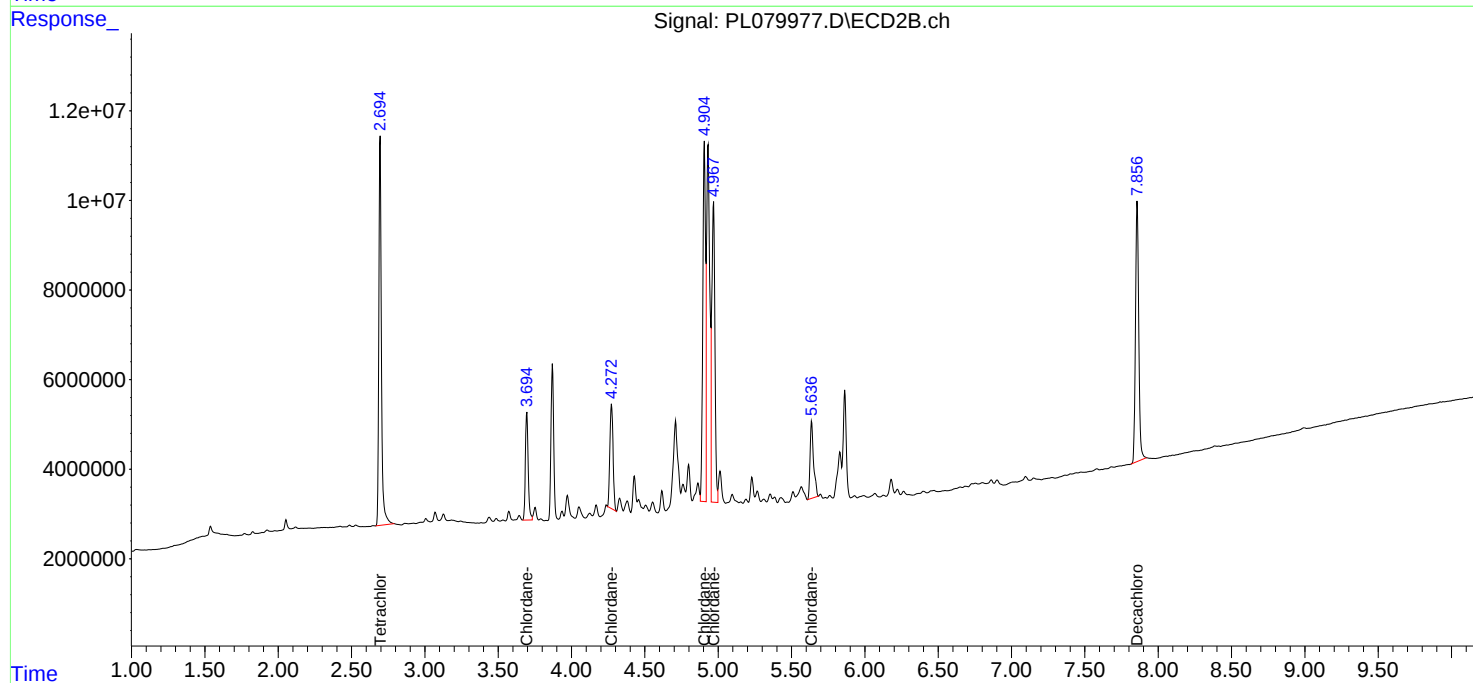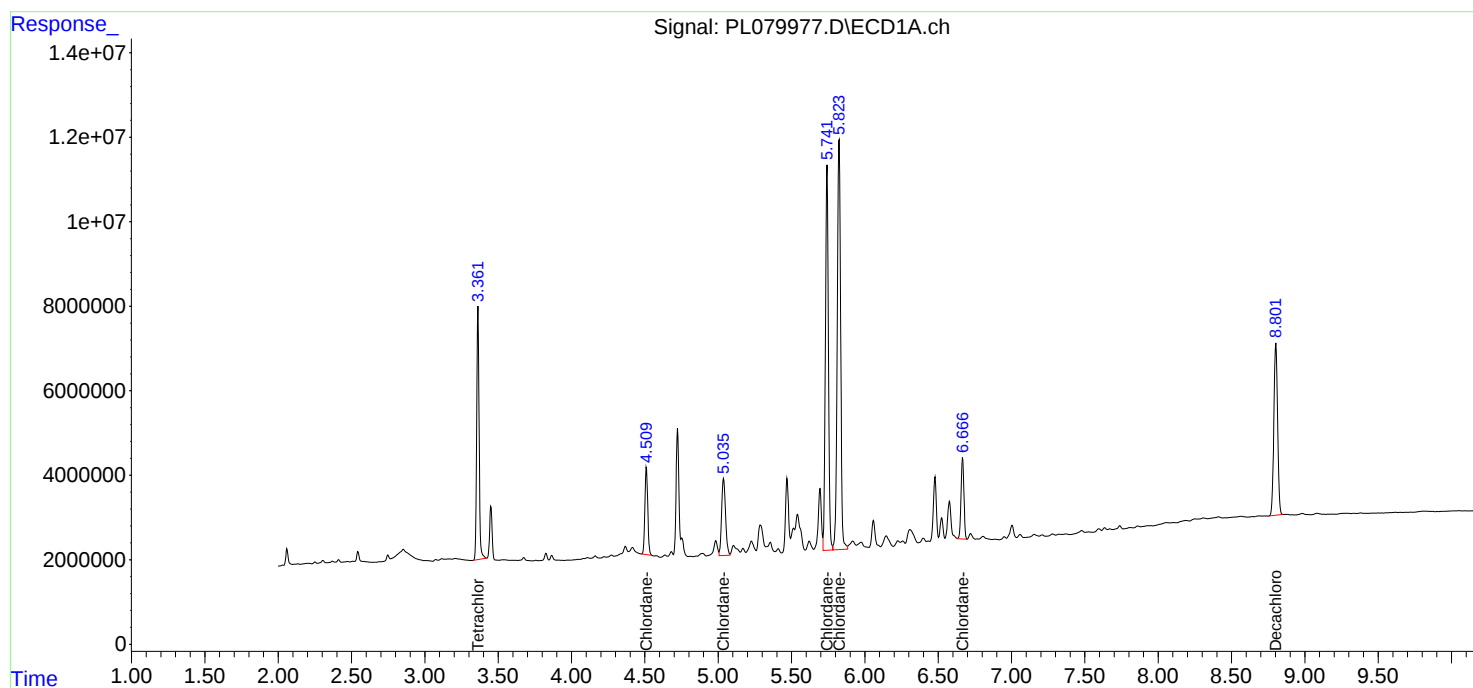


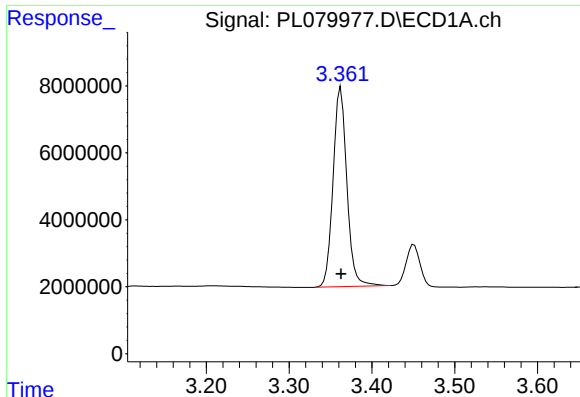

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 68969334
Conc: 50.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL123022CHLOR

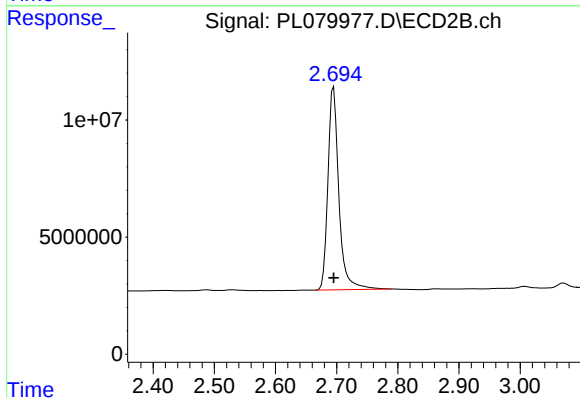


#1 Tetrachloro-m-xylene

R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 107661120
Conc: 52.11 ng/ml

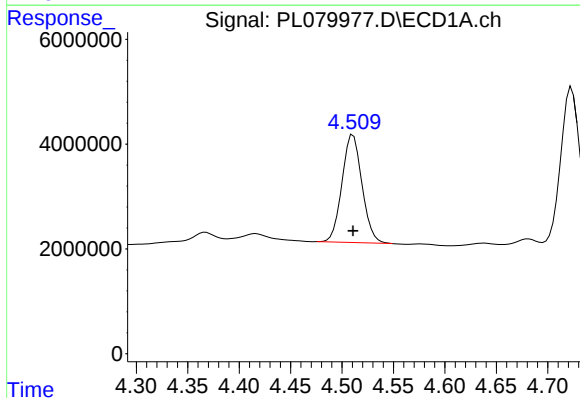


#23 Chlordane-1

R.T.: 4.511 min
Delta R.T.: 0.000 min
Response: 27850467
Conc: 517.53 ng/ml

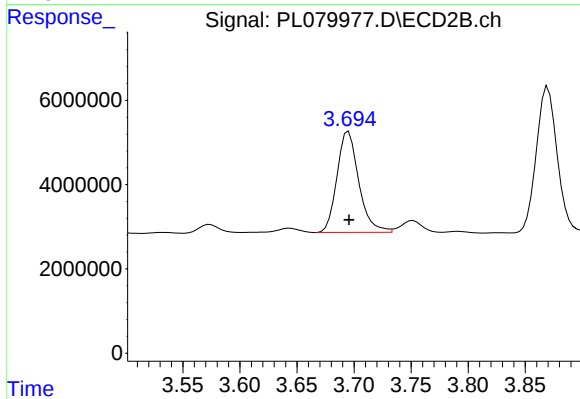

#23 Chlordane-1


R.T.: 3.695 min
Delta R.T.: 0.000 min
Response: 31884888
Conc: 506.83 ng/ml

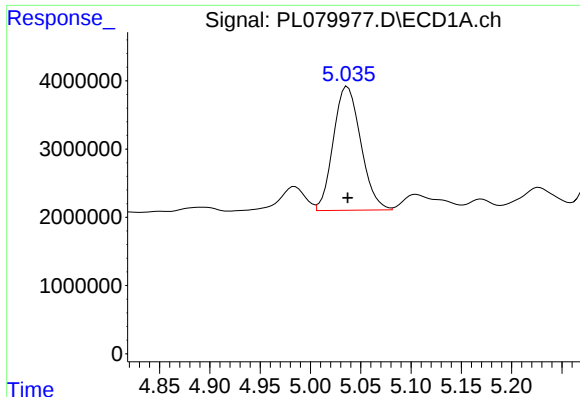

#24 Chlordane-2


R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 34365472
Conc: 506.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL123022CHLOR

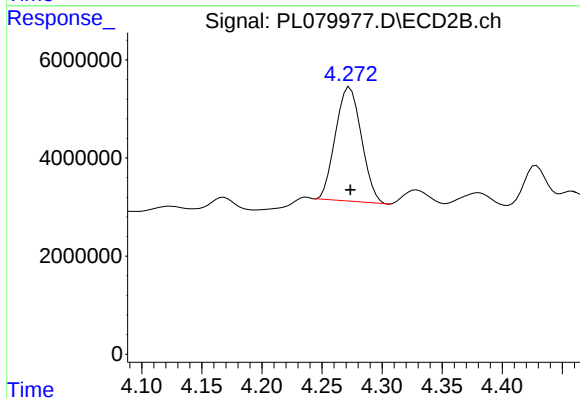


#24 Chlordane-2

R.T.: 4.273 min
Delta R.T.: 0.000 min
Response: 35000465
Conc: 515.93 ng/ml

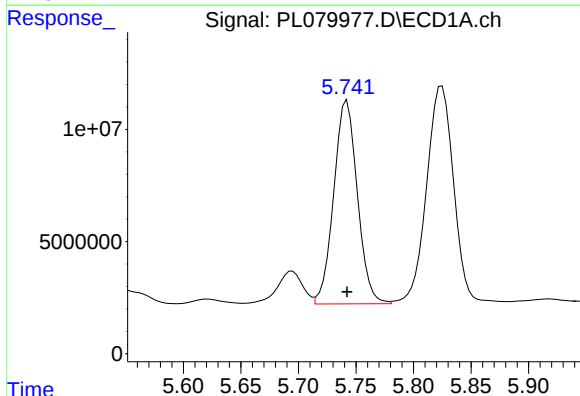


#25 Chlordane-3

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 129751449
Conc: 509.74 ng/ml

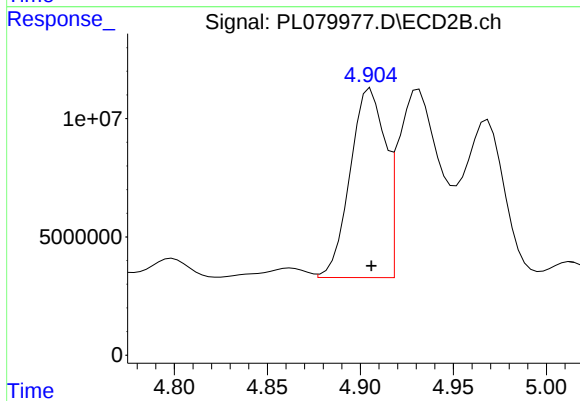

#25 Chlordane-3


R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 104300798
Conc: 514.96 ng/ml

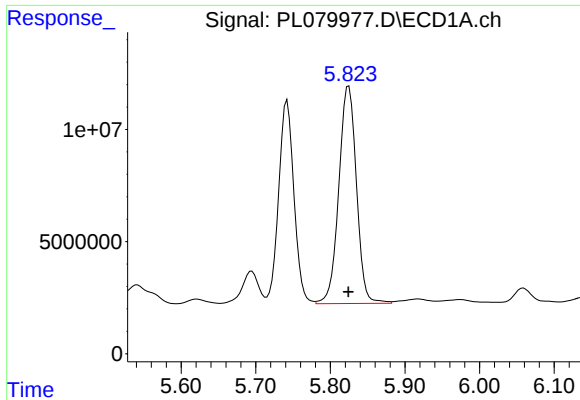

#26 Chlordane-4


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 159130923
Conc: 515.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL123022CHLOR

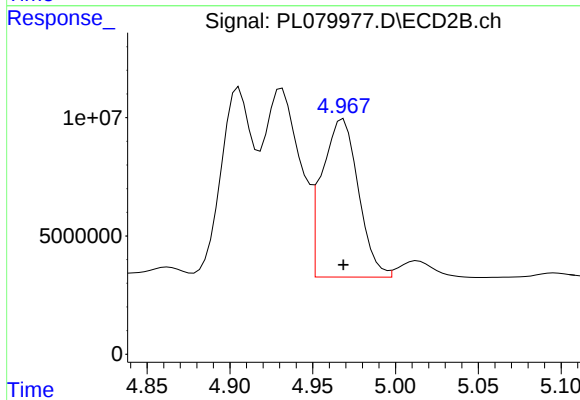


#26 Chlordane-4

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 102228154
Conc: 510.89 ng/ml

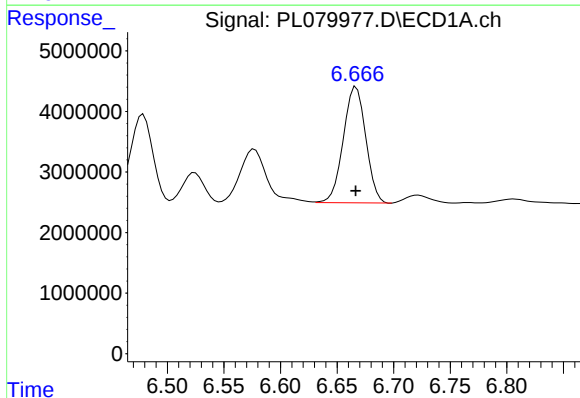


#27 Chlordane-5

R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 26478309
Conc: 489.09 ng/ml

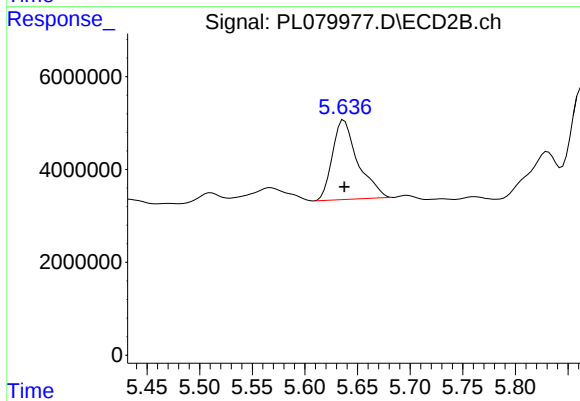

#27 Chlordane-5


R.T.: 5.637 min
Delta R.T.: 0.000 min
Response: 28683655
Conc: 529.03 ng/ml

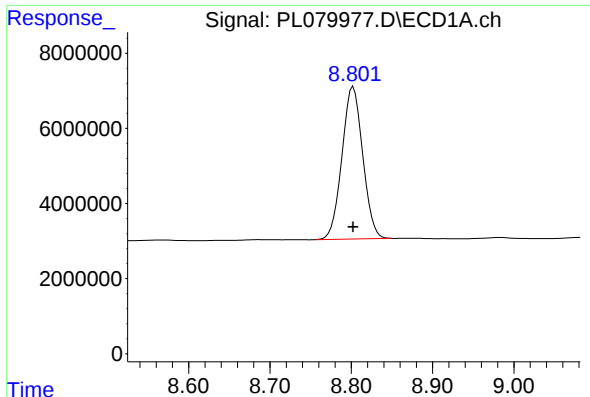

#28 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 71823980
Conc: 51.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL123022CHLOR

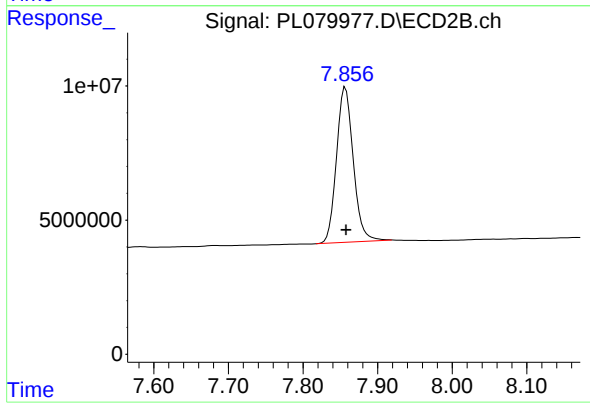

#28 Decachlorobiphenyl

R.T.: 7.857 min
Delta R.T.: 0.000 min
Response: 90550111
Conc: 52.51 ng/ml