

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123024\
 Data File : PL093565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2024 13:14
 Operator : AR\AJ
 Sample : P5391-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-07-12272024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 02:22:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.774	14191505	7341386	5.732	2.522 #
28)	SA Decachlor...	9.057	7.914	3279764	5116313	1.774	1.713
Target Compounds							
5)	MB Aldrin	0.000	4.215	0	1209900	N.D.	0.295 #
6)	B beta-BHC	0.000	3.914	0	969237	N.D.	0.539 #
7)	B delta-BHC	0.000	4.126	0	1666979	N.D.	0.394 #
9)	A Endosulfan I	0.000	5.127f	0	78933	N.D.	0.023 #
10)	B gamma-Chl...	0.000	4.980	0	552078	N.D.	0.143 #
11)	B alpha-Chl...	0.000	5.022f	0	1272698	N.D.	0.334 #
13)	MA Dieldrin	0.000	5.357	0	471496	N.D.	0.122 #
14)	MA Endrin	0.000	5.631	0	78352	N.D.	0.024 #
23)	Chlordane-1	0.000	3.804f	0	785821	N.D.	6.507 #
24)	Chlordane-2	0.000	4.323f	0	528919	N.D.	3.810 #
25)	Chlordane-3	0.000	4.980	0	552078	N.D.	1.301 #
26)	Chlordane-4	0.000	5.022f	0	1272698	N.D.	3.094 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123024\
Data File : PL093565.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2024 13:14
Operator : AR\AJ
Sample : P5391-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 02:22:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

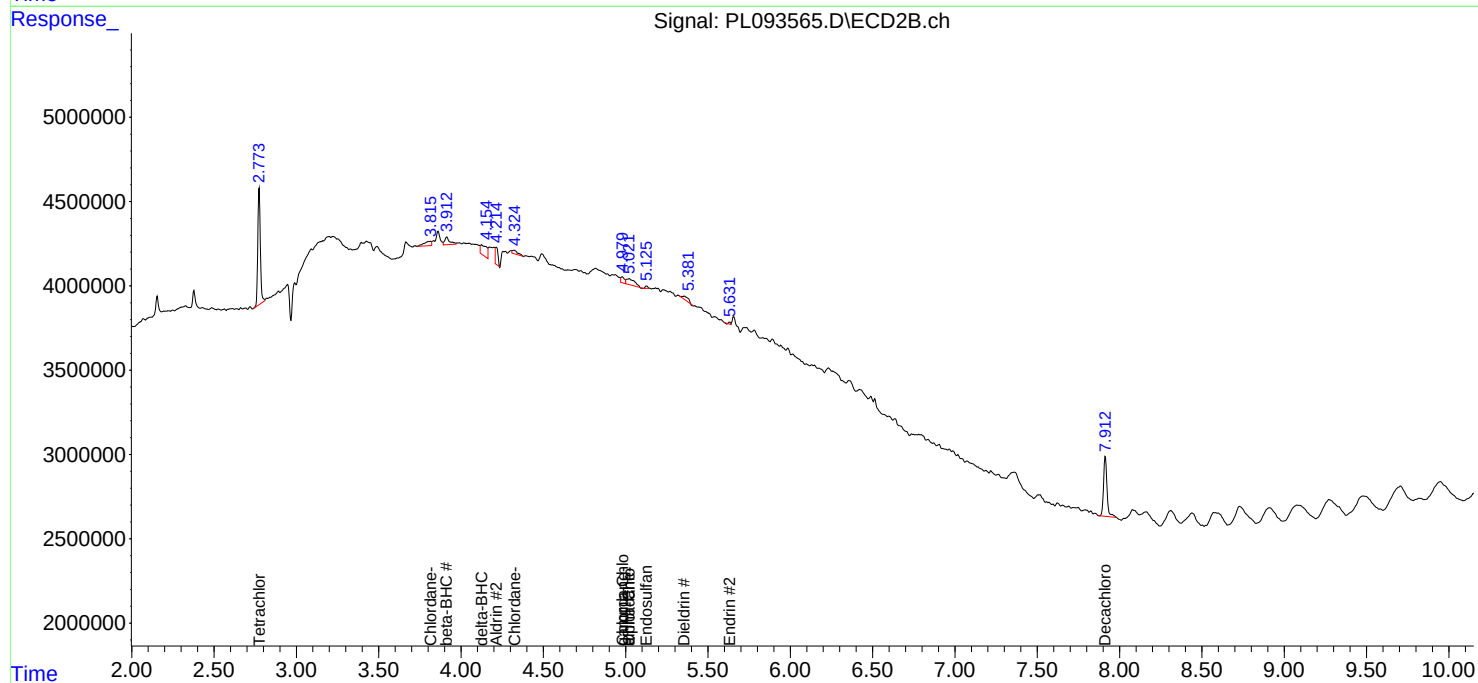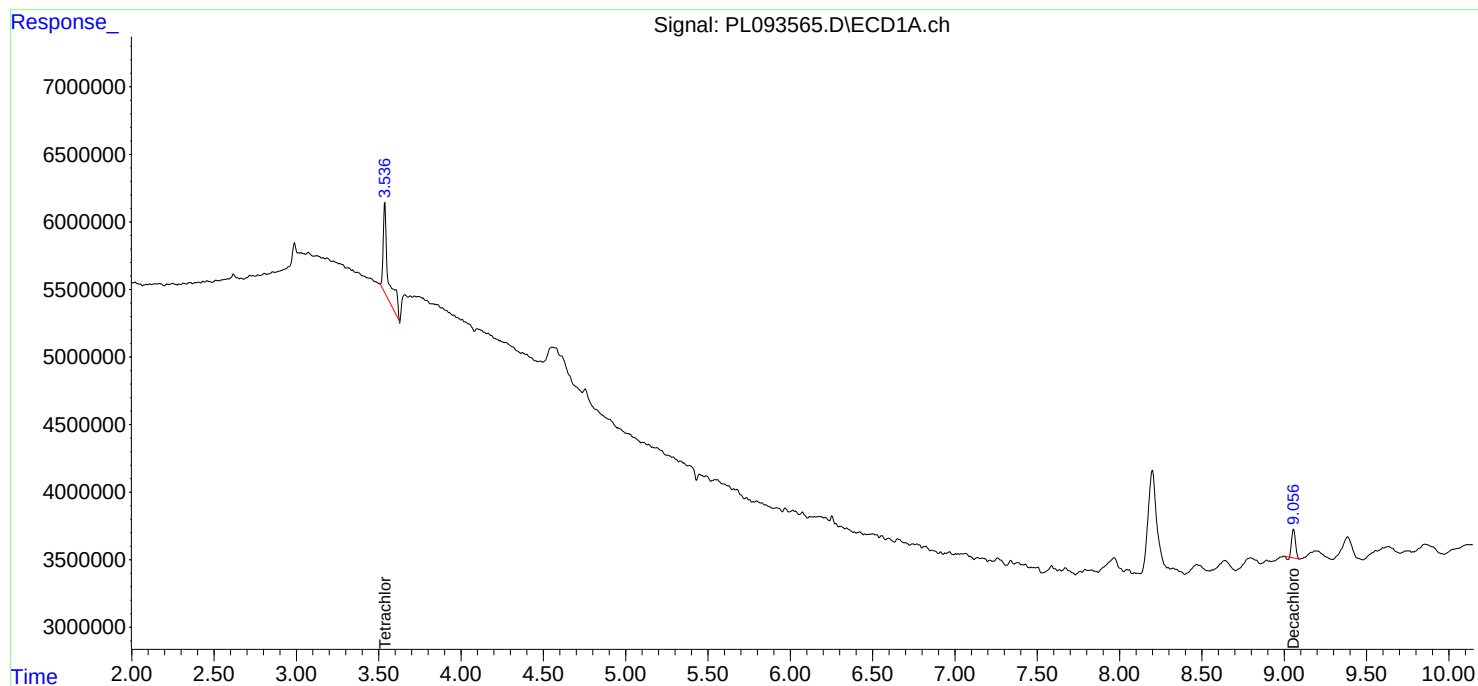


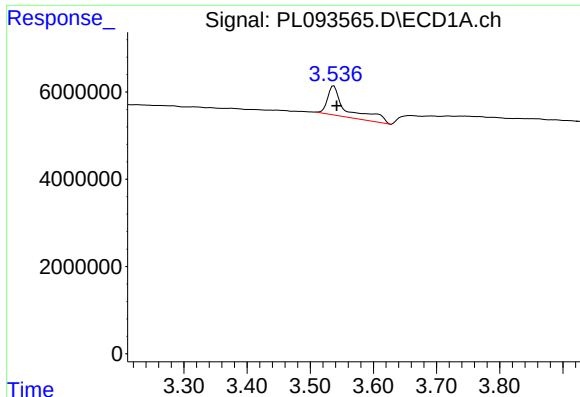

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: -0.005 min
Response: 14191505
Conc: 5.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024

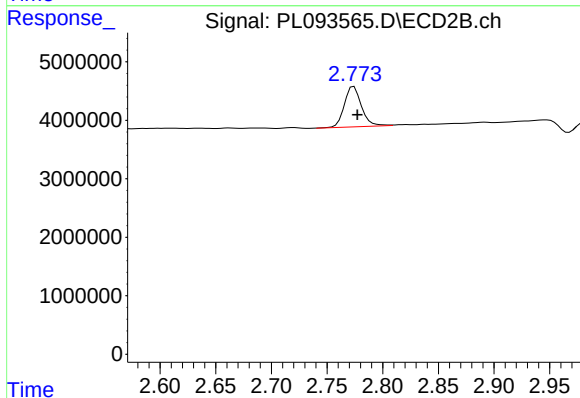


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: -0.003 min
Response: 7341386
Conc: 2.52 ng/ml

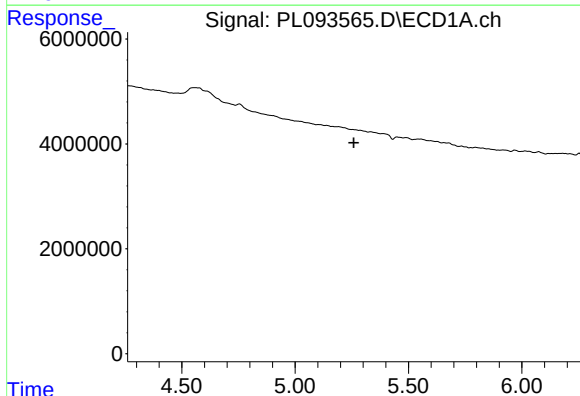


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.259 min
Response: 0
Conc: N.D.

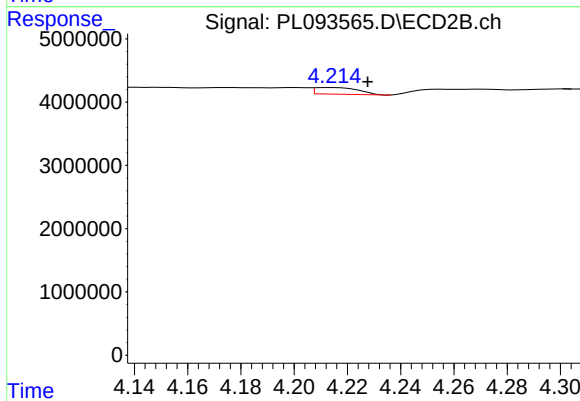

#5 Aldrin


R.T.: 4.215 min
Delta R.T.: -0.013 min
Response: 1209900
Conc: 0.29 ng/ml

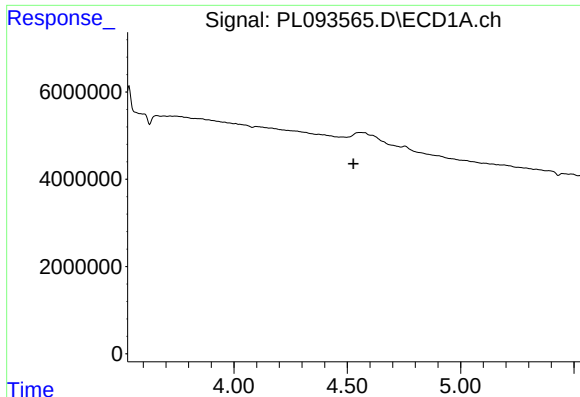

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024

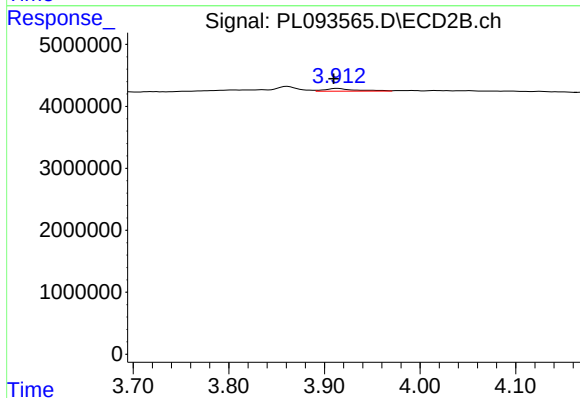


#6 beta-BHC

R.T.: 3.914 min
Delta R.T.: 0.004 min
Response: 969237
Conc: 0.54 ng/ml

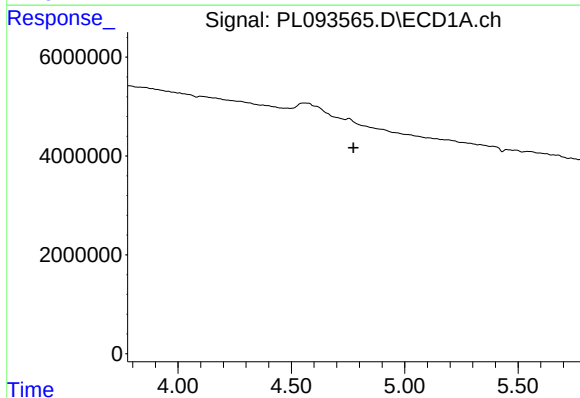


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.775 min
Response: 0
Conc: N.D.

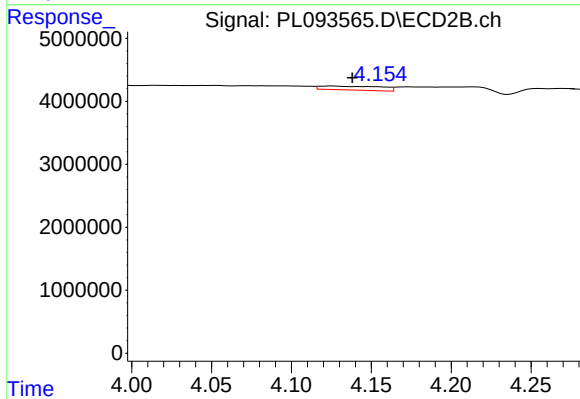

#7 delta-BHC


R.T.: 4.126 min
Delta R.T.: -0.012 min
Response: 1666979
Conc: 0.39 ng/ml

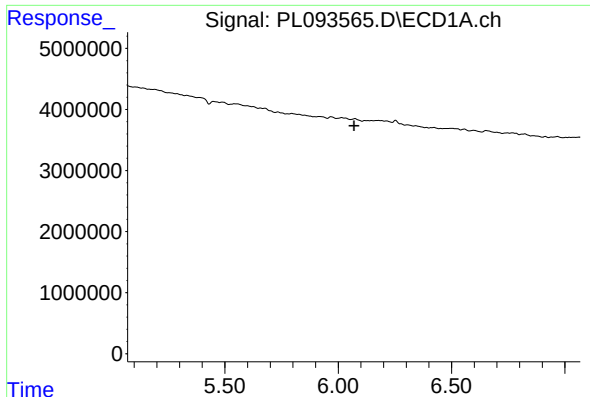

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024

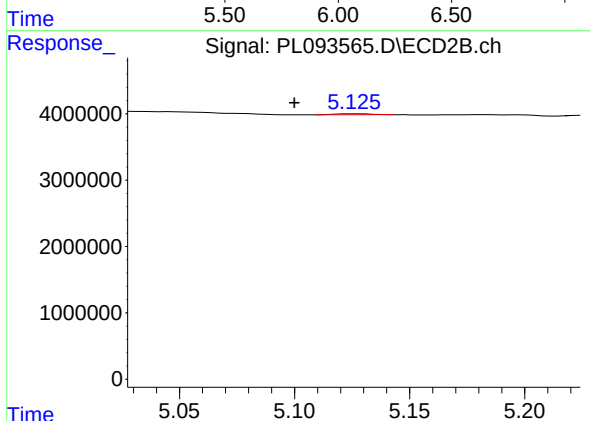


#9 Endosulfan I

R.T.: 5.127 min
Delta R.T.: 0.027 min
Response: 78933
Conc: 0.02 ng/ml

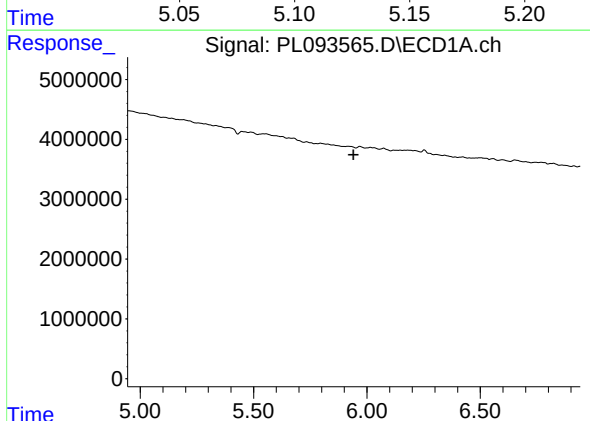


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

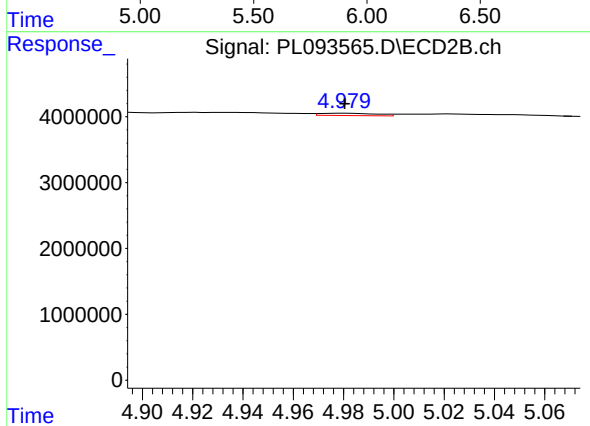

#10 gamma-Chlordane


R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 552078
Conc: 0.14 ng/ml

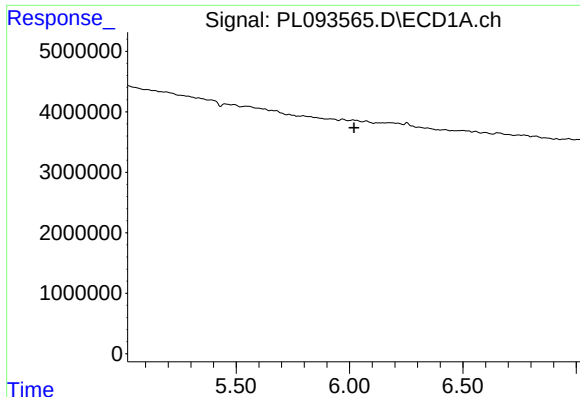

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024

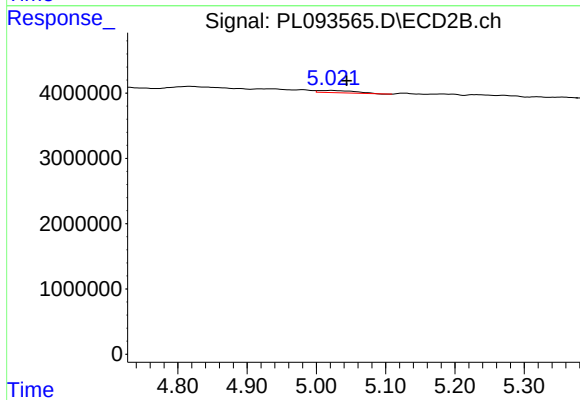


#11 alpha-Chlordane

R.T.: 5.022 min
Delta R.T.: -0.022 min
Response: 1272698
Conc: 0.33 ng/ml

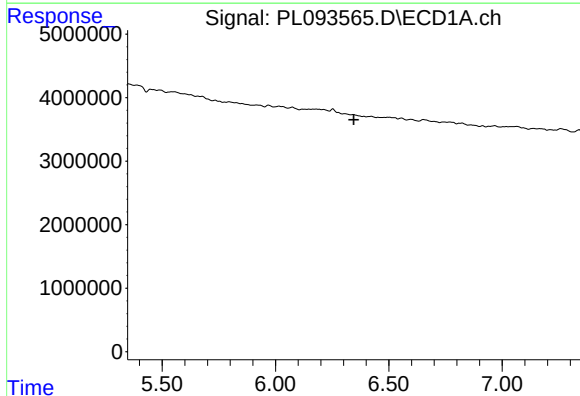


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.346 min
Response: 0
Conc: N.D.

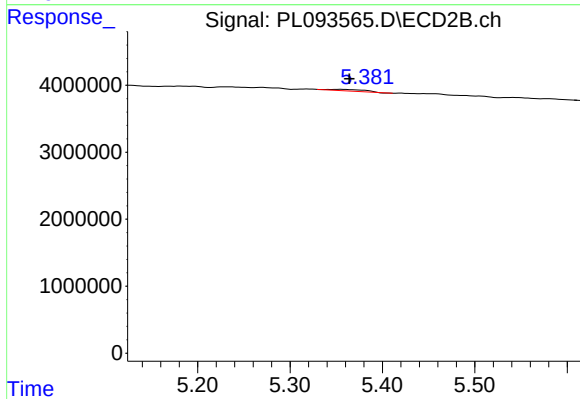

#13 Dieldrin


R.T.: 5.357 min
Delta R.T.: -0.008 min
Response: 471496
Conc: 0.12 ng/ml

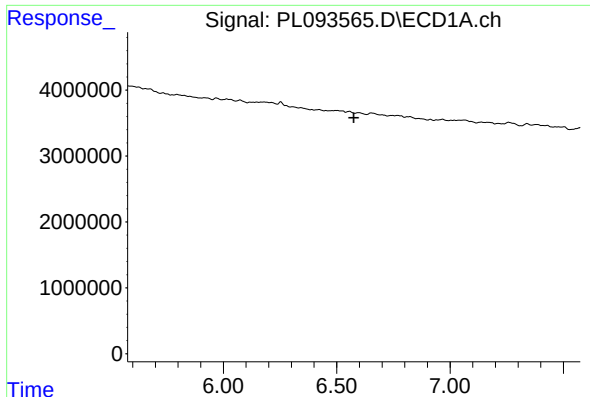

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024

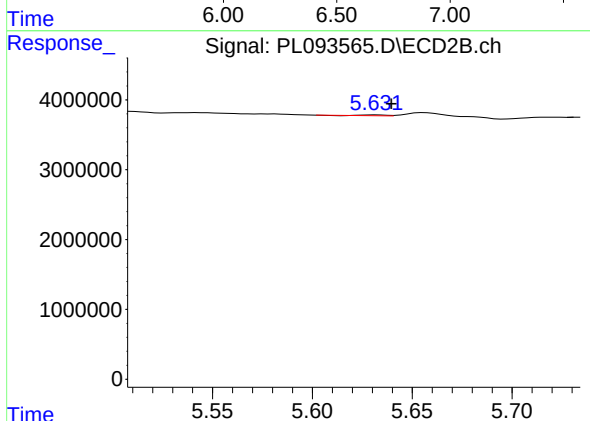


#14 Endrin

R.T.: 5.631 min
Delta R.T.: -0.008 min
Response: 78352
Conc: 0.02 ng/ml

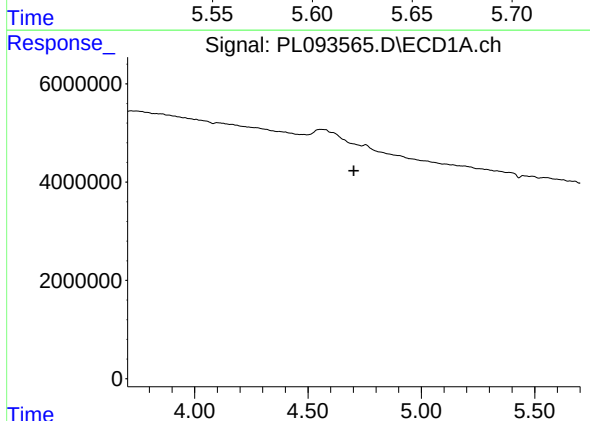


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.702 min
Response: 0
Conc: N.D.

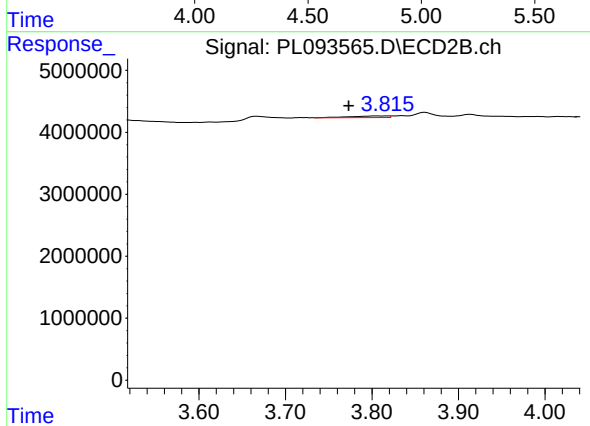

#23 Chlordane-1


R.T.: 3.804 min
Delta R.T.: 0.031 min
Response: 785821
Conc: 6.51 ng/ml

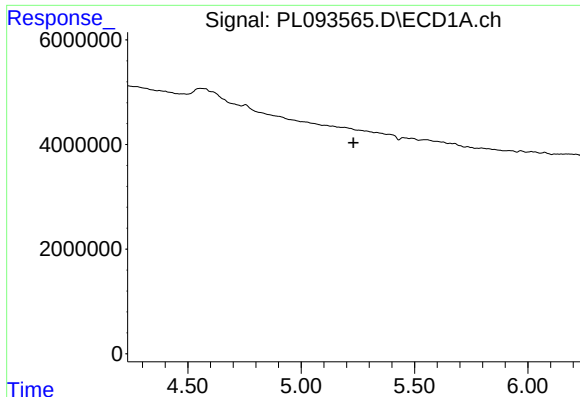

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024

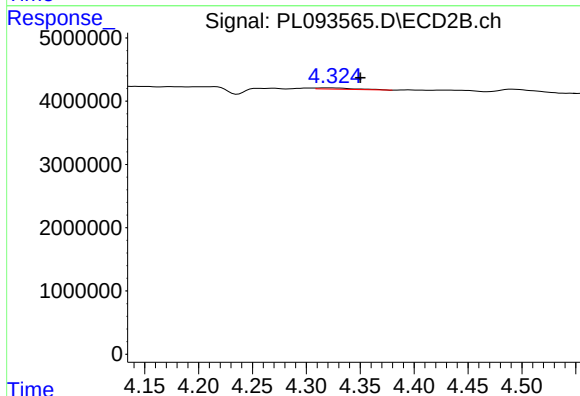


#24 Chlordane-2

R.T.: 4.323 min
Delta R.T.: -0.027 min
Response: 528919
Conc: 3.81 ng/ml

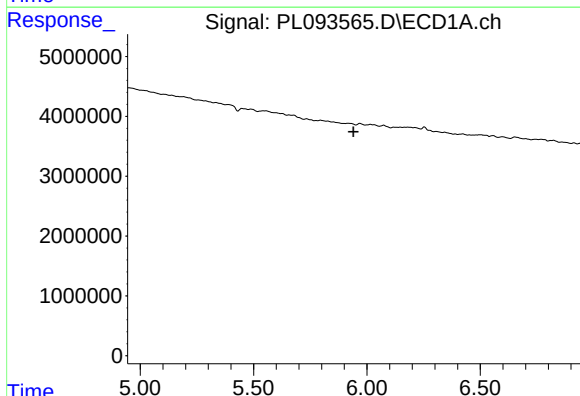


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

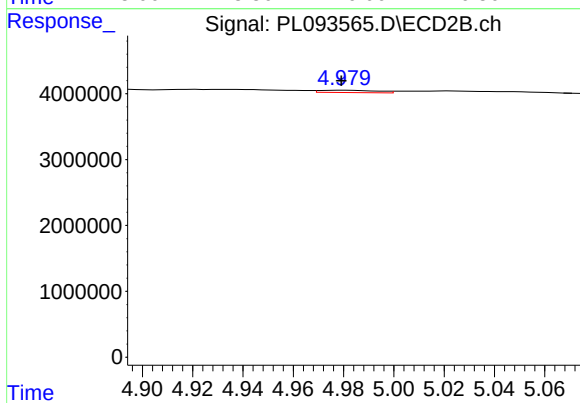

#25 Chlordane-3


R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 552078
Conc: 1.30 ng/ml

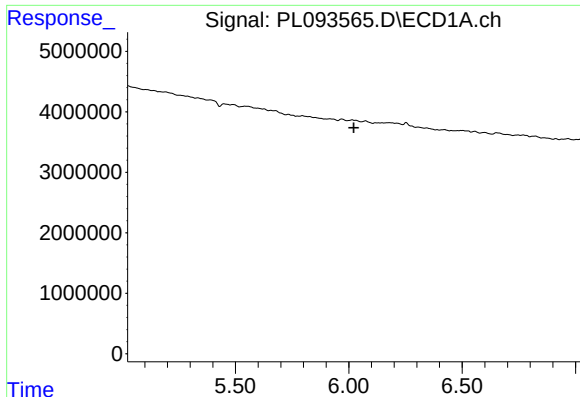

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024

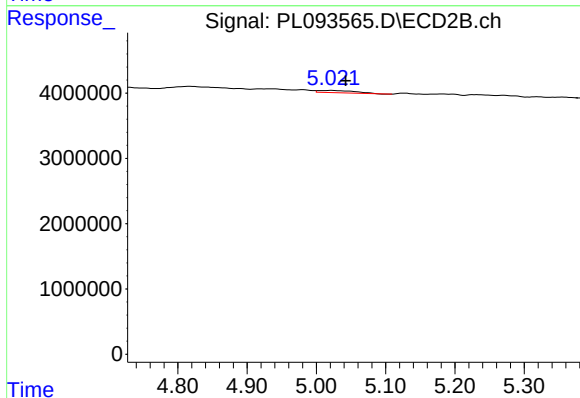


#26 Chlordane-4

R.T.: 5.022 min
Delta R.T.: -0.020 min
Response: 1272698
Conc: 3.09 ng/ml

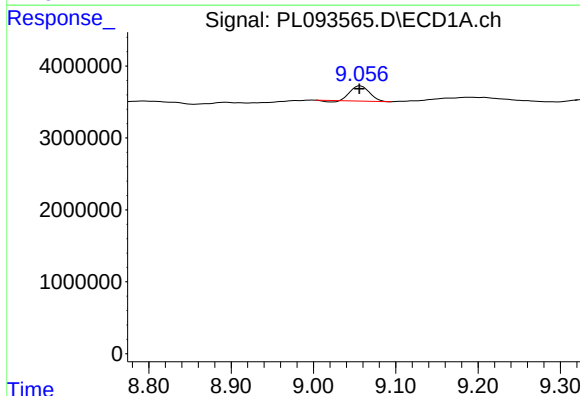

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: 0.001 min
Response: 3279764
Conc: 1.77 ng/ml

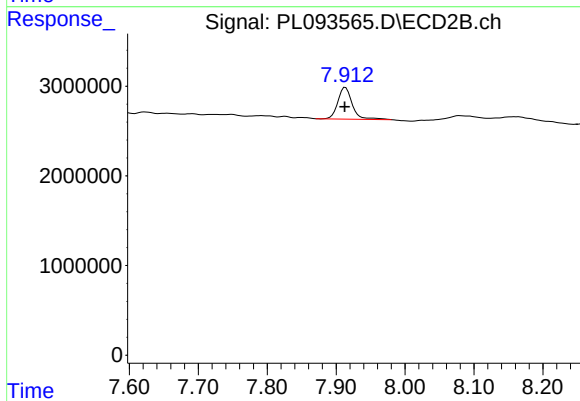

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.001 min
Response: 5116313
Conc: 1.71 ng/ml