

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123024\
 Data File : PL093565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2024 13:14
 Operator : AR\AJ
 Sample : P5391-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-07-12272024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/31/2024
 Supervised By :Ankita Jodhani 12/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 02:22:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.774	6988208	7341386	2.823m	2.522
28) SA Decachlor...	9.056	7.912	3851136	4891614	2.083m	1.638m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123024\
Data File : PL093565.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2024 13:14
Operator : AR\AJ
Sample : P5391-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-07-12272024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/31/2024
Supervised By :Ankita Jodhani 12/31/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 02:22:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

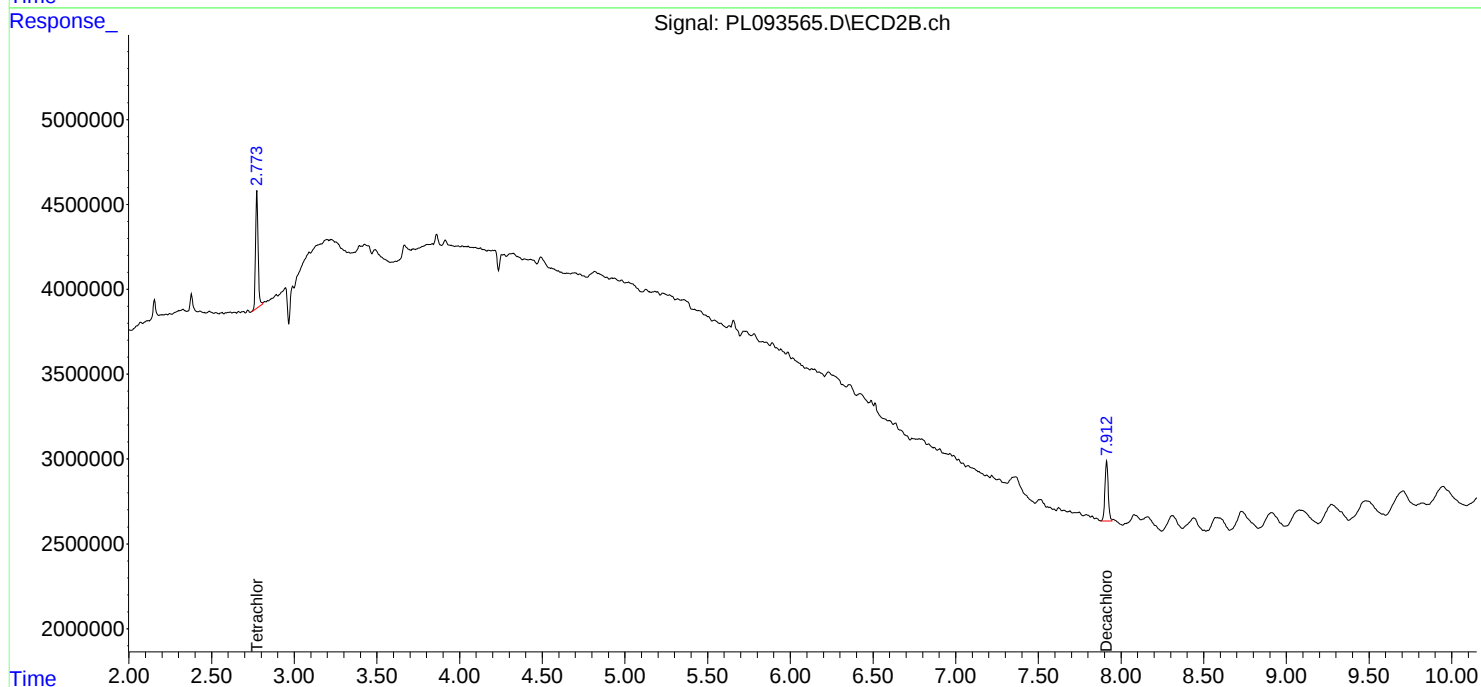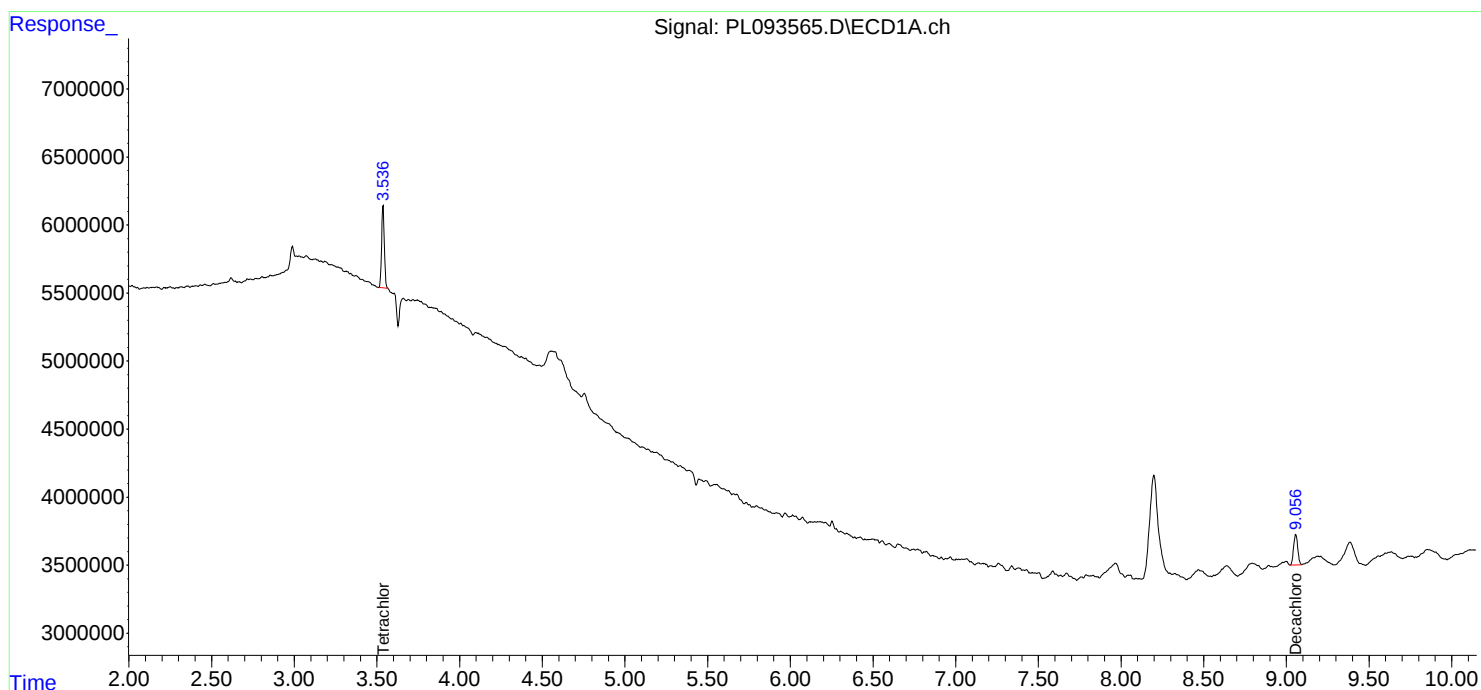

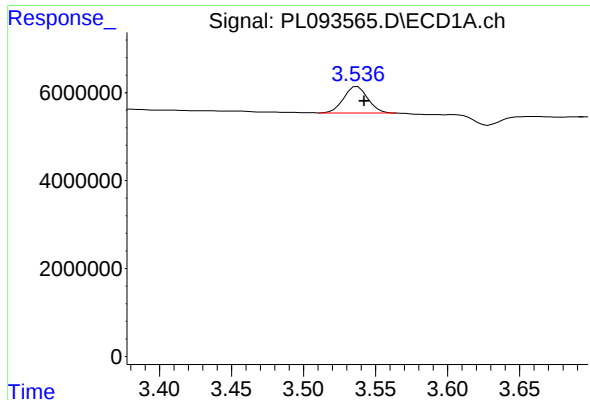


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.006 min
Response: 6988208
Conc: 2.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-12272024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/31/2024
Supervised By :Ankita Jodhani 12/31/2024

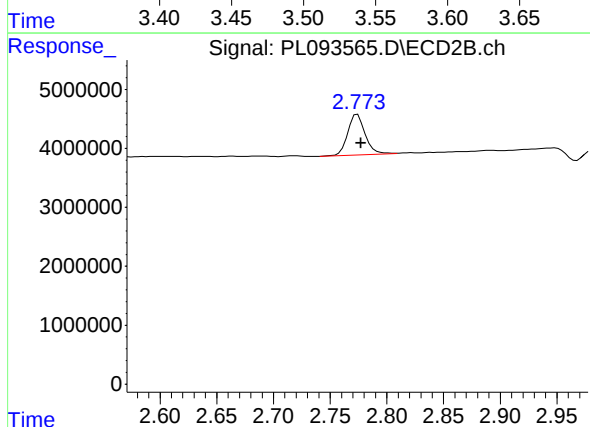


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: -0.003 min
Response: 7341386
Conc: 2.52 ng/ml

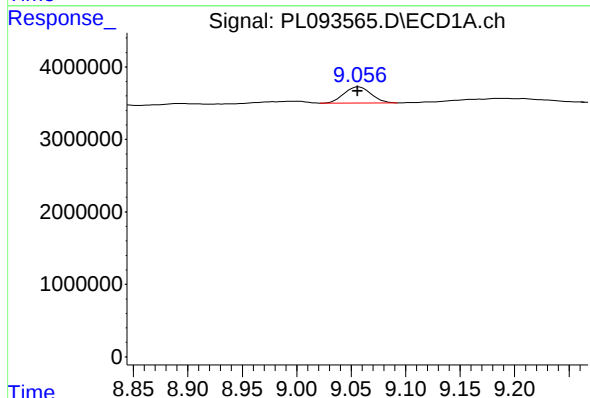

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 3851136
Conc: 2.08 ng/ml m

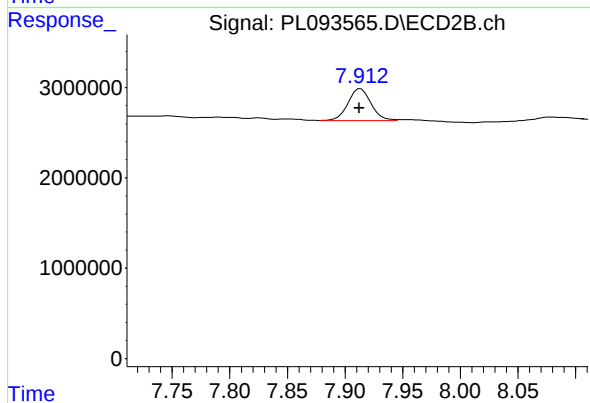

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 4891614
Conc: 1.64 ng/ml m