

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123119\
 Data File : PL055407.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2019 09:24
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:37:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.925	0	20455797	N.D. 8.026 #
9) A	Endosulfan I	0.000	6.284	0	4155109	N.D. 1.678 #
10) B	gamma-Chl...	0.000	6.131f	0	2103730	N.D. 0.793 #
12) B	4,4'-DDE	5.742f	6.368f	63938398	1335403	4.798 0.548 #
14) MA	Endrin	0.000	6.754	0	7880465	N.D. 3.672 #
25)	Chlordane-3	0.000	6.131f	0	2103730	N.D. 6.537 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123119\
Data File : PL055407.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2019 09:24
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:37:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

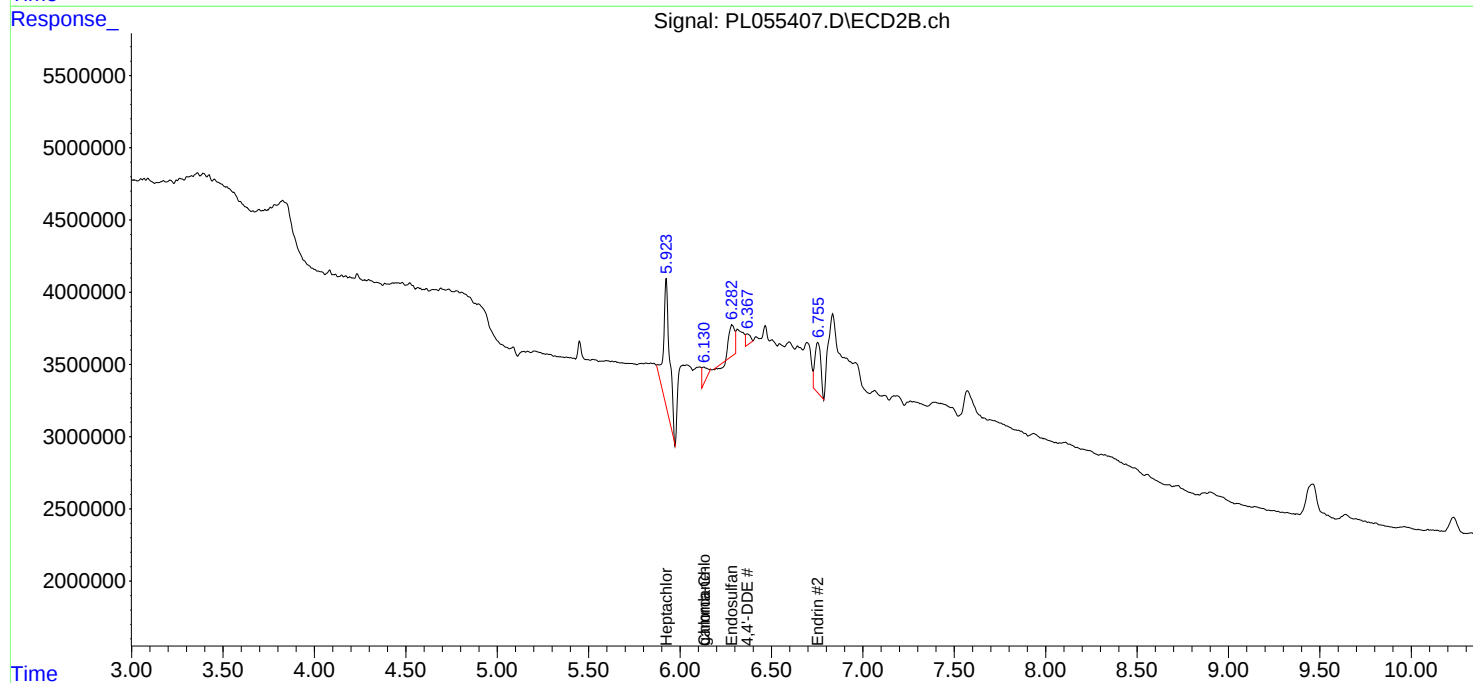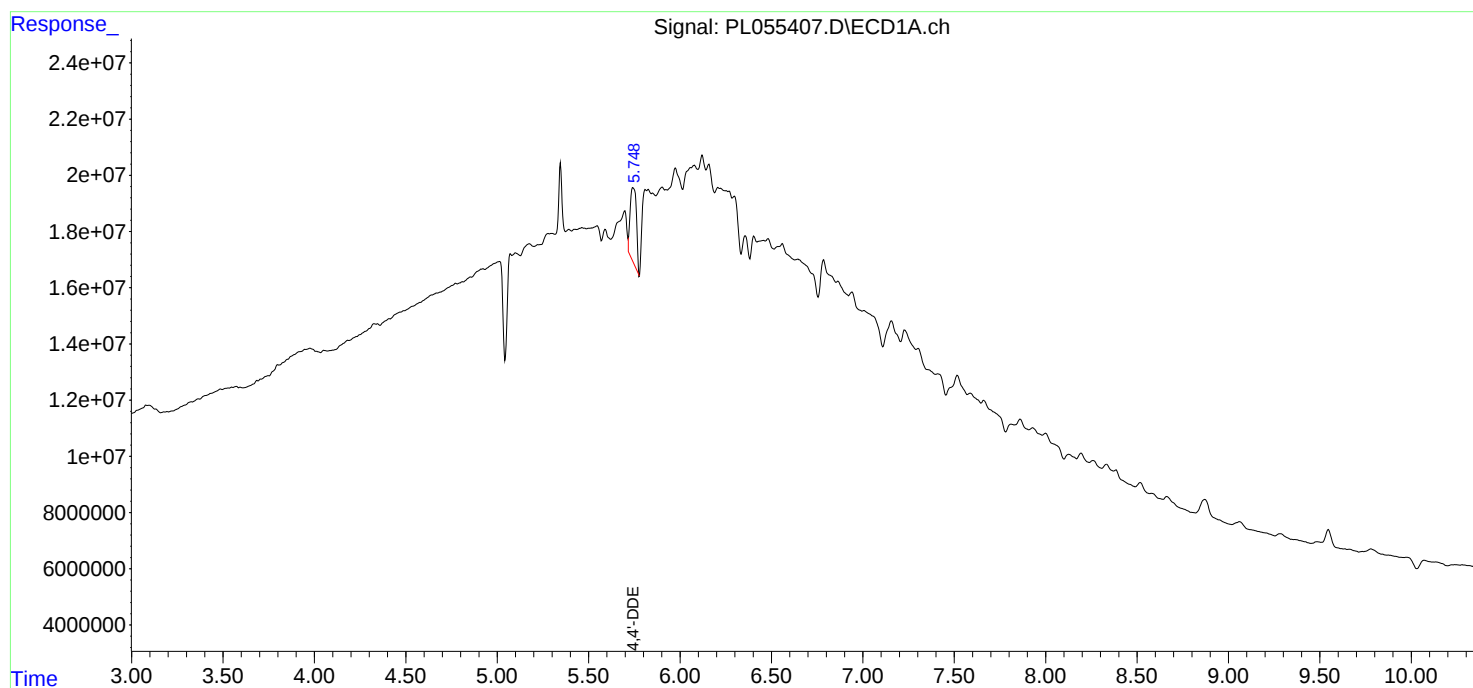


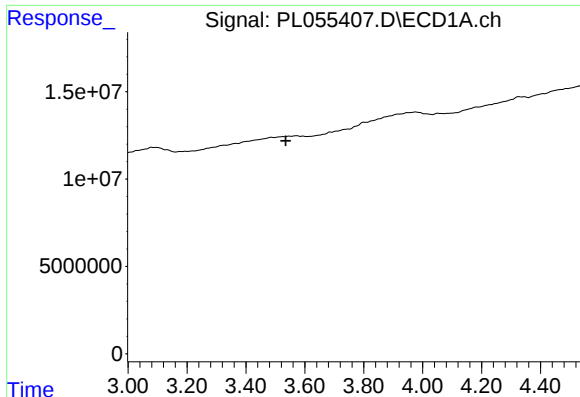

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

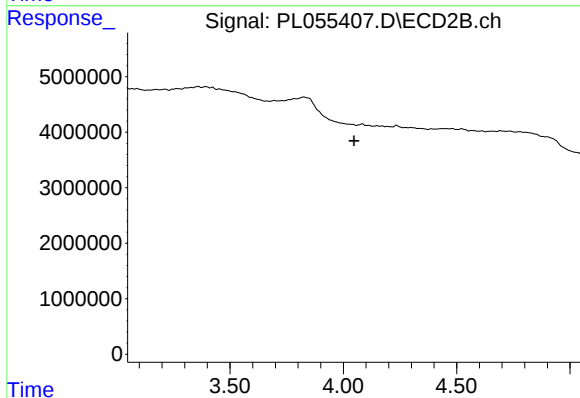


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.047 min
Response: 0
Conc: N.D.

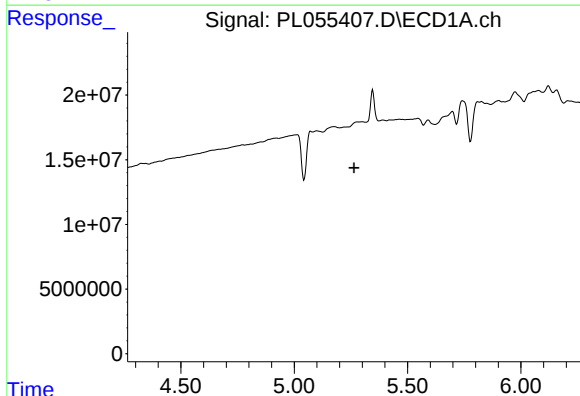


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

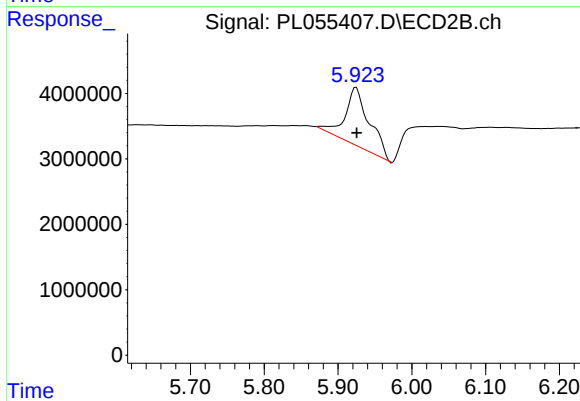

#8 Heptachlor epoxide


R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 20455797
Conc: 8.03 ng/ml

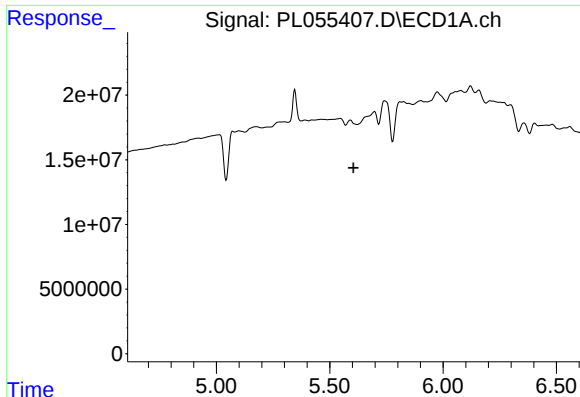

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.605 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

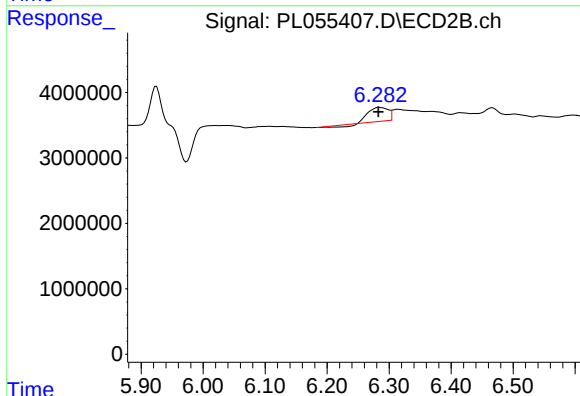


#9 Endosulfan I

R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 4155109
Conc: 1.68 ng/ml

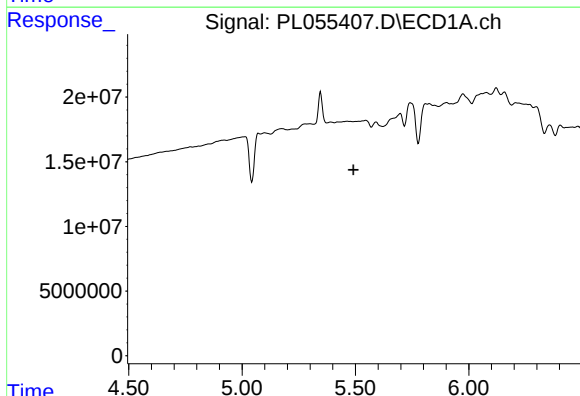


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

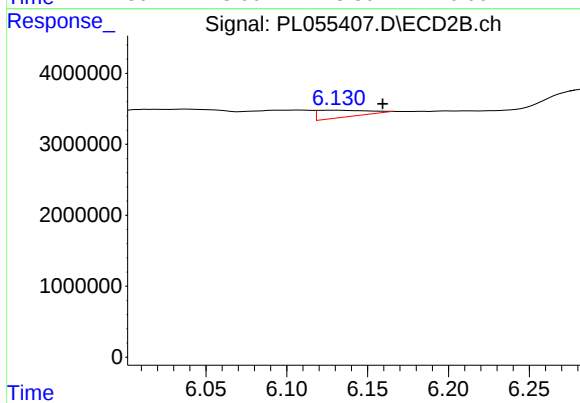

#10 gamma-Chlordane


R.T.: 6.131 min
Delta R.T.: -0.028 min
Response: 2103730
Conc: 0.79 ng/ml

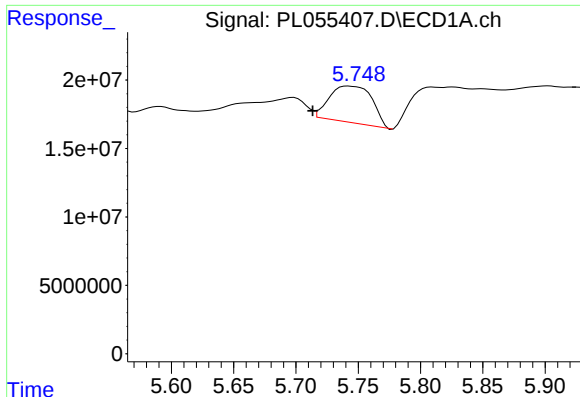

#12 4,4'-DDE


R.T.: 5.742 min
Delta R.T.: 0.029 min
Response: 63938398
Conc: 4.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

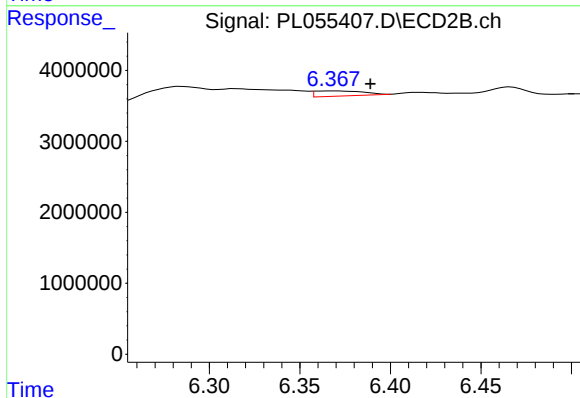


#12 4,4'-DDE

R.T.: 6.368 min
Delta R.T.: -0.021 min
Response: 1335403
Conc: 0.55 ng/ml

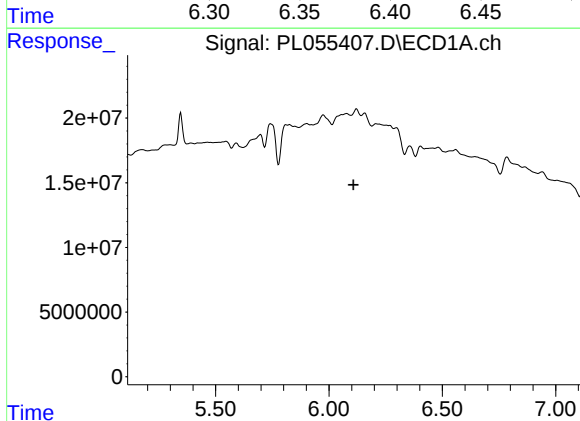


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.108 min
Response: 0
Conc: N.D.

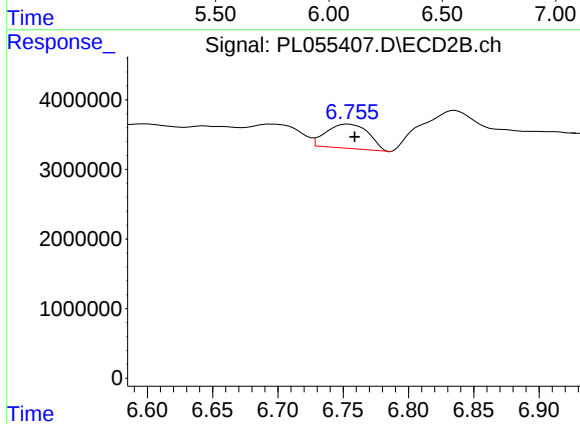

#14 Endrin


R.T.: 6.754 min
Delta R.T.: -0.005 min
Response: 7880465
Conc: 3.67 ng/ml

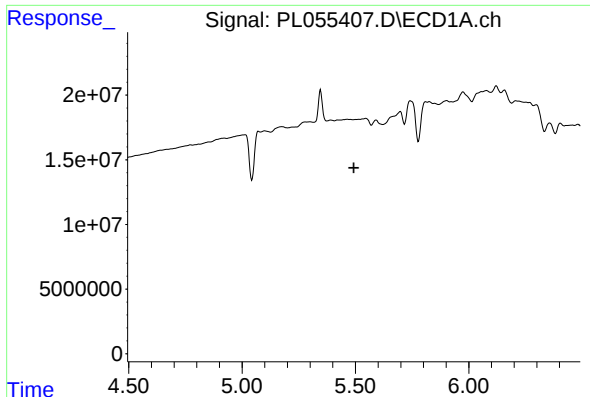

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

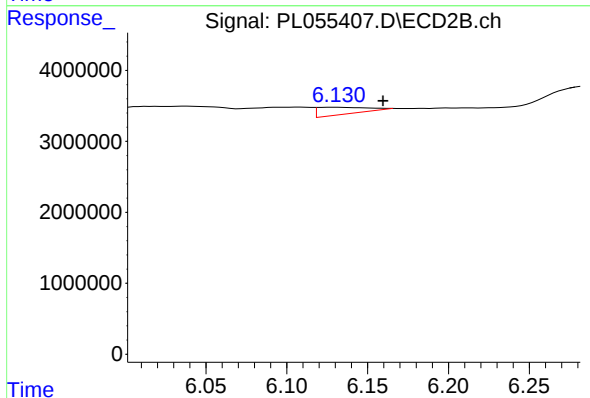


#25 Chlordane-3

R.T.: 6.131 min
Delta R.T.: -0.028 min
Response: 2103730
Conc: 6.54 ng/ml

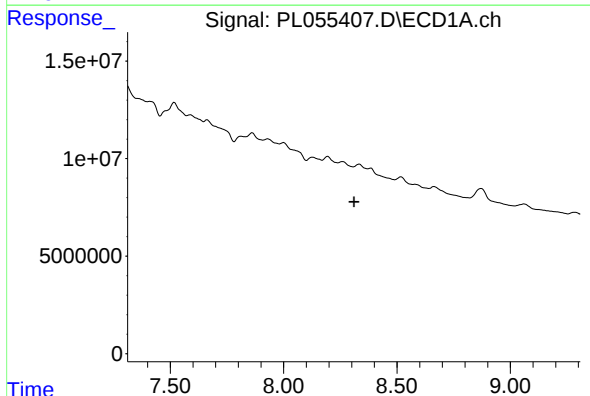

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.310 min
Response: 0
Conc: N.D.

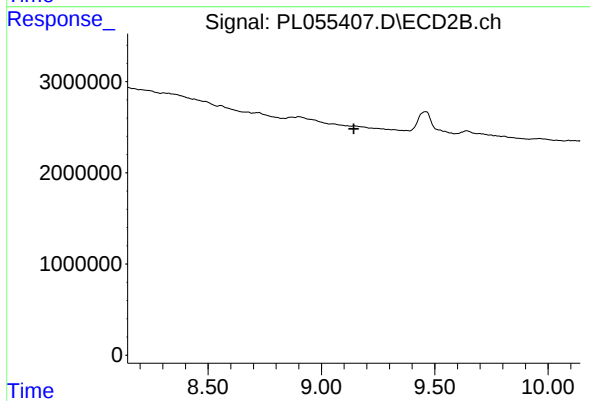

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.143 min
Response: 0
Conc: N.D.