

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123119\
 Data File : PL055421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2019 14:22
 Operator : SG\AJ
 Sample : K6471-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MC-123019-0-2-COMP-B8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:41:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	117.0E6	33397817	11.127	12.640
28)	SA Decachlor...	8.316	9.152	99165323	24581782	10.687	11.136
Target Compounds							
10)	B gamma-Chl...	0.000	6.131f	0	2000101	N.D.	0.754 #
11)	B alpha-Chl...	0.000	6.237	0	5249829	N.D.	2.002 #
12)	B 4,4'-DDE	5.716	6.393	542.7E6	109.5E6	40.727	44.924
16)	A 4,4'-DDD	0.000	6.889	0	6875269	N.D.	3.617 #
17)	MA 4,4'-DDT	6.474	7.185	46658573	9814925	4.635	5.001
20)	A Methoxychlor	7.006	0.000	26881075	0	5.578	N.D. #
25)	Chlordane-3	0.000	6.131f	0	2000101	N.D.	6.215 #
26)	Chlordane-4	0.000	6.237	0	5249829	N.D.	13.658 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123119\
Data File : PL055421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2019 14:22
Operator : SG\AJ
Sample : K6471-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MC-123019-0-2-COMP-B8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:41:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

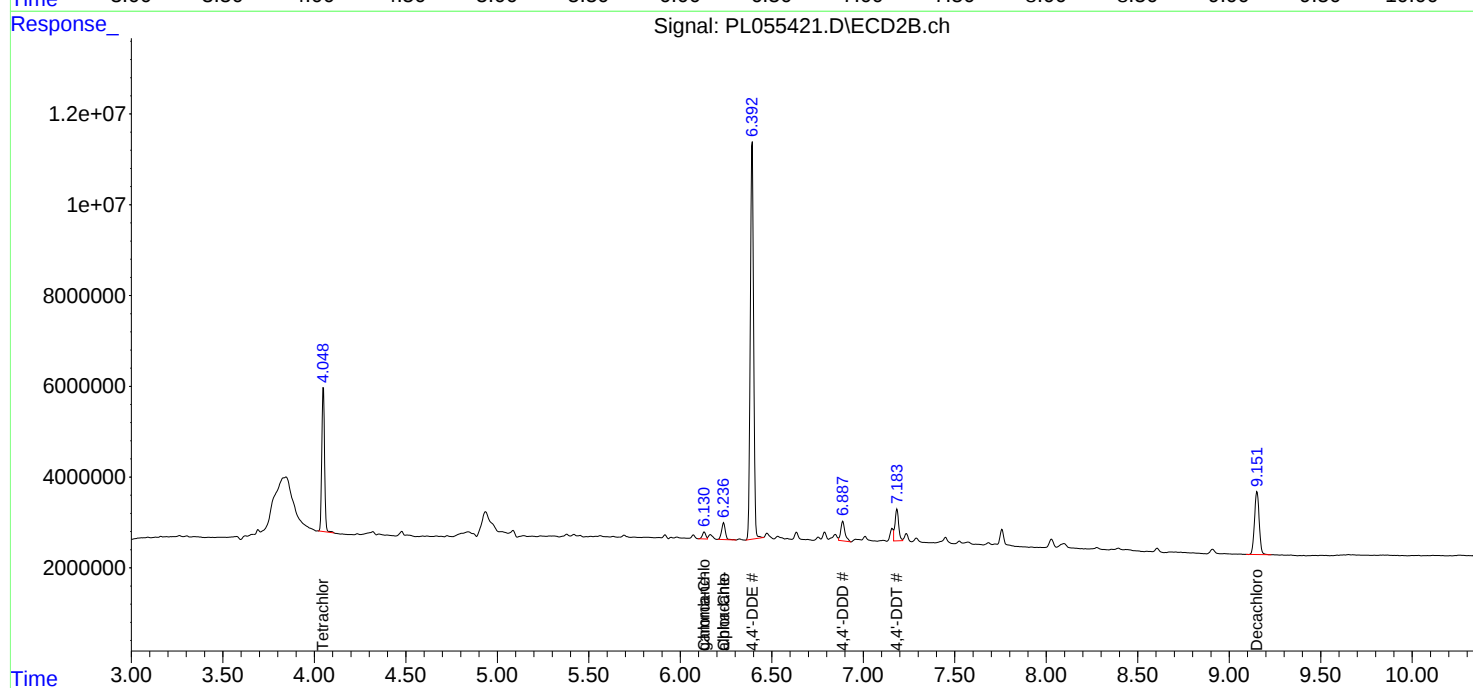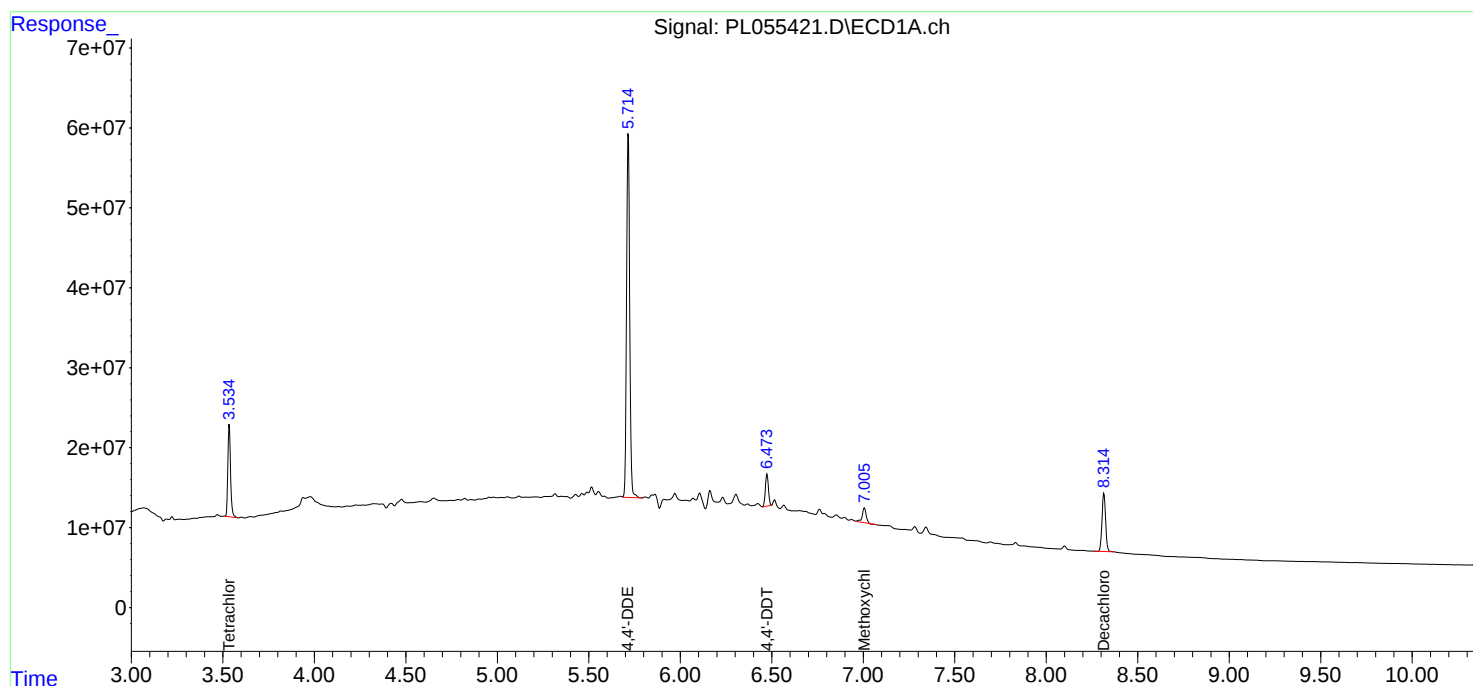


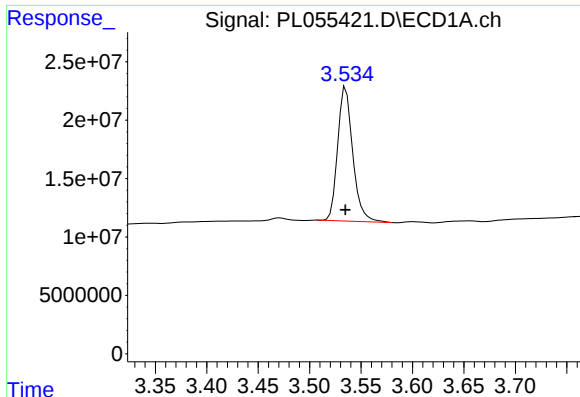

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 117019607
Conc: 11.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
MC-123019-0-2-COMP-B8

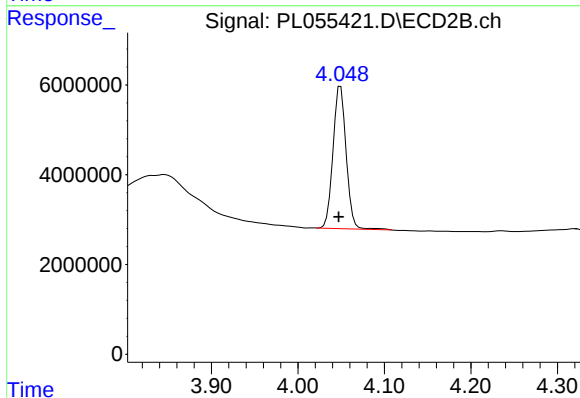


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 33397817
Conc: 12.64 ng/ml

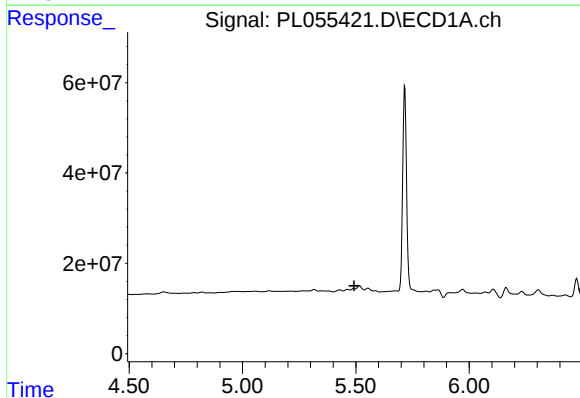


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

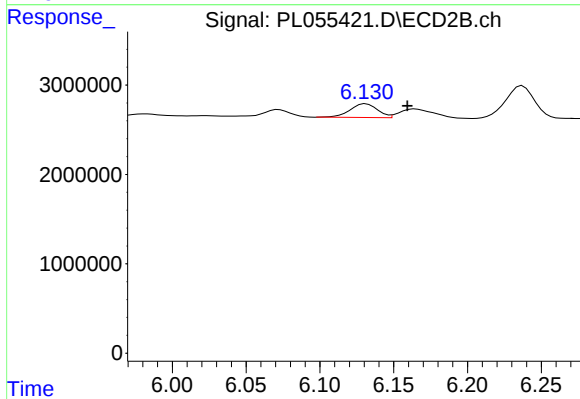

#10 gamma-Chlordane


R.T.: 6.131 min
Delta R.T.: -0.028 min
Response: 2000101
Conc: 0.75 ng/ml

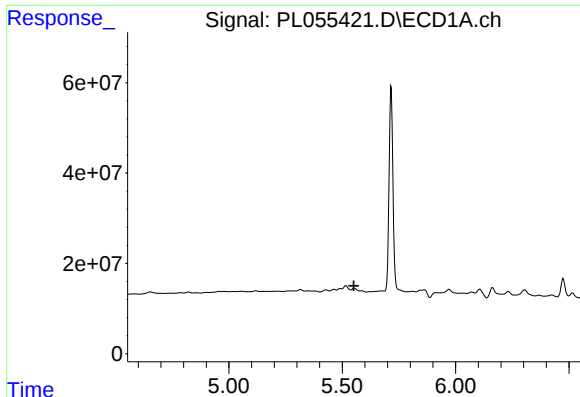

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MC-123019-0-2-COMP-B8

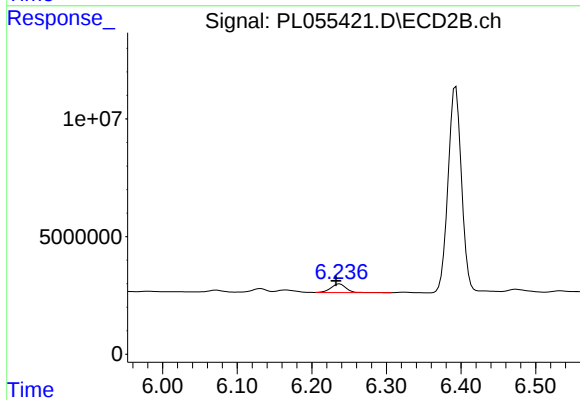


#11 alpha-Chlordane

R.T.: 6.237 min
Delta R.T.: 0.005 min
Response: 5249829
Conc: 2.00 ng/ml

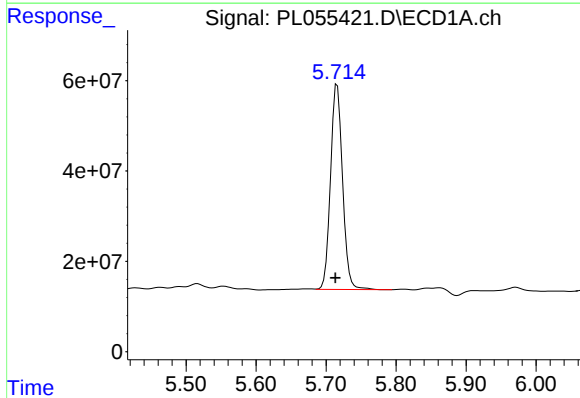


#12 4,4'-DDE

R.T.: 5.716 min
Delta R.T.: 0.003 min
Response: 542739782
Conc: 40.73 ng/ml

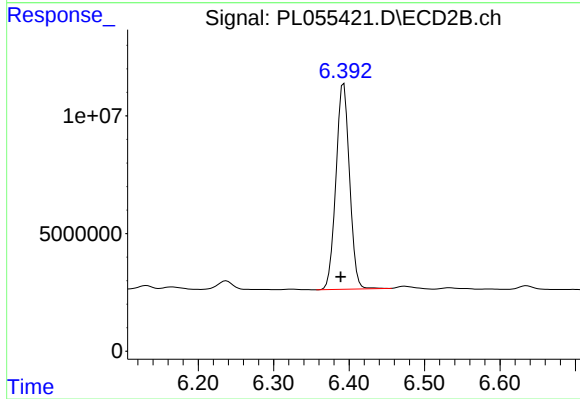

#12 4,4'-DDE


R.T.: 6.393 min
Delta R.T.: 0.004 min
Response: 109535839
Conc: 44.92 ng/ml

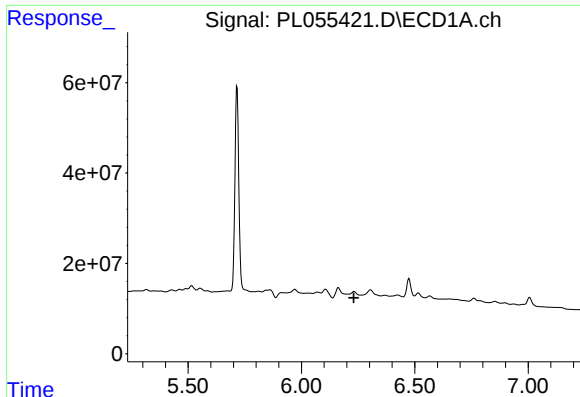

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MC-123019-0-2-COMP-B8

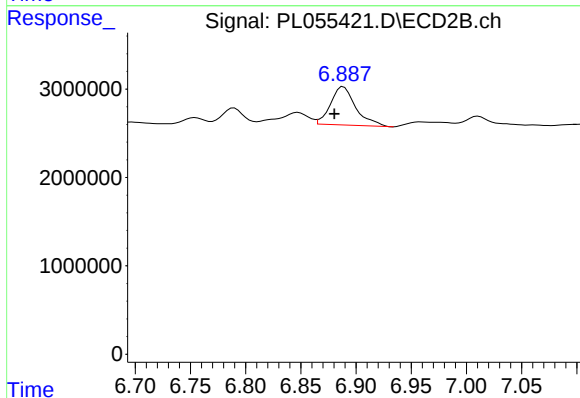


#16 4,4'-DDD

R.T.: 6.889 min
Delta R.T.: 0.008 min
Response: 6875269
Conc: 3.62 ng/ml

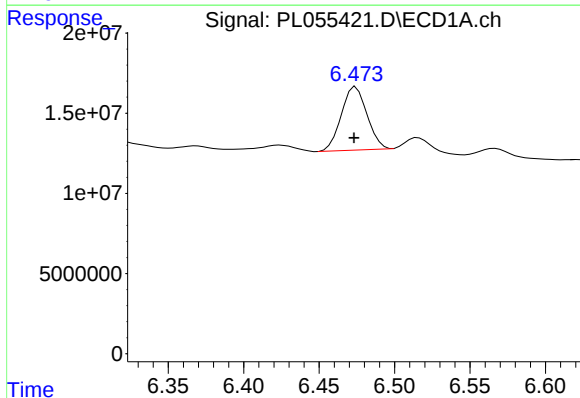


#17 4,4'-DDT

R.T.: 6.474 min
Delta R.T.: 0.001 min
Response: 46658573
Conc: 4.63 ng/ml

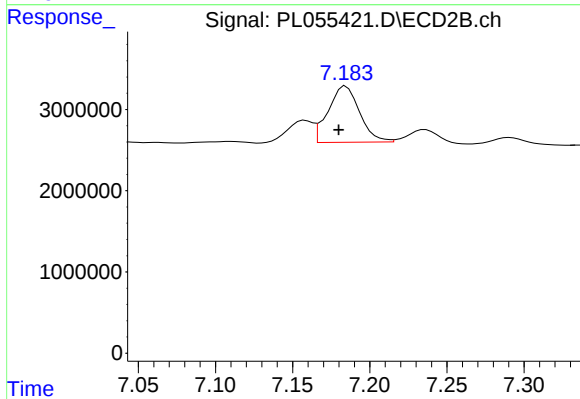

#17 4,4'-DDT


R.T.: 7.185 min
Delta R.T.: 0.005 min
Response: 9814925
Conc: 5.00 ng/ml

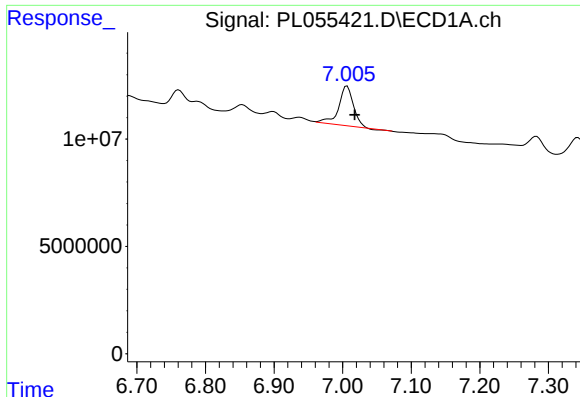

#20 Methoxychlor


R.T.: 7.006 min
Delta R.T.: -0.011 min
Response: 26881075
Conc: 5.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
MC-123019-0-2-COMP-B8

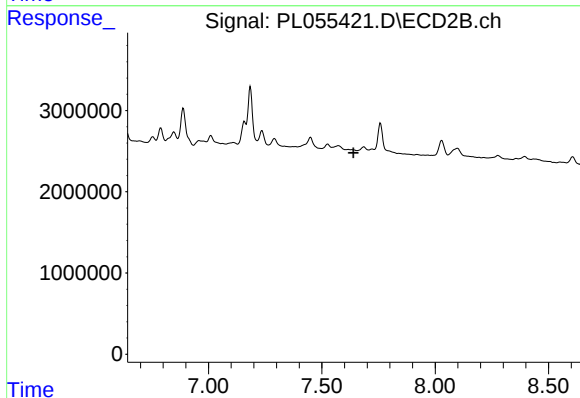


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.640 min
Response: 0
Conc: N.D.

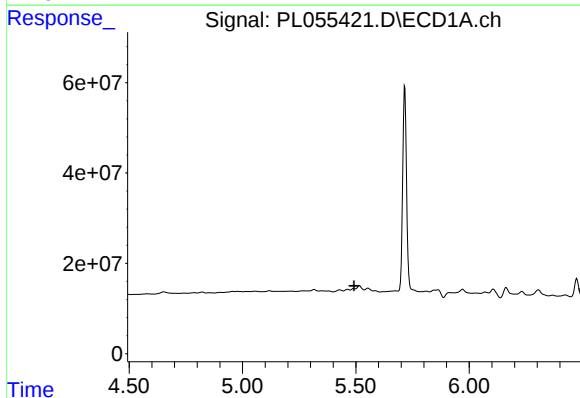


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

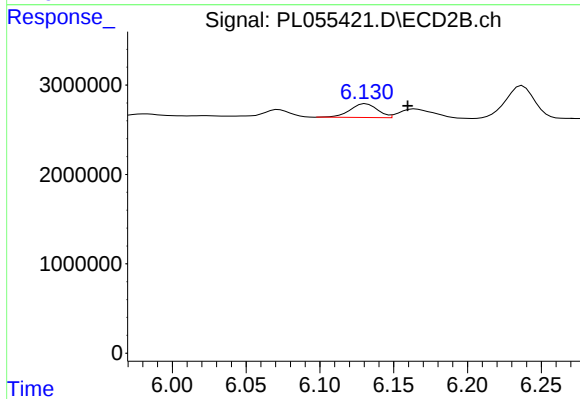

#25 Chlordane-3


R.T.: 6.131 min
Delta R.T.: -0.028 min
Response: 2000101
Conc: 6.22 ng/ml

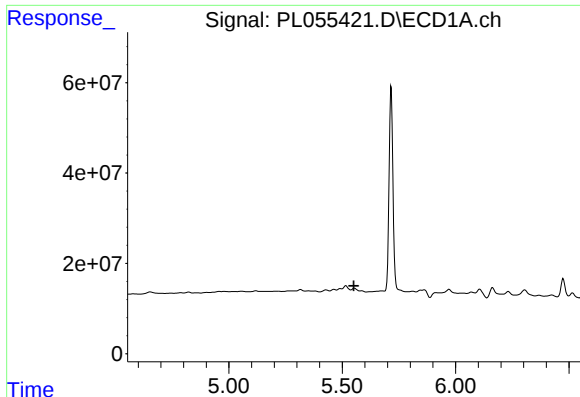

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MC-123019-0-2-COMP-B8

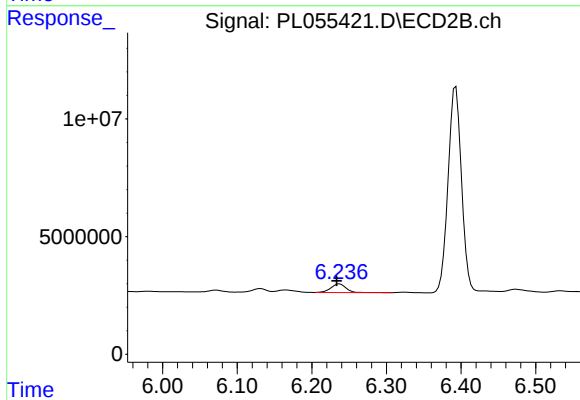


#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: 0.004 min
Response: 5249829
Conc: 13.66 ng/ml

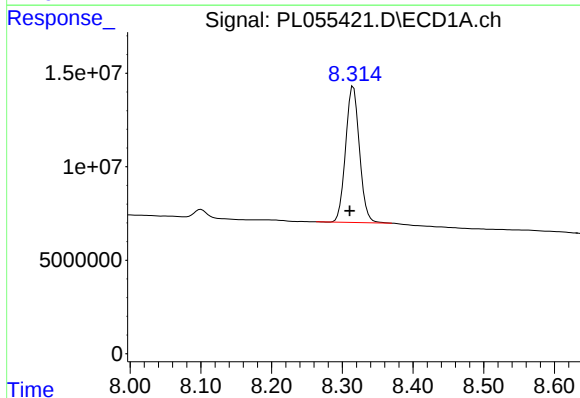

#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: 0.005 min
Response: 99165323
Conc: 10.69 ng/ml

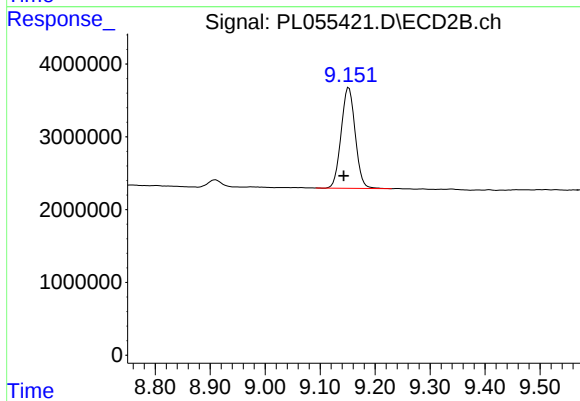

#28 Decachlorobiphenyl

R.T.: 9.152 min
Delta R.T.: 0.009 min
Response: 24581782
Conc: 11.14 ng/ml