

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123119\
 Data File : PL055445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2019 20:21
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:45:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	221.9E6	62667329	21.098	23.717
28)	SA Decachlor...	8.314	9.151	191.4E6	47211686	20.627	21.387
Target Compounds							
8)	B Heptachlo...	0.000	5.923	0	10081769	N.D.	3.955 #
14)	MA Endrin	0.000	6.760	0	5425120	N.D.	2.528 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123119\
Data File : PL055445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2019 20:21
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:45:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

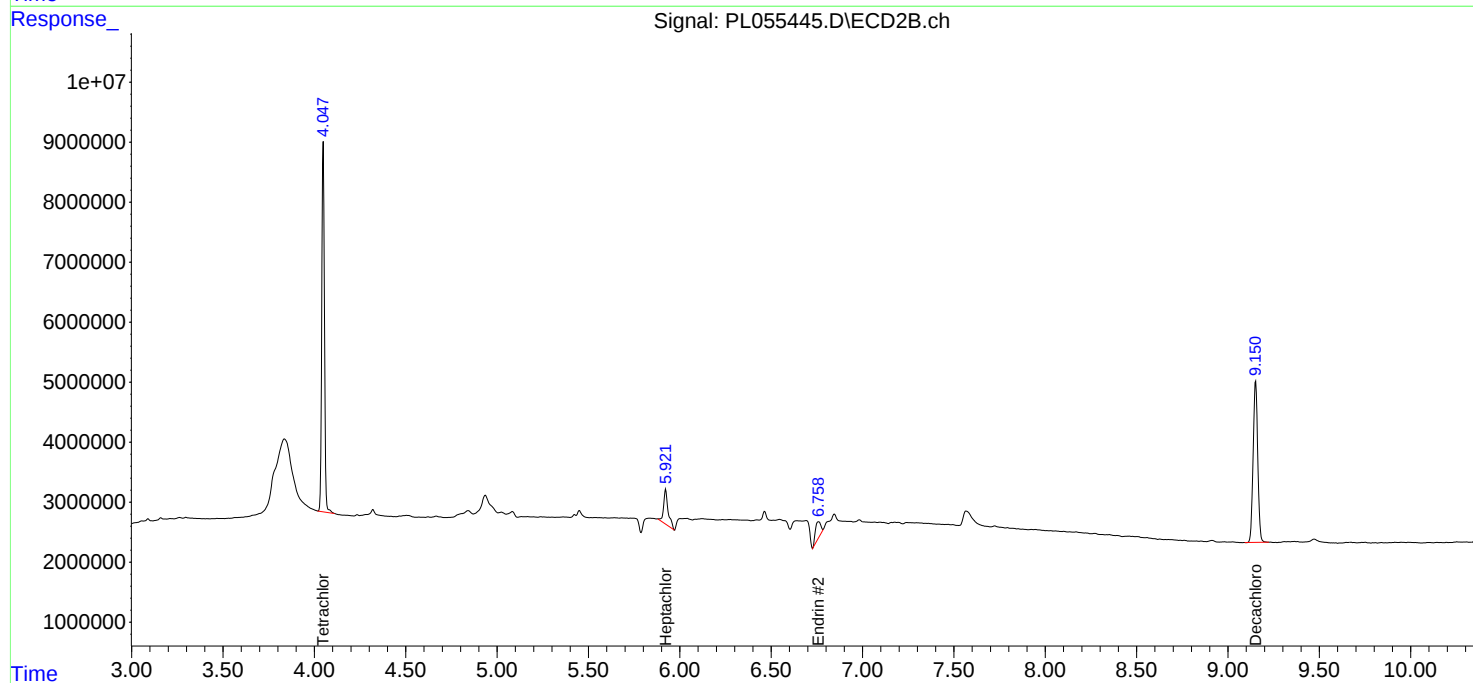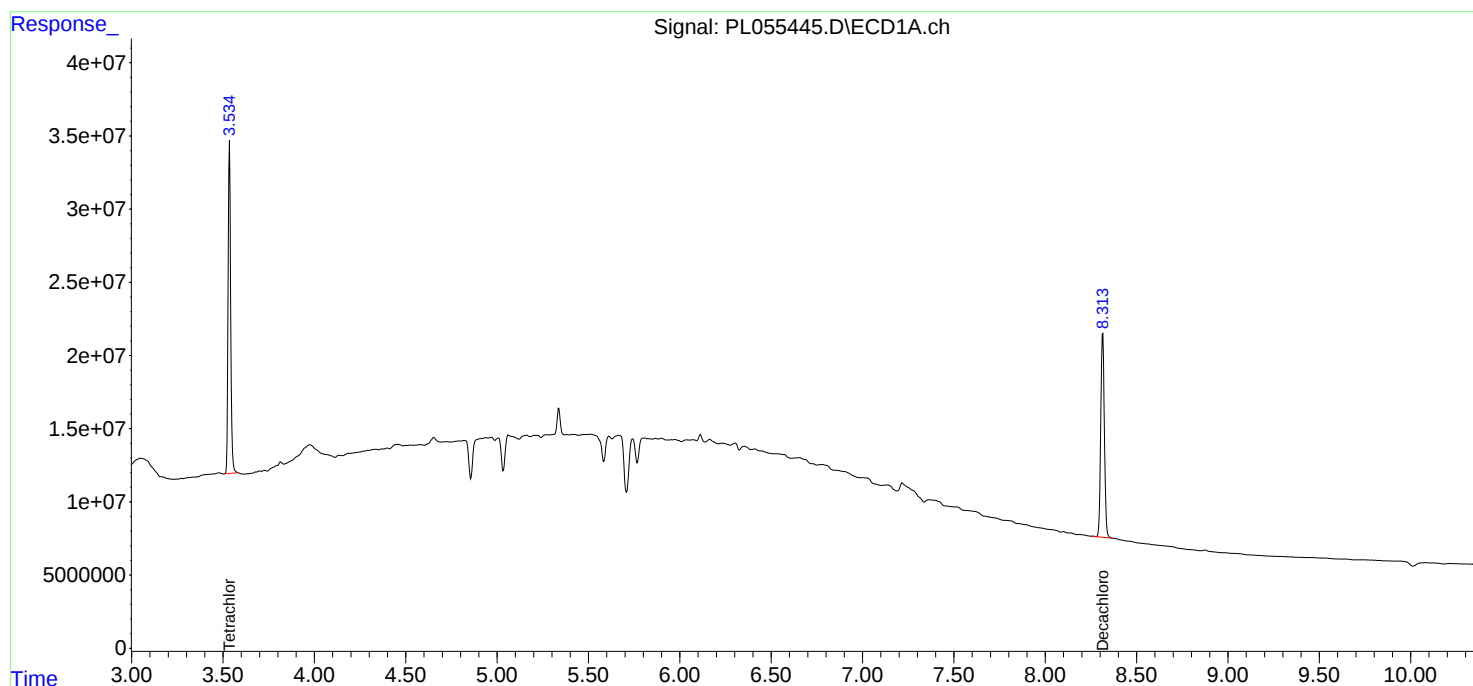


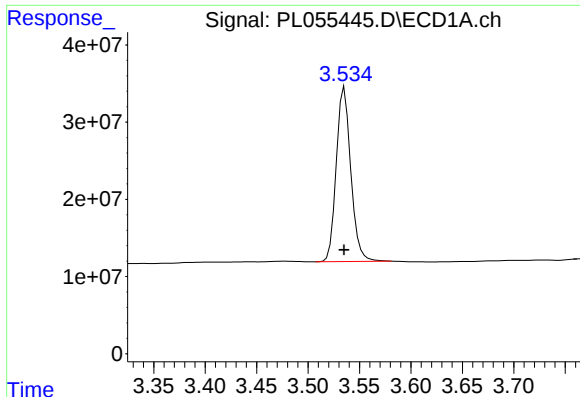

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 221874621
Conc: 21.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

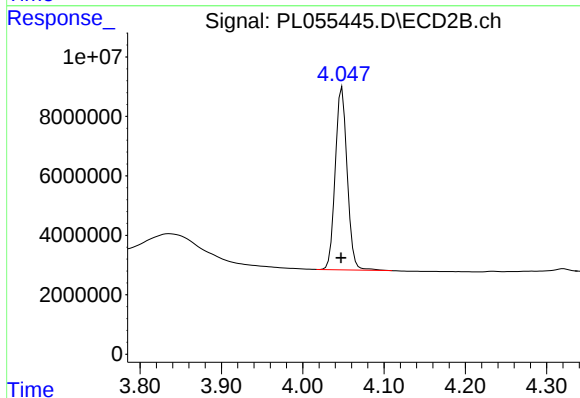


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.001 min
Response: 62667329
Conc: 23.72 ng/ml

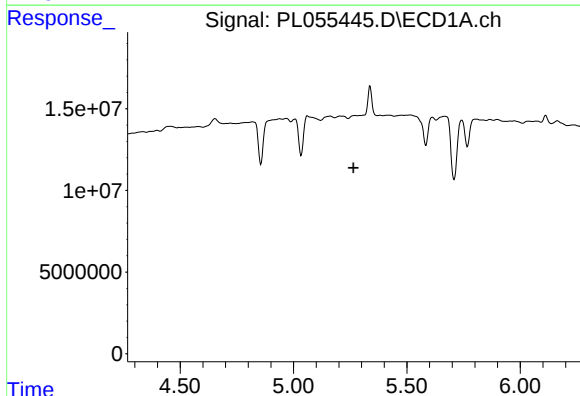


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

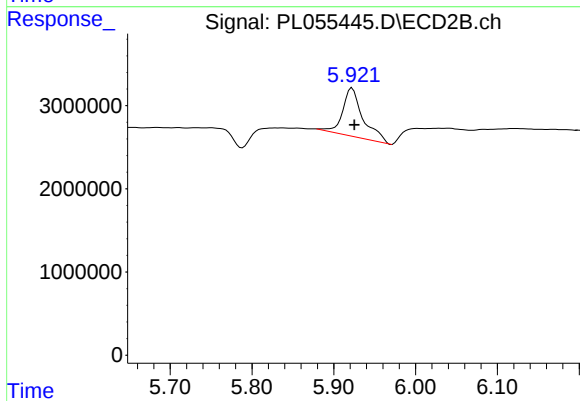

#8 Heptachlor epoxide


R.T.: 5.923 min
Delta R.T.: -0.003 min
Response: 10081769
Conc: 3.96 ng/ml

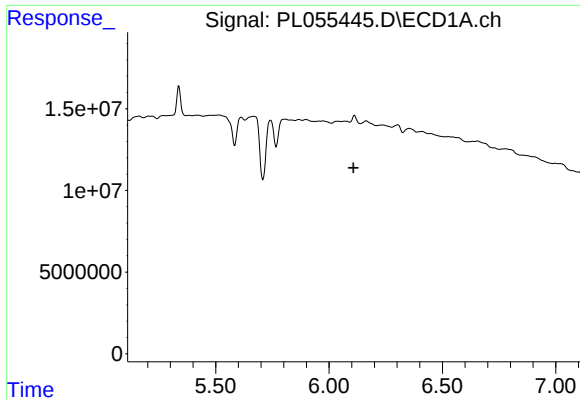

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

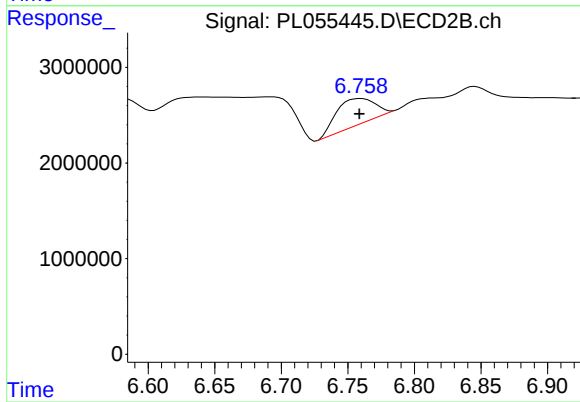


#14 Endrin

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 5425120
Conc: 2.53 ng/ml

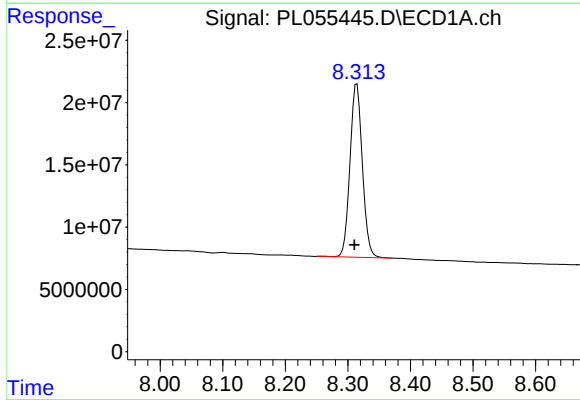

#28 Decachlorobiphenyl

R.T.: 8.314 min
Delta R.T.: 0.004 min
Response: 191389297
Conc: 20.63 ng/ml

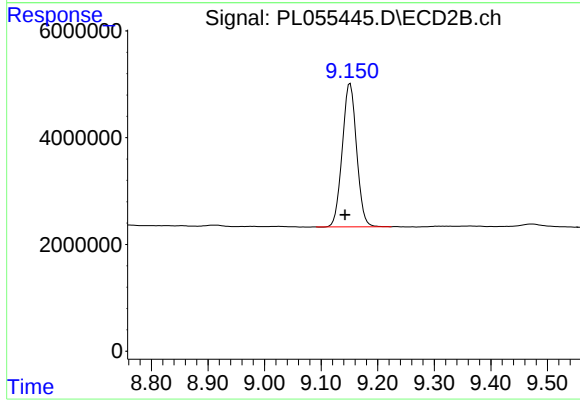

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.009 min
Response: 47211686
Conc: 21.39 ng/ml