

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
 Data File : PL063881.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 12:52
 Operator : AR\AJ
 Sample : L5244-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 17:11:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.111	6964468	5462556	2.323	2.140
28)	SA Decachlor...	8.185	9.271	6560381	4709698	2.381	2.389
Target Compounds							
9)	A Endosulfan I	5.499f	0.000	3634675	0	1.050	N.D. #
10)	B gamma-Chl...	5.376	6.254	6257053	4753118	1.646	1.718
11)	B alpha-Chl...	5.433	6.329	6180870	5560969	1.648	2.015
19)	B Endosulfa...	6.660f	0.000	1996343	0	0.634	N.D. #
25)	Chlordane-3	5.376	6.254	6257053	4753118	19.148	13.872 #
26)	Chlordane-4	5.433	6.329	6180870	5560969	23.101	13.529 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
Data File : PL063881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 12:52
Operator : AR\AJ
Sample : L5244-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 17:11:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

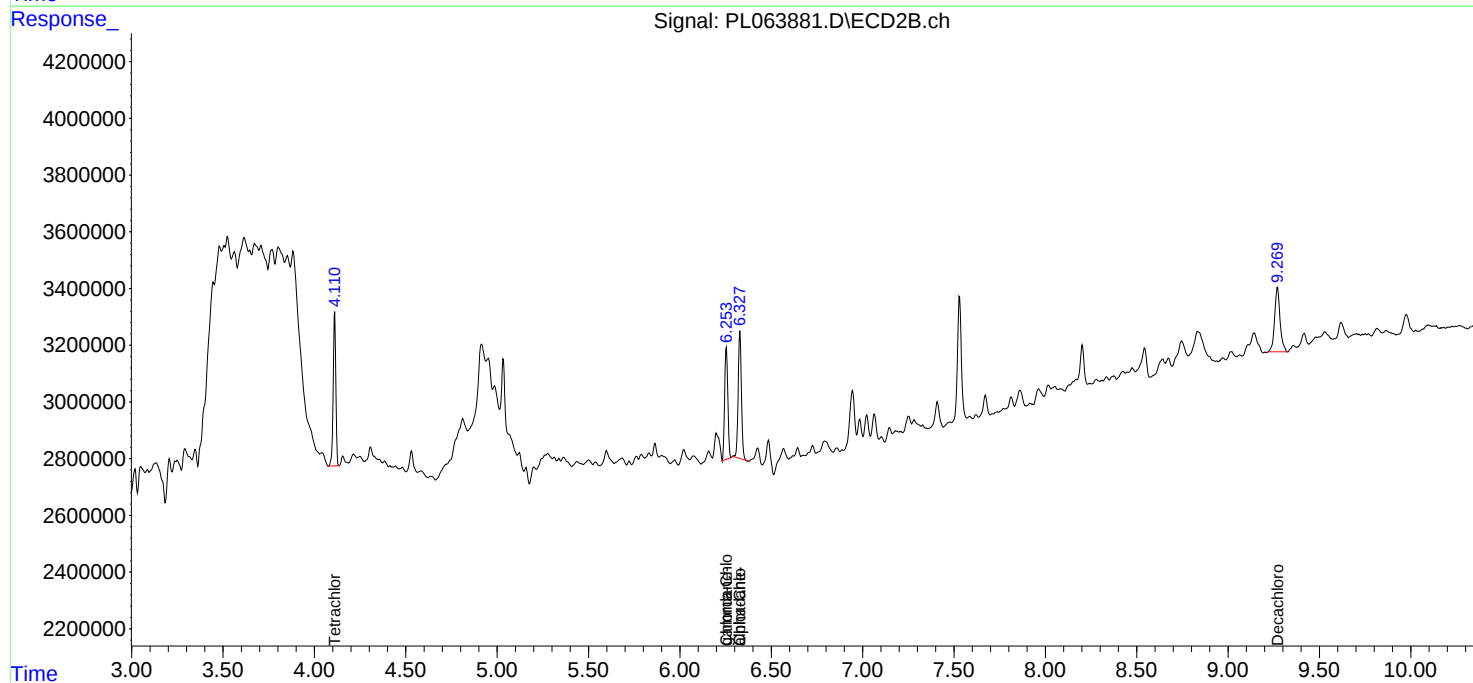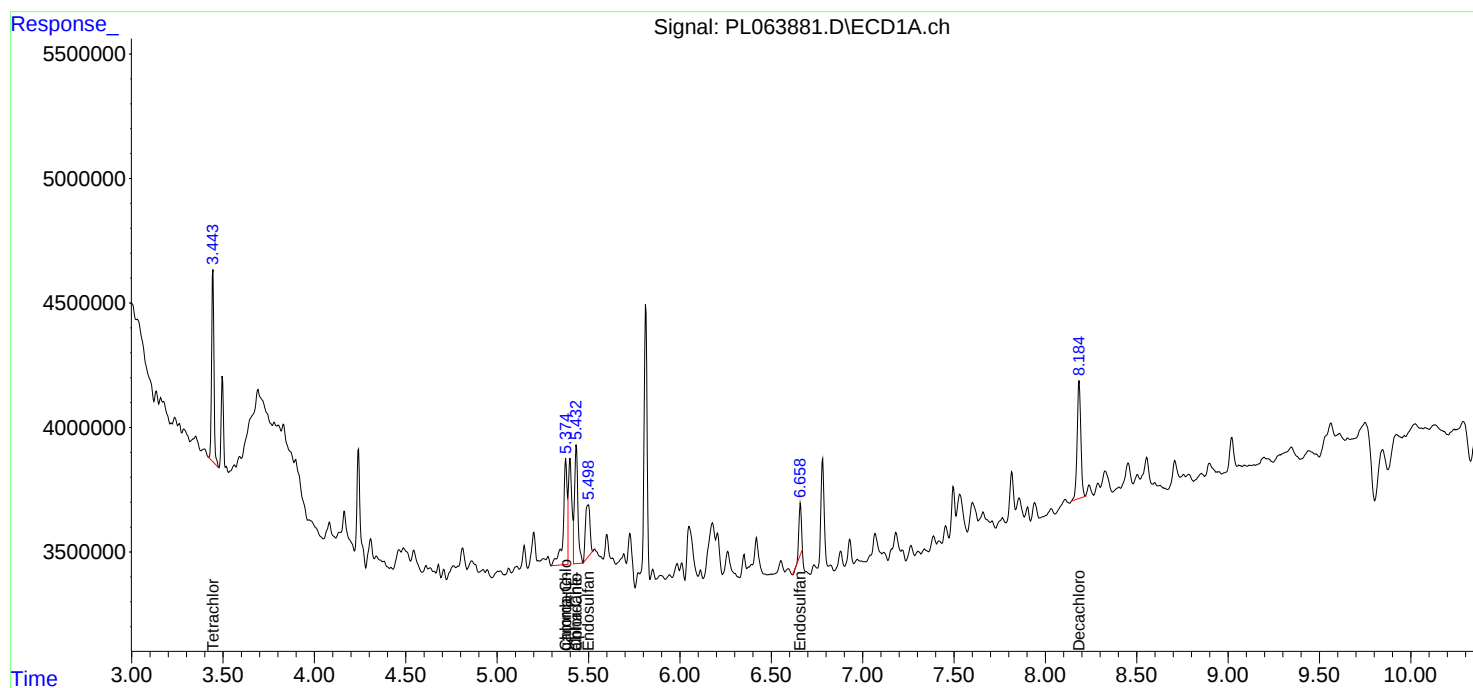


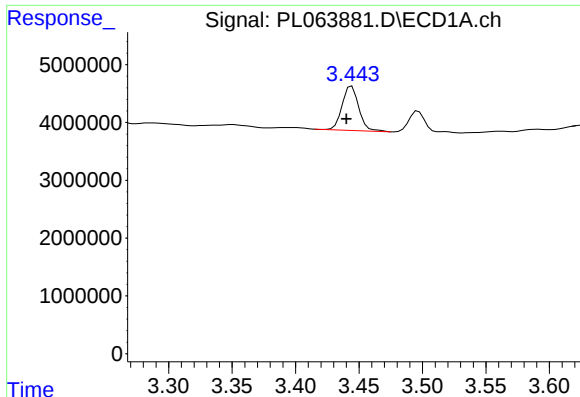

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.004 min
Response: 6964468
Conc: 2.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

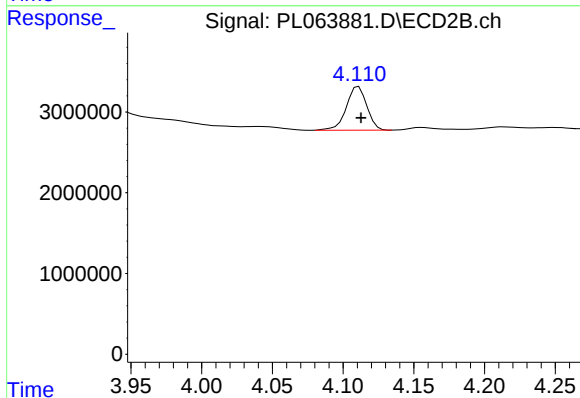


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 5462556
Conc: 2.14 ng/ml

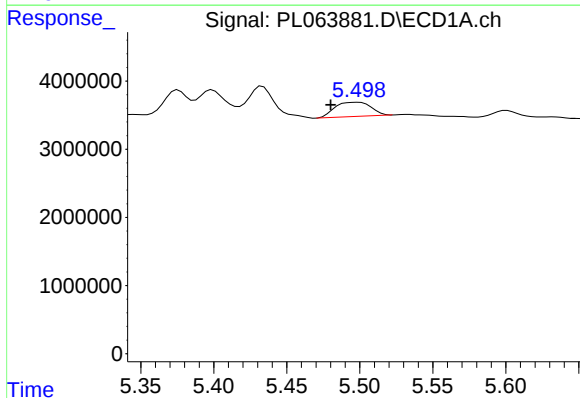


#9 Endosulfan I

R.T.: 5.499 min
Delta R.T.: 0.019 min
Response: 3634675
Conc: 1.05 ng/ml

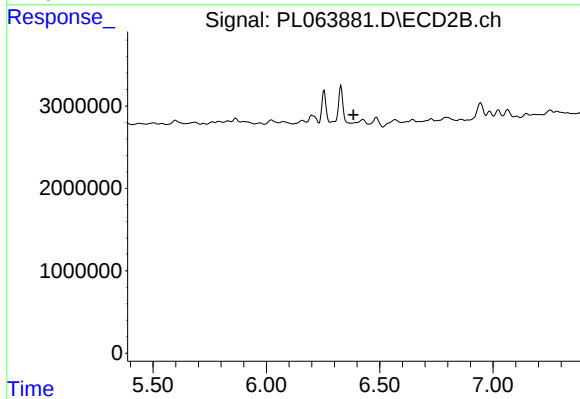

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

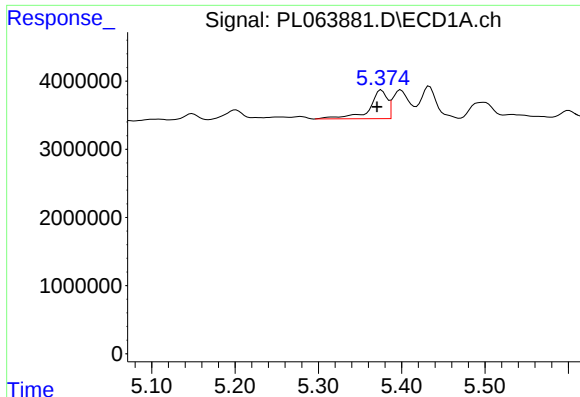

#10 gamma-Chlordane


R.T.: 5.376 min
Delta R.T.: 0.005 min
Response: 6257053
Conc: 1.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

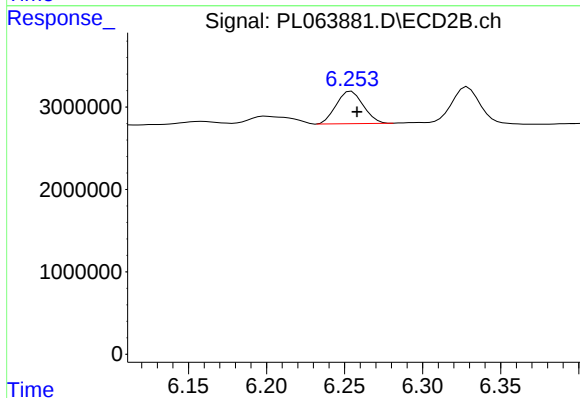


#10 gamma-Chlordane

R.T.: 6.254 min
Delta R.T.: -0.003 min
Response: 4753118
Conc: 1.72 ng/ml

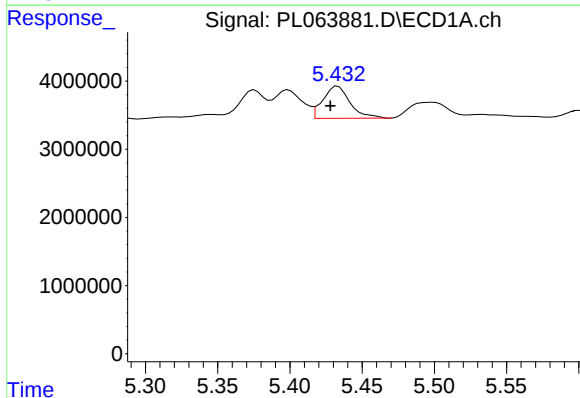


#11 alpha-Chlordane

R.T.: 5.433 min
Delta R.T.: 0.005 min
Response: 6180870
Conc: 1.65 ng/ml

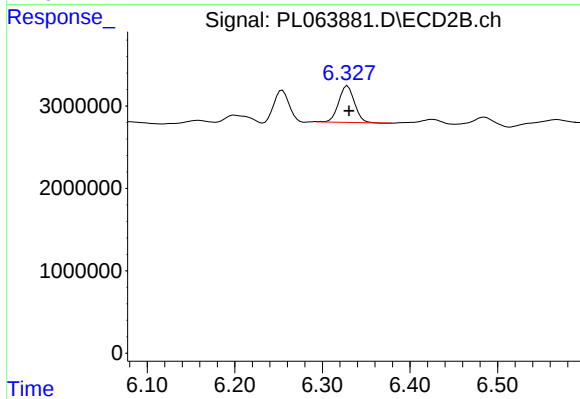

#11 alpha-Chlordane


R.T.: 6.329 min
Delta R.T.: -0.002 min
Response: 5560969
Conc: 2.01 ng/ml

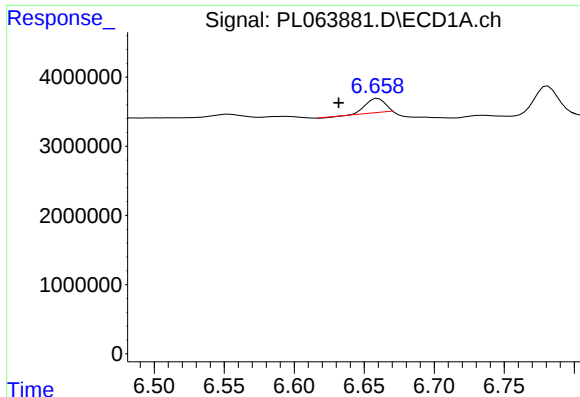

#19 Endosulfan Sulfate


R.T.: 6.660 min
Delta R.T.: 0.028 min
Response: 1996343
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

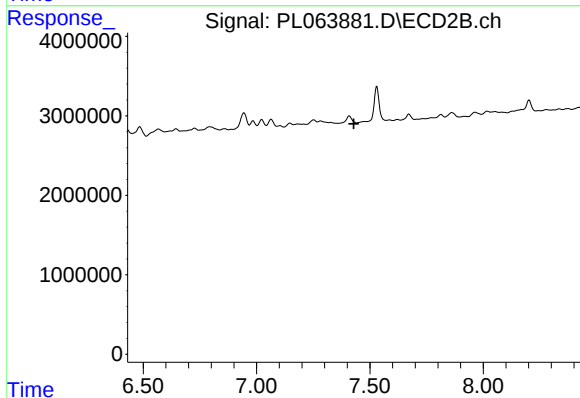


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

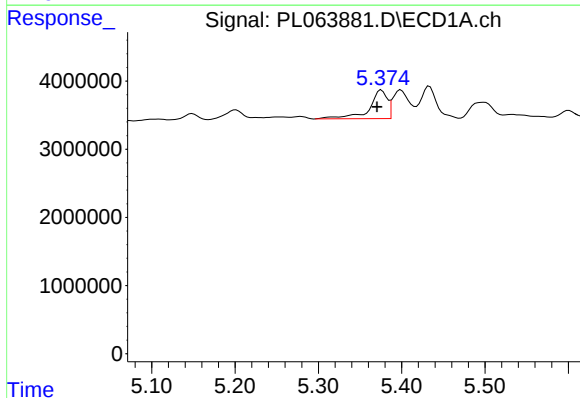


#25 Chlordane-3

R.T.: 5.376 min
Delta R.T.: 0.005 min
Response: 6257053
Conc: 19.15 ng/ml

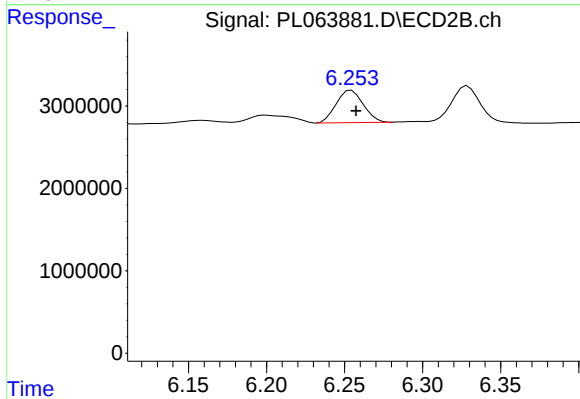

#25 Chlordane-3


R.T.: 6.254 min
Delta R.T.: -0.003 min
Response: 4753118
Conc: 13.87 ng/ml

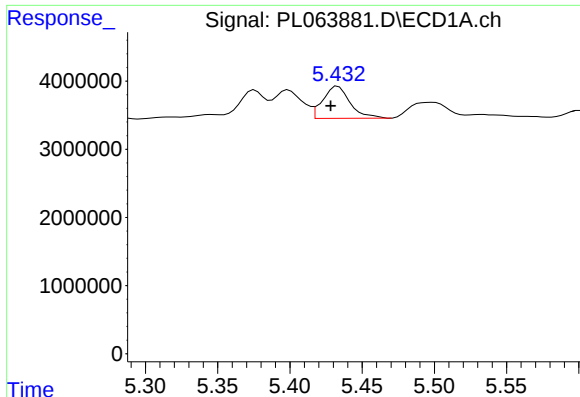

#26 Chlordane-4


R.T.: 5.433 min
Delta R.T.: 0.005 min
Response: 6180870
Conc: 23.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

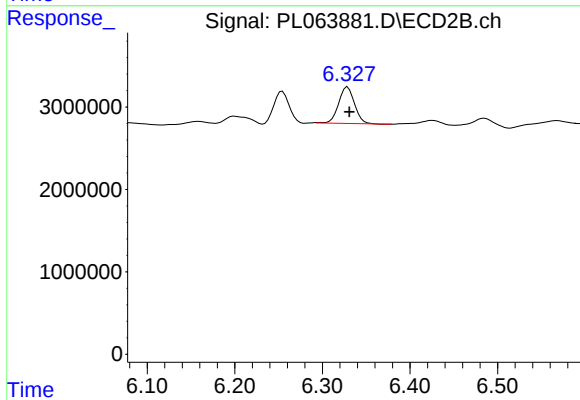


#26 Chlordane-4

R.T.: 6.329 min
Delta R.T.: -0.002 min
Response: 5560969
Conc: 13.53 ng/ml

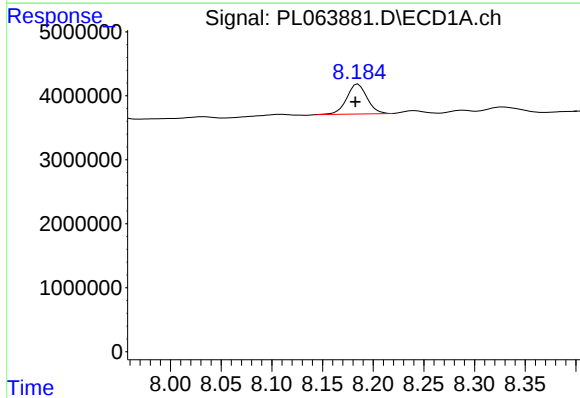

#28 Decachlorobiphenyl

R.T.: 8.185 min
Delta R.T.: 0.003 min
Response: 6560381
Conc: 2.38 ng/ml

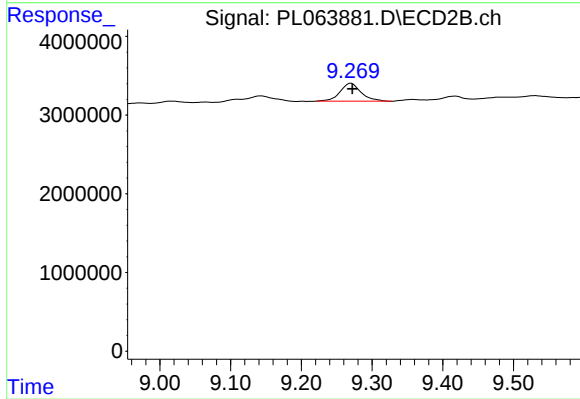

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: -0.002 min
Response: 4709698
Conc: 2.39 ng/ml