

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
 Data File : PL063890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 16:27
 Operator : AR\AJ
 Sample : L5241-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:34:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.110	69027140	52472732	23.025	20.553
28)	SA Decachlor...	8.174	9.264	47661368	29882175	17.299	15.156
Target Compounds							
11)	B alpha-Chl...	5.413	0.000	12738898	0	3.396	N.D. #
15)	B Endosulfa...	6.253	0.000	2611608	0	0.792	N.D. #
26)	Chlordane-4	5.413f	0.000	12738898	0	47.611	N.D. #
27)	Chlordane-5	6.253	0.000	2611608	0	24.285	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
Data File : PL063890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 16:27
Operator : AR\AJ
Sample : L5241-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:34:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

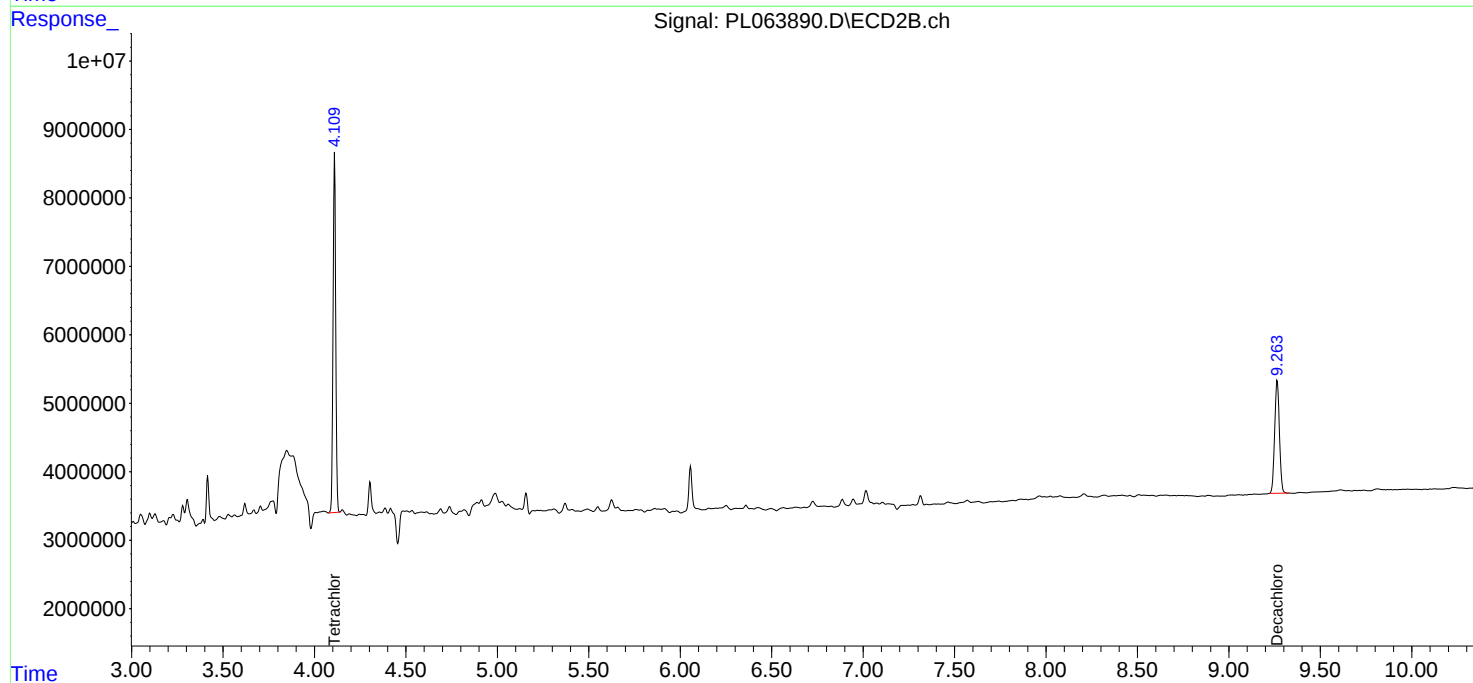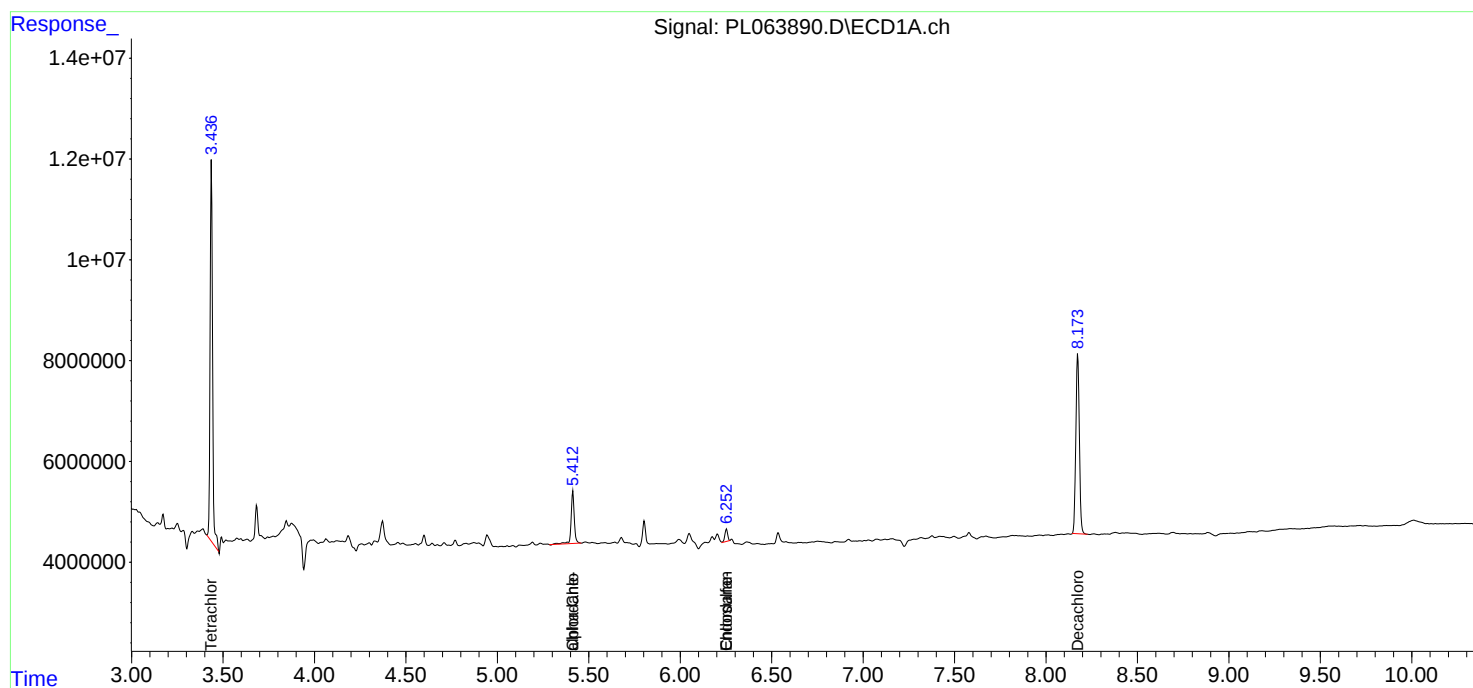


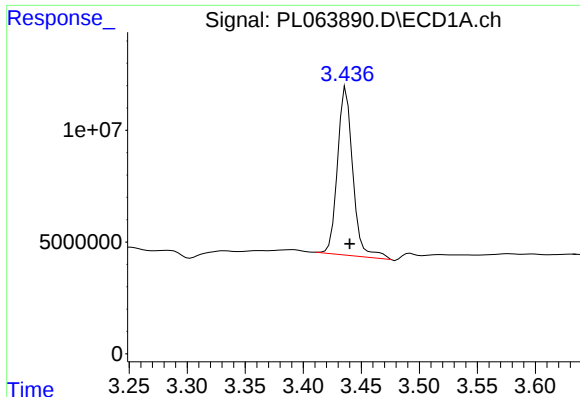

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: -0.003 min
Response: 69027140
Conc: 23.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

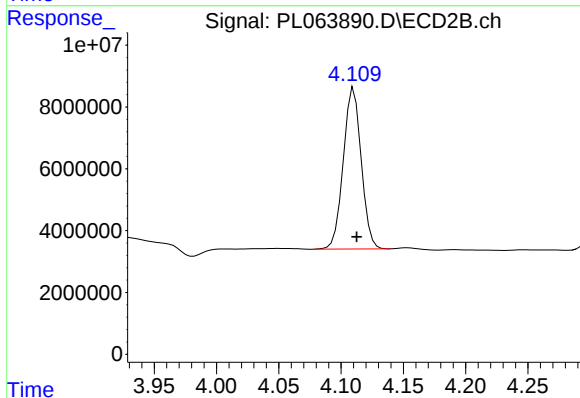


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.002 min
Response: 52472732
Conc: 20.55 ng/ml

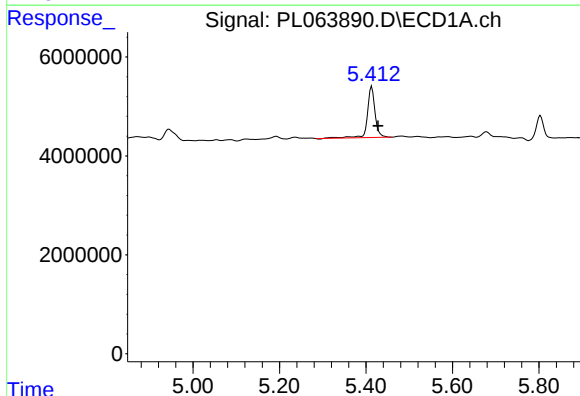


#11 alpha-Chlordane

R.T.: 5.413 min
Delta R.T.: -0.015 min
Response: 12738898
Conc: 3.40 ng/ml

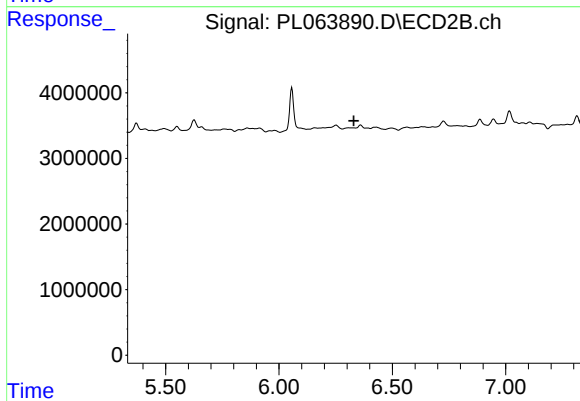

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.331 min
Response: 0
Conc: N.D.

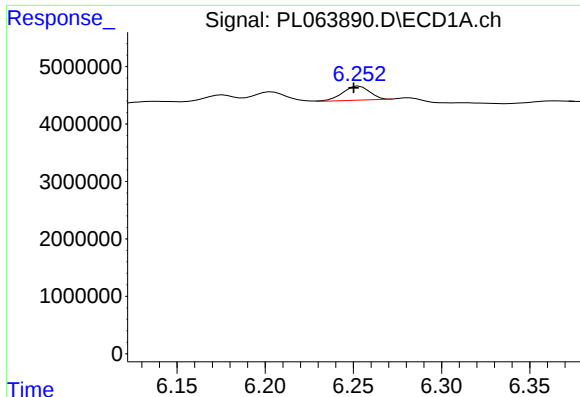

#15 Endosulfan II


R.T.: 6.253 min
Delta R.T.: 0.003 min
Response: 2611608
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

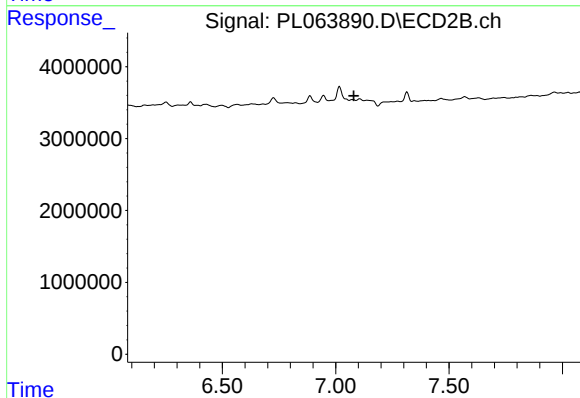


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.080 min
Response: 0
Conc: N.D.

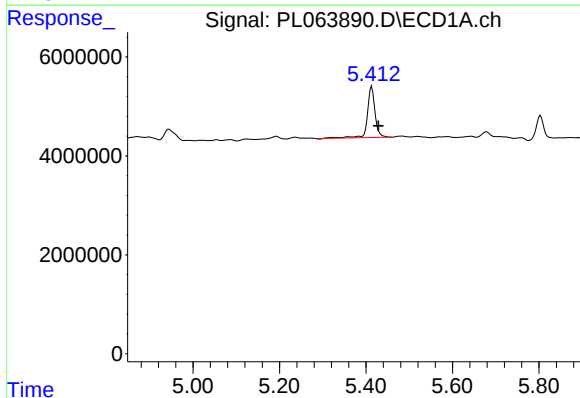


#26 Chlordane-4

R.T.: 5.413 min
Delta R.T.: -0.015 min
Response: 12738898
Conc: 47.61 ng/ml

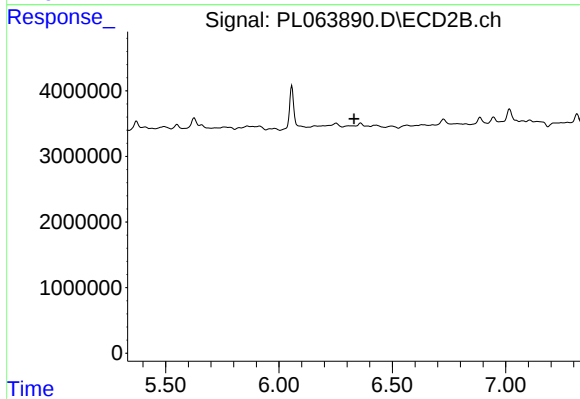

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

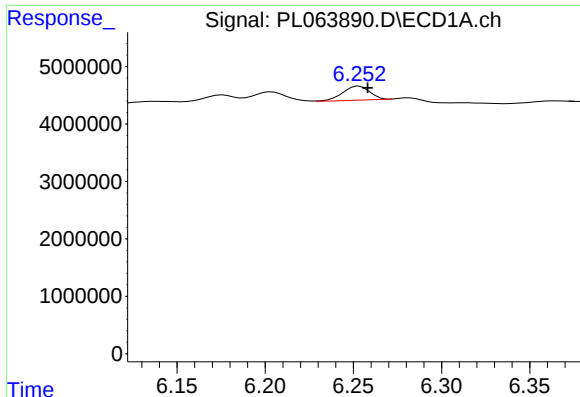

#27 Chlordane-5


R.T.: 6.253 min
Delta R.T.: -0.005 min
Response: 2611608
Conc: 24.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

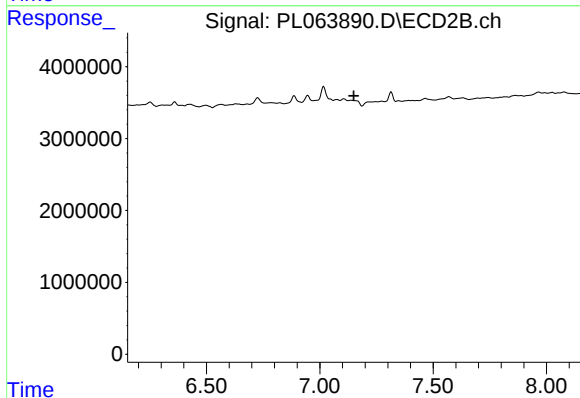


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.150 min
Response: 0
Conc: N.D.

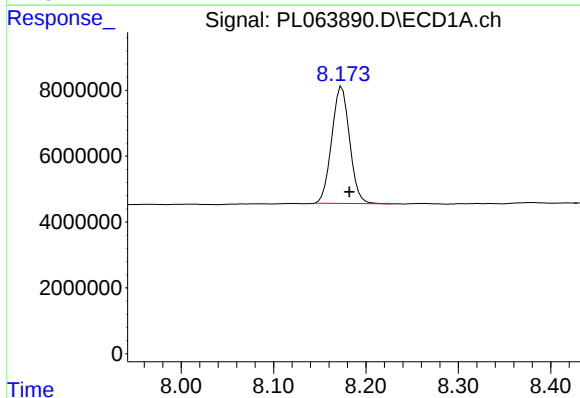

#28 Decachlorobiphenyl

R.T.: 8.174 min
Delta R.T.: -0.008 min
Response: 47661368
Conc: 17.30 ng/ml

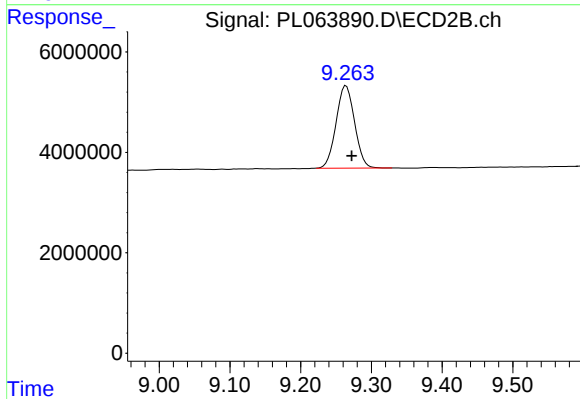

#28 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.008 min
Response: 29882175
Conc: 15.16 ng/ml