

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
 Data File : PL063893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 17:10
 Operator : AR\AJ
 Sample : L5241-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:35:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.111	67153986	50429050	22.400	19.753
28)	SA Decachlor...	8.174	9.265	40781723	25813964	14.802	13.093
Target Compounds							
3)	MA gamma-BHC...	0.000	4.800	0	4238598	N.D.	1.243 #
11)	B alpha-Chl...	5.414	0.000	14573745	0	3.885	N.D. #
14)	MA Endrin	0.000	6.888f	0	3381948	N.D.	1.743 #
20)	A Methoxychlor	6.923f	0.000	4822004	0	3.670	N.D. #
26)	Chlordane-4	5.414	0.000	14573745	0	54.469	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
Data File : PL063893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 17:10
Operator : AR\AJ
Sample : L5241-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:35:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

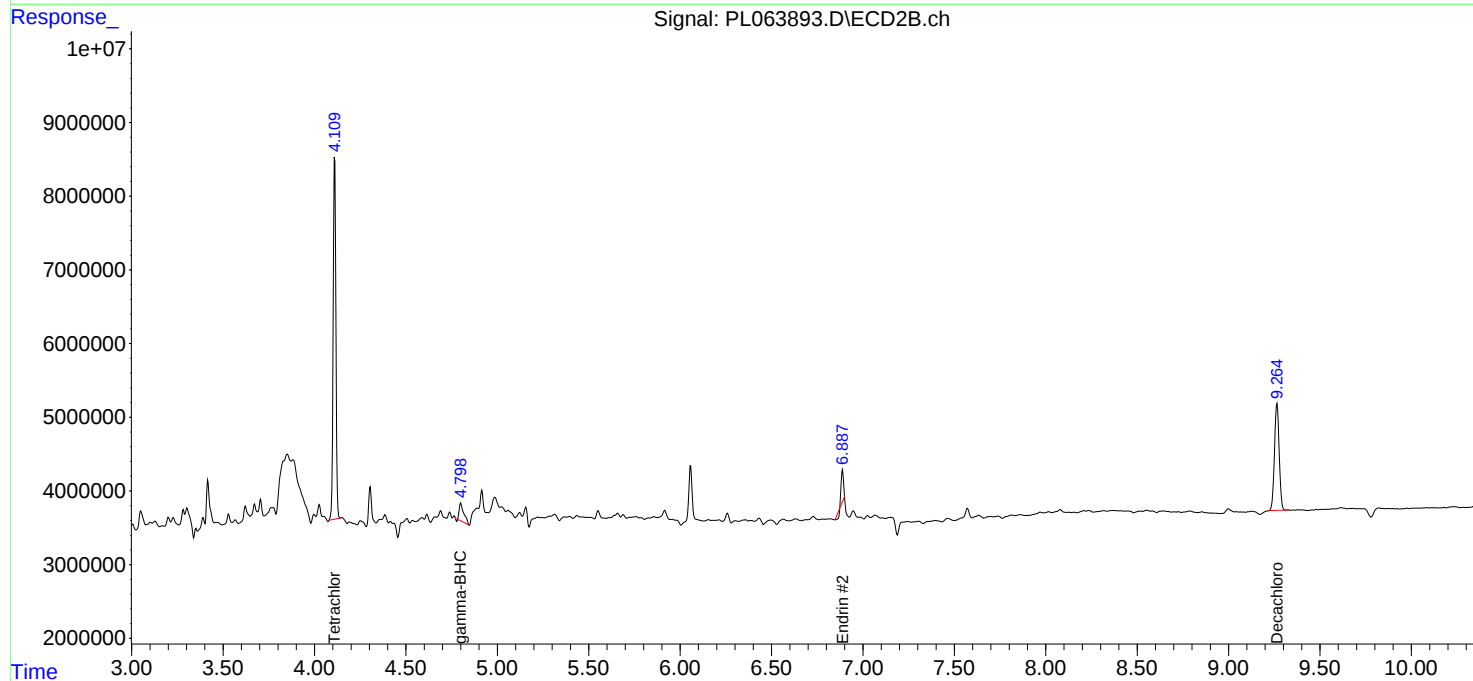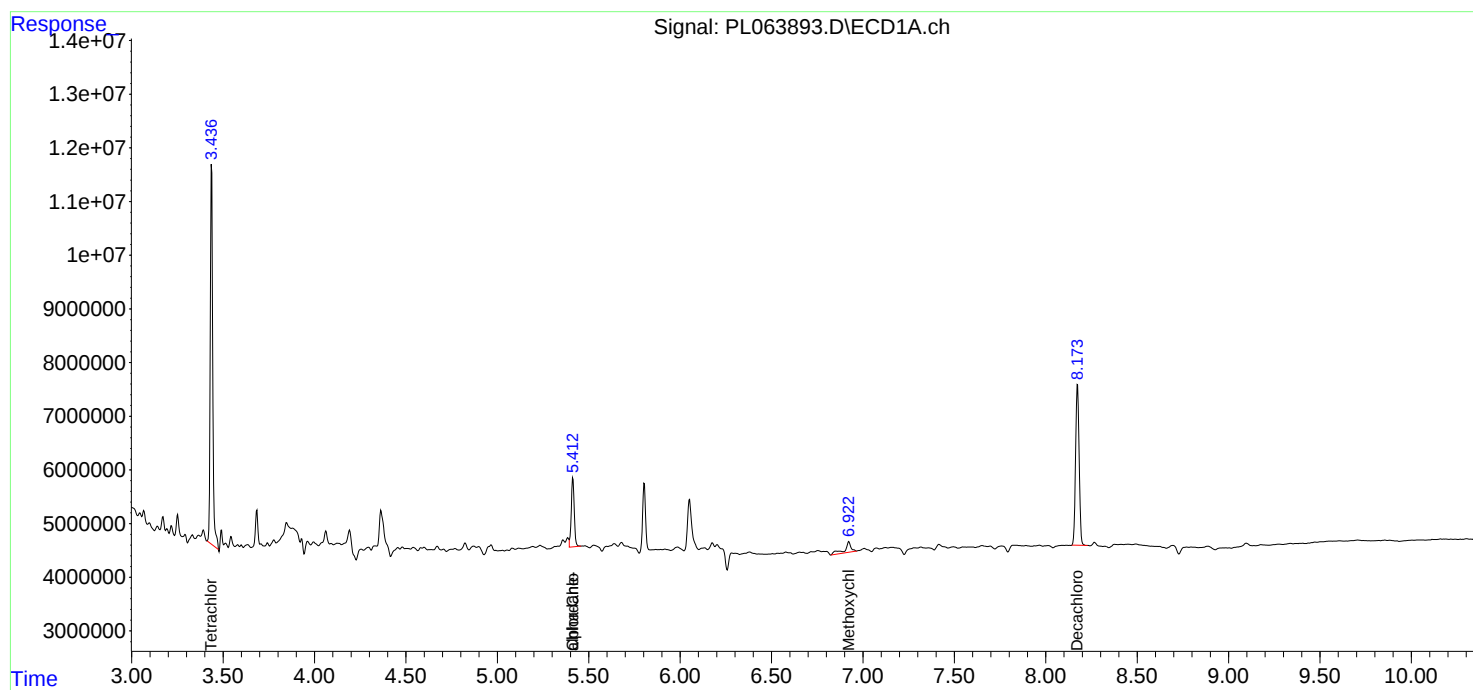


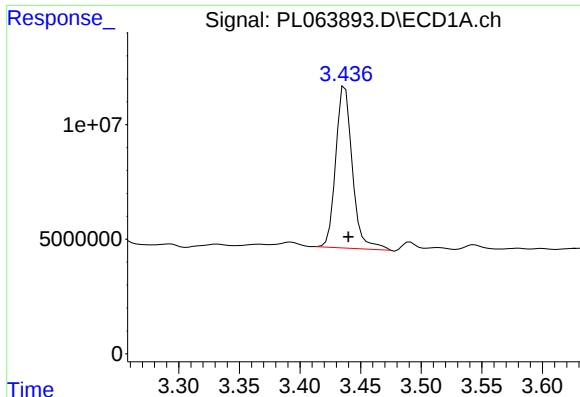

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: -0.003 min
Response: 67153986
Conc: 22.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

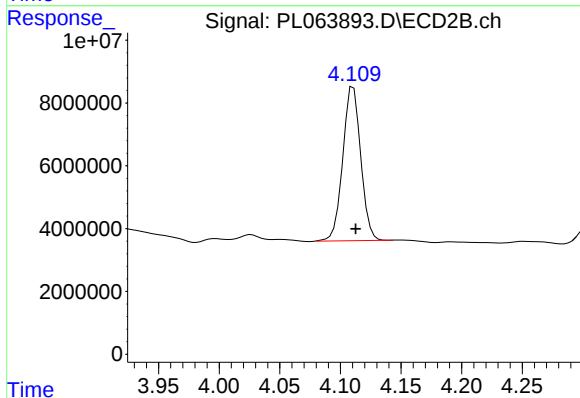


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 50429050
Conc: 19.75 ng/ml

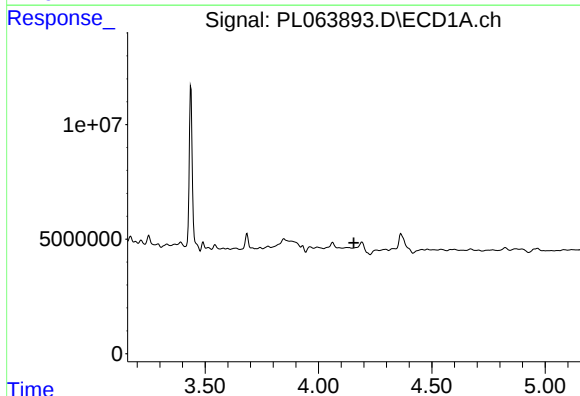


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

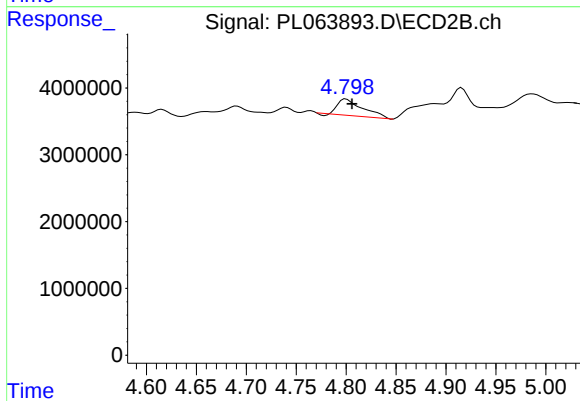

#3 gamma-BHC (Lindane)


R.T.: 4.800 min
Delta R.T.: -0.006 min
Response: 4238598
Conc: 1.24 ng/ml

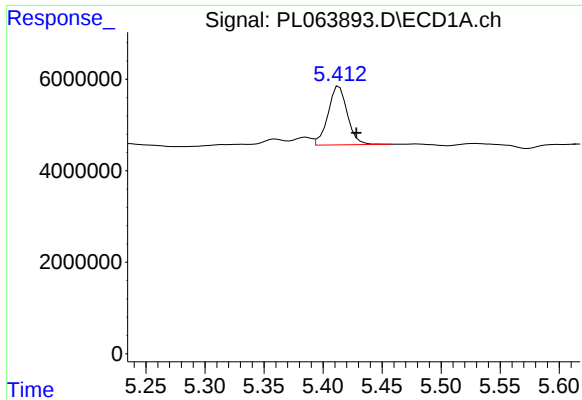

#11 alpha-Chlordane


R.T.: 5.414 min
Delta R.T.: -0.014 min
Response: 14573745
Conc: 3.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

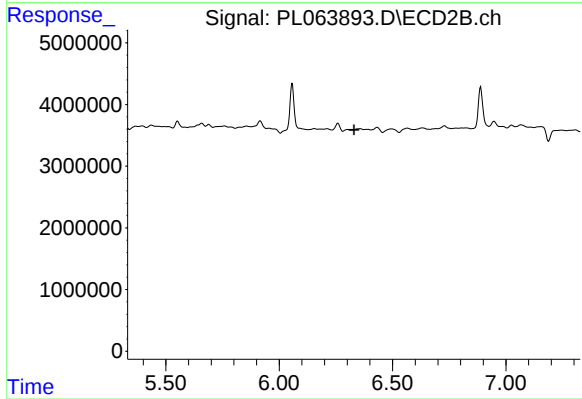


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

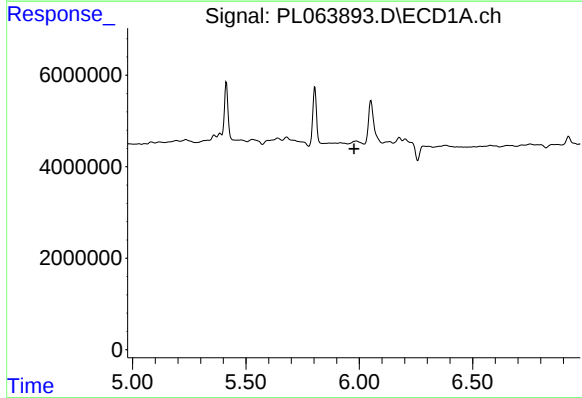


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

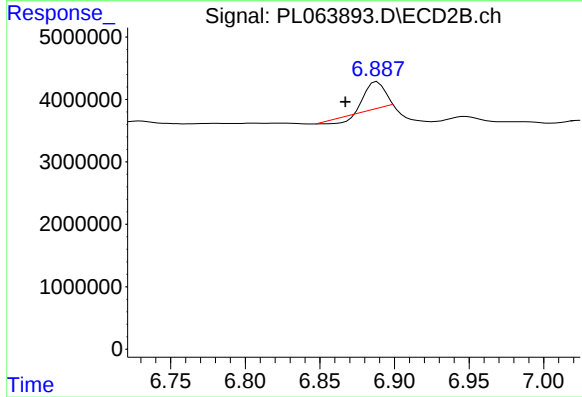

#14 Endrin


R.T.: 6.888 min
Delta R.T.: 0.021 min
Response: 3381948
Conc: 1.74 ng/ml

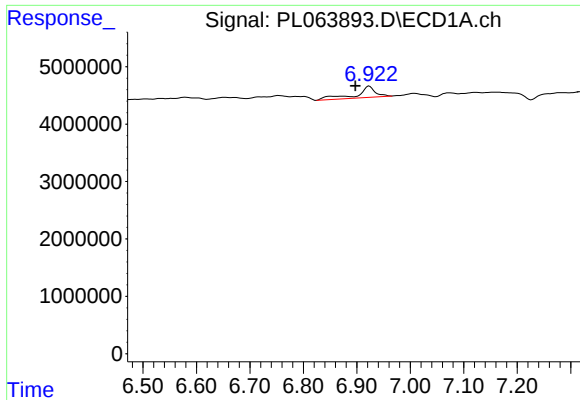

#20 Methoxychlor


R.T.: 6.923 min
Delta R.T.: 0.026 min
Response: 4822004
Conc: 3.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

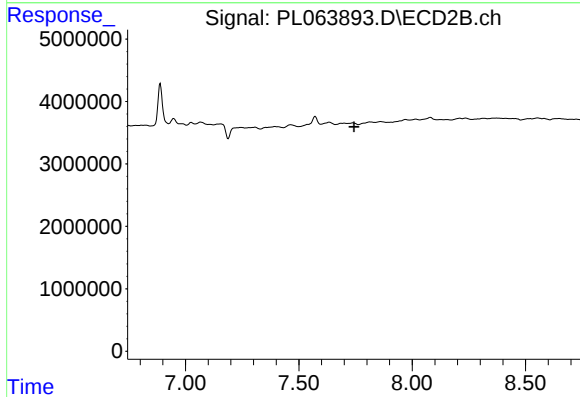


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.743 min
Response: 0
Conc: N.D.

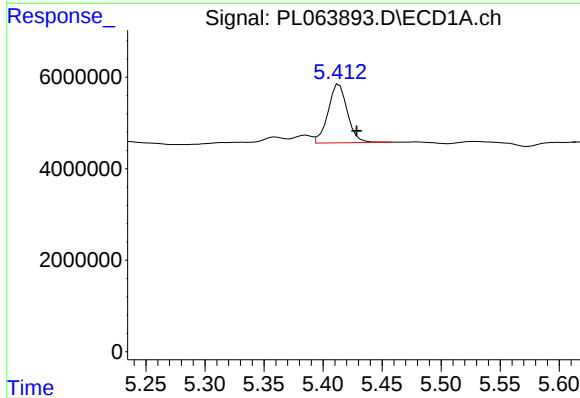


#26 Chlordane-4

R.T.: 5.414 min
Delta R.T.: -0.015 min
Response: 14573745
Conc: 54.47 ng/ml

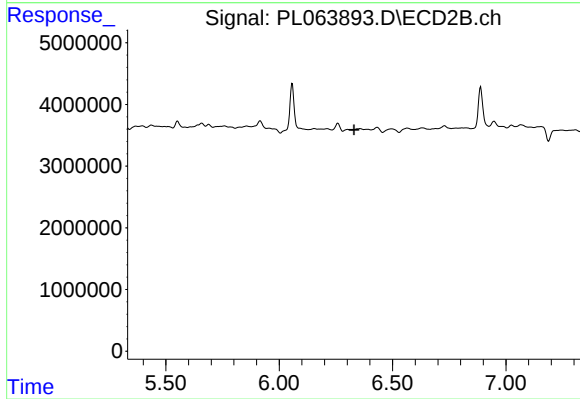

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

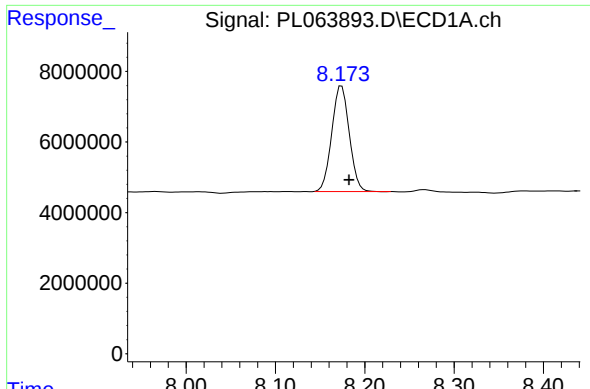

#28 Decachlorobiphenyl

R.T.: 8.174 min
Delta R.T.: -0.008 min
Response: 40781723
Conc: 14.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

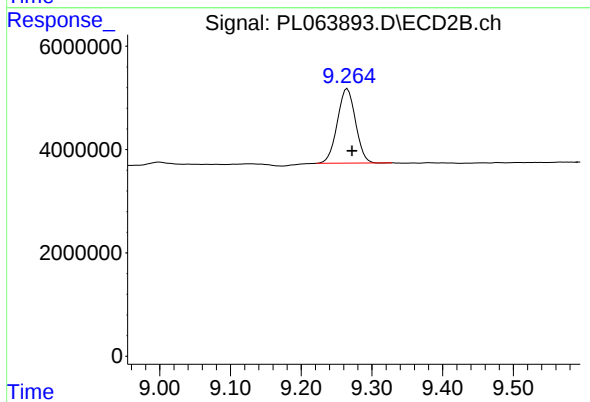

#28 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.007 min
Response: 25813964
Conc: 13.09 ng/ml