

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
 Data File : PL063895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 17:39
 Operator : AR\AJ
 Sample : L5241-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:35:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.111	68137456	54959772	22.728	21.527
28)	SA Decachlor...	8.174	9.265	57222207	36287854	20.769	18.405
Target Compounds							
2)	A alpha-BHC	3.903f	0.000	1548021	0	0.310	N.D. #
3)	MA gamma-BHC...	4.154	0.000	2122621	0	0.464	N.D. #
6)	B beta-BHC	4.374f	4.989	6967493	2980583	3.605	1.698 #
9)	A Endosulfan I	5.479	0.000	2705914	0	0.782	N.D. #
11)	B alpha-Chl...	5.413	0.000	5479448	0	1.461	N.D. #
26)	Chlordane-4	5.413f	0.000	5479448	0	20.479	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
Data File : PL063895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 17:39
Operator : AR\AJ
Sample : L5241-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:35:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

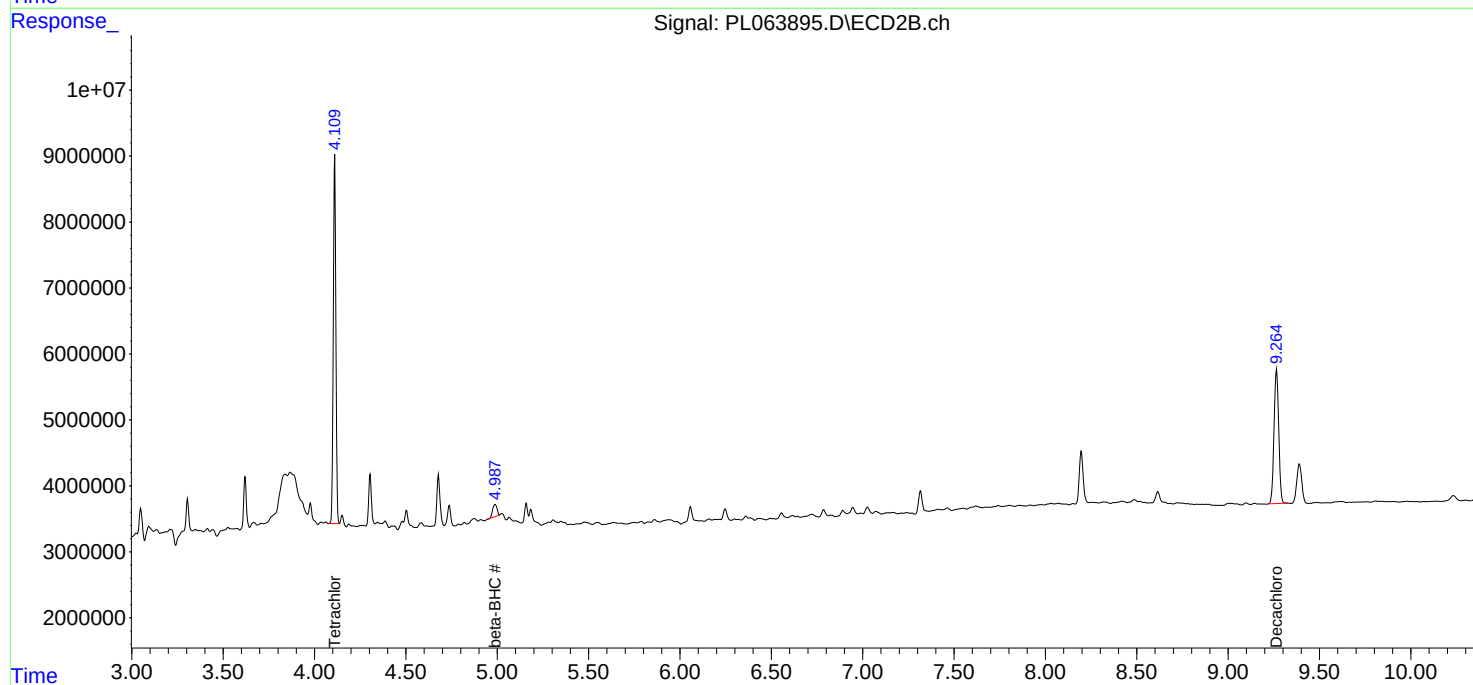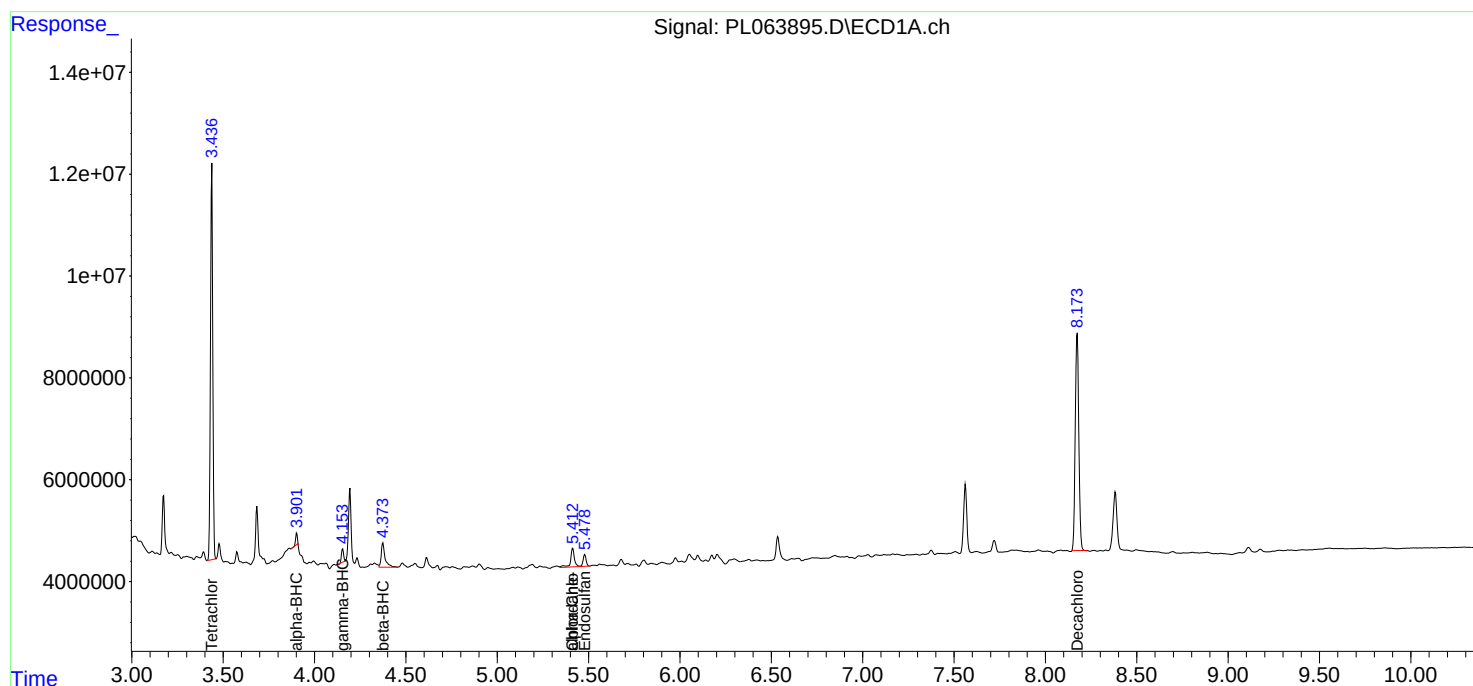


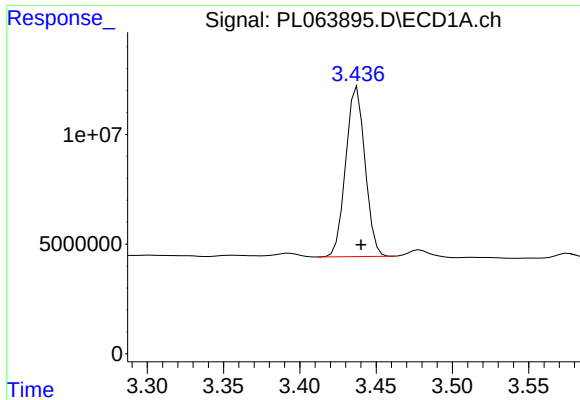

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 68137456
Conc: 22.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

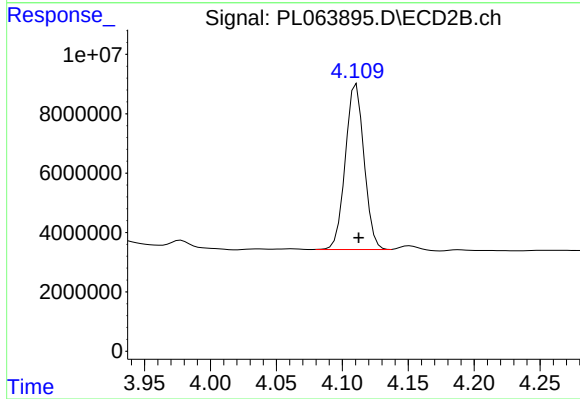


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 54959772
Conc: 21.53 ng/ml

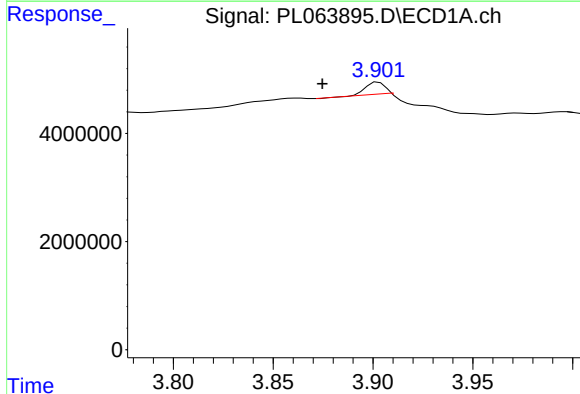


#2 alpha-BHC

R.T.: 3.903 min
Delta R.T.: 0.028 min
Response: 1548021
Conc: 0.31 ng/ml

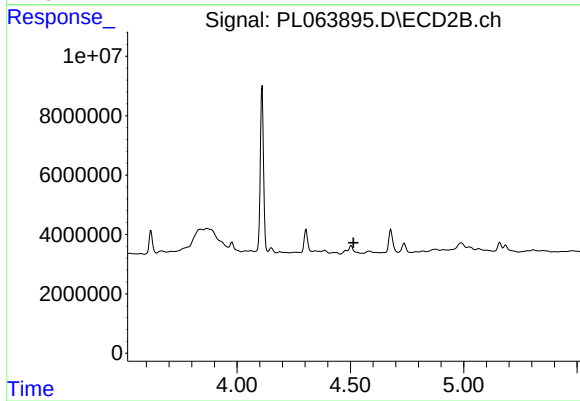

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.514 min
Response: 0
Conc: N.D.

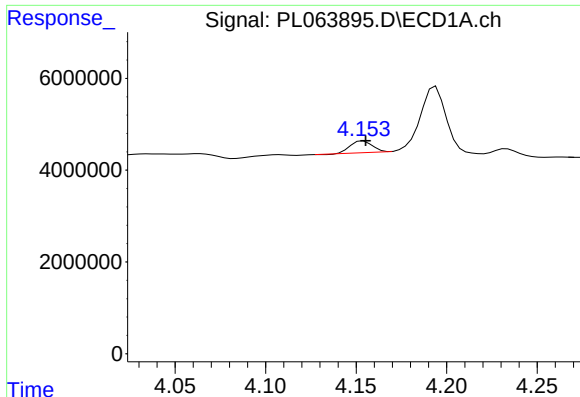

#3 gamma-BHC (Lindane)


R.T.: 4.154 min
Delta R.T.: -0.001 min
Response: 2122621
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

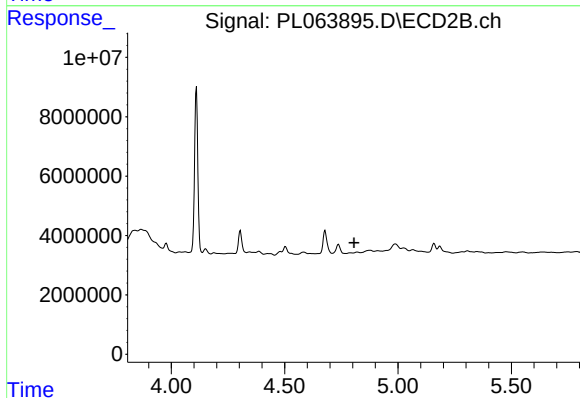


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.806 min
Response: 0
Conc: N.D.

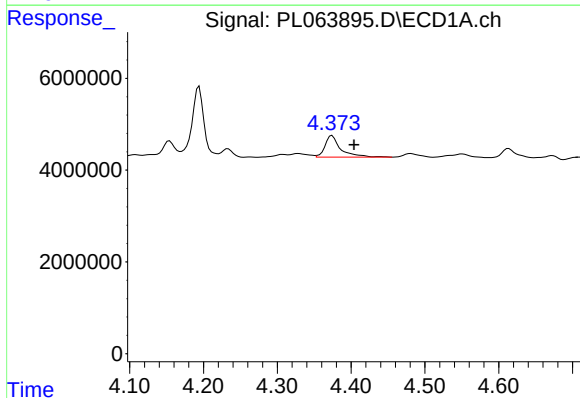


#6 beta-BHC

R.T.: 4.374 min
Delta R.T.: -0.030 min
Response: 6967493
Conc: 3.60 ng/ml

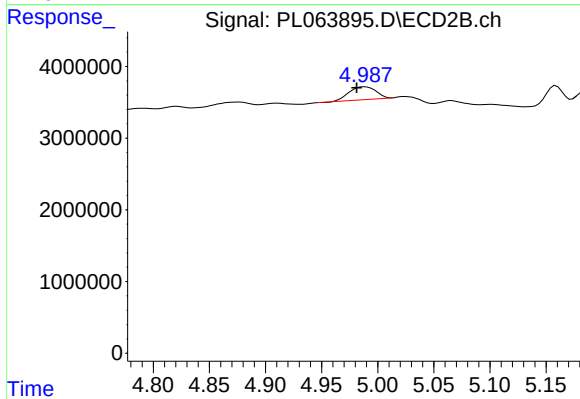

#6 beta-BHC


R.T.: 4.989 min
Delta R.T.: 0.007 min
Response: 2980583
Conc: 1.70 ng/ml

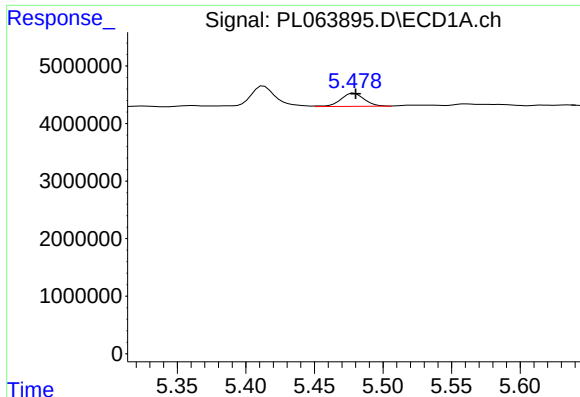

#9 Endosulfan I


R.T.: 5.479 min
Delta R.T.: -0.001 min
Response: 2705914
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

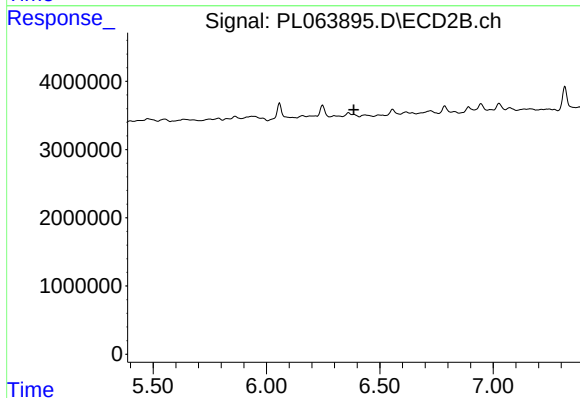


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

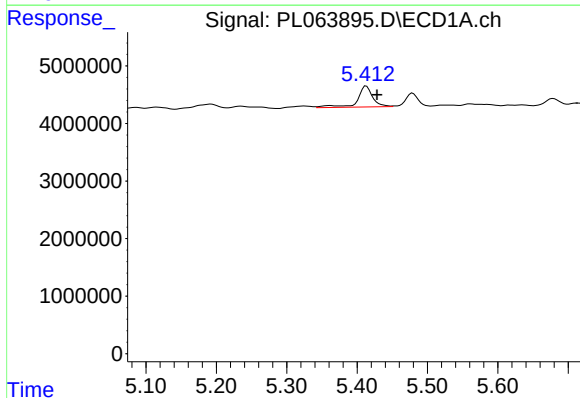


#11 alpha-Chlordane

R.T.: 5.413 min
Delta R.T.: -0.015 min
Response: 5479448
Conc: 1.46 ng/ml

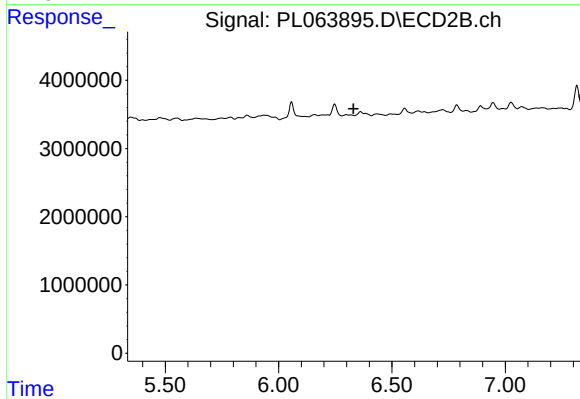

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

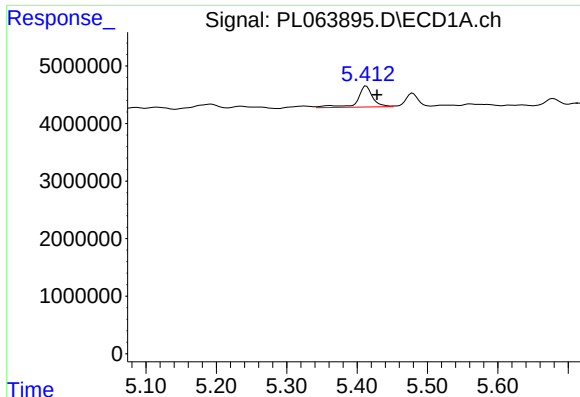

#26 Chlordane-4


R.T.: 5.413 min
Delta R.T.: -0.015 min
Response: 5479448
Conc: 20.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

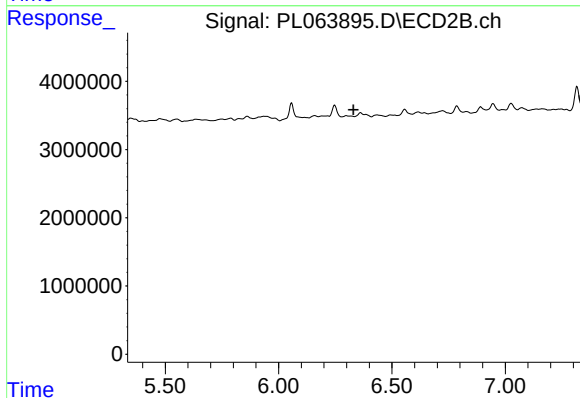


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

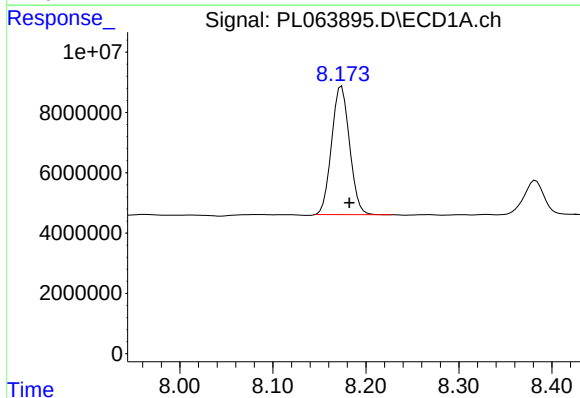

#28 Decachlorobiphenyl

R.T.: 8.174 min
Delta R.T.: -0.008 min
Response: 57222207
Conc: 20.77 ng/ml

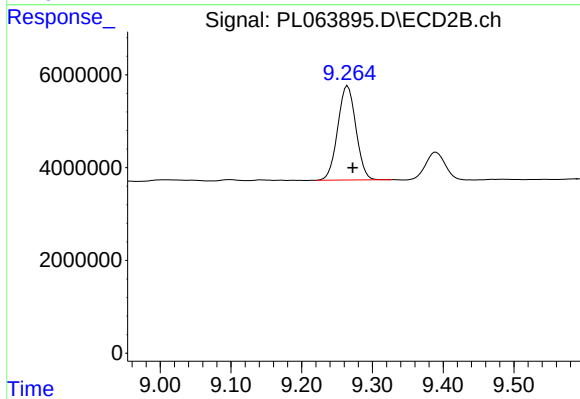

#28 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.007 min
Response: 36287854
Conc: 18.41 ng/ml