

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
 Data File : PL063896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 17:54
 Operator : AR\AJ
 Sample : L5242-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:36:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.111	59567102	48922961	19.869	19.163
28)	SA Decachlor...	8.173	9.265	51447699	33423410	18.673	16.952
Target Compounds							
6)	B beta-BHC	4.374f	4.987	6025891	4111072	3.118	2.342
9)	A Endosulfan I	5.493	0.000	2968862	0	0.857	N.D. #
10)	B gamma-Chl...	0.000	6.253	0	4307464	N.D.	1.557 #
25)	Chlordane-3	0.000	6.253	0	4307464	N.D.	12.571 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
Data File : PL063896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 17:54
Operator : AR\AJ
Sample : L5242-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:36:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

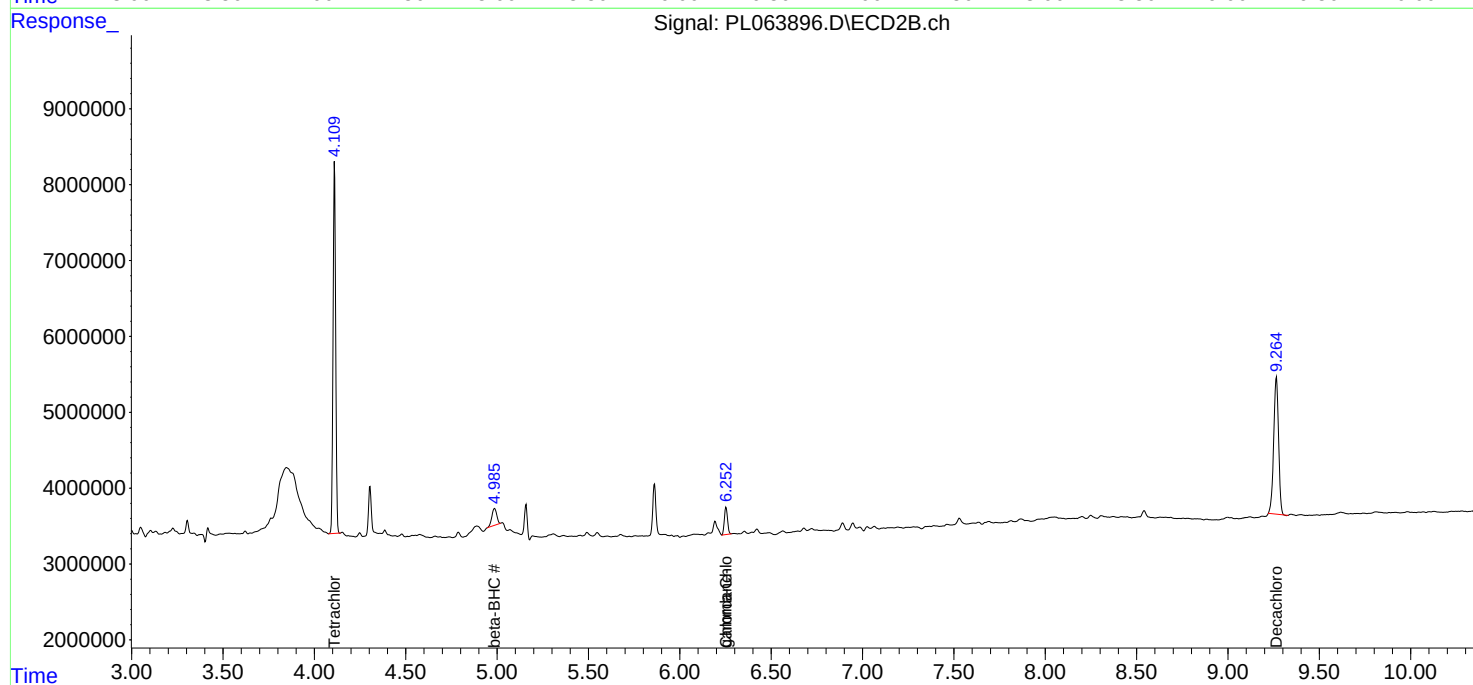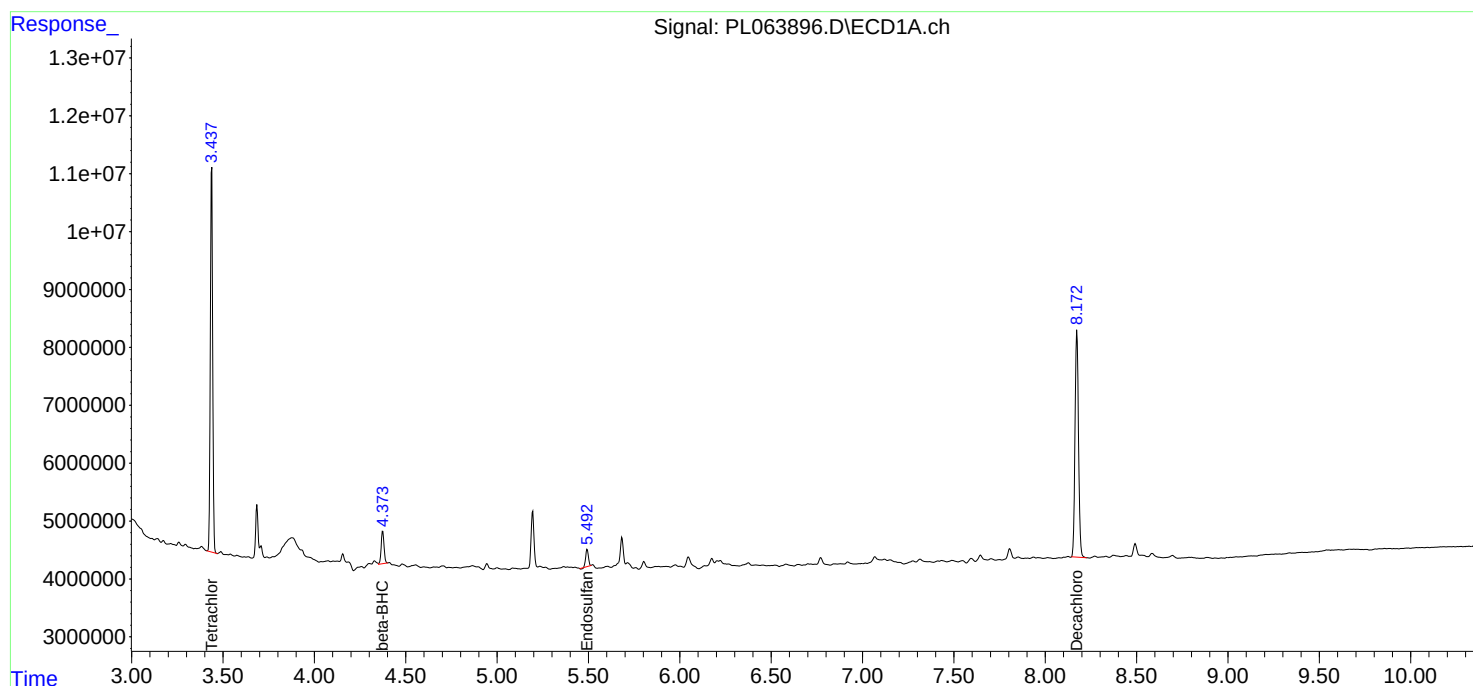


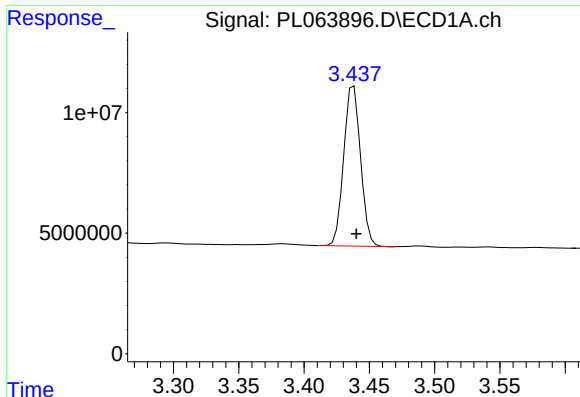

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 59567102
Conc: 19.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

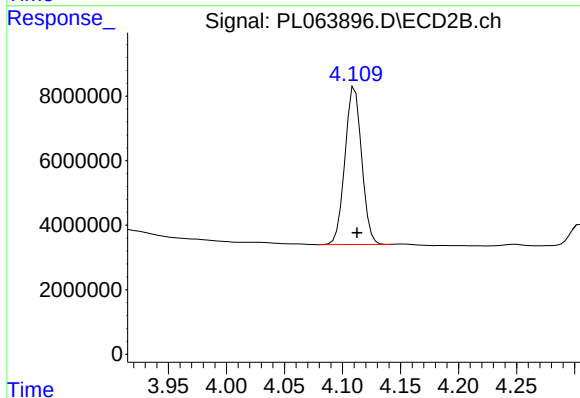


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 48922961
Conc: 19.16 ng/ml

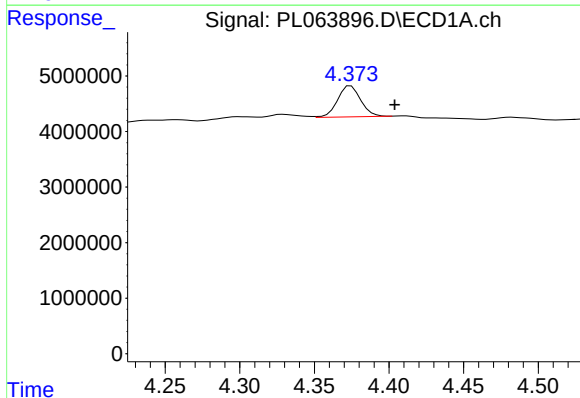


#6 beta-BHC

R.T.: 4.374 min
Delta R.T.: -0.029 min
Response: 6025891
Conc: 3.12 ng/ml

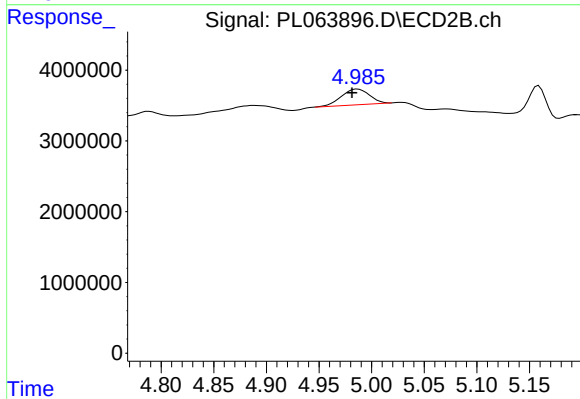

#6 beta-BHC


R.T.: 4.987 min
Delta R.T.: 0.005 min
Response: 4111072
Conc: 2.34 ng/ml

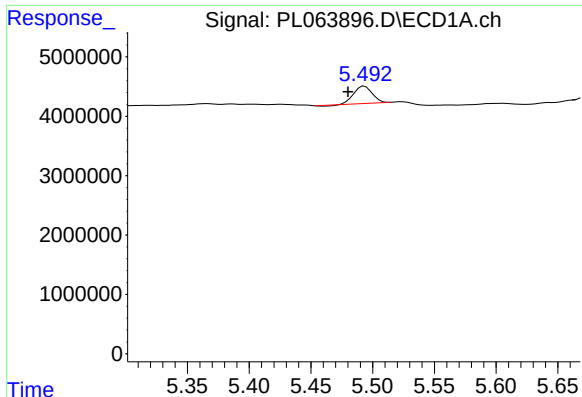

#9 Endosulfan I


R.T.: 5.493 min
Delta R.T.: 0.013 min
Response: 2968862
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

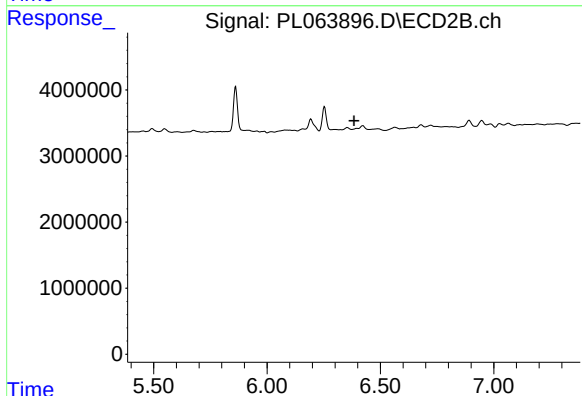


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

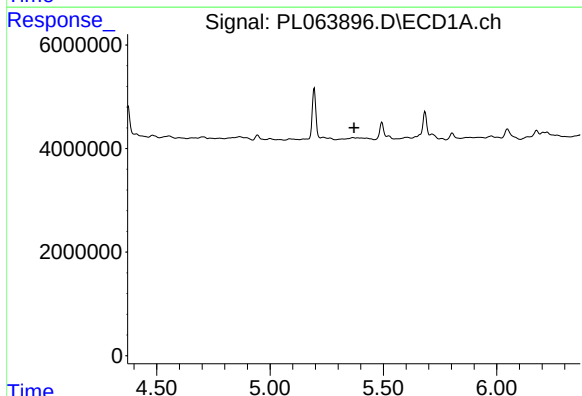


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.370 min
Response: 0
Conc: N.D.

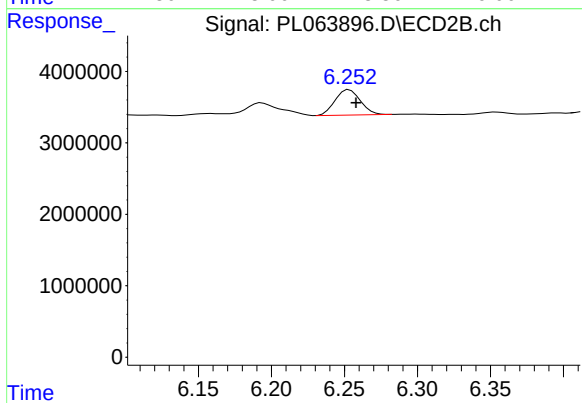

#10 gamma-Chlordane


R.T.: 6.253 min
Delta R.T.: -0.005 min
Response: 4307464
Conc: 1.56 ng/ml

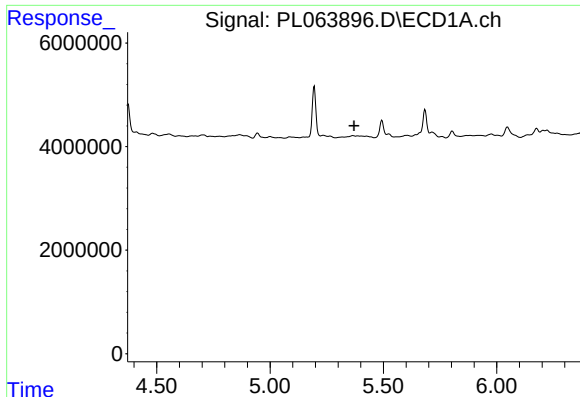

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

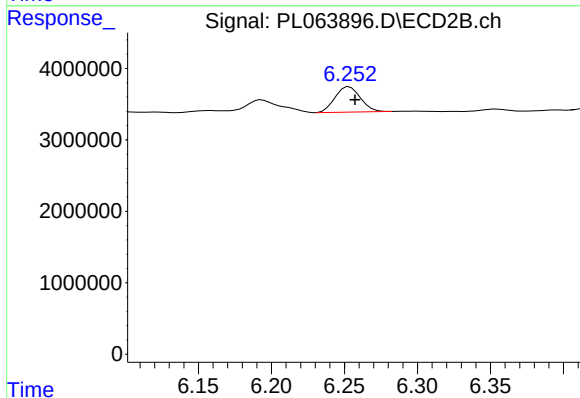


#25 Chlordane-3

R.T.: 6.253 min
Delta R.T.: -0.004 min
Response: 4307464
Conc: 12.57 ng/ml

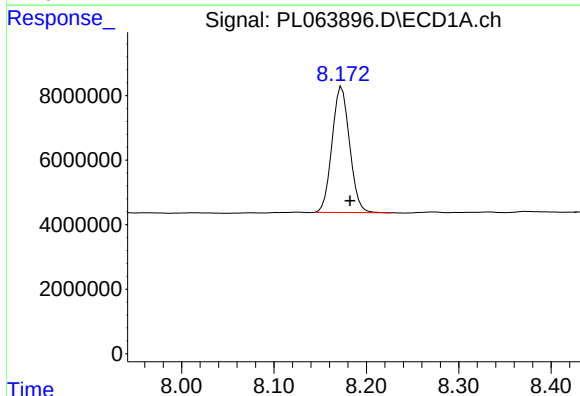

#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: -0.009 min
Response: 51447699
Conc: 18.67 ng/ml

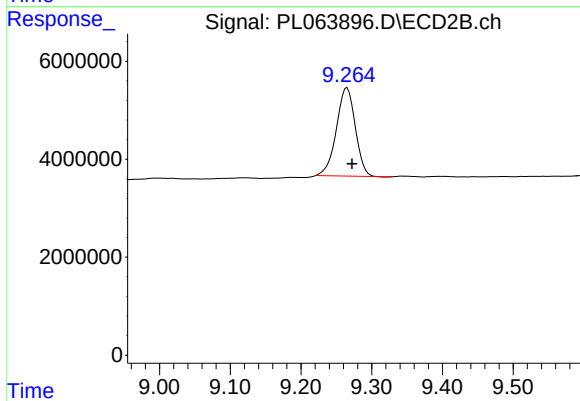

#28 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.007 min
Response: 33423410
Conc: 16.95 ng/ml