

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
 Data File : PL063900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 18:51
 Operator : AR\AJ
 Sample : L5242-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:37:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.110	64834274	53711350	21.626	21.038
28)	SA Decachlor...	8.173	9.264	59763450	38717065	21.692	19.637
Target Compounds							
3)	MA gamma-BHC...	4.156	4.787f	5952228	2640853	1.302	0.774 #
6)	B beta-BHC	4.374f	4.989	3812315	3840124	1.972	2.188
9)	A Endosulfan I	5.493	0.000	6831781	0	1.973	N.D. #
10)	B gamma-Chl...	0.000	6.253	0	12080701	N.D.	4.366 #
15)	B Endosulfa...	6.223f	0.000	4862458	0	1.475	N.D. #
25)	Chlordane-3	0.000	6.253	0	12080701	N.D.	35.258 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
Data File : PL063900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 18:51
Operator : AR\AJ
Sample : L5242-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:37:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

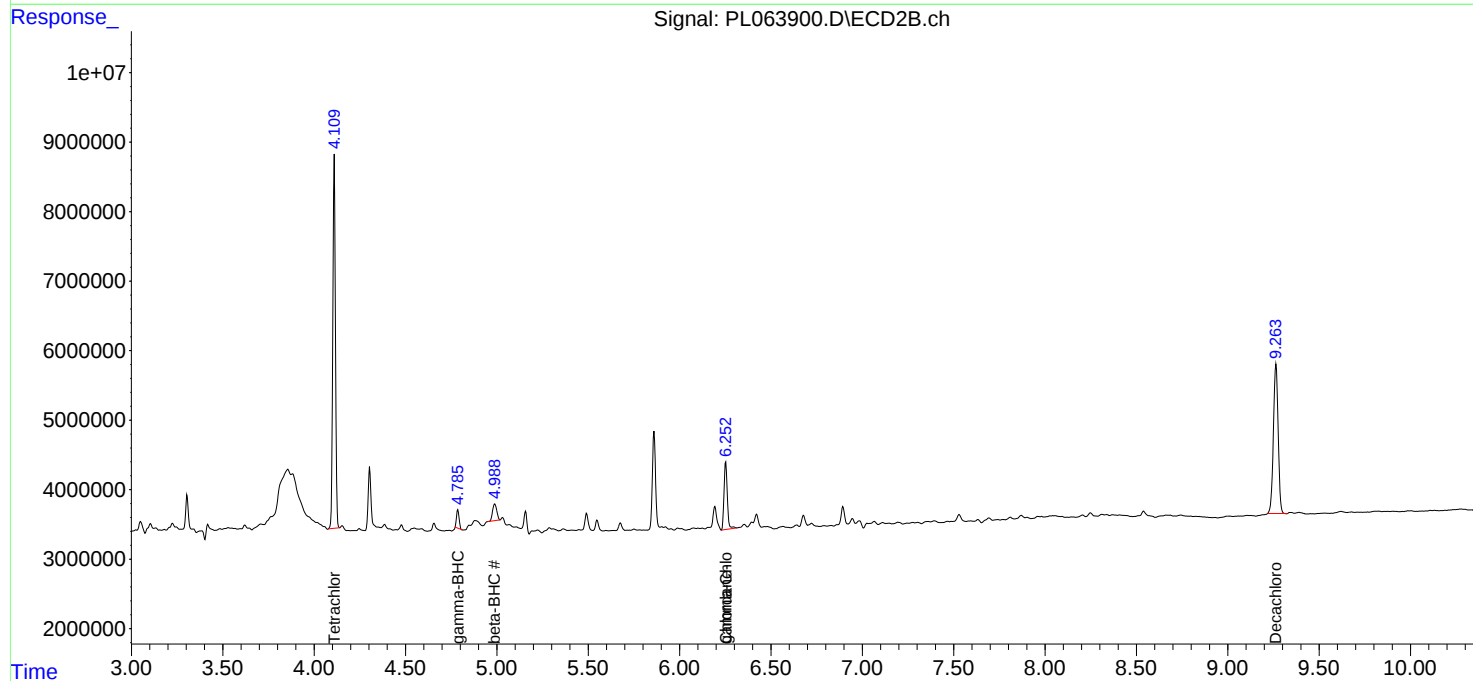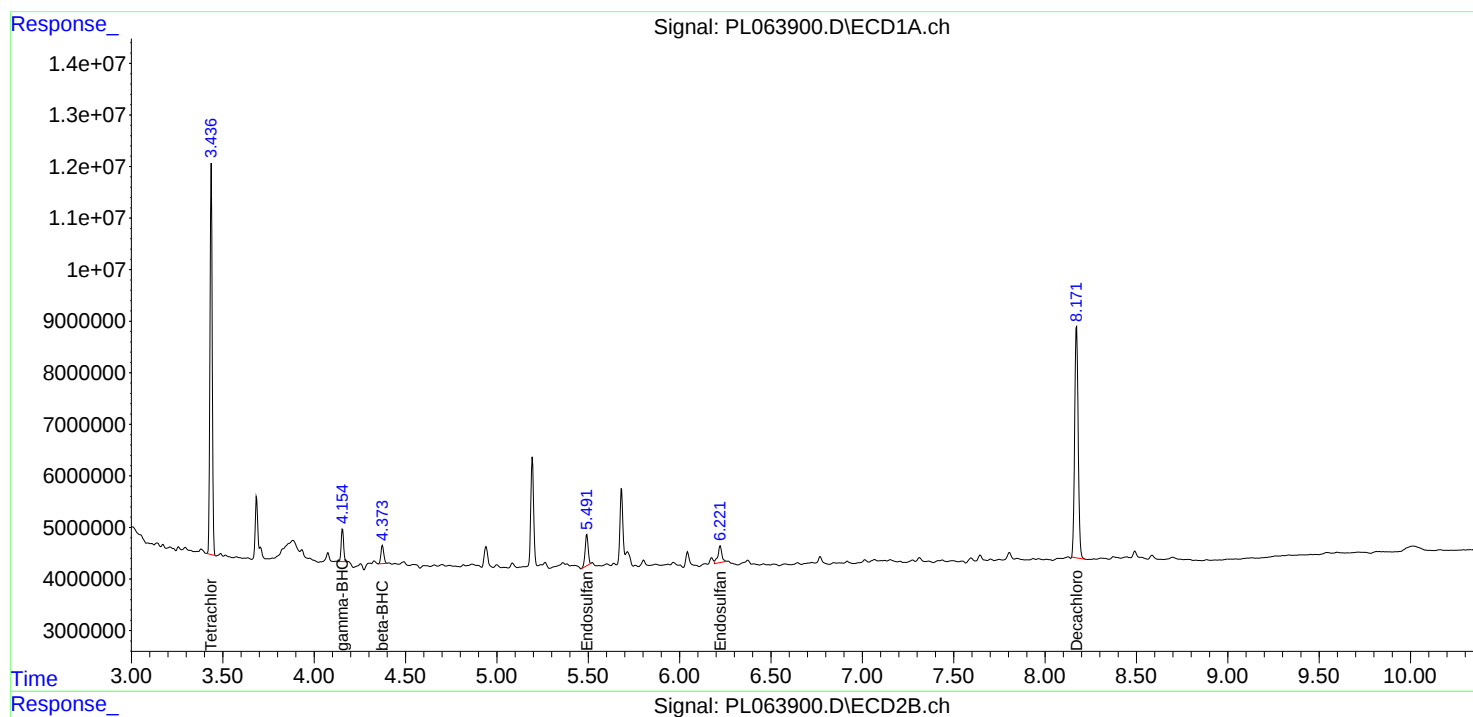


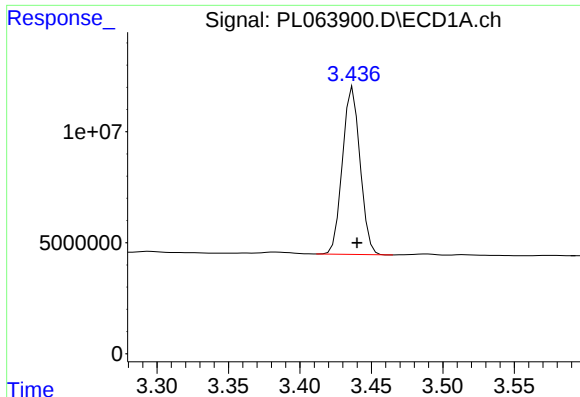

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: -0.003 min
Response: 64834274
Conc: 21.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

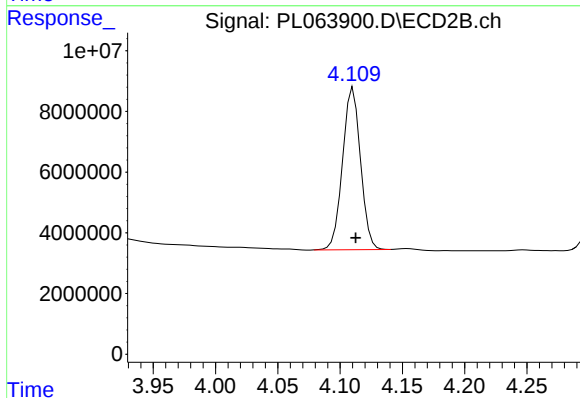


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.002 min
Response: 53711350
Conc: 21.04 ng/ml

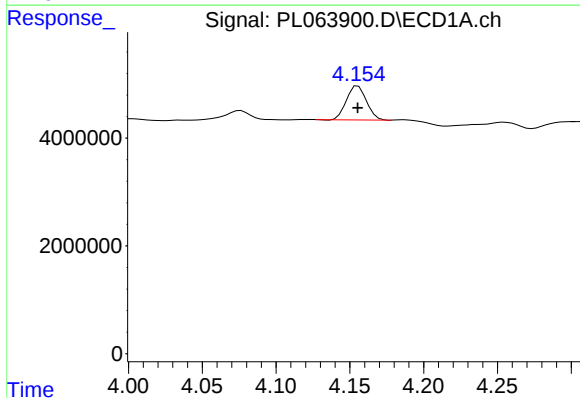


#3 gamma-BHC (Lindane)

R.T.: 4.156 min
Delta R.T.: 0.000 min
Response: 5952228
Conc: 1.30 ng/ml

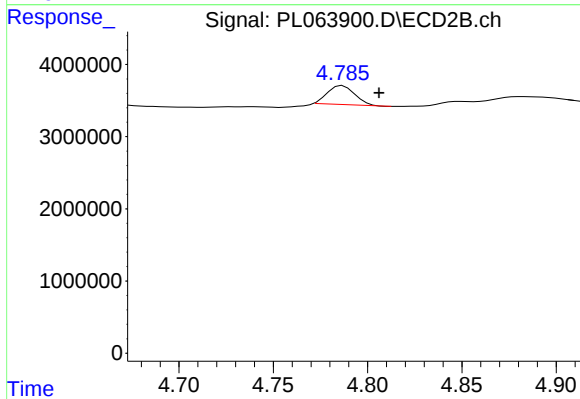

#3 gamma-BHC (Lindane)


R.T.: 4.787 min
Delta R.T.: -0.019 min
Response: 2640853
Conc: 0.77 ng/ml

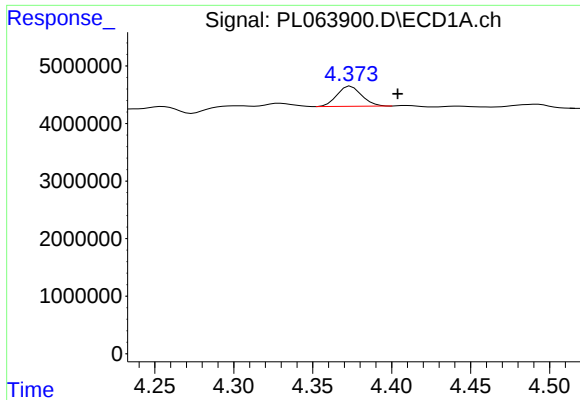

#6 beta-BHC


R.T.: 4.374 min
Delta R.T.: -0.030 min
Response: 3812315
Conc: 1.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

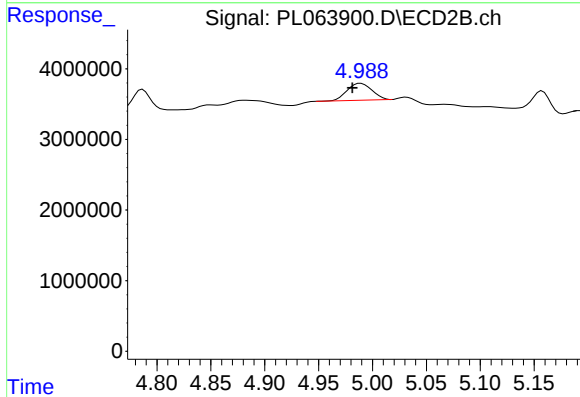


#6 beta-BHC

R.T.: 4.989 min
Delta R.T.: 0.008 min
Response: 3840124
Conc: 2.19 ng/ml

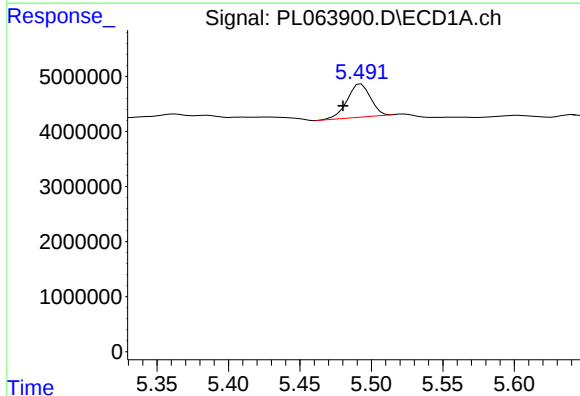


#9 Endosulfan I

R.T.: 5.493 min
Delta R.T.: 0.013 min
Response: 6831781
Conc: 1.97 ng/ml

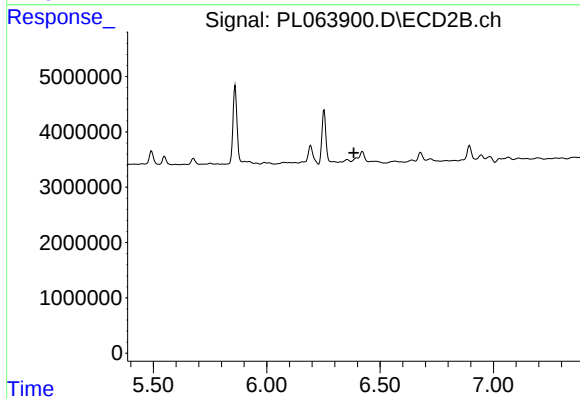

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

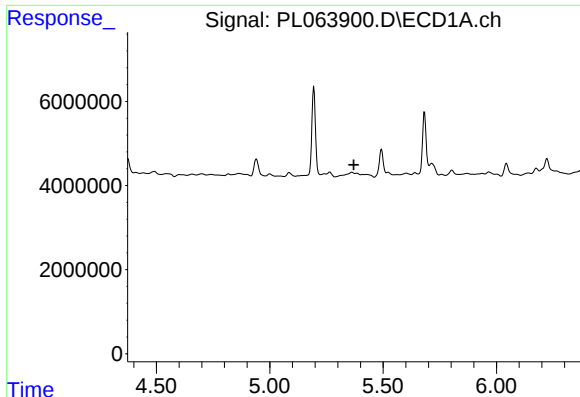

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

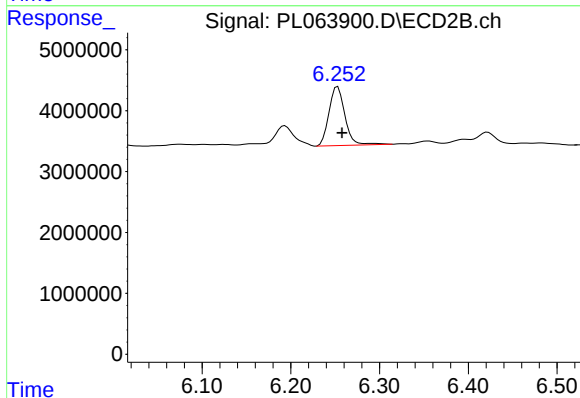


#10 gamma-Chlordane

R.T.: 6.253 min
Delta R.T.: -0.005 min
Response: 12080701
Conc: 4.37 ng/ml

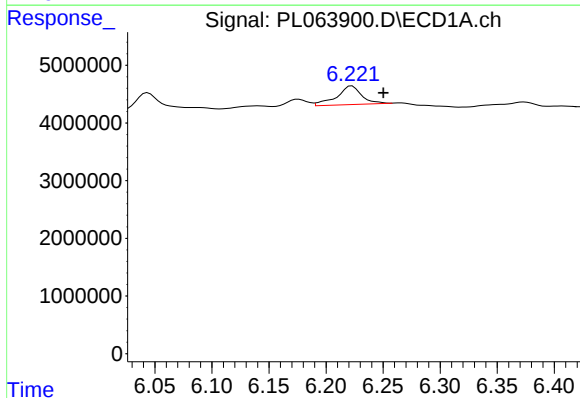


#15 Endosulfan II

R.T.: 6.223 min
Delta R.T.: -0.028 min
Response: 4862458
Conc: 1.48 ng/ml

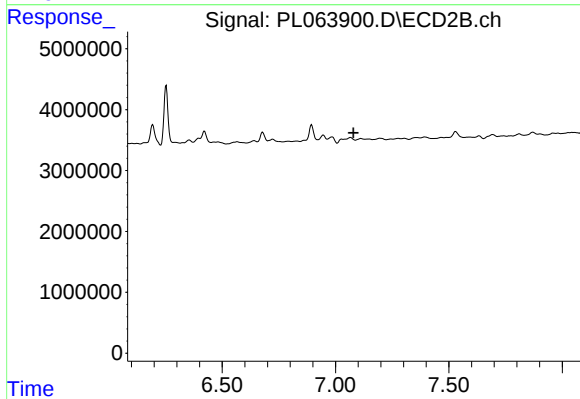

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.080 min
Response: 0
Conc: N.D.

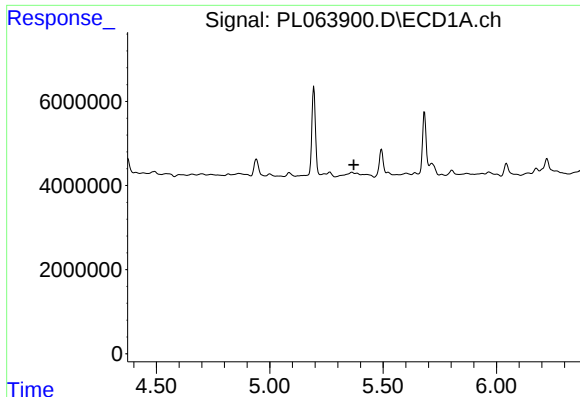

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

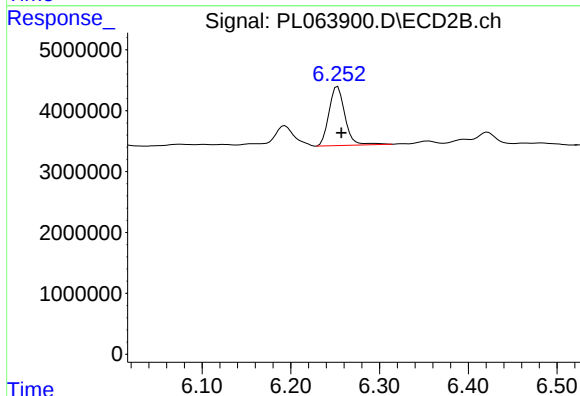


#25 Chlordane-3

R.T.: 6.253 min
Delta R.T.: -0.004 min
Response: 12080701
Conc: 35.26 ng/ml

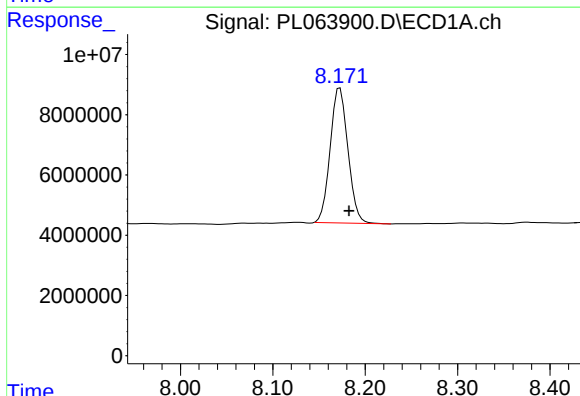

#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: -0.010 min
Response: 59763450
Conc: 21.69 ng/ml

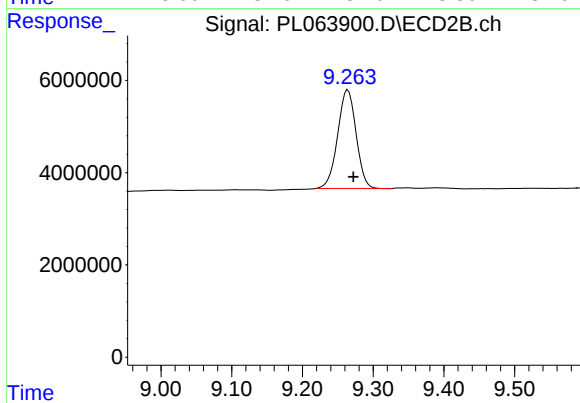

#28 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.008 min
Response: 38717065
Conc: 19.64 ng/ml