

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
 Data File : PL063902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 19:19
 Operator : AR\AJ
 Sample : L5242-21
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:37:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.110	64351049	53050183	21.465	20.779
28)	SA Decachlor...	8.173	9.263	49739496	38996271	18.053	19.779
Target Compounds							
3)	MA gamma-BHC...	4.156	4.787f	20863171	8569886	4.564	2.512 #
6)	B beta-BHC	4.374f	0.000	2949133	0	1.526	N.D. #
9)	A Endosulfan I	5.493	0.000	10609927	0	3.064	N.D. #
10)	B gamma-Chl...	5.360	6.253	1386980	46730473	0.365	16.889 #
15)	B Endosulfa...	6.224f	0.000	12169445	0	3.692	N.D. #
17)	MA 4,4'-DDT	6.375f	0.000	3197968	0	1.207	N.D. #
20)	A Methoxychlor	6.918f	0.000	5031145	0	3.830	N.D. #
25)	Chlordane-3	5.360	6.253	1386980	46730473	4.245	136.385 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
Data File : PL063902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 19:19
Operator : AR\AJ
Sample : L5242-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:37:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

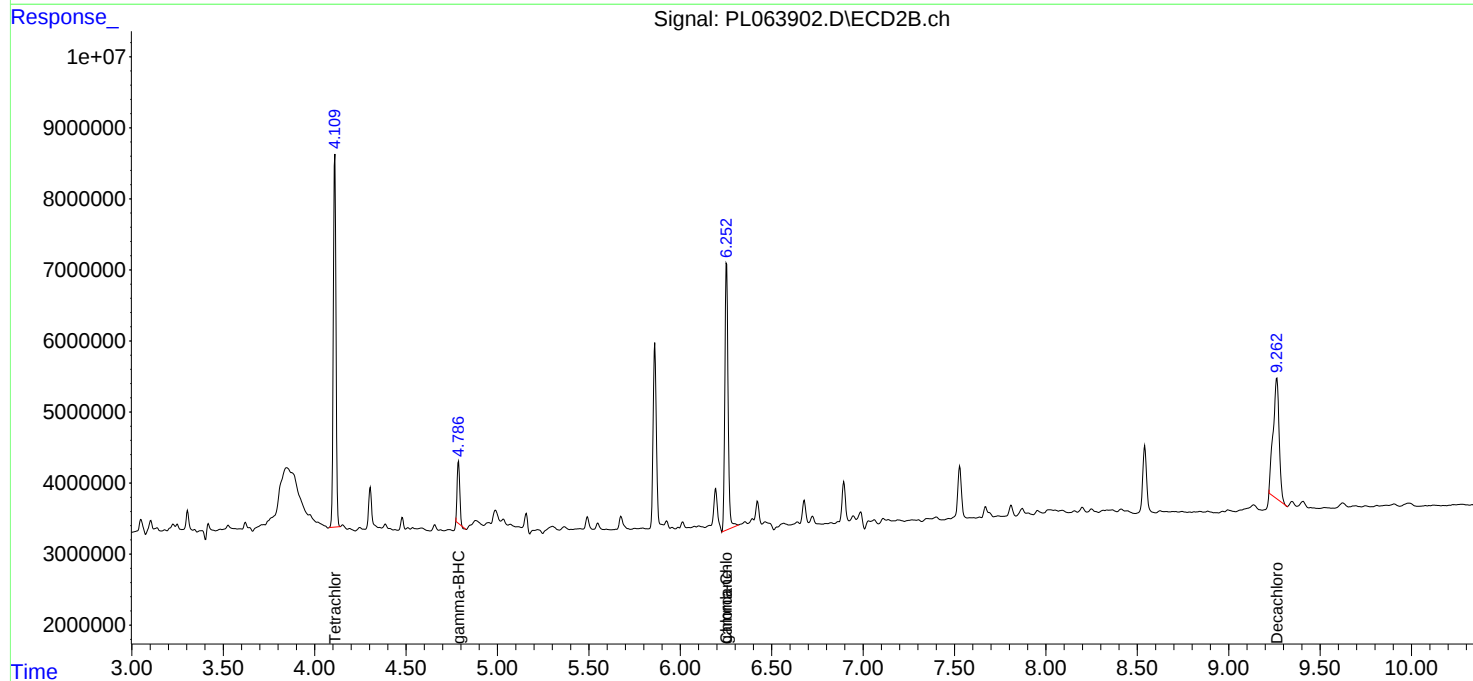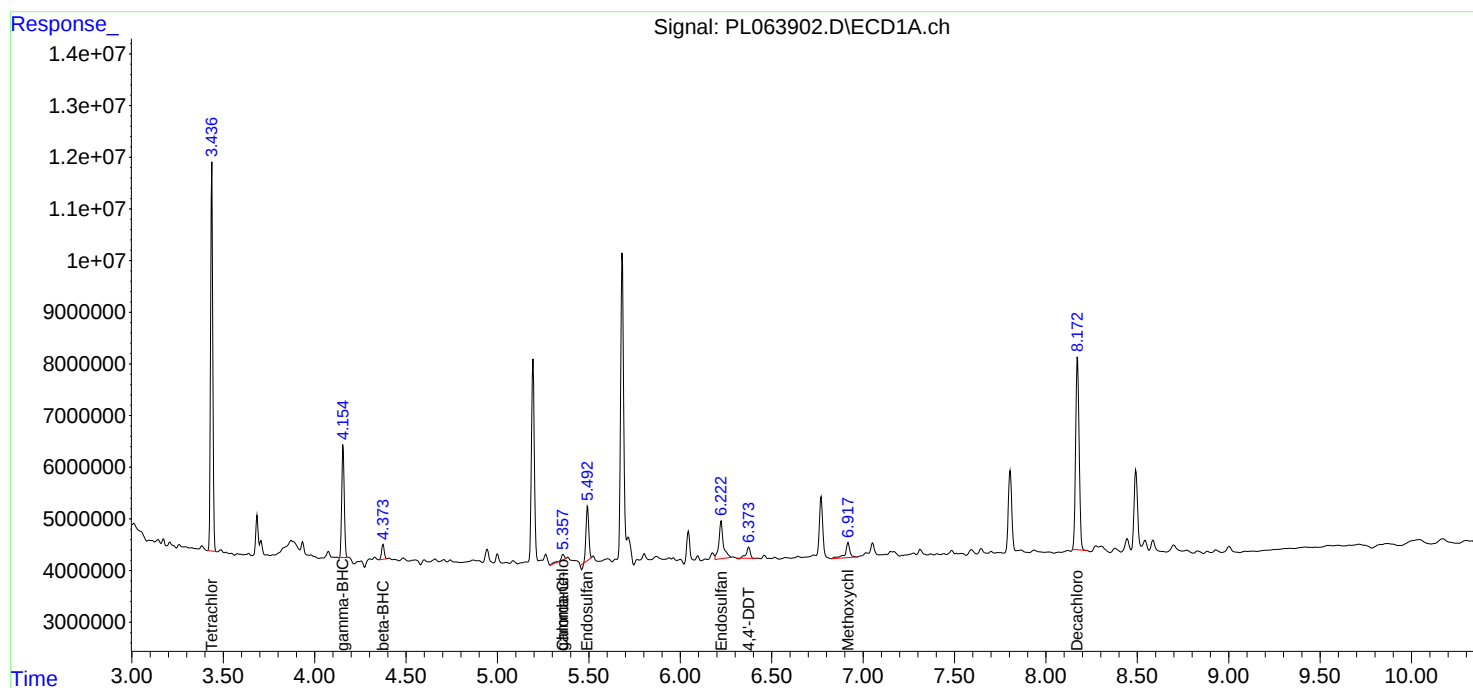


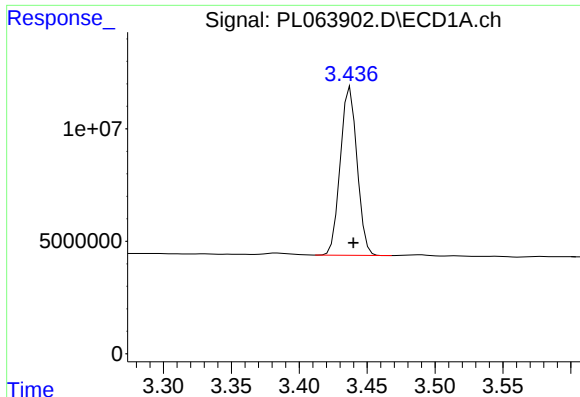

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 64351049
Conc: 21.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

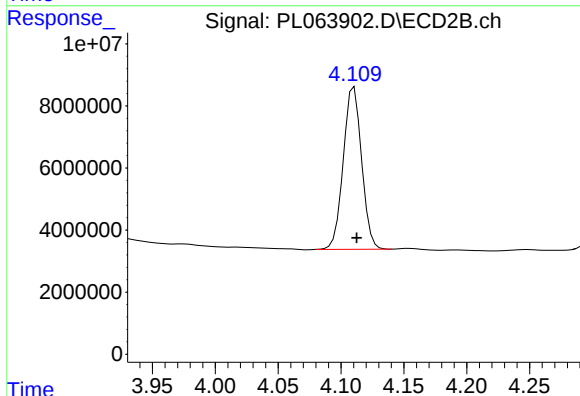


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.002 min
Response: 53050183
Conc: 20.78 ng/ml

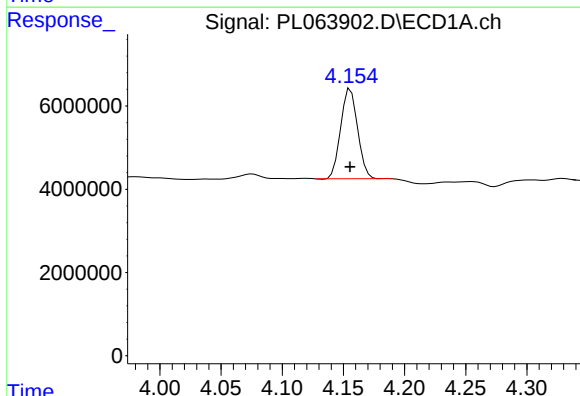


#3 gamma-BHC (Lindane)

R.T.: 4.156 min
Delta R.T.: 0.000 min
Response: 20863171
Conc: 4.56 ng/ml

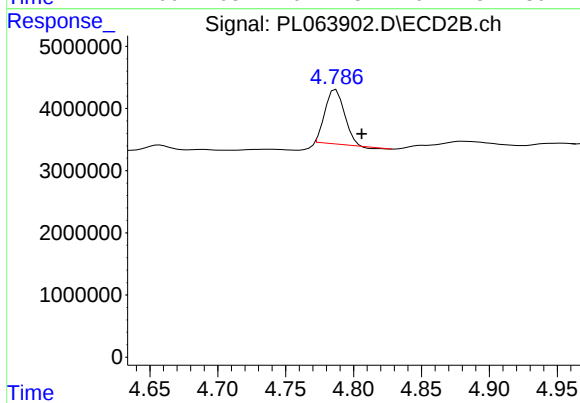

#3 gamma-BHC (Lindane)


R.T.: 4.787 min
Delta R.T.: -0.019 min
Response: 8569886
Conc: 2.51 ng/ml

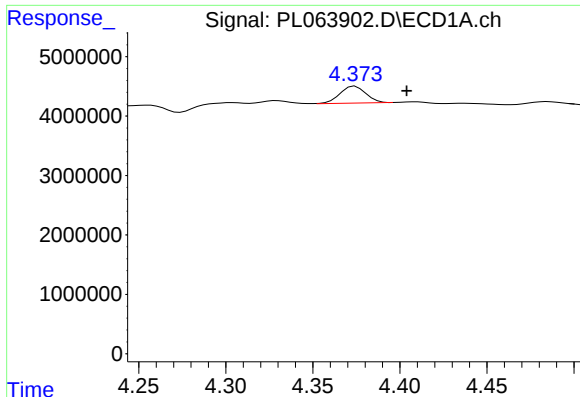

#6 beta-BHC


R.T.: 4.374 min
Delta R.T.: -0.030 min
Response: 2949133
Conc: 1.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

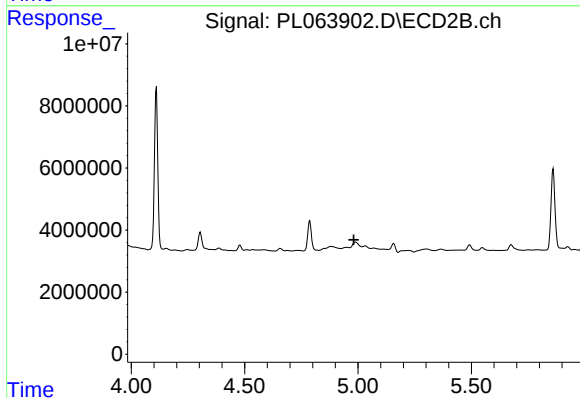


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.981 min
Response: 0
Conc: N.D.

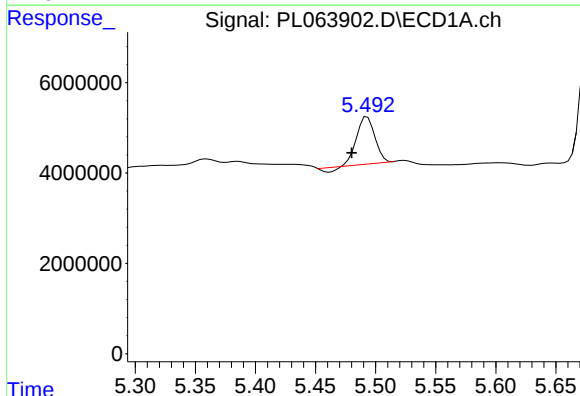


#9 Endosulfan I

R.T.: 5.493 min
Delta R.T.: 0.013 min
Response: 10609927
Conc: 3.06 ng/ml

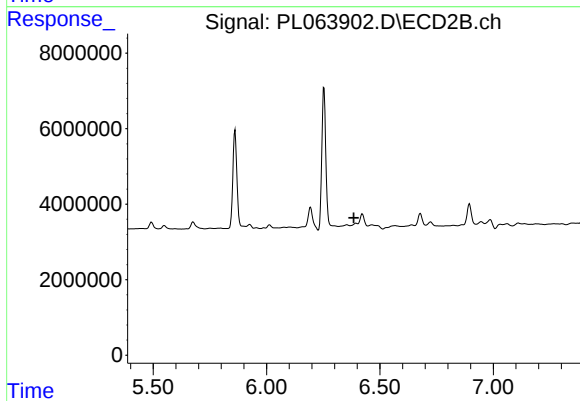

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

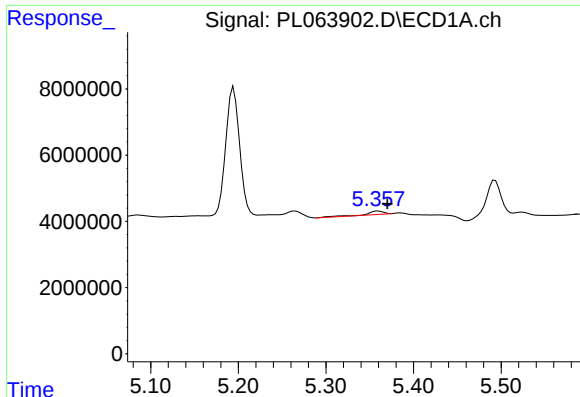

#10 gamma-Chlordane


R.T.: 5.360 min
Delta R.T.: -0.011 min
Response: 1386980
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

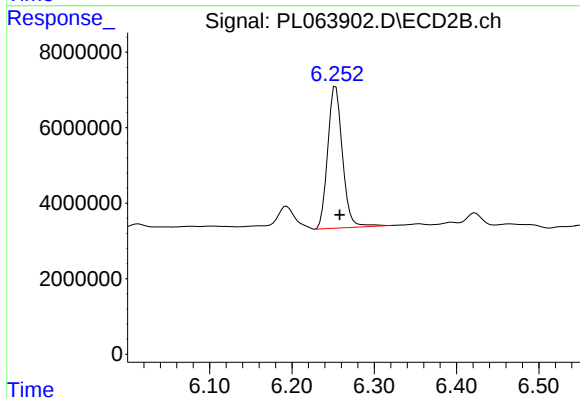


#10 gamma-Chlordane

R.T.: 6.253 min
Delta R.T.: -0.005 min
Response: 46730473
Conc: 16.89 ng/ml

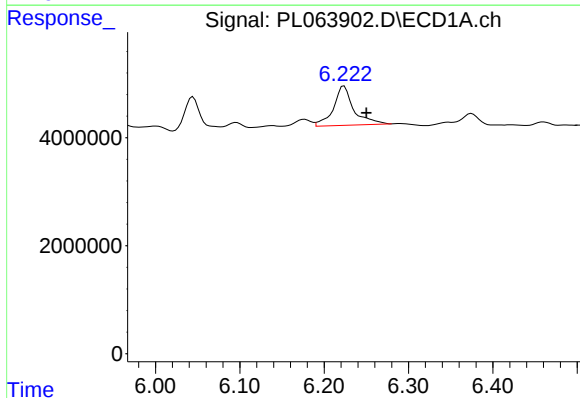


#15 Endosulfan II

R.T.: 6.224 min
Delta R.T.: -0.027 min
Response: 12169445
Conc: 3.69 ng/ml

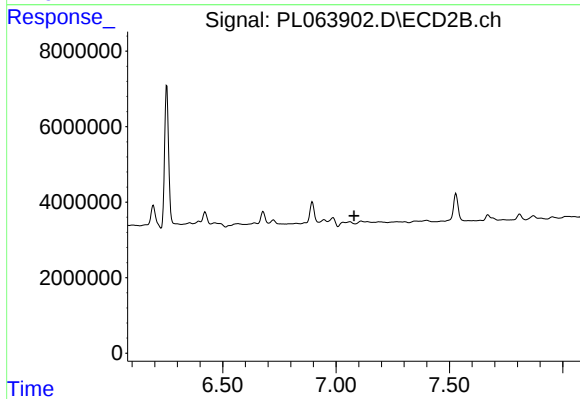

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.080 min
Response: 0
Conc: N.D.

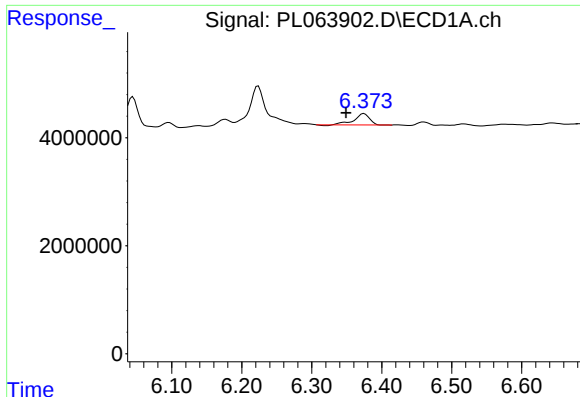

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: 0.026 min
Response: 3197968
Conc: 1.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

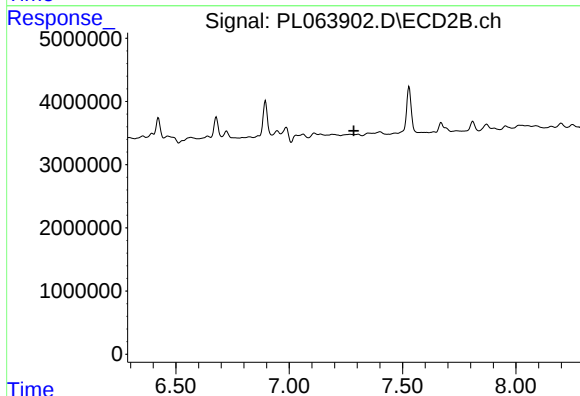


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.284 min
Response: 0
Conc: N.D.

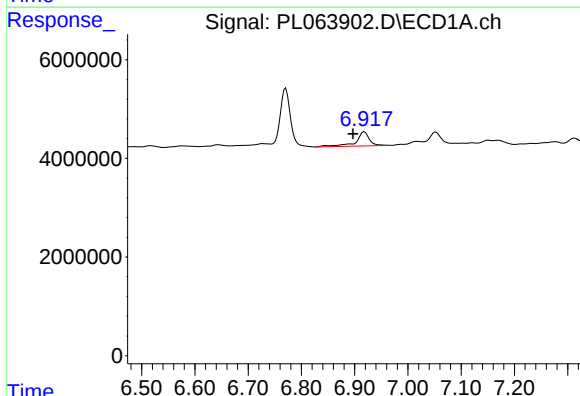


#20 Methoxychlor

R.T.: 6.918 min
Delta R.T.: 0.021 min
Response: 5031145
Conc: 3.83 ng/ml

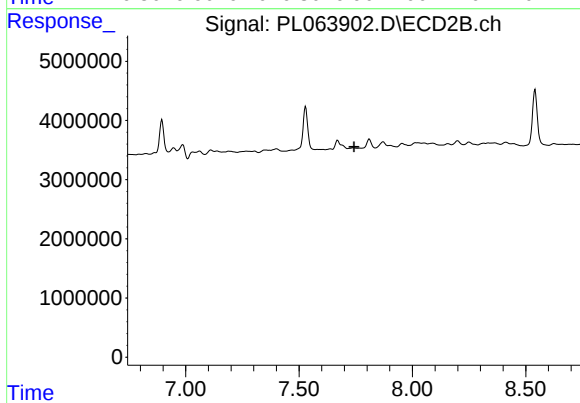

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.743 min
Response: 0
Conc: N.D.

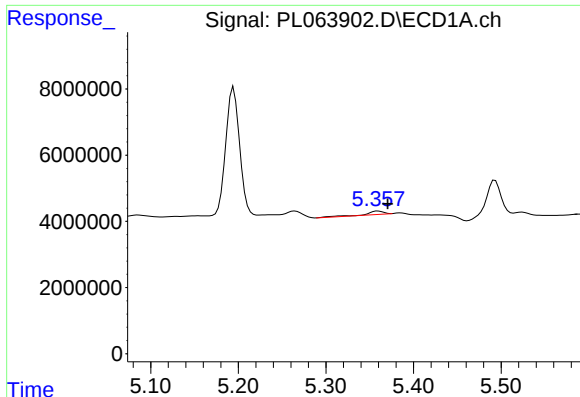

#25 Chlordane-3


R.T.: 5.360 min
Delta R.T.: -0.011 min
Response: 1386980
Conc: 4.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

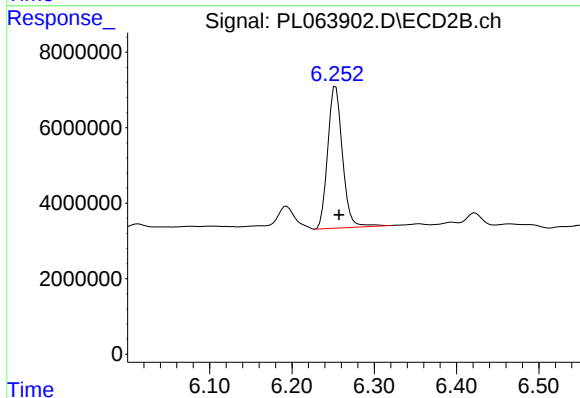


#25 Chlordane-3

R.T.: 6.253 min
Delta R.T.: -0.004 min
Response: 46730473
Conc: 136.38 ng/ml

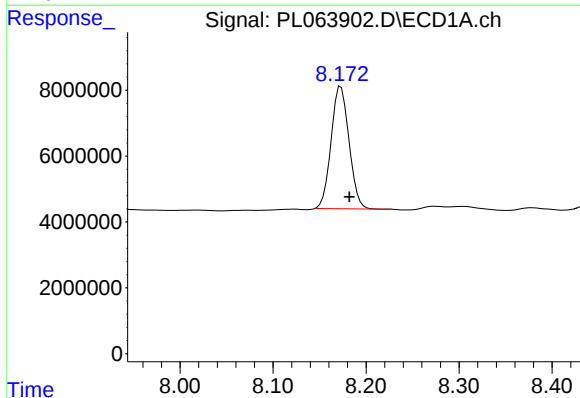

#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: -0.009 min
Response: 49739496
Conc: 18.05 ng/ml

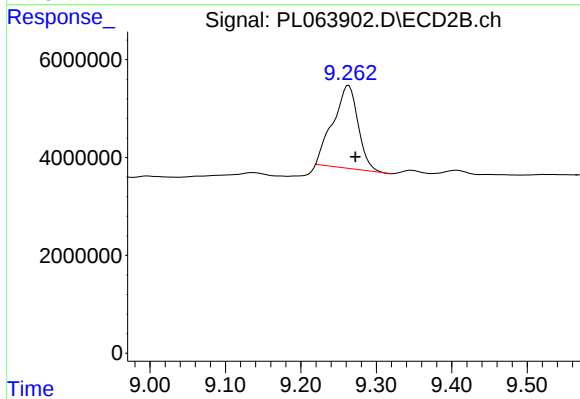

#28 Decachlorobiphenyl

R.T.: 9.263 min
Delta R.T.: -0.009 min
Response: 38996271
Conc: 19.78 ng/ml