

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
 Data File : PL063882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2020 13:06
 Operator : AR\AJ
 Sample : L5244-01MS 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-01-123020MS

Manual Integrations
 APPROVED

Ankita
 1/4/2021 2:25:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 17:12:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.110	8173220	6164438	2.726	2.415
28)	SA Decachlor...	8.176	9.265	6342179	3469950	2.302	1.760m
Target Compounds							
2)	A alpha-BHC	3.871	4.512	23069915	17517570	4.621	4.863
3)	MA gamma-BHC...	4.152	4.803	23748820	16218407	5.195	4.754
4)	MA Heptachlor	4.453	5.315	24274288	18005544	5.764	5.639
5)	MB Aldrin	4.698	5.625	22028931	14872314	5.515	5.196
6)	B beta-BHC	4.402	4.979	12342598	10440338	6.386	5.948
7)	B delta-BHC	4.604	5.200	16834752	11635751	3.714	3.539
8)	B Heptachlor...	5.140	6.019	21976371	14744325	5.850	5.313
9)	A Endosulfan I	5.476	6.381	22176964	13425200	6.405	5.337
10)	B gamma-Chl...	5.365	6.253	27507620	19809757	7.235m	7.160
11)	B alpha-Chl...	5.424	6.327	25515234	19668456	6.802	7.126
12)	B 4,4'-DDE	5.591	6.483	18783831	14063386	5.464	5.694
13)	MA Dieldrin	5.717	6.641	22240739	13277540	6.136m	5.097
14)	MA Endrin	5.973	6.863	18177721	10500759	6.237	5.411
15)	B Endosulfa...	6.246	7.076	17632891	11900765	5.349	5.048
16)	A 4,4'-DDD	6.105	6.981	14544054	10759890	4.973	5.089
17)	MA 4,4'-DDT	6.345	7.280	15590734	10670955	5.883	5.485
18)	B Endrin al...	6.414	7.201	16928334	8903679	6.117	4.416 #
19)	B Endosulfa...	6.627	7.424	19246695	10986888	6.112	4.885
20)	A Methoxychlor	6.892	7.739	8586276	5585467	6.536m	5.294
21)	B Endrin ke...	7.114	7.904	16423063	11458148	4.724	4.646
22)	Mirex	7.301	8.356	14556670	9519613	5.797	5.277

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL123120\
Data File : PL063882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2020 13:06
Operator : AR\AJ
Sample : L5244-01MS 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 17:12:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

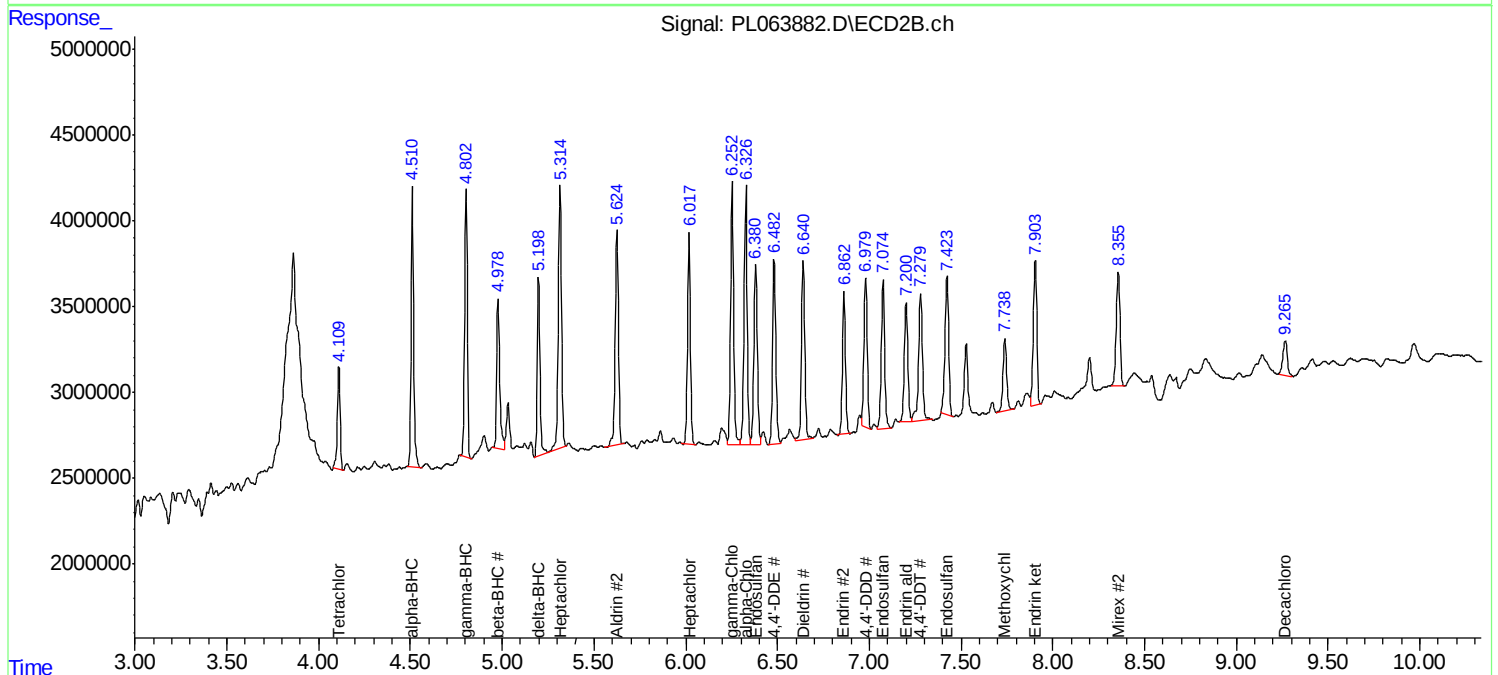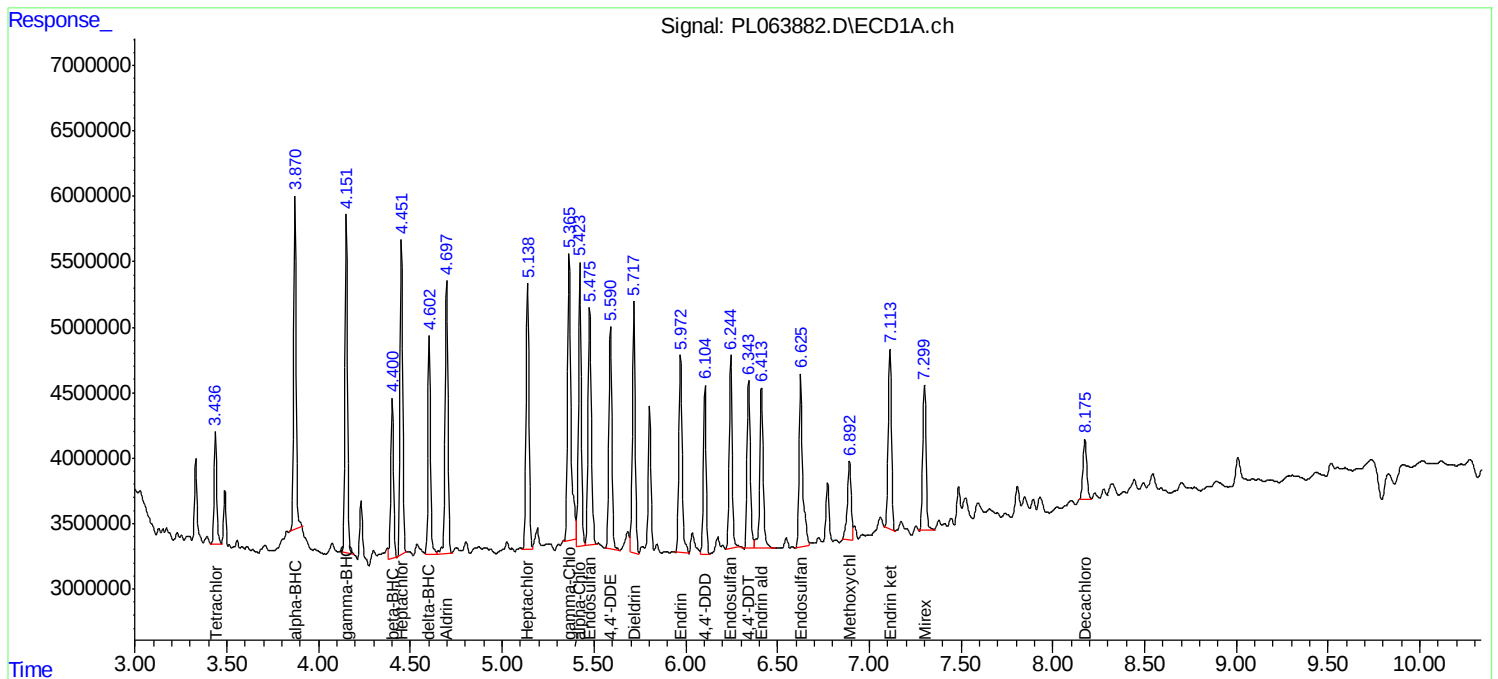




#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: -0.003 min
Response: 8173220
Conc: 2.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

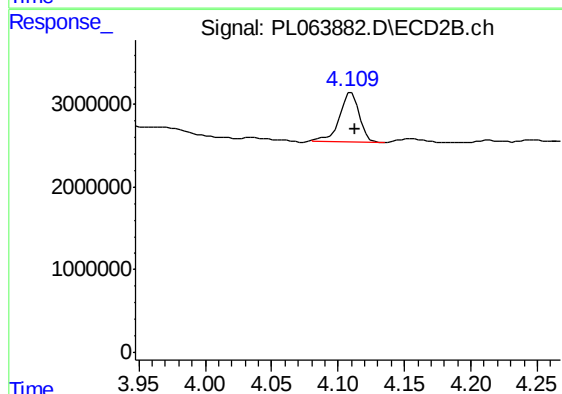


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.002 min
Response: 6164438
Conc: 2.41 ng/ml

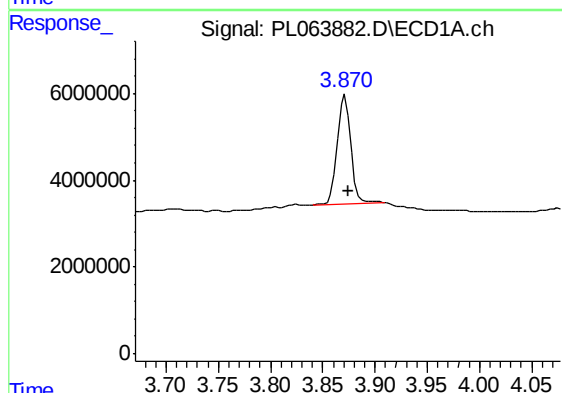


#2 alpha-BHC

R.T.: 3.871 min
Delta R.T.: -0.003 min
Response: 23069915
Conc: 4.62 ng/ml

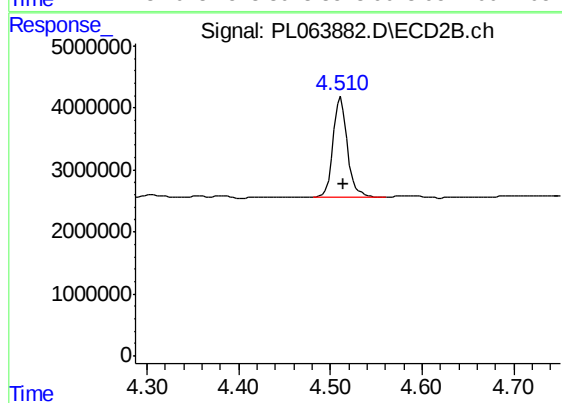

#2 alpha-BHC

R.T.: 4.512 min
Delta R.T.: -0.003 min
Response: 17517570
Conc: 4.86 ng/ml

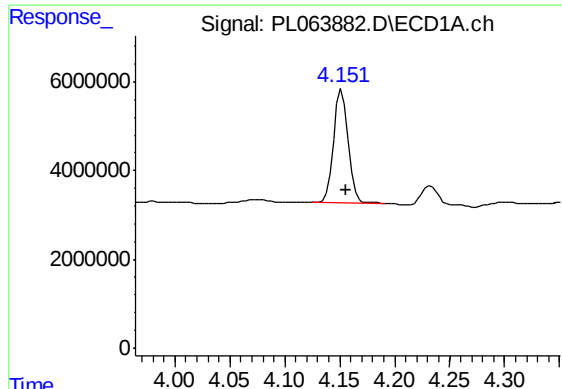


#3 gamma-BHC (Lindane)

R.T.: 4.152 min
Delta R.T.: -0.003 min
Response: 23748820
Conc: 5.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

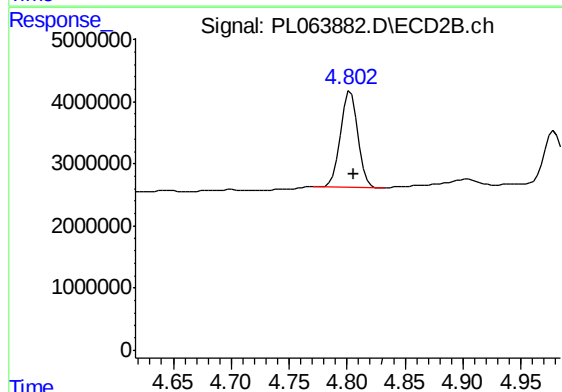


#3 gamma-BHC (Lindane)

R.T.: 4.803 min
Delta R.T.: -0.003 min
Response: 16218407
Conc: 4.75 ng/ml




#4 Heptachlor

R.T.: 4.453 min
Delta R.T.: -0.003 min
Response: 24274288
Conc: 5.76 ng/ml

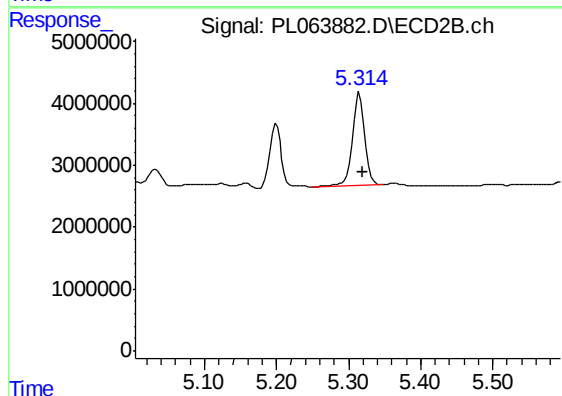

#4 Heptachlor

R.T.: 5.315 min
Delta R.T.: -0.003 min
Response: 18005544
Conc: 5.64 ng/ml

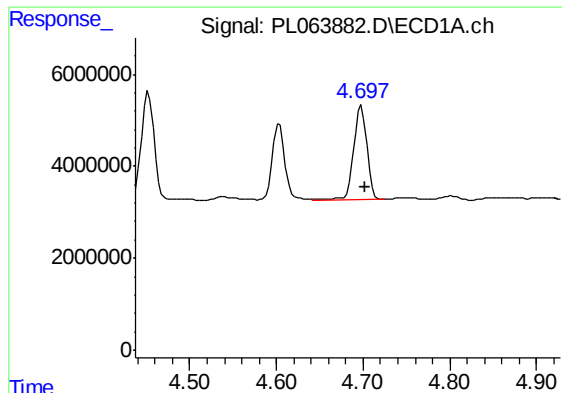


#5 Aldrin

R.T.: 4.698 min
Delta R.T.: -0.004 min
Response: 22028931
Conc: 5.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

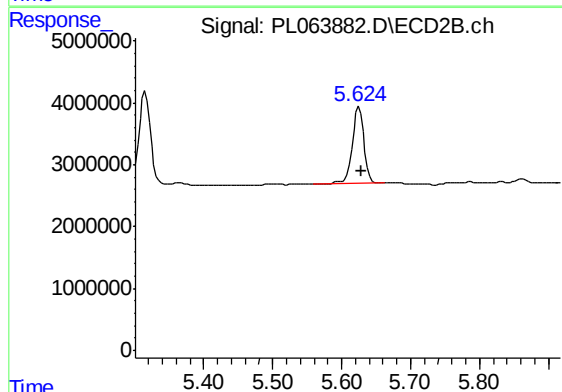


#5 Aldrin

R.T.: 5.625 min
Delta R.T.: -0.004 min
Response: 14872314
Conc: 5.20 ng/ml

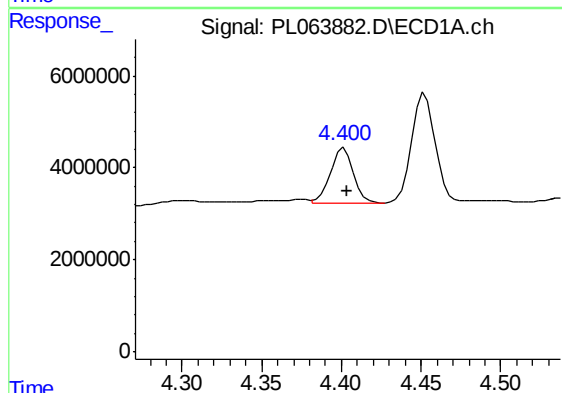


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.002 min
Response: 12342598
Conc: 6.39 ng/ml

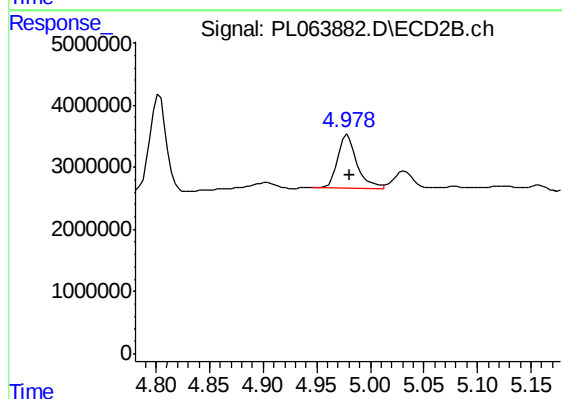

#6 beta-BHC

R.T.: 4.979 min
Delta R.T.: -0.002 min
Response: 10440338
Conc: 5.95 ng/ml




#7 delta-BHC

R.T.: 4.604 min
Delta R.T.: -0.003 min
Response: 16834752
Conc: 3.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

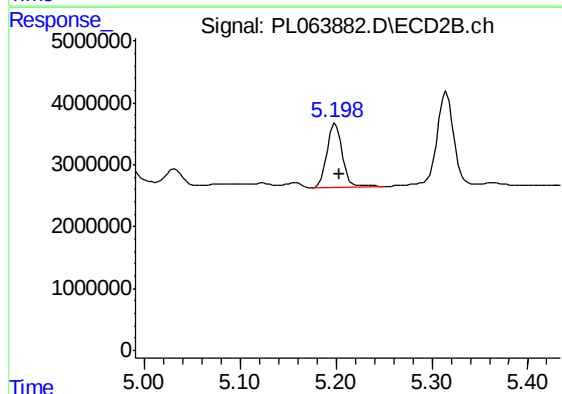


#7 delta-BHC

R.T.: 5.200 min
Delta R.T.: -0.004 min
Response: 11635751
Conc: 3.54 ng/ml




#8 Heptachlor epoxide

R.T.: 5.140 min
Delta R.T.: -0.004 min
Response: 21976371
Conc: 5.85 ng/ml

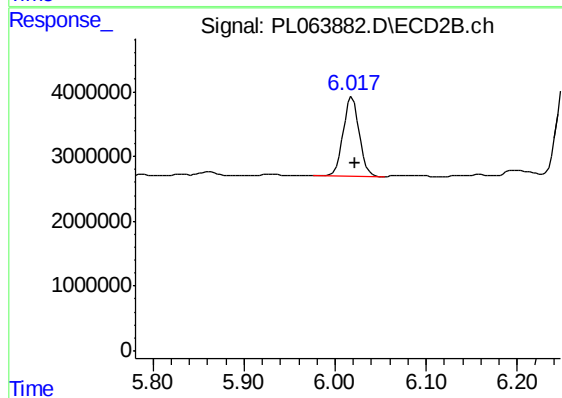

#8 Heptachlor epoxide

R.T.: 6.019 min
Delta R.T.: -0.004 min
Response: 14744325
Conc: 5.31 ng/ml




#9 Endosulfan I

R.T.: 5.476 min
Delta R.T.: -0.004 min
Response: 22176964
Conc: 6.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

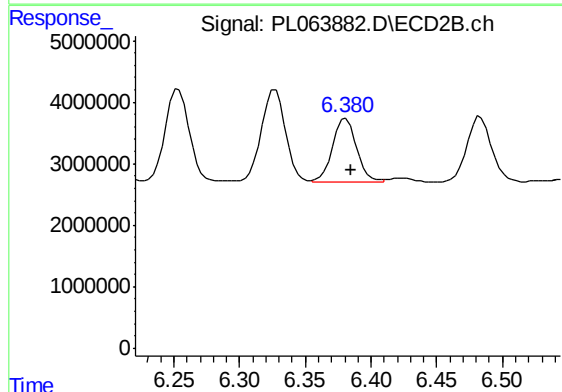


#9 Endosulfan I

R.T.: 6.381 min
Delta R.T.: -0.003 min
Response: 13425200
Conc: 5.34 ng/ml

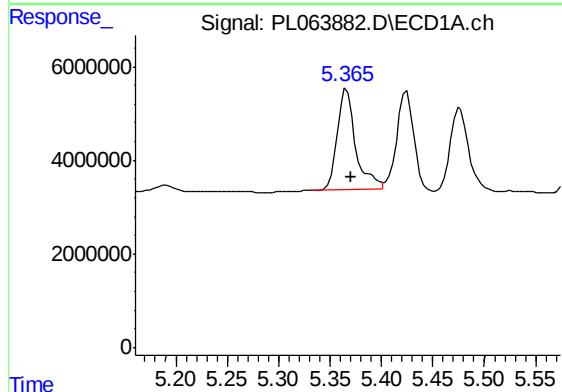


#10 gamma-Chlordane

R.T.: 5.365 min
Delta R.T.: -0.005 min
Response: 27507620
Conc: 7.24 ng/ml m

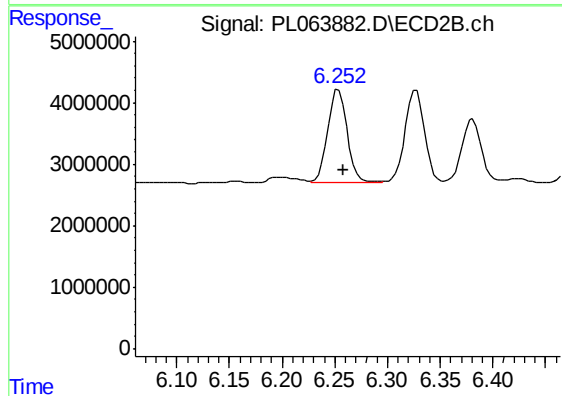

#10 gamma-Chlordane

R.T.: 6.253 min
Delta R.T.: -0.004 min
Response: 19809757
Conc: 7.16 ng/ml




#11 alpha-Chlordane

R.T.: 5.424 min
Delta R.T.: -0.004 min
Response: 25515234
Conc: 6.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

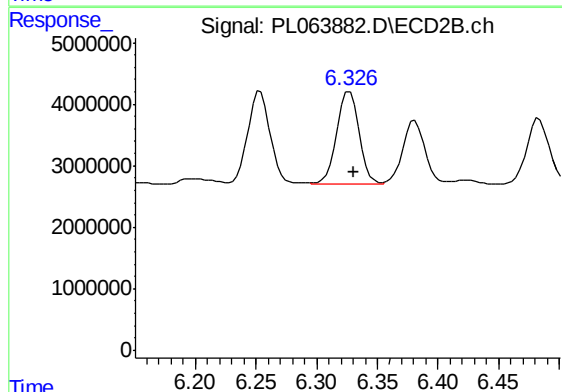


#11 alpha-Chlordane

R.T.: 6.327 min
Delta R.T.: -0.003 min
Response: 19668456
Conc: 7.13 ng/ml

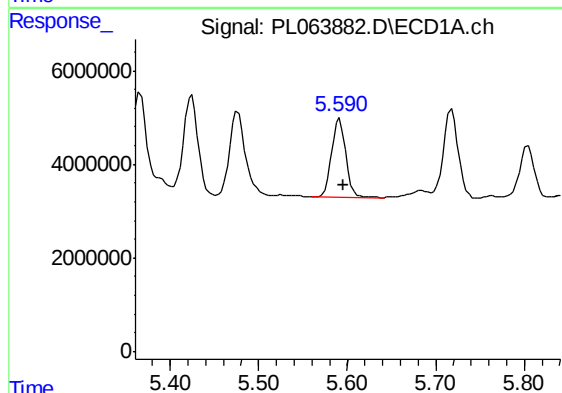


#12 4,4'-DDE

R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 18783831
Conc: 5.46 ng/ml

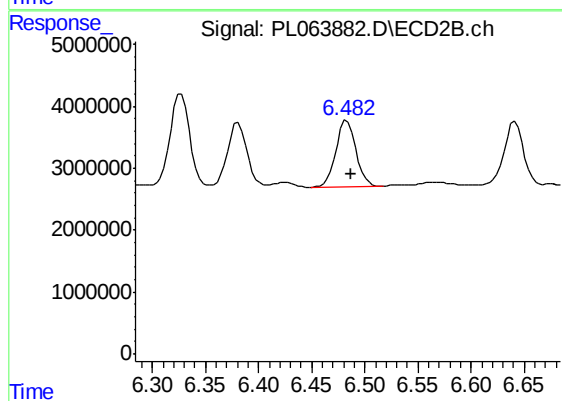

#12 4,4'-DDE

R.T.: 6.483 min
Delta R.T.: -0.003 min
Response: 14063386
Conc: 5.69 ng/ml

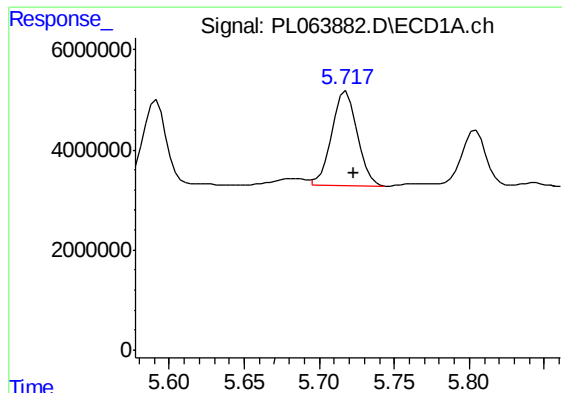


#13 Dieldrin

R.T.: 5.717 min
Delta R.T.: -0.006 min
Response: 22240739
Conc: 6.14 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

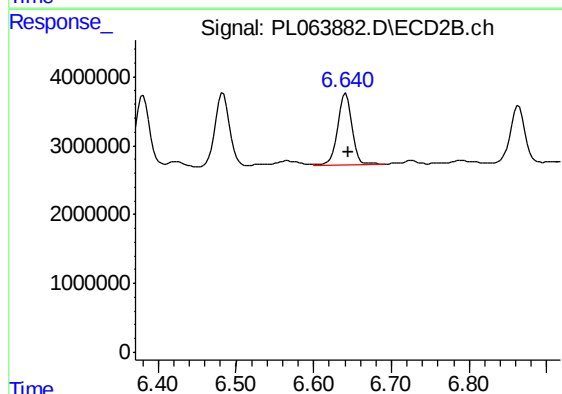


#13 Dieldrin

R.T.: 6.641 min
Delta R.T.: -0.004 min
Response: 13277540
Conc: 5.10 ng/ml

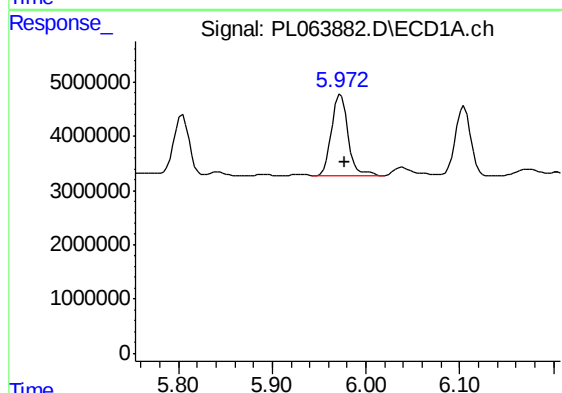


#14 Endrin

R.T.: 5.973 min
Delta R.T.: -0.004 min
Response: 18177721
Conc: 6.24 ng/ml

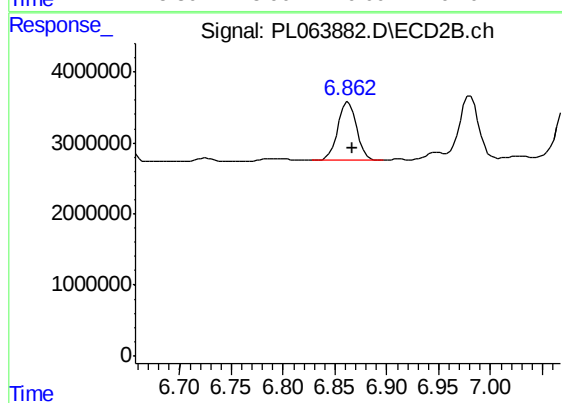

#14 Endrin

R.T.: 6.863 min
Delta R.T.: -0.004 min
Response: 10500759
Conc: 5.41 ng/ml




#15 Endosulfan II

R.T.: 6.246 min
Delta R.T.: -0.004 min
Response: 17632891
Conc: 5.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

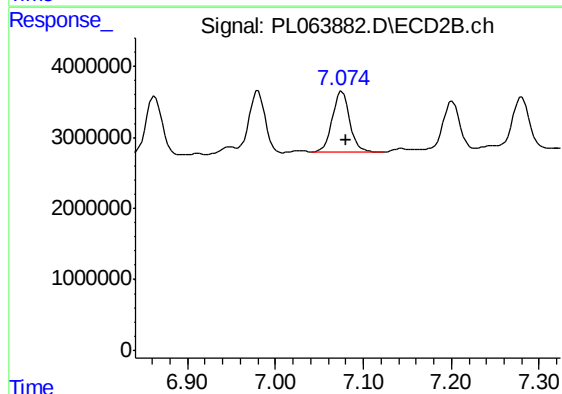


#15 Endosulfan II

R.T.: 7.076 min
Delta R.T.: -0.004 min
Response: 11900765
Conc: 5.05 ng/ml




#16 4,4'-DDD

R.T.: 6.105 min
Delta R.T.: -0.004 min
Response: 14544054
Conc: 4.97 ng/ml

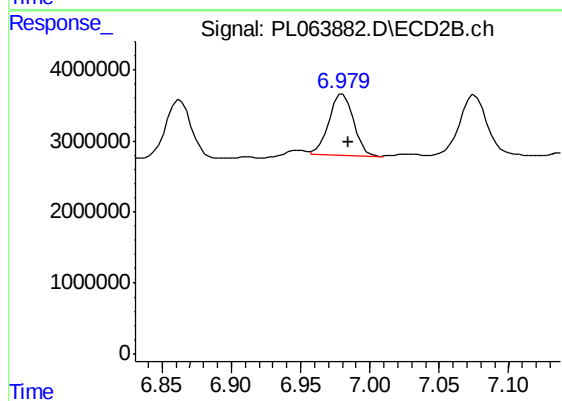

#16 4,4'-DDD

R.T.: 6.981 min
Delta R.T.: -0.004 min
Response: 10759890
Conc: 5.09 ng/ml




#17 4,4'-DDT

R.T.: 6.345 min
Delta R.T.: -0.005 min
Response: 15590734
Conc: 5.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

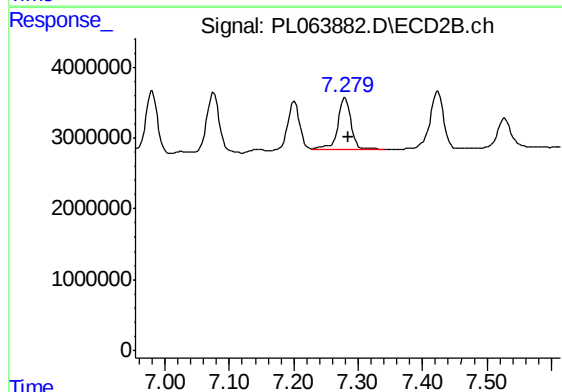


#17 4,4'-DDT

R.T.: 7.280 min
Delta R.T.: -0.004 min
Response: 10670955
Conc: 5.49 ng/ml

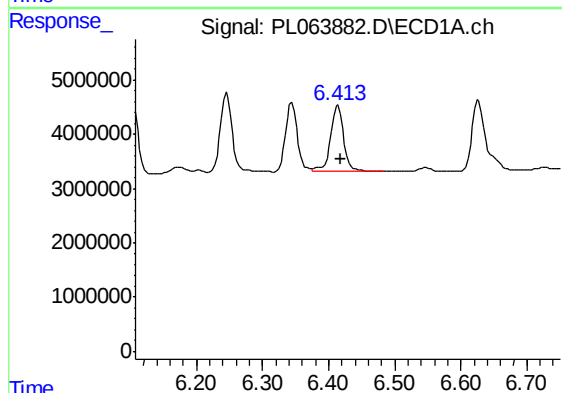


#18 Endrin aldehyde

R.T.: 6.414 min
Delta R.T.: -0.005 min
Response: 16928334
Conc: 6.12 ng/ml

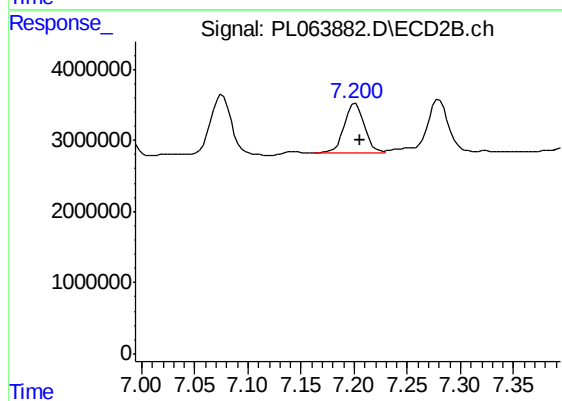

#18 Endrin aldehyde

R.T.: 7.201 min
Delta R.T.: -0.004 min
Response: 8903679
Conc: 4.42 ng/ml




#19 Endosulfan Sulfate

R.T.: 6.627 min
Delta R.T.: -0.005 min
Response: 19246695
Conc: 6.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

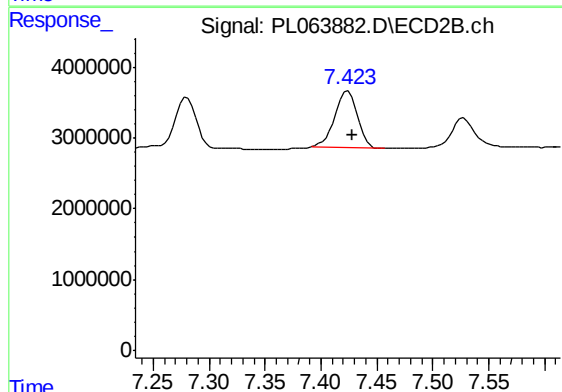


#19 Endosulfan Sulfate

R.T.: 7.424 min
Delta R.T.: -0.004 min
Response: 10986888
Conc: 4.89 ng/ml




#20 Methoxychlor

R.T.: 6.892 min
Delta R.T.: -0.005 min
Response: 8586276
Conc: 6.54 ng/ml m

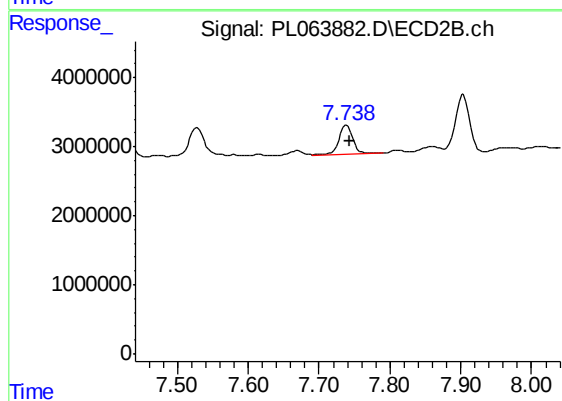

#20 Methoxychlor

R.T.: 7.739 min
Delta R.T.: -0.004 min
Response: 5585467
Conc: 5.29 ng/ml




#21 Endrin ketone

R.T.: 7.114 min
Delta R.T.: -0.005 min
Response: 16423063
Conc: 4.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS


Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

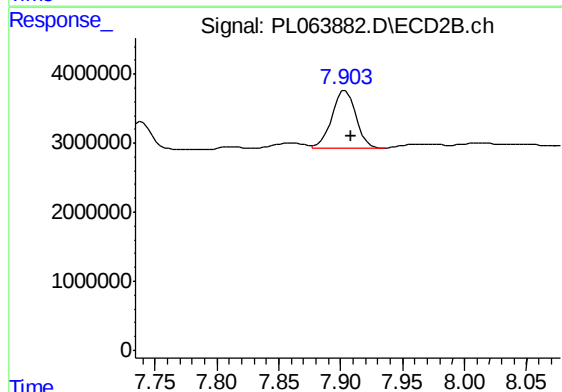


#21 Endrin ketone

R.T.: 7.904 min
Delta R.T.: -0.005 min
Response: 11458148
Conc: 4.65 ng/ml




#22 Mirex

R.T.: 7.301 min
Delta R.T.: -0.006 min
Response: 14556670
Conc: 5.80 ng/ml

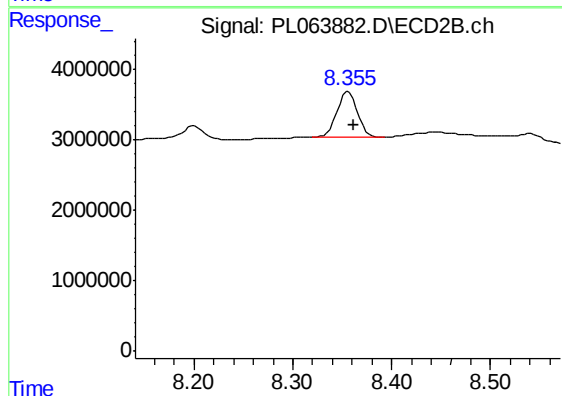

#22 Mirex

R.T.: 8.356 min
Delta R.T.: -0.005 min
Response: 9519613
Conc: 5.28 ng/ml

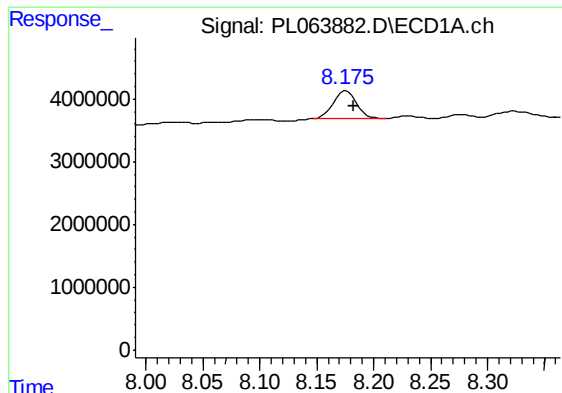


#28 Decachlorobiphenyl

R.T.: 8.176 min
Delta R.T.: -0.006 min
Response: 6342179
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-123020MS

Manual Integrations
APPROVED

Ankita
1/4/2021 2:25:54 PM

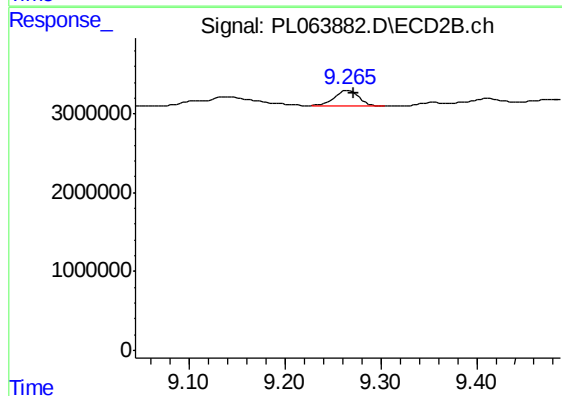

#28 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.007 min
Response: 3469950
Conc: 1.76 ng/ml m