

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033120\
 Data File : PL057684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2020 12:57
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 05:21:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.956	239.5E6	47229949	25.833	21.769
28)	SA Decachlor...	8.206	8.977	224.8E6	46055353	21.243	20.770
Target Compounds							
2)	A alpha-BHC	3.894	0.000	6403392	0	0.402	N.D. #
4)	MA Heptachlor	0.000	5.139	0	691418	N.D.	0.220 #
15)	B Endosulfa...	6.275	0.000	2033696	0	0.187	N.D. #
20)	A Methoxychlor	6.937f	0.000	299626	0	0.056	N.D. #
22)	Mirex	7.335	0.000	604389	0	0.075	N.D. #
23)	Chlordane-1	4.356f	0.000	2596019	0	7.998	N.D. #
24)	Chlordane-2	4.833	0.000	2503872	0	6.891	N.D. #
27)	Chlordane-5	6.275	0.000	2033696	0	5.589	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033120\
Data File : PL057684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2020 12:57
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 05:21:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

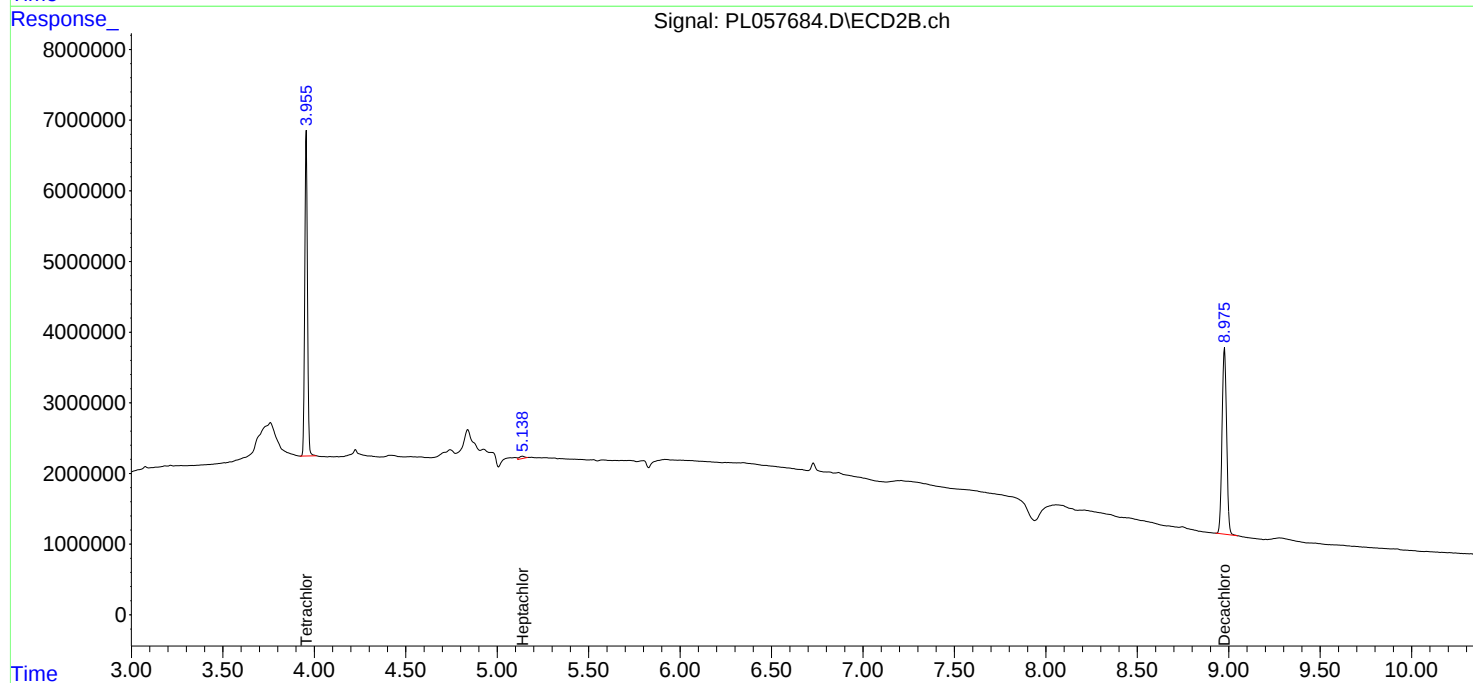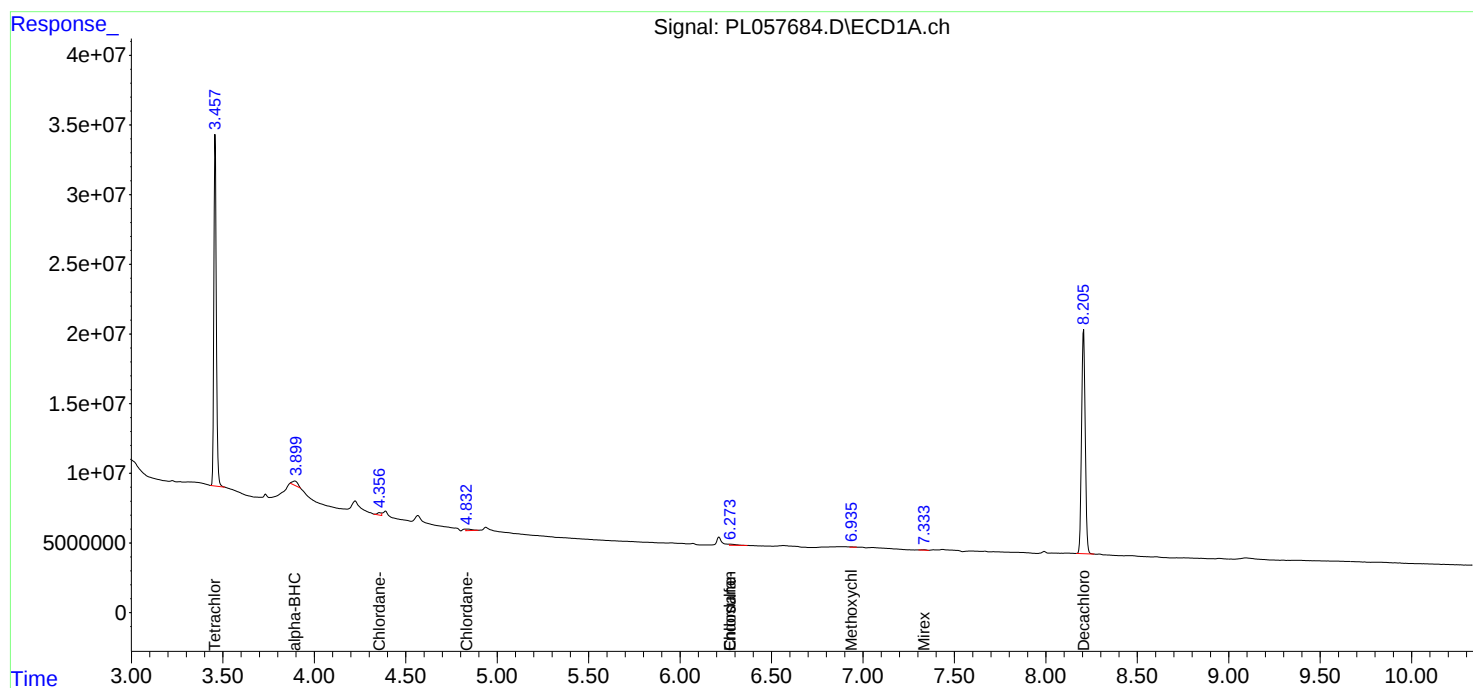


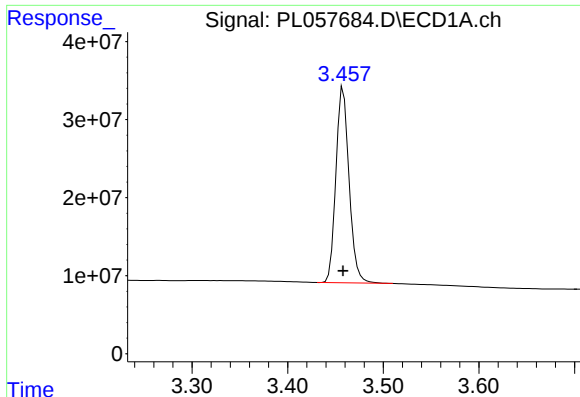

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 239458265
Conc: 25.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

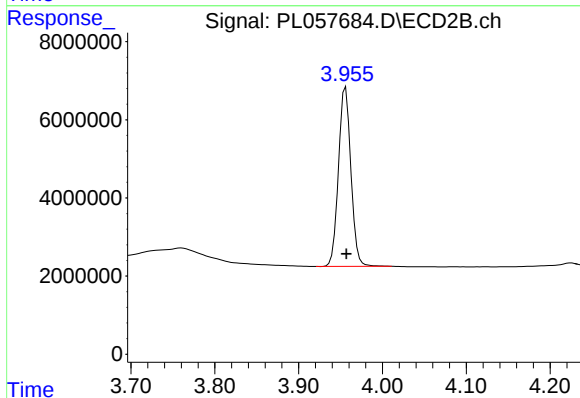


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 47229949
Conc: 21.77 ng/ml

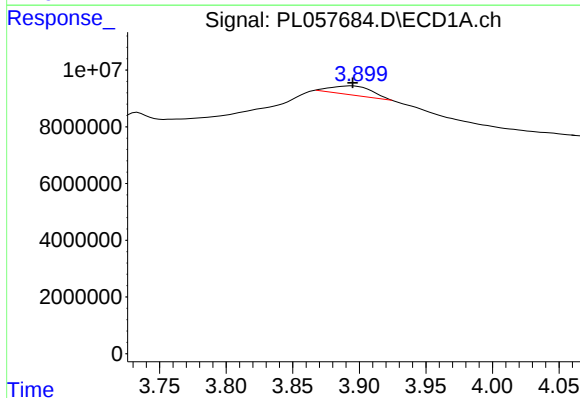


#2 alpha-BHC

R.T.: 3.894 min
Delta R.T.: 0.000 min
Response: 6403392
Conc: 0.40 ng/ml

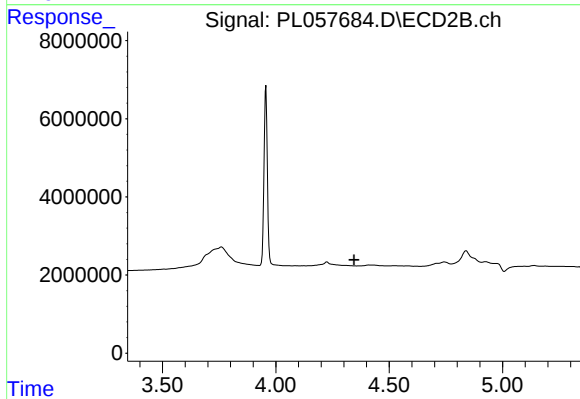

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

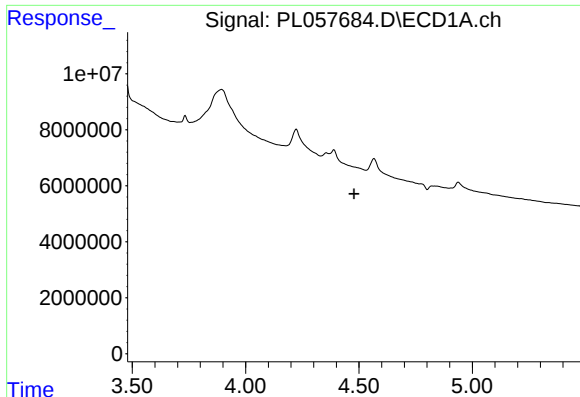

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

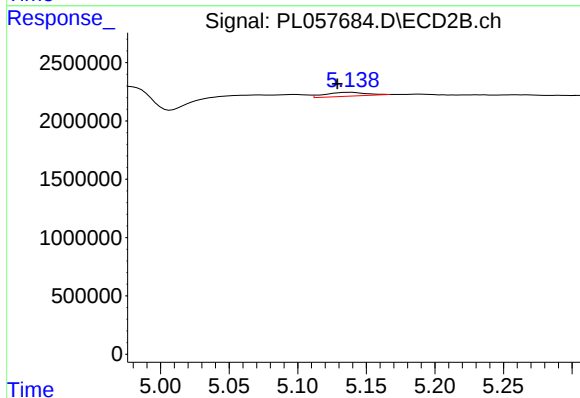


#4 Heptachlor

R.T.: 5.139 min
Delta R.T.: 0.010 min
Response: 691418
Conc: 0.22 ng/ml

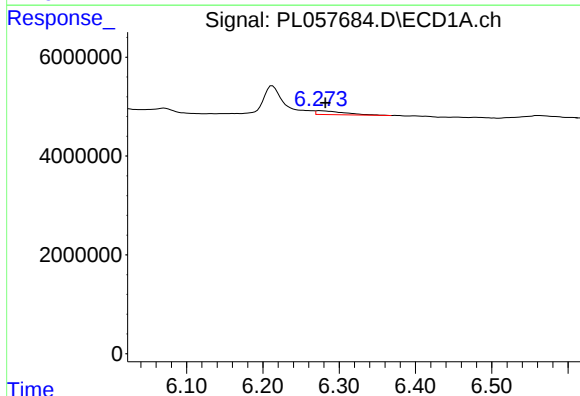


#15 Endosulfan II

R.T.: 6.275 min
Delta R.T.: -0.007 min
Response: 2033696
Conc: 0.19 ng/ml

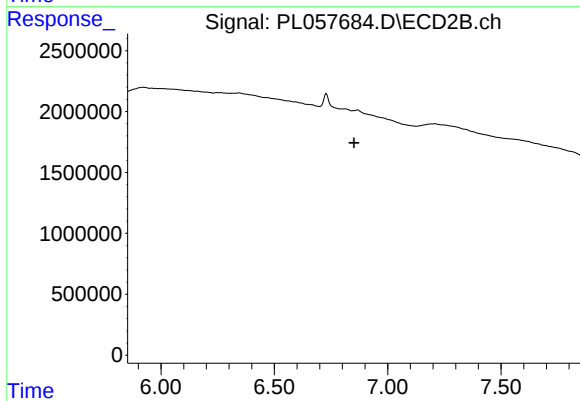

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

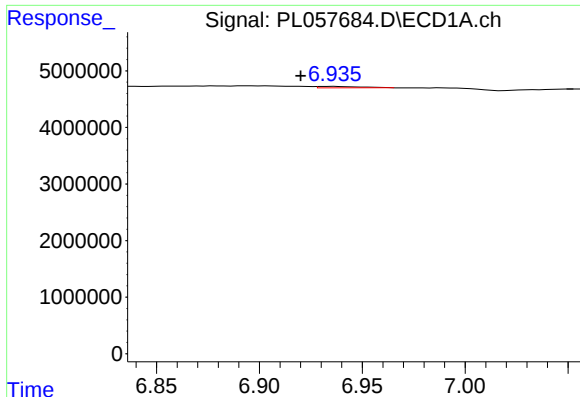

#20 Methoxychlor


R.T.: 6.937 min
Delta R.T.: 0.017 min
Response: 299626
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

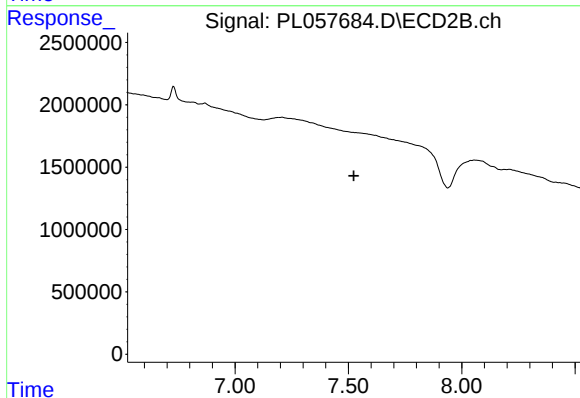


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.524 min
Response: 0
Conc: N.D.

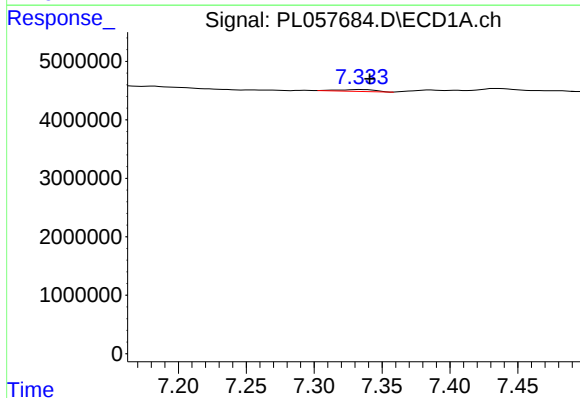


#22 Mirex

R.T.: 7.335 min
Delta R.T.: -0.006 min
Response: 604389
Conc: 0.07 ng/ml

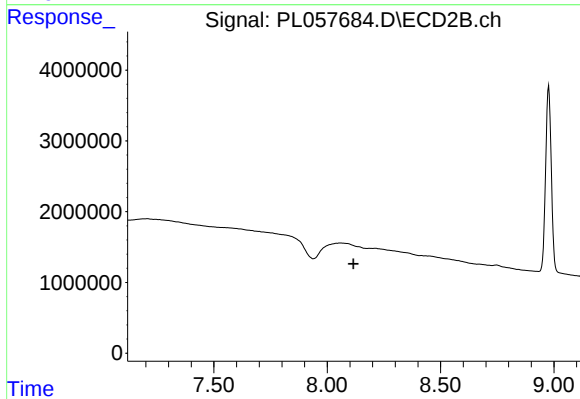

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

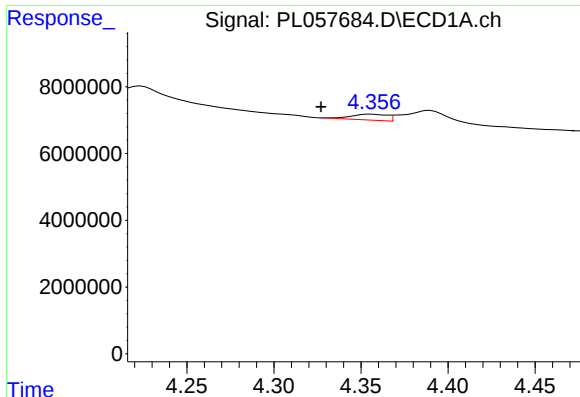

#23 Chlordane-1


R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 2596019
Conc: 8.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

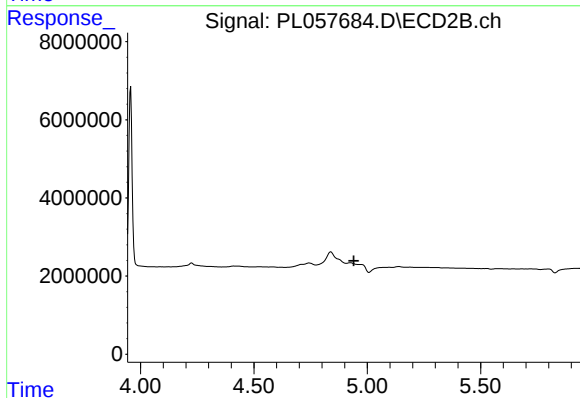


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

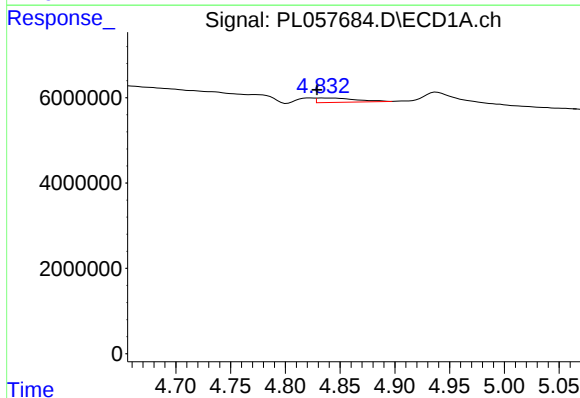


#24 Chlordane-2

R.T.: 4.833 min
Delta R.T.: 0.004 min
Response: 2503872
Conc: 6.89 ng/ml

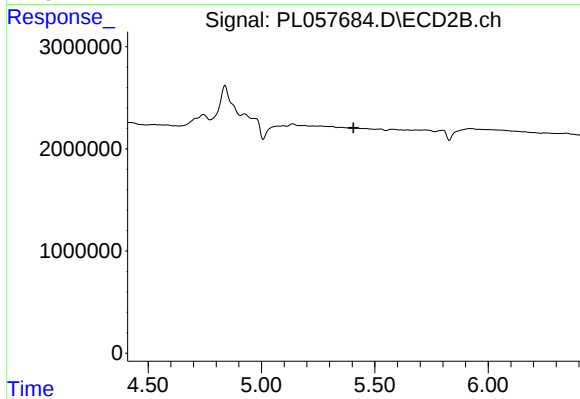

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

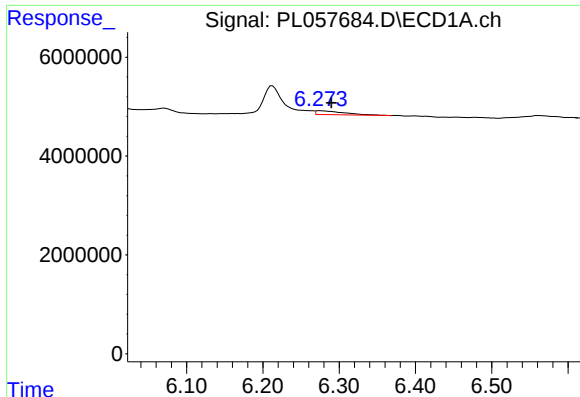

#27 Chlordane-5


R.T.: 6.275 min
Delta R.T.: -0.015 min
Response: 2033696
Conc: 5.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

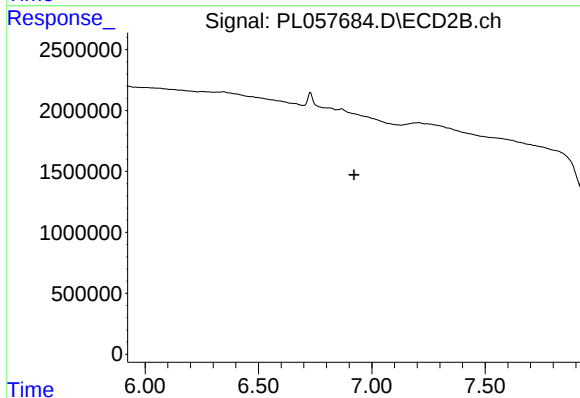


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

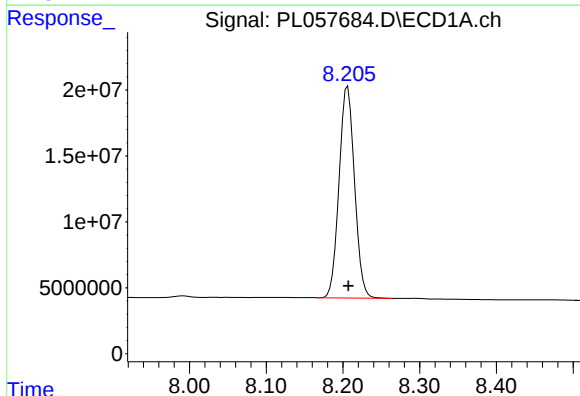

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 224780497
Conc: 21.24 ng/ml

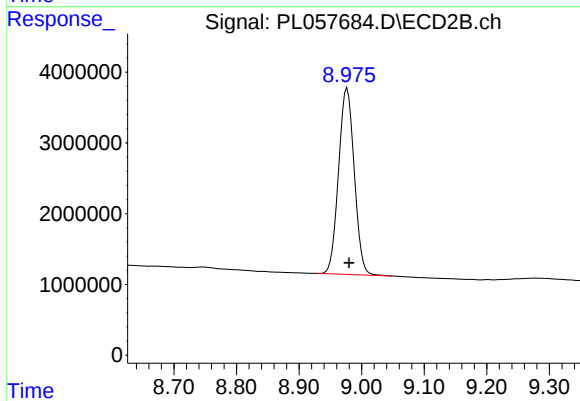

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.003 min
Response: 46055353
Conc: 20.77 ng/ml