

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033120\
 Data File : PL057696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2020 17:24
 Operator : AJ\MA
 Sample : L1752-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-033020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 05:27:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	236.2E6	48462891	25.480	22.338
28)	SA Decachlor...	8.206	8.979	182.1E6	41928546	17.207	18.909
Target Compounds							
4)	MA Heptachlor	0.000	5.140	0	1070748	N.D.	0.340 #
5)	MB Aldrin	4.715	0.000	1898159	0	0.138	N.D. #
15)	B Endosulfa...	6.292	0.000	3338438	0	0.307	N.D. #
16)	A 4,4'-DDD	6.129	0.000	504965	0	0.052	N.D. #
22)	Mirex	7.342	0.000	681112	0	0.084	N.D. #
23)	Chlordane-1	4.351f	0.000	1968233	0	6.064	N.D. #
24)	Chlordane-2	4.853f	0.000	10325058	0	28.415	N.D. #
27)	Chlordane-5	6.292	0.000	3338438	0	9.175	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033120\
Data File : PL057696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2020 17:24
Operator : AJ\MA
Sample : L1752-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HD-02-033020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 05:27:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

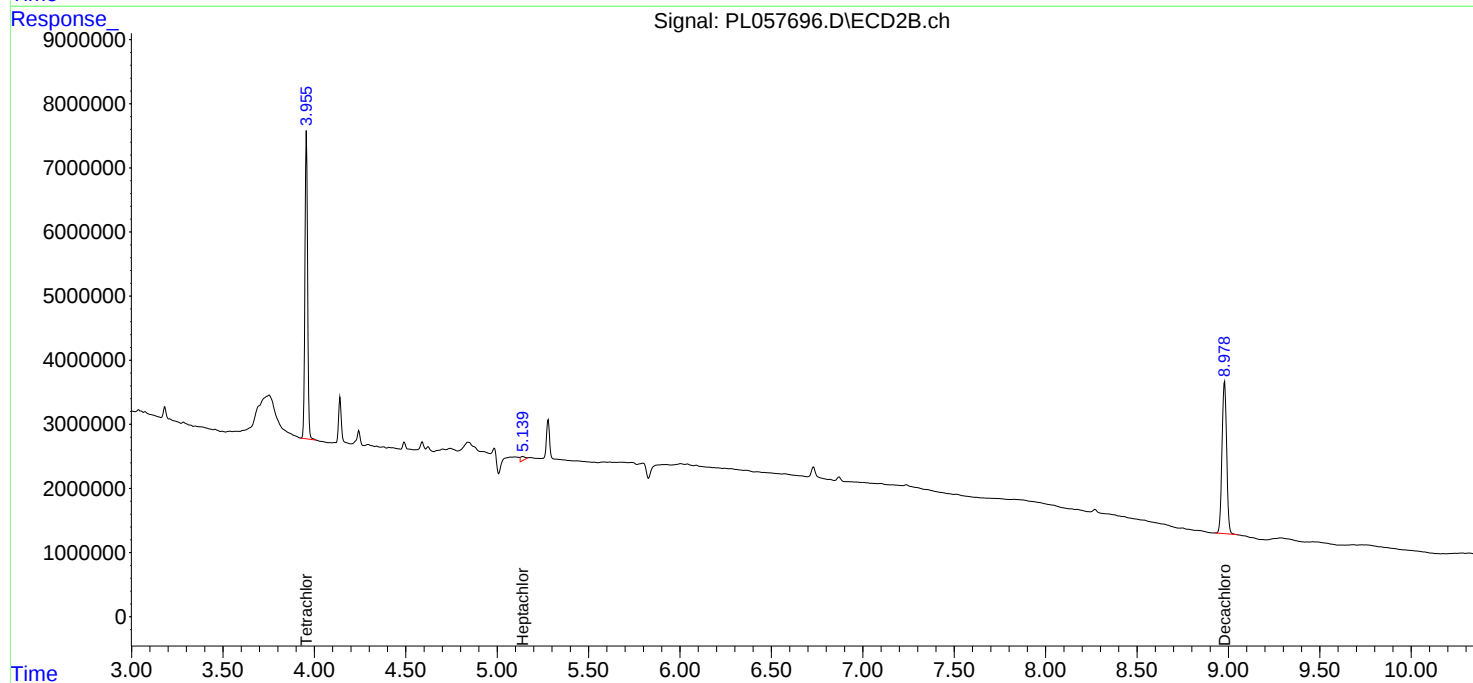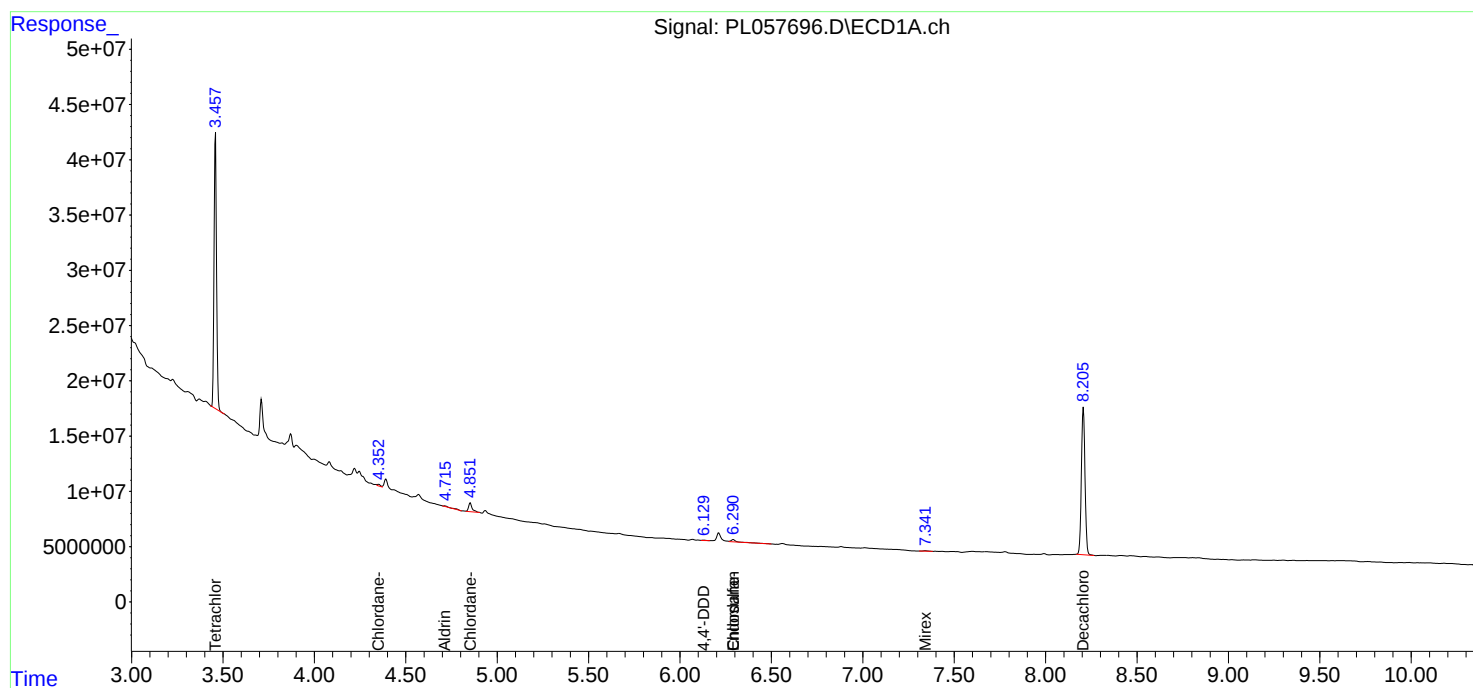


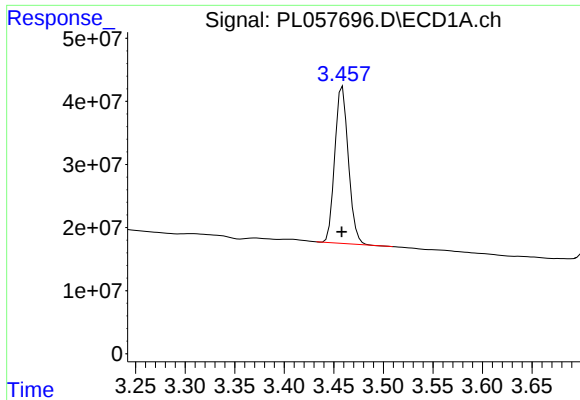

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 236182150
Conc: 25.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-033020

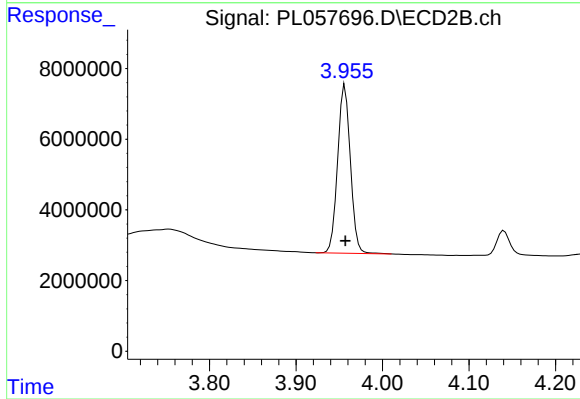


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 48462891
Conc: 22.34 ng/ml

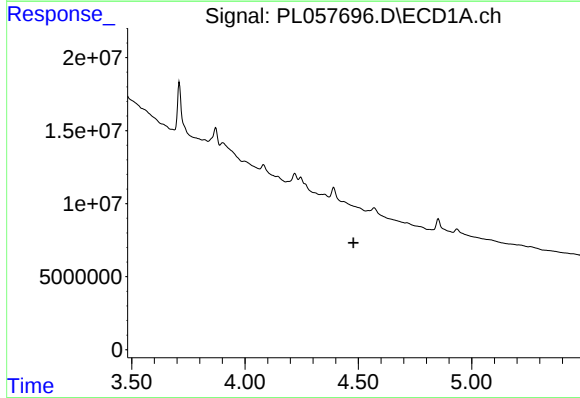


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

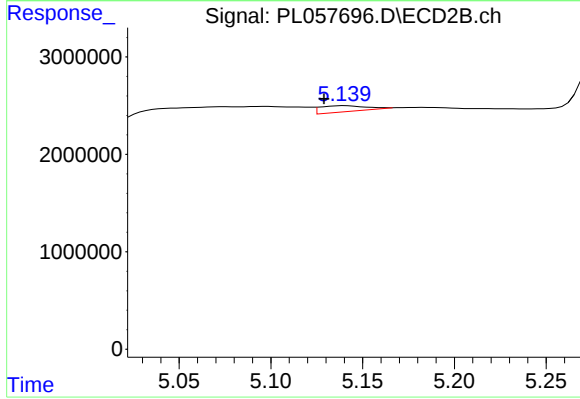

#4 Heptachlor


R.T.: 5.140 min
Delta R.T.: 0.011 min
Response: 1070748
Conc: 0.34 ng/ml

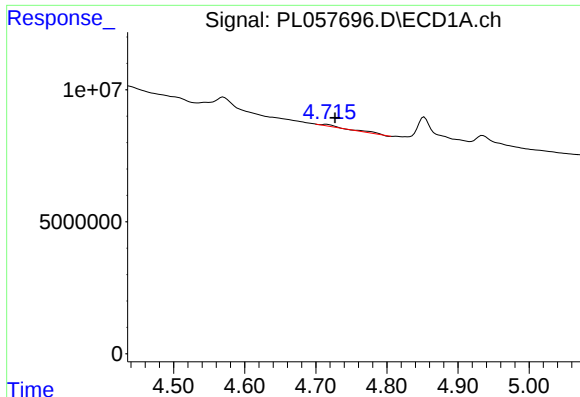

#5 Aldrin


R.T.: 4.715 min
Delta R.T.: -0.012 min
Response: 1898159
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-033020

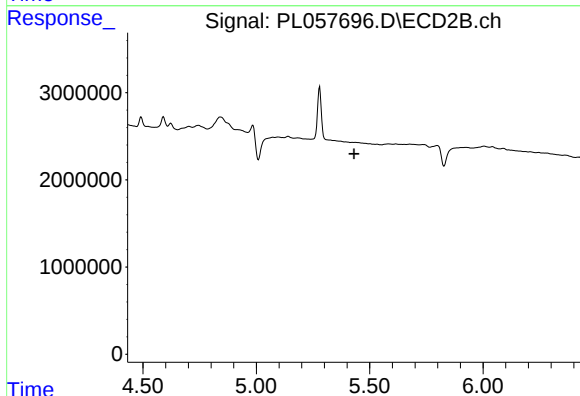


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

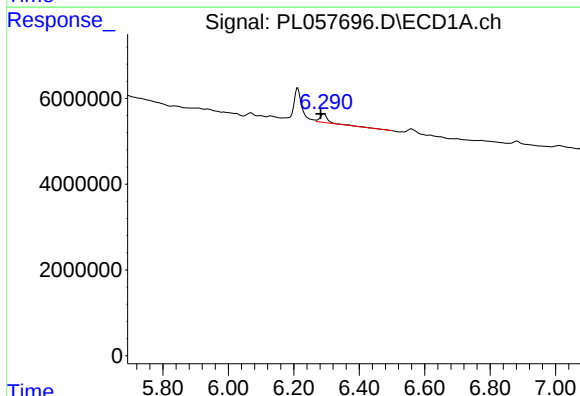


#15 Endosulfan II

R.T.: 6.292 min
Delta R.T.: 0.010 min
Response: 3338438
Conc: 0.31 ng/ml

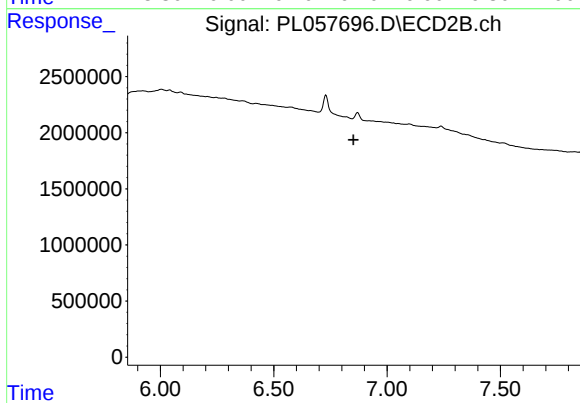

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

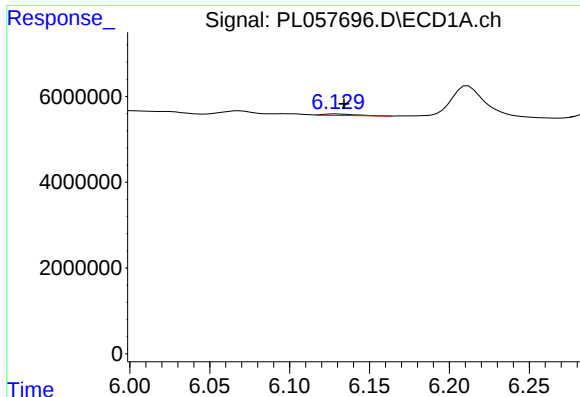

#16 4,4'-DDD


R.T.: 6.129 min
Delta R.T.: -0.005 min
Response: 504965
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-033020

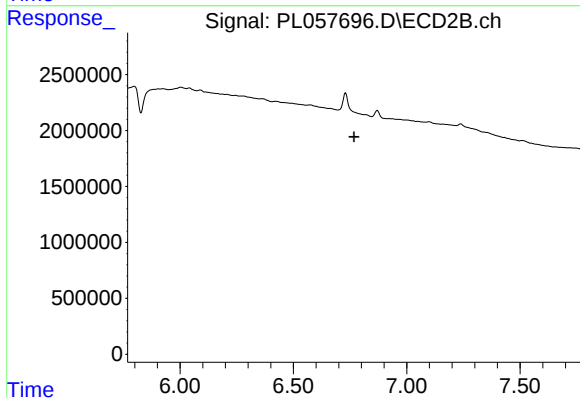


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

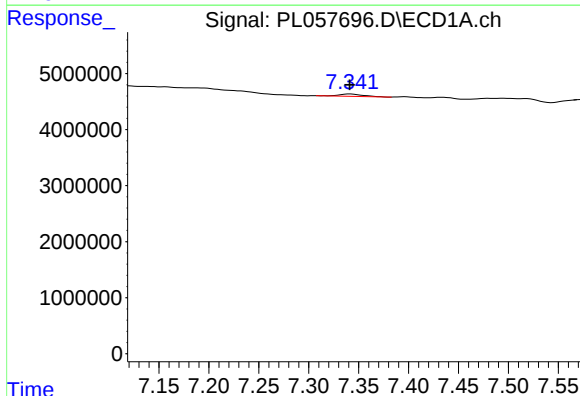


#22 Mirex

R.T.: 7.342 min
Delta R.T.: 0.001 min
Response: 681112
Conc: 0.08 ng/ml

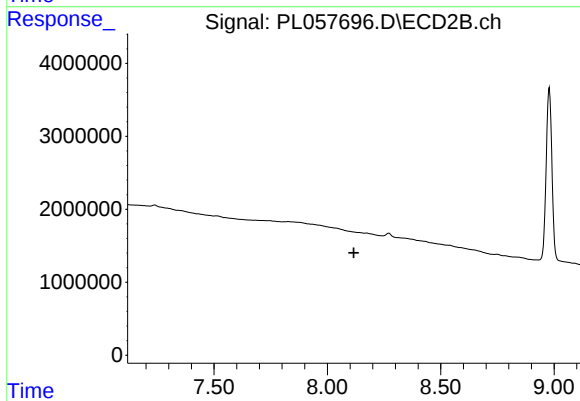

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

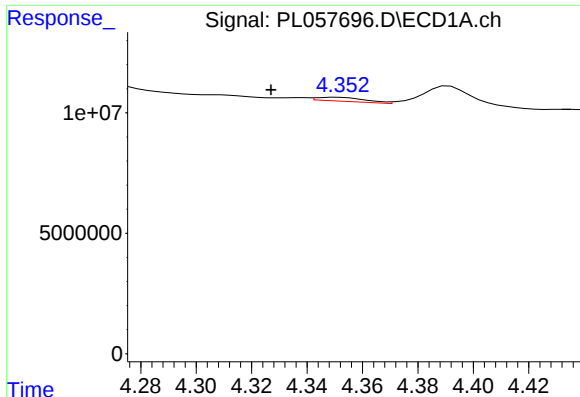

#23 Chlordane-1


R.T.: 4.351 min
Delta R.T.: 0.024 min
Response: 1968233
Conc: 6.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-033020

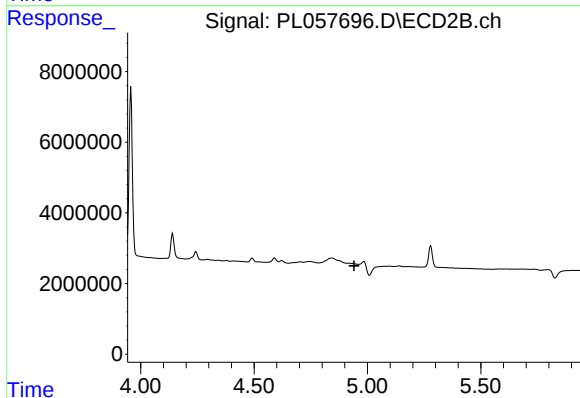


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

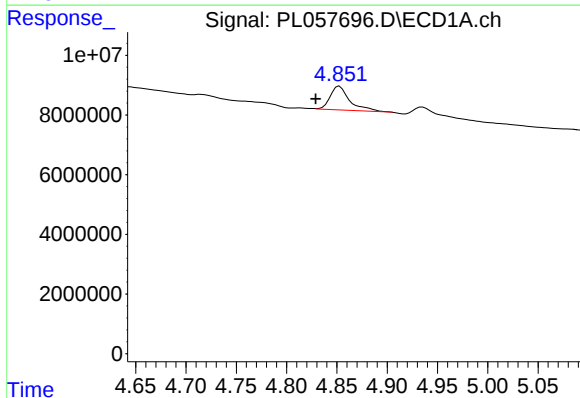


#24 Chlordane-2

R.T.: 4.853 min
Delta R.T.: 0.024 min
Response: 10325058
Conc: 28.41 ng/ml

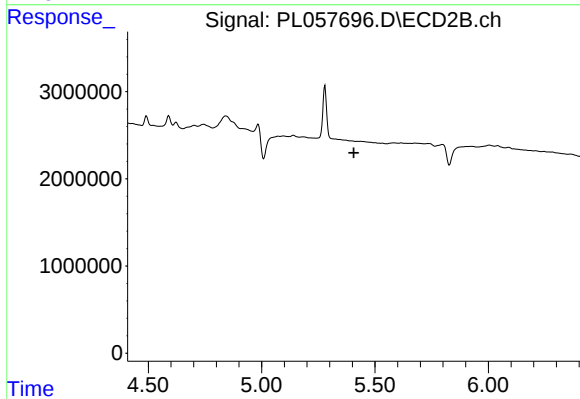

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

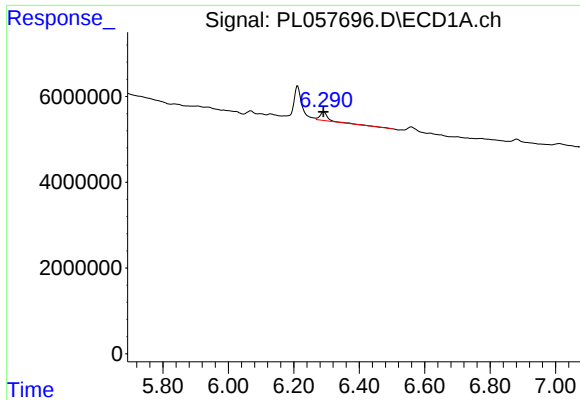

#27 Chlordane-5


R.T.: 6.292 min
Delta R.T.: 0.002 min
Response: 3338438
Conc: 9.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-033020

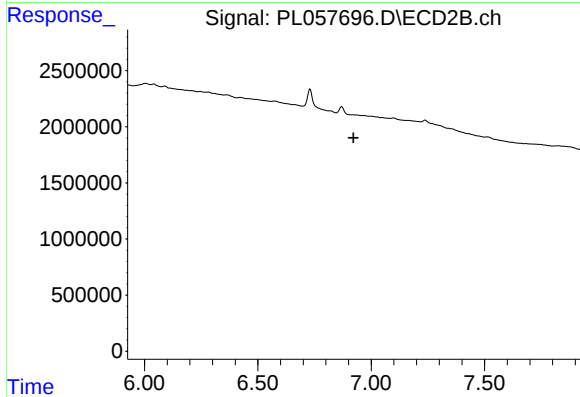


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

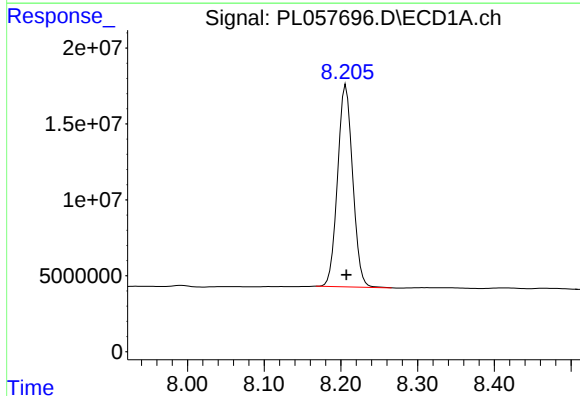

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 182076135
Conc: 17.21 ng/ml

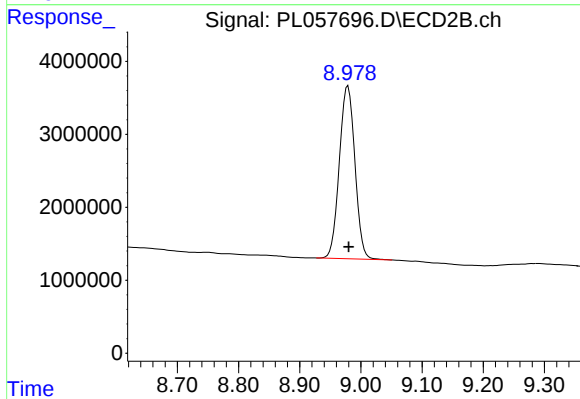

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.001 min
Response: 41928546
Conc: 18.91 ng/ml