

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033120\
 Data File : PL057707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2020 20:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 05:29:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	228.8E6	45679053	24.688	21.055
28)	SA Decachlor...	8.205	8.979	196.3E6	43288212	18.552	19.522
Target Compounds							
2)	A alpha-BHC	3.887	0.000	4430918	0	0.278	N.D. #
4)	MA Heptachlor	0.000	5.137	0	4020459	N.D.	1.277 #
14)	MA Endrin	6.007	0.000	369848	0	0.032	N.D. #
18)	B Endrin al...	6.451	0.000	586331	0	0.063	N.D. #
21)	B Endrin ke...	7.164	0.000	252982	0	0.022	N.D. #
22)	Mirex	7.337	0.000	617194	0	0.076	N.D. #
23)	Chlordane-1	4.354f	0.000	1864740	0	5.745	N.D. #
24)	Chlordane-2	4.830	0.000	3393259	0	9.338	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033120\
Data File : PL057707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2020 20:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 05:29:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

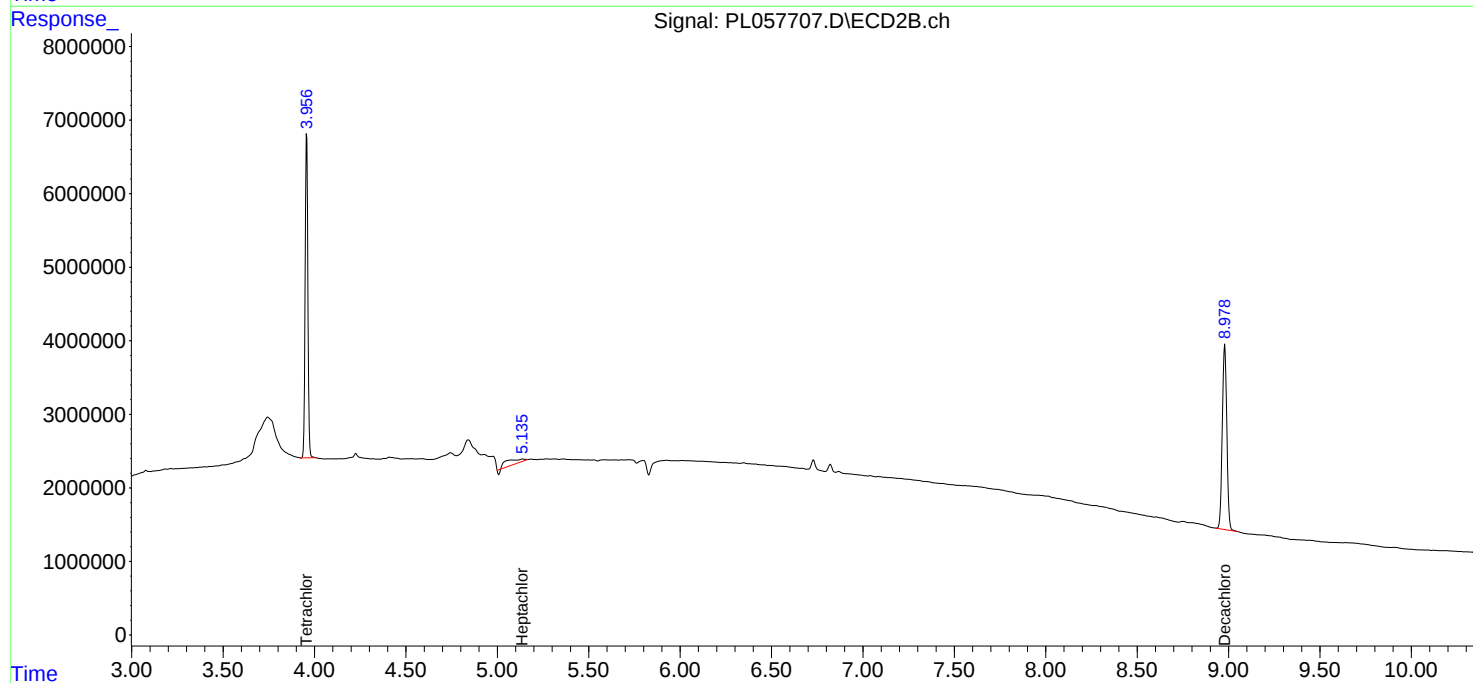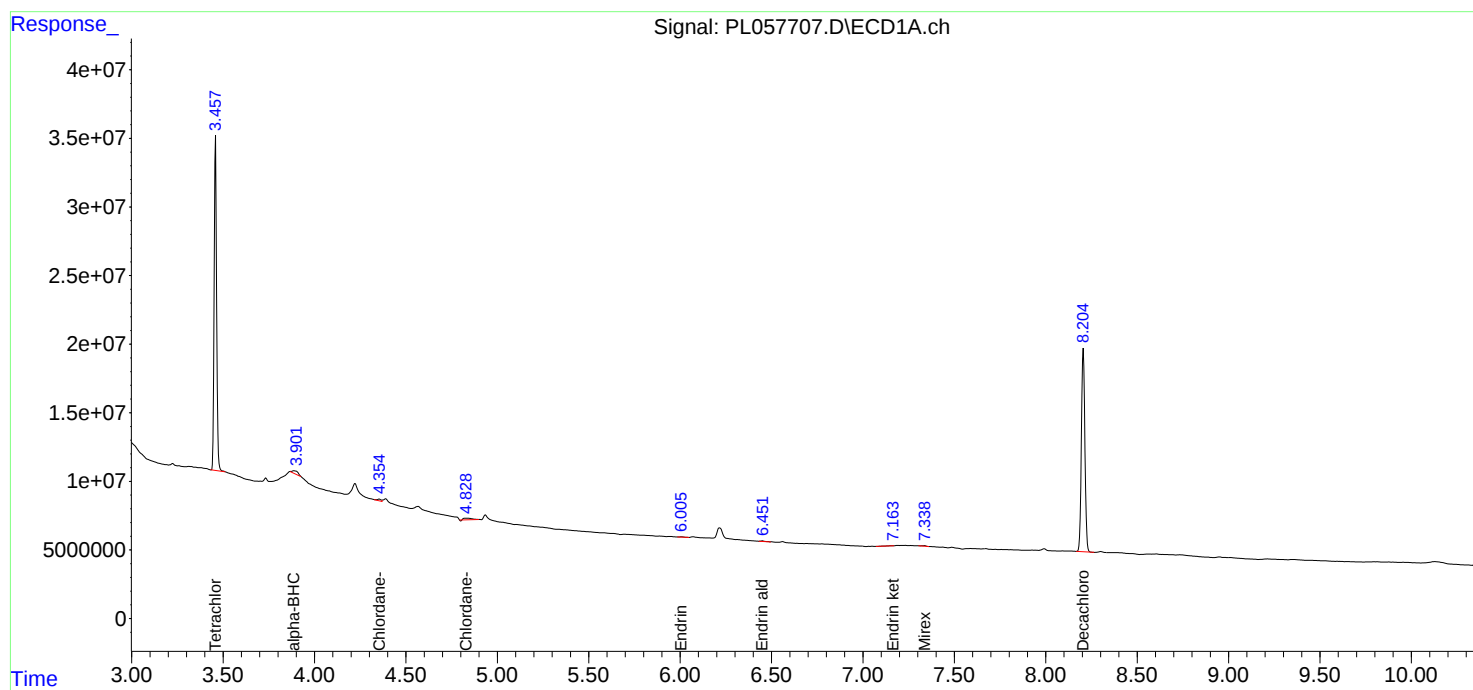


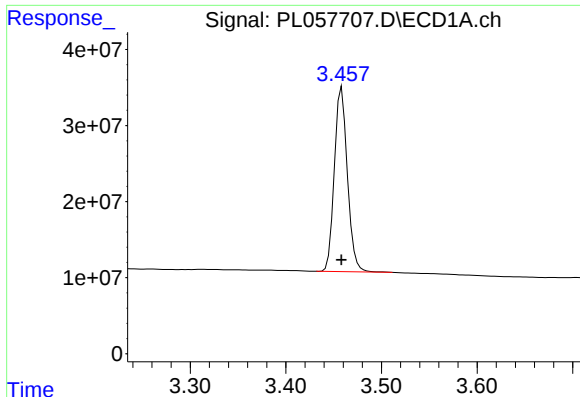

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 228847632
Conc: 24.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

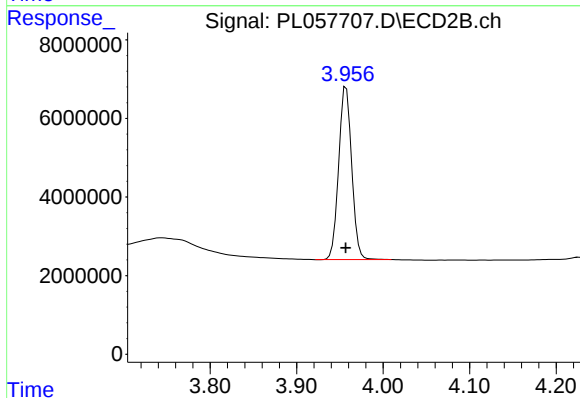


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 45679053
Conc: 21.05 ng/ml

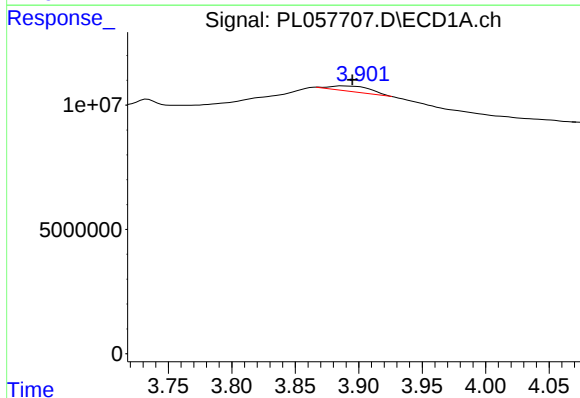


#2 alpha-BHC

R.T.: 3.887 min
Delta R.T.: -0.008 min
Response: 4430918
Conc: 0.28 ng/ml

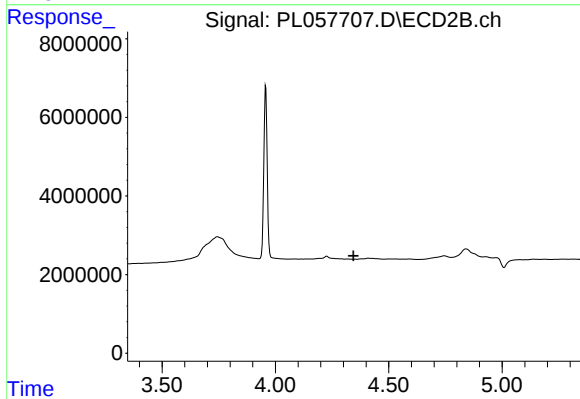

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

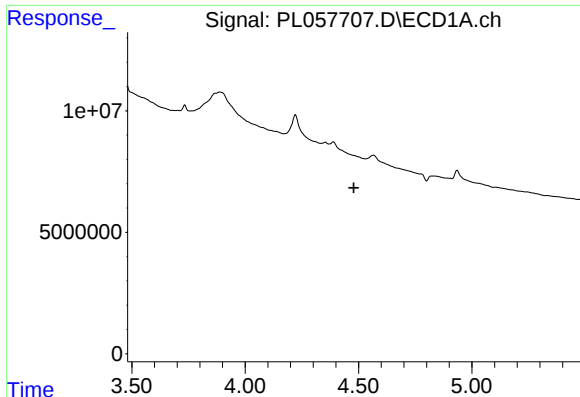

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

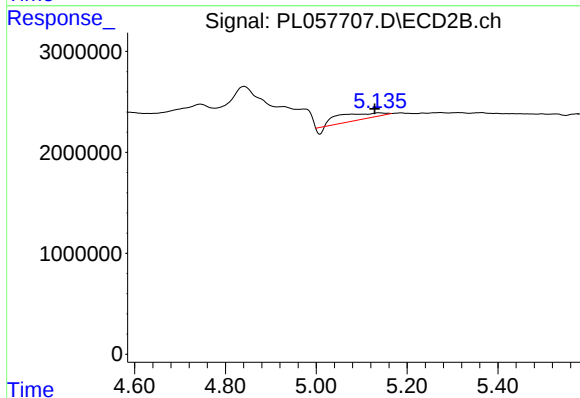


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 4020459
Conc: 1.28 ng/ml

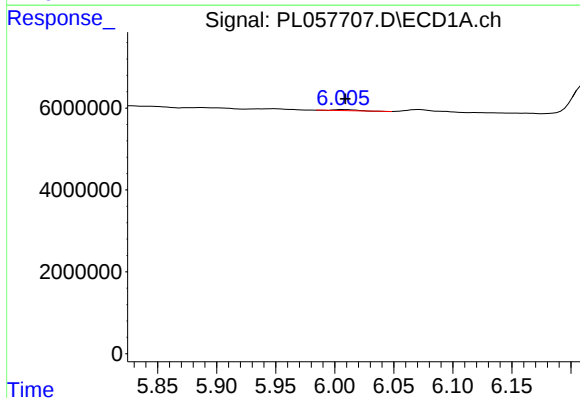


#14 Endrin

R.T.: 6.007 min
Delta R.T.: -0.002 min
Response: 369848
Conc: 0.03 ng/ml

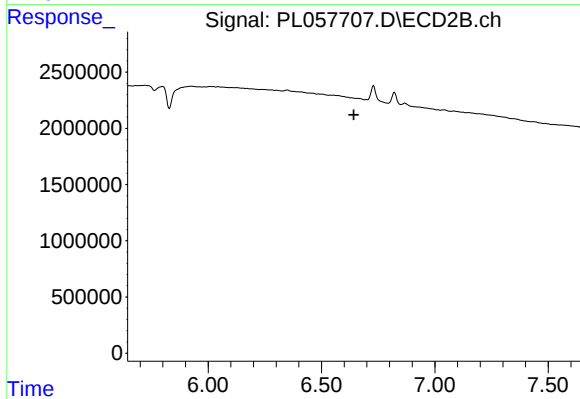

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

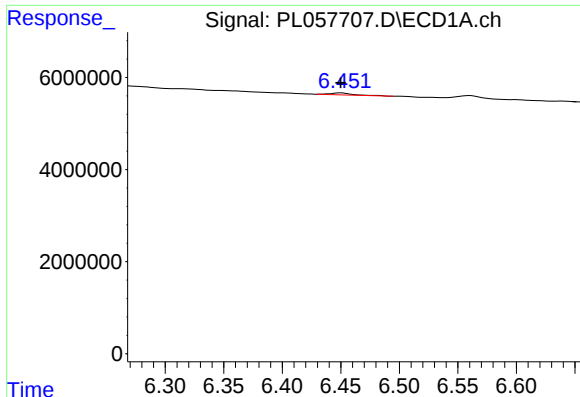

#18 Endrin aldehyde


R.T.: 6.451 min
Delta R.T.: 0.000 min
Response: 586331
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

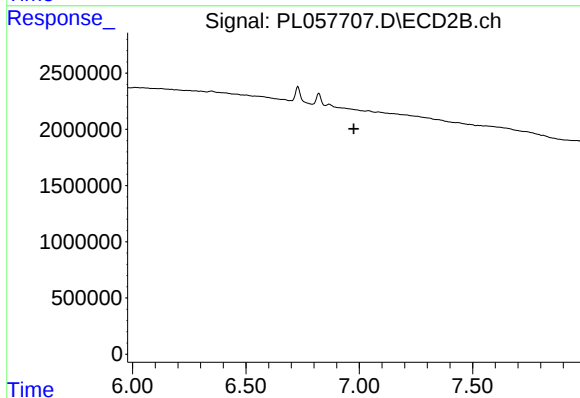


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

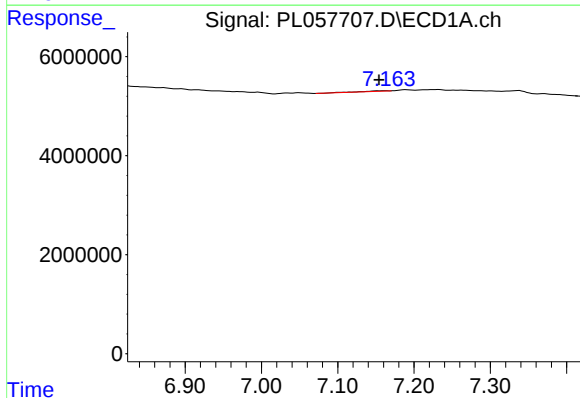


#21 Endrin ketone

R.T.: 7.164 min
Delta R.T.: 0.010 min
Response: 252982
Conc: 0.02 ng/ml

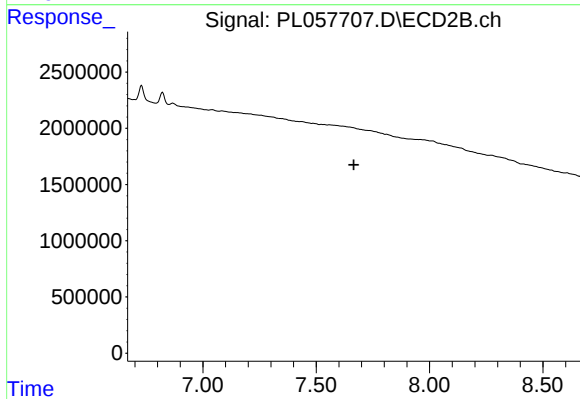

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.666 min
Response: 0
Conc: N.D.

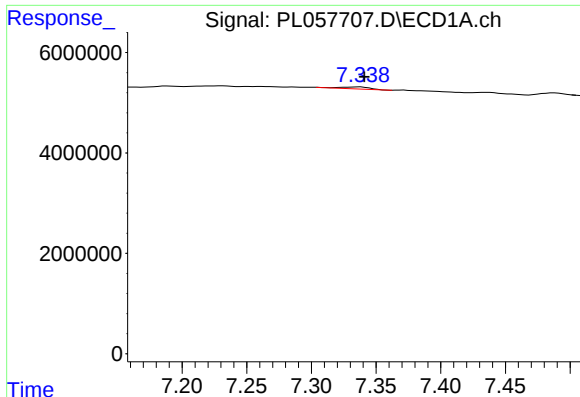

#22 Mirex


R.T.: 7.337 min
Delta R.T.: -0.004 min
Response: 617194
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

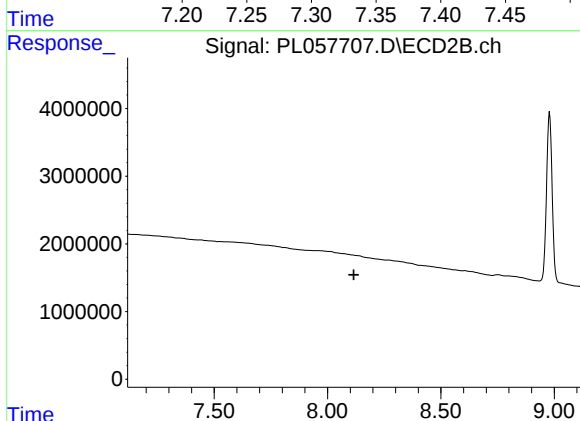


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

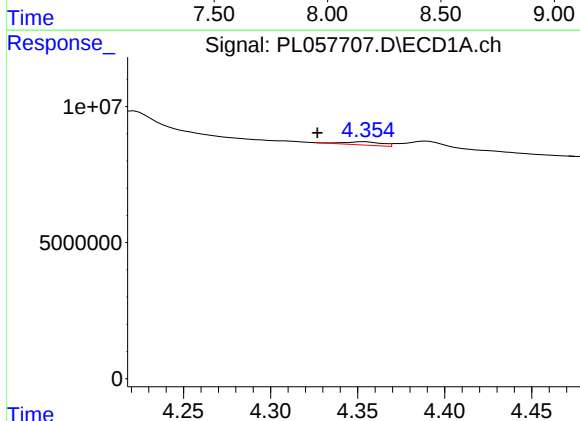


#23 Chlordane-1

R.T.: 4.354 min
Delta R.T.: 0.027 min
Response: 1864740
Conc: 5.75 ng/ml

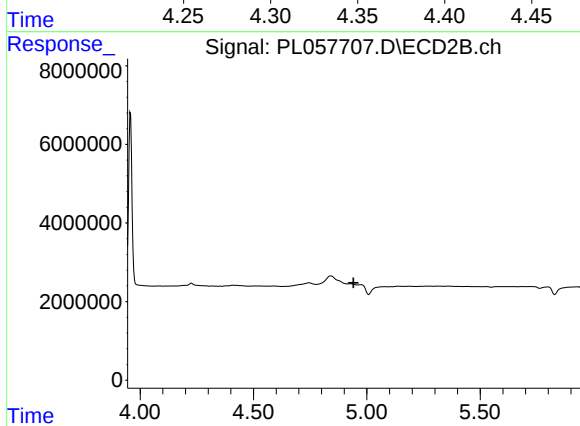

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

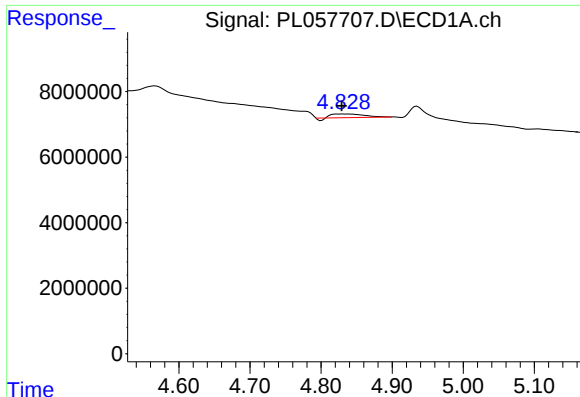

#24 Chlordane-2


R.T.: 4.830 min
Delta R.T.: 0.001 min
Response: 3393259
Conc: 9.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

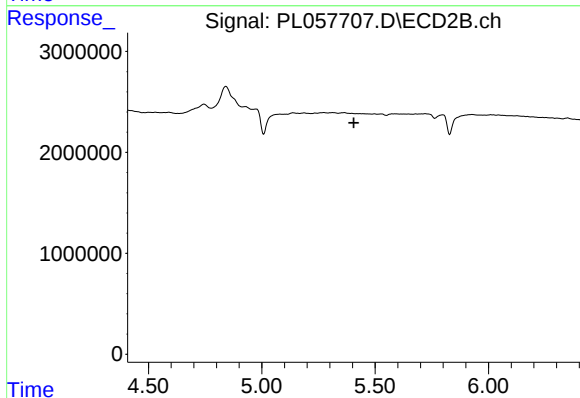


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

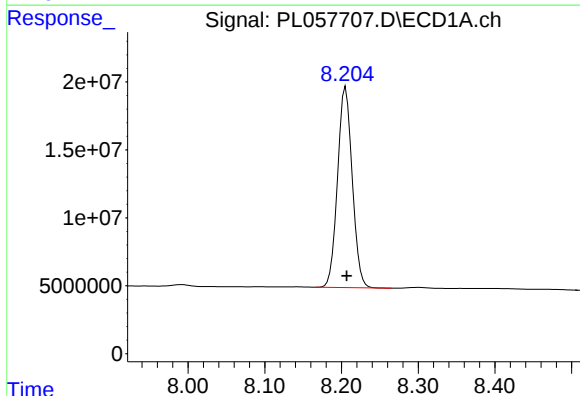

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 196304087
Conc: 18.55 ng/ml

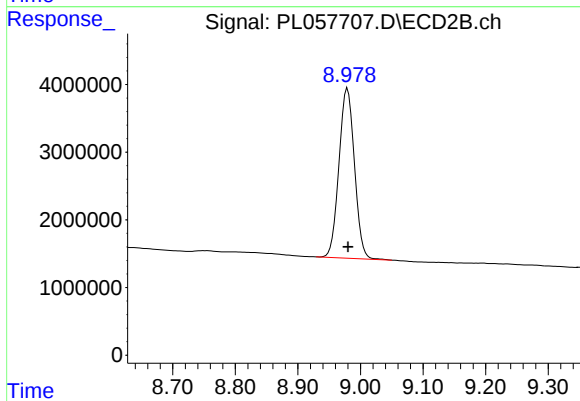

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: 0.000 min
Response: 43288212
Conc: 19.52 ng/ml