

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082225\
 Data File : PL096943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2025 09:18
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 04:09:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
7) B	delta-BHC	4.759f	0.000	12630083	0	2.807	N.D. #
8) B	Heptachlo...	5.647	0.000	171.9E6	0	33.403	N.D. #
14) MA	Endrin	0.000	5.714	0	134.3E6	N.D.	22.735 #
15) B	Endosulfa...	6.777f	6.005	21741611	38592240	4.936	6.748 #
18) B	Endrin al...	6.873	0.000	23721627	0	9.119	N.D. #
24)	Chlordane-2	5.185f	4.406	126.2E6	54848822	692.959	234.328 #
27)	Chlordane-5	0.000	6.005	0	38592240	N.D.	171.276 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082225\
Data File : PL096943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2025 09:18
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 04:09:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25 μ m

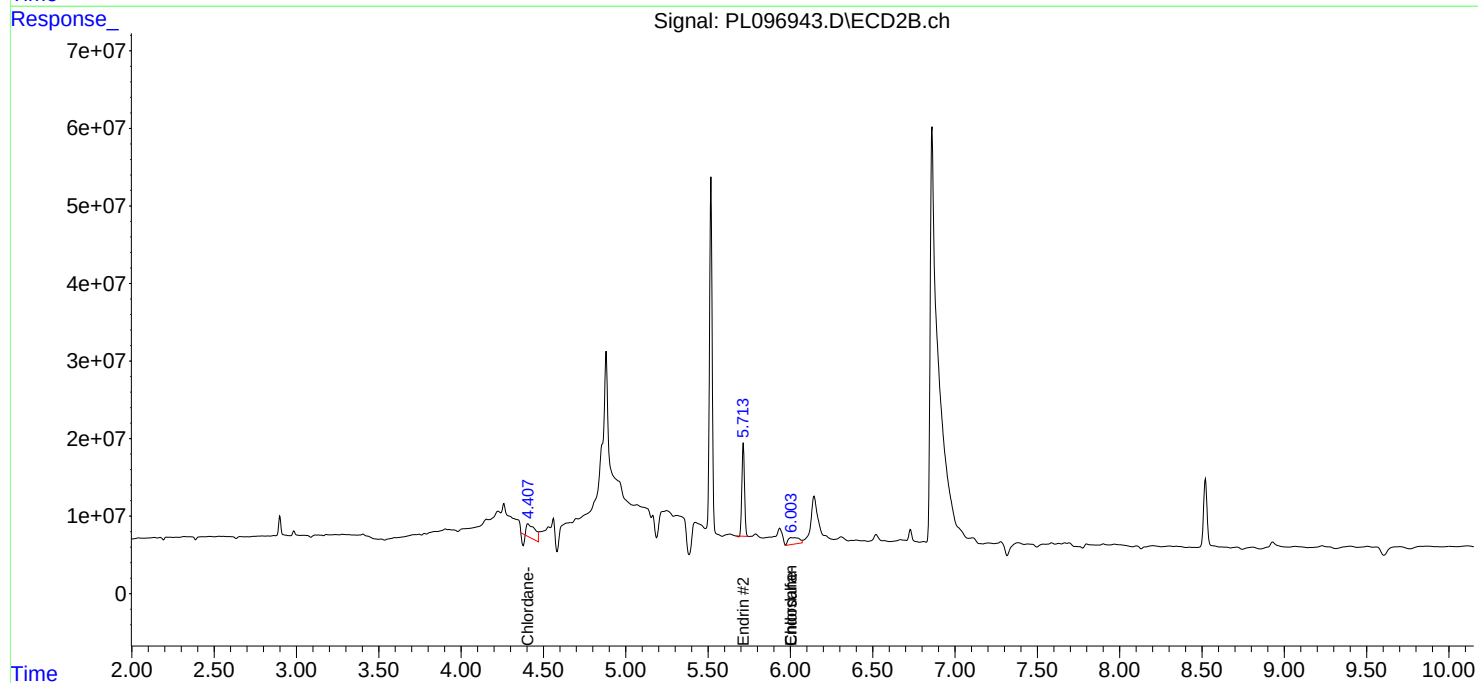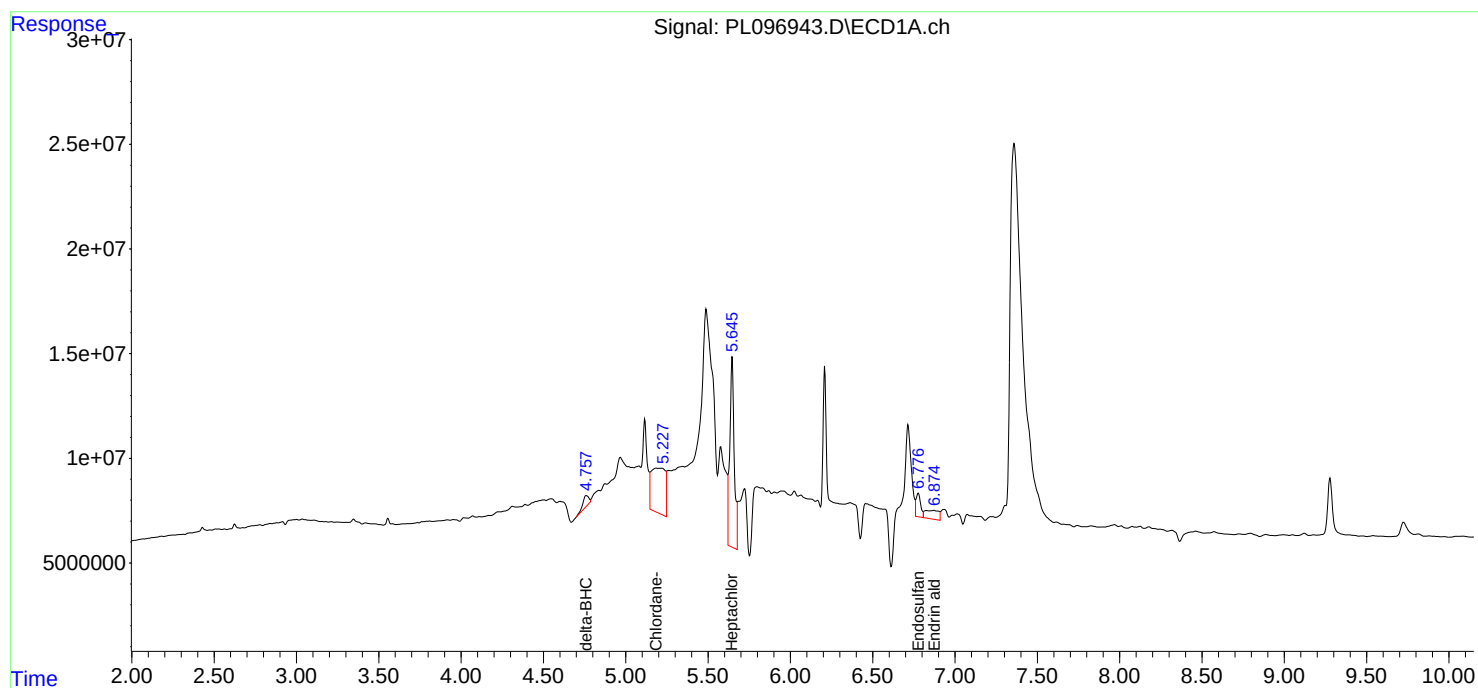


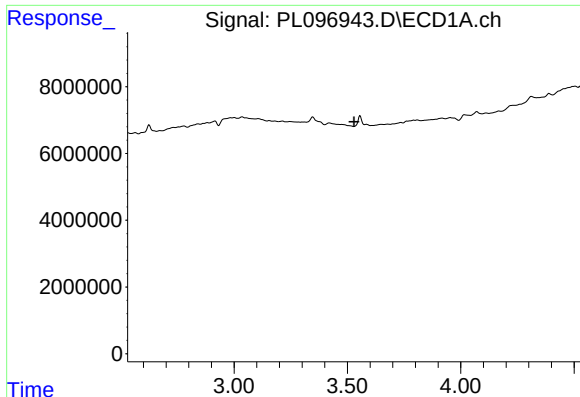

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

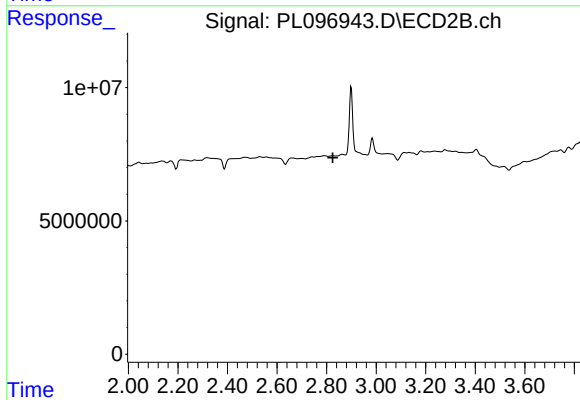


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.825 min
Response: 0
Conc: N.D.

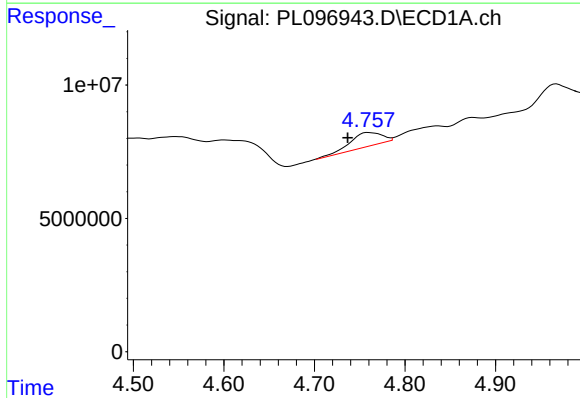


#7 delta-BHC

R.T.: 4.759 min
Delta R.T.: 0.022 min
Response: 12630083
Conc: 2.81 ng/ml

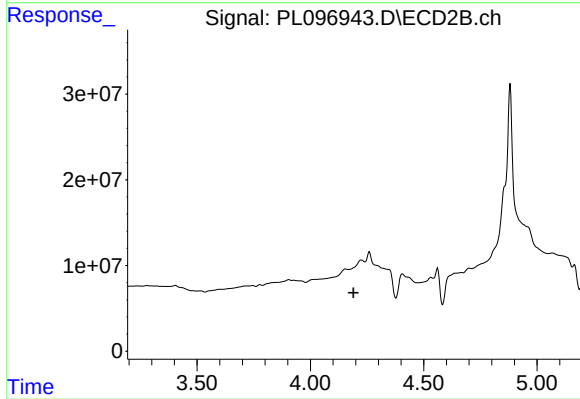

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.191 min
Response: 0
Conc: N.D.

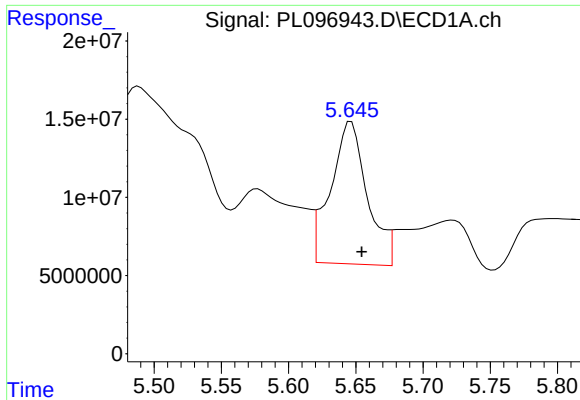

#8 Heptachlor epoxide


R.T.: 5.647 min
Delta R.T.: -0.008 min
Response: 171883370
Conc: 33.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

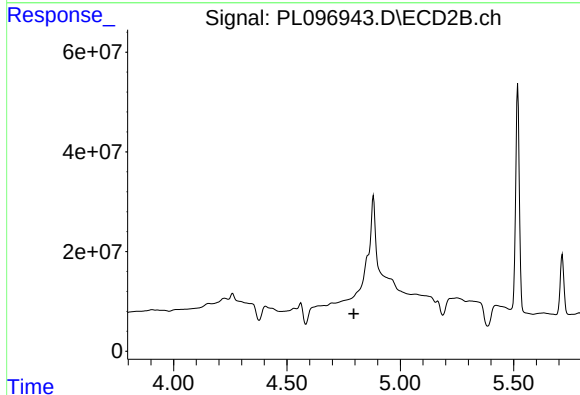


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.795 min
Response: 0
Conc: N.D.

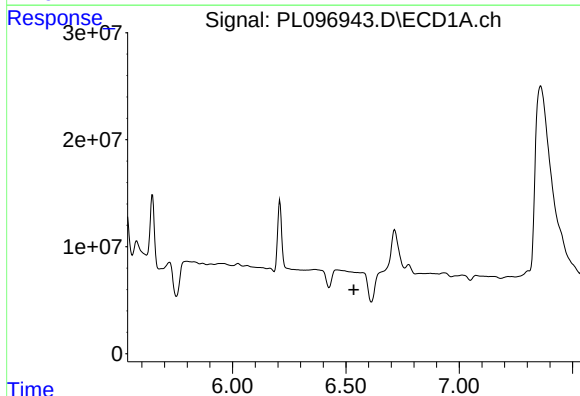


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.534 min
Response: 0
Conc: N.D.

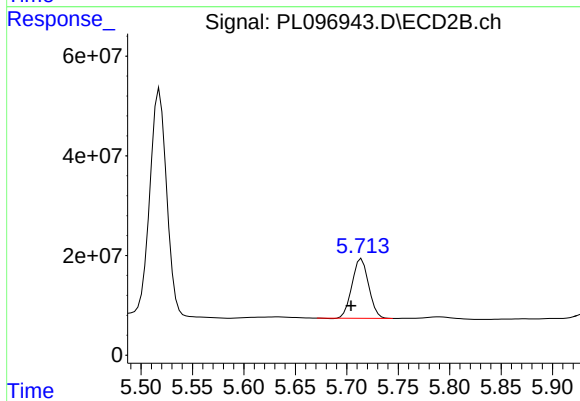

#14 Endrin


R.T.: 5.714 min
Delta R.T.: 0.010 min
Response: 134302890
Conc: 22.74 ng/ml

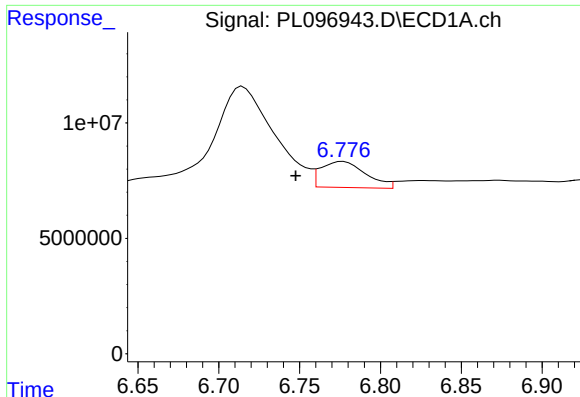

#15 Endosulfan II


R.T.: 6.777 min
Delta R.T.: 0.029 min
Response: 21741611
Conc: 4.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

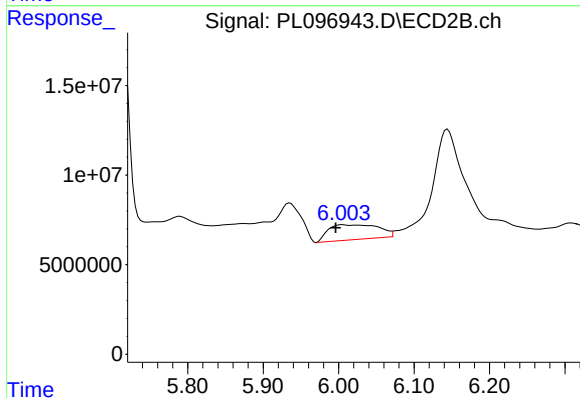


#15 Endosulfan II

R.T.: 6.005 min
Delta R.T.: 0.009 min
Response: 38592240
Conc: 6.75 ng/ml

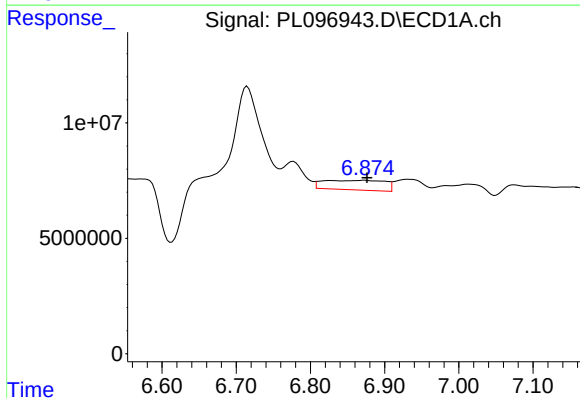


#18 Endrin aldehyde

R.T.: 6.873 min
Delta R.T.: -0.004 min
Response: 23721627
Conc: 9.12 ng/ml

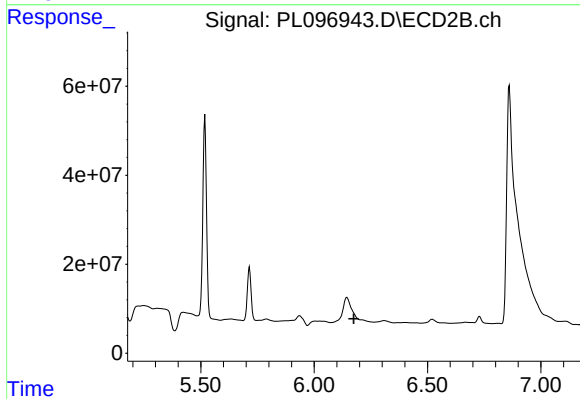

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.175 min
Response: 0
Conc: N.D.

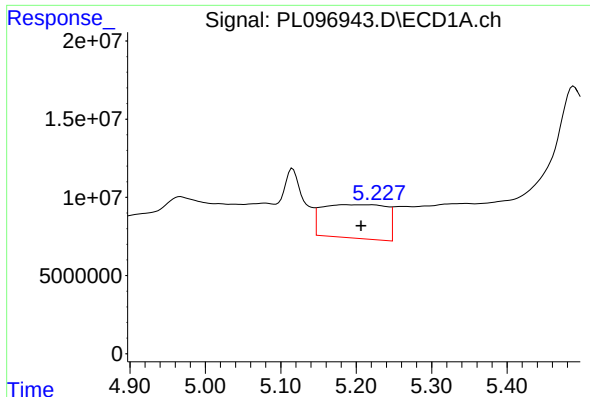

#24 Chlordane-2


R.T.: 5.185 min
Delta R.T.: -0.022 min
Response: 126239588
Conc: 692.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

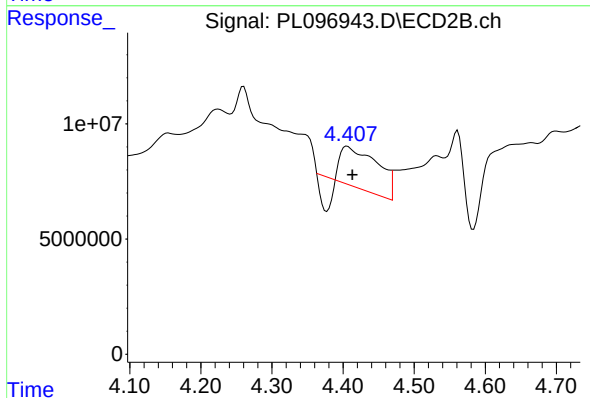


#24 Chlordane-2

R.T.: 4.406 min
Delta R.T.: -0.008 min
Response: 54848822
Conc: 234.33 ng/ml

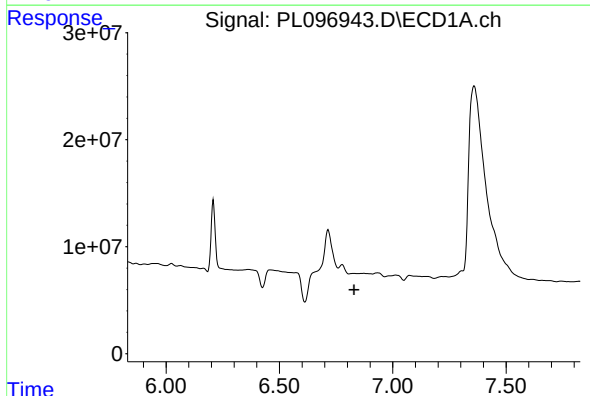


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

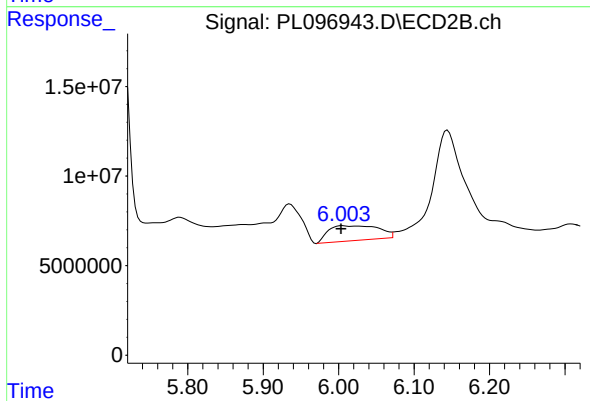

#27 Chlordane-5


R.T.: 6.005 min
Delta R.T.: 0.001 min
Response: 38592240
Conc: 171.28 ng/ml

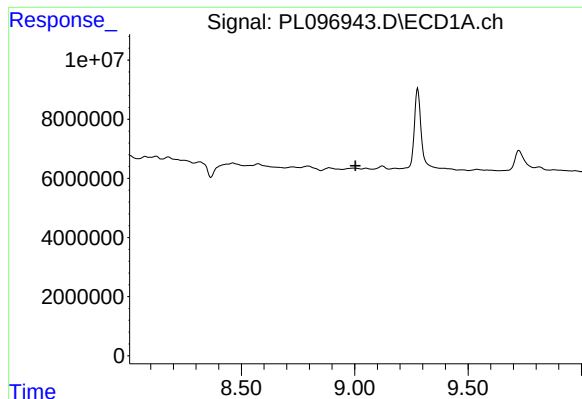

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

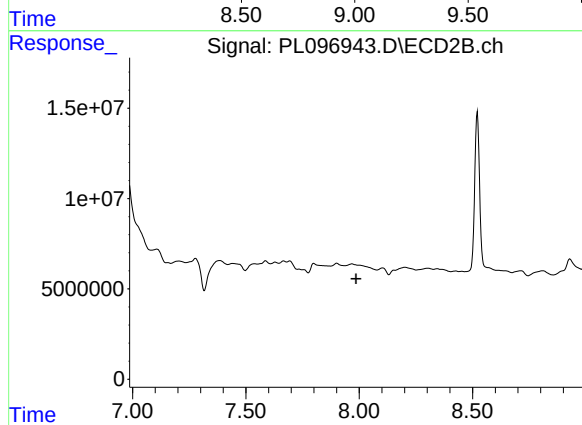

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.987 min
Response: 0
Conc: N.D.